

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012120\
 Data File : PL055969.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 21:48
 Operator : AJ\MA
 Sample : L1211-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B1-0-15

Manual Integrations
 APPROVED

Ankita
 1/22/2020 11:00:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 01:21:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.966	205.7E6	64050451	21.457	22.663
28)	SA Decachlor...	8.233	8.953	202.2E6	49255158	19.340	21.500
Target Compounds							
16)	A 4,4'-DDD	6.162	6.751	12952437	2373995	1.301m	1.030m
17)	MA 4,4'-DDT	6.402	7.045	10038824	1660239	0.992	0.735m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012120\
Data File : PL055969.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 21:48
Operator : AJ\MA
Sample : L1211-01
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
B1-0-15


Manual Integrations
APPROVED

Ankita
1/22/2020 11:00:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 01:21:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

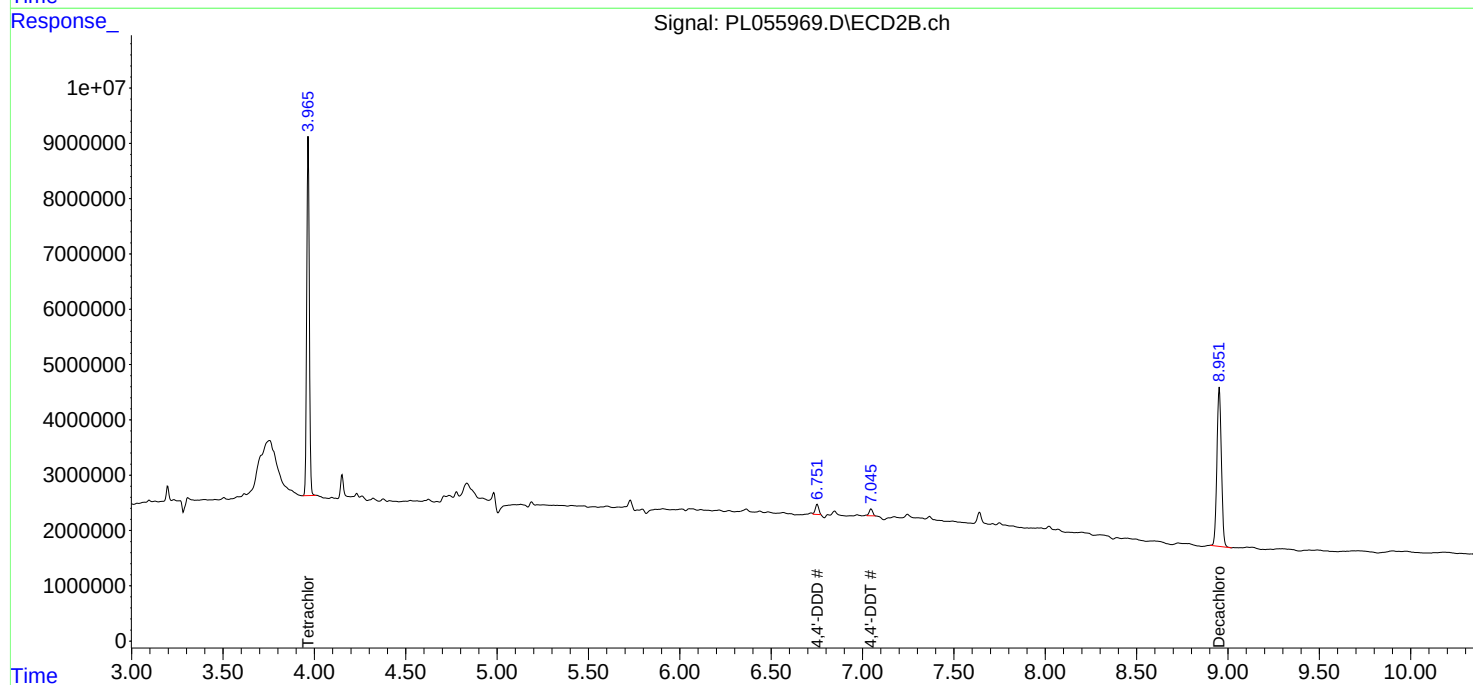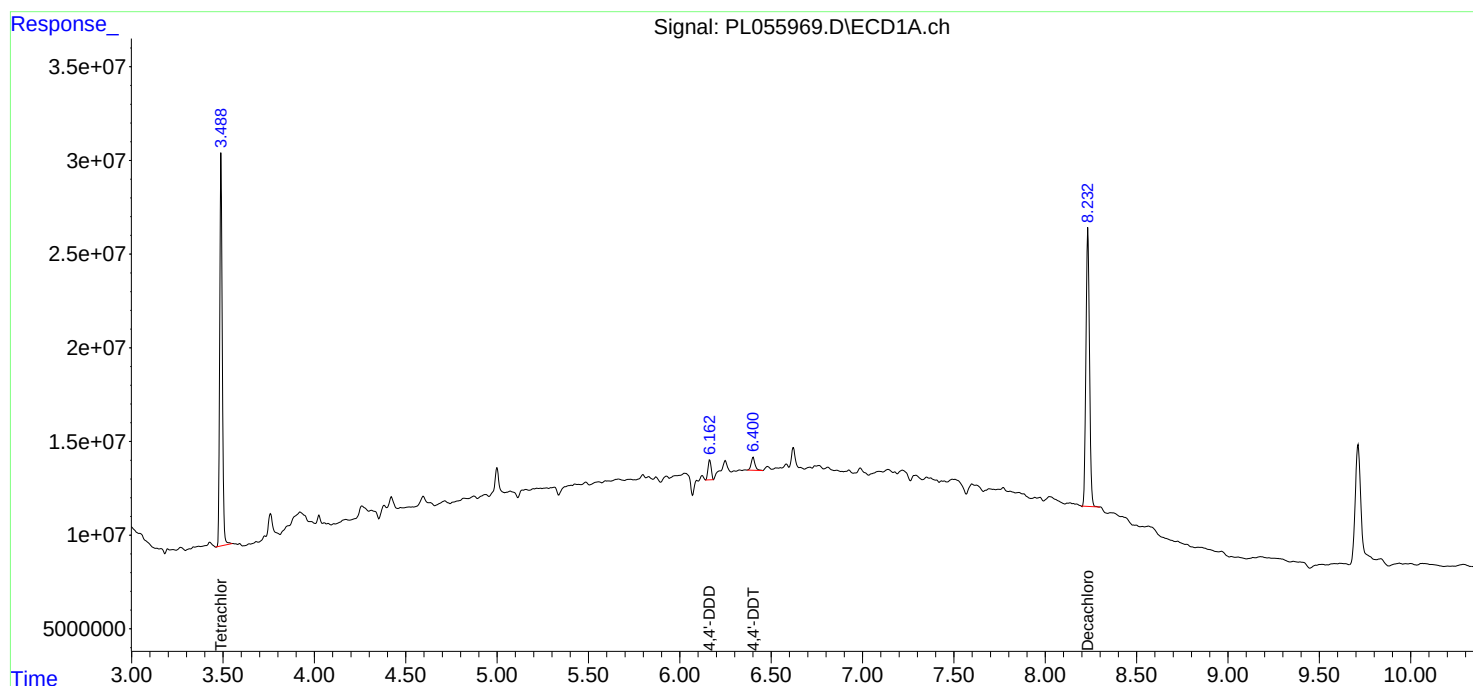

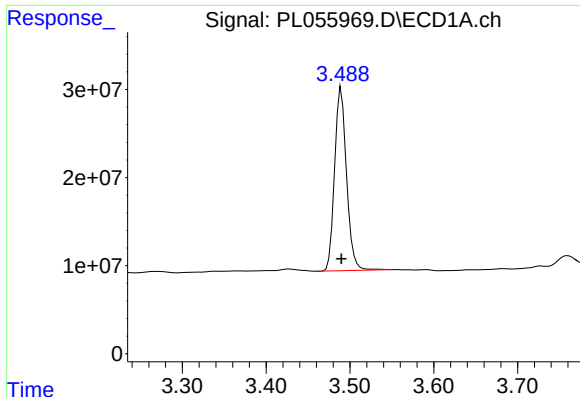


#1 Tetrachloro-m-xylene

R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 205654503
Conc: 21.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
B1-0-15


Manual Integrations
APPROVED

Ankita
1/22/2020 11:00:29 AM

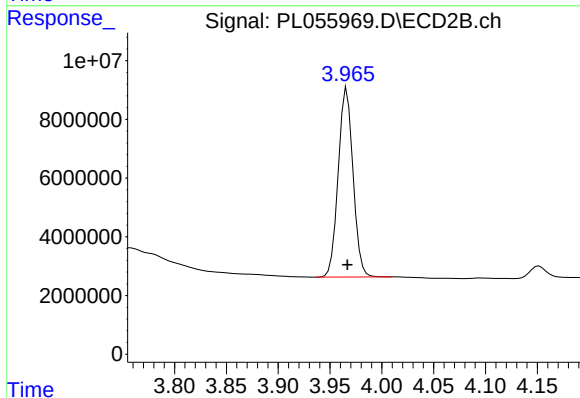


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 64050451
Conc: 22.66 ng/ml

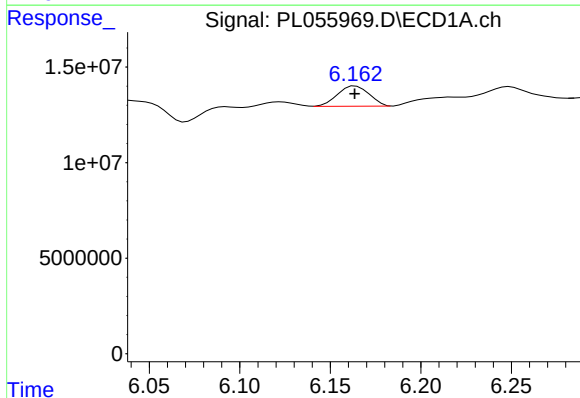


#16 4,4'-DDD

R.T.: 6.162 min
Delta R.T.: -0.001 min
Response: 12952437
Conc: 1.30 ng/ml m

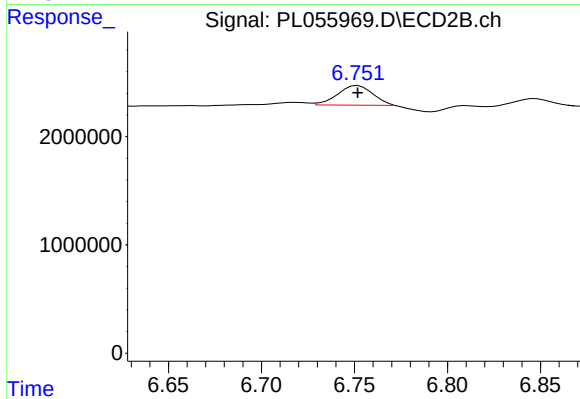

#16 4,4'-DDD

R.T.: 6.751 min
Delta R.T.: -0.001 min
Response: 2373995
Conc: 1.03 ng/ml m

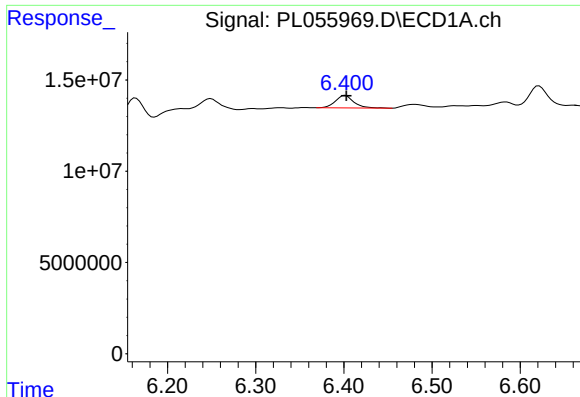


#17 4,4'-DDT

R.T.: 6.402 min
Delta R.T.: -0.001 min
Response: 10038824
Conc: 0.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
B1-0-15


Manual Integrations
APPROVED

Ankita
1/22/2020 11:00:29 AM

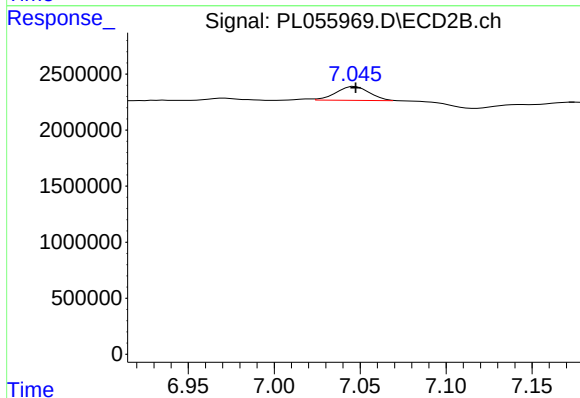


#17 4,4'-DDT

R.T.: 7.045 min
Delta R.T.: -0.002 min
Response: 1660239
Conc: 0.74 ng/ml m

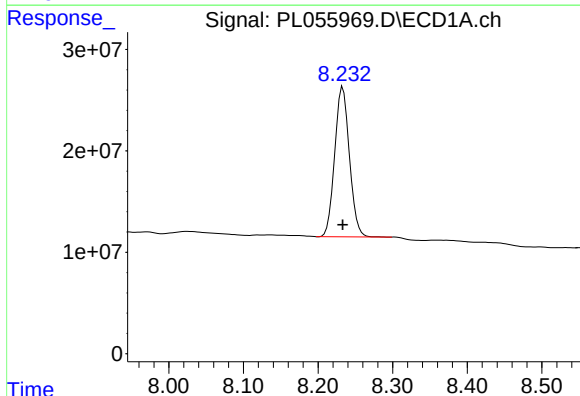

#28 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: 0.000 min
Response: 202213262
Conc: 19.34 ng/ml

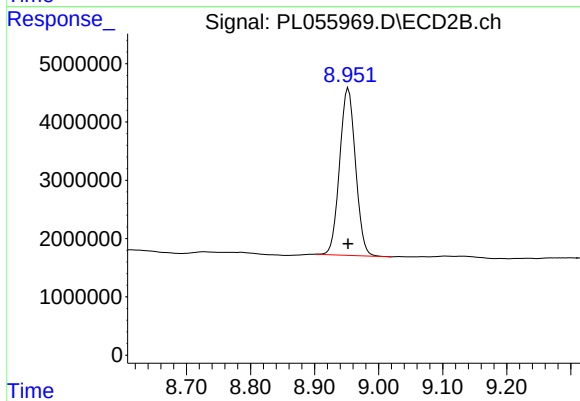

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: 0.000 min
Response: 49255158
Conc: 21.50 ng/ml