

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012121\
 Data File : PL064269.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2021 19:30
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA201

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 03:11:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012121CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 21 03:09:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.108	29098798	23838723	9.883	9.816
27)	SA Decachlor...	8.167	9.269	63343288	48827846	20.886	20.749
Target Compounds							
2)	A alpha-BHC	3.868	4.509	42177090	29386083	9.424	9.263
3)	MA gamma-BHC...	4.148	4.801	41748377	28755075	9.765	9.420
4)	MA Heptachlor	4.448	5.314	41610234	31820052	9.726	9.744
9)	A Endosulfan I	5.470	6.381	34354201	25390541	9.870	9.723
13)	MA Dieldrin	5.712	6.641	74423446	53194315	19.188	18.982
14)	MA Endrin	5.967	6.863	67955832	44057055	19.526	18.947
16)	A 4,4'-DDD	6.097	6.982	56711415	43001172	19.042	19.340
17)	MA 4,4'-DDT	6.337	7.281	57681549	40084475	18.924	18.440
20)	A Methoxychlor	6.885	7.741	165.4E6	128.3E6	101.308	99.607

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012121\
Data File : PL064269.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2021 19:30
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 03:11:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012121CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 21 03:09:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

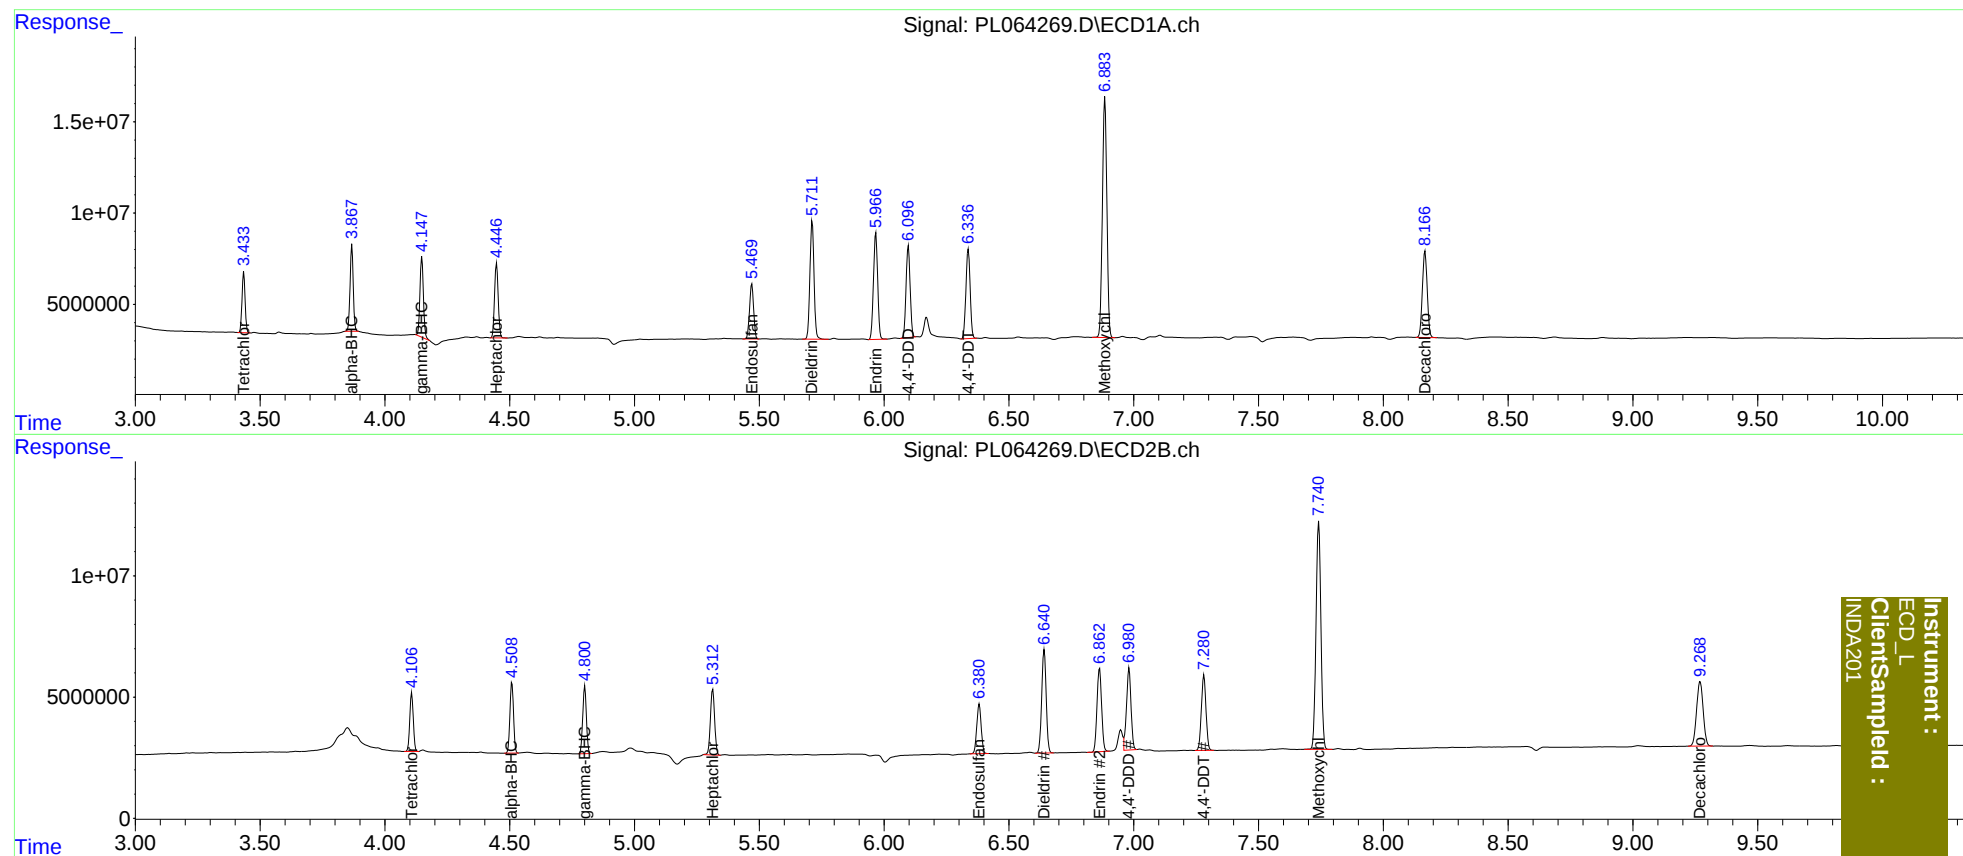


Instrument :
ECD_L
ClientSampled :
INDA201

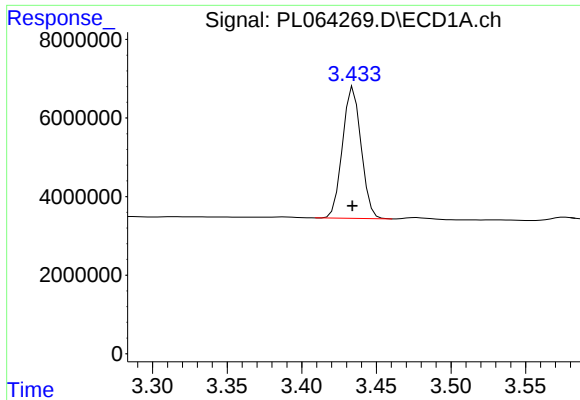

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 29098798
Conc: 9.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA201

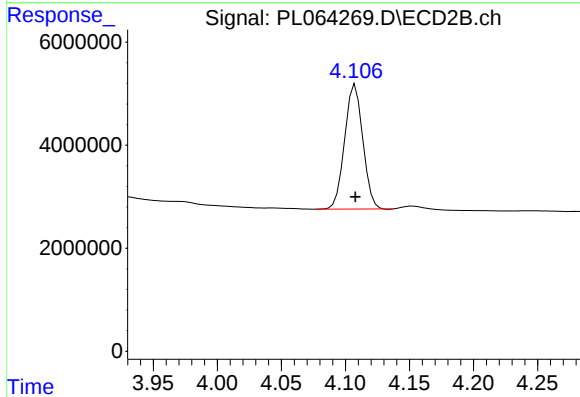


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 23838723
Conc: 9.82 ng/ml

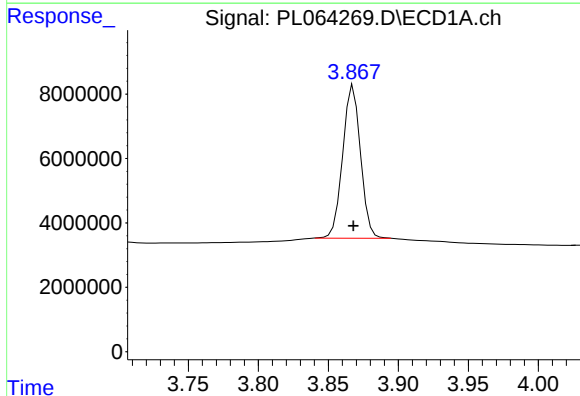


#2 alpha-BHC

R.T.: 3.868 min
Delta R.T.: 0.000 min
Response: 42177090
Conc: 9.42 ng/ml

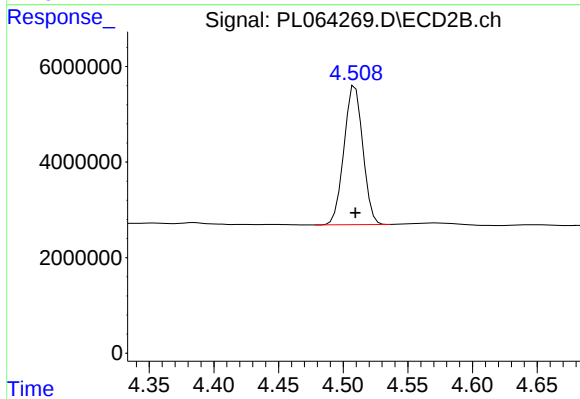

#2 alpha-BHC


R.T.: 4.509 min
Delta R.T.: 0.000 min
Response: 29386083
Conc: 9.26 ng/ml

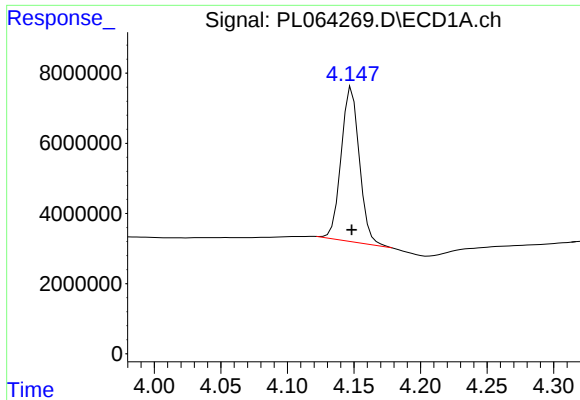

#3 gamma-BHC (Lindane)


R.T.: 4.148 min
Delta R.T.: 0.000 min
Response: 41748377
Conc: 9.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA201

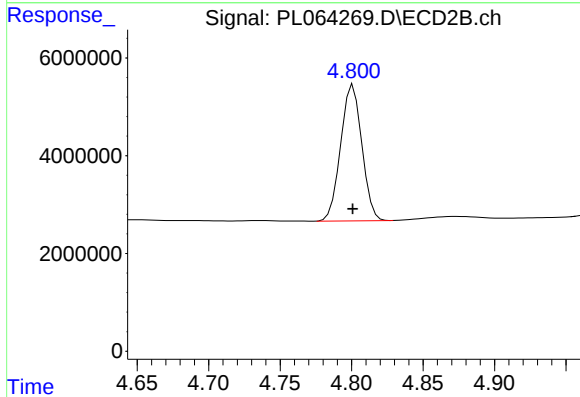


#3 gamma-BHC (Lindane)

R.T.: 4.801 min
Delta R.T.: 0.000 min
Response: 28755075
Conc: 9.42 ng/ml

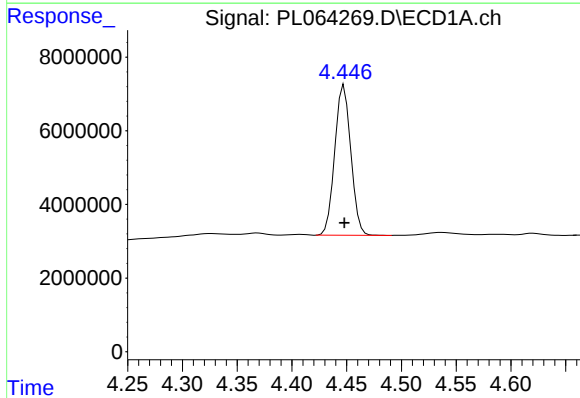


#4 Heptachlor

R.T.: 4.448 min
Delta R.T.: 0.000 min
Response: 41610234
Conc: 9.73 ng/ml

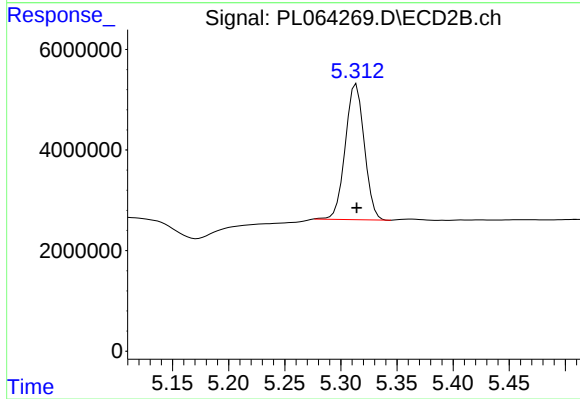

#4 Heptachlor


R.T.: 5.314 min
Delta R.T.: 0.000 min
Response: 31820052
Conc: 9.74 ng/ml

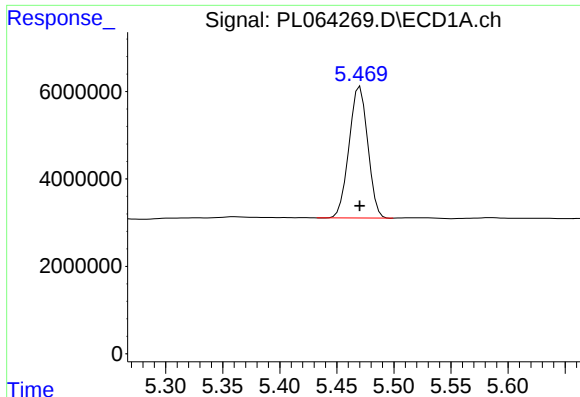

#9 Endosulfan I


R.T.: 5.470 min
Delta R.T.: 0.000 min
Response: 34354201
Conc: 9.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA201

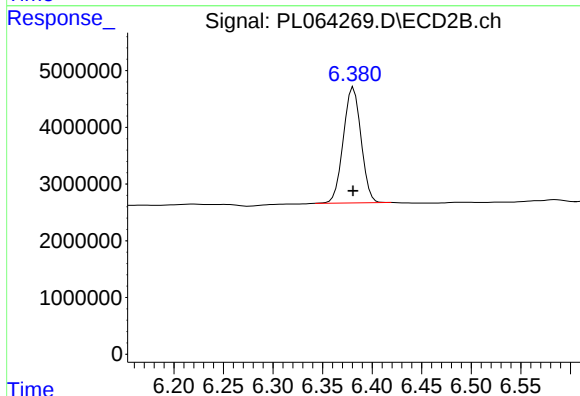


#9 Endosulfan I

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 25390541
Conc: 9.72 ng/ml

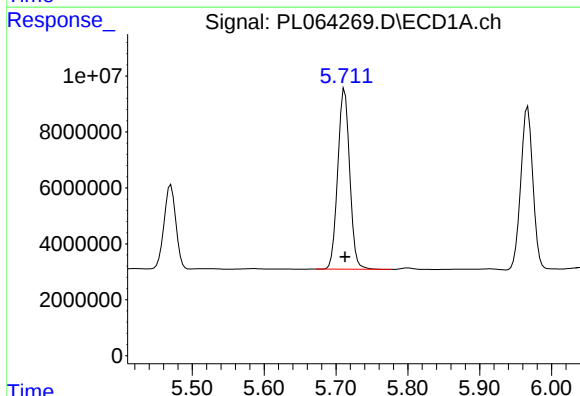


#13 Dieldrin

R.T.: 5.712 min
Delta R.T.: 0.000 min
Response: 74423446
Conc: 19.19 ng/ml

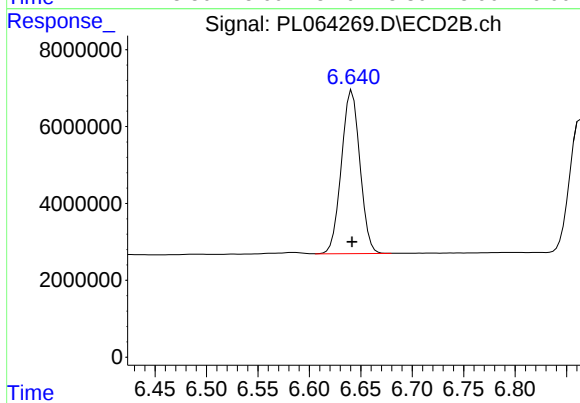

#13 Dieldrin


R.T.: 6.641 min
Delta R.T.: 0.000 min
Response: 53194315
Conc: 18.98 ng/ml

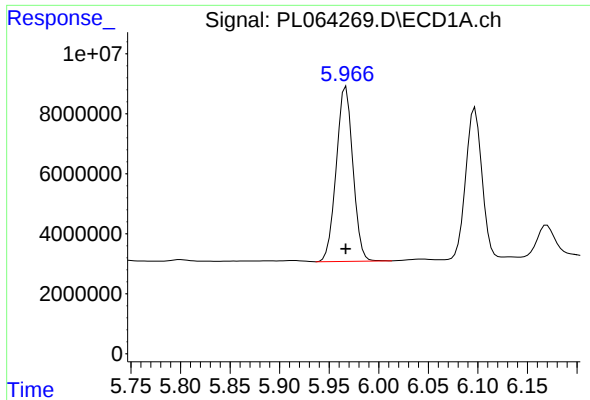

#14 Endrin


R.T.: 5.967 min
Delta R.T.: 0.000 min
Response: 67955832
Conc: 19.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA201

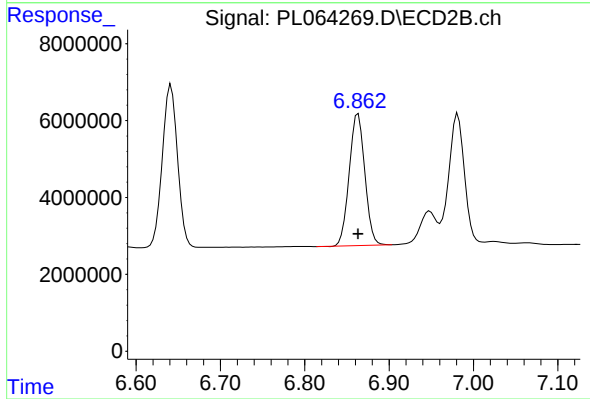


#14 Endrin

R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 44057055
Conc: 18.95 ng/ml

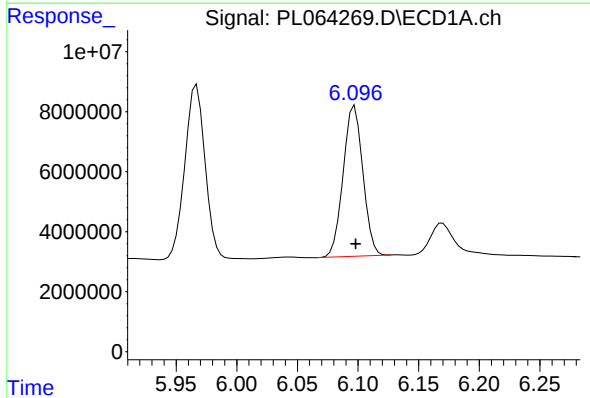


#16 4,4'-DDD

R.T.: 6.097 min
Delta R.T.: 0.000 min
Response: 56711415
Conc: 19.04 ng/ml

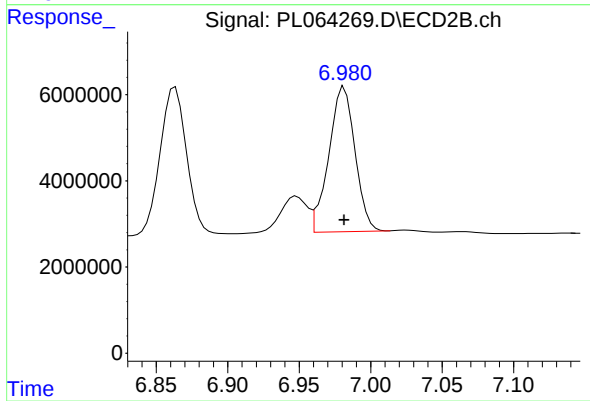

#16 4,4'-DDD


R.T.: 6.982 min
Delta R.T.: 0.000 min
Response: 43001172
Conc: 19.34 ng/ml

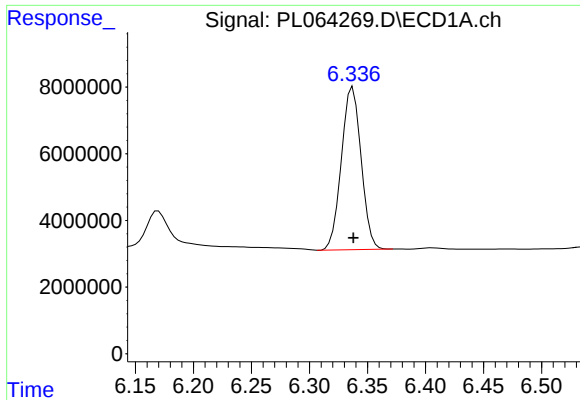

#17 4,4'-DDT


R.T.: 6.337 min
Delta R.T.: 0.000 min
Response: 57681549
Conc: 18.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA201

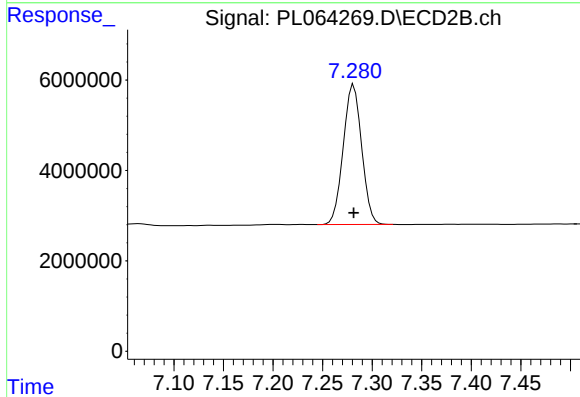


#17 4,4'-DDT

R.T.: 7.281 min
Delta R.T.: 0.000 min
Response: 40084475
Conc: 18.44 ng/ml

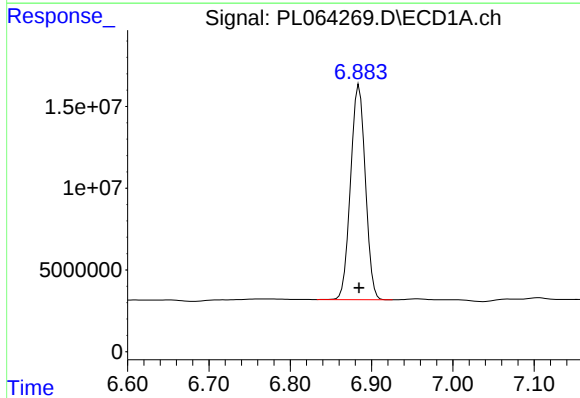


#20 Methoxychlor

R.T.: 6.885 min
Delta R.T.: 0.000 min
Response: 165449744
Conc: 101.31 ng/ml

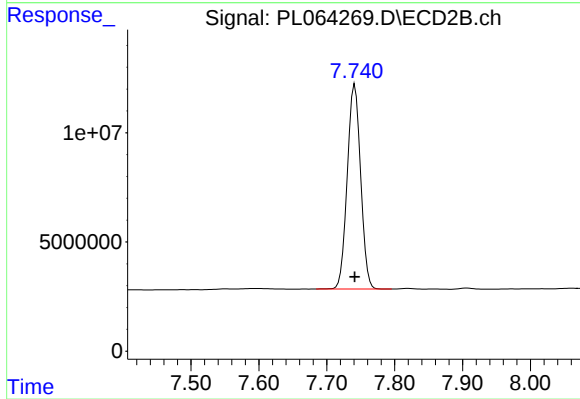

#20 Methoxychlor


R.T.: 7.741 min
Delta R.T.: 0.000 min
Response: 128307997
Conc: 99.61 ng/ml

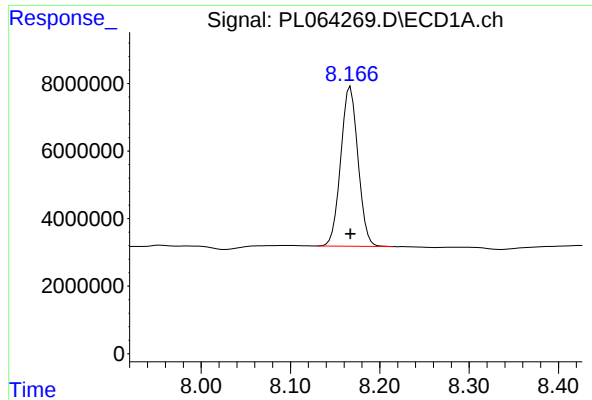

#27 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 63343288
Conc: 20.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA201

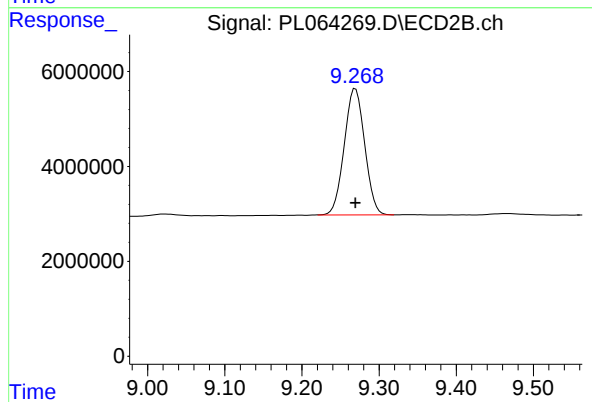

#27 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.000 min
Response: 48827846
Conc: 20.75 ng/ml