

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012121\
 Data File : PL064271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2021 19:58
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA301

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 03:11:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012121CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 21 03:09:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.108	58884990	48572229	20.000	20.000
27)	SA Decachlor...	8.167	9.269	121.3E6	94128548	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.868	4.509	89513682	63447199	20.000	20.000
3)	MA gamma-BHC...	4.148	4.801	85508470	61052774	20.000	20.000
4)	MA Heptachlor	4.448	5.314	85568677	65308761	20.000	20.000
9)	A Endosulfan I	5.470	6.381	69612519	52227940	20.000	20.000
13)	MA Dieldrin	5.713	6.641	155.1E6	112.1E6	40.000	40.000
14)	MA Endrin	5.967	6.863	139.2E6	93012484	40.000	40.000
16)	A 4,4'-DDD	6.098	6.981	119.1E6	88937863	40.000	40.000
17)	MA 4,4'-DDT	6.338	7.281	121.9E6	86949802	40.000	40.000
20)	A Methoxychlor	6.885	7.741	326.6E6	257.6E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012121\
Data File : PL064271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2021 19:58
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 03:11:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012121CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 21 03:09:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

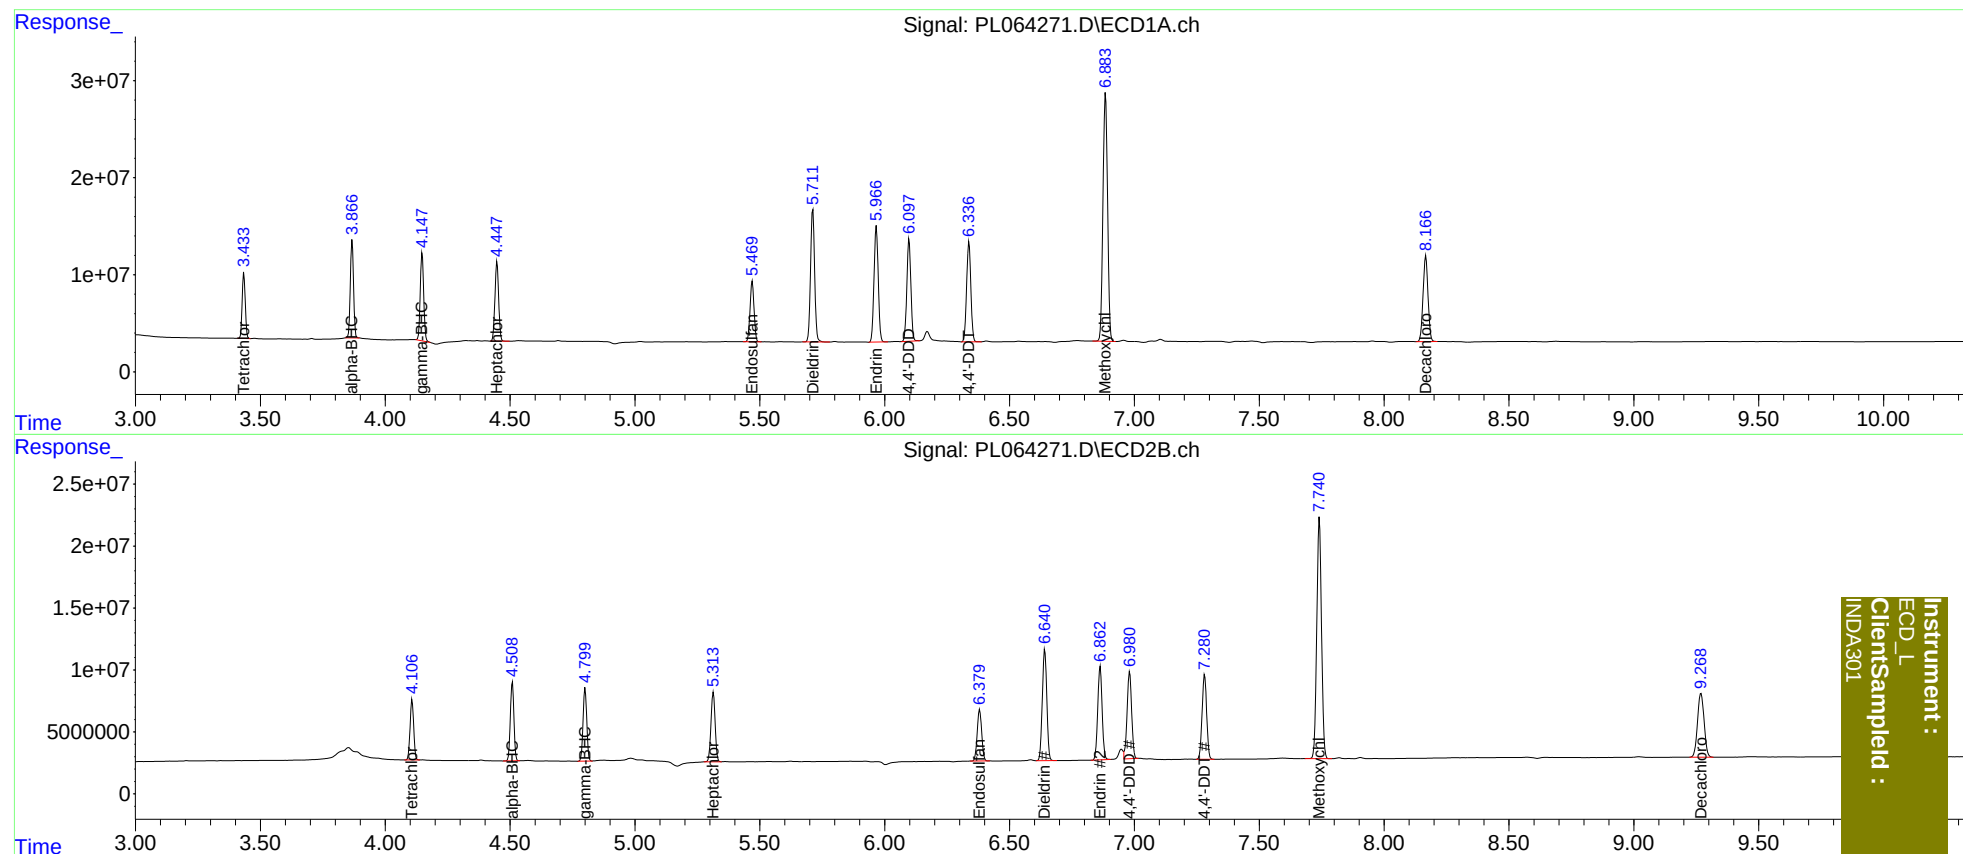


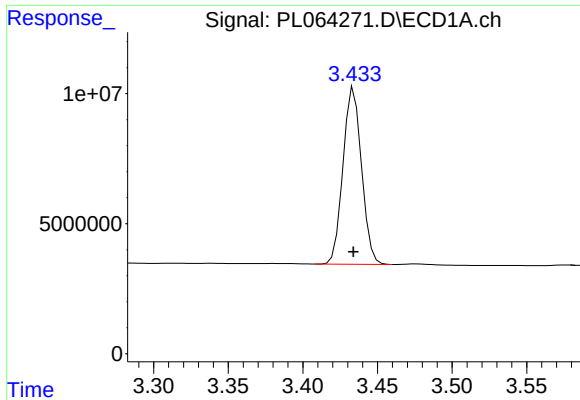

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 58884990
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA301

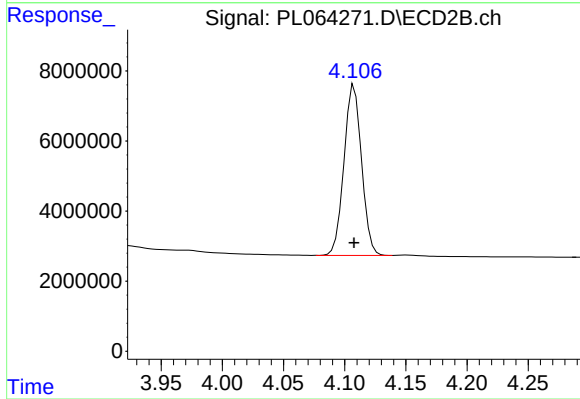


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 48572229
Conc: 20.00 ng/ml

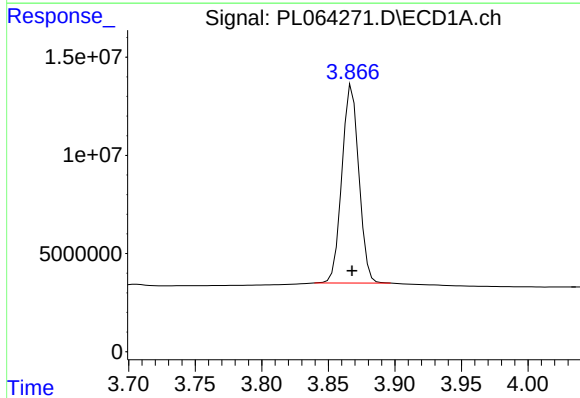


#2 alpha-BHC

R.T.: 3.868 min
Delta R.T.: 0.000 min
Response: 89513682
Conc: 20.00 ng/ml

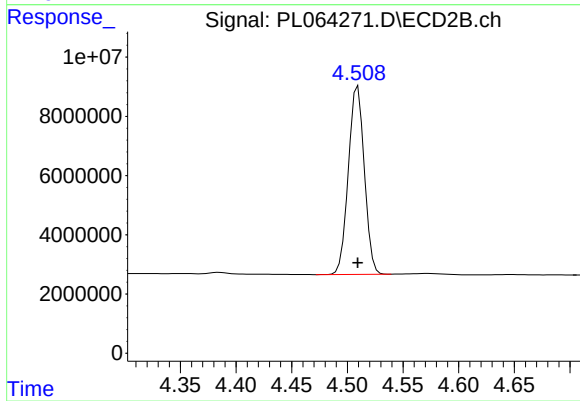

#2 alpha-BHC

R.T.: 4.509 min
Delta R.T.: 0.000 min
Response: 63447199
Conc: 20.00 ng/ml

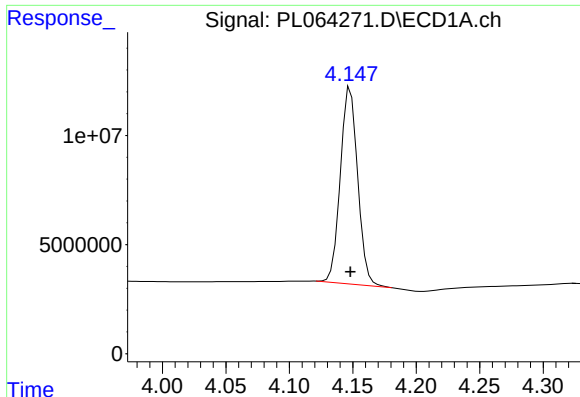

#3 gamma-BHC (Lindane)


R.T.: 4.148 min

Delta R.T.: 0.000 min

Response: 85508470

Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA301

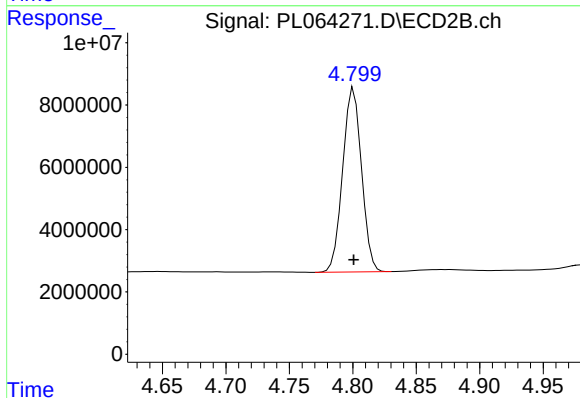


#3 gamma-BHC (Lindane)

R.T.: 4.801 min

Delta R.T.: 0.000 min

Response: 61052774

Conc: 20.00 ng/ml

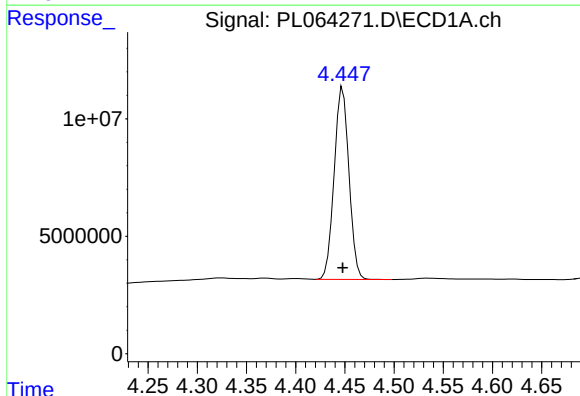


#4 Heptachlor

R.T.: 4.448 min

Delta R.T.: 0.000 min

Response: 85568677

Conc: 20.00 ng/ml

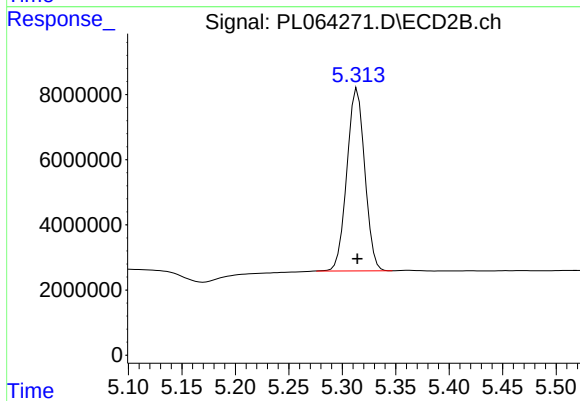


#4 Heptachlor

R.T.: 5.314 min

Delta R.T.: 0.000 min

Response: 65308761


Conc: 20.00 ng/ml

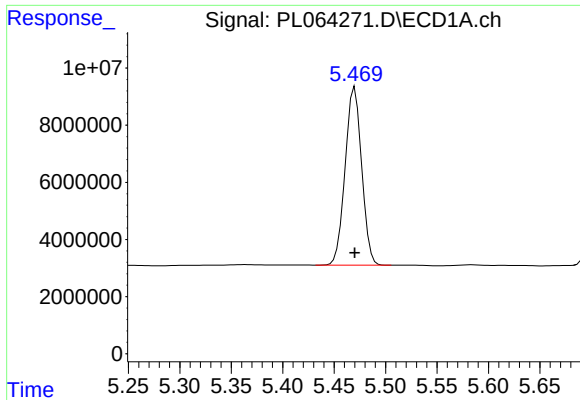

#9 Endosulfan I


R.T.: 5.470 min
Delta R.T.: 0.000 min
Response: 69612519
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA301

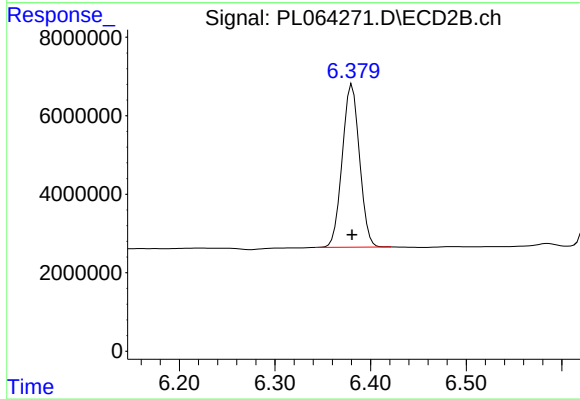


#9 Endosulfan I

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 52227940
Conc: 20.00 ng/ml

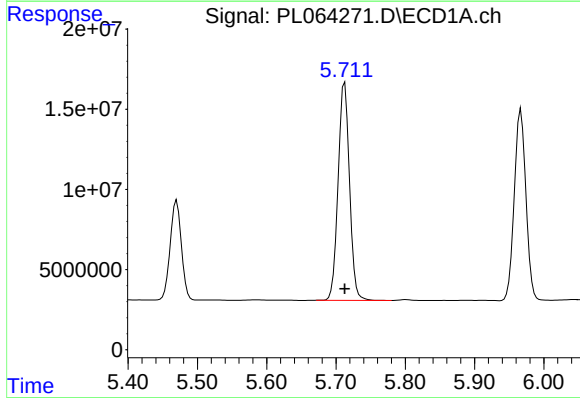


#13 Dieldrin

R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 155145803
Conc: 40.00 ng/ml

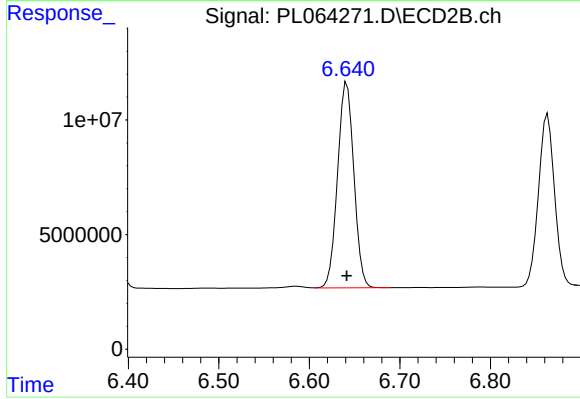

#13 Dieldrin


R.T.: 6.641 min
Delta R.T.: 0.000 min
Response: 112094448
Conc: 40.00 ng/ml

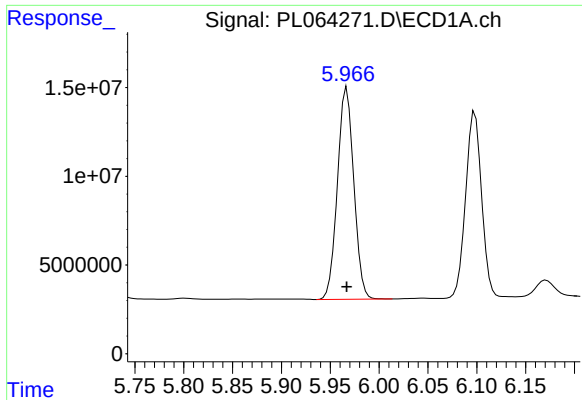

#14 Endrin


R.T.: 5.967 min
Delta R.T.: 0.000 min
Response: 139212739
Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA301

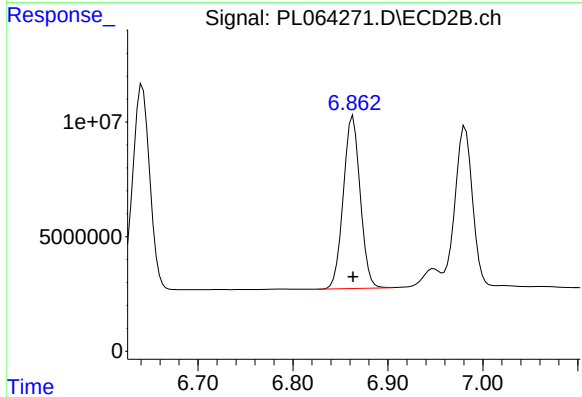


#14 Endrin

R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 93012484
Conc: 40.00 ng/ml

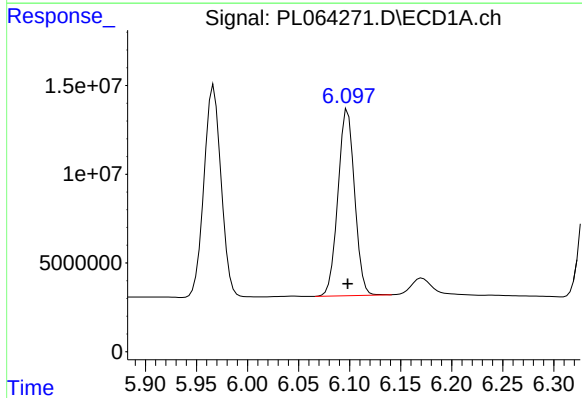


#16 4,4'-DDD

R.T.: 6.098 min
Delta R.T.: 0.000 min
Response: 119130473
Conc: 40.00 ng/ml

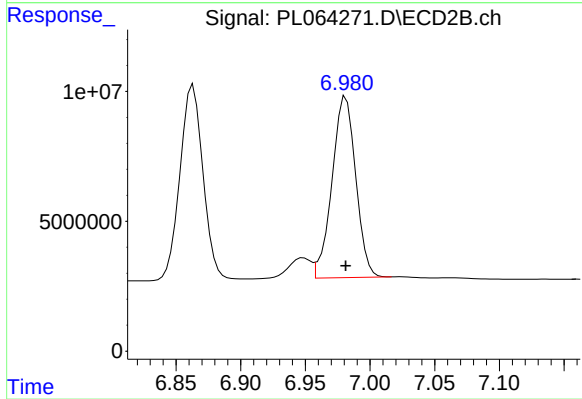

#16 4,4'-DDD


R.T.: 6.981 min
Delta R.T.: 0.000 min
Response: 88937863
Conc: 40.00 ng/ml

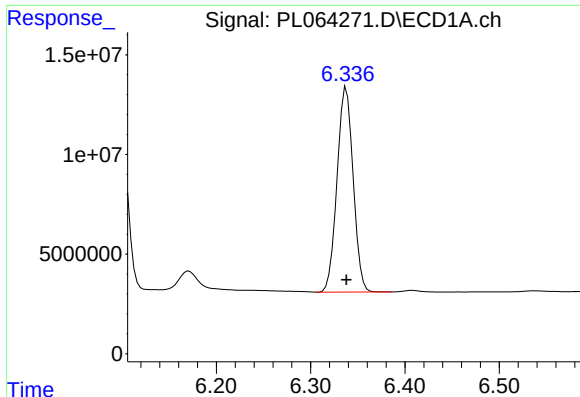

#17 4,4'-DDT


R.T.: 6.338 min
Delta R.T.: 0.000 min
Response: 121923433
Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA301

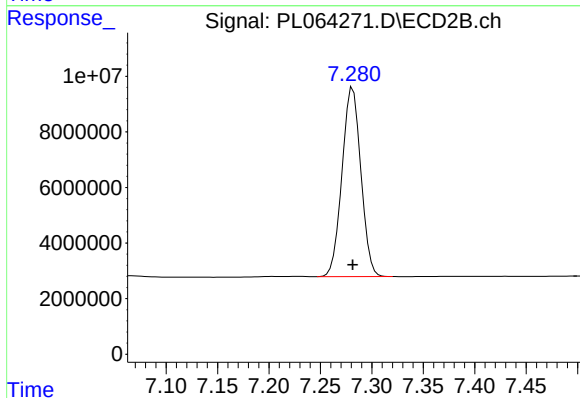


#17 4,4'-DDT

R.T.: 7.281 min
Delta R.T.: 0.000 min
Response: 86949802
Conc: 40.00 ng/ml

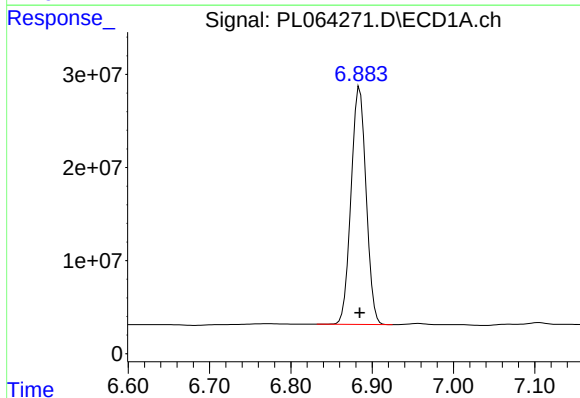


#20 Methoxychlor

R.T.: 6.885 min
Delta R.T.: 0.000 min
Response: 326628680
Conc: 200.00 ng/ml

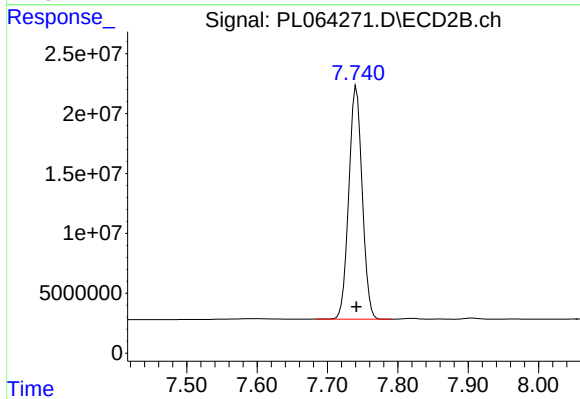

#20 Methoxychlor


R.T.: 7.741 min
Delta R.T.: 0.000 min
Response: 257628828
Conc: 200.00 ng/ml

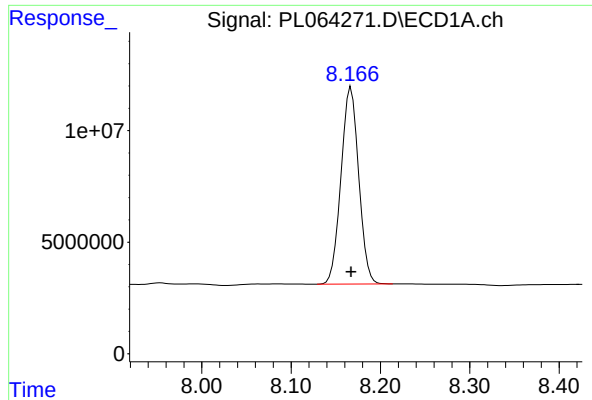

#27 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 121314032
Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA301

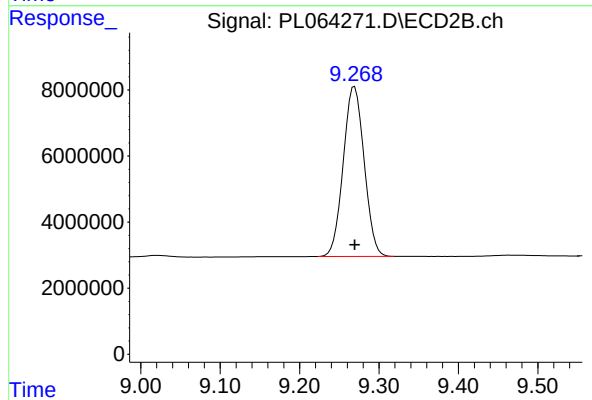

#27 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.000 min
Response: 94128548
Conc: 40.00 ng/ml