

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012121\
 Data File : PL064273.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2021 20:27
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA401

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 03:11:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012121CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 21 03:09:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.108	119.3E6	99633221	40.506	41.025
27)	SA Decachlor...	8.167	9.269	231.8E6	181.2E6	76.427	77.016
Target Compounds							
2)	A alpha-BHC	3.868	4.510	189.9E6	138.7E6	42.430	43.729
3)	MA gamma-BHC...	4.149	4.801	177.5E6	131.1E6	41.512	42.941
4)	MA Heptachlor	4.448	5.314	175.9E6	135.5E6	41.117	41.482
9)	A Endosulfan I	5.470	6.381	140.9E6	107.3E6	40.473	41.100
13)	MA Dieldrin	5.712	6.641	320.3E6	238.2E6	82.580	84.983
14)	MA Endrin	5.967	6.863	282.9E6	196.5E6	81.283	84.510
16)	A 4,4'-DDD	6.098	6.982	243.9E6	194.0E6	81.890	87.248
17)	MA 4,4'-DDT	6.337	7.281	252.5E6	186.8E6	82.831	85.940
20)	A Methoxychlor	6.885	7.741	629.4E6	516.3E6	385.399	400.779


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012121\
Data File : PL064273.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2021 20:27
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 03:11:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012121CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 21 03:09:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

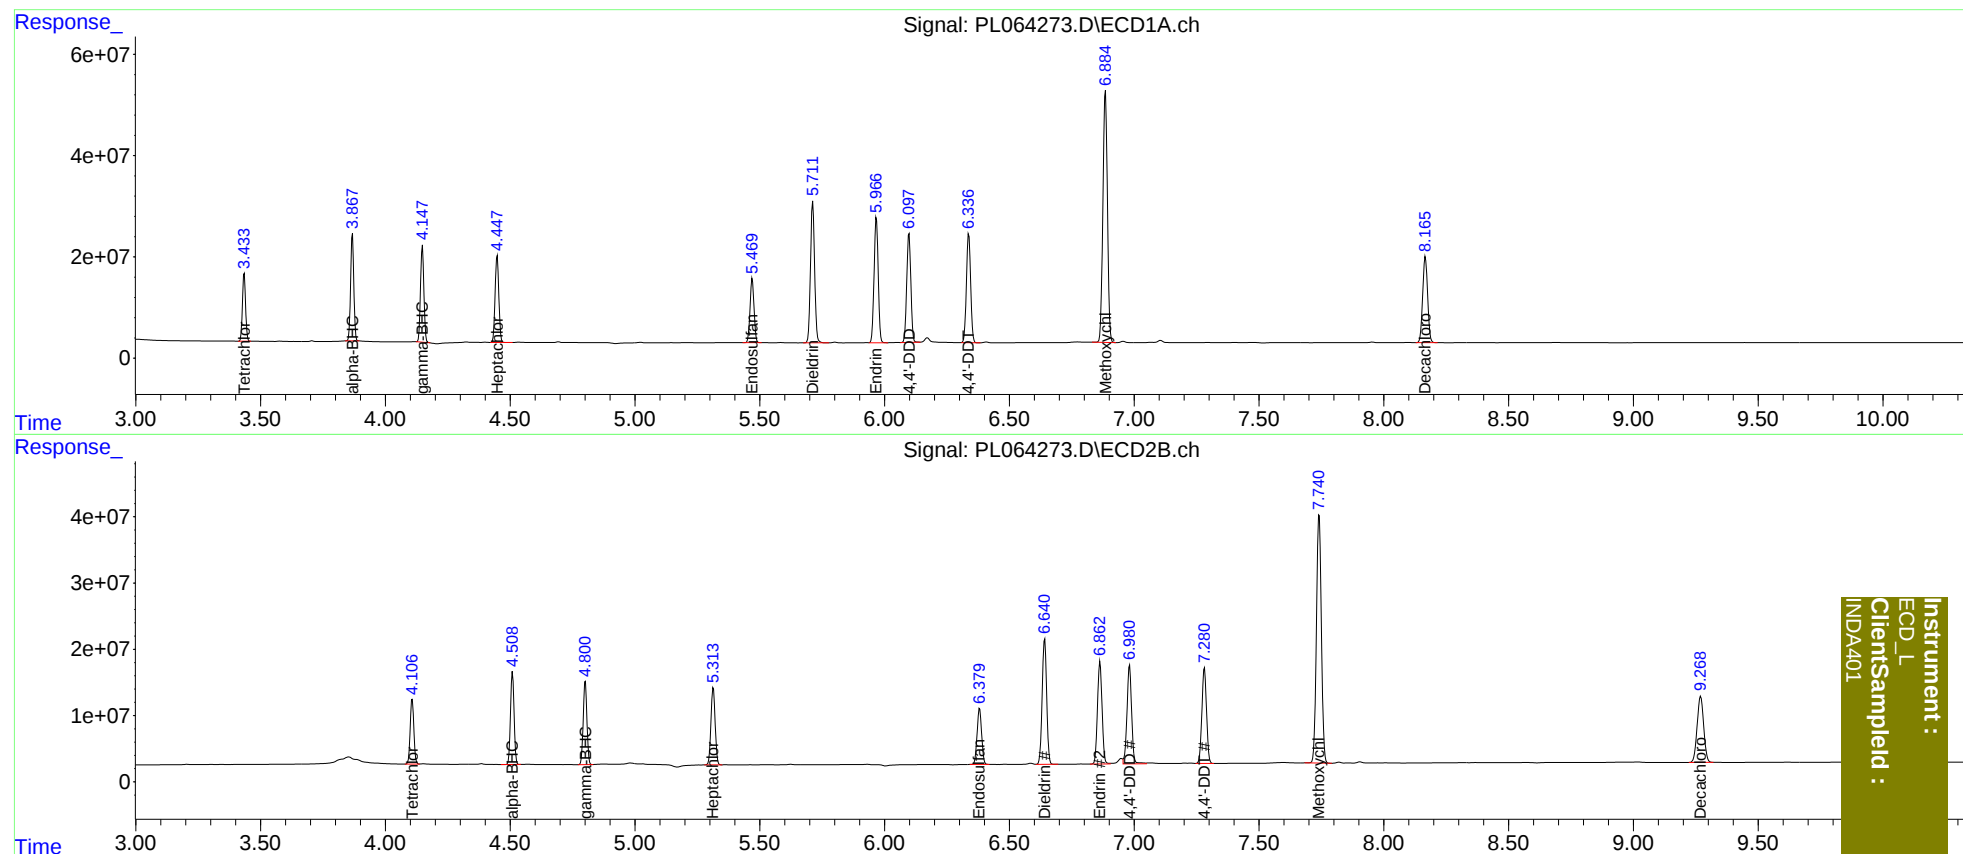


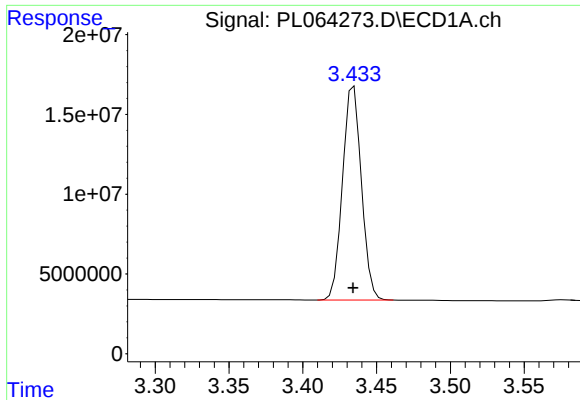

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 119259838
Conc: 40.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA401

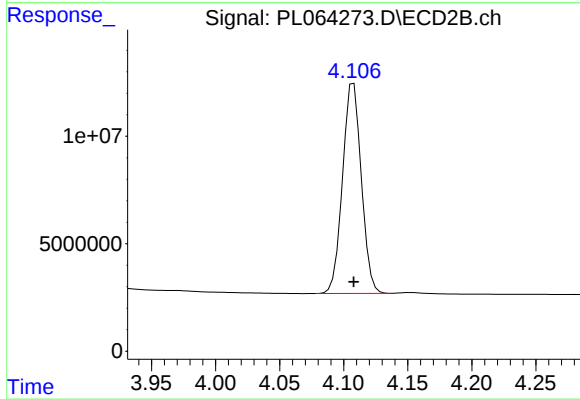


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 99633221
Conc: 41.02 ng/ml

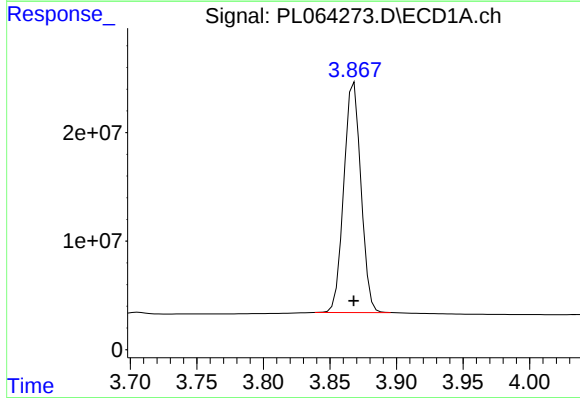


#2 alpha-BHC

R.T.: 3.868 min
Delta R.T.: 0.000 min
Response: 189902287
Conc: 42.43 ng/ml

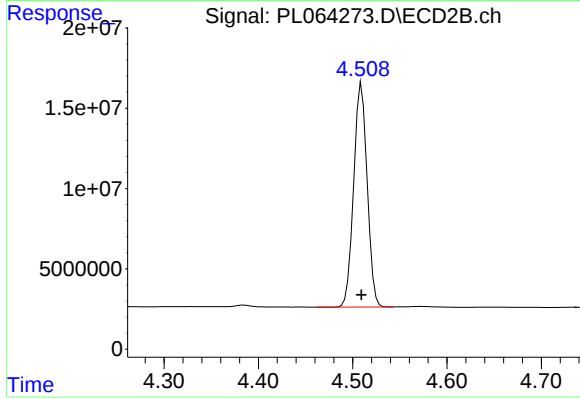

#2 alpha-BHC


R.T.: 4.510 min
Delta R.T.: 0.000 min
Response: 138725207
Conc: 43.73 ng/ml

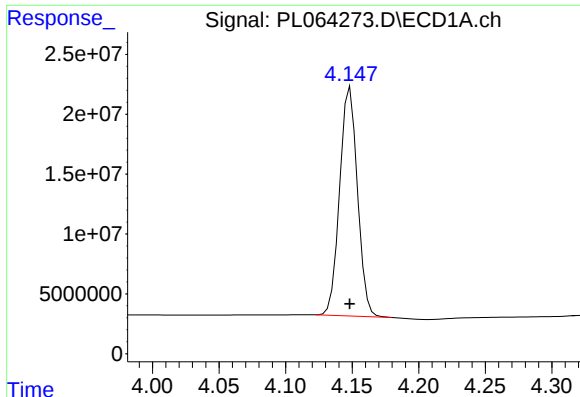

#3 gamma-BHC (Lindane)


R.T.: 4.149 min
Delta R.T.: 0.000 min
Response: 177480497
Conc: 41.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA401

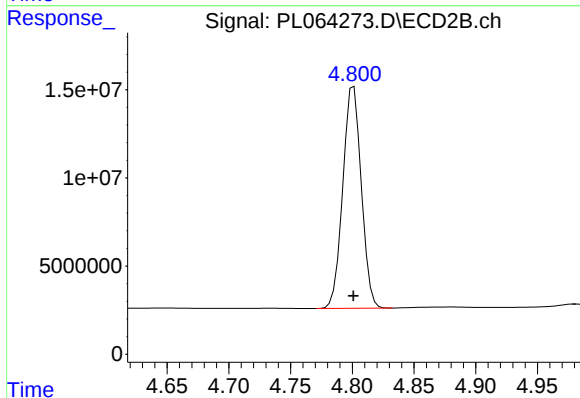


#3 gamma-BHC (Lindane)

R.T.: 4.801 min
Delta R.T.: 0.000 min
Response: 131083359
Conc: 42.94 ng/ml

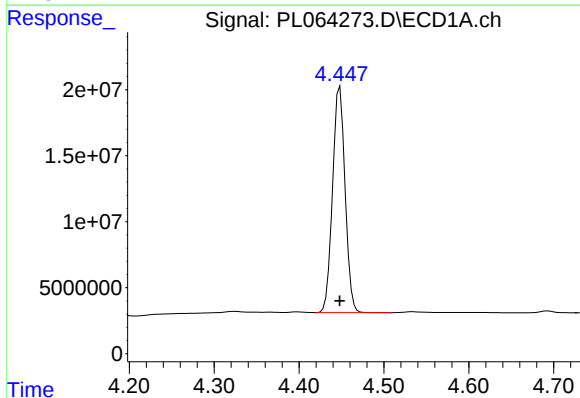


#4 Heptachlor

R.T.: 4.448 min
Delta R.T.: 0.000 min
Response: 175916852
Conc: 41.12 ng/ml

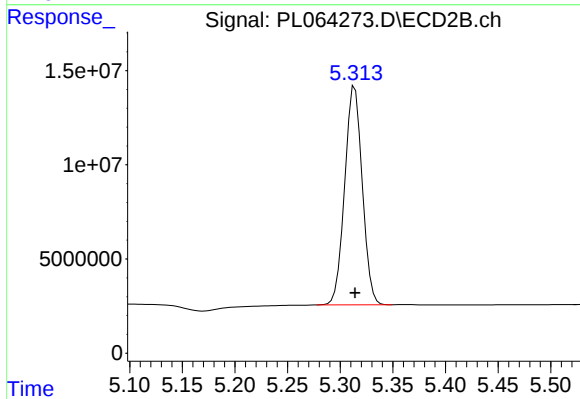

#4 Heptachlor


R.T.: 5.314 min
Delta R.T.: 0.000 min
Response: 135457325
Conc: 41.48 ng/ml

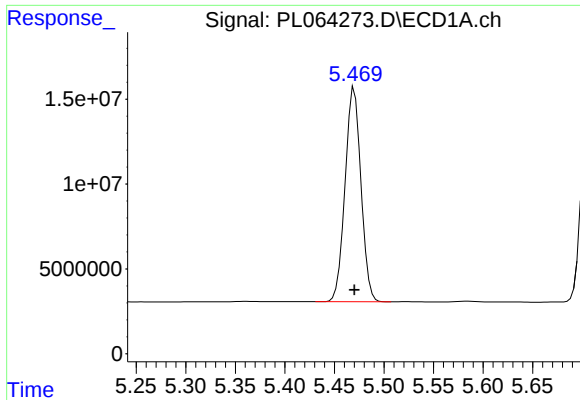

#9 Endosulfan I


R.T.: 5.470 min
Delta R.T.: 0.000 min
Response: 140870561
Conc: 40.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA401

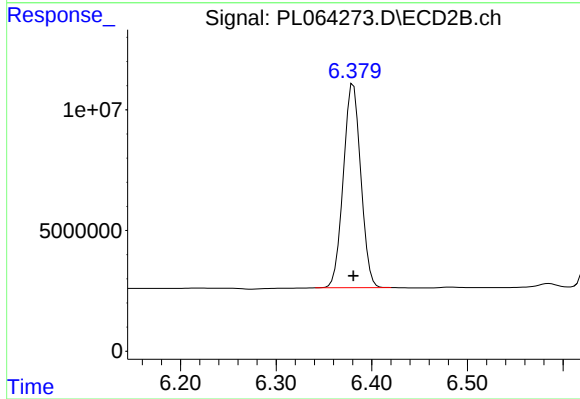


#9 Endosulfan I

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 107327315
Conc: 41.10 ng/ml

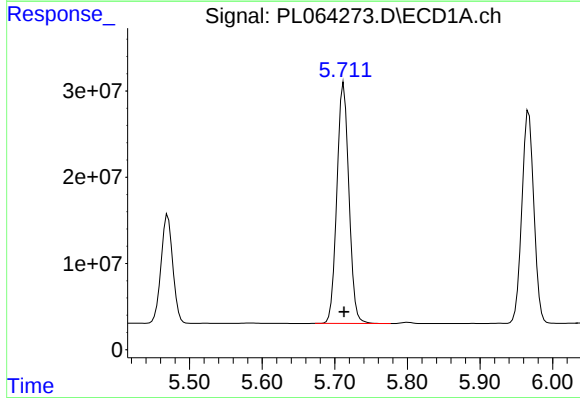


#13 Dieldrin

R.T.: 5.712 min
Delta R.T.: 0.000 min
Response: 320297538
Conc: 82.58 ng/ml

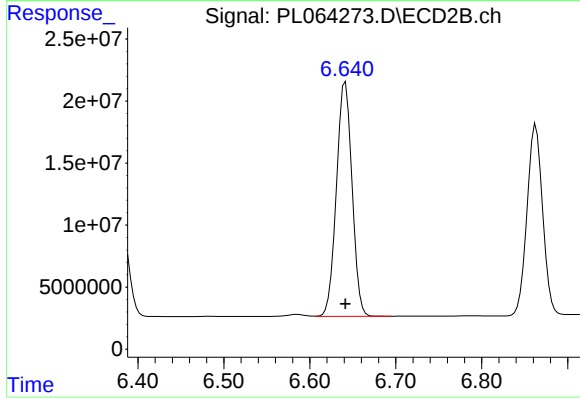

#13 Dieldrin


R.T.: 6.641 min
Delta R.T.: 0.000 min
Response: 238152513
Conc: 84.98 ng/ml

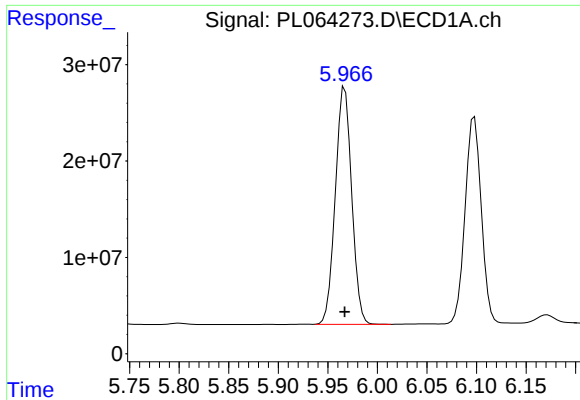

#14 Endrin


R.T.: 5.967 min
Delta R.T.: 0.000 min
Response: 282892187
Conc: 81.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA401

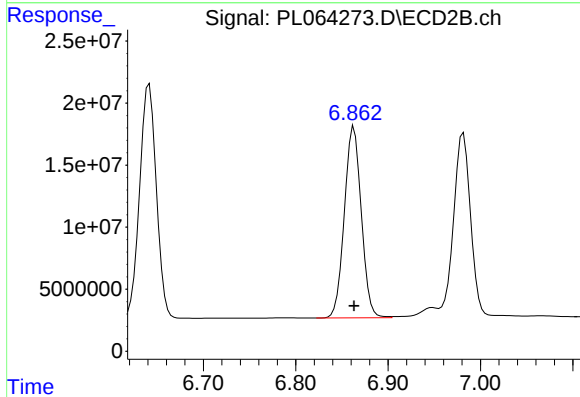


#14 Endrin

R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 196511249
Conc: 84.51 ng/ml

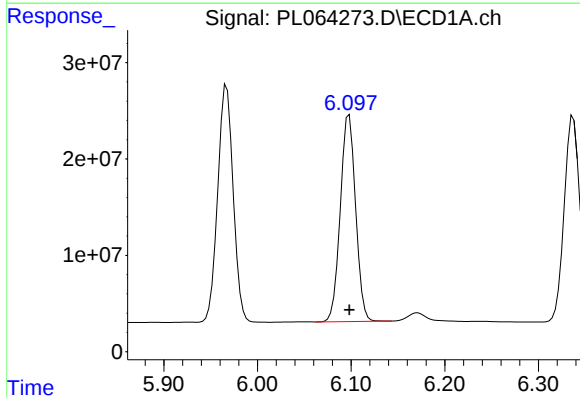


#16 4,4'-DDD

R.T.: 6.098 min
Delta R.T.: 0.000 min
Response: 243889782
Conc: 81.89 ng/ml

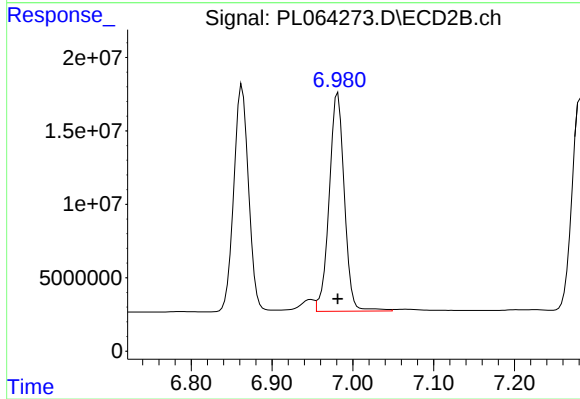

#16 4,4'-DDD


R.T.: 6.982 min
Delta R.T.: 0.000 min
Response: 193990534
Conc: 87.25 ng/ml

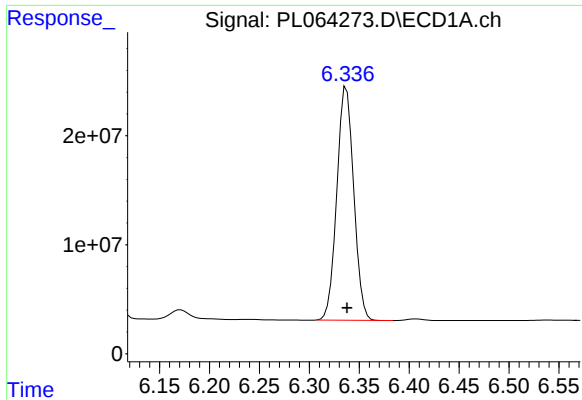

#17 4,4'-DDT


R.T.: 6.337 min
Delta R.T.: 0.000 min
Response: 252476759
Conc: 82.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA401

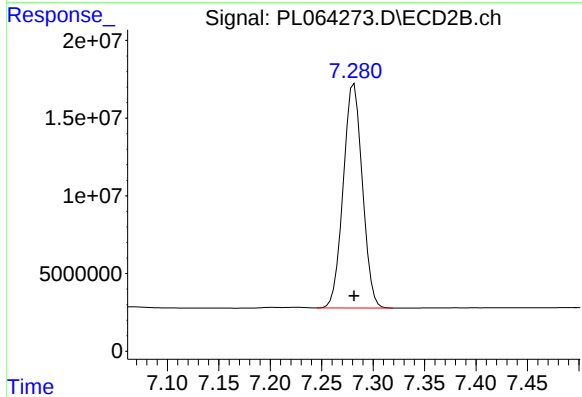


#17 4,4'-DDT

R.T.: 7.281 min
Delta R.T.: 0.000 min
Response: 186812400
Conc: 85.94 ng/ml

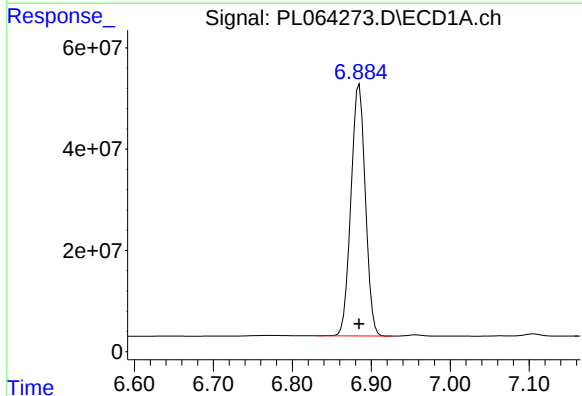


#20 Methoxychlor

R.T.: 6.885 min
Delta R.T.: 0.000 min
Response: 629412054
Conc: 385.40 ng/ml

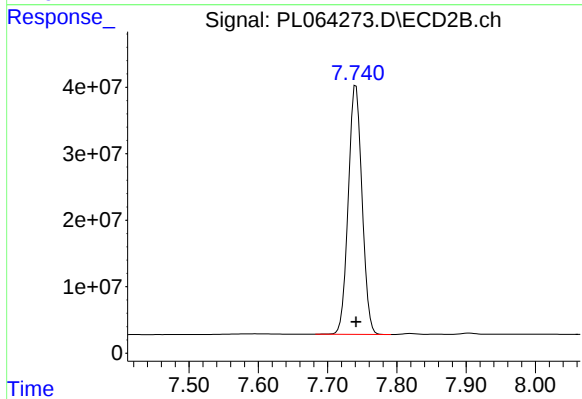

#20 Methoxychlor


R.T.: 7.741 min
Delta R.T.: 0.000 min
Response: 516261724
Conc: 400.78 ng/ml

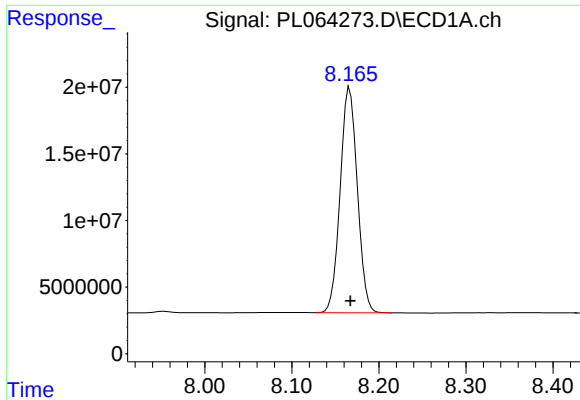

#27 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 231791481
Conc: 76.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA401

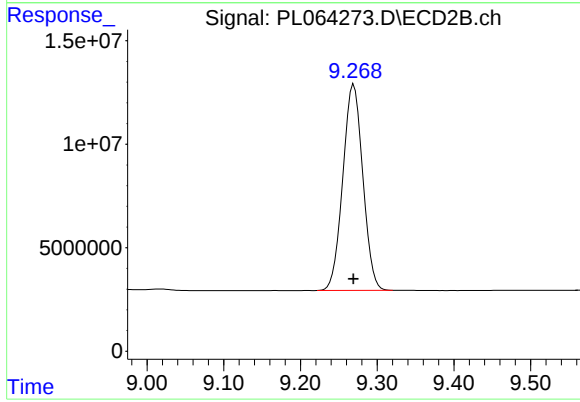

#27 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.000 min
Response: 181235861
Conc: 77.02 ng/ml