

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012121\
 Data File : PL064275.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2021 20:55
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA501

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 03:12:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012121CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 21 03:09:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.108	226.9E6	192.5E6	77.059	79.253
27)	SA Decachlor...	8.166	9.270	422.6E6	326.8E6	139.341	138.879
Target Compounds							
2)	A alpha-BHC	3.868	4.510	374.9E6	284.4E6	83.755	89.636
3)	MA gamma-BHC...	4.148	4.802	346.2E6	263.5E6	80.973	86.308
4)	MA Heptachlor	4.448	5.315	335.4E6	264.7E6	78.390	81.069
9)	A Endosulfan I	5.470	6.381	265.5E6	205.1E6	76.280	78.549
13)	MA Dieldrin	5.712	6.642	613.6E6	469.8E6	158.209	167.641
14)	MA Endrin	5.967	6.864	538.9E6	376.0E6	154.837	161.686
16)	A 4,4'-DDD	6.097	6.982	476.5E6	372.5E6	159.998	167.528
17)	MA 4,4'-DDT	6.337	7.282	495.7E6	365.5E6	162.614	168.156
20)	A Methoxychlor	6.884	7.741	1130.0E6	944.6E6	691.927	733.277


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012121\
Data File : PL064275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2021 20:55
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 03:12:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012121CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 21 03:09:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

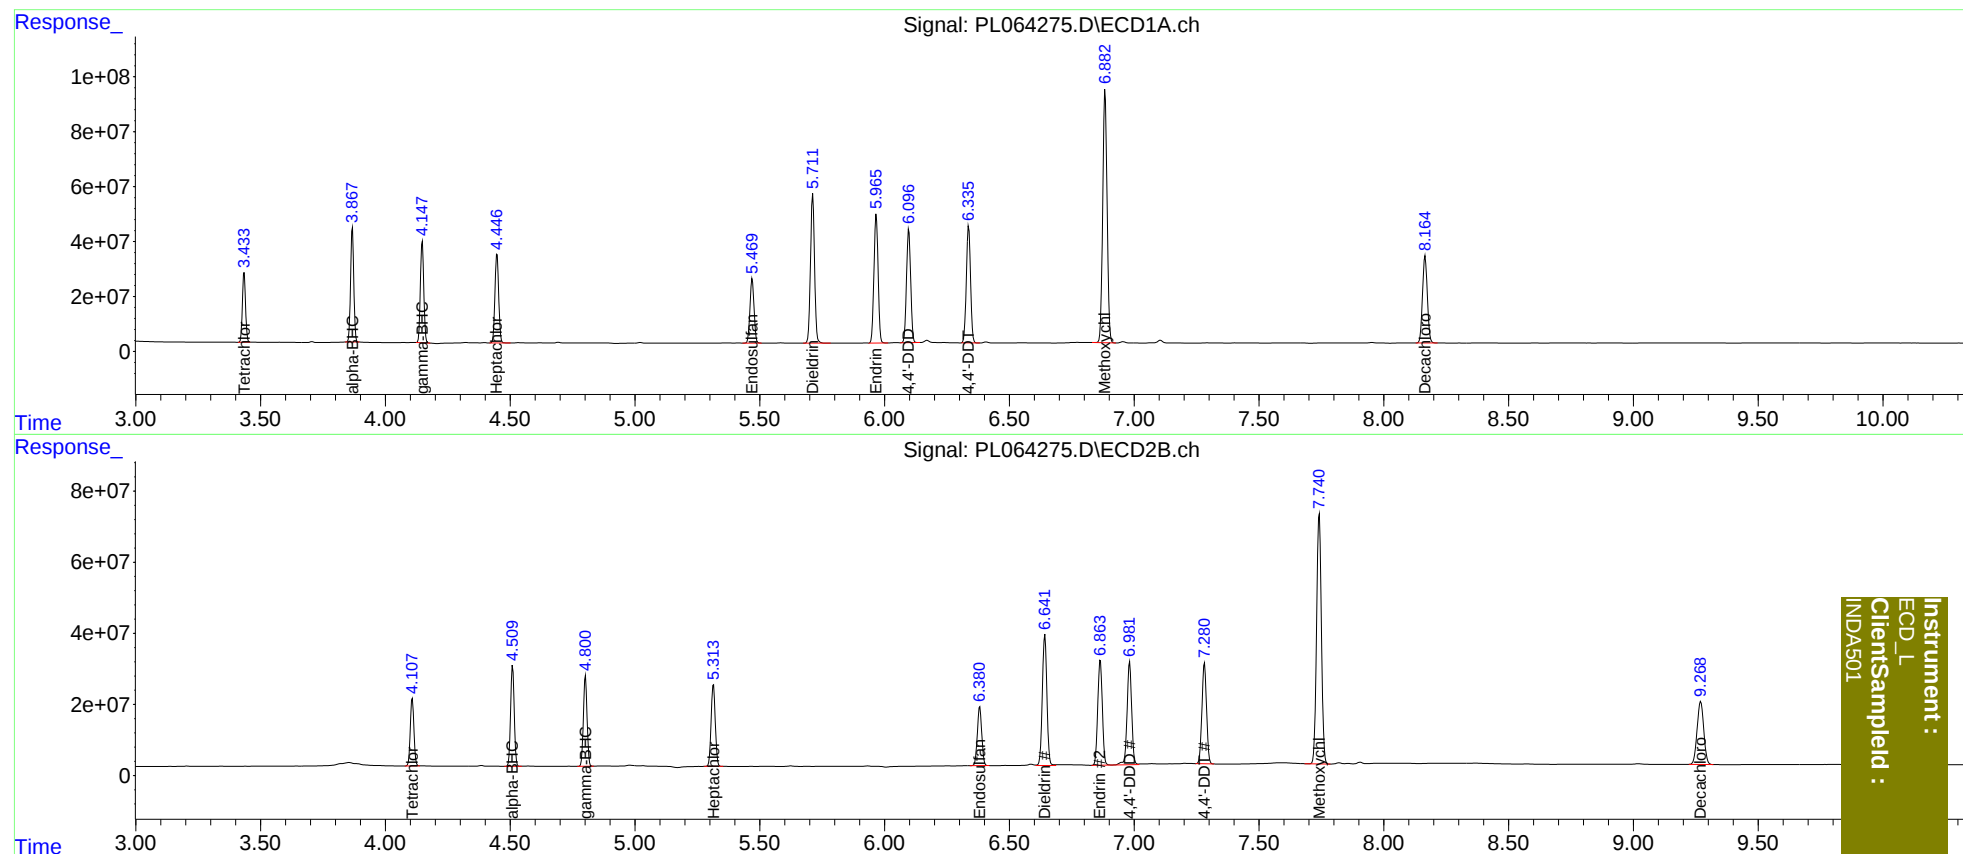


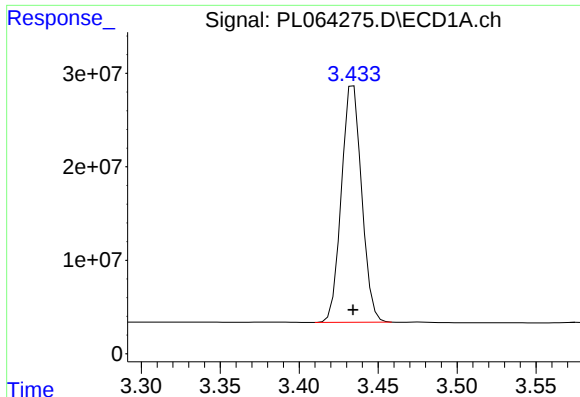

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 226882360
Conc: 77.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

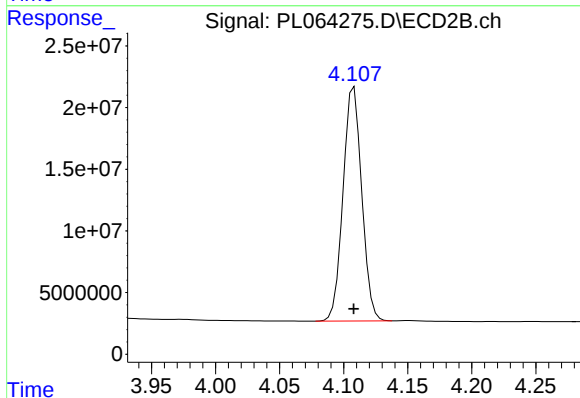


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 192475542
Conc: 79.25 ng/ml

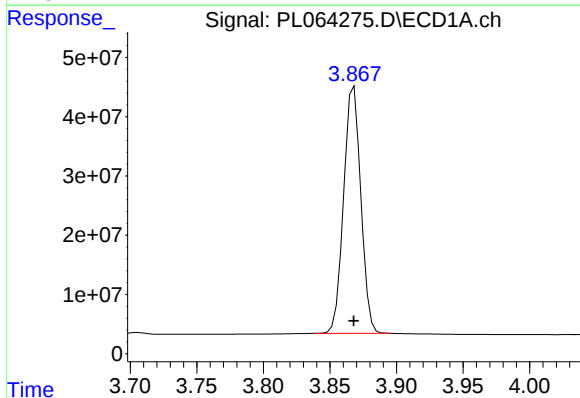


#2 alpha-BHC

R.T.: 3.868 min
Delta R.T.: 0.000 min
Response: 374860863
Conc: 83.75 ng/ml

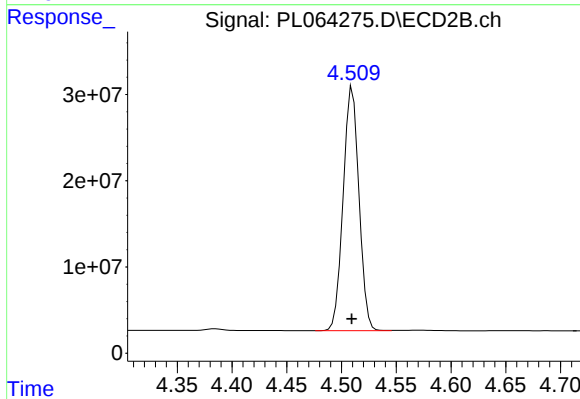

#2 alpha-BHC


R.T.: 4.510 min
Delta R.T.: 0.000 min
Response: 284356344
Conc: 89.64 ng/ml

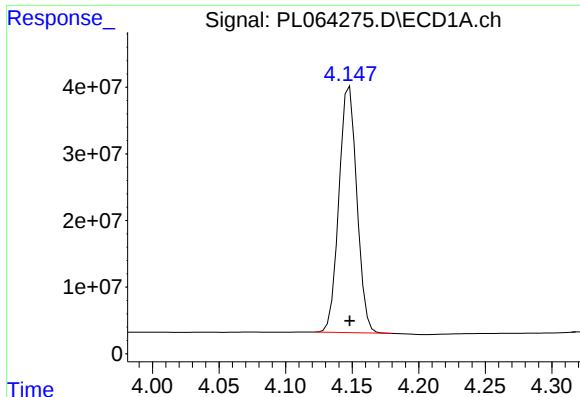

#3 gamma-BHC (Lindane)


R.T.: 4.148 min
Delta R.T.: 0.000 min
Response: 346193728
Conc: 80.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

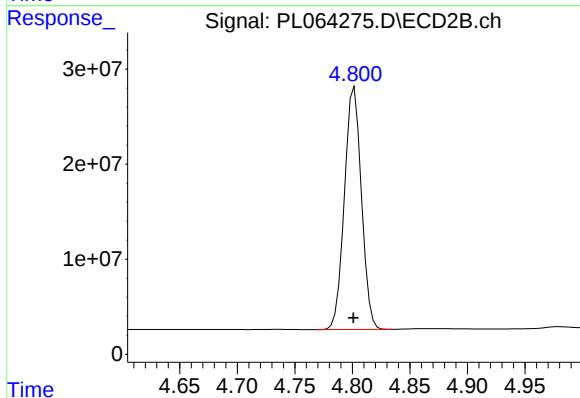


#3 gamma-BHC (Lindane)

R.T.: 4.802 min
Delta R.T.: 0.000 min
Response: 263468291
Conc: 86.31 ng/ml

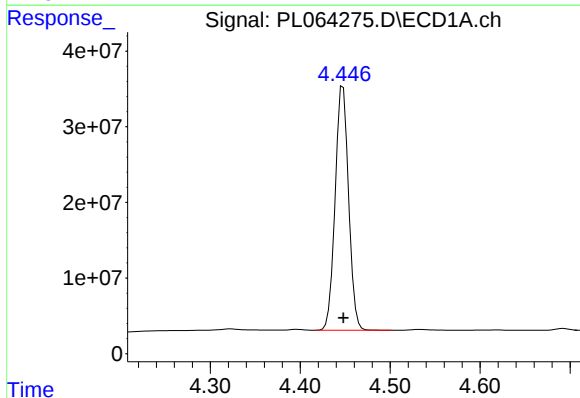


#4 Heptachlor

R.T.: 4.448 min
Delta R.T.: 0.000 min
Response: 335387606
Conc: 78.39 ng/ml

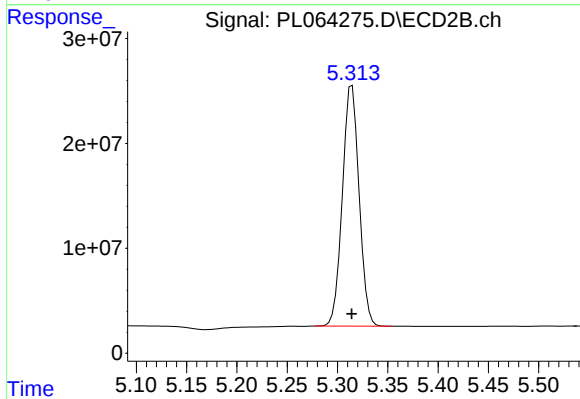

#4 Heptachlor


R.T.: 5.315 min
Delta R.T.: 0.000 min
Response: 264724188
Conc: 81.07 ng/ml

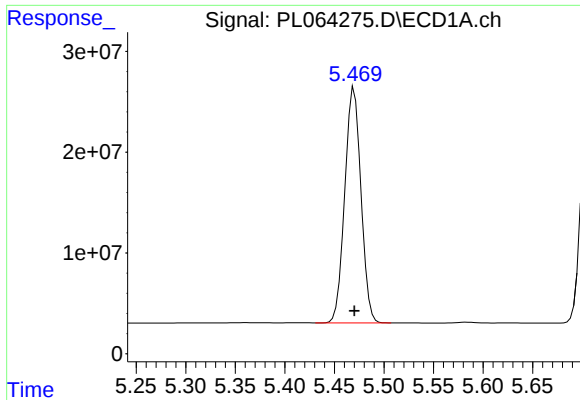

#9 Endosulfan I


R.T.: 5.470 min
Delta R.T.: 0.000 min
Response: 265502749
Conc: 76.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

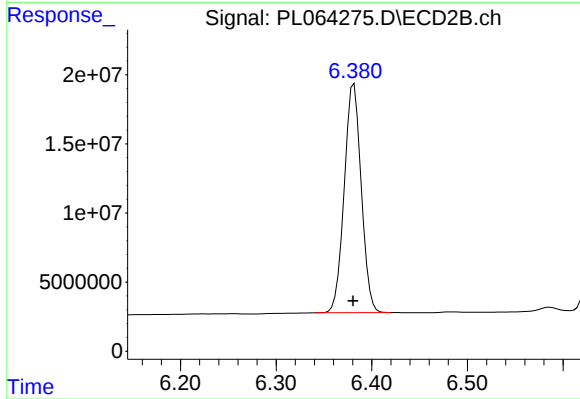


#9 Endosulfan I

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 205122344
Conc: 78.55 ng/ml

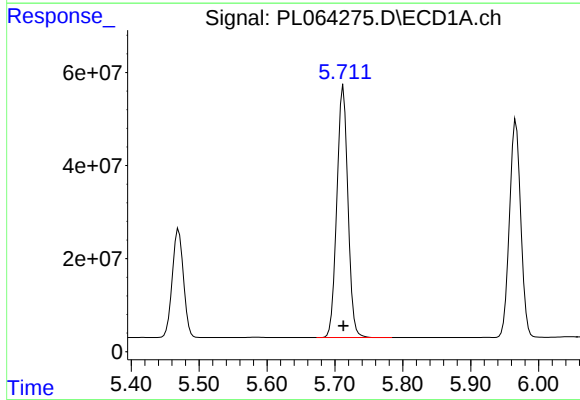


#13 Dieldrin

R.T.: 5.712 min
Delta R.T.: 0.000 min
Response: 613635842
Conc: 158.21 ng/ml

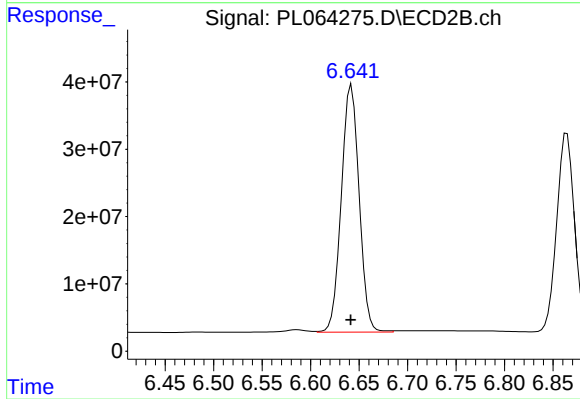

#13 Dieldrin


R.T.: 6.642 min
Delta R.T.: 0.000 min
Response: 469789690
Conc: 167.64 ng/ml

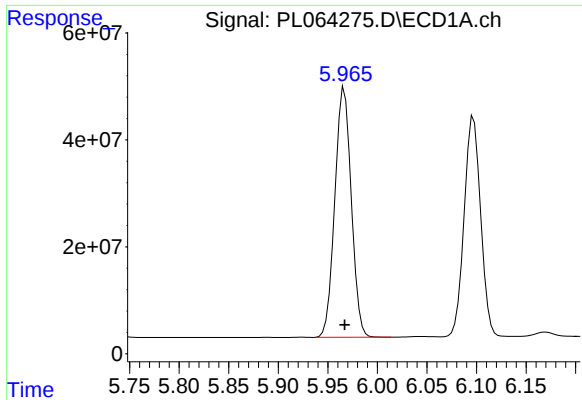

#14 Endrin


R.T.: 5.967 min
Delta R.T.: 0.000 min
Response: 538883797
Conc: 154.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

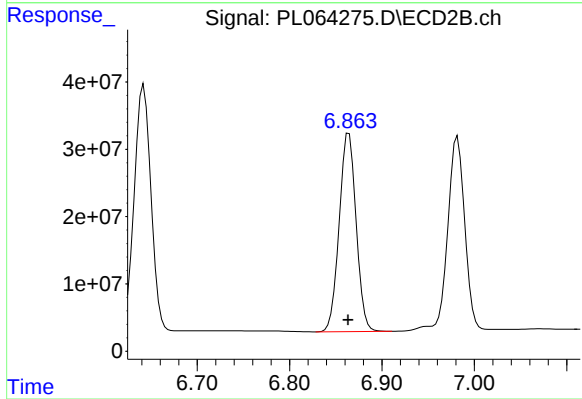


#14 Endrin

R.T.: 6.864 min
Delta R.T.: 0.001 min
Response: 375971220
Conc: 161.69 ng/ml

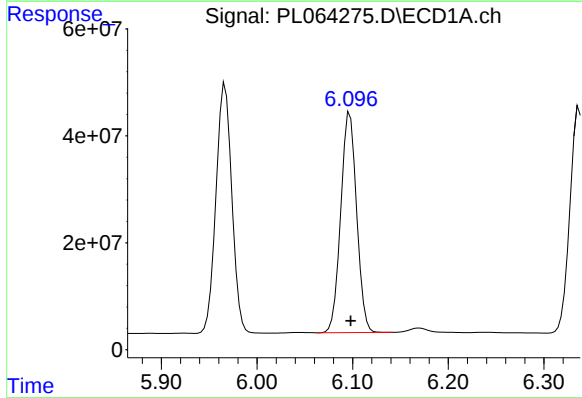


#16 4,4'-DDD

R.T.: 6.097 min
Delta R.T.: -0.001 min
Response: 476516348
Conc: 160.00 ng/ml

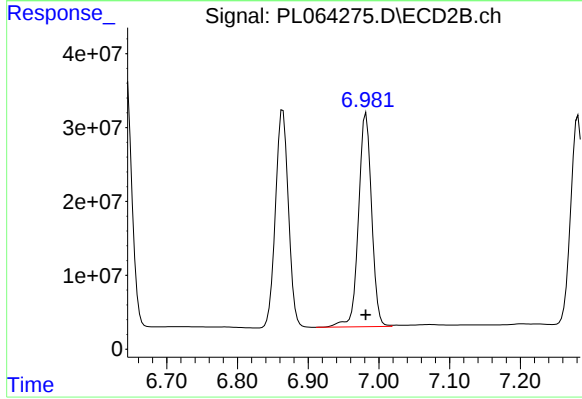

#16 4,4'-DDD


R.T.: 6.982 min
Delta R.T.: 0.000 min
Response: 372489334
Conc: 167.53 ng/ml

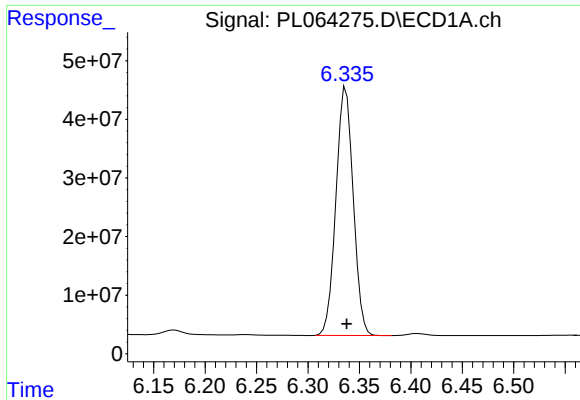

#17 4,4'-DDT


R.T.: 6.337 min
Delta R.T.: 0.000 min
Response: 495660989
Conc: 162.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

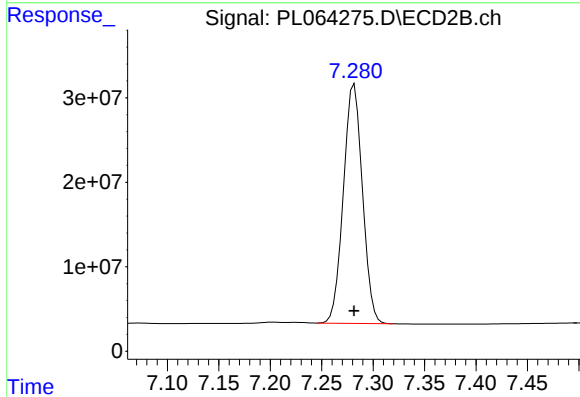


#17 4,4'-DDT

R.T.: 7.282 min
Delta R.T.: 0.000 min
Response: 365528787
Conc: 168.16 ng/ml

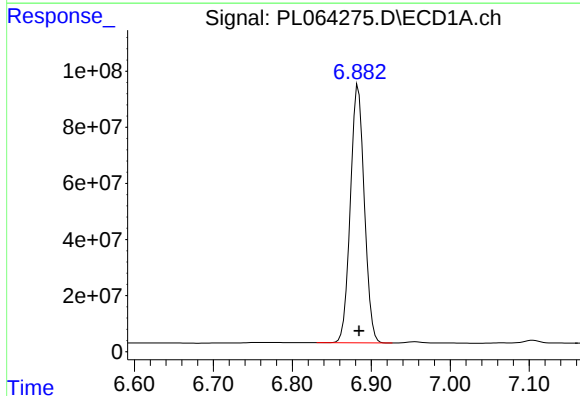


#20 Methoxychlor

R.T.: 6.884 min
Delta R.T.: -0.001 min
Response: 1130016588
Conc: 691.93 ng/ml

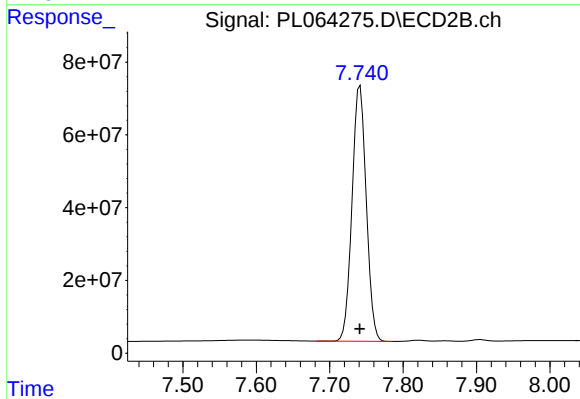

#20 Methoxychlor


R.T.: 7.741 min
Delta R.T.: 0.000 min
Response: 944565851
Conc: 733.28 ng/ml

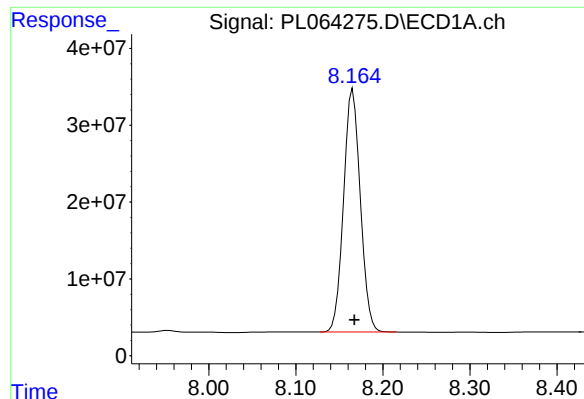

#27 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: -0.002 min
Response: 422600911
Conc: 139.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

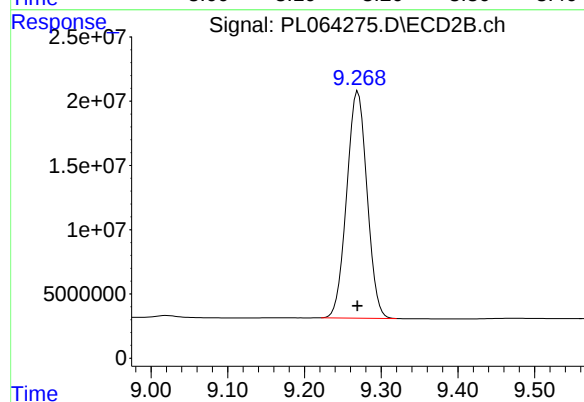

#27 Decachlorobiphenyl

R.T.: 9.270 min
Delta R.T.: 0.000 min
Response: 326811142
Conc: 138.88 ng/ml