

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012122\
 Data File : PL072158.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2022 12:09
 Operator : AR\AJ
 Sample : PB142173BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 01:57:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.491	9847927	28882340	17.738	17.783
28)	SA Decachlor...	10.316	11.382	16571192	30280388	18.652	18.767
Target Compounds							
3)	MA gamma-BHC...	0.000	6.499f	0	118936	N.D.	0.053 #
7)	B delta-BHC	0.000	7.015f	0	2742904	N.D.	1.115 #
9)	A Endosulfan I	0.000	8.374	0	9711	N.D.	0.005 #
10)	B gamma-Chl...	0.000	8.223	0	340408	N.D.	0.168 #
11)	B alpha-Chl...	0.000	8.332f	0	85860	N.D.	0.043 #
15)	B Endosulfa...	0.000	9.146f	0	440113	N.D.	0.257 #
16)	A 4,4'-DDD	0.000	9.046	0	643947	N.D.	0.450 #
17)	MA 4,4'-DDT	0.000	9.347	0	64960	N.D.	0.041 #
20)	A Methoxychlor	0.000	9.845	0	16222	N.D.	0.020 #
22)	Mirex	0.000	10.489f	0	311095	N.D.	0.249 #
25)	Chlordane-3	0.000	8.223	0	340408	N.D.	1.225 #
26)	Chlordane-4	0.000	8.332f	0	85860	N.D.	0.259 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012122\
Data File : PL072158.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2022 12:09
Operator : AR\AJ
Sample : PB142173BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 01:57:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

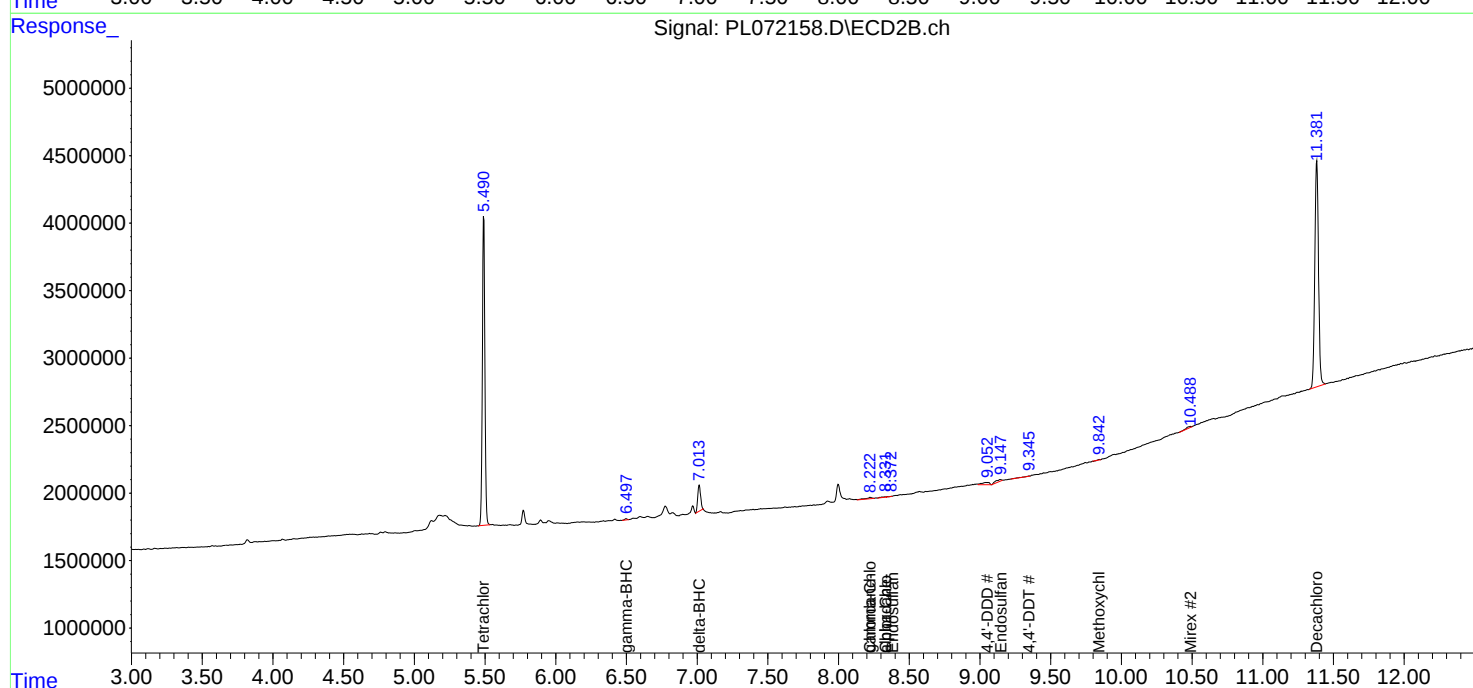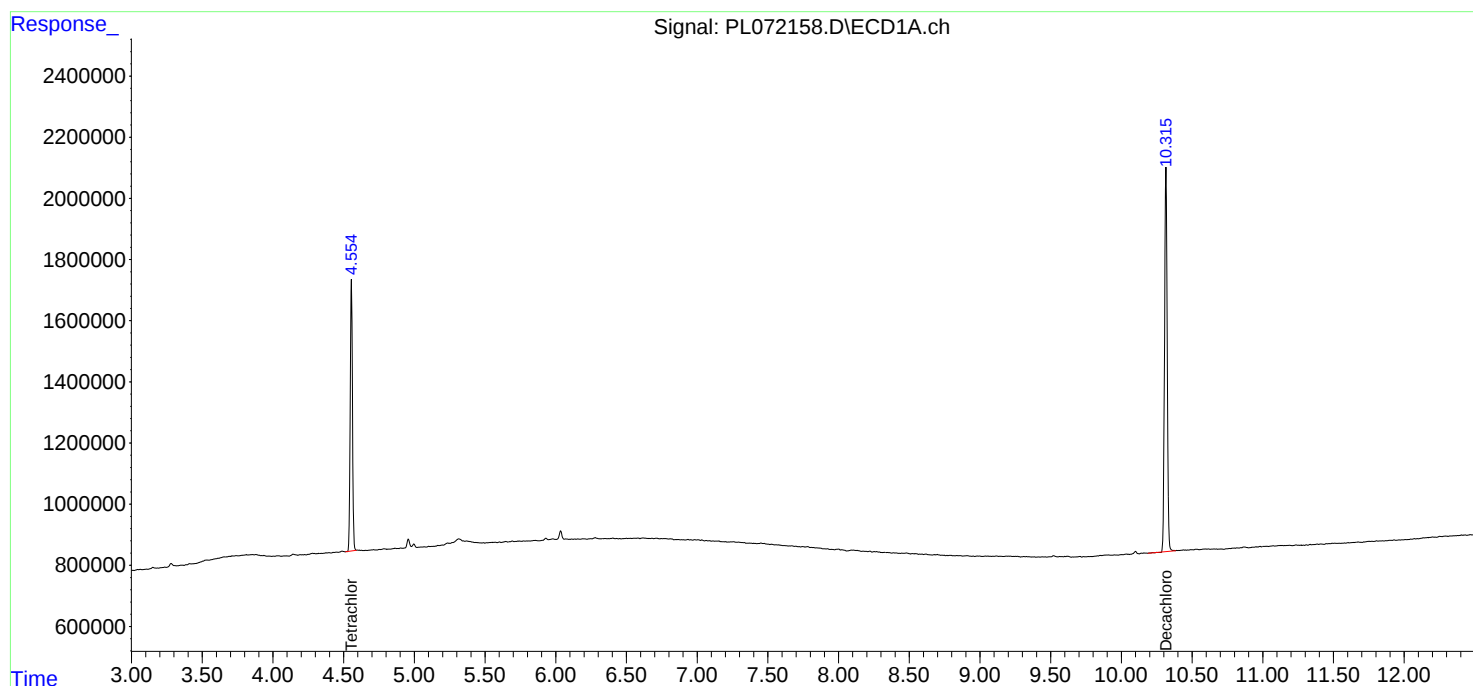


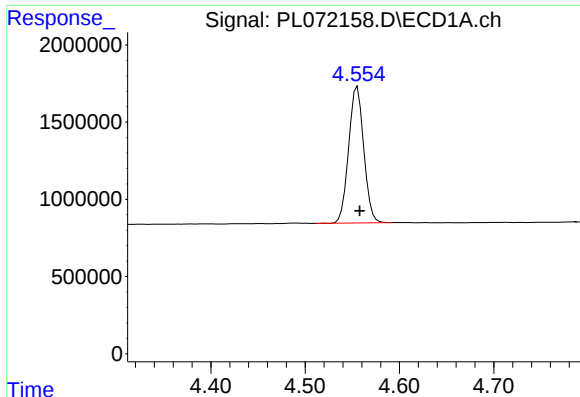

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 9847927
Conc: 17.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

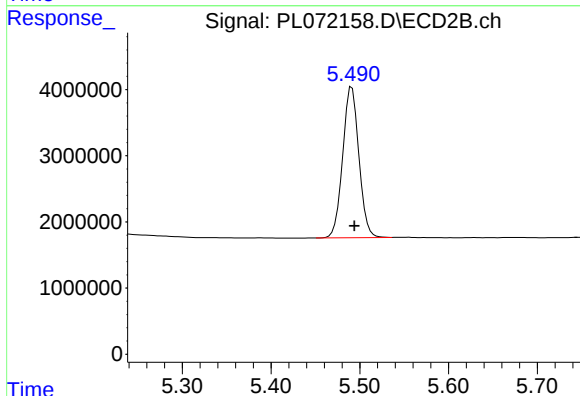


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 28882340
Conc: 17.78 ng/ml

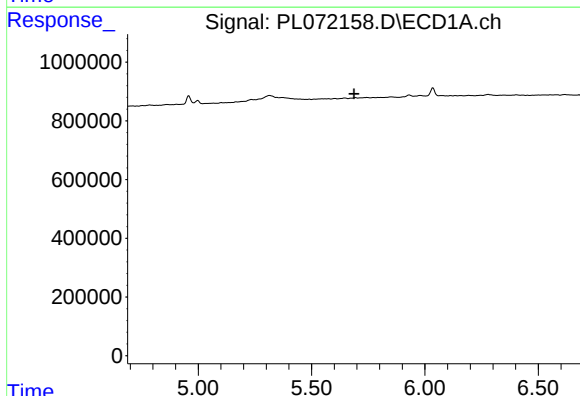


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.688 min
Response: 0
Conc: N.D.

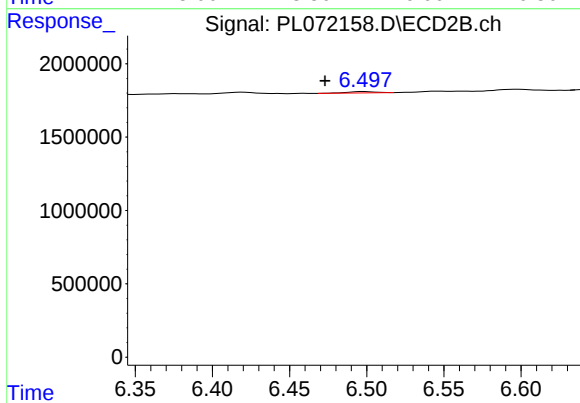

#3 gamma-BHC (Lindane)


R.T.: 6.499 min
Delta R.T.: 0.026 min
Response: 118936
Conc: 0.05 ng/ml

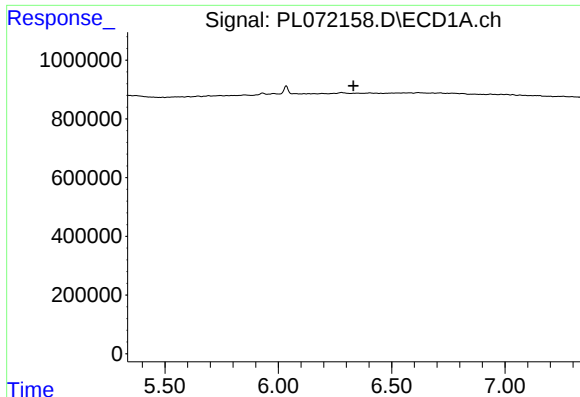

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

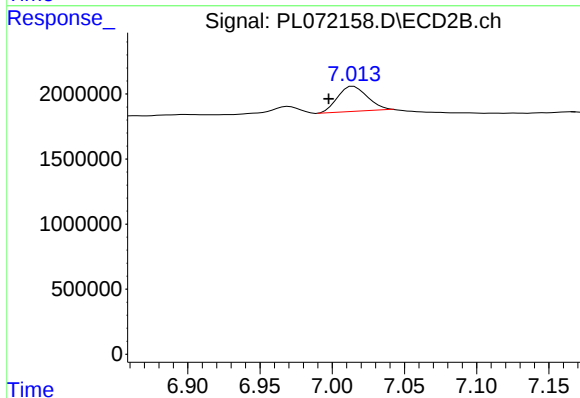


#7 delta-BHC

R.T.: 7.015 min
Delta R.T.: 0.017 min
Response: 2742904
Conc: 1.11 ng/ml

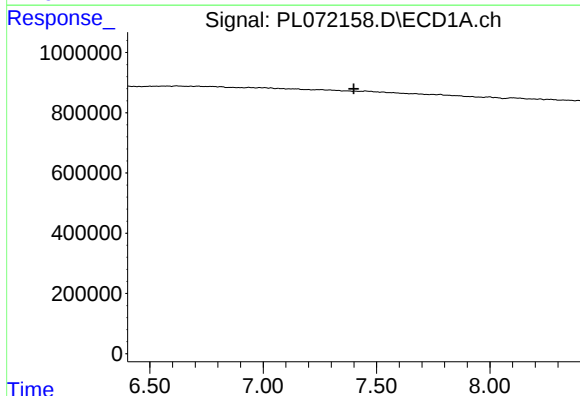


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.400 min
Response: 0
Conc: N.D.

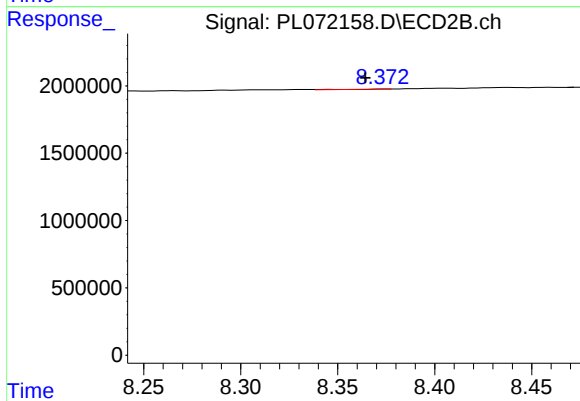

#9 Endosulfan I


R.T.: 8.374 min
Delta R.T.: 0.010 min
Response: 9711
Conc: 0.01 ng/ml

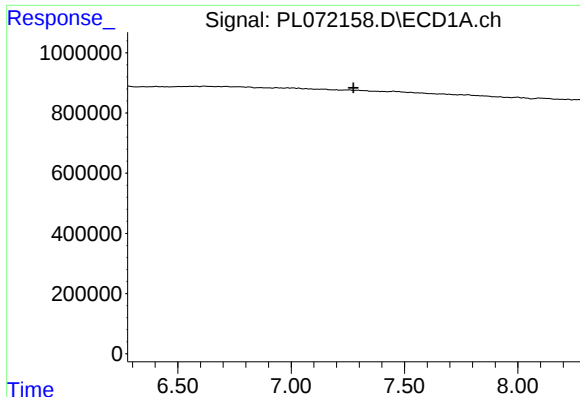

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

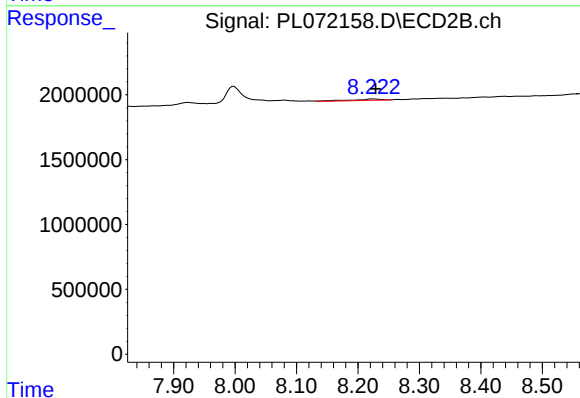


#10 gamma-Chlordane

R.T.: 8.223 min
Delta R.T.: -0.006 min
Response: 340408
Conc: 0.17 ng/ml

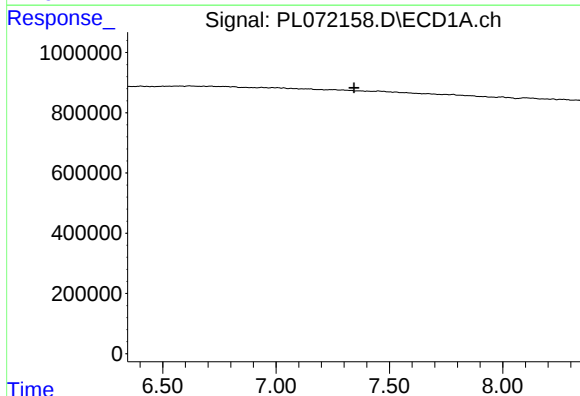


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

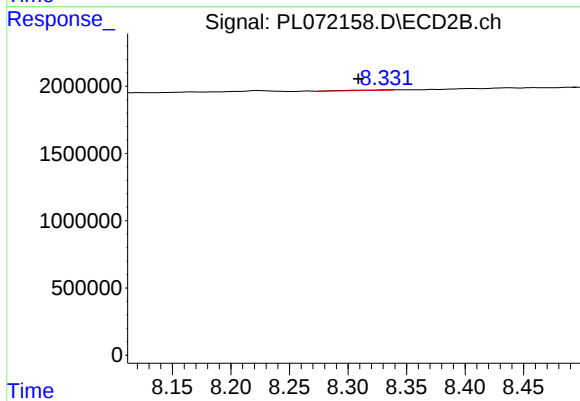

#11 alpha-Chlordane


R.T.: 8.332 min
Delta R.T.: 0.023 min
Response: 85860
Conc: 0.04 ng/ml

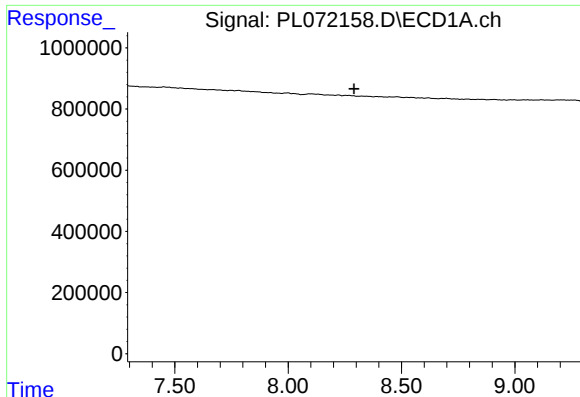

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

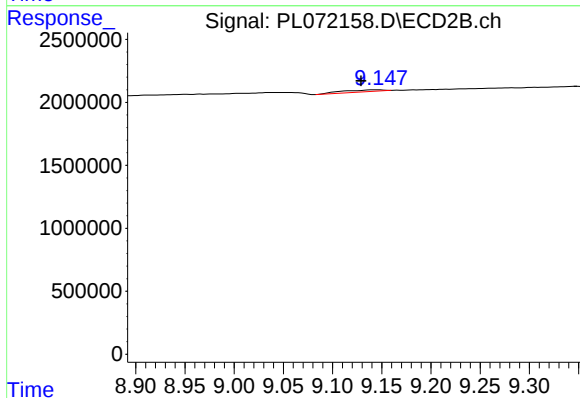


#15 Endosulfan II

R.T.: 9.146 min
Delta R.T.: 0.017 min
Response: 440113
Conc: 0.26 ng/ml

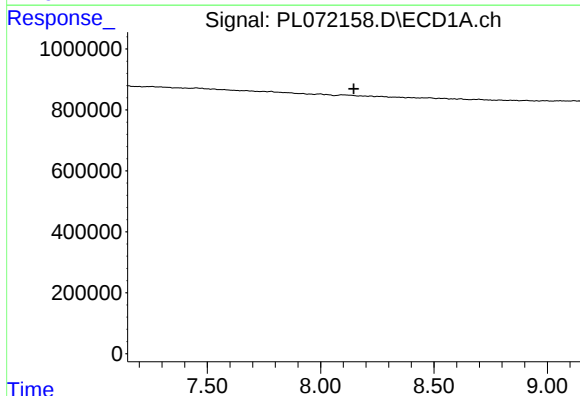


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

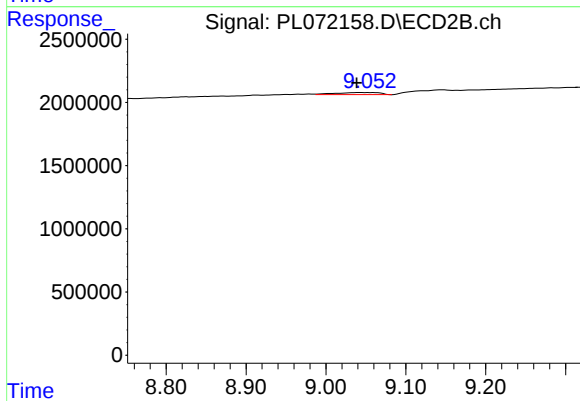

#16 4,4'-DDD


R.T.: 9.046 min
Delta R.T.: 0.008 min
Response: 643947
Conc: 0.45 ng/ml

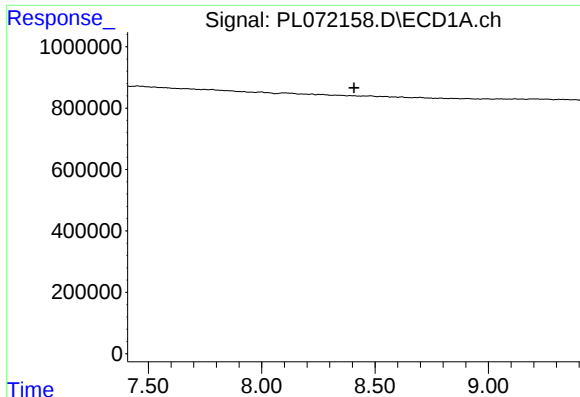

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

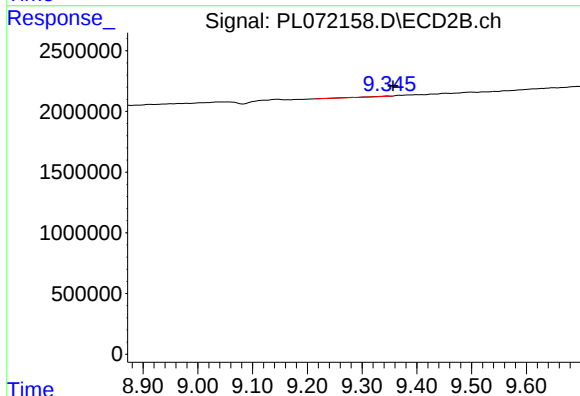


#17 4,4'-DDT

R.T.: 9.347 min
Delta R.T.: -0.010 min
Response: 64960
Conc: 0.04 ng/ml

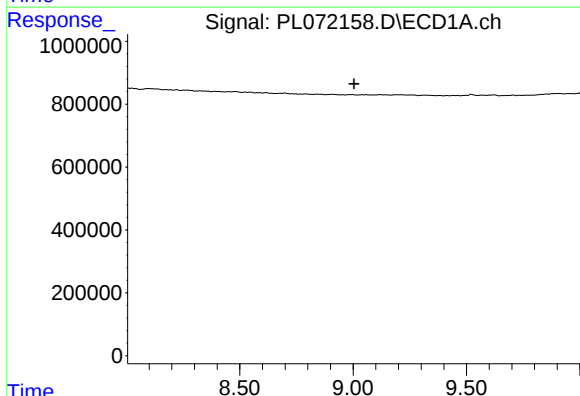


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

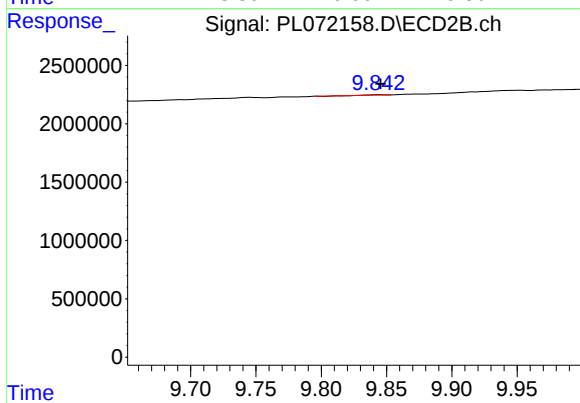

#20 Methoxychlor


R.T.: 9.845 min
Delta R.T.: 0.000 min
Response: 16222
Conc: 0.02 ng/ml

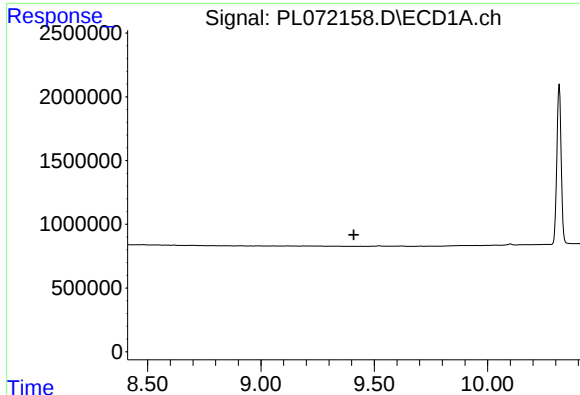

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

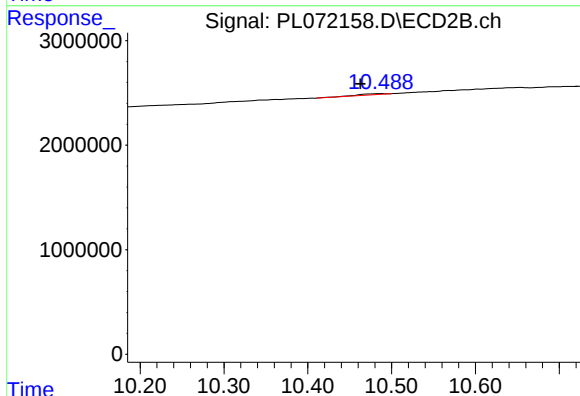


#22 Mirex

R.T.: 10.489 min
Delta R.T.: 0.026 min
Response: 311095
Conc: 0.25 ng/ml

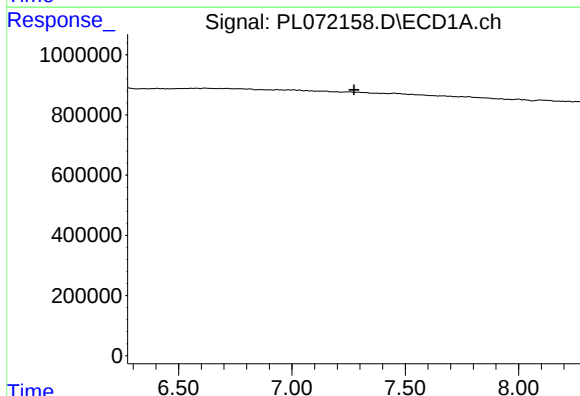


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

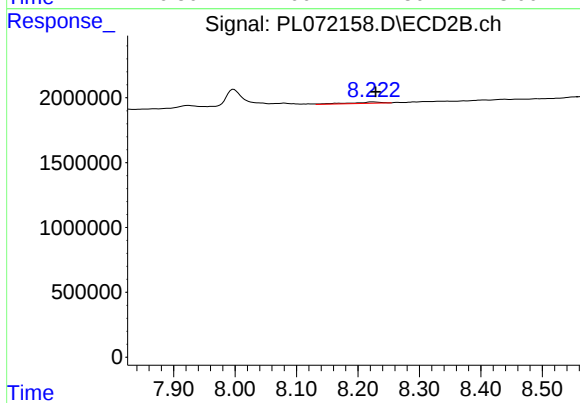

#25 Chlordane-3


R.T.: 8.223 min
Delta R.T.: -0.006 min
Response: 340408
Conc: 1.23 ng/ml

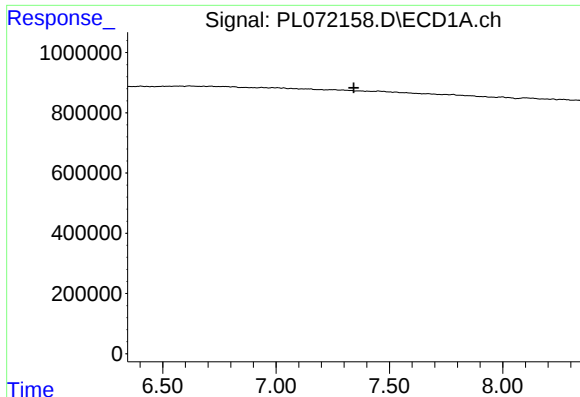

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

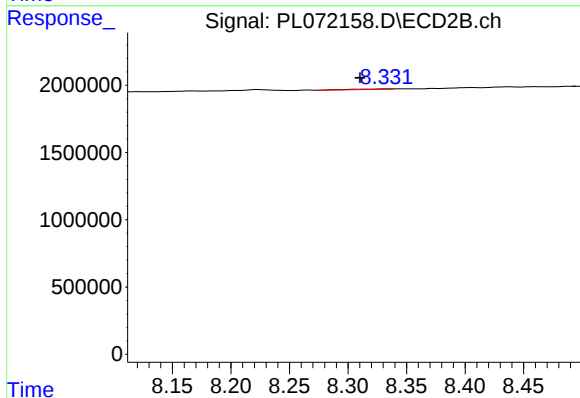


#26 Chlordane-4

R.T.: 8.332 min
Delta R.T.: 0.022 min
Response: 85860
Conc: 0.26 ng/ml

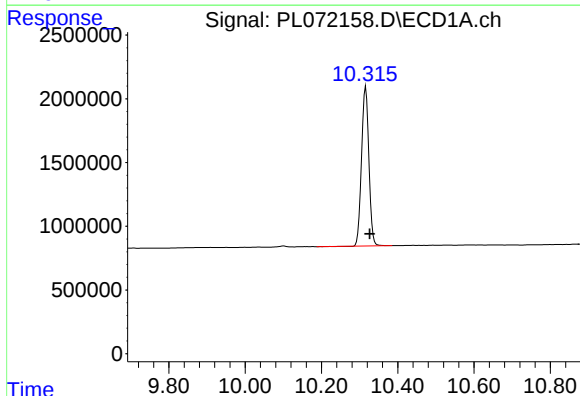

#28 Decachlorobiphenyl

R.T.: 10.316 min
Delta R.T.: -0.010 min
Response: 16571192
Conc: 18.65 ng/ml

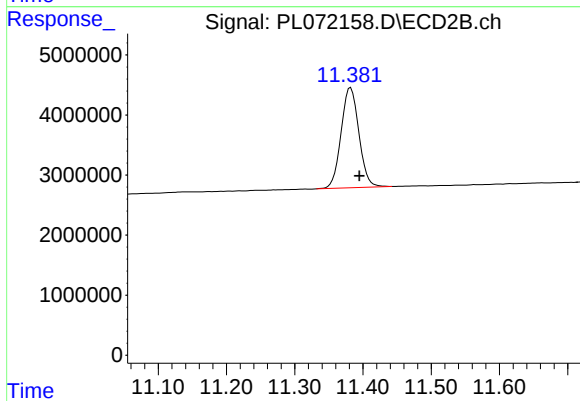

#28 Decachlorobiphenyl

R.T.: 11.382 min
Delta R.T.: -0.013 min
Response: 30280388
Conc: 18.77 ng/ml