

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012122\
 Data File : PL072162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2022 13:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 01:58:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.491	9771500	28085803	17.600	17.293
28)	SA Decachlor...	10.317	11.381	15150740	27547911	17.053	17.073
Target Compounds							
7)	B delta-BHC	0.000	7.017f	0	816194	N.D.	0.332 #
10)	B gamma-Chl...	0.000	8.227	0	70422	N.D.	0.035 #
11)	B alpha-Chl...	0.000	8.324f	0	232186	N.D.	0.117 #
15)	B Endosulfa...	0.000	9.151f	0	506100	N.D.	0.295 #
16)	A 4,4'-DDD	0.000	9.024	0	1125318	N.D.	0.787 #
17)	MA 4,4'-DDT	0.000	9.384f	0	1074240	N.D.	0.680 #
19)	B Endosulfa...	8.718	0.000	275478	0	0.376	N.D. #
21)	B Endrin ke...	0.000	10.004	0	1777036	N.D.	1.074 #
25)	Chlordane-3	0.000	8.227	0	70422	N.D.	0.253 #
26)	Chlordane-4	0.000	8.324	0	232186	N.D.	0.699 #
27)	Chlordane-5	0.000	9.181f	0	238625	N.D.	3.911 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012122\
Data File : PL072162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2022 13:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 01:58:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

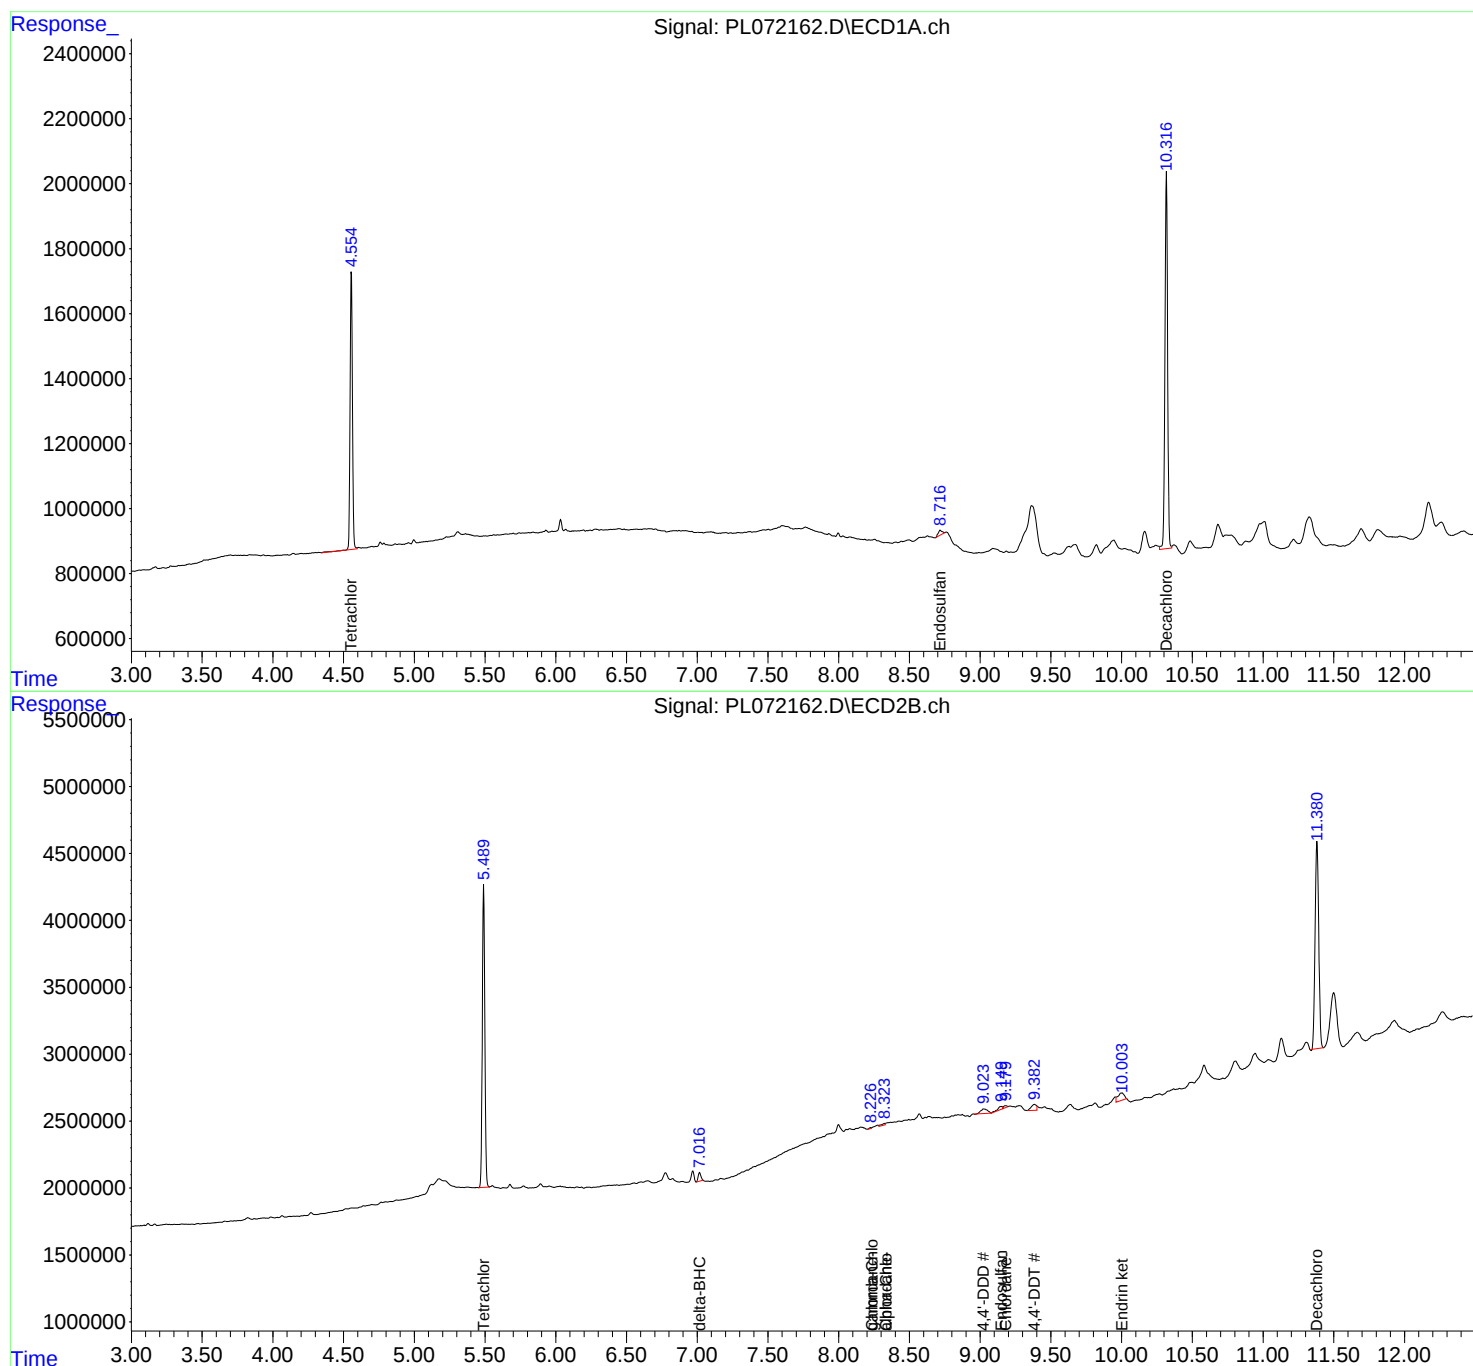


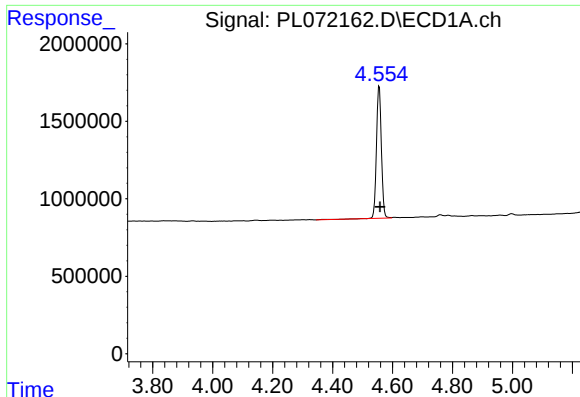

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 9771500
Conc: 17.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

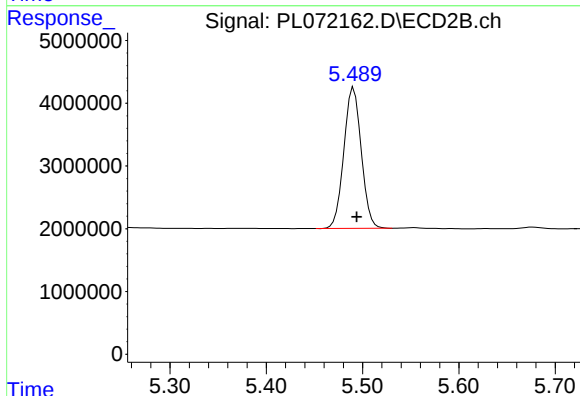


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 28085803
Conc: 17.29 ng/ml

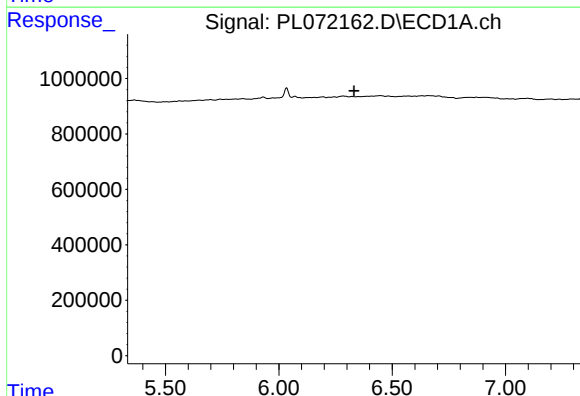


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

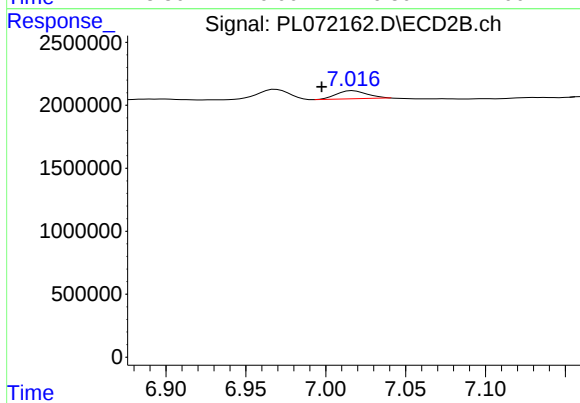

#7 delta-BHC


R.T.: 7.017 min
Delta R.T.: 0.019 min
Response: 816194
Conc: 0.33 ng/ml

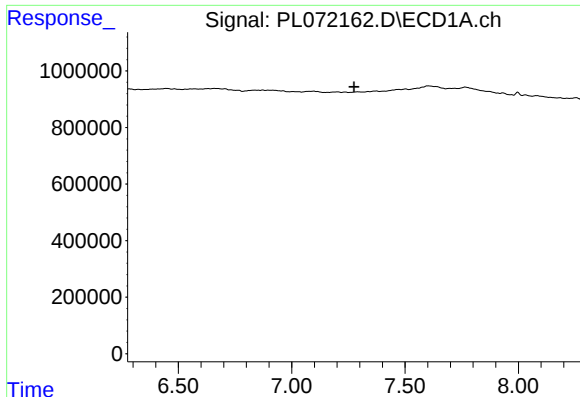

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

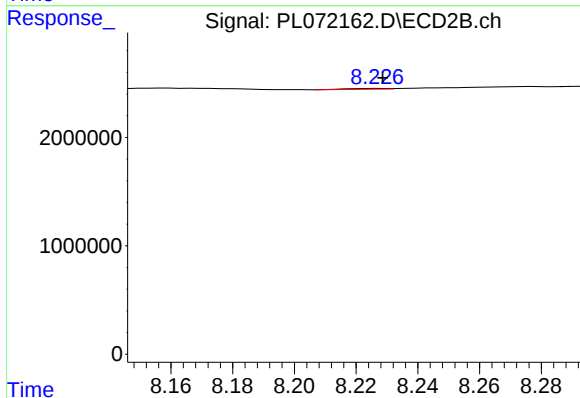


#10 gamma-Chlordane

R.T.: 8.227 min
Delta R.T.: -0.001 min
Response: 70422
Conc: 0.03 ng/ml

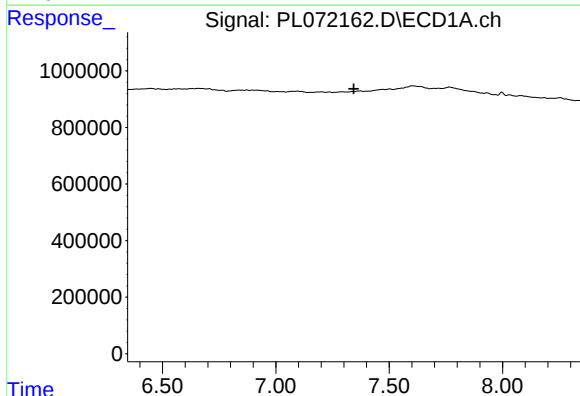


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

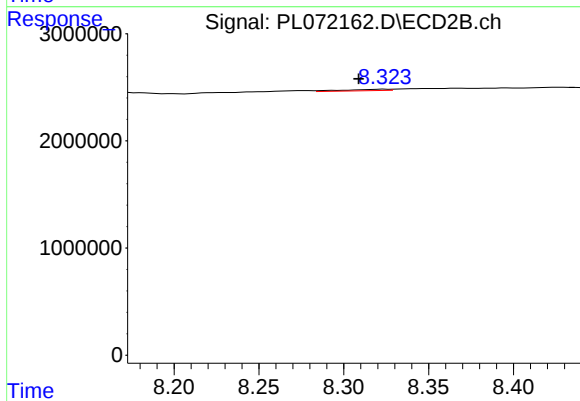

#11 alpha-Chlordane


R.T.: 8.324 min
Delta R.T.: 0.015 min
Response: 232186
Conc: 0.12 ng/ml

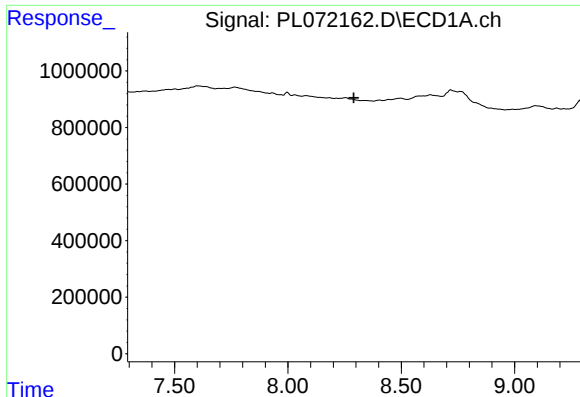

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

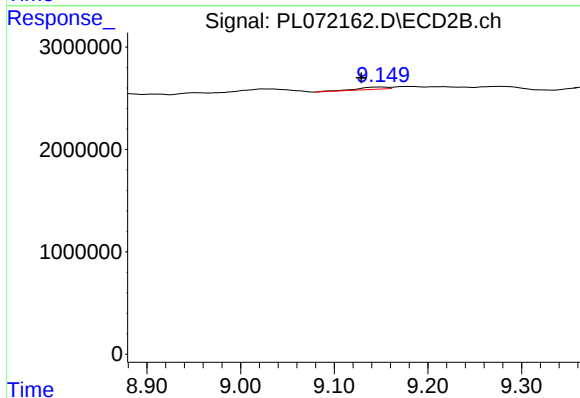


#15 Endosulfan II

R.T.: 9.151 min
Delta R.T.: 0.021 min
Response: 506100
Conc: 0.30 ng/ml

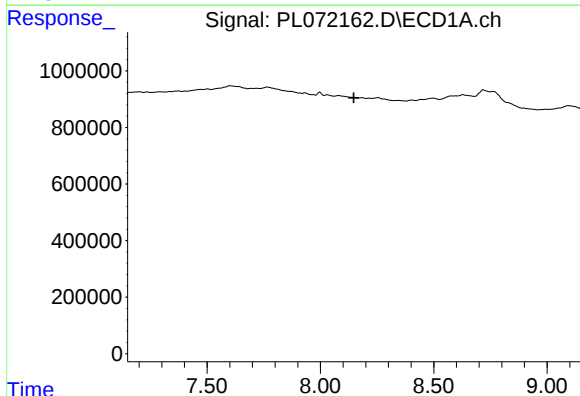


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

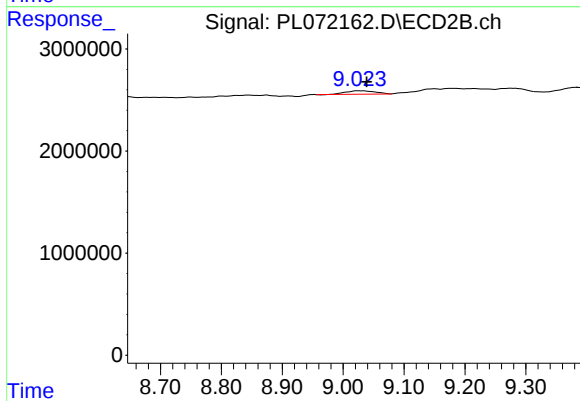

#16 4,4'-DDD


R.T.: 9.024 min
Delta R.T.: -0.014 min
Response: 1125318
Conc: 0.79 ng/ml

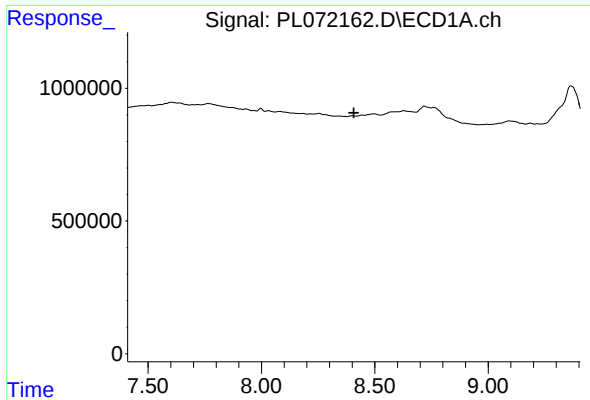

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

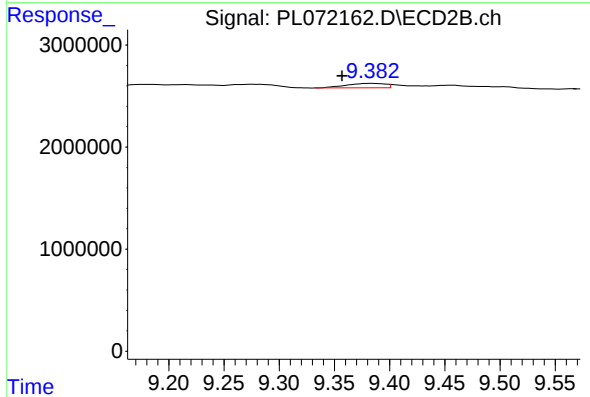


#17 4,4'-DDT

R.T.: 9.384 min
Delta R.T.: 0.027 min
Response: 1074240
Conc: 0.68 ng/ml

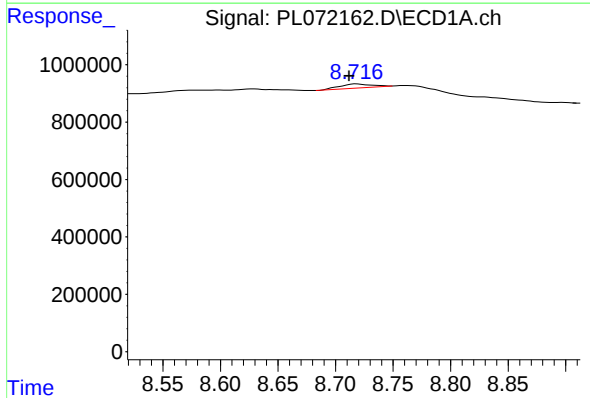


#19 Endosulfan Sulfate

R.T.: 8.718 min
Delta R.T.: 0.006 min
Response: 275478
Conc: 0.38 ng/ml

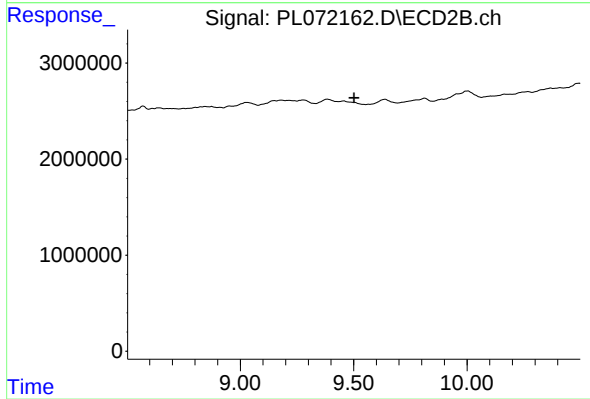

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.502 min
Response: 0
Conc: N.D.

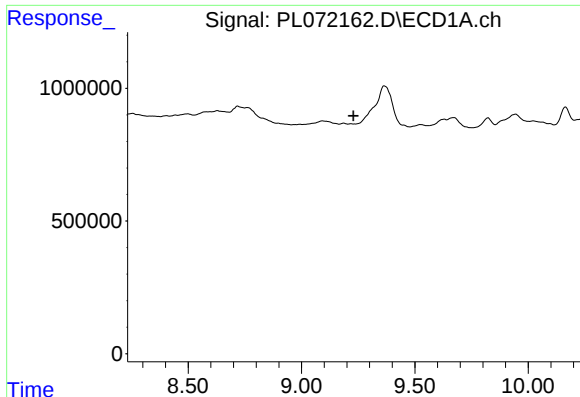

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.229 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

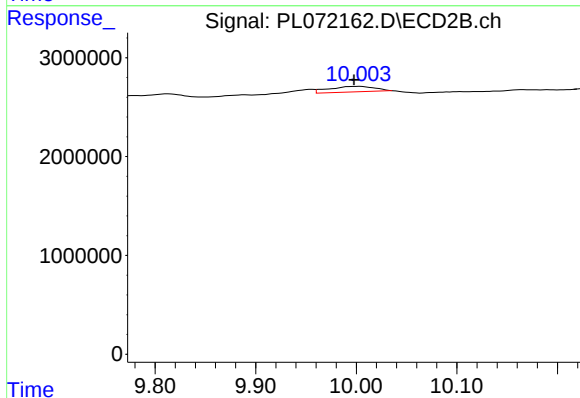


#21 Endrin ketone

R.T.: 10.004 min
Delta R.T.: 0.006 min
Response: 1777036
Conc: 1.07 ng/ml

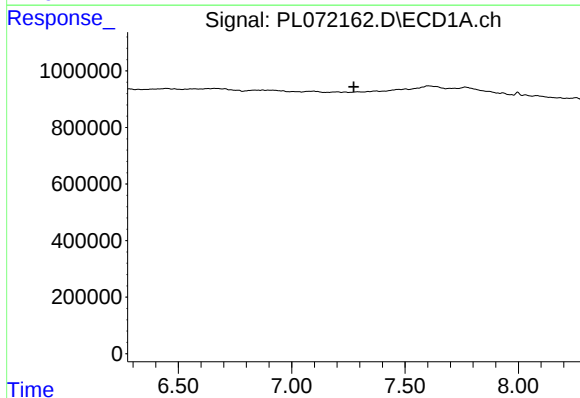


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

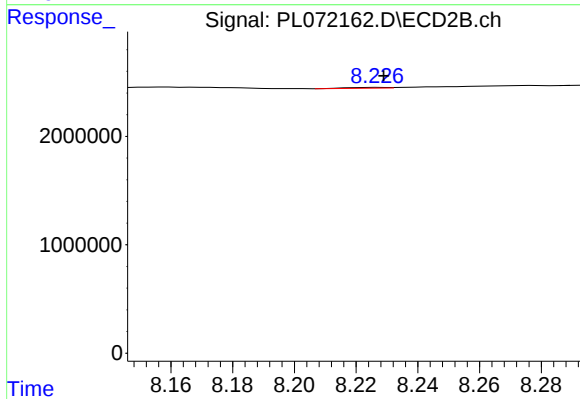

#25 Chlordane-3

R.T.: 8.227 min
Delta R.T.: -0.002 min
Response: 70422
Conc: 0.25 ng/ml

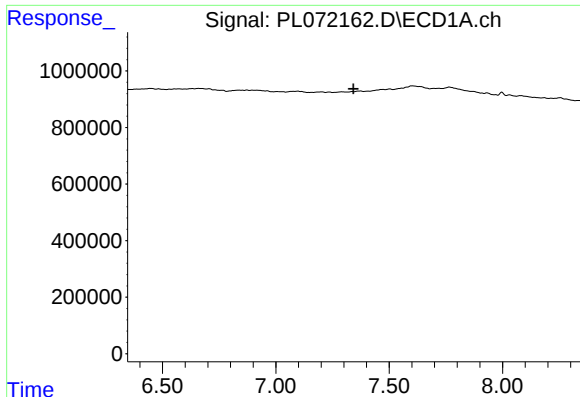

#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#26 Chlordane-4


R.T.: 8.324 min
Delta R.T.: 0.014 min
Response: 232186
Conc: 0.70 ng/ml

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

#27 Chlordane-5


R.T.: 9.181 min
Delta R.T.: -0.018 min
Response: 238625
Conc: 3.91 ng/ml

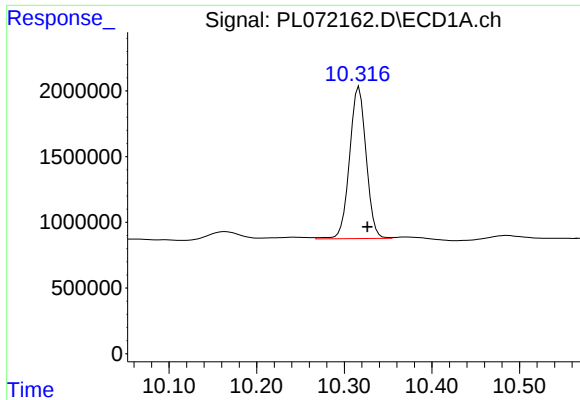

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: -0.010 min
Response: 15150740
Conc: 17.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

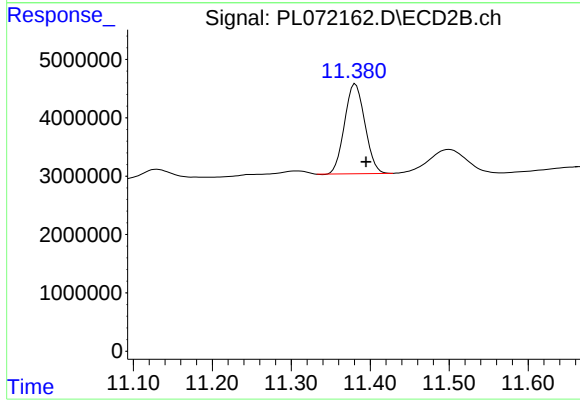

#28 Decachlorobiphenyl

R.T.: 11.381 min
Delta R.T.: -0.014 min
Response: 27547911
Conc: 17.07 ng/ml