

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012122\
 Data File : PL072167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2022 14:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 02:00:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.491	9823070	28821374	17.693	17.746
28)	SA Decachlor...	10.316	11.382	14997462	27899268	16.881	17.291
Target Compounds							
5)	MB Aldrin	0.000	7.508f	0	96443	N.D.	0.044 #
7)	B delta-BHC	0.000	7.017f	0	509541	N.D.	0.207 #
10)	B gamma-Chl...	0.000	8.247f	0	306754	N.D.	0.152 #
11)	B alpha-Chl...	0.000	8.316	0	88162	N.D.	0.044 #
14)	MA Endrin	7.996f	0.000	176677	0	0.252	N.D. #
16)	A 4,4'-DDD	0.000	9.068f	0	259156	N.D.	0.181 #
22)	Mirex	0.000	10.479f	0	341399	N.D.	0.274 #
25)	Chlordane-3	0.000	8.247f	0	306754	N.D.	1.104 #
26)	Chlordane-4	0.000	8.316	0	88162	N.D.	0.265 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012122\
Data File : PL072167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2022 14:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 02:00:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

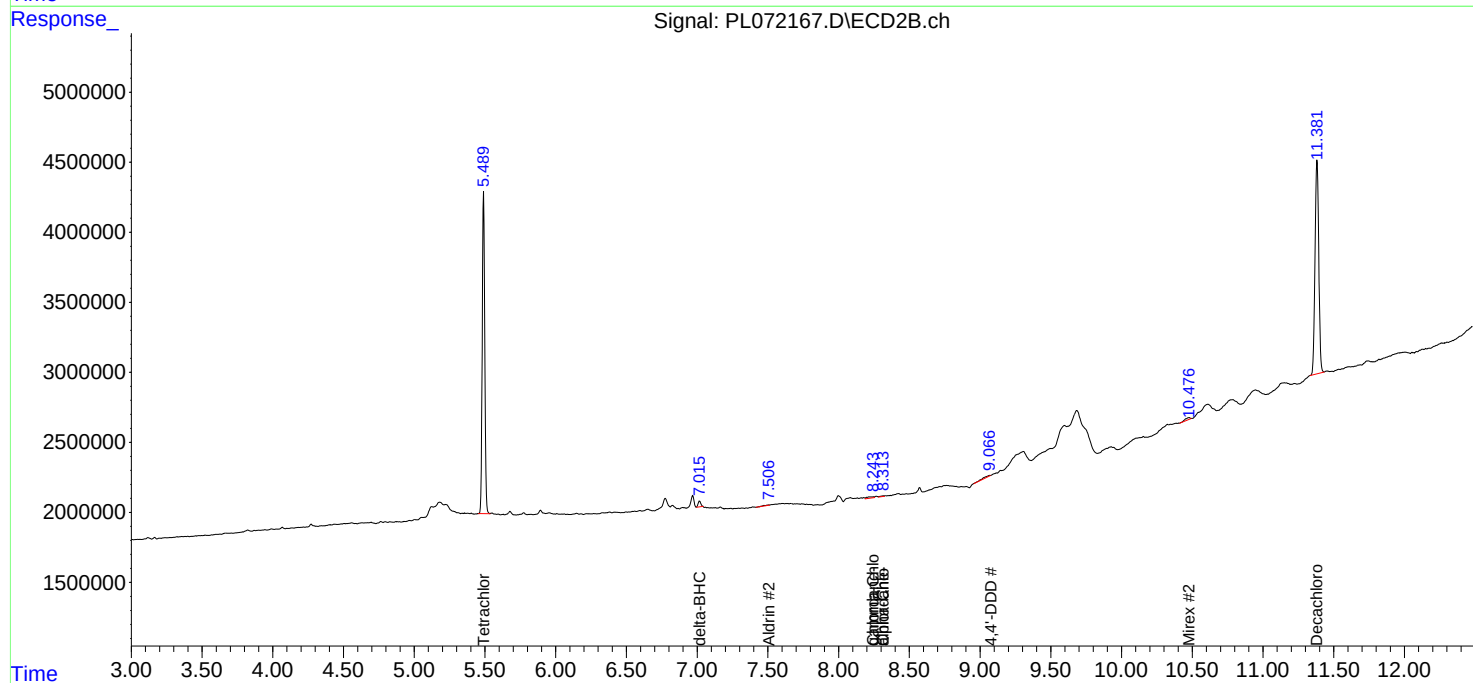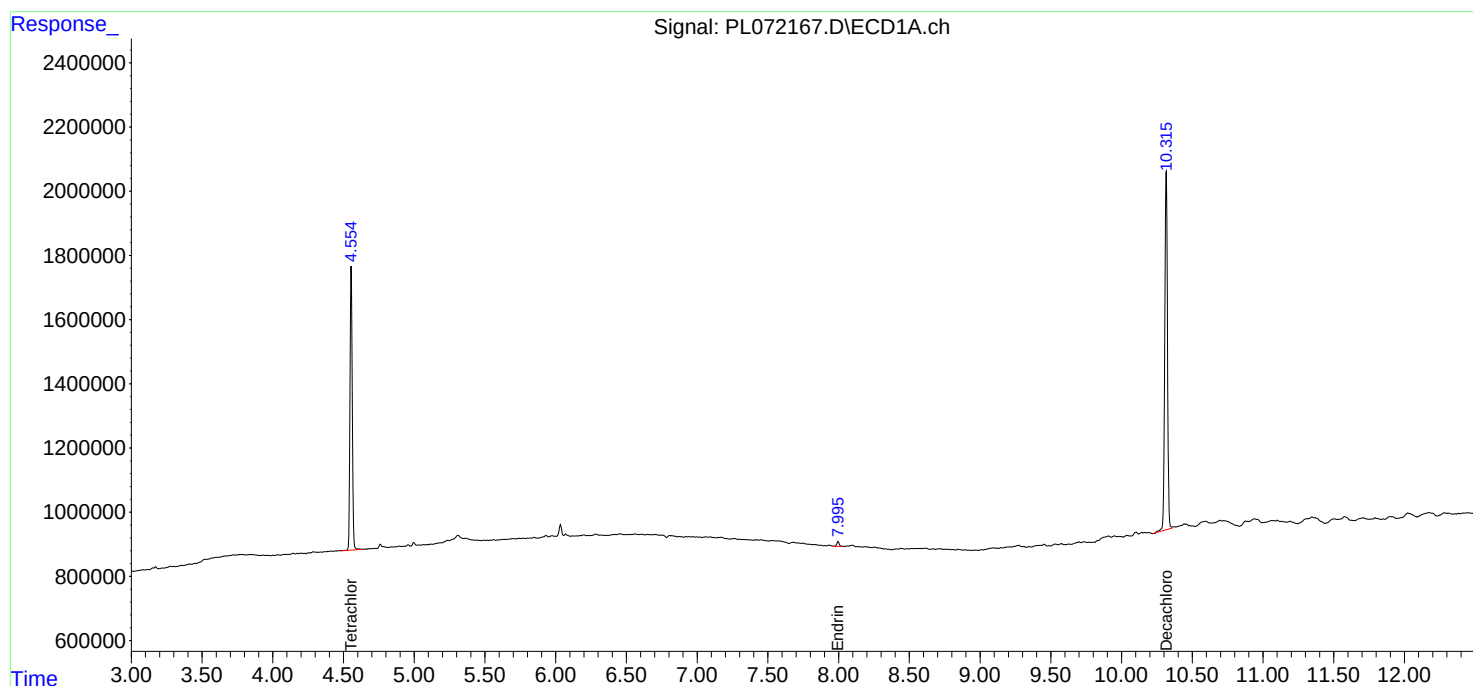


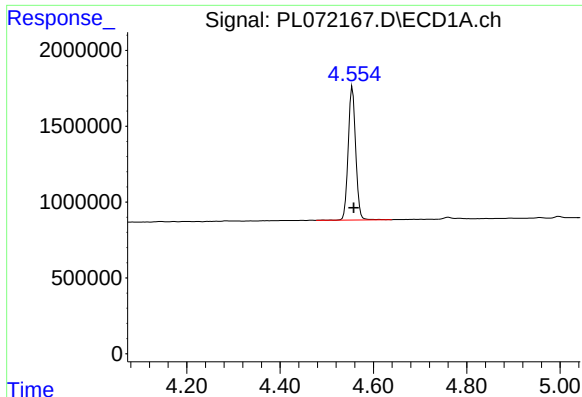

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 9823070
Conc: 17.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

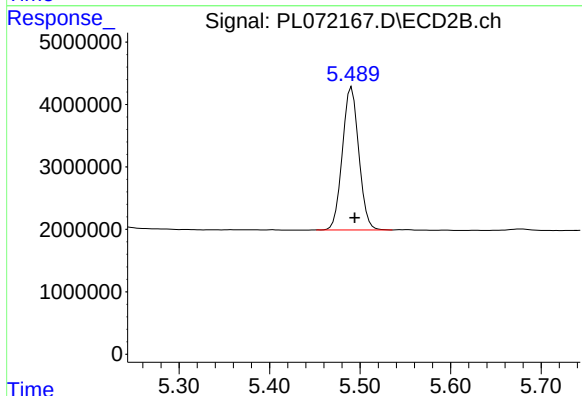


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 28821374
Conc: 17.75 ng/ml

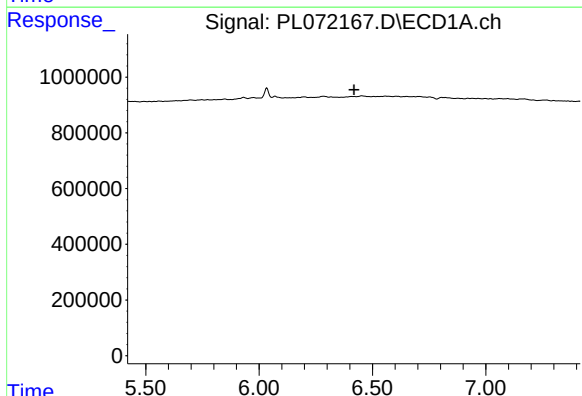


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.419 min
Response: 0
Conc: N.D.

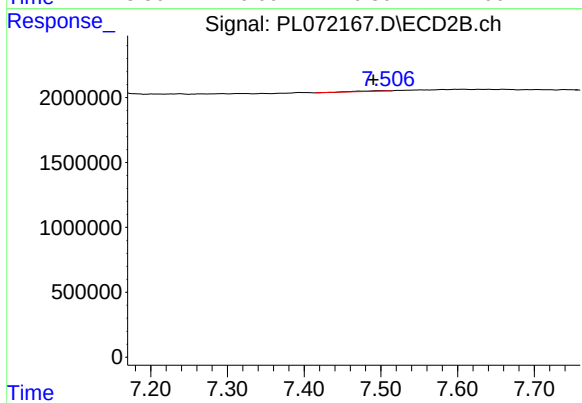

#5 Aldrin


R.T.: 7.508 min
Delta R.T.: 0.017 min
Response: 96443
Conc: 0.04 ng/ml

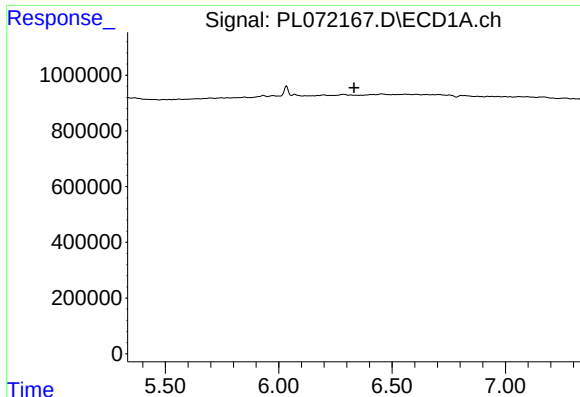

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

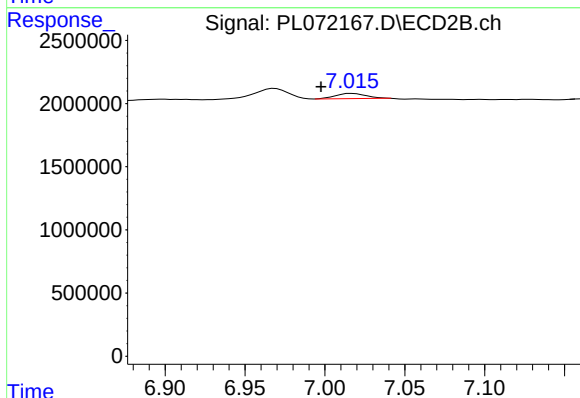


#7 delta-BHC

R.T.: 7.017 min
Delta R.T.: 0.019 min
Response: 509541
Conc: 0.21 ng/ml

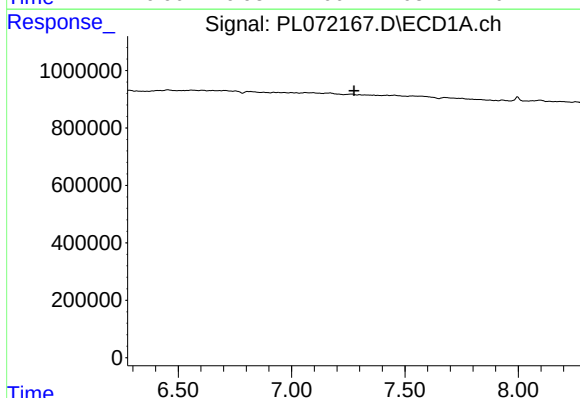


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.275 min
Response: 0
Conc: N.D.

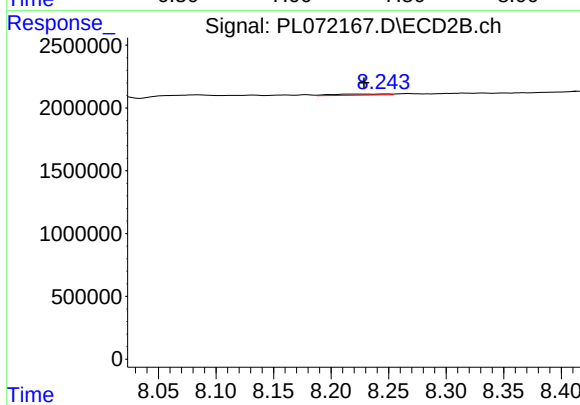

#10 gamma-Chlordane


R.T.: 8.247 min
Delta R.T.: 0.018 min
Response: 306754
Conc: 0.15 ng/ml

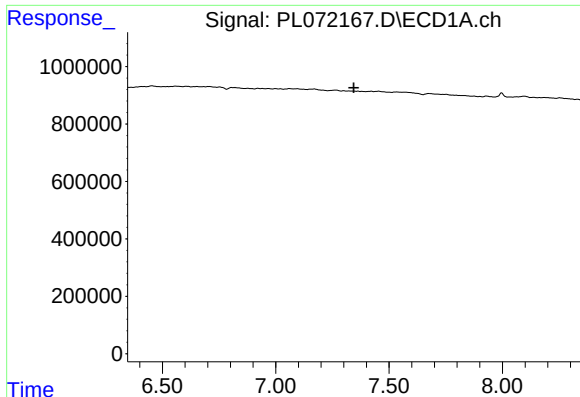

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

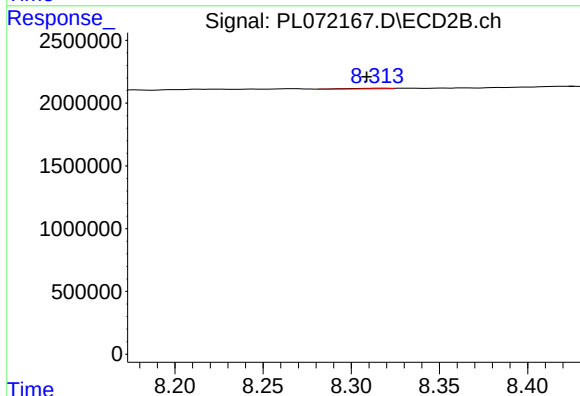


#11 alpha-Chlordane

R.T.: 8.316 min
Delta R.T.: 0.007 min
Response: 88162
Conc: 0.04 ng/ml

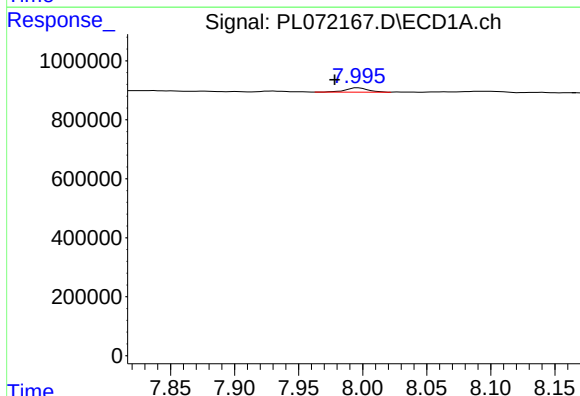


#14 Endrin

R.T.: 7.996 min
Delta R.T.: 0.018 min
Response: 176677
Conc: 0.25 ng/ml

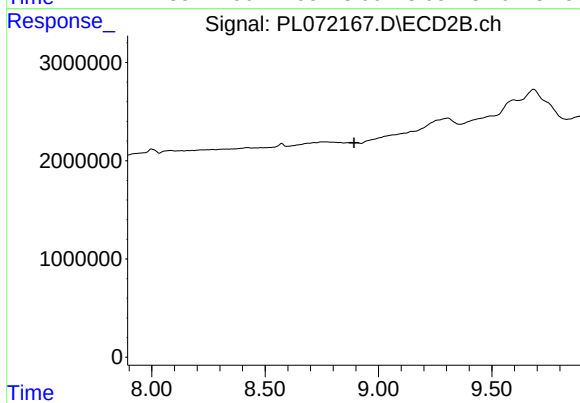

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.893 min
Response: 0
Conc: N.D.

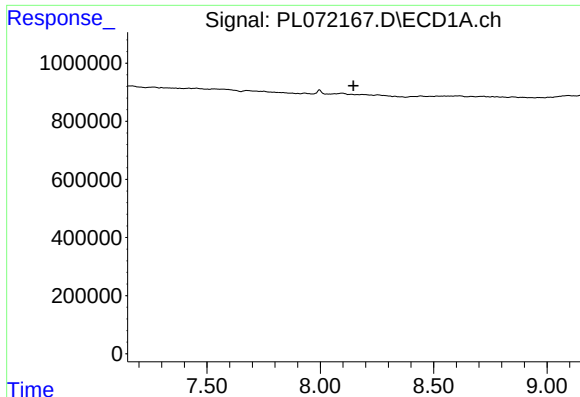

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

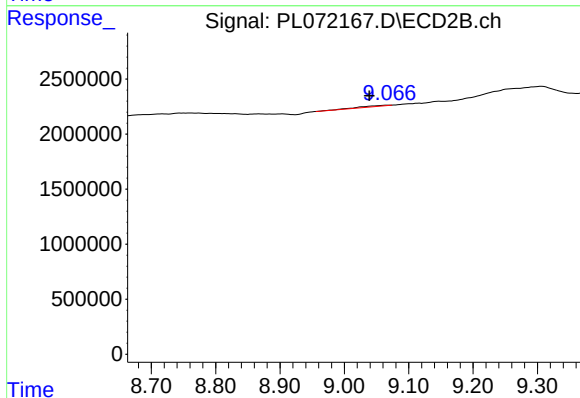


#16 4,4'-DDD

R.T.: 9.068 min
Delta R.T.: 0.029 min
Response: 259156
Conc: 0.18 ng/ml

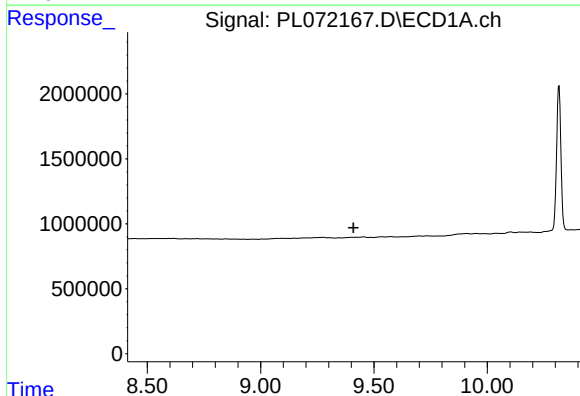


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 9.410 min
Response: 0
Conc: N.D.

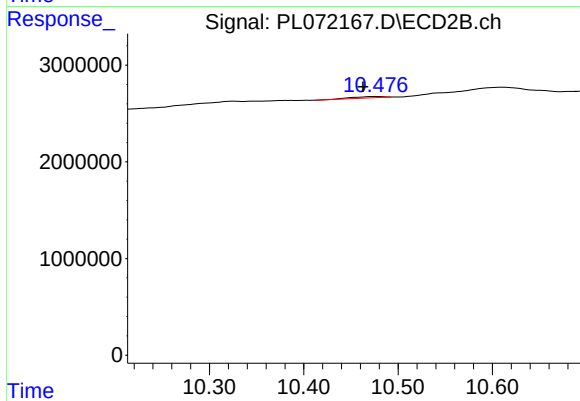

#22 Mirex


R.T.: 10.479 min
Delta R.T.: 0.016 min
Response: 341399
Conc: 0.27 ng/ml

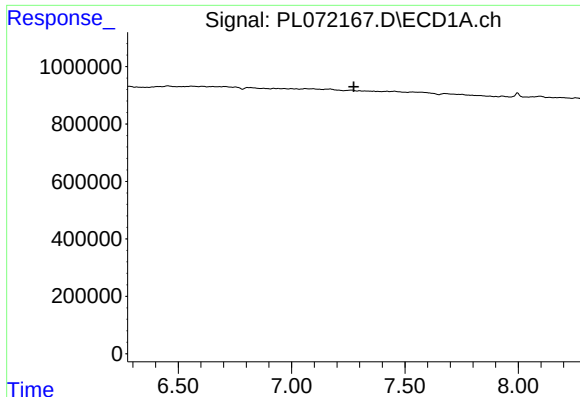

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

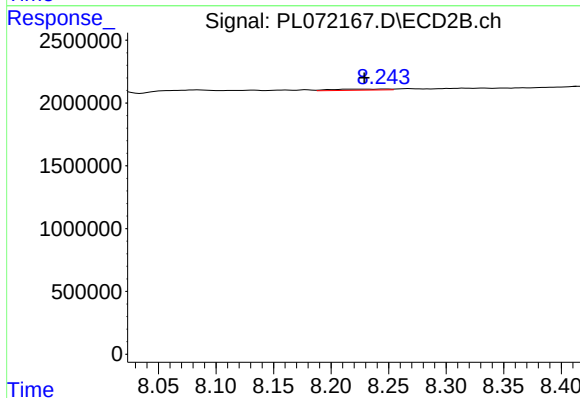


#25 Chlordane-3

R.T.: 8.247 min
Delta R.T.: 0.018 min
Response: 306754
Conc: 1.10 ng/ml

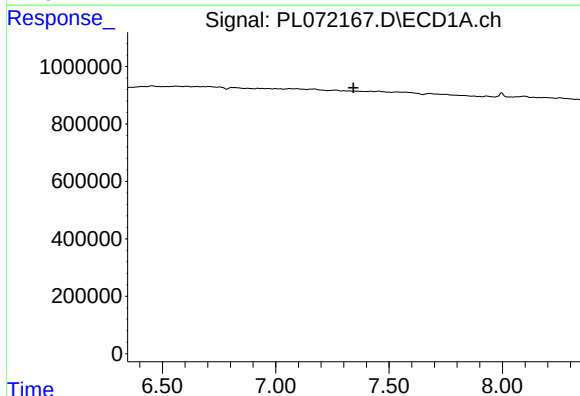


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

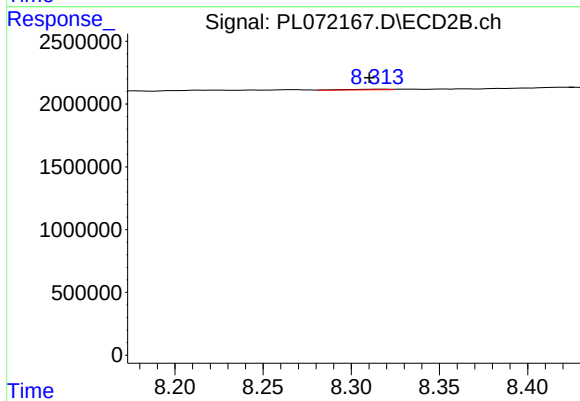

#26 Chlordane-4


R.T.: 8.316 min
Delta R.T.: 0.006 min
Response: 88162
Conc: 0.27 ng/ml

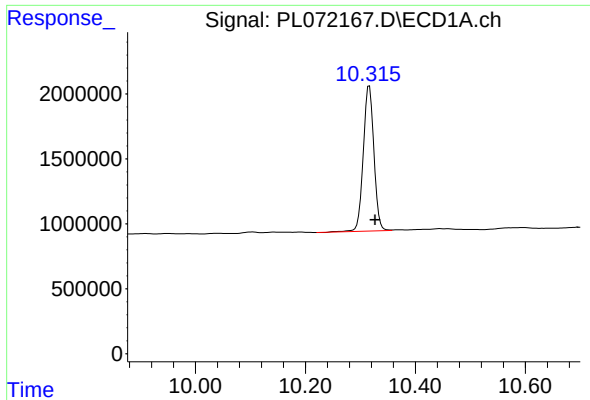

#28 Decachlorobiphenyl

R.T.: 10.316 min
Delta R.T.: -0.010 min
Response: 14997462
Conc: 16.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

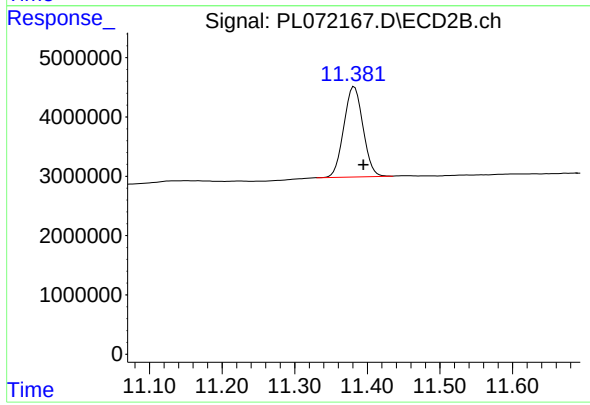

#28 Decachlorobiphenyl

R.T.: 11.382 min
Delta R.T.: -0.013 min
Response: 27899268
Conc: 17.29 ng/ml