

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012125\
 Data File : PL093734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2025 12:18
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 13:44:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 13:40:02 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.773	170.7E6	268.0E6	73.024	73.568
28)	SA Decachlor...	9.053	7.909	130.0E6	235.4E6	73.251	73.627
Target Compounds							
23)	Chlordane-1	4.700	3.771	79014350	89542504	727.966	725.097
24)	Chlordane-2	5.230	4.347	79888393	103.7E6	734.901	737.524
25)	Chlordane-3	5.940	4.977	270.7E6	316.6E6	735.837	729.311
26)	Chlordane-4	6.021	5.039	323.0E6	306.7E6	732.713	730.400
27)	Chlordane-5	6.870	5.935	60172092	113.7E6	729.580	741.701



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012125\
Data File : PL093734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2025 12:18
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 13:44:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 13:40:02 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

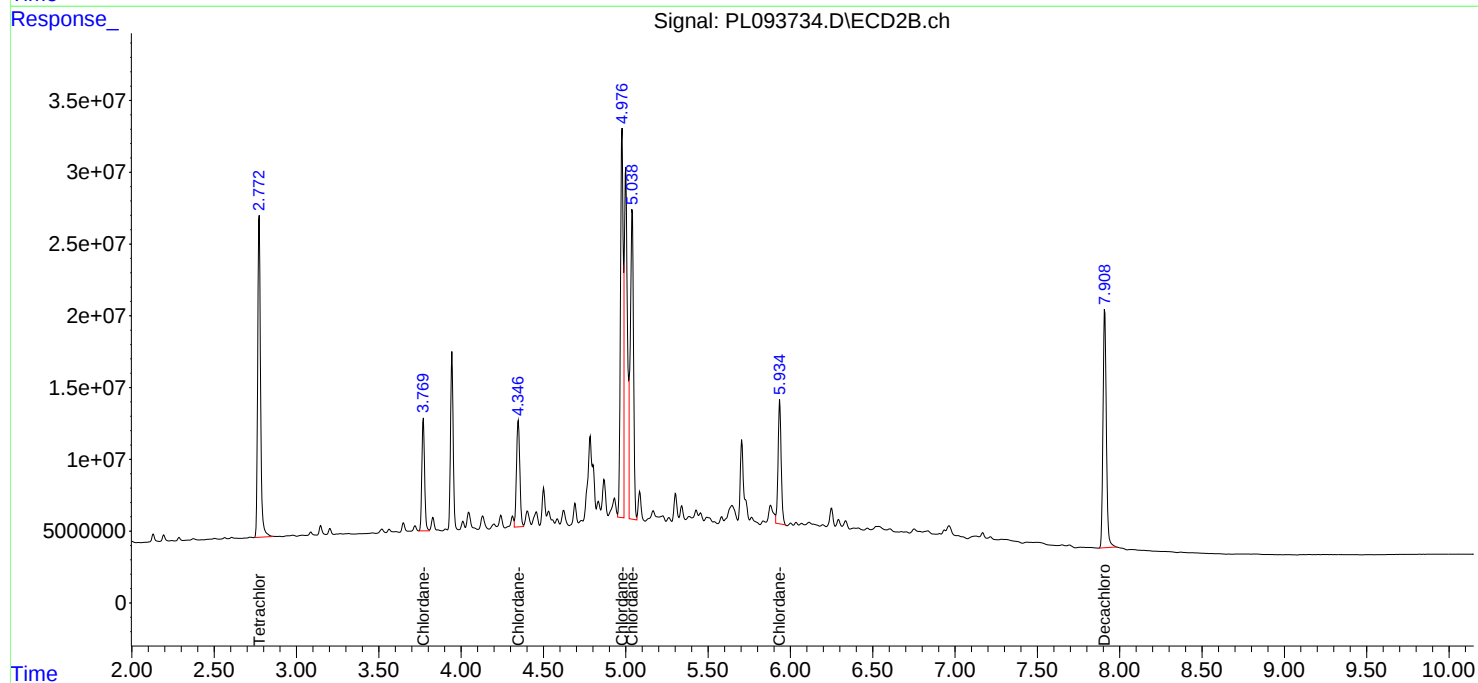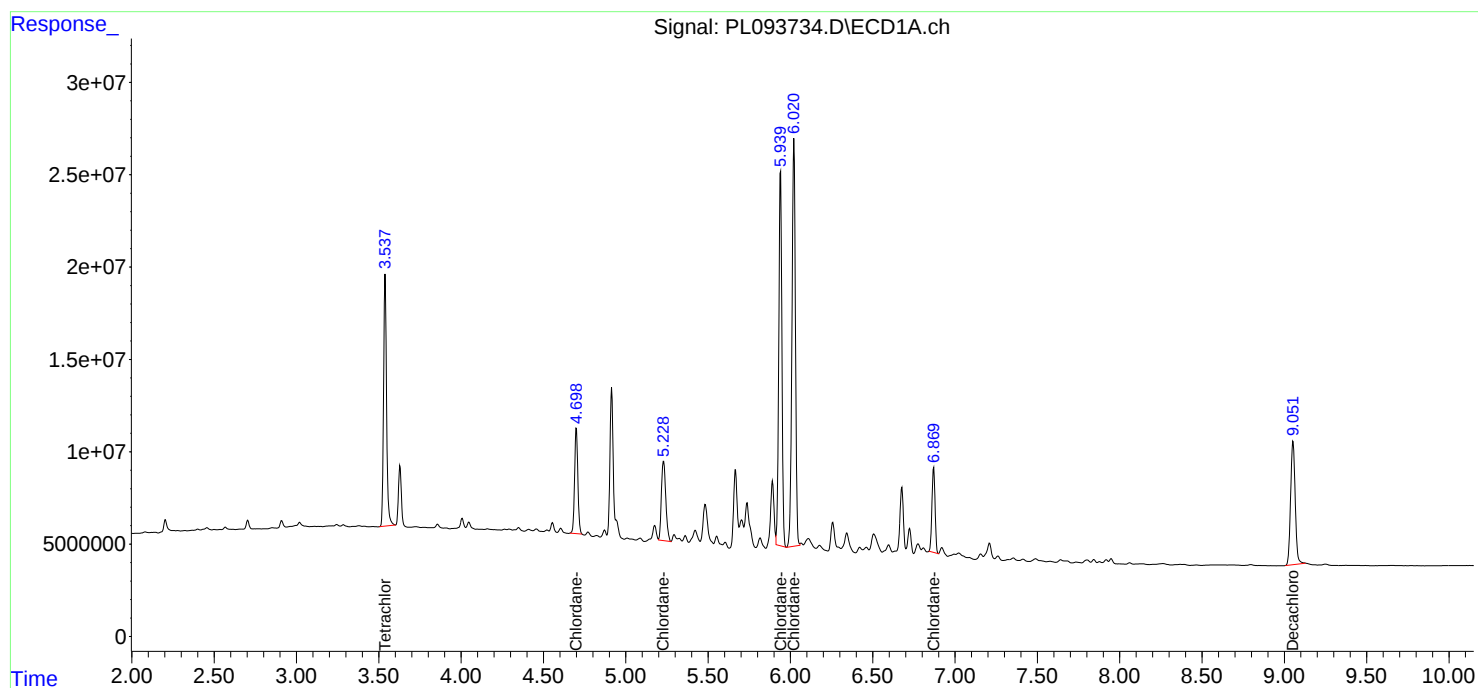


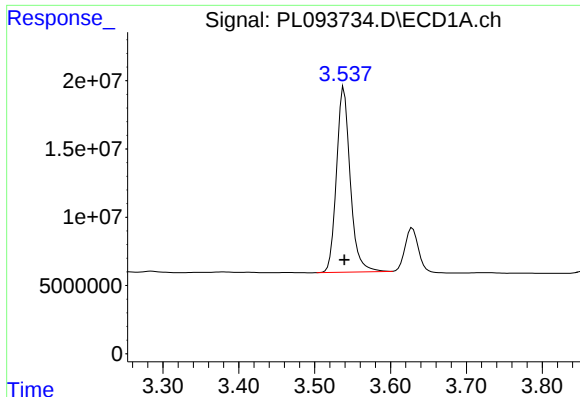

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 170673319
Conc: 73.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

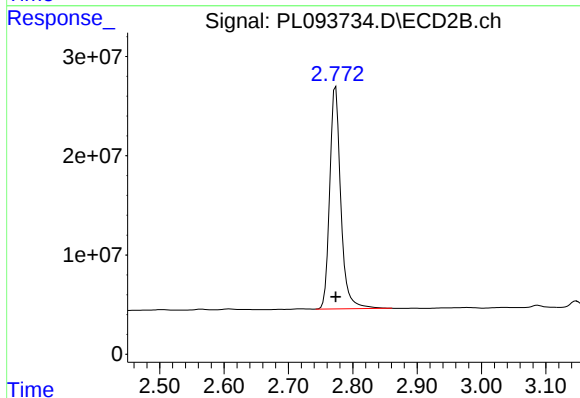


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 267989629
Conc: 73.57 ng/ml

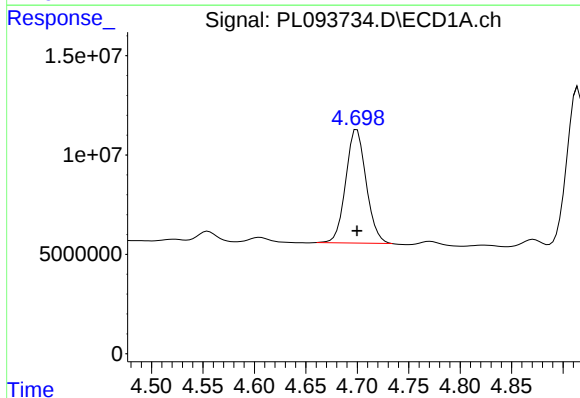


#23 Chlordane-1

R.T.: 4.700 min
Delta R.T.: 0.000 min
Response: 79014350
Conc: 727.97 ng/ml

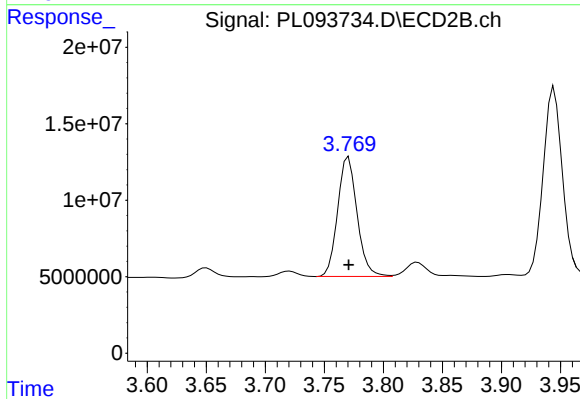

#23 Chlordane-1


R.T.: 3.771 min
Delta R.T.: 0.000 min
Response: 89542504
Conc: 725.10 ng/ml

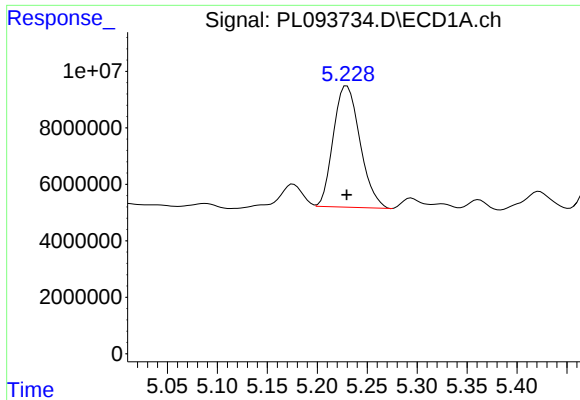

#24 Chlordane-2


R.T.: 5.230 min
Delta R.T.: 0.000 min
Response: 79888393
Conc: 734.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

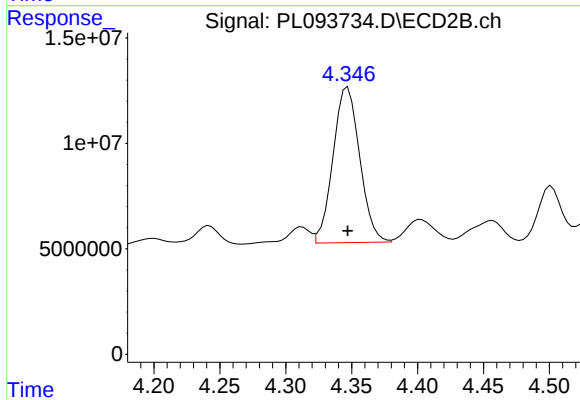


#24 Chlordane-2

R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 103747205
Conc: 737.52 ng/ml

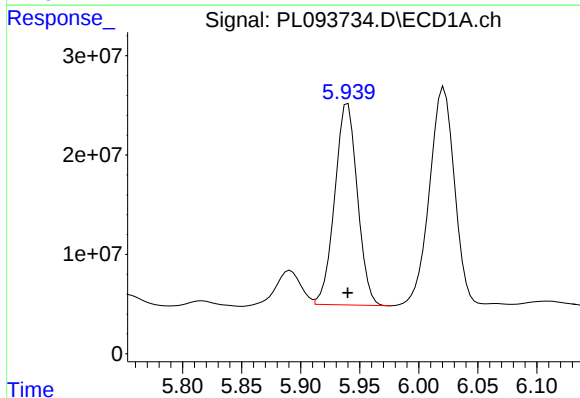


#25 Chlordane-3

R.T.: 5.940 min
Delta R.T.: 0.000 min
Response: 270693702
Conc: 735.84 ng/ml

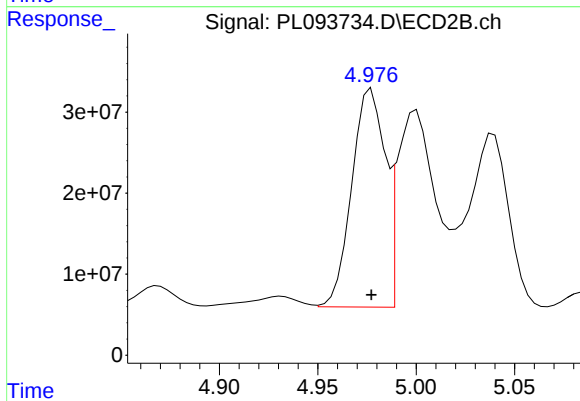

#25 Chlordane-3


R.T.: 4.977 min
Delta R.T.: 0.000 min
Response: 316644419
Conc: 729.31 ng/ml

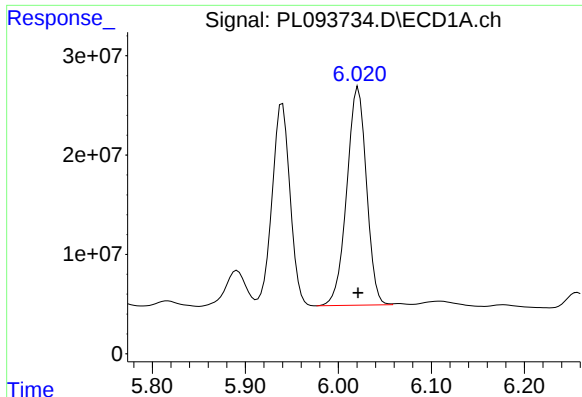

#26 Chlordane-4


R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 323007076
Conc: 732.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

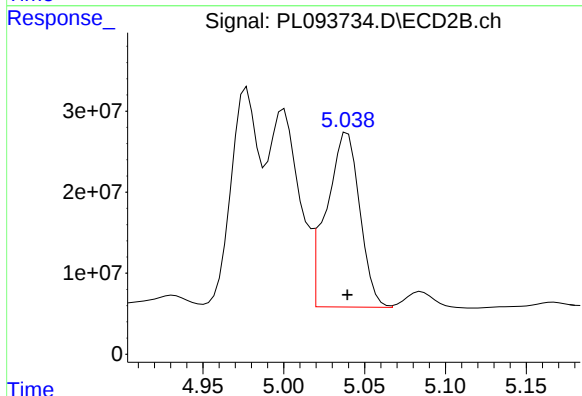


#26 Chlordane-4

R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 306650307
Conc: 730.40 ng/ml

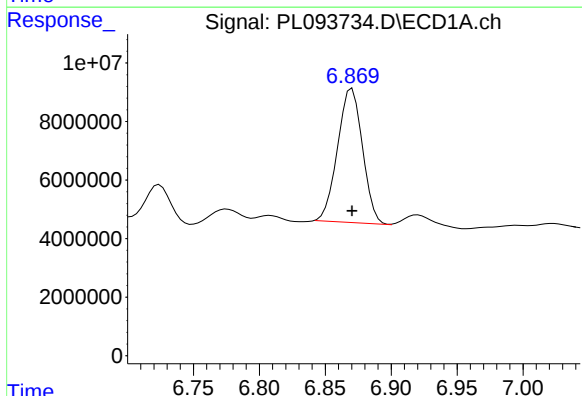


#27 Chlordane-5

R.T.: 6.870 min
Delta R.T.: 0.000 min
Response: 60172092
Conc: 729.58 ng/ml

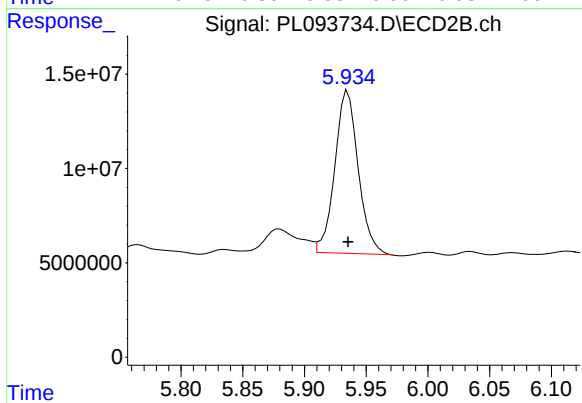

#27 Chlordane-5


R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 113715312
Conc: 741.70 ng/ml

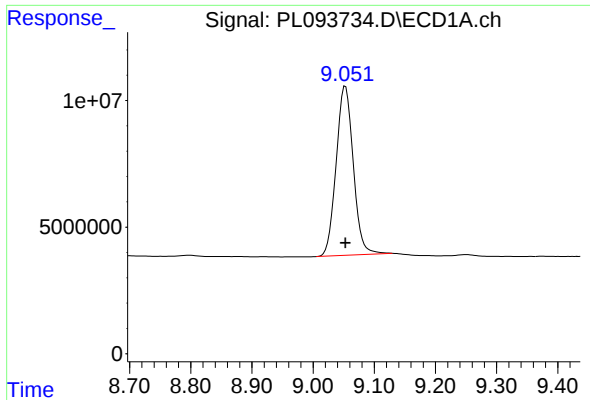

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: 0.000 min
Response: 129983339
Conc: 73.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

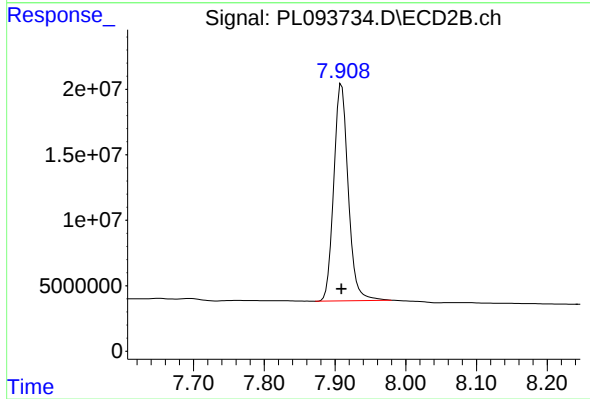

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: 0.000 min
Response: 235398109
Conc: 73.63 ng/ml