

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012125\
 Data File : PL093736.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2025 12:45
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 13:45:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 13:40:02 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.774	63515097	91692646	26.597	25.128
28)	SA Decachlor...	9.053	7.910	50369349	85481249	27.456	26.280
Target Compounds							
23)	Chlordane-1	4.699	3.770	30176040	31473339	270.438	253.631
24)	Chlordane-2	5.228	4.347	30681935	37368798	273.429	261.556
25)	Chlordane-3	5.939	4.977	98573557	108.8E6	263.230	250.525
26)	Chlordane-4	6.021	5.040	118.0E6	106.0E6	263.059	251.930
27)	Chlordane-5	6.870	5.935	22980330	38357980	270.878	250.141


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012125\
Data File : PL093736.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2025 12:45
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 13:45:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 13:40:02 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

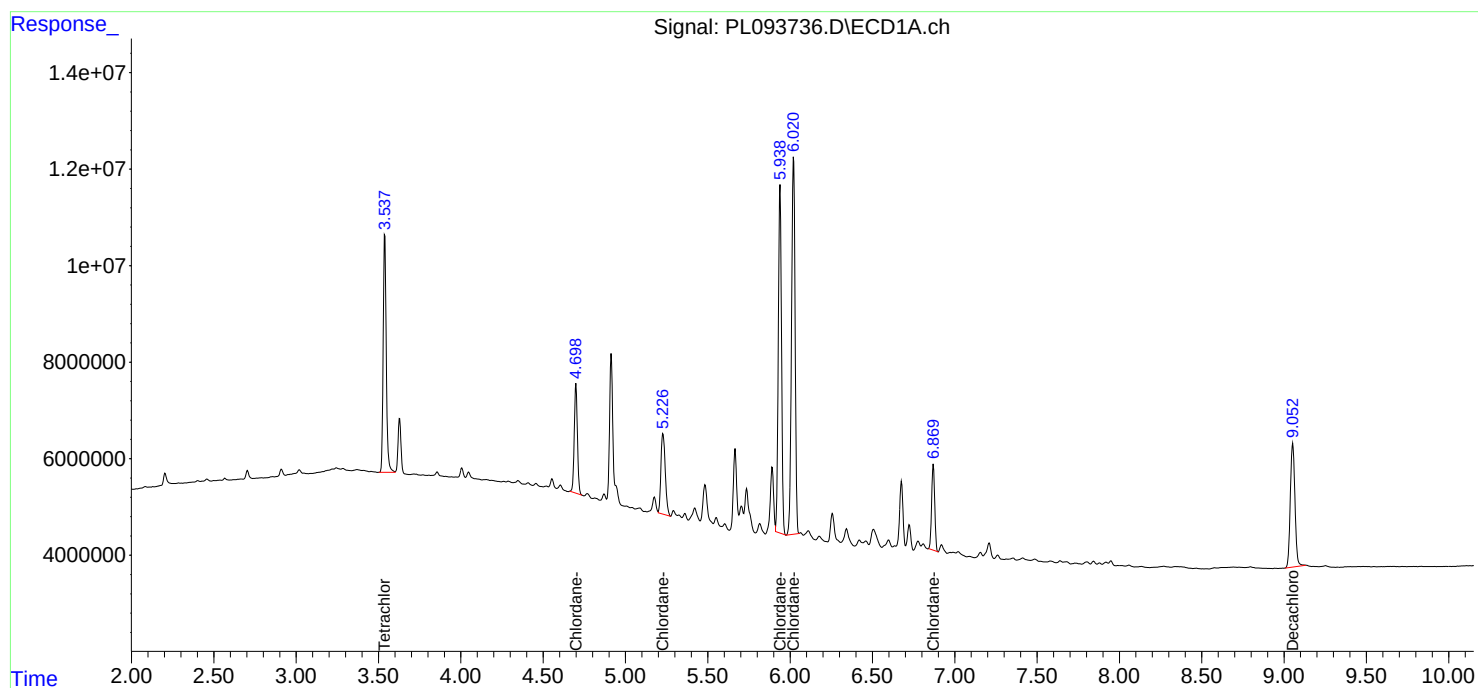


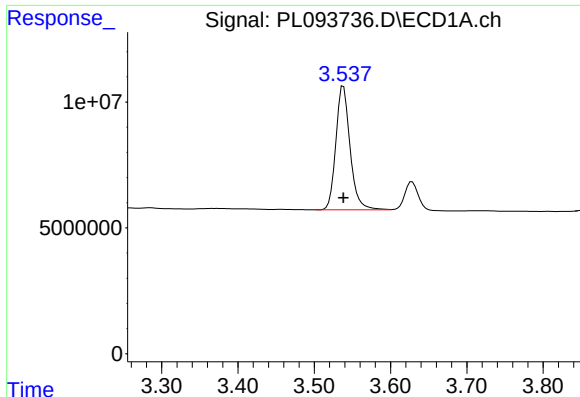

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 63515097
Conc: 26.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

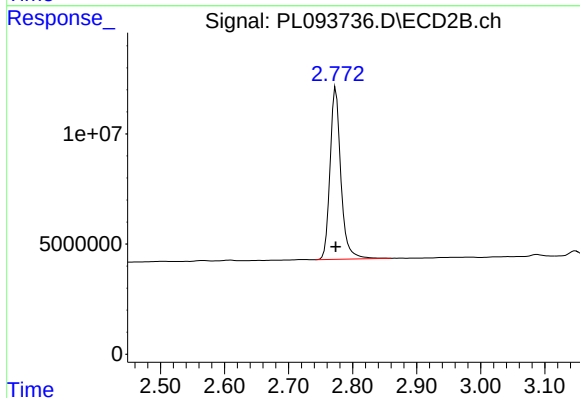


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 91692646
Conc: 25.13 ng/ml

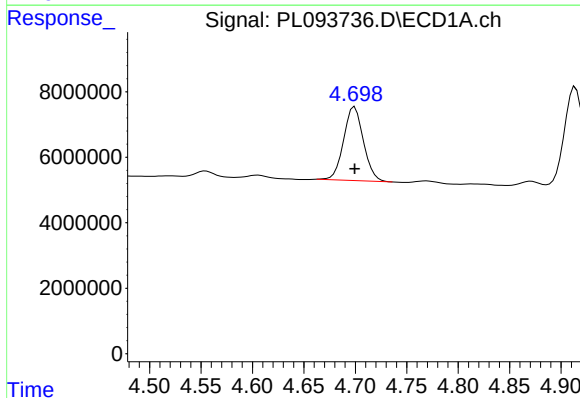


#23 Chlordane-1

R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 30176040
Conc: 270.44 ng/ml

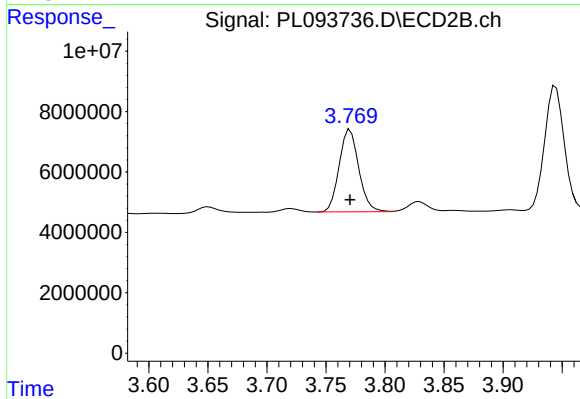

#23 Chlordane-1


R.T.: 3.770 min
Delta R.T.: 0.000 min
Response: 31473339
Conc: 253.63 ng/ml

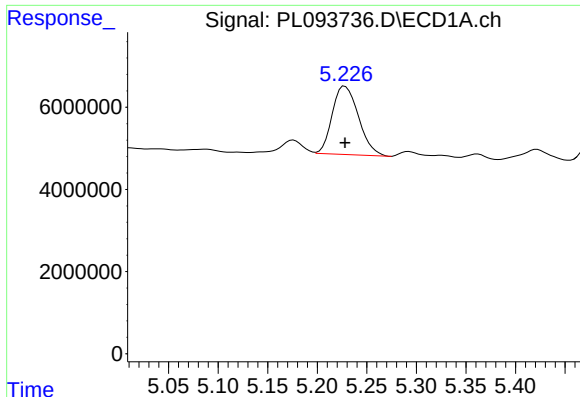

#24 Chlordane-2


R.T.: 5.228 min
Delta R.T.: 0.000 min
Response: 30681935
Conc: 273.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

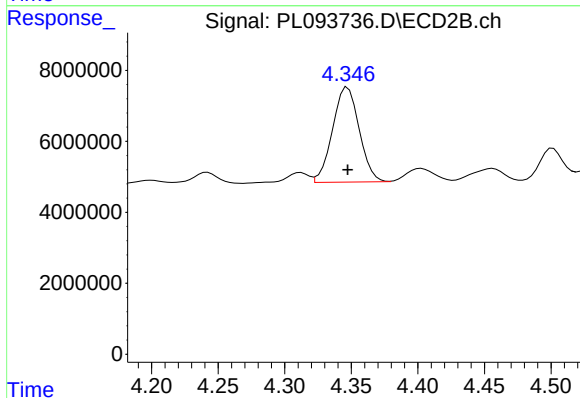


#24 Chlordane-2

R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 37368798
Conc: 261.56 ng/ml

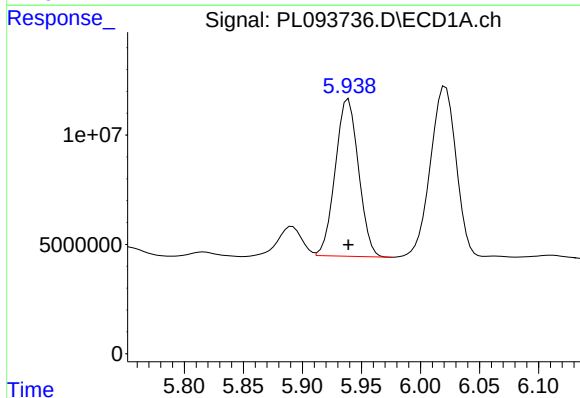


#25 Chlordane-3

R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 98573557
Conc: 263.23 ng/ml

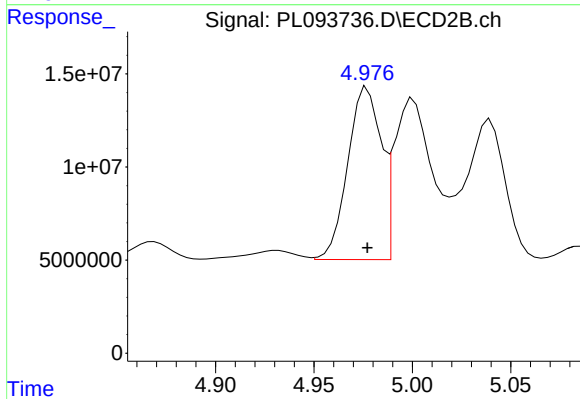

#25 Chlordane-3


R.T.: 4.977 min
Delta R.T.: 0.000 min
Response: 108846335
Conc: 250.52 ng/ml

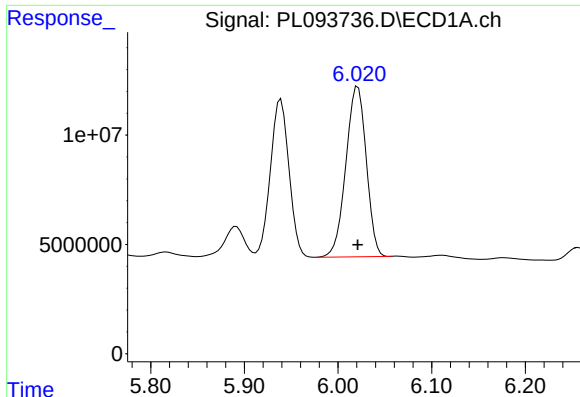

#26 Chlordane-4


R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 118020898
Conc: 263.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

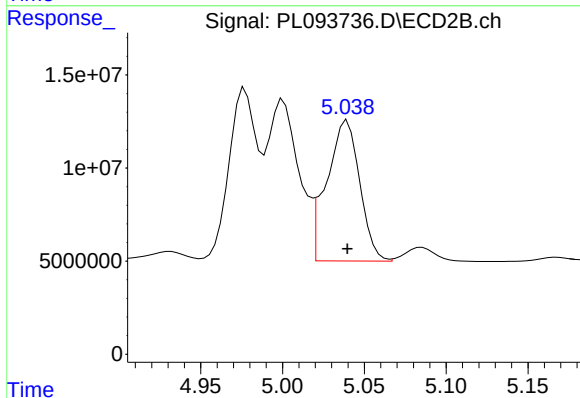


#26 Chlordane-4

R.T.: 5.040 min
Delta R.T.: 0.000 min
Response: 106043140
Conc: 251.93 ng/ml

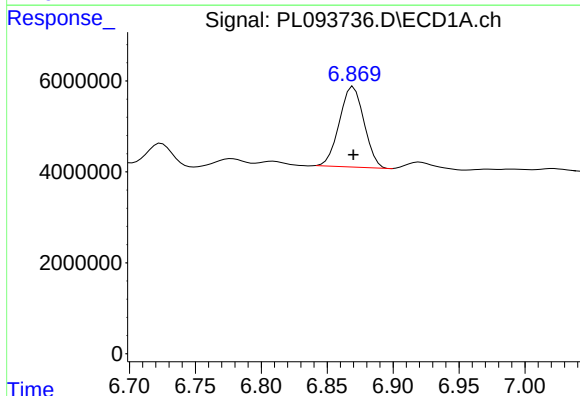


#27 Chlordane-5

R.T.: 6.870 min
Delta R.T.: 0.000 min
Response: 22980330
Conc: 270.88 ng/ml

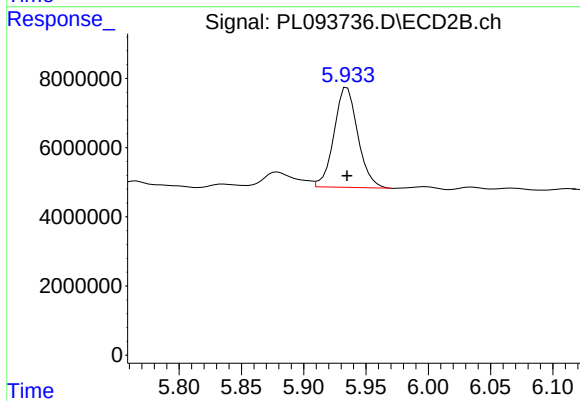

#27 Chlordane-5


R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 38357980
Conc: 250.14 ng/ml

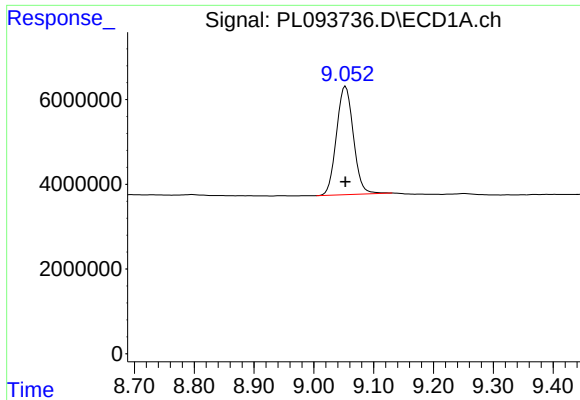

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: 0.000 min
Response: 50369349
Conc: 27.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

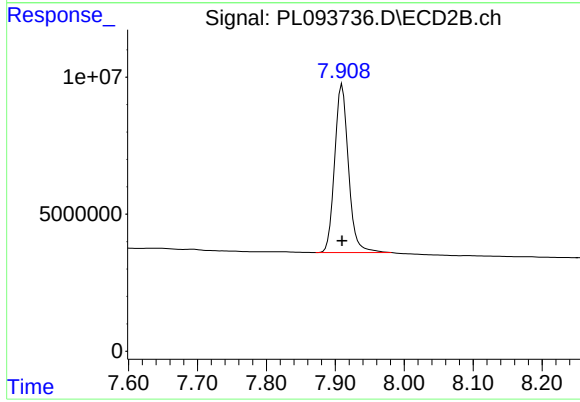

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: 0.000 min
Response: 85481249
Conc: 26.28 ng/ml