

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012125\
 Data File : PL093727.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2025 10:43
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 14:04:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 14:02:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.774	48739758	56764042	18.100	17.390
28)	SA Decachlor...	9.053	7.910	37826748	61983547	18.082	17.689
Target Compounds							
9)	A Endosulfan I	6.068	5.097	24505533	31106405	9.272	8.023
10)	B gamma-Chl...	5.939	4.977	26686746	36721665	9.574	8.666
12)	B 4,4'-DDE	6.191	5.230	45047667	71134812	18.503	17.742
13)	MA Dieldrin	6.343	5.361	50553851	73721045	18.212	17.162
19)	B Endosulfa...	7.157	6.333	42219467	62907773	18.650	17.641
20)	A Methoxychlor	7.499	6.609	83993166	151.6E6	80.500	84.806
21)	B Endrin ke...	7.642	6.838	44318803	70010295	17.569	16.688



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012125\
Data File : PL093727.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2025 10:43
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 14:04:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 14:02:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

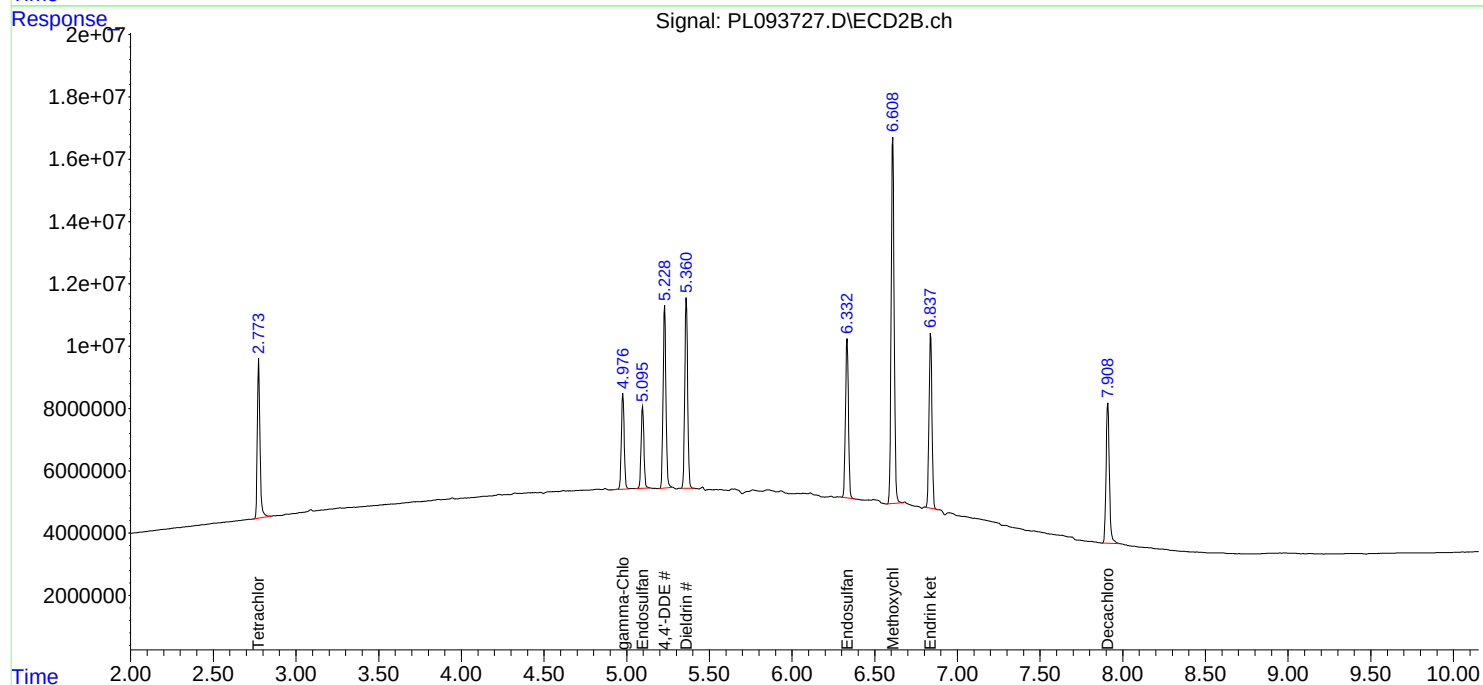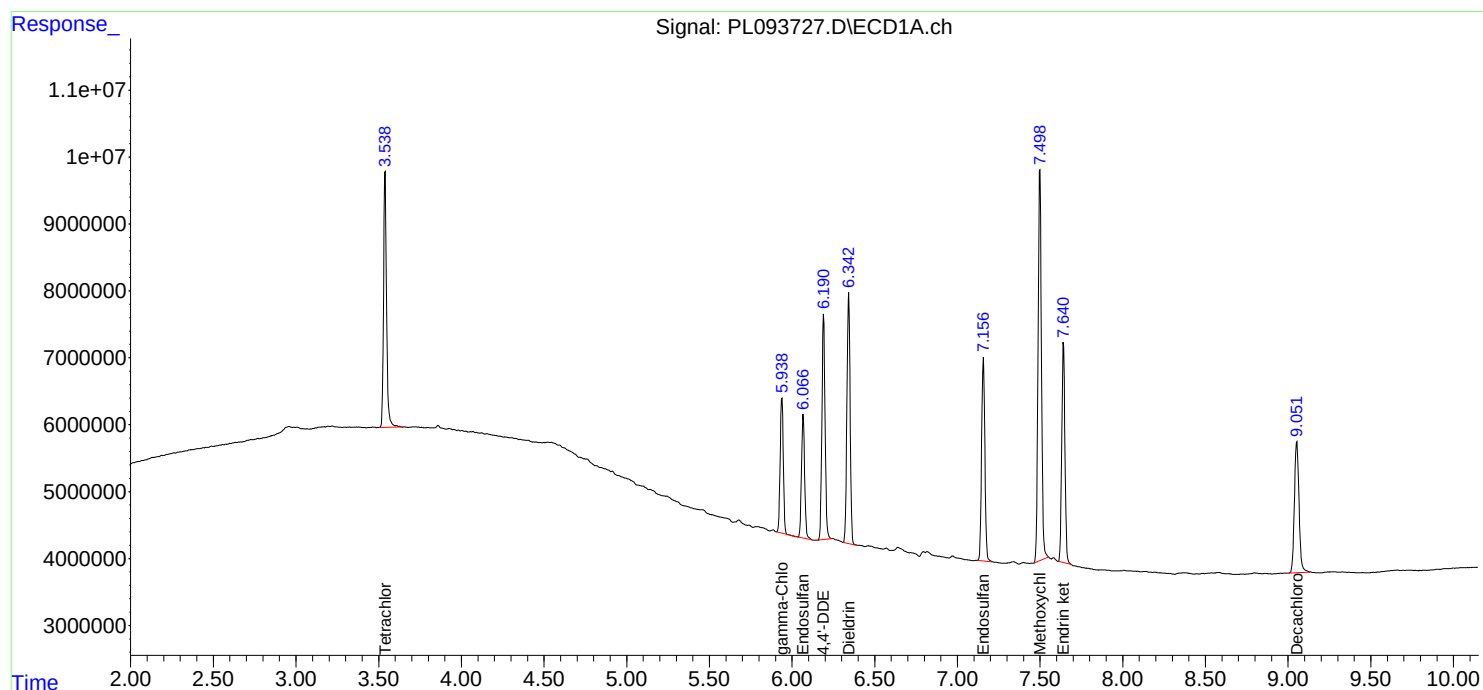


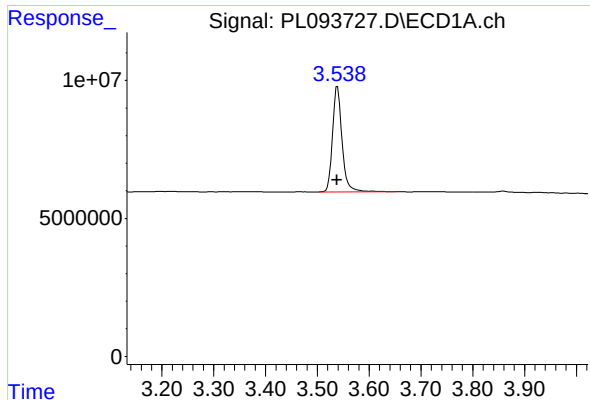

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.001 min
Response: 48739758
Conc: 18.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

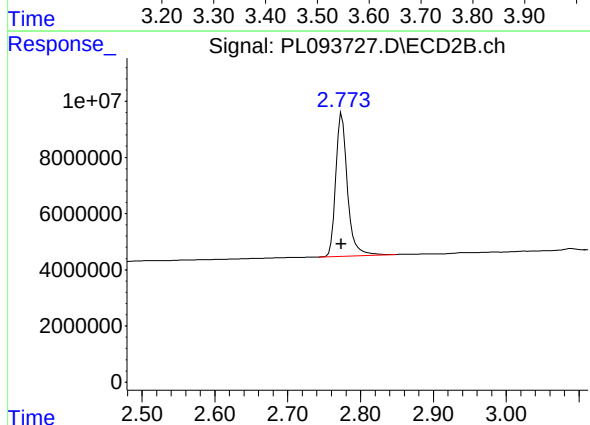


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 56764042
Conc: 17.39 ng/ml

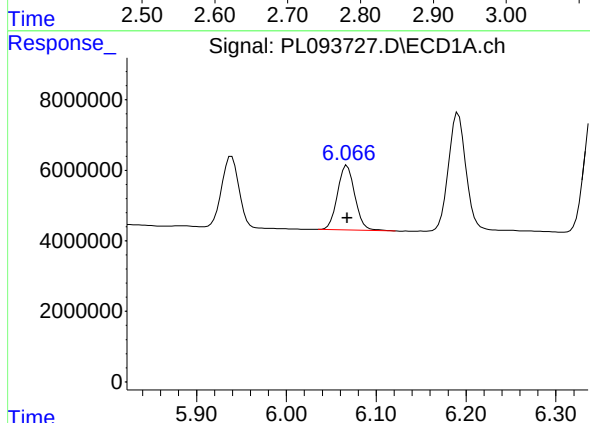


#9 Endosulfan I

R.T.: 6.068 min
Delta R.T.: 0.000 min
Response: 24505533
Conc: 9.27 ng/ml

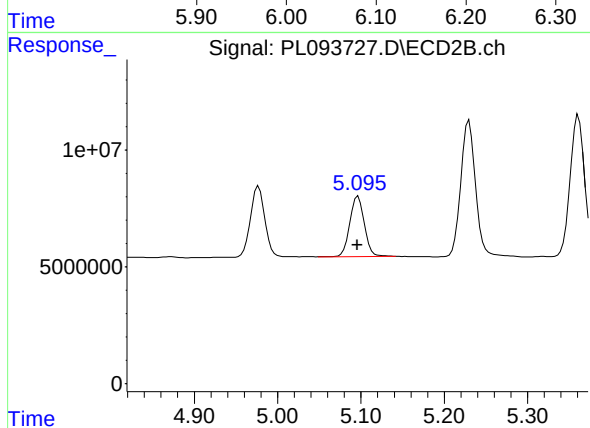

#9 Endosulfan I


R.T.: 5.097 min
Delta R.T.: 0.000 min
Response: 31106405
Conc: 8.02 ng/ml

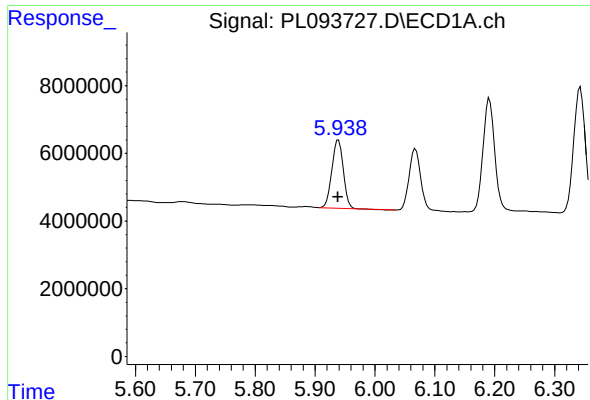

#10 gamma-Chlordane


R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 26686746
Conc: 9.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

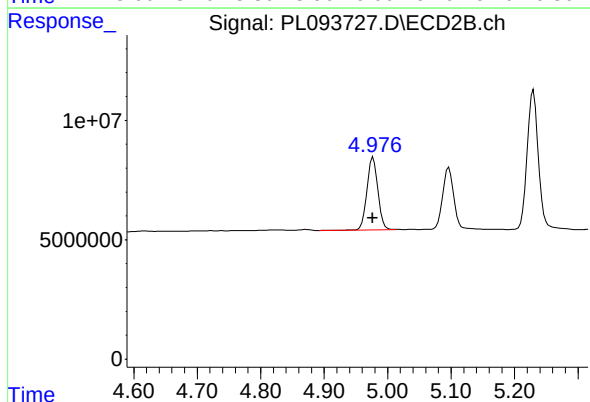


#10 gamma-Chlordane

R.T.: 4.977 min
Delta R.T.: 0.000 min
Response: 36721665
Conc: 8.67 ng/ml

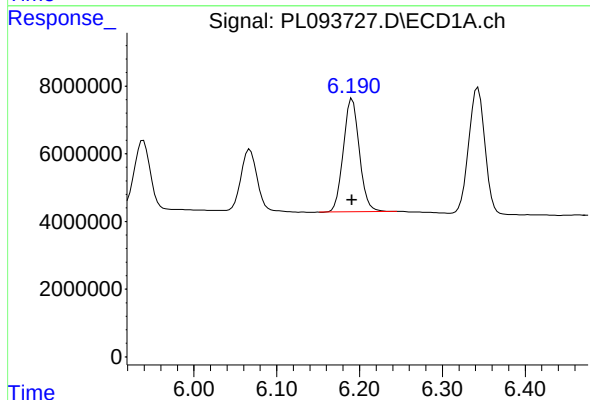


#12 4,4'-DDE

R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 45047667
Conc: 18.50 ng/ml

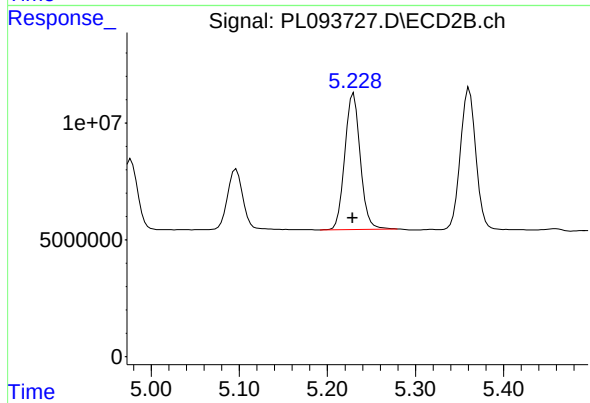

#12 4,4'-DDE


R.T.: 5.230 min
Delta R.T.: 0.001 min
Response: 71134812
Conc: 17.74 ng/ml

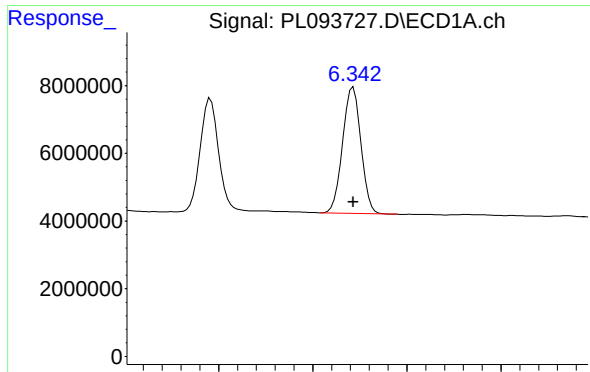

#13 Dieldrin


R.T.: 6.343 min
Delta R.T.: 0.000 min
Response: 50553851
Conc: 18.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

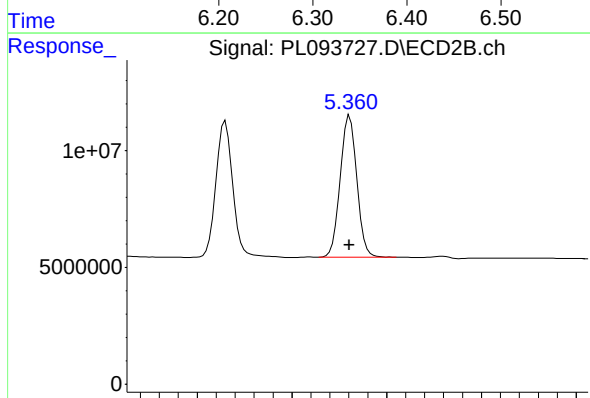


#13 Dieldrin

R.T.: 5.361 min
Delta R.T.: 0.000 min
Response: 73721045
Conc: 17.16 ng/ml

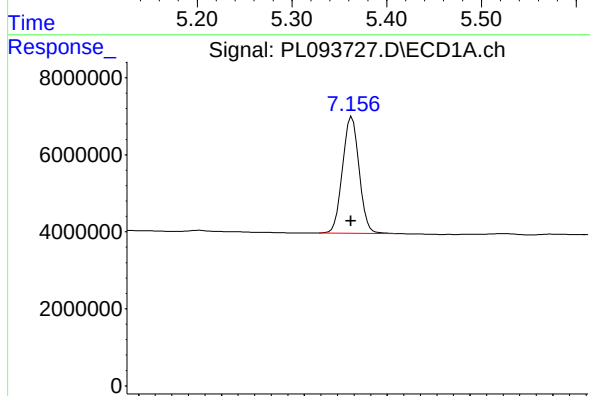


#19 Endosulfan Sulfate

R.T.: 7.157 min
Delta R.T.: 0.001 min
Response: 42219467
Conc: 18.65 ng/ml

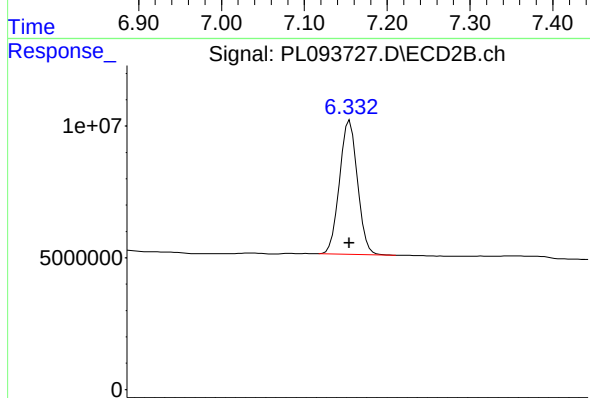

#19 Endosulfan Sulfate


R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 62907773
Conc: 17.64 ng/ml

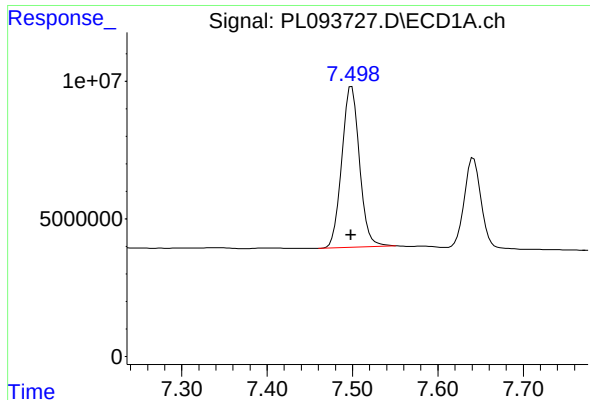

#20 Methoxychlor


R.T.: 7.499 min
Delta R.T.: 0.000 min
Response: 83993166
Conc: 80.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

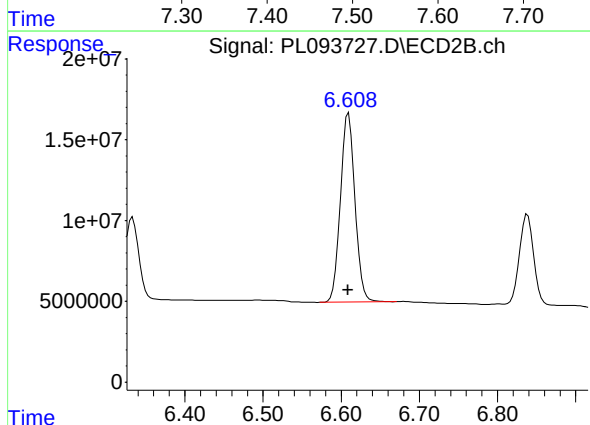


#20 Methoxychlor

R.T.: 6.609 min
Delta R.T.: 0.000 min
Response: 151645256
Conc: 84.81 ng/ml

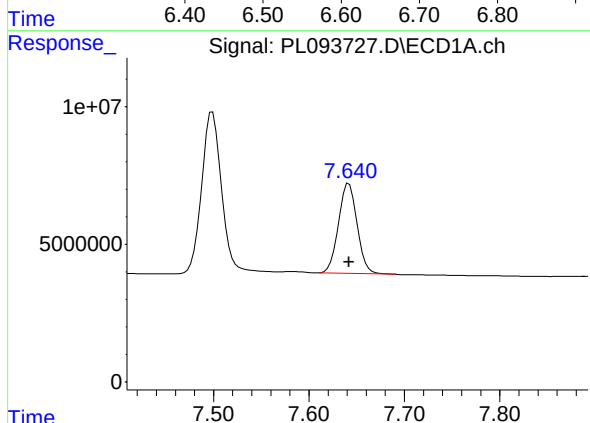


#21 Endrin ketone

R.T.: 7.642 min
Delta R.T.: 0.000 min
Response: 44318803
Conc: 17.57 ng/ml

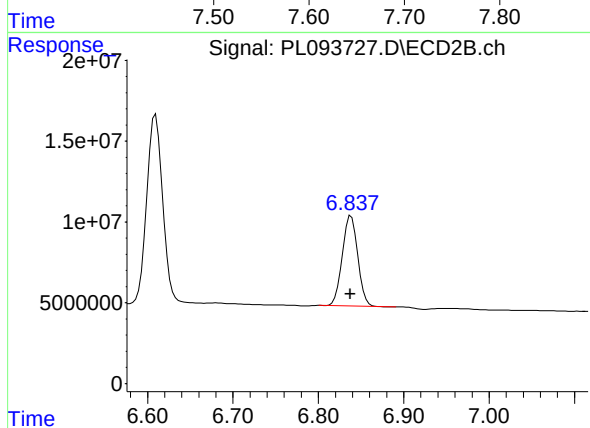

#21 Endrin ketone


R.T.: 6.838 min
Delta R.T.: 0.000 min
Response: 70010295
Conc: 16.69 ng/ml

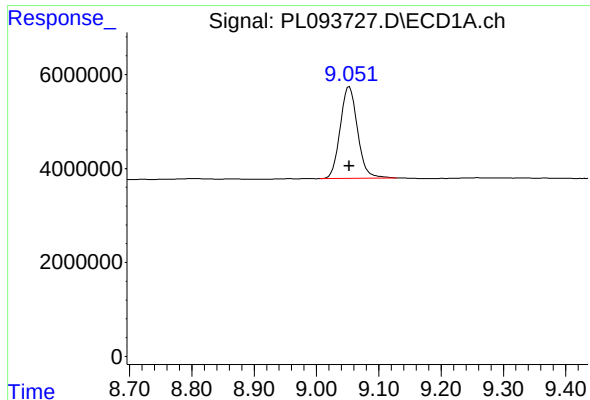

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: 0.000 min
Response: 37826748
Conc: 18.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

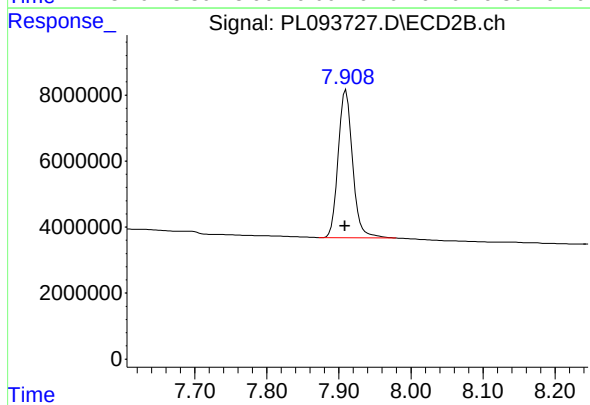

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: 0.001 min
Response: 61983547
Conc: 17.69 ng/ml