

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012219\
 Data File : PL044117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2019 12:57
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 00:40:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 23 00:38:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.985	311.4E6	103.7E6	50.000	50.000
28)	SA Decachlor...	8.048	9.040	335.3E6	105.7E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.213	4.978	127.8E6	49773086	500.000	500.000
24)	Chlordane-2	4.705	5.445	143.6E6	55638776	500.000	500.000
25)	Chlordane-3	5.263	6.090	431.0E6	173.7E6	500.000	500.000
26)	Chlordane-4	5.319	6.164	385.2E6	209.9E6	500.000	500.000
27)	Chlordane-5	6.143	6.967	121.1E6	37808277	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012219\
Data File : PL044117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2019 12:57
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 00:40:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
Quant Title : GC Extractables
QLast Update : Wed Jan 23 00:38:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

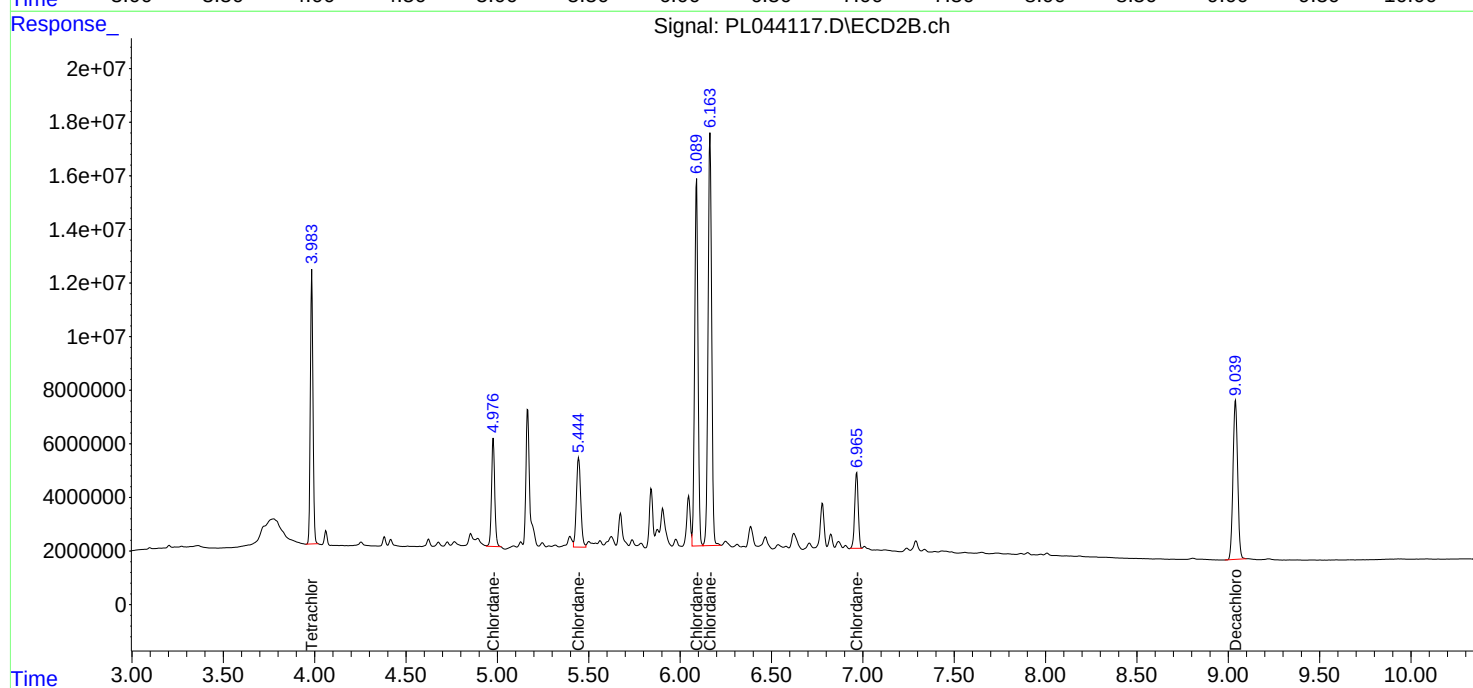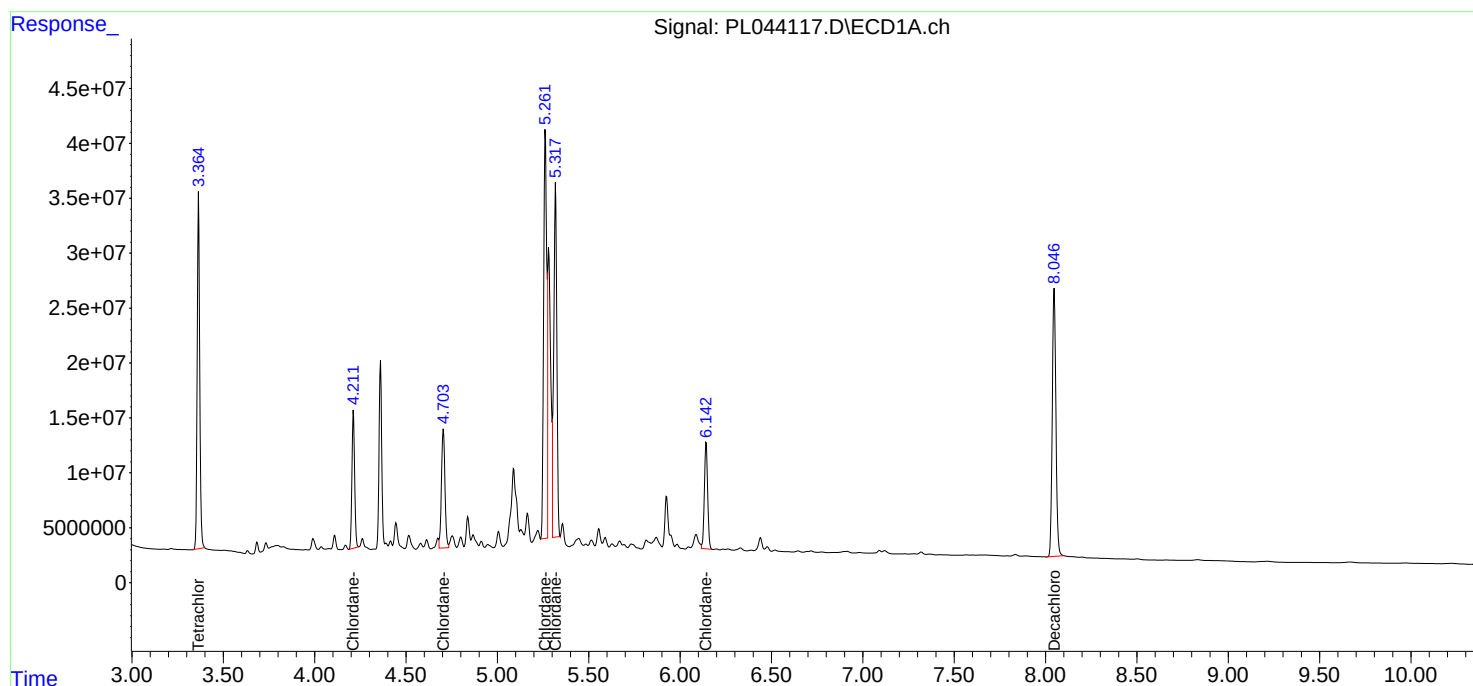


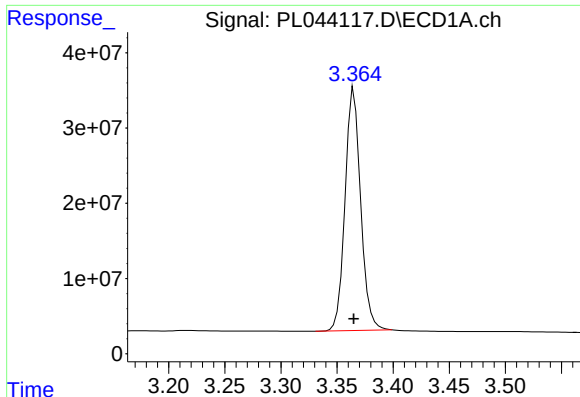

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: 0.000 min
Response: 311422736
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

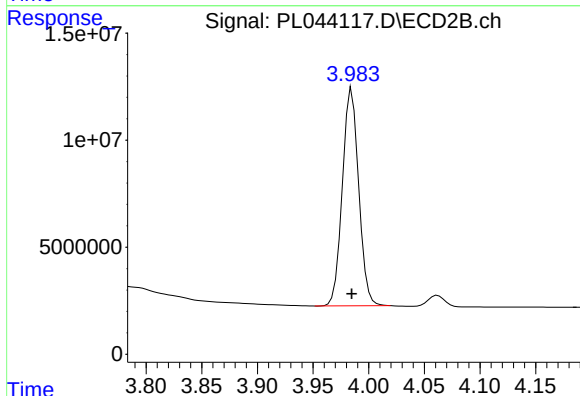


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 103666918
Conc: 50.00 ng/ml

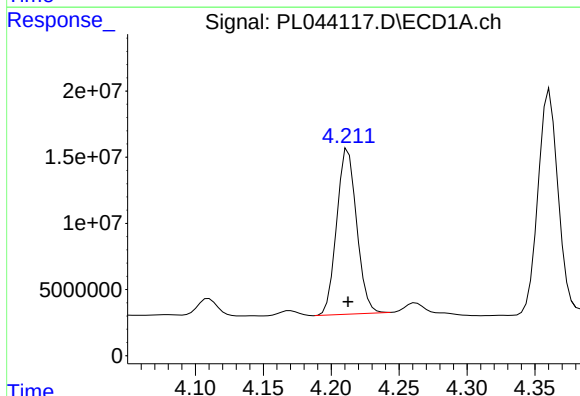


#23 Chlordane-1

R.T.: 4.213 min
Delta R.T.: 0.000 min
Response: 127798737
Conc: 500.00 ng/ml

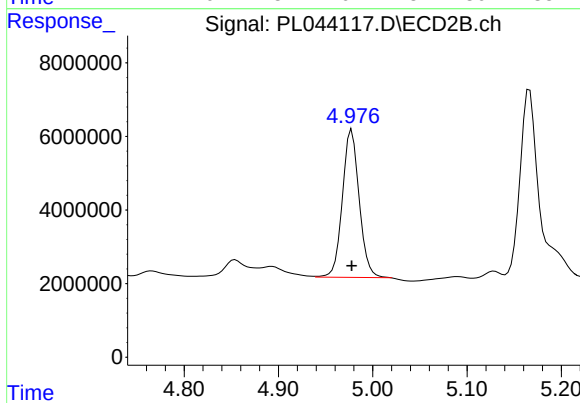

#23 Chlordane-1


R.T.: 4.978 min
Delta R.T.: 0.000 min
Response: 49773086
Conc: 500.00 ng/ml

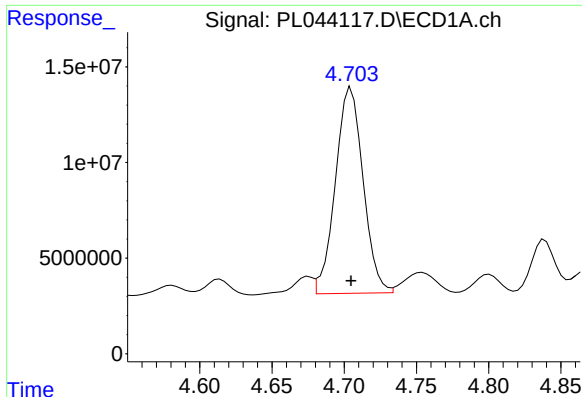

#24 Chlordane-2


R.T.: 4.705 min
Delta R.T.: 0.000 min
Response: 143550424
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

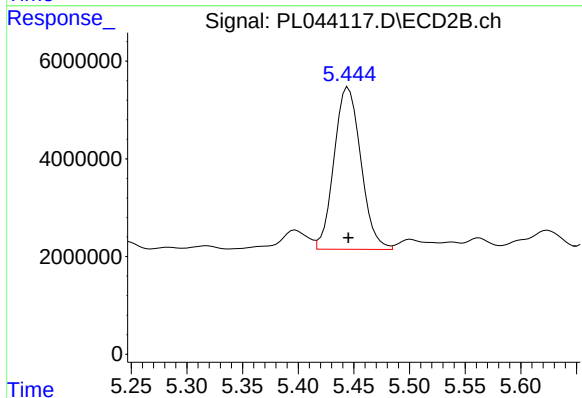


#24 Chlordane-2

R.T.: 5.445 min
Delta R.T.: 0.000 min
Response: 55638776
Conc: 500.00 ng/ml

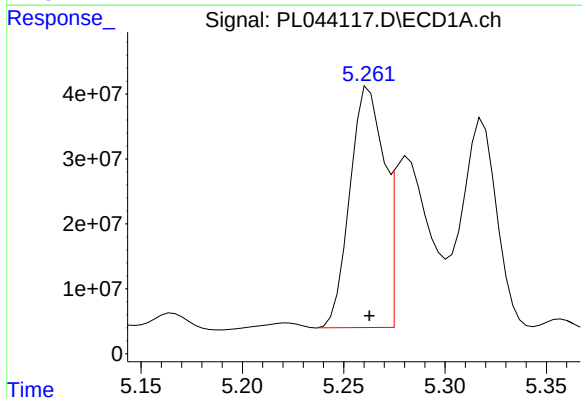


#25 Chlordane-3

R.T.: 5.263 min
Delta R.T.: 0.000 min
Response: 430990306
Conc: 500.00 ng/ml

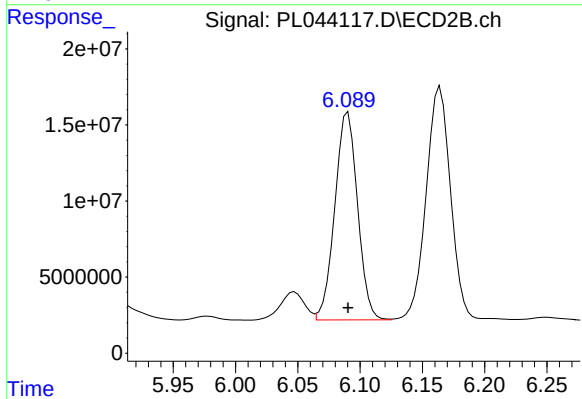

#25 Chlordane-3


R.T.: 6.090 min
Delta R.T.: 0.000 min
Response: 173747652
Conc: 500.00 ng/ml

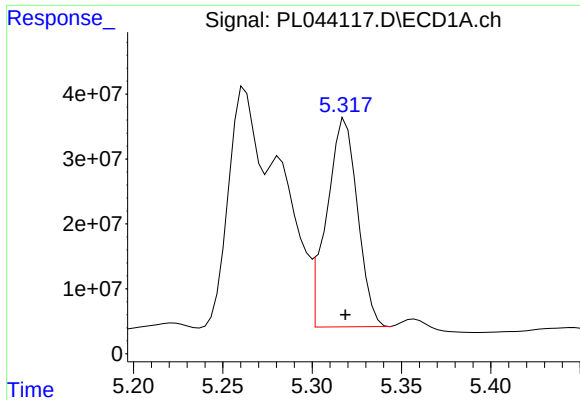

#26 Chlordane-4


R.T.: 5.319 min
Delta R.T.: 0.000 min
Response: 385214531
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

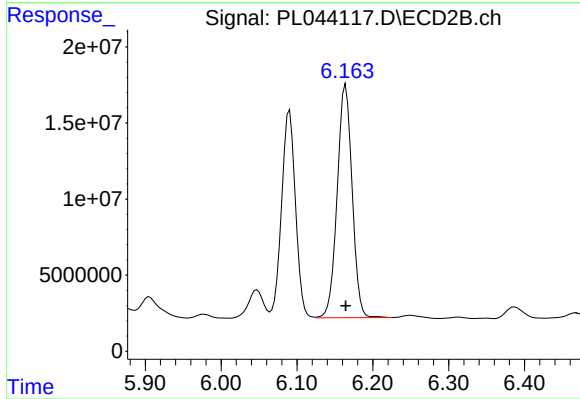


#26 Chlordane-4

R.T.: 6.164 min
Delta R.T.: 0.000 min
Response: 209916694
Conc: 500.00 ng/ml

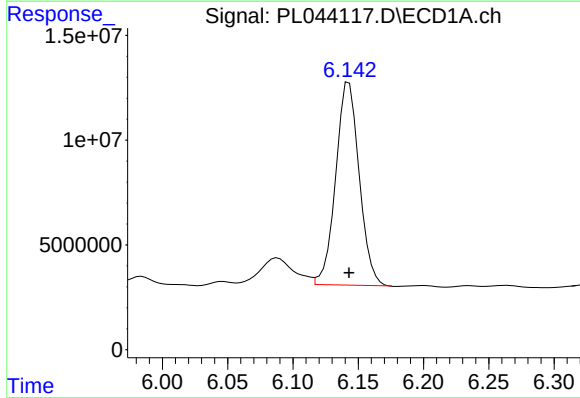


#27 Chlordane-5

R.T.: 6.143 min
Delta R.T.: 0.000 min
Response: 121144139
Conc: 500.00 ng/ml

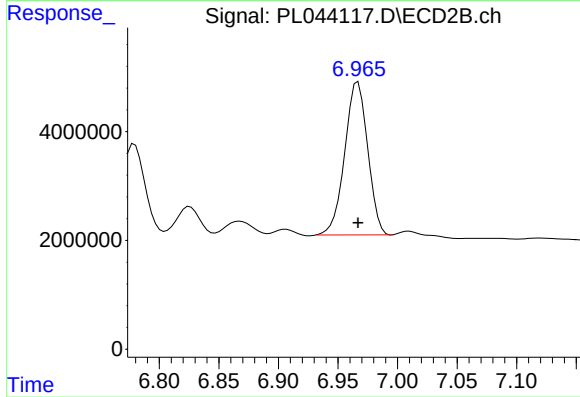

#27 Chlordane-5


R.T.: 6.967 min
Delta R.T.: 0.000 min
Response: 37808277
Conc: 500.00 ng/ml

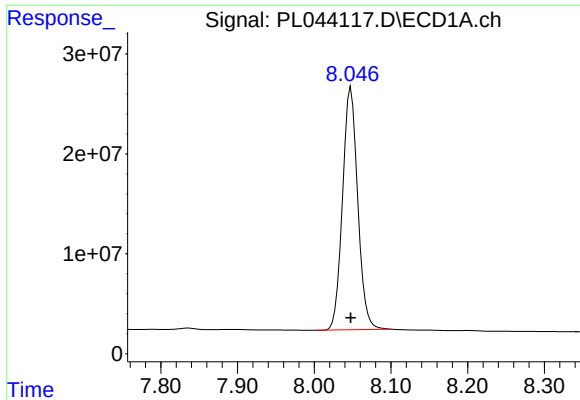

#28 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: 0.000 min
Response: 335263385
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

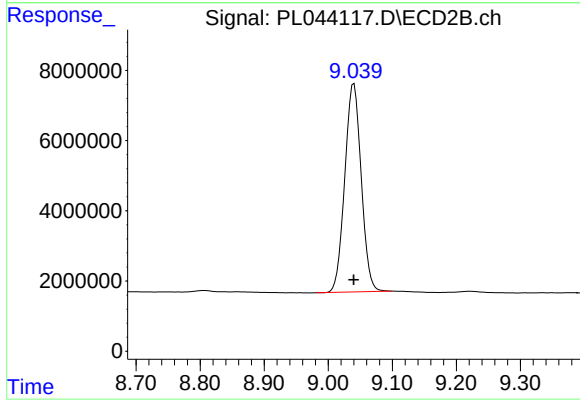

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 105711117
Conc: 50.00 ng/ml