

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012219\
 Data File : PL044126.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2019 15:18
 Operator : AJ\SJ
 Sample : K1171-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EB6-011619-S-001

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 02:20:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 23 00:42:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.366	3.985	107.4E6	37355611	17.722	17.125
28)	SA Decachlor...	8.048	9.041	79640676	26740758	11.484	12.054
Target Compounds							
12)	B 4,4'-DDE	5.486	6.320	123.6E6	38493952	18.240	17.937
14)	MA Endrin	5.869	6.714	24733512	4733695	3.688	2.349 #
16)	A 4,4'-DDD	0.000	6.810	0	3809558	N.D.	2.221 #
17)	MA 4,4'-DDT	6.233	7.108	128.2E6	14063367	25.149	8.570 #
18)	B Endrin al...	6.316	0.000	8882797	0	1.571	N.D. #
19)	B Endosulfa...	6.457f	7.233	82213409	12816976	14.416	6.666 #
20)	A Methoxychlor	0.000	7.509f	0	3444608	N.D.	3.368 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012219\
Data File : PL044126.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2019 15:18
Operator : AJ\SJ
Sample : K1171-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
EB6-011619-S-001

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 02:20:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
Quant Title : GC Extractables
QLast Update : Wed Jan 23 00:42:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

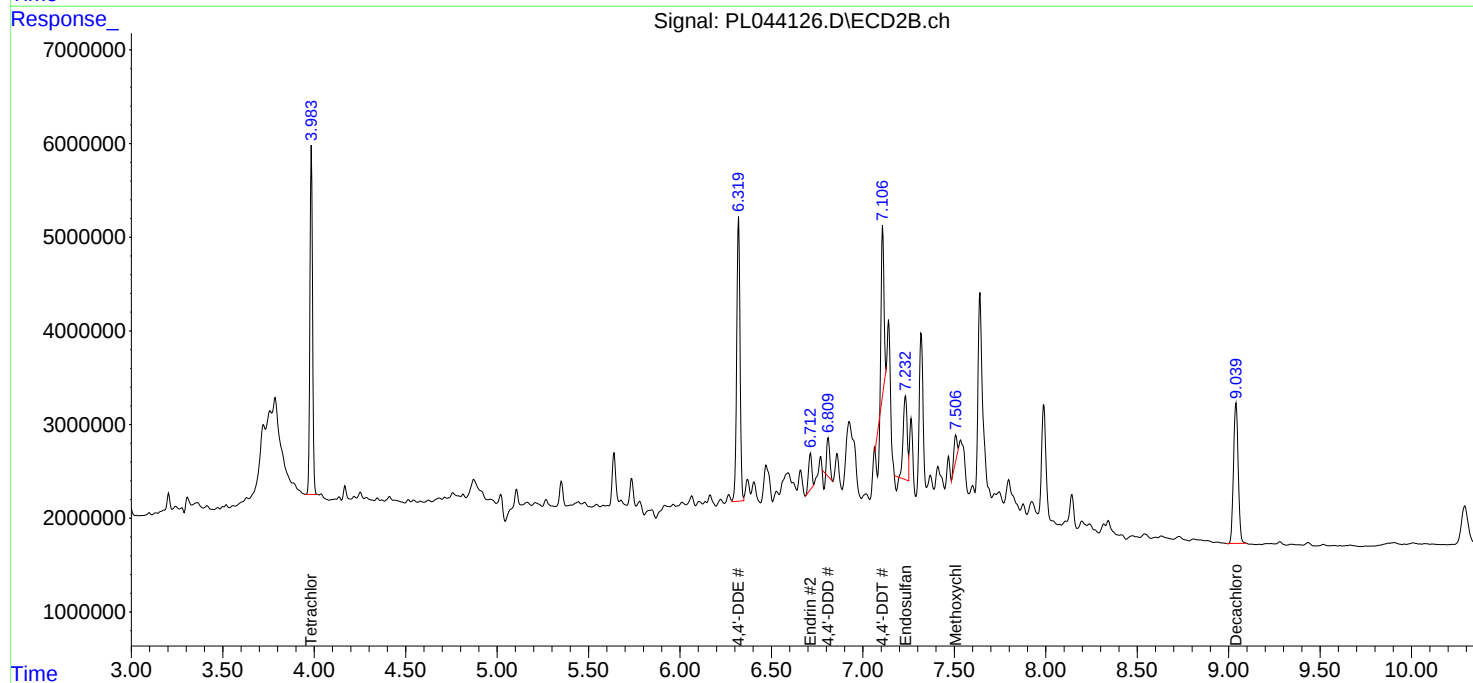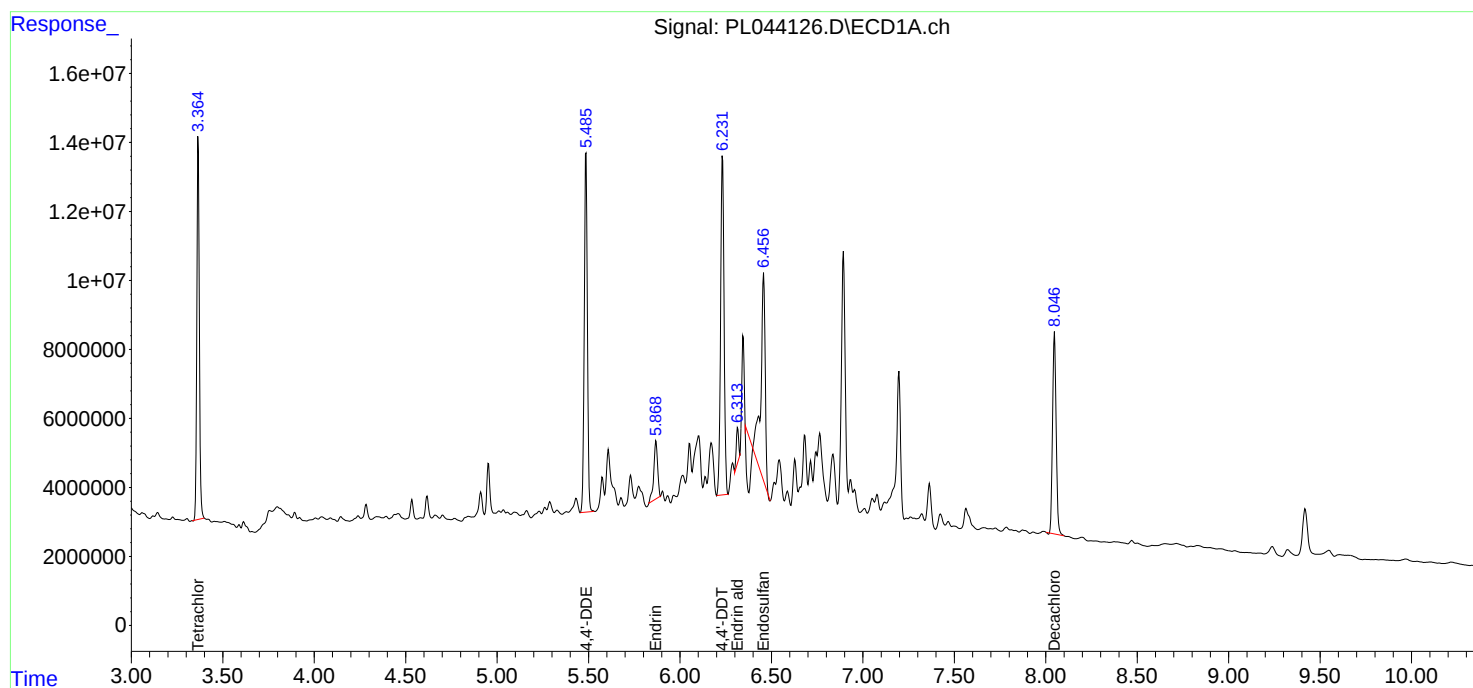


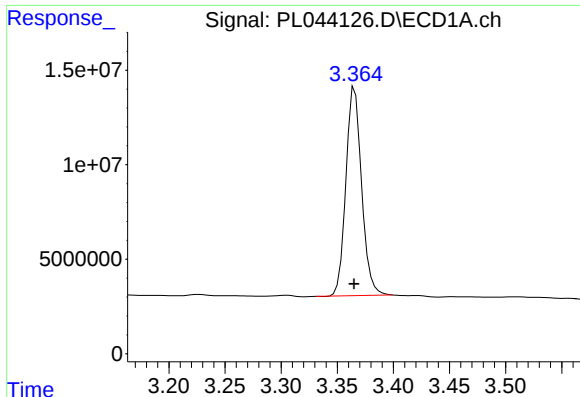

#1 Tetrachloro-m-xylene


R.T.: 3.366 min
Delta R.T.: 0.000 min
Response: 107401236
Conc: 17.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB6-011619-S-001

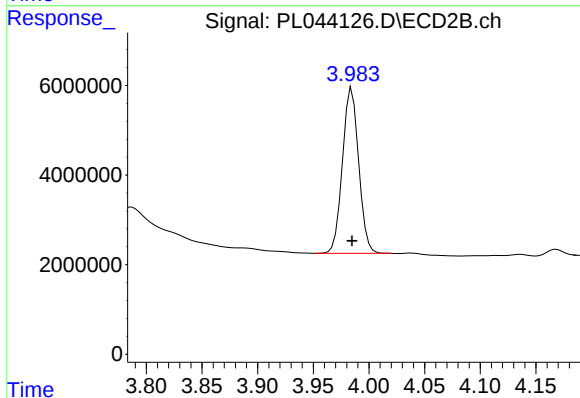


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 37355611
Conc: 17.13 ng/ml

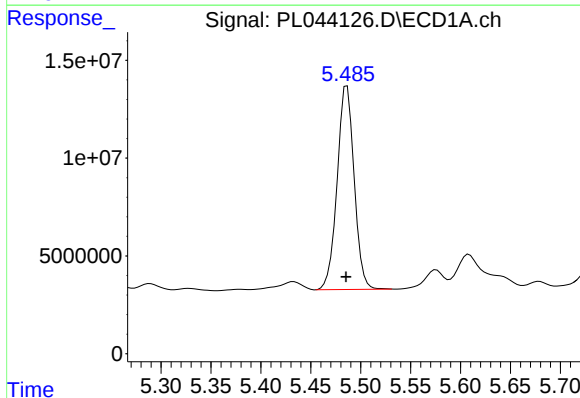


#12 4,4'-DDE

R.T.: 5.486 min
Delta R.T.: 0.000 min
Response: 123551501
Conc: 18.24 ng/ml

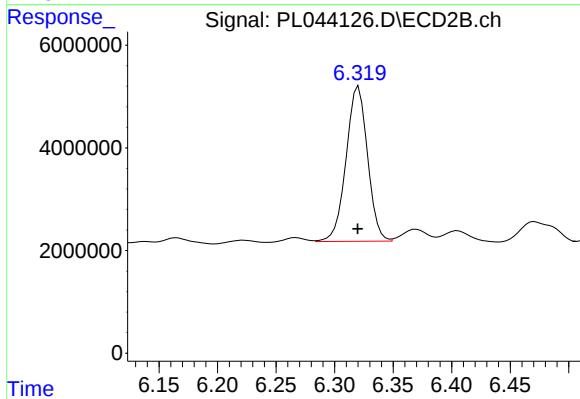

#12 4,4'-DDE


R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 38493952
Conc: 17.94 ng/ml

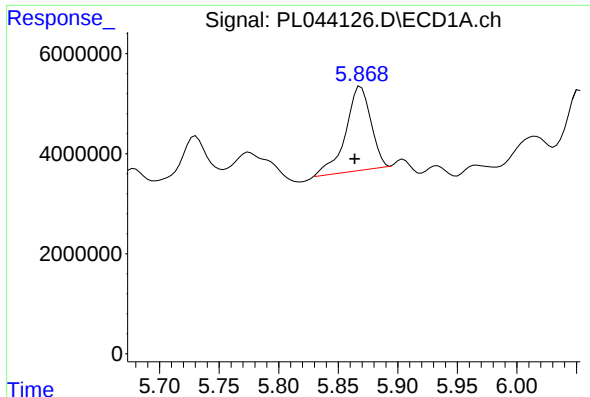

#14 Endrin


R.T.: 5.869 min
Delta R.T.: 0.005 min
Response: 24733512
Conc: 3.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB6-011619-S-001

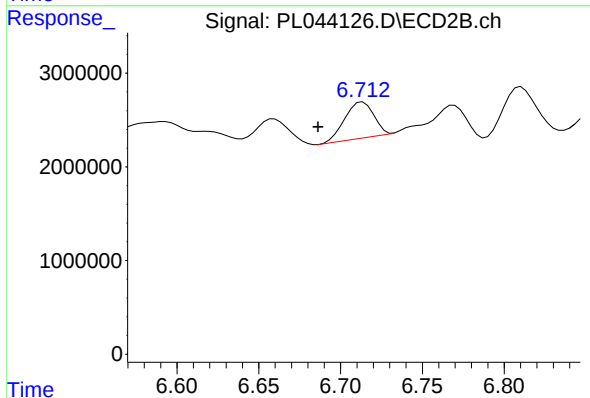


#14 Endrin

R.T.: 6.714 min
Delta R.T.: 0.027 min
Response: 4733695
Conc: 2.35 ng/ml

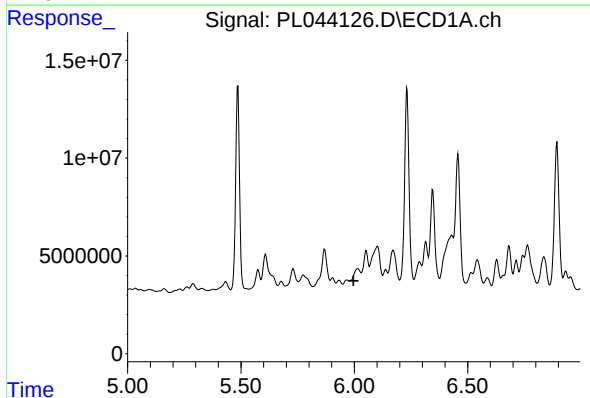


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.997 min
Response: 0
Conc: N.D.

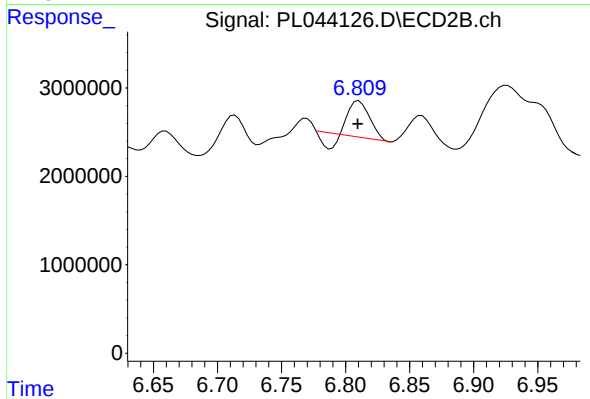

#16 4,4'-DDD


R.T.: 6.810 min
Delta R.T.: 0.000 min
Response: 3809558
Conc: 2.22 ng/ml

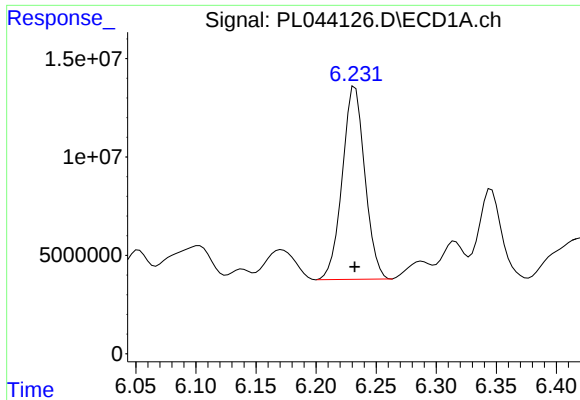

#17 4,4'-DDT


R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 128207918
Conc: 25.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB6-011619-S-001

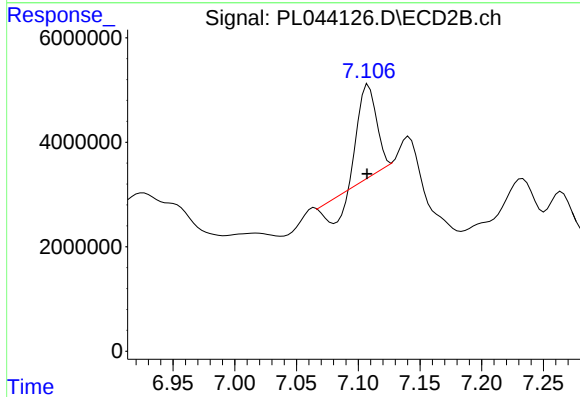


#17 4,4'-DDT

R.T.: 7.108 min
Delta R.T.: 0.001 min
Response: 14063367
Conc: 8.57 ng/ml

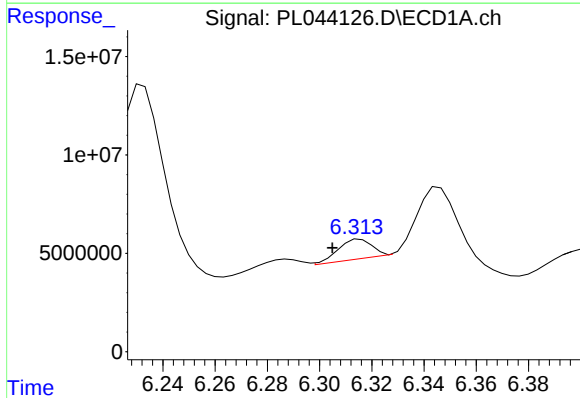


#18 Endrin aldehyde

R.T.: 6.316 min
Delta R.T.: 0.011 min
Response: 8882797
Conc: 1.57 ng/ml

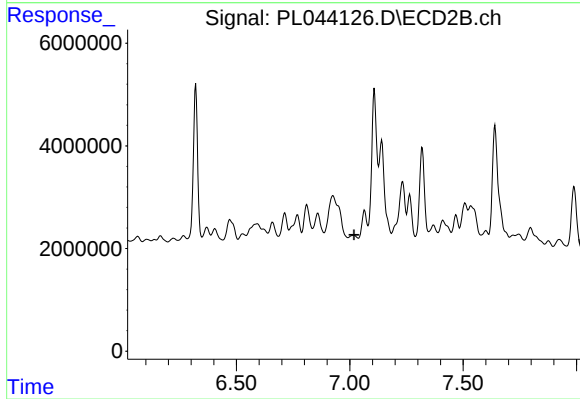

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.019 min
Response: 0
Conc: N.D.

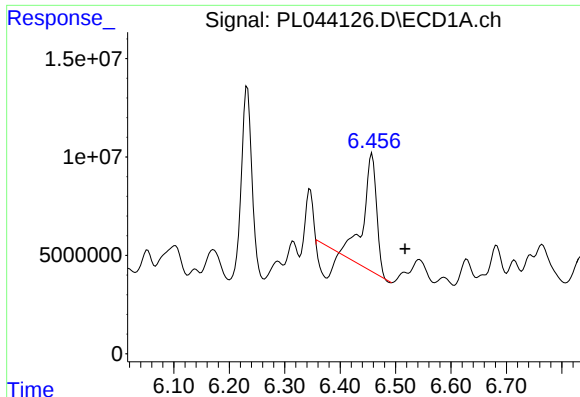

#19 Endosulfan Sulfate


R.T.: 6.457 min
Delta R.T.: -0.059 min
Response: 82213409
Conc: 14.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB6-011619-S-001

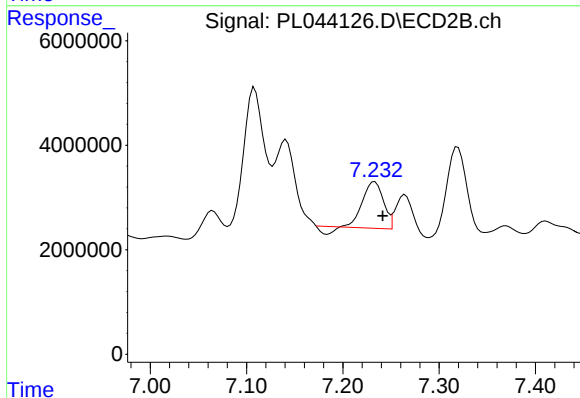


#19 Endosulfan Sulfate

R.T.: 7.233 min
Delta R.T.: -0.008 min
Response: 12816976
Conc: 6.67 ng/ml

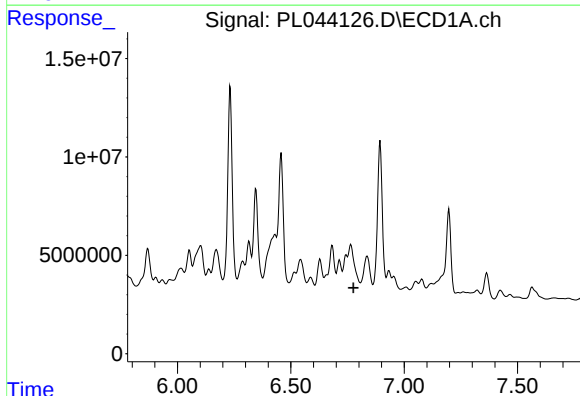


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.777 min
Response: 0
Conc: N.D.

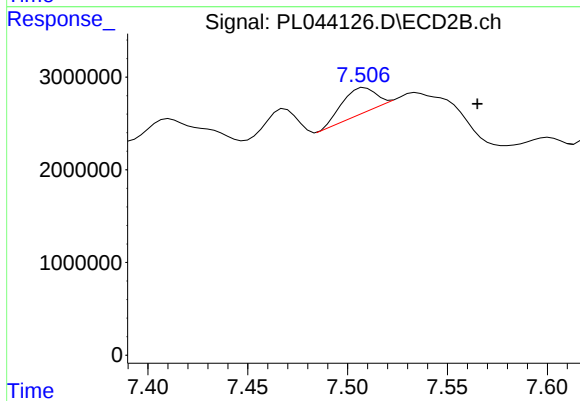

#20 Methoxychlor


R.T.: 7.509 min
Delta R.T.: -0.056 min
Response: 3444608
Conc: 3.37 ng/ml

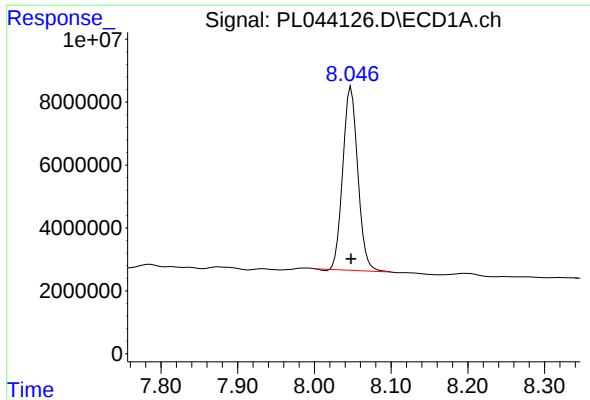

#28 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: 0.000 min
Response: 79640676
Conc: 11.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB6-011619-S-001

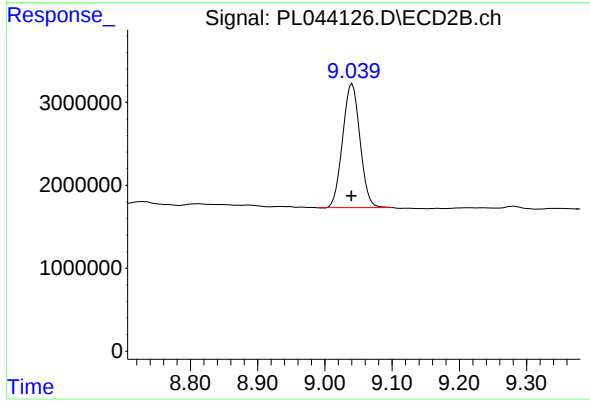

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.001 min
Response: 26740758
Conc: 12.05 ng/ml