

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012220\
 Data File : PL055991.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2020 14:02
 Operator : AJ\MA
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 16:57:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.491	3.963	535.5E6	142.5E6	55.872	50.413
28)	SA Decachlor...	8.236	8.952	534.9E6	109.4E6	51.162	47.744
Target Compounds							
23)	Chlordane-1	4.361	4.940	183.3E6	52942520	499.957	502.788
24)	Chlordane-2	4.862	5.401	214.7E6	54211395	496.033	491.729
25)	Chlordane-3	5.431	6.039	648.6E6	195.0E6	520.873	491.167
26)	Chlordane-4	5.488	6.112	533.4E6	228.7E6	517.272	487.162
27)	Chlordane-5	6.323	6.908	199.0E6	41564636	508.723	507.343



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012220\
Data File : PL055991.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2020 14:02
Operator : AJ\MA
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 16:57:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

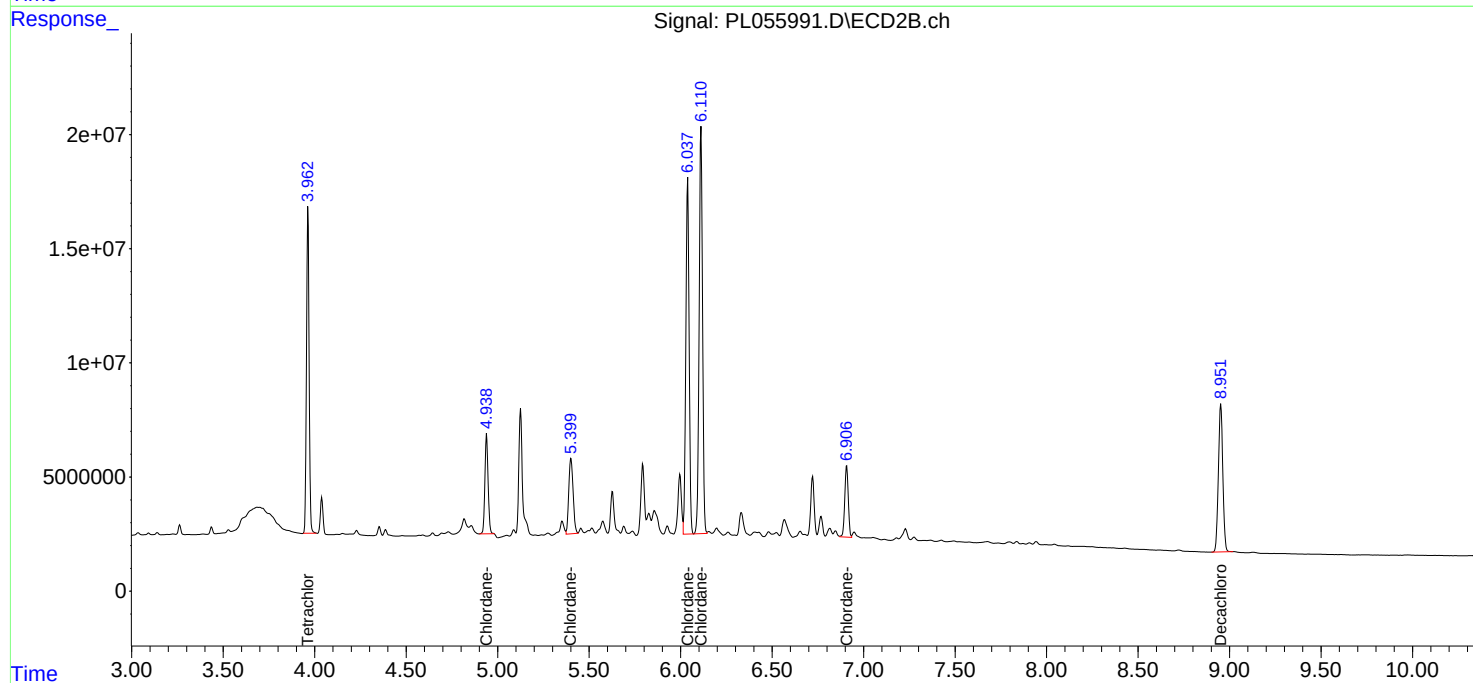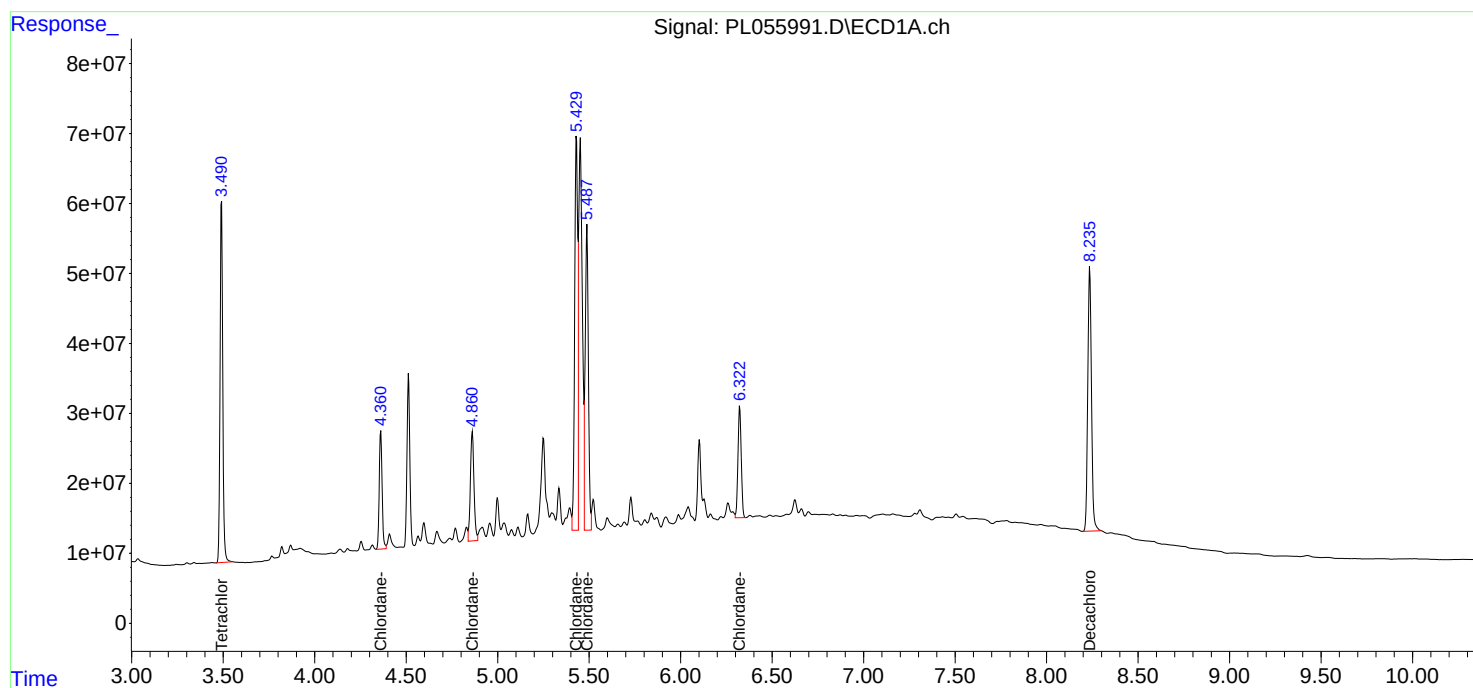


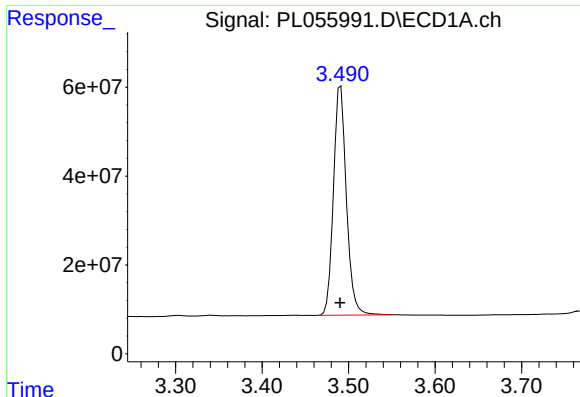

#1 Tetrachloro-m-xylene


R.T.: 3.491 min
Delta R.T.: 0.001 min
Response: 535502907
Conc: 55.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

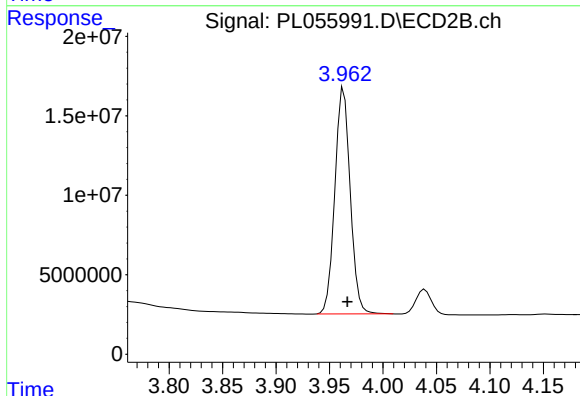


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: -0.003 min
Response: 142478525
Conc: 50.41 ng/ml

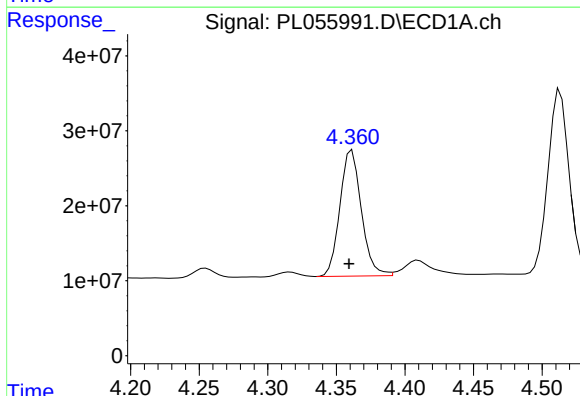


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.002 min
Response: 183304922
Conc: 499.96 ng/ml

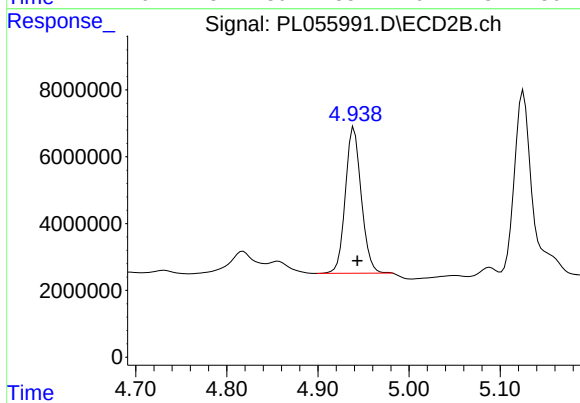

#23 Chlordane-1


R.T.: 4.940 min
Delta R.T.: -0.004 min
Response: 52942520
Conc: 502.79 ng/ml

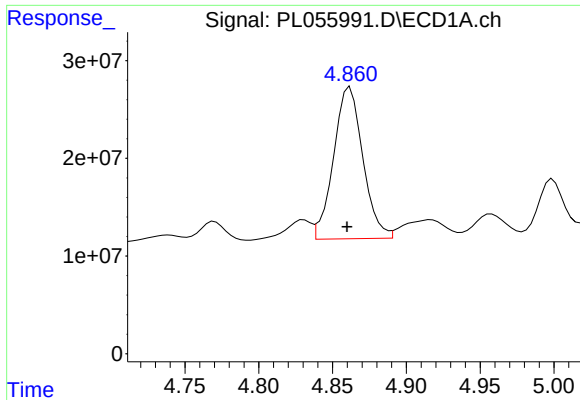

#24 Chlordane-2


R.T.: 4.862 min
Delta R.T.: 0.002 min
Response: 214656087
Conc: 496.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

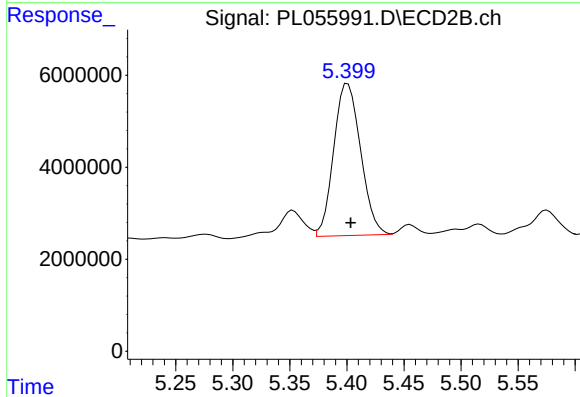


#24 Chlordane-2

R.T.: 5.401 min
Delta R.T.: -0.002 min
Response: 54211395
Conc: 491.73 ng/ml

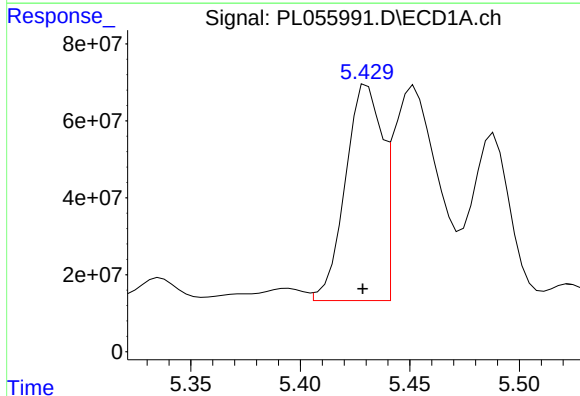


#25 Chlordane-3

R.T.: 5.431 min
Delta R.T.: 0.002 min
Response: 648637929
Conc: 520.87 ng/ml

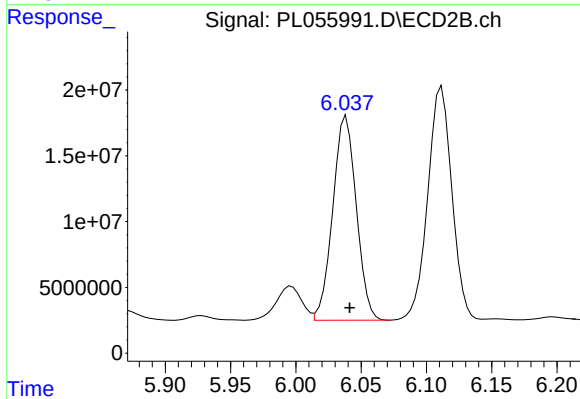

#25 Chlordane-3


R.T.: 6.039 min
Delta R.T.: -0.003 min
Response: 194952563
Conc: 491.17 ng/ml

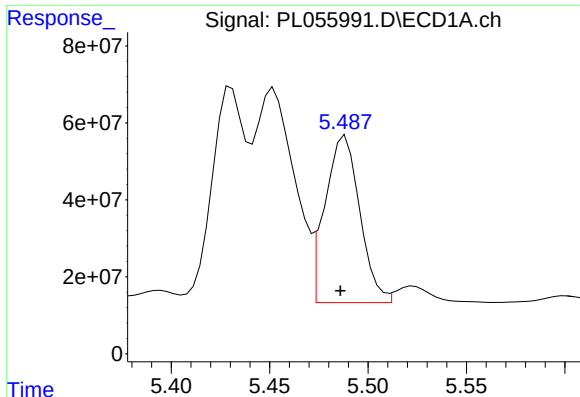

#26 Chlordane-4


R.T.: 5.488 min
Delta R.T.: 0.003 min
Response: 533383962
Conc: 517.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

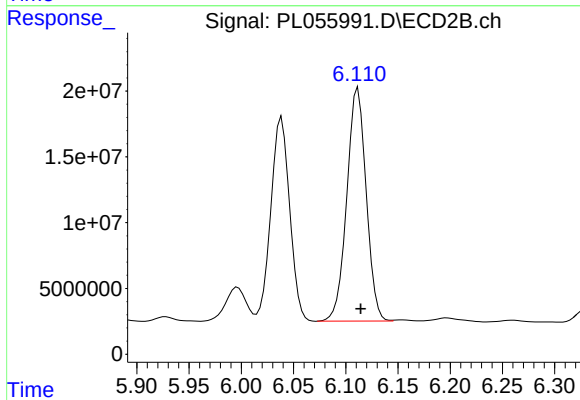


#26 Chlordane-4

R.T.: 6.112 min
Delta R.T.: -0.003 min
Response: 228686075
Conc: 487.16 ng/ml

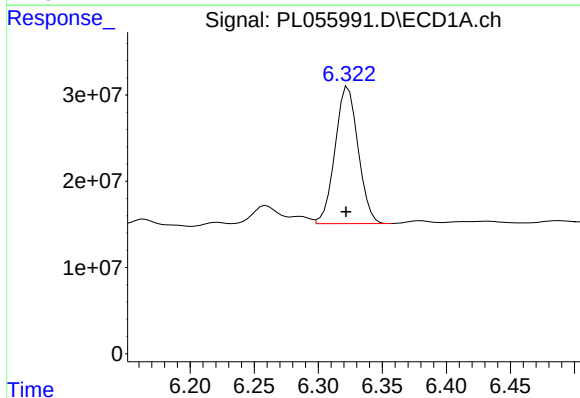


#27 Chlordane-5

R.T.: 6.323 min
Delta R.T.: 0.002 min
Response: 198969278
Conc: 508.72 ng/ml

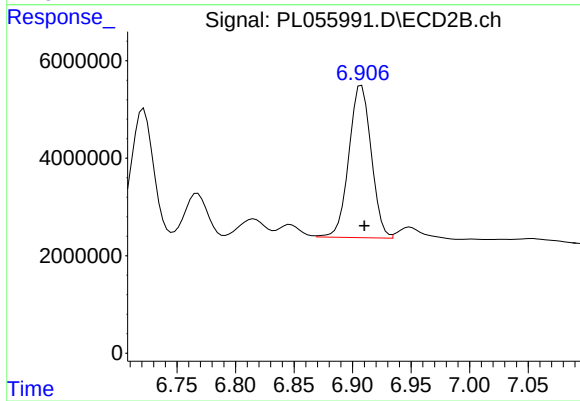

#27 Chlordane-5


R.T.: 6.908 min
Delta R.T.: -0.002 min
Response: 41564636
Conc: 507.34 ng/ml

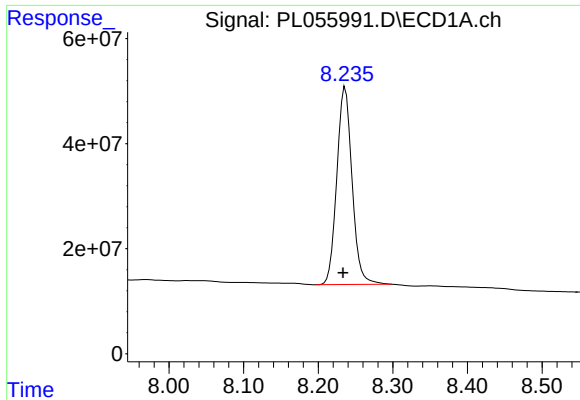

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: 0.003 min
Response: 534935365
Conc: 51.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

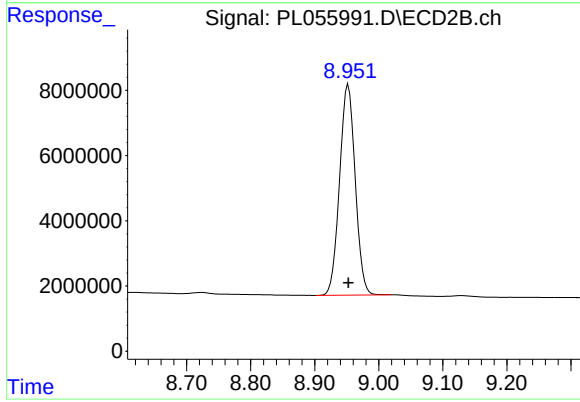

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: 0.000 min
Response: 109379622
Conc: 47.74 ng/ml