

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012220\
 Data File : PL055996.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2020 15:16
 Operator : AJ\MA
 Sample : L1213-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Ankita
 1/23/2020 9:46:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 16:57:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	3.966	136.8E6	36243689	14.275	12.824
28)	SA Decachlor...	8.233	8.952	130.9E6	32542003	12.519	14.204
Target Compounds							
12)	B 4,4'-DDE	5.648	6.265	12344687	3904639	0.945	1.333m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012220\
Data File : PL055996.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2020 15:16
Operator : AJ\MA
Sample : L1213-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
1/23/2020 9:46:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 16:57:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

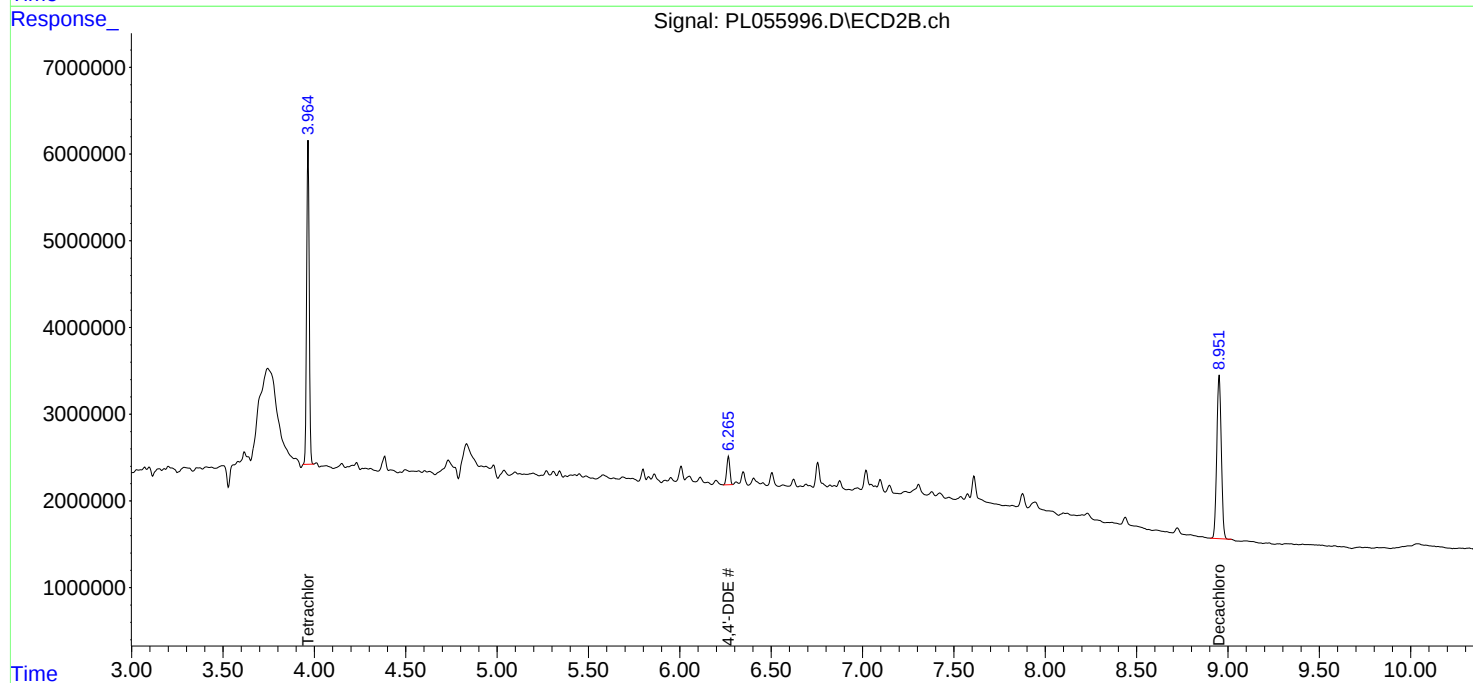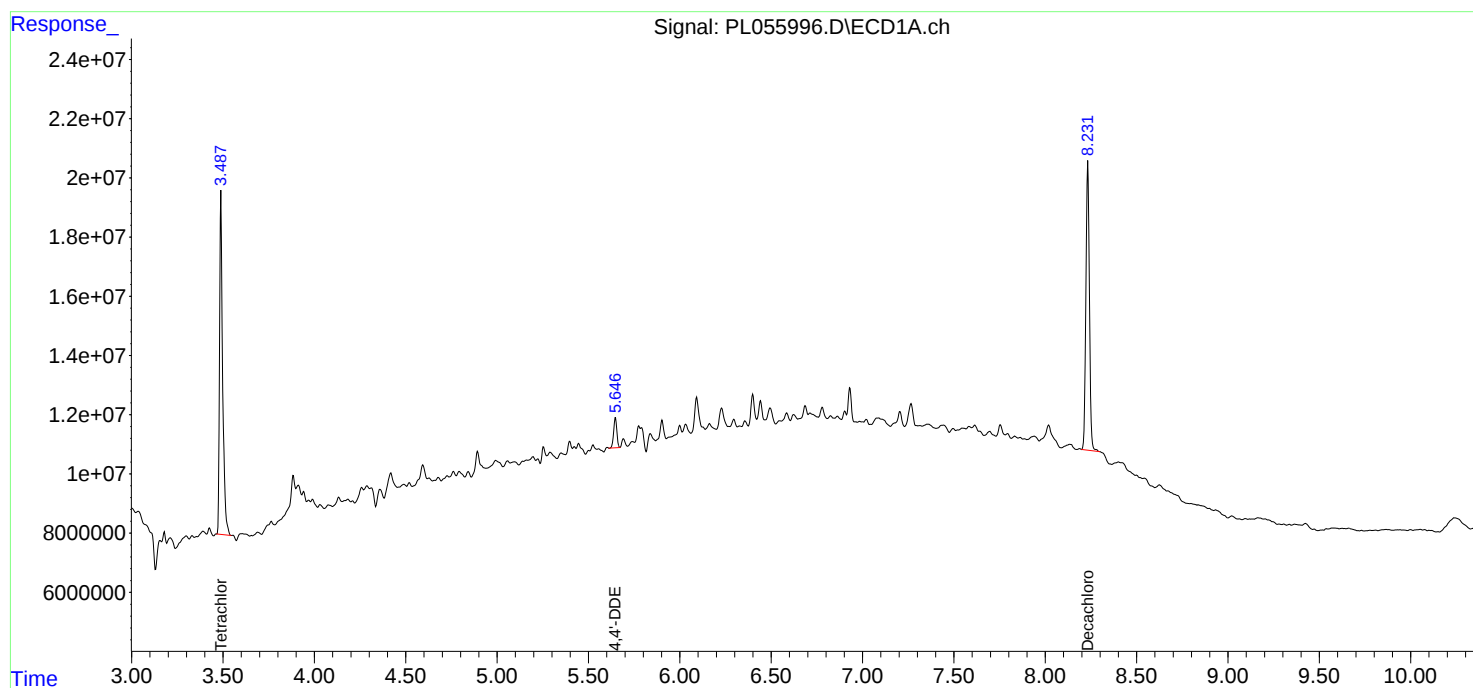

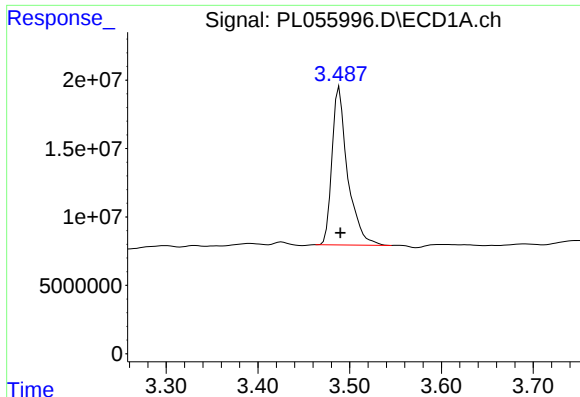


#1 Tetrachloro-m-xylene

R.T.: 3.489 min
Delta R.T.: -0.001 min
Response: 136818333
Conc: 14.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
1/23/2020 9:46:01 AM

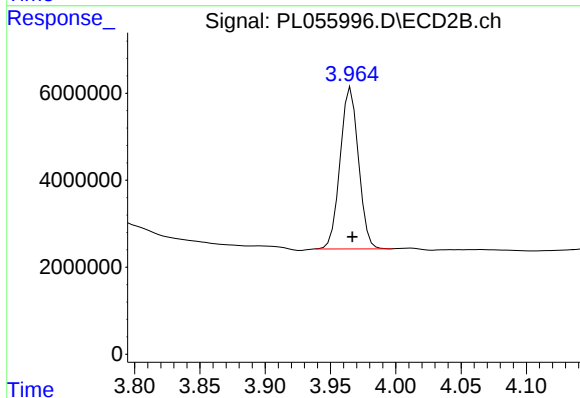


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: -0.001 min
Response: 36243689
Conc: 12.82 ng/ml

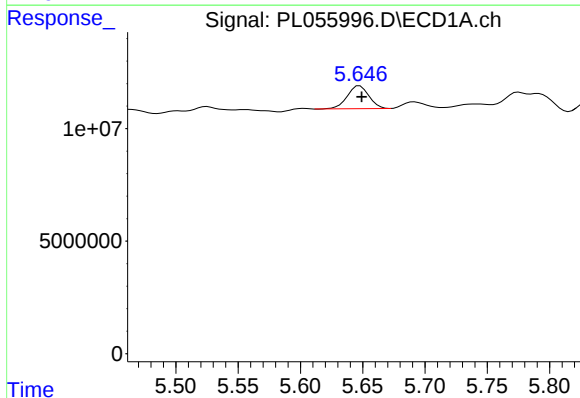


#12 4,4'-DDE

R.T.: 5.648 min
Delta R.T.: -0.002 min
Response: 12344687
Conc: 0.95 ng/ml

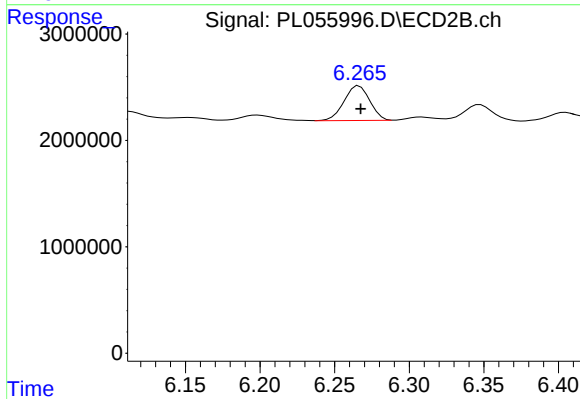

#12 4,4'-DDE

R.T.: 6.265 min
Delta R.T.: -0.002 min
Response: 3904639
Conc: 1.33 ng/ml m

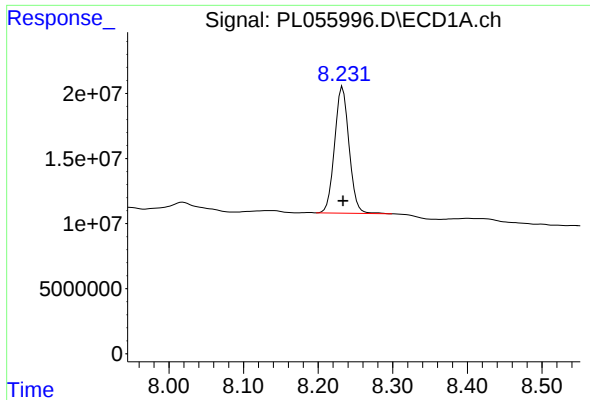


#28 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: 0.000 min
Response: 130890413
Conc: 12.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

Manual Integrations
APPROVED

Ankita
1/23/2020 9:46:01 AM

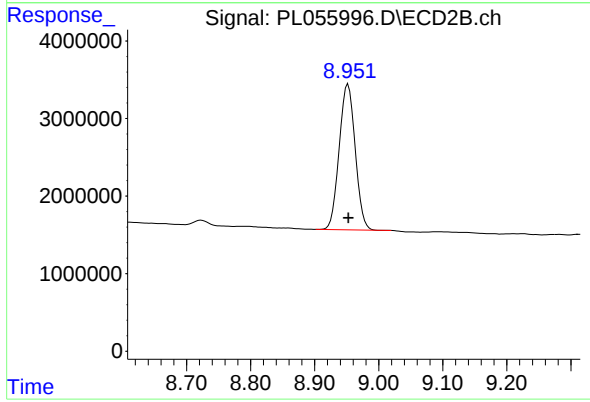

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: 0.000 min
Response: 32542003
Conc: 14.20 ng/ml