

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012221\
 Data File : PL064292.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2021 10:00
 Operator : AR\AJ
 Sample : L5214-02
 Misc : TOX MDL 100 PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT1-2021-02

Manual Integrations
 APPROVED

Ankita
 1/22/2021 9:58:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 04:35:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012121CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 21 03:31:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	4.109	62826373	48727858	21.605	20.200
27)	SA Decachlor...	8.170	9.273	116.9E6	89021387	38.837	38.355
Target Compounds							
22)	Toxaphene-1	5.678	6.540	3406382	1622320	118.301	99.247
23)	Toxaphene-2	6.274	6.833	8483440	2012032	108.756	112.002m
24)	Toxaphene-3	6.521	7.321	8758162	5224821	103.524	97.189
25)	Toxaphene-4	6.872	7.409	5780385	4733281	93.727	89.613
26)	Toxaphene-5	7.003	7.830	9519342	4129839	112.516	100.084

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012221\
Data File : PL064292.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2021 10:00
Operator : AR\AJ
Sample : L5214-02
Misc : TOX MDL 100 PPB
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 04:35:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012121CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 21 03:31:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

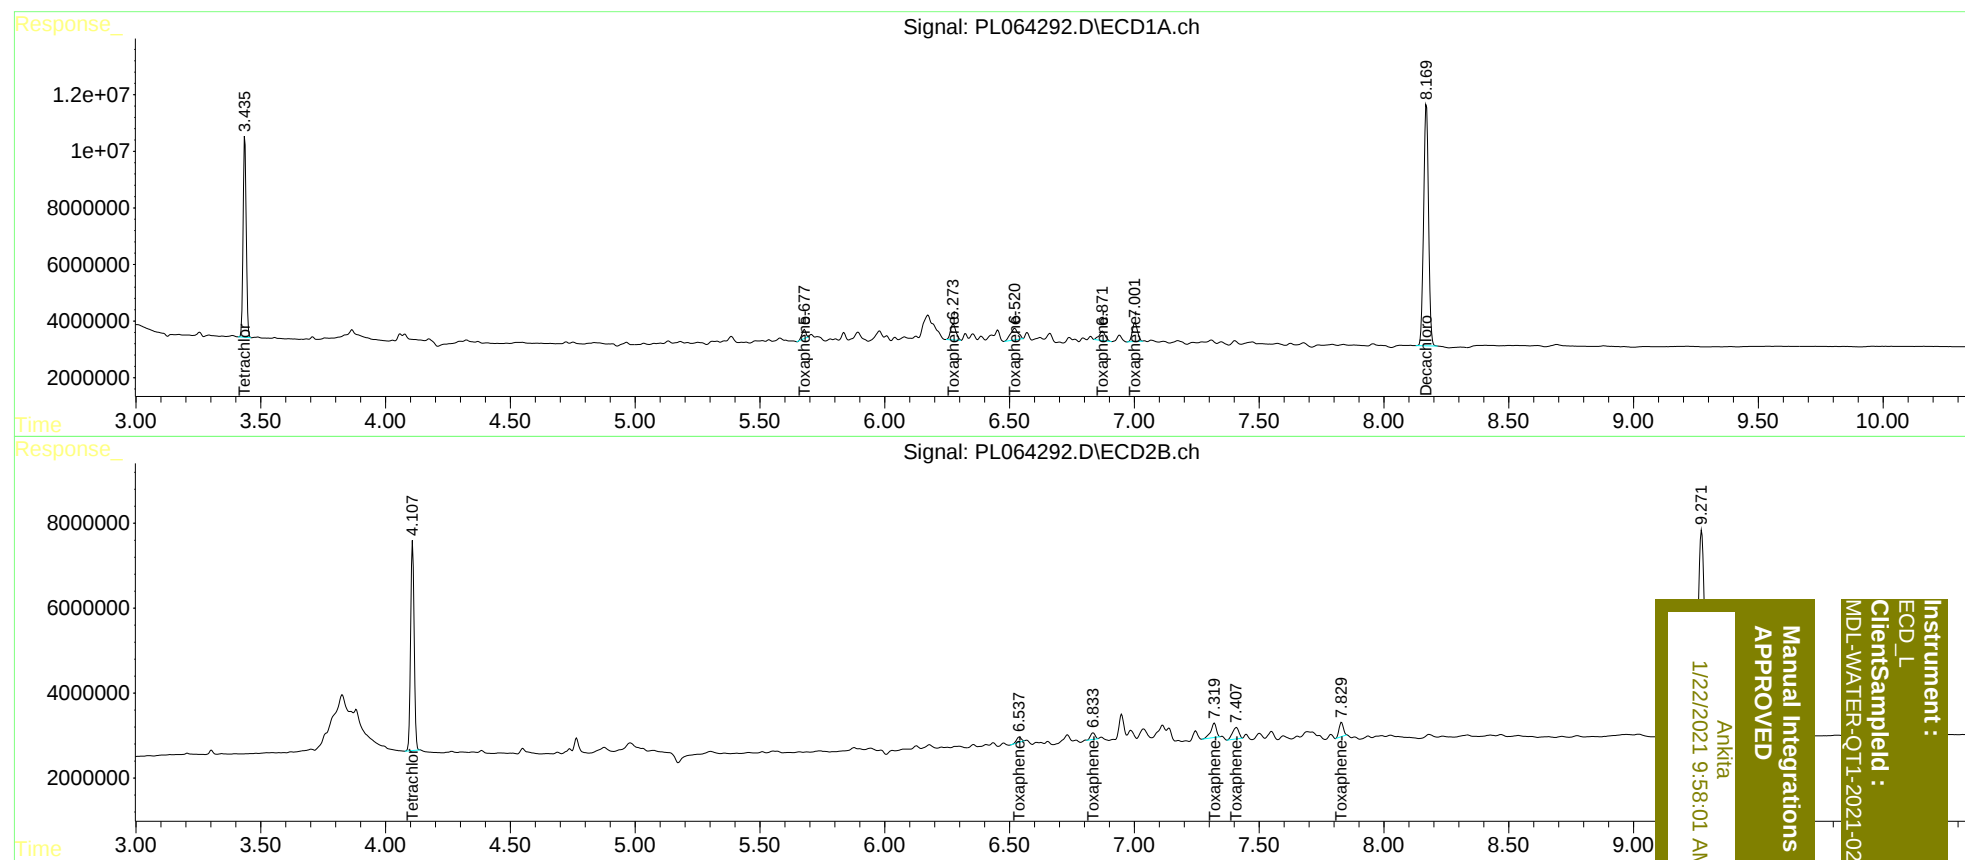

12.276
Ankita
1/22/2021 9:58:01 AM

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sample :
MDL-WATER-QT1-2021-02