

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012221\
 Data File : PL064291.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2021 09:45
 Operator : AR\AJ
 Sample : L5214-02
 Misc : PEST MDL 1 PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT1-2021-02

Manual Integrations
 APPROVED

Ankita
 1/22/2021 9:57:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 01:58:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012121CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 21 03:31:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.108	66829733	54345544	22.982	22.529
27)	SA Decachlor...	8.168	9.272	131.3E6	98864988	43.629	42.596
Target Compounds							
2)	A alpha-BHC	3.868	4.509	4702787	2622588	1.052	0.826
3)	MA gamma-BHC...	4.149	4.802	3637408	2504082	0.842	0.821
4)	MA Heptachlor	4.448	5.314	4497828	4075838	1.065	1.255
5)	MB Aldrin	4.694	5.625	3693497	2845040	0.953	0.985
6)	B beta-BHC	4.397	4.979	1764547	3197475	0.956m	1.800 #
7)	B delta-BHC	4.600	5.200	4086959	2793224	0.987	1.022
8)	B Heptachlo...	5.135	6.021	4074884	2120659	1.098	0.886
9)	A Endosulfan I	5.471	6.382	3459613	2591513	1.009	1.008
10)	B trans-Chl...	5.361	6.253	4276661	2763350	1.101	0.964m
11)	B cis-Chlor...	5.419	6.328	4132519	3057457	1.095	1.053
12)	B 4,4'-DDE	5.586	6.484	3790847	1987367	1.070	0.750 #
13)	MA Dieldrin	5.713	6.643	3668428	2565492	0.960	0.921
14)	MA Endrin	5.967	6.863	3688587	1904265	1.076m	0.831m
15)	B Endosulfa...	6.240	7.076	3439960	2430860	1.122	1.077m
16)	A 4,4'-DDD	6.098	6.980	2617473	2443359	0.899	1.091m
17)	MA 4,4'-DDT	6.340	7.283	2731014	1205948	0.913	0.565 #
18)	B Endrin al...	6.409	7.203	3120366	2006054	1.185	1.016
19)	B Endosulfa...	6.620	7.427	3626357	2334770	1.135m	1.037
20)	A Methoxychlor	6.886	7.741	1598393	990374	1.008	0.786m
21)	B Endrin ke...	7.107	7.906	3575556	2042853	1.064	0.909

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012221\
Data File : PL064291.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2021 09:45
Operator : AR\AJ
Sample : L5214-02
Misc : PEST MDL 1 PPB
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 01:58:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012121CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 21 03:31:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

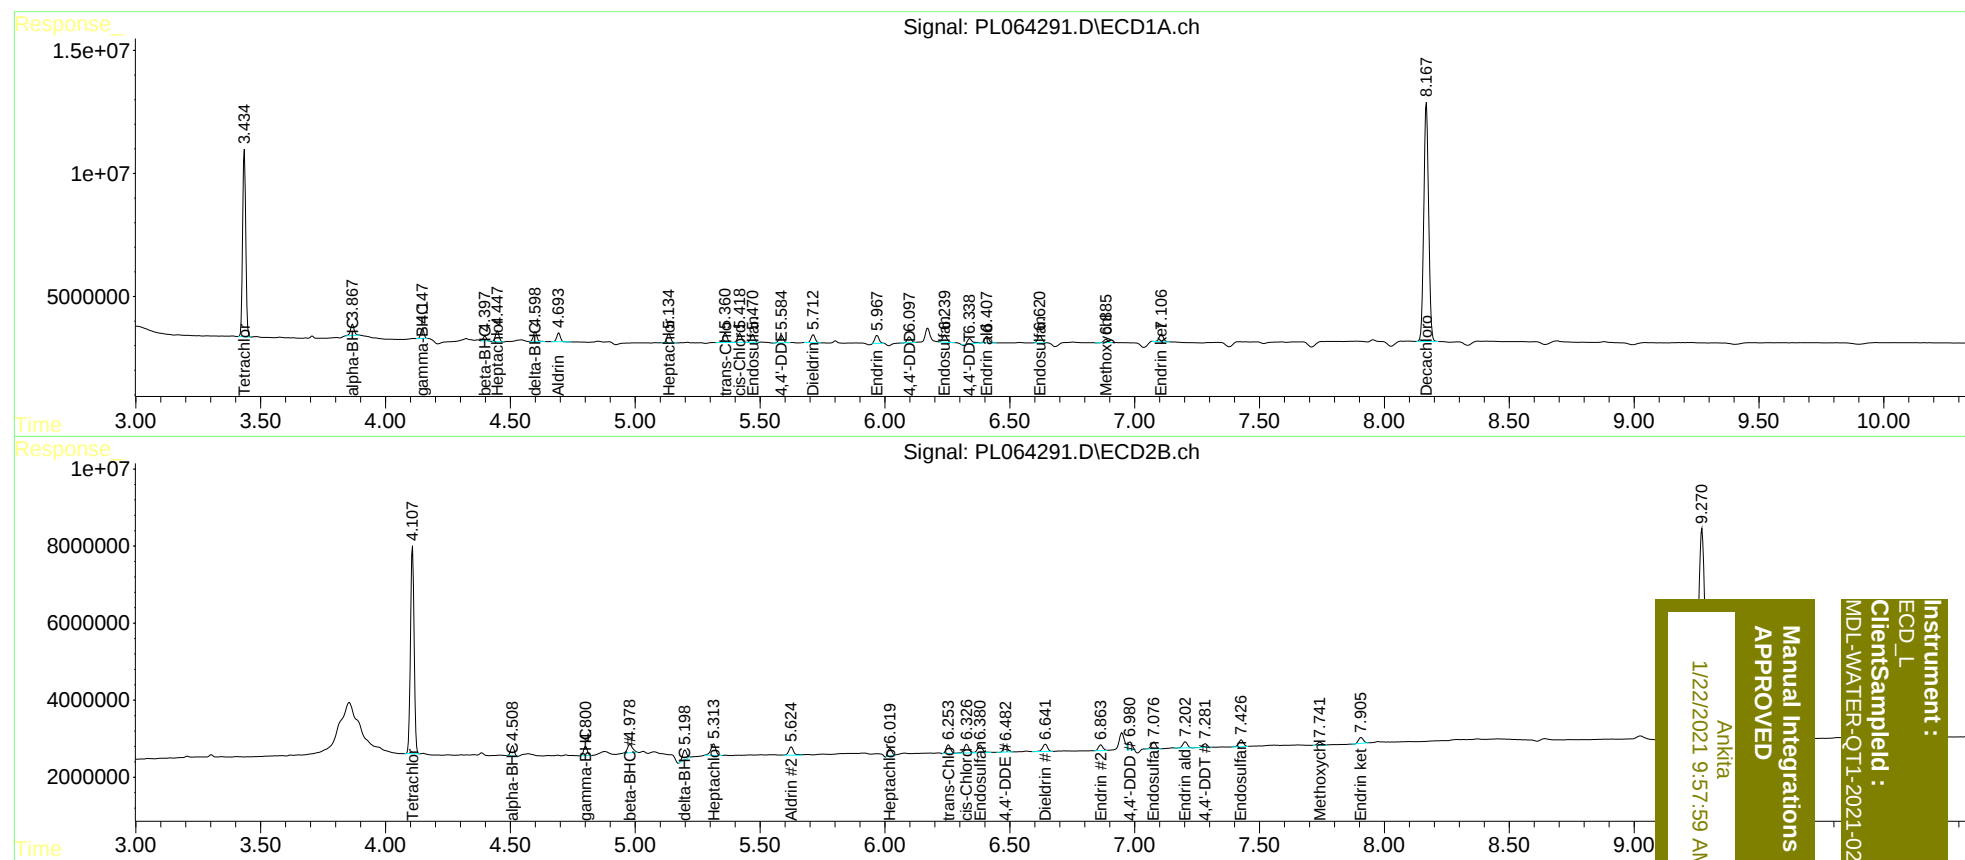

0.276
Ankita
1/22/2021 9:57:59 AM

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sample :
MDL-WATER-QT1-2021-02