

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012320\
 Data File : PL056004.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2020 10:10
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 16:59:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	8.257f	0.000	9066228	0	0.867	N.D. #
Target Compounds							
2)	A alpha-BHC	3.934	0.000	1569262	0	0.095	N.D. #
8)	B Heptachlo...	5.215	5.794f	2756204	461857	0.200	0.155
9)	A Endosulfan I	5.537	0.000	2714991	0	0.209	N.D. #
11)	B alpha-Chl...	5.490	0.000	16216105	0	1.173	N.D. #
14)	MA Endrin	6.062f	6.638	7883161	603141	0.624	0.238 #
16)	A 4,4'-DDD	6.162	0.000	3438563	0	0.345	N.D. #
19)	B Endosulfa...	6.715f	0.000	14440118	0	1.335	N.D. #
21)	B Endrin ke...	7.164f	0.000	5457579	0	0.434	N.D. #
24)	Chlordane-2	4.863	0.000	8999301	0	20.796	N.D. #
26)	Chlordane-4	5.490	0.000	16216105	0	15.726	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012320\
Data File : PL056004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2020 10:10
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 16:59:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

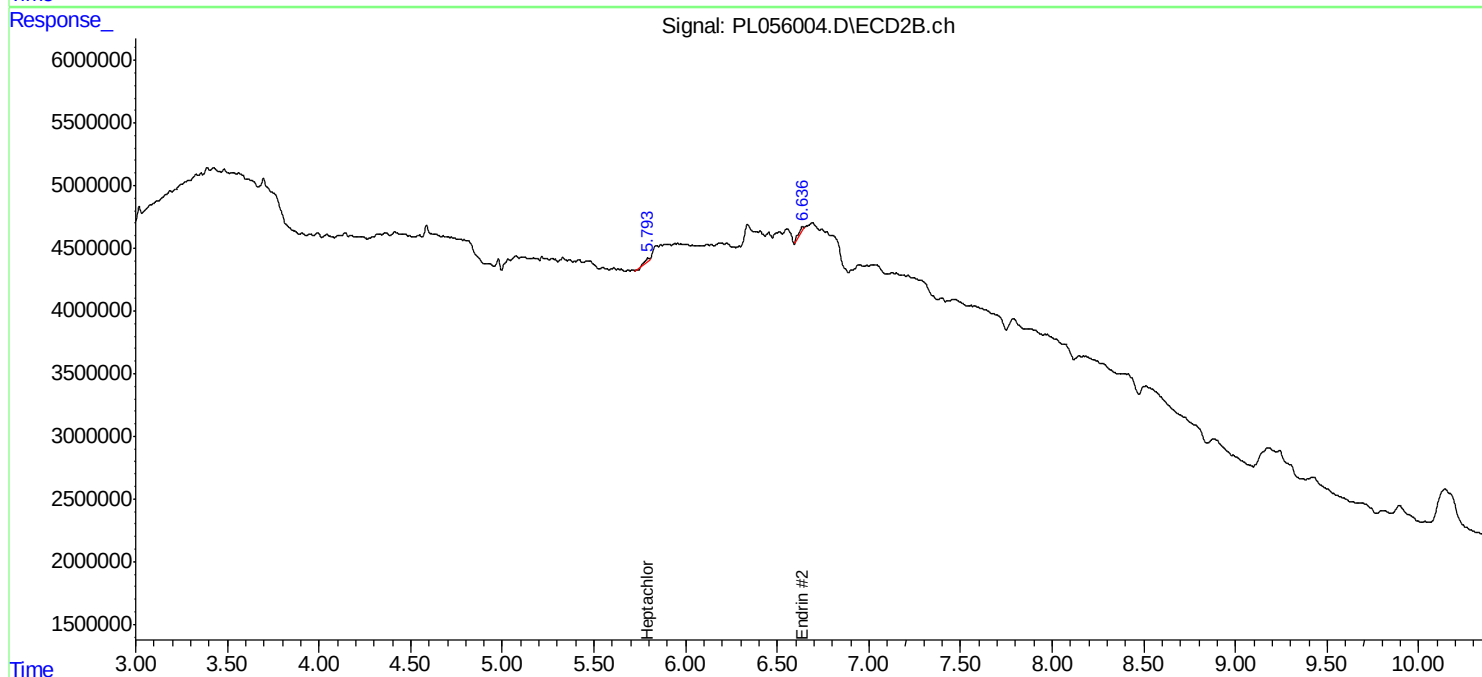


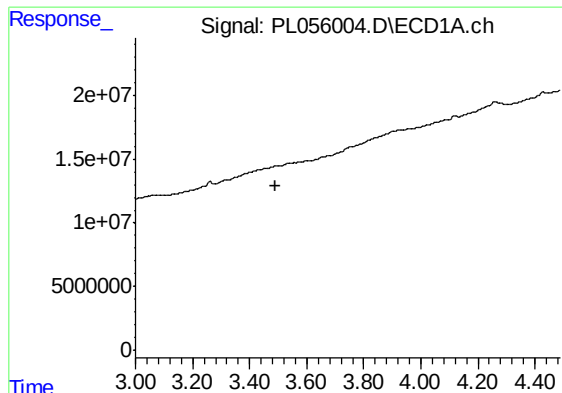

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

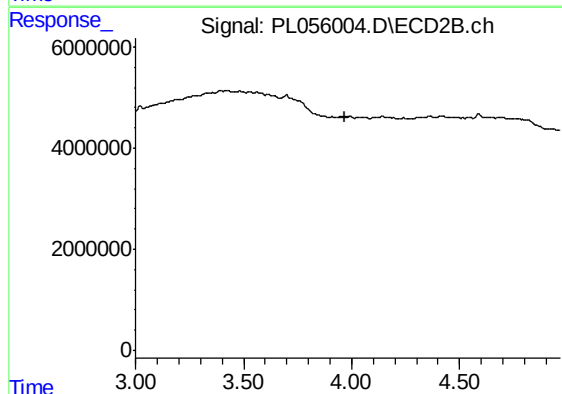


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.967 min
Response: 0
Conc: N.D.

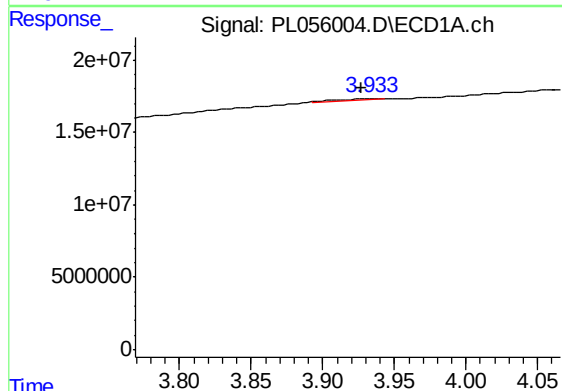


#2 alpha-BHC

R.T.: 3.934 min
Delta R.T.: 0.007 min
Response: 1569262
Conc: 0.09 ng/ml

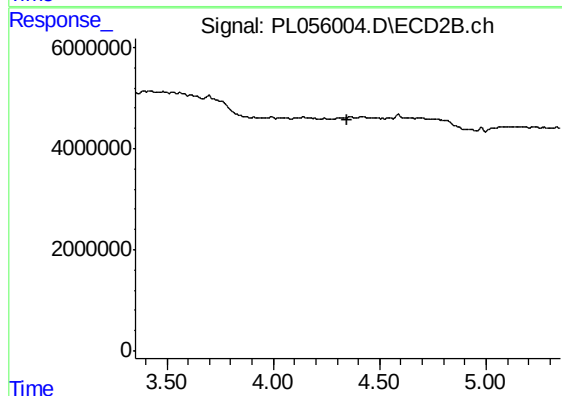

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.350 min
Response: 0
Conc: N.D.

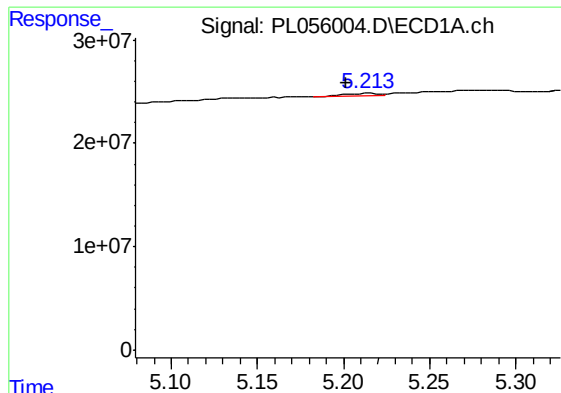

#8 Heptachlor epoxide


R.T.: 5.215 min
Delta R.T.: 0.014 min
Response: 2756204
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

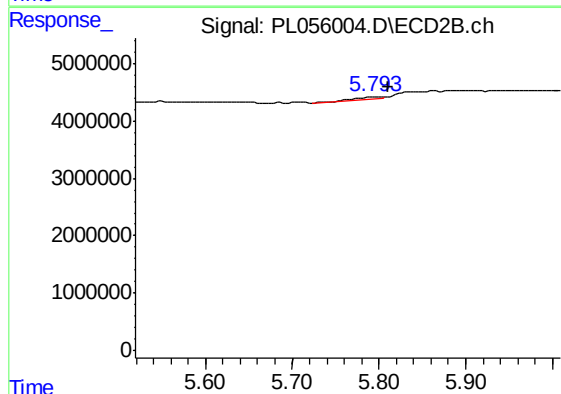


#8 Heptachlor epoxide

R.T.: 5.794 min
Delta R.T.: -0.016 min
Response: 461857
Conc: 0.15 ng/ml

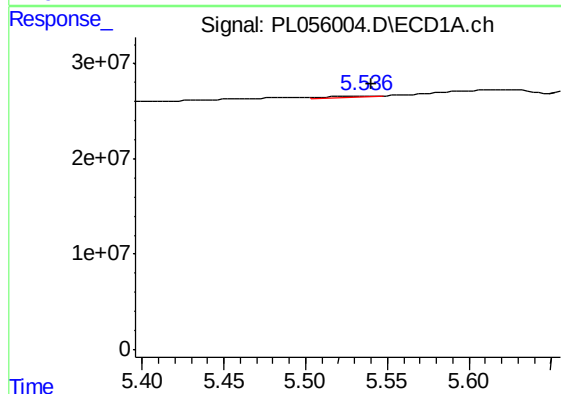


#9 Endosulfan I

R.T.: 5.537 min
Delta R.T.: -0.003 min
Response: 2714991
Conc: 0.21 ng/ml

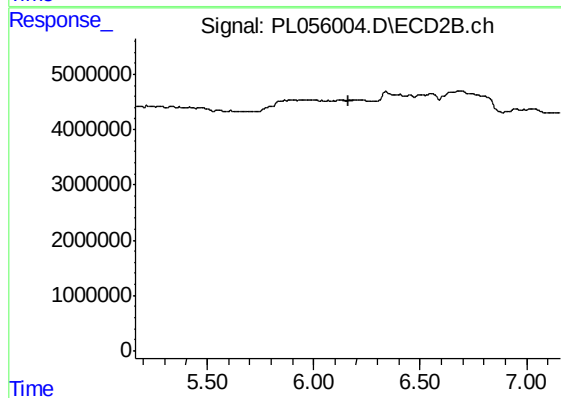

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

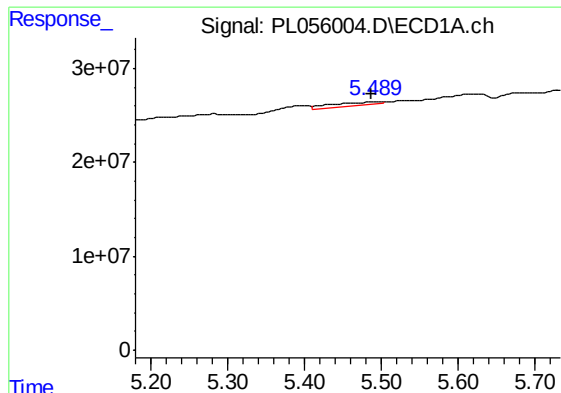

#11 alpha-Chlordane


R.T.: 5.490 min
Delta R.T.: 0.004 min
Response: 16216105
Conc: 1.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

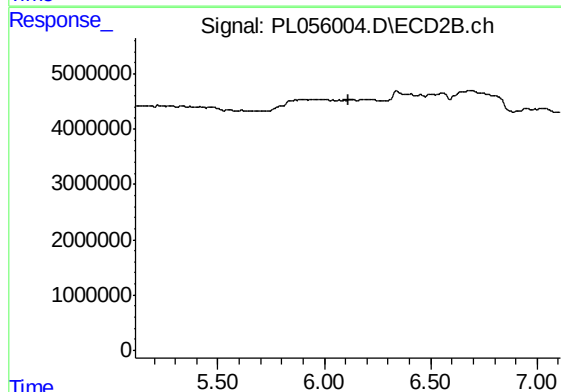


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

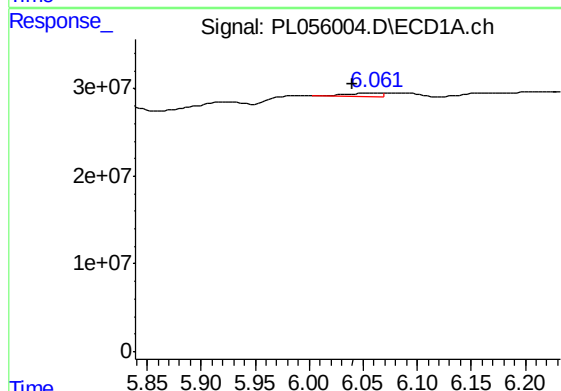


#14 Endrin

R.T.: 6.062 min
Delta R.T.: 0.022 min
Response: 7883161
Conc: 0.62 ng/ml

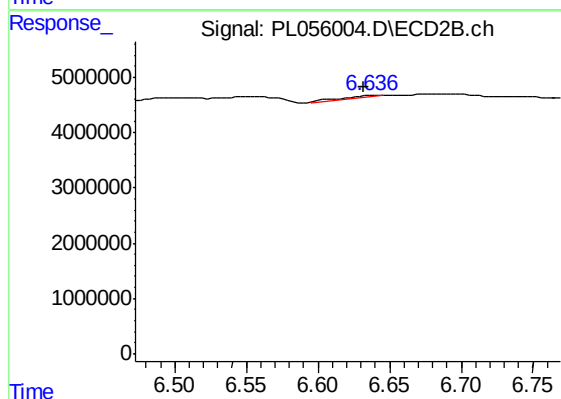

#14 Endrin


R.T.: 6.638 min
Delta R.T.: 0.006 min
Response: 603141
Conc: 0.24 ng/ml

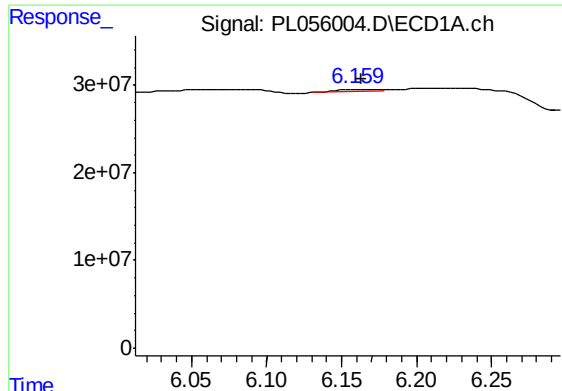

#16 4,4'-DDD


R.T.: 6.162 min
Delta R.T.: -0.002 min
Response: 3438563
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

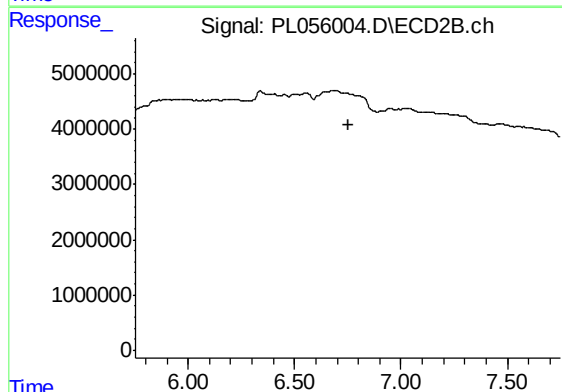


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.752 min
Response: 0
Conc: N.D.

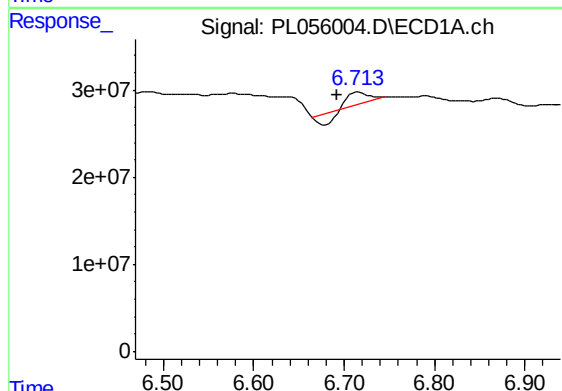


#19 Endosulfan Sulfate

R.T.: 6.715 min
Delta R.T.: 0.023 min
Response: 14440118
Conc: 1.34 ng/ml

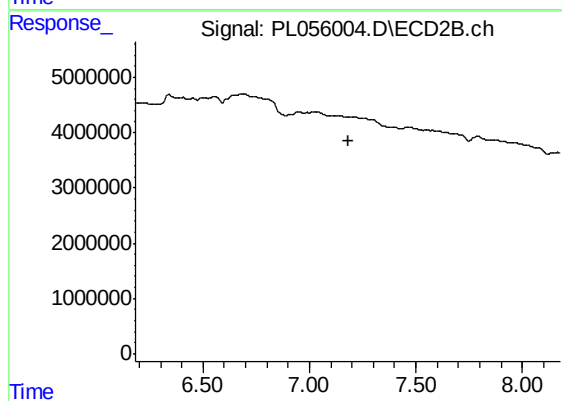

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

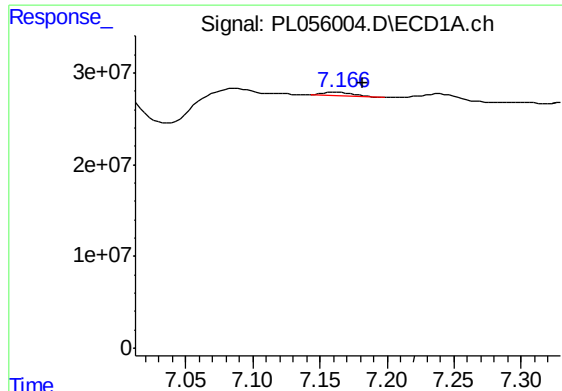

#21 Endrin ketone


R.T.: 7.164 min
Delta R.T.: -0.018 min
Response: 5457579
Conc: 0.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

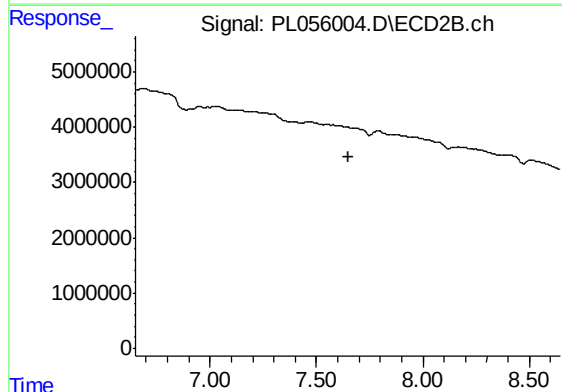


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.649 min
Response: 0
Conc: N.D.

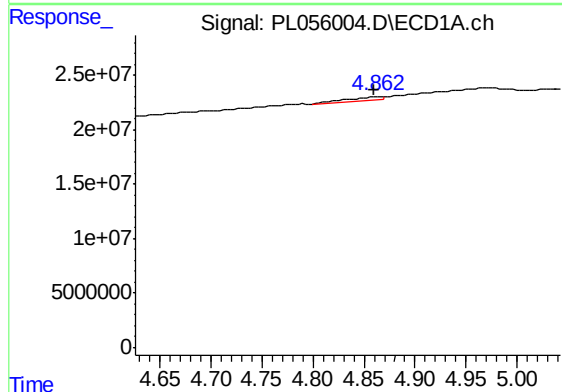


#24 Chlordane-2

R.T.: 4.863 min
Delta R.T.: 0.003 min
Response: 8999301
Conc: 20.80 ng/ml

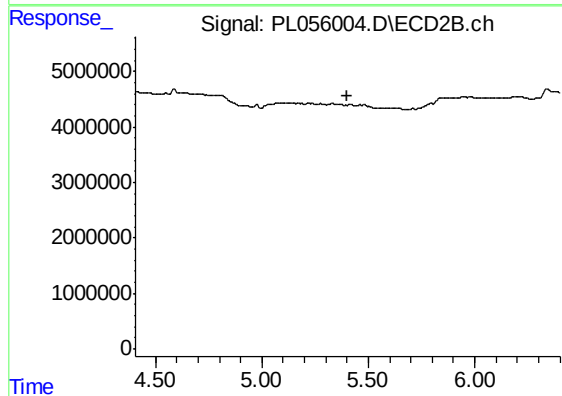

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.403 min
Response: 0
Conc: N.D.

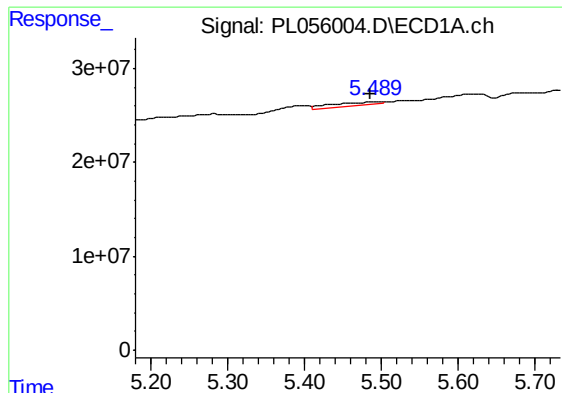

#26 Chlordane-4


R.T.: 5.490 min
Delta R.T.: 0.005 min
Response: 16216105
Conc: 15.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

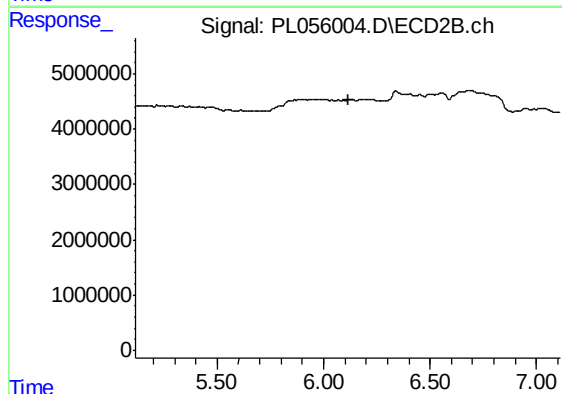


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

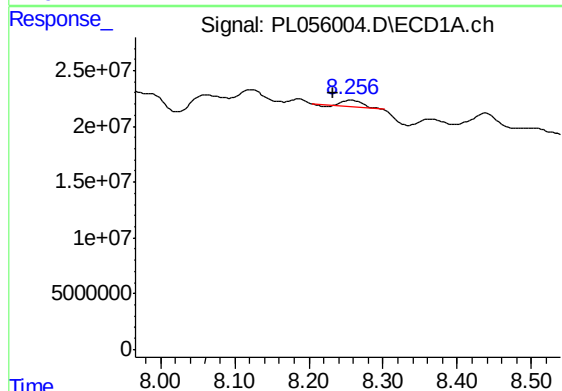

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.023 min
Response: 9066228
Conc: 0.87 ng/ml

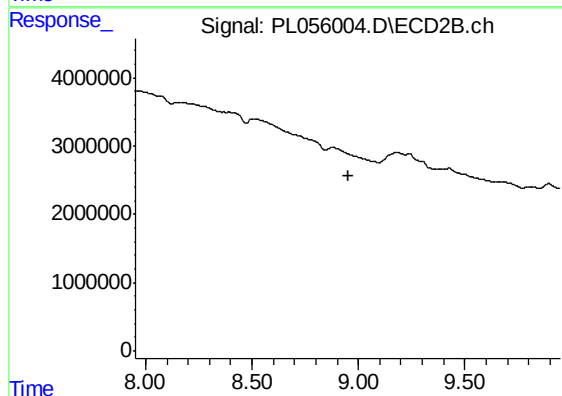

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.952 min
Response: 0
Conc: N.D.