

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012321\
 Data File : PL064300.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2021 12:32
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 17:02:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
3) MA	gamma-BHC...	0.000	4.824f	0	6017688	N.D. 1.708 #
4) MA	Heptachlor	0.000	5.284f	0	6414026	N.D. 1.786 #
8) B	Heptachlo...	0.000	6.017	0	15147685	N.D. 5.815 #
9) A	Endosulfan I	5.474	0.000	1229105	0	0.348 N.D. #
10) B	gamma-Chl...	5.346f	0.000	17653277	0	4.557 N.D. #
11) B	alpha-Chl...	5.435	0.000	7134139	0	1.865 N.D. #
13) MA	Dieldrin	5.697f	0.000	35934105	0	9.661 N.D. #
14) MA	Endrin	5.985f	0.000	6786677	0	1.954 N.D. #
25)	Chlordane-3	5.346f	0.000	17653277	0	44.182 N.D. #
26)	Chlordane-4	5.435	0.000	7134139	0	21.682 N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012321\
Data File : PL064300.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2021 12:32
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 17:02:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

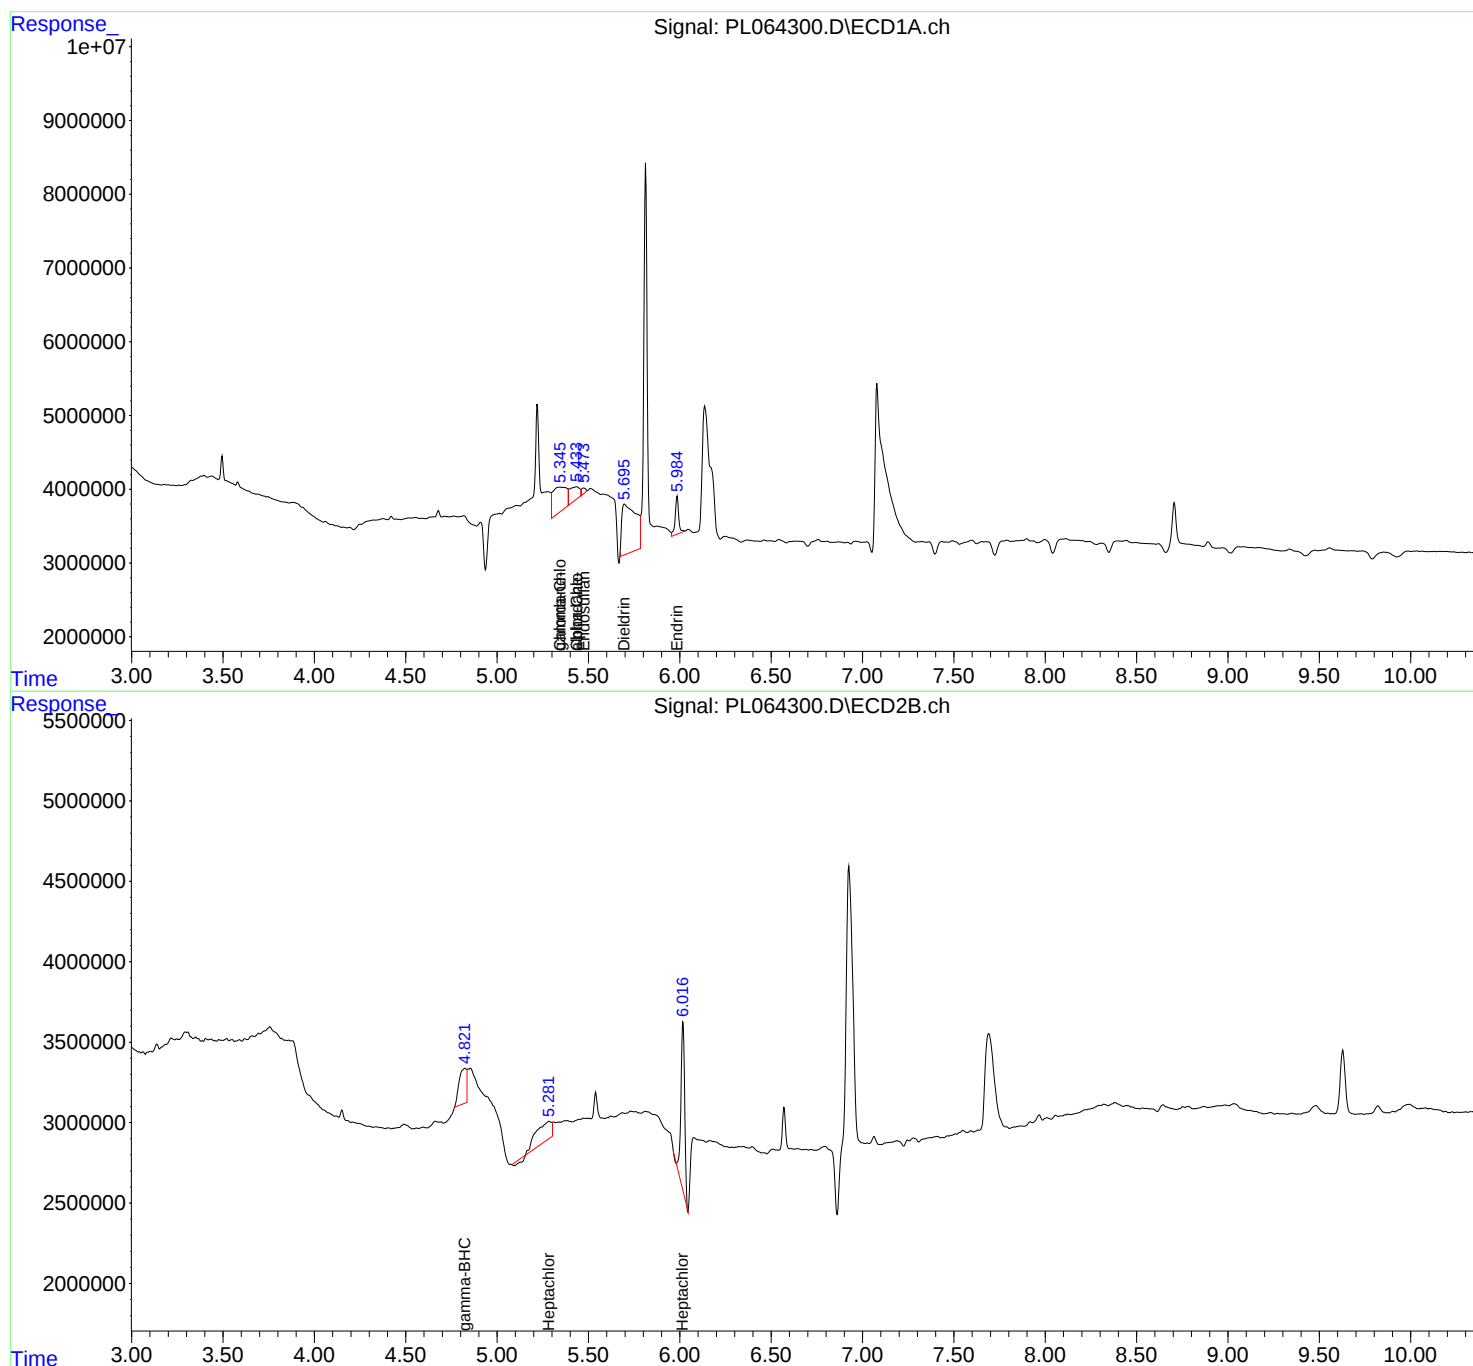


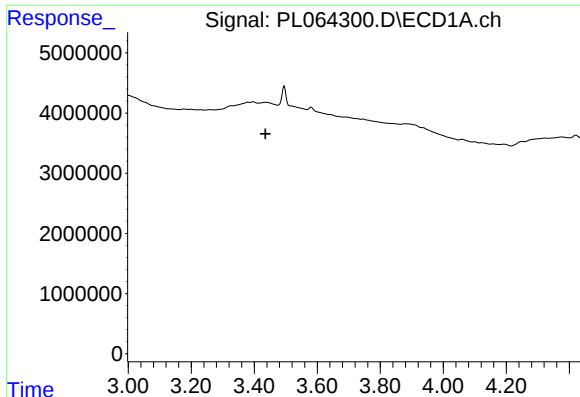

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

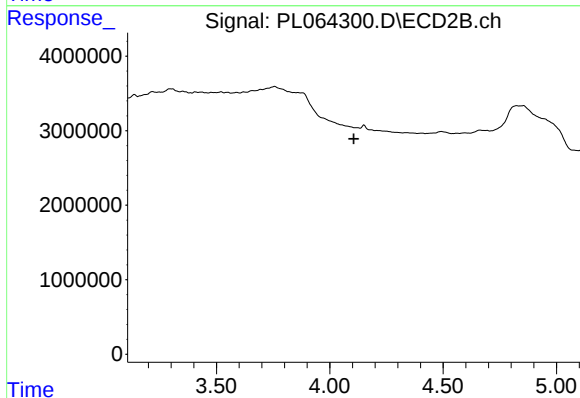


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.106 min
Response: 0
Conc: N.D.

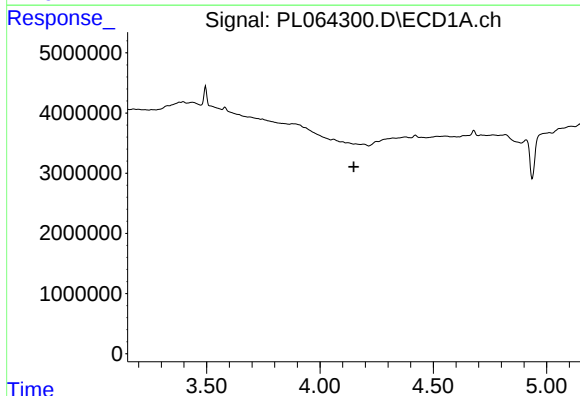


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.150 min
Response: 0
Conc: N.D.

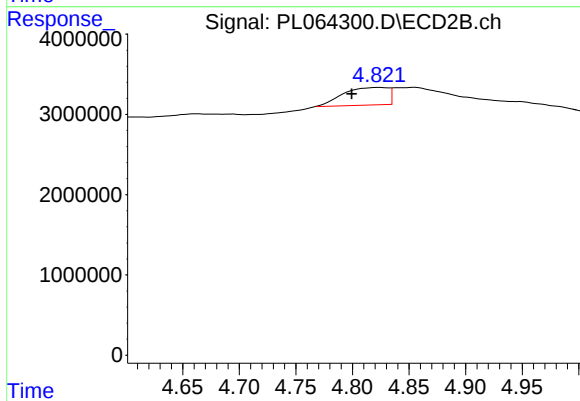

#3 gamma-BHC (Lindane)


R.T.: 4.824 min
Delta R.T.: 0.025 min
Response: 6017688
Conc: 1.71 ng/ml

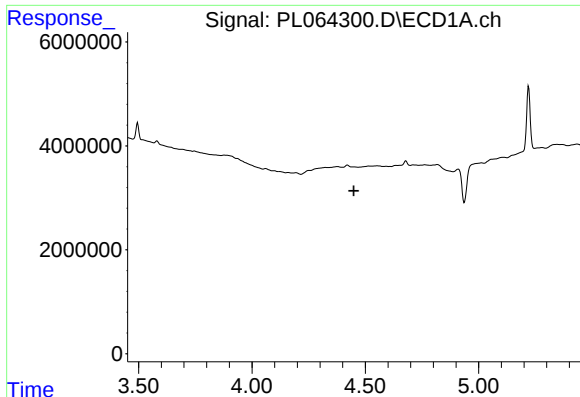

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

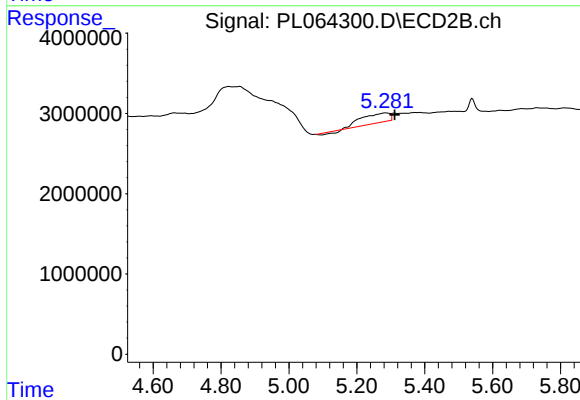


#4 Heptachlor

R.T.: 5.284 min
Delta R.T.: -0.028 min
Response: 6414026
Conc: 1.79 ng/ml

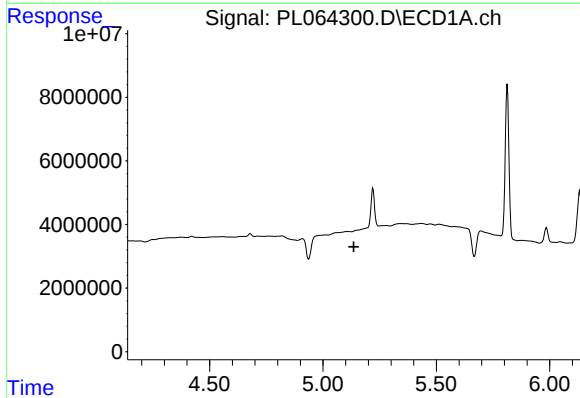


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.135 min
Response: 0
Conc: N.D.

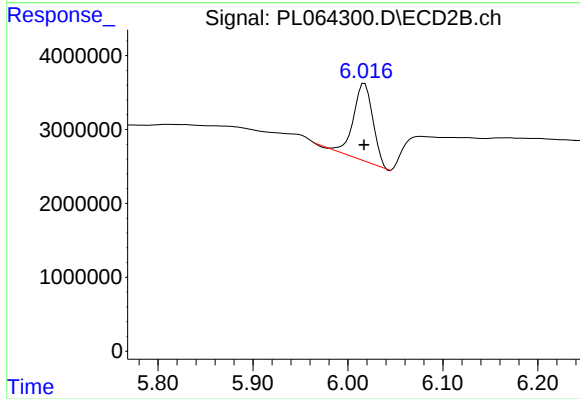

#8 Heptachlor epoxide


R.T.: 6.017 min
Delta R.T.: 0.000 min
Response: 15147685
Conc: 5.81 ng/ml

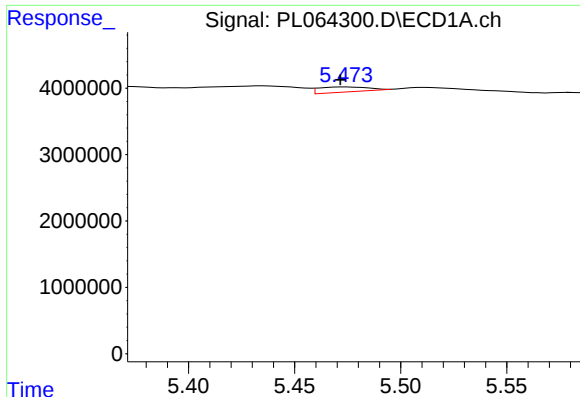

#9 Endosulfan I


R.T.: 5.474 min
Delta R.T.: 0.002 min
Response: 1229105
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

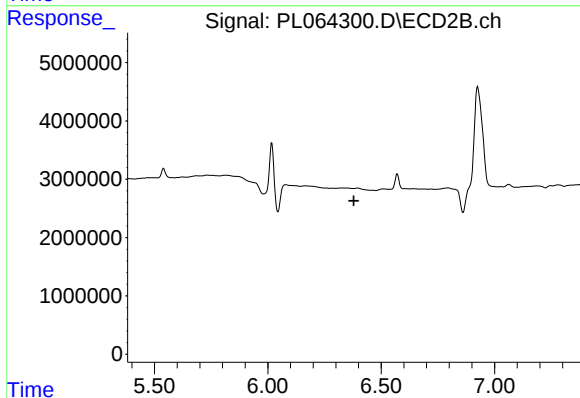


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.379 min
Response: 0
Conc: N.D.

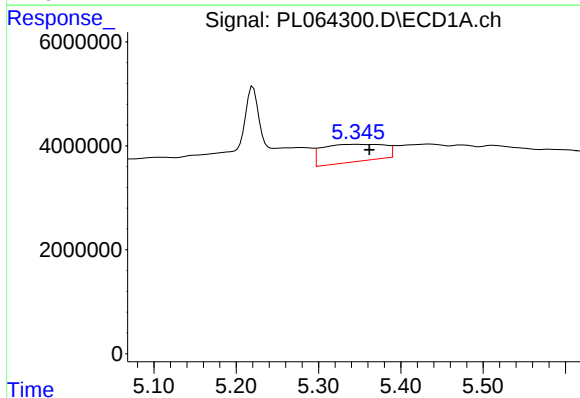


#10 gamma-Chlordane

R.T.: 5.346 min
Delta R.T.: -0.015 min
Response: 17653277
Conc: 4.56 ng/ml

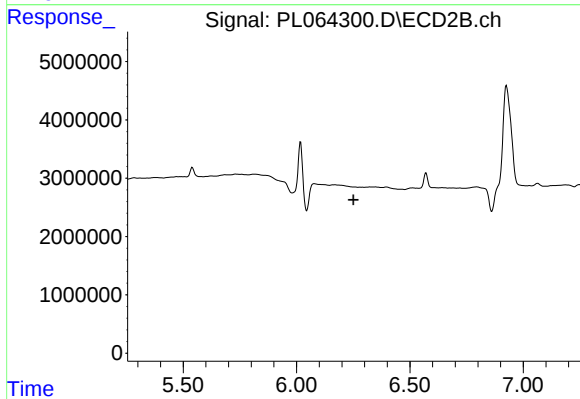

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.252 min
Response: 0
Conc: N.D.

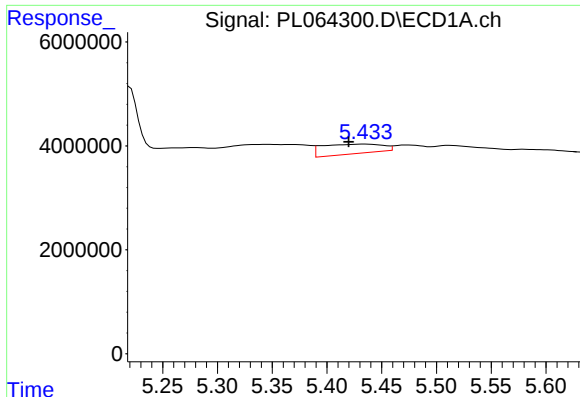

#11 alpha-Chlordane


R.T.: 5.435 min
Delta R.T.: 0.015 min
Response: 7134139
Conc: 1.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

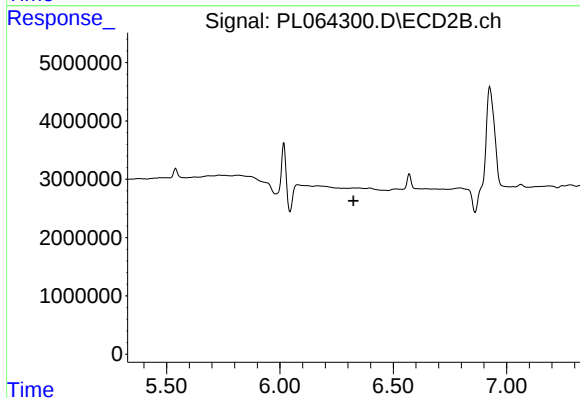


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.325 min
Response: 0
Conc: N.D.

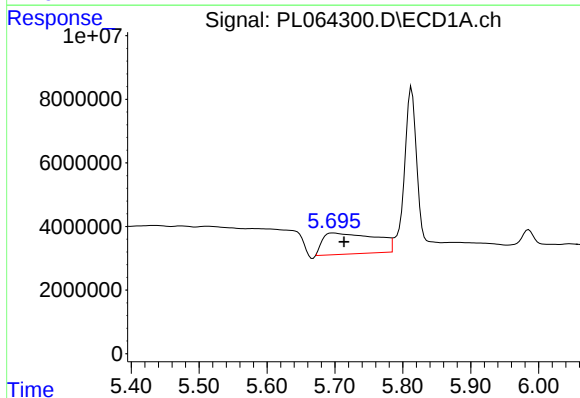


#13 Dieldrin

R.T.: 5.697 min
Delta R.T.: -0.016 min
Response: 35934105
Conc: 9.66 ng/ml

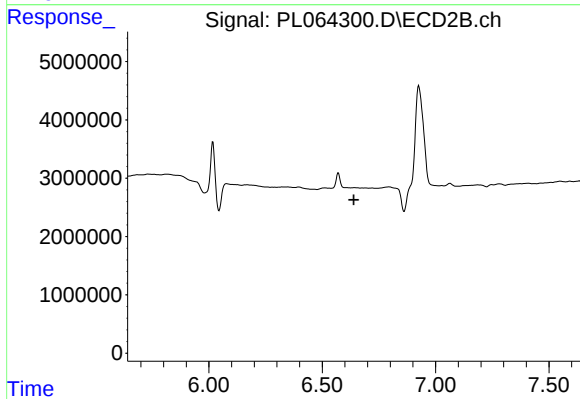

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.639 min
Response: 0
Conc: N.D.

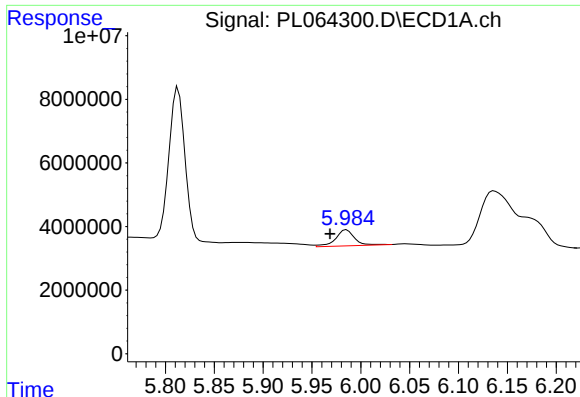

#14 Endrin


R.T.: 5.985 min
Delta R.T.: 0.017 min
Response: 6786677
Conc: 1.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

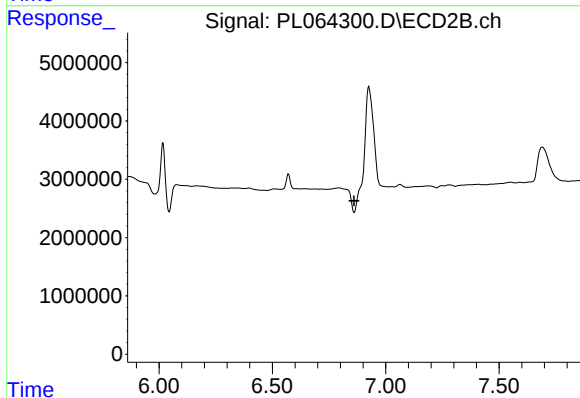


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.861 min
Response: 0
Conc: N.D.

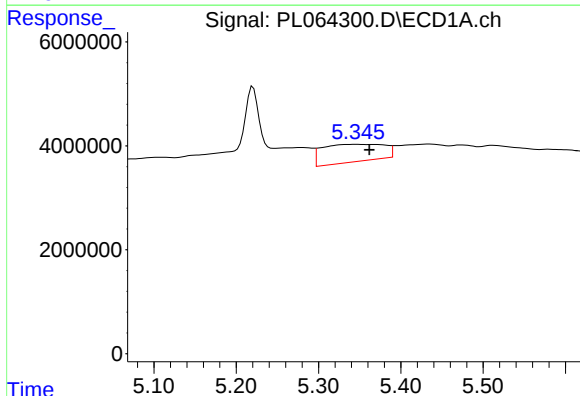


#25 Chlordane-3

R.T.: 5.346 min
Delta R.T.: -0.016 min
Response: 17653277
Conc: 44.18 ng/ml

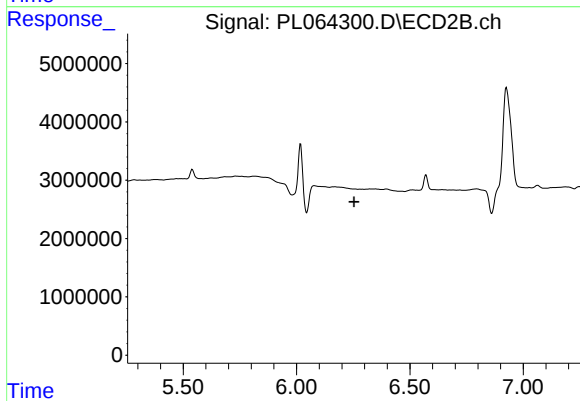

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.255 min
Response: 0
Conc: N.D.

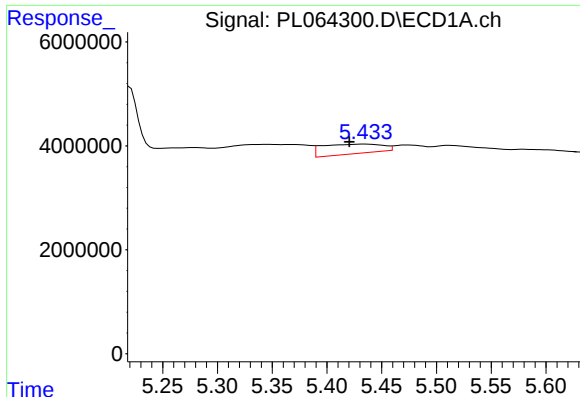

#26 Chlordane-4


R.T.: 5.435 min
Delta R.T.: 0.014 min
Response: 7134139
Conc: 21.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

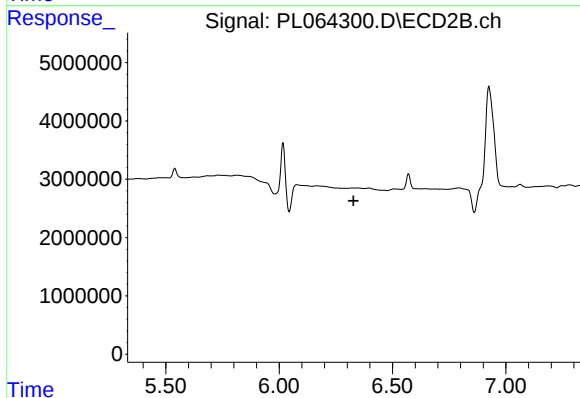


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.328 min
Response: 0
Conc: N.D.

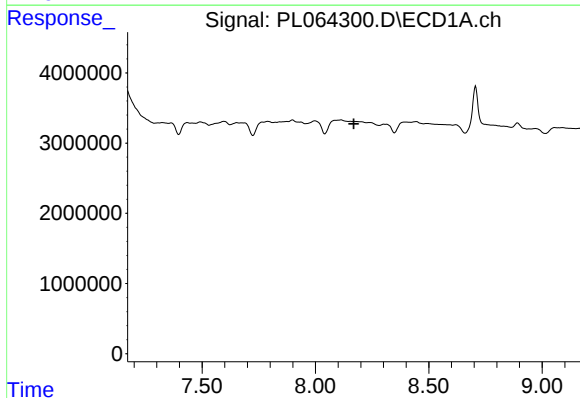

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.169 min
Response: 0
Conc: N.D.

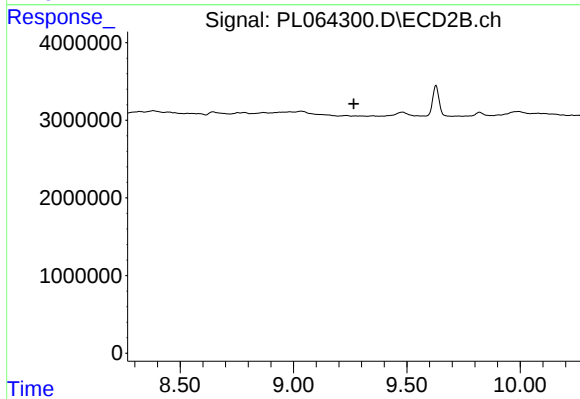

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.266 min
Response: 0
Conc: N.D.