

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012321\
 Data File : PL064301.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2021 12:47
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 17:02:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.108	57122944	46007750	19.051	17.997
28)	SA Decachlor...	8.171	9.273	60276983	44727450	19.750	18.845
Target Compounds							
4)	MA Heptachlor	0.000	5.304	0	1219870	N.D.	0.340 #
7)	B delta-BHC	0.000	5.223f	0	3275599	N.D.	1.032 #
16)	A 4,4'-DDD	0.000	6.950f	0	6769523	N.D.	3.054 #
23)	Chlordane-1	4.325f	0.000	1382609	0	11.872	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012321\
Data File : PL064301.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2021 12:47
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 17:02:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

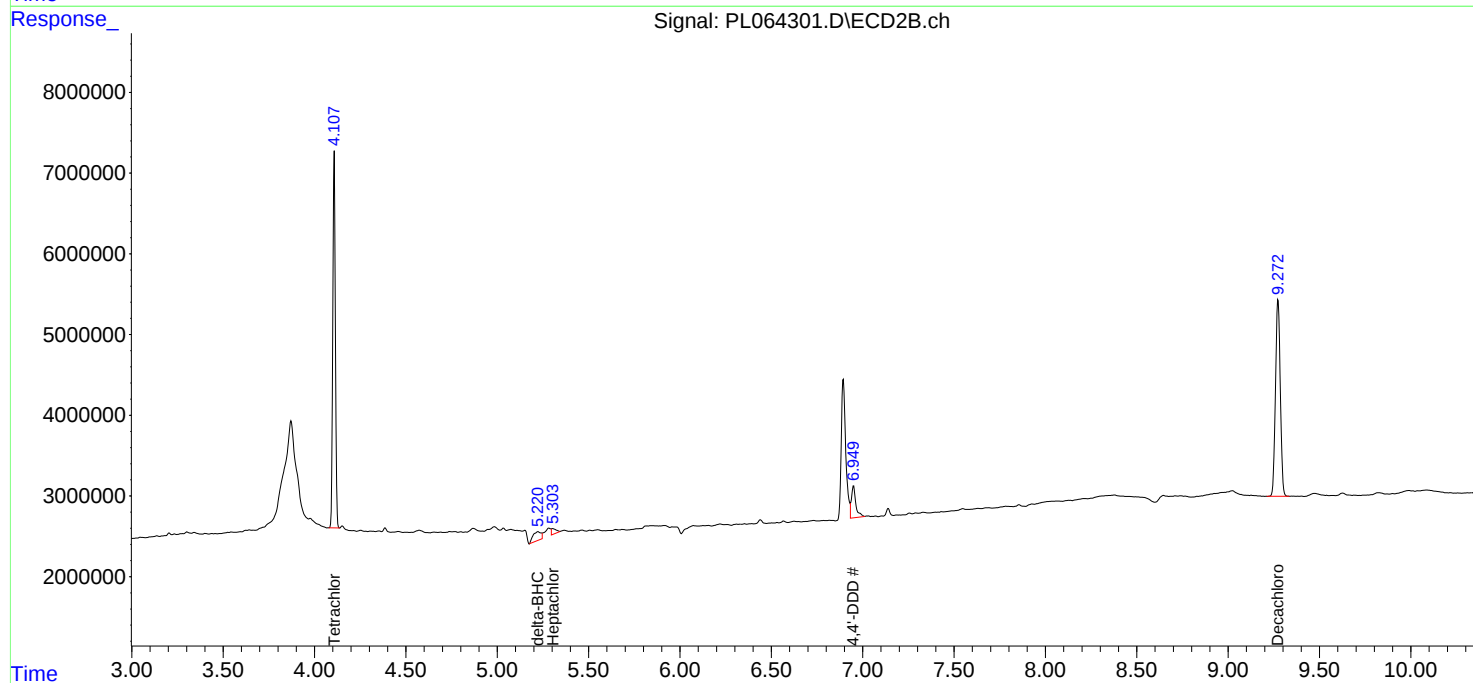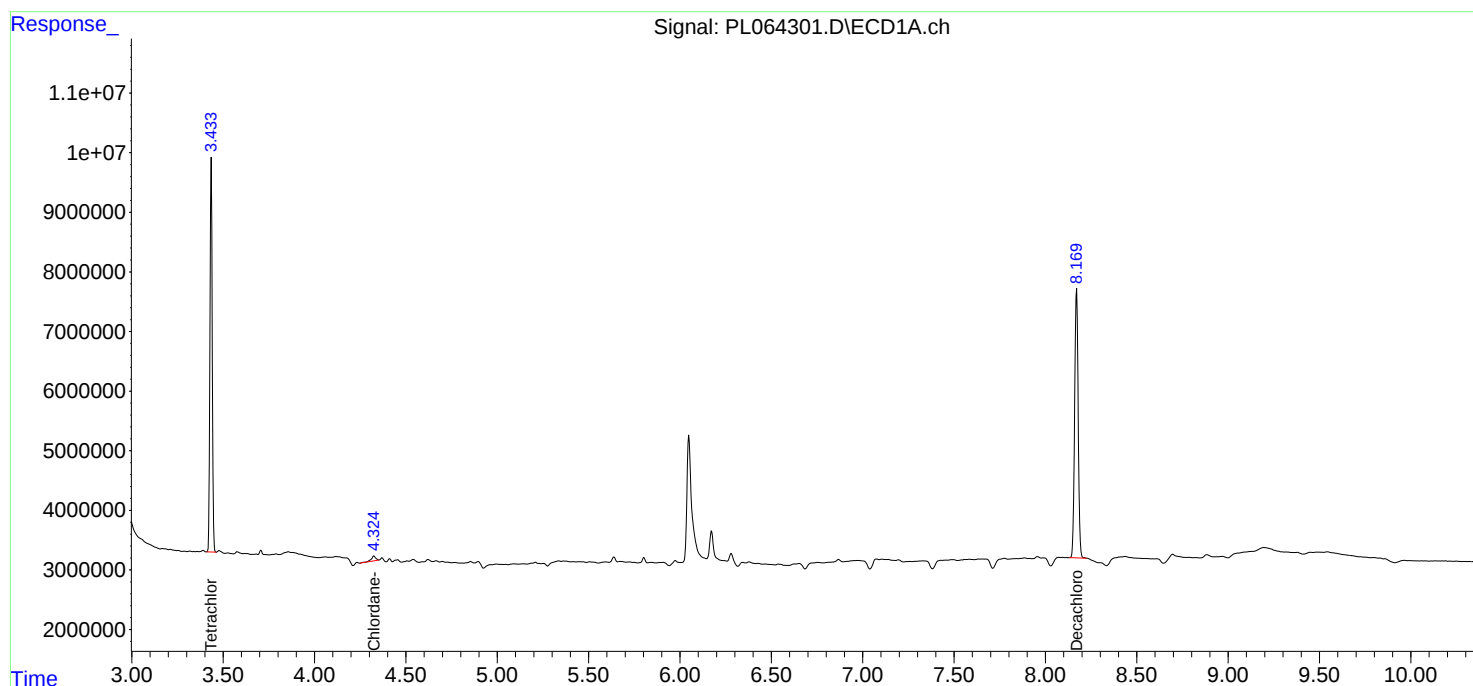


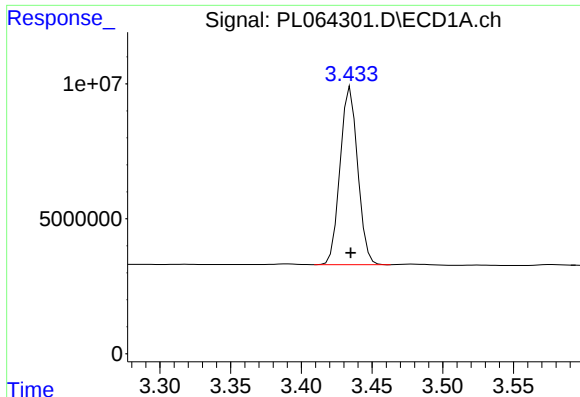

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 57122944
Conc: 19.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

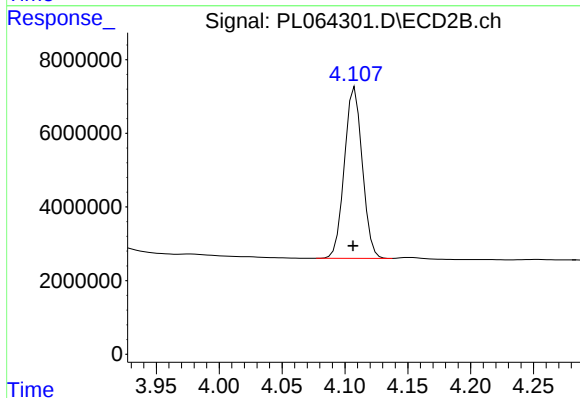


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.002 min
Response: 46007750
Conc: 18.00 ng/ml

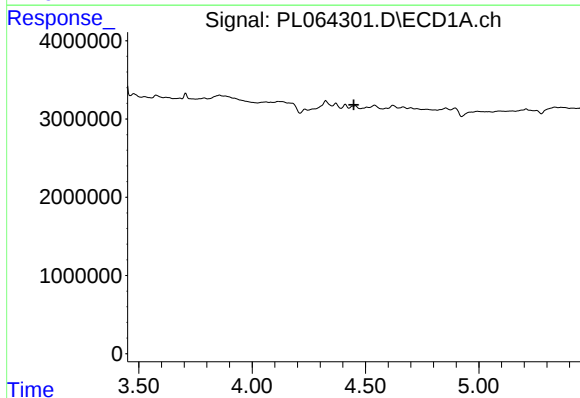


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

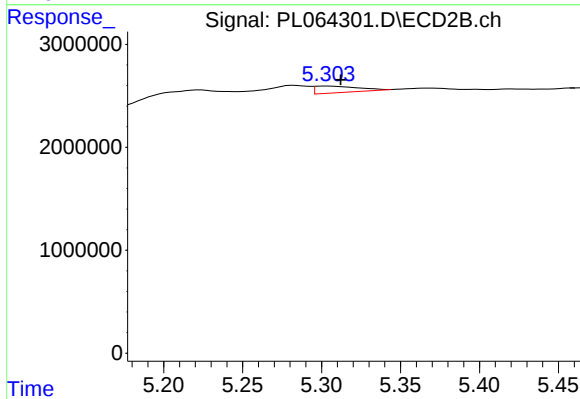

#4 Heptachlor


R.T.: 5.304 min
Delta R.T.: -0.008 min
Response: 1219870
Conc: 0.34 ng/ml

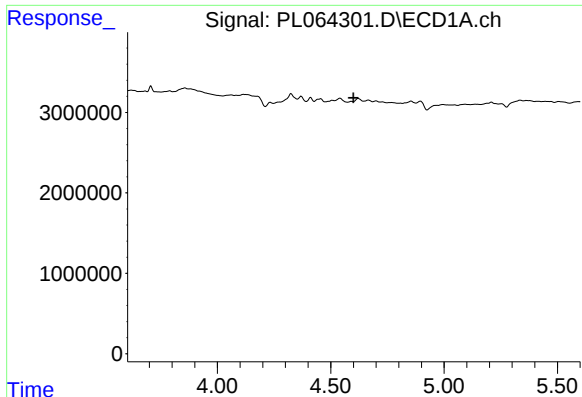

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.601 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

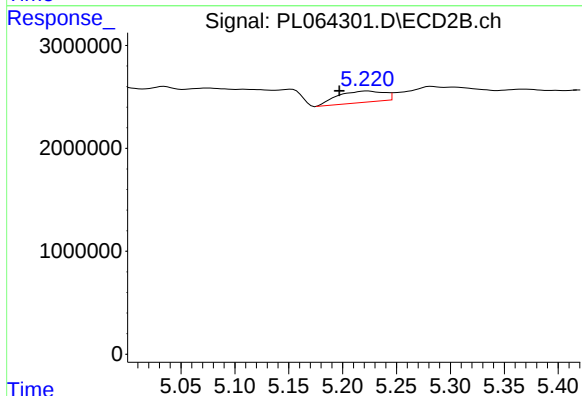


#7 delta-BHC

R.T.: 5.223 min
Delta R.T.: 0.026 min
Response: 3275599
Conc: 1.03 ng/ml

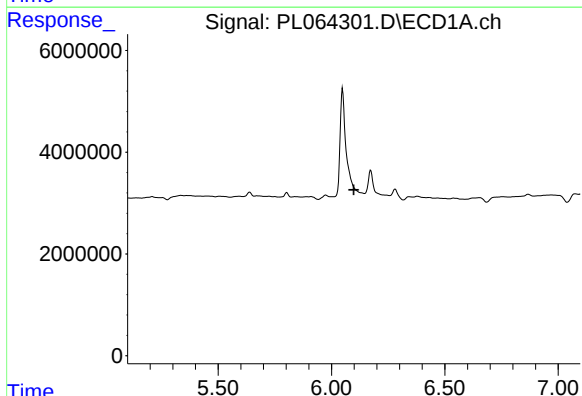


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.099 min
Response: 0
Conc: N.D.

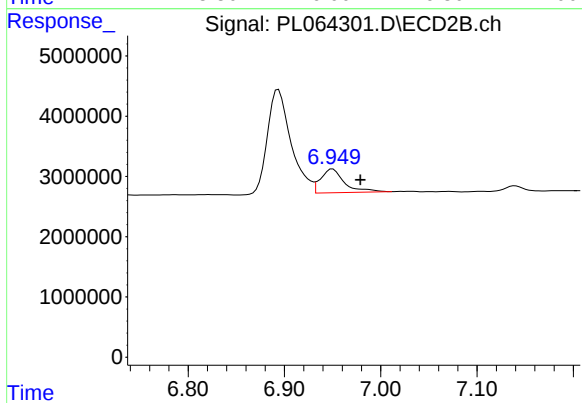

#16 4,4'-DDD


R.T.: 6.950 min
Delta R.T.: -0.029 min
Response: 6769523
Conc: 3.05 ng/ml

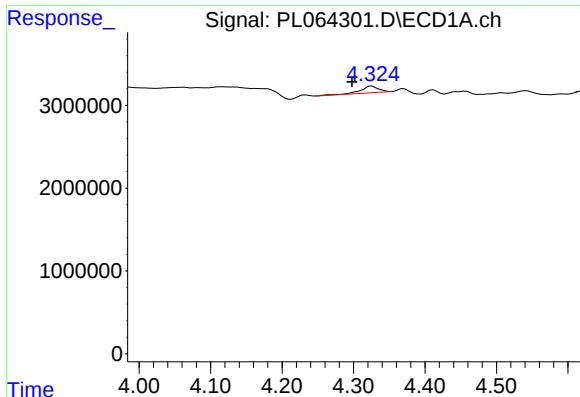

#23 Chlordane-1


R.T.: 4.325 min
Delta R.T.: 0.027 min
Response: 1382609
Conc: 11.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

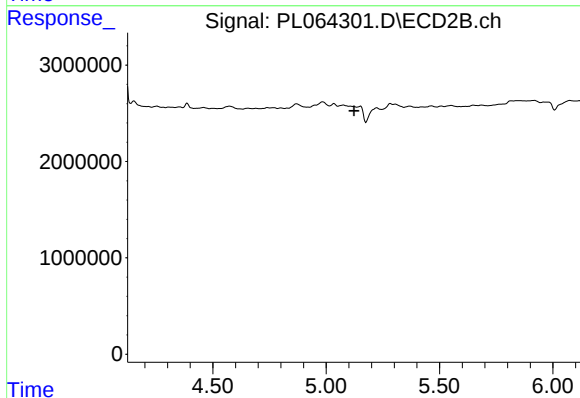


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.123 min
Response: 0
Conc: N.D.

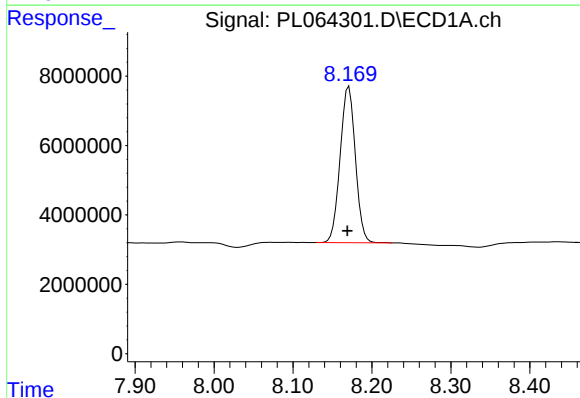

#28 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: 0.002 min
Response: 60276983
Conc: 19.75 ng/ml

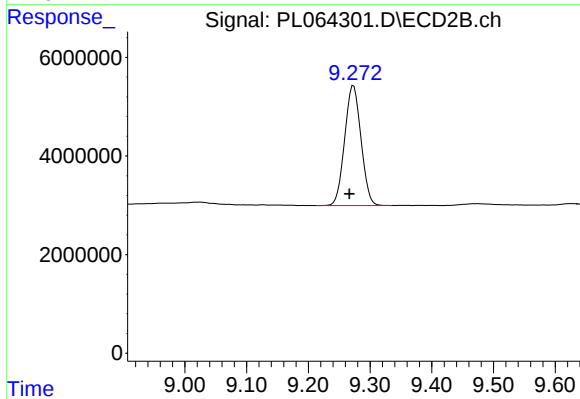

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.007 min
Response: 44727450
Conc: 18.85 ng/ml