

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012321\
 Data File : PL064306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2021 15:11
 Operator : AR\AJ
 Sample : M1179-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 17:03:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.109	56312990	45538455	18.780	17.813
28)	SA Decachlor...	8.170	9.274	57901270	43484710	18.971	18.322
Target Compounds							
2)	A alpha-BHC	0.000	4.479f	0	1155280	N.D.	0.316 #
4)	MA Heptachlor	0.000	5.284f	0	20902485	N.D.	5.820 #
8)	B Heptachlo...	5.152f	0.000	27202368	0	7.178	N.D. #
10)	B gamma-Chl...	5.335f	0.000	3833039	0	0.990	N.D. #
11)	B alpha-Chl...	5.398f	6.331	13144634	401005	3.435	0.132 #
16)	A 4,4'-DDD	0.000	6.951f	0	12477575	N.D.	5.629 #
25)	Chlordane-3	5.335f	0.000	3833039	0	9.593	N.D. #
26)	Chlordane-4	5.398f	6.331	13144634	401005	39.950	0.811 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012321\
Data File : PL064306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2021 15:11
Operator : AR\AJ
Sample : M1179-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 17:03:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

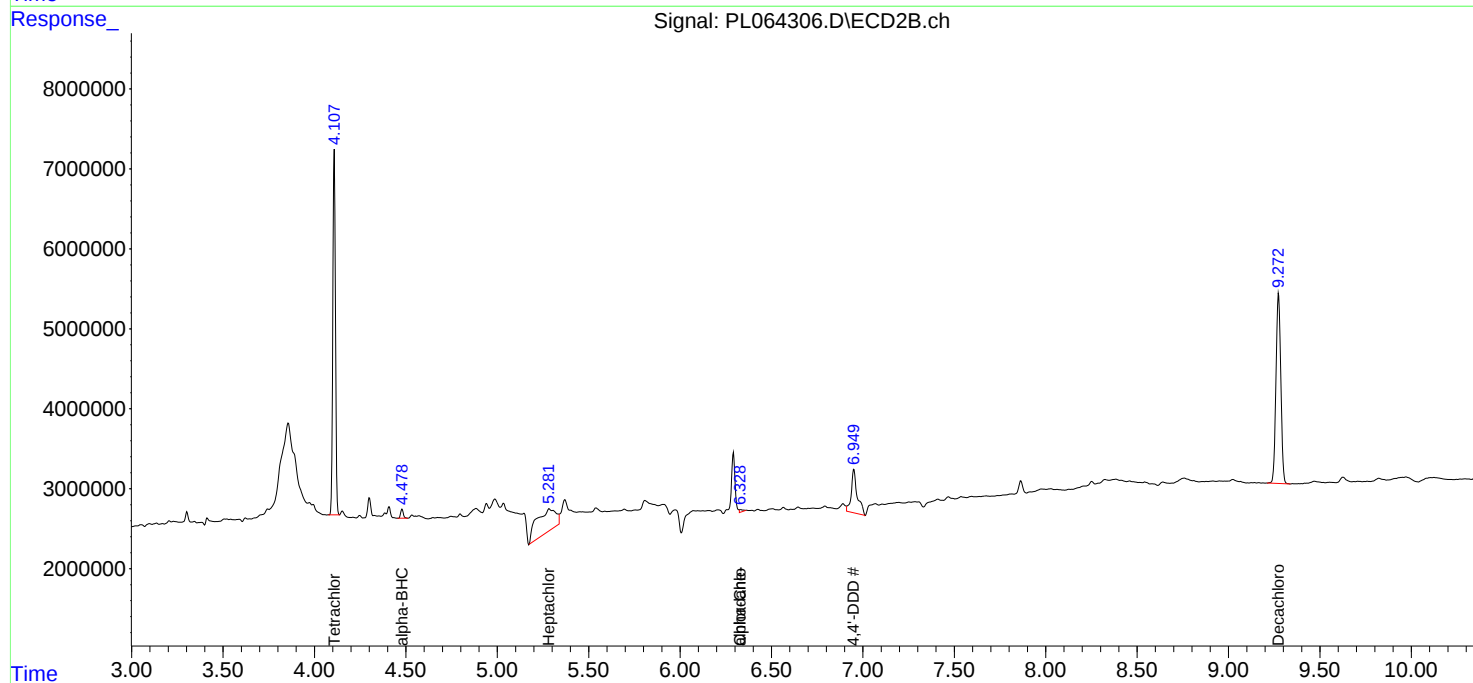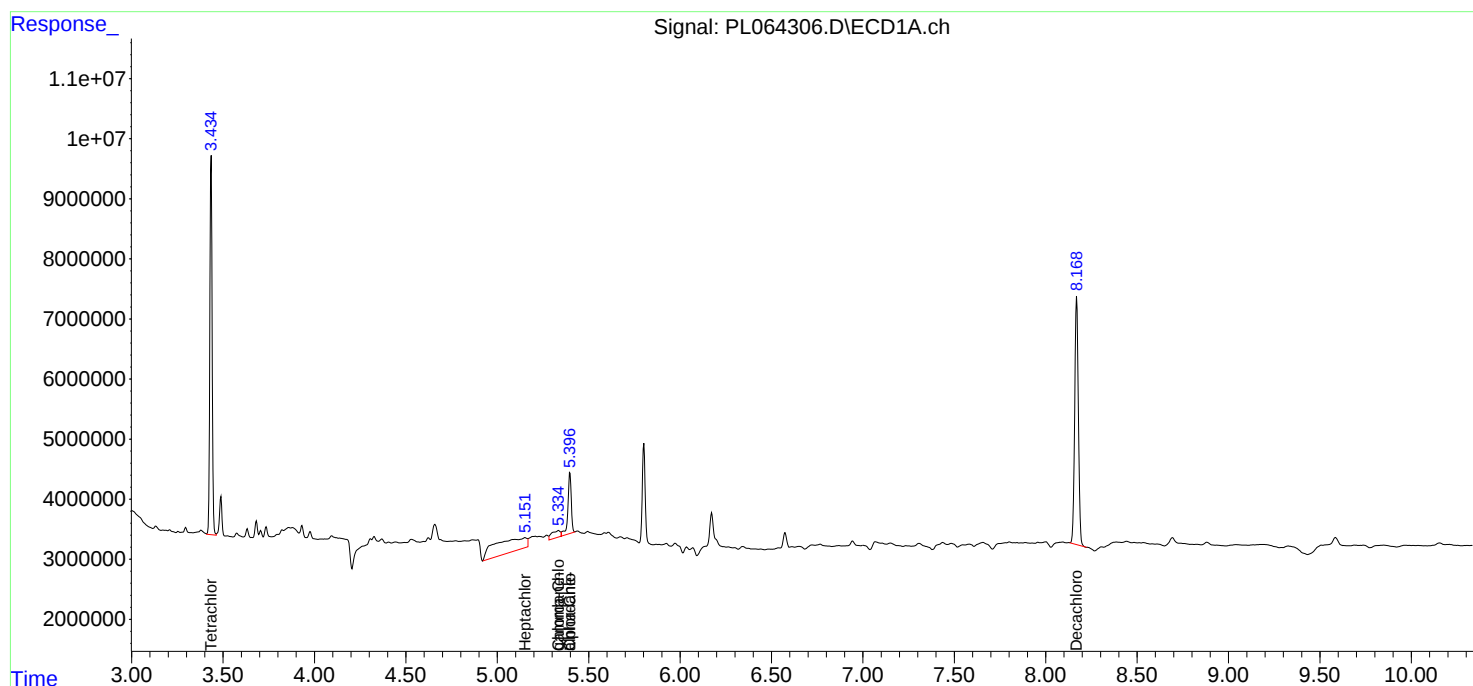


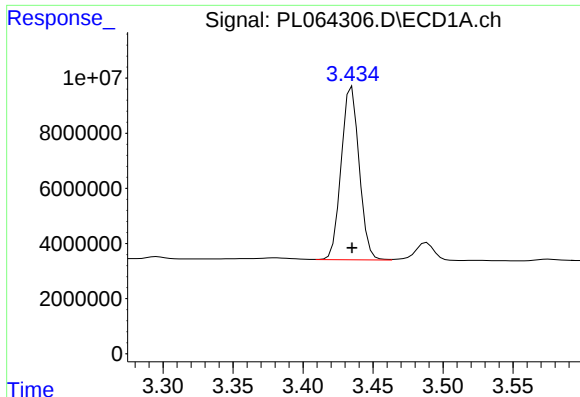

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 56312990
Conc: 18.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

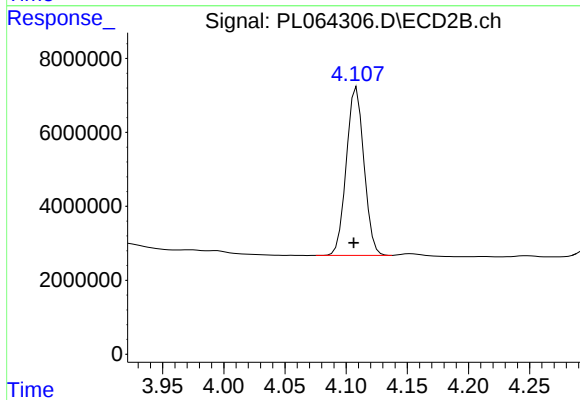


#1 Tetrachloro-m-xylene

R.T.: 4.109 min
Delta R.T.: 0.002 min
Response: 45538455
Conc: 17.81 ng/ml

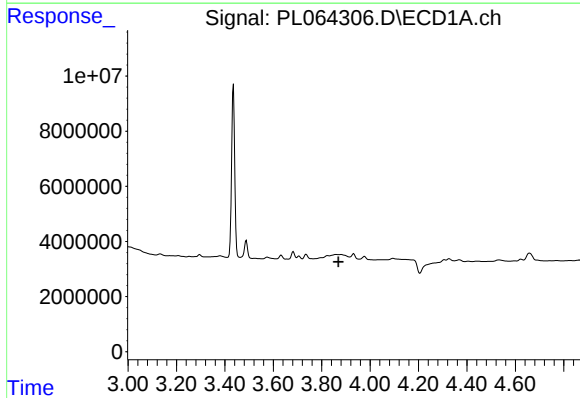


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.869 min
Response: 0
Conc: N.D.

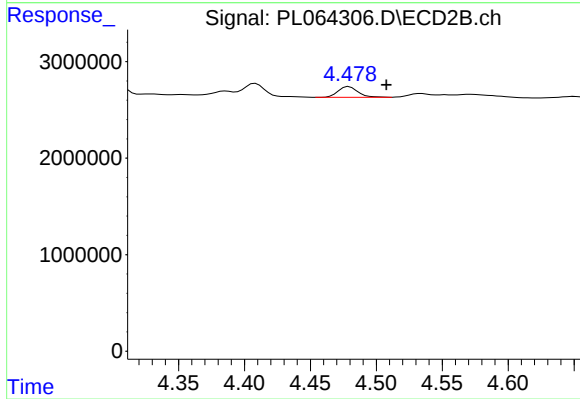

#2 alpha-BHC


R.T.: 4.479 min
Delta R.T.: -0.028 min
Response: 1155280
Conc: 0.32 ng/ml

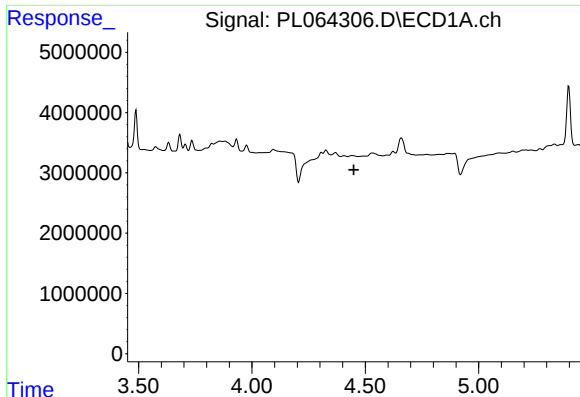

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

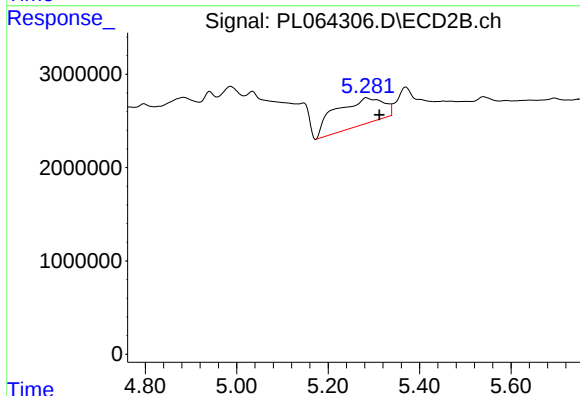


#4 Heptachlor

R.T.: 5.284 min
Delta R.T.: -0.028 min
Response: 20902485
Conc: 5.82 ng/ml

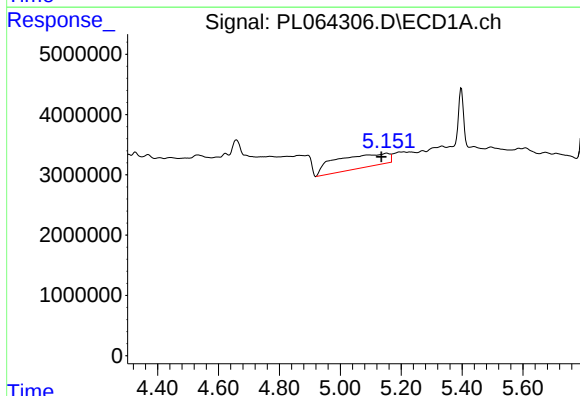


#8 Heptachlor epoxide

R.T.: 5.152 min
Delta R.T.: 0.017 min
Response: 27202368
Conc: 7.18 ng/ml

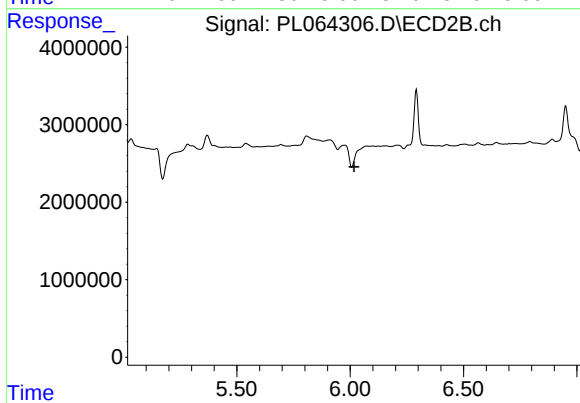

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.017 min
Response: 0
Conc: N.D.

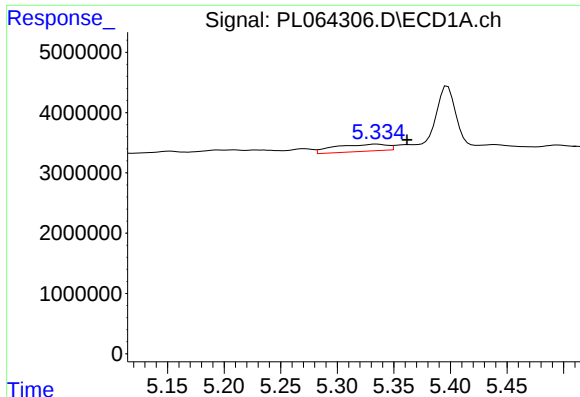

#10 gamma-Chlordane


R.T.: 5.335 min
Delta R.T.: -0.026 min
Response: 3833039
Conc: 0.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

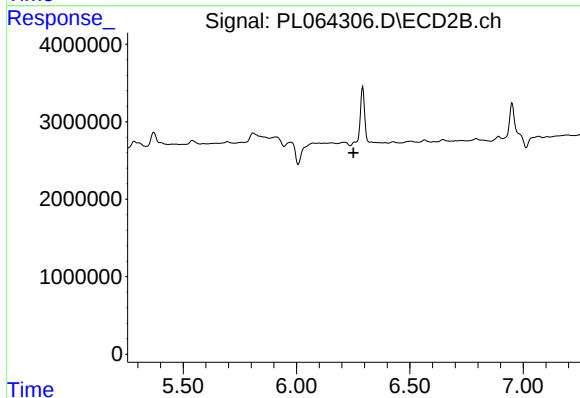


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.252 min
Response: 0
Conc: N.D.

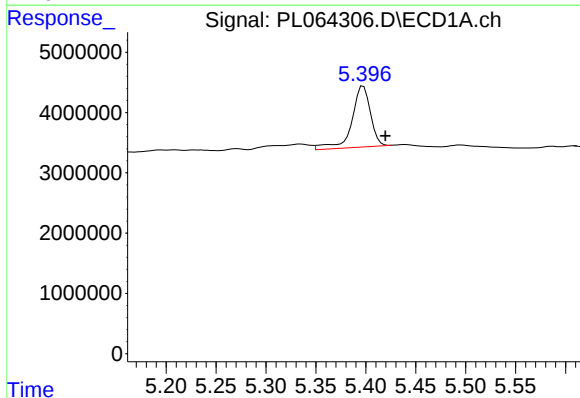


#11 alpha-Chlordane

R.T.: 5.398 min
Delta R.T.: -0.022 min
Response: 13144634
Conc: 3.44 ng/ml

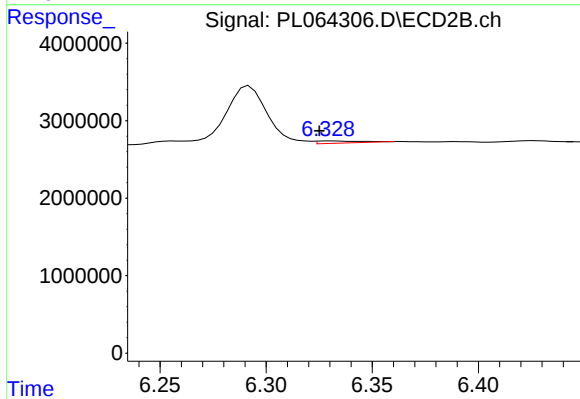

#11 alpha-Chlordane


R.T.: 6.331 min
Delta R.T.: 0.006 min
Response: 401005
Conc: 0.13 ng/ml

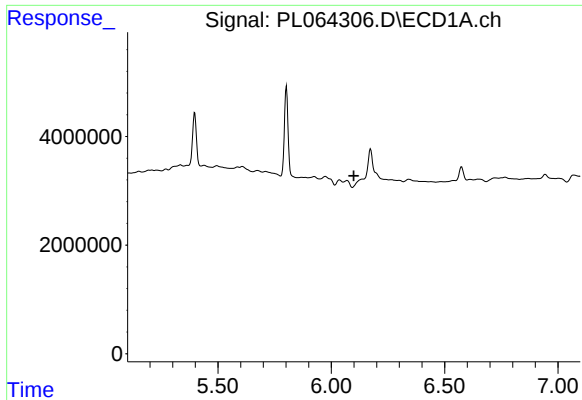

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

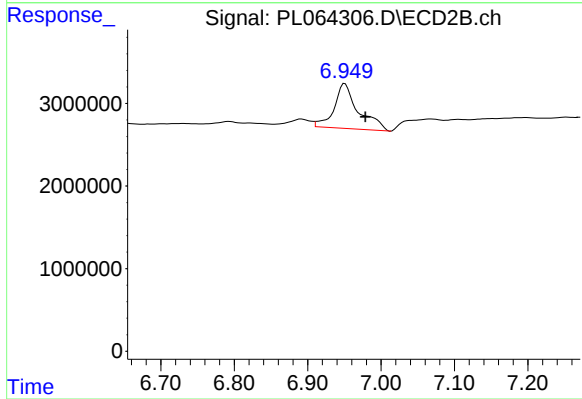


#16 4,4'-DDD

R.T.: 6.951 min
Delta R.T.: -0.028 min
Response: 12477575
Conc: 5.63 ng/ml

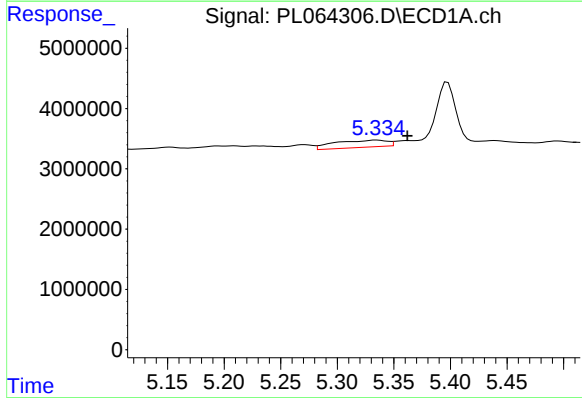


#25 Chlordane-3

R.T.: 5.335 min
Delta R.T.: -0.027 min
Response: 3833039
Conc: 9.59 ng/ml

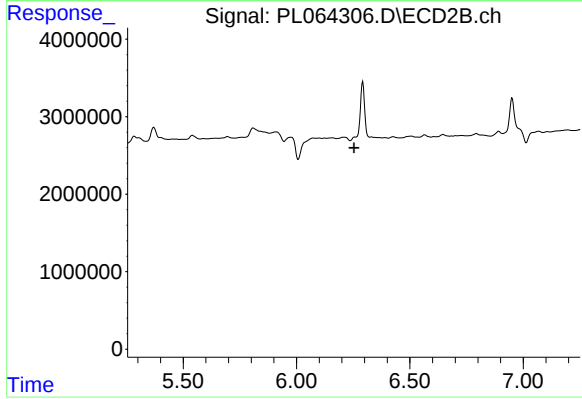

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.255 min
Response: 0
Conc: N.D.

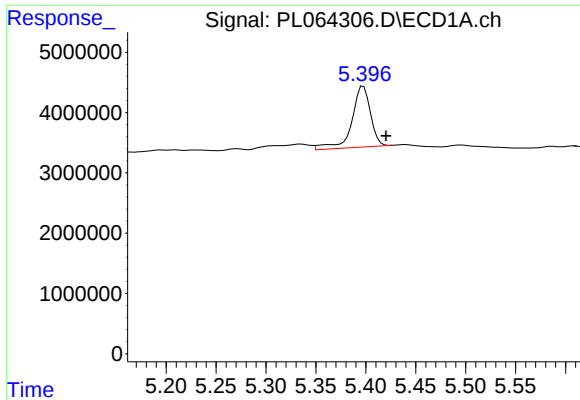

#26 Chlordane-4


R.T.: 5.398 min
Delta R.T.: -0.023 min
Response: 13144634
Conc: 39.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

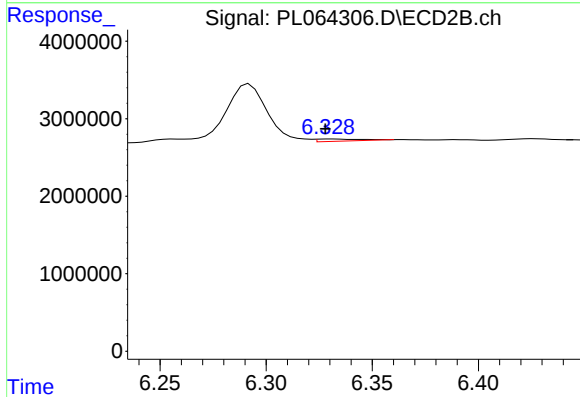


#26 Chlordane-4

R.T.: 6.331 min
Delta R.T.: 0.003 min
Response: 401005
Conc: 0.81 ng/ml

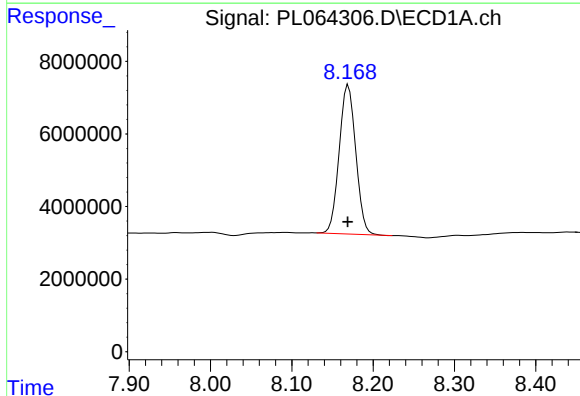

#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: 0.000 min
Response: 57901270
Conc: 18.97 ng/ml

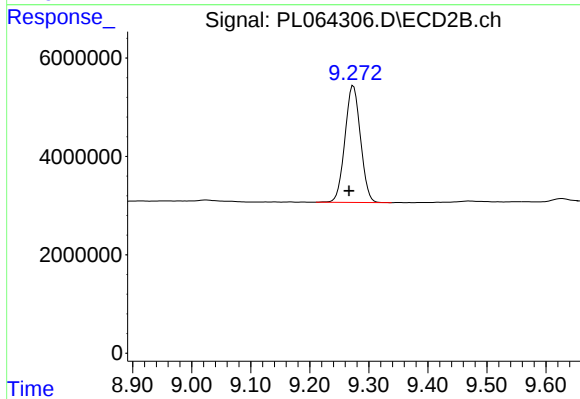

#28 Decachlorobiphenyl

R.T.: 9.274 min
Delta R.T.: 0.008 min
Response: 43484710
Conc: 18.32 ng/ml