

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012321\
 Data File : PL064315.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2021 17:53
 Operator : AR\AJ
 Sample : M1169-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 02:13:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.110	65187590	53717185	21.740	21.012
28)	SA Decachlor...	8.169	9.273	64582933	48853223	21.160	20.584
Target Compounds							
4)	MA Heptachlor	0.000	5.309	0	8813378	N.D.	2.454 #
7)	B delta-BHC	0.000	5.218f	0	7031267	N.D.	2.215 #
10)	B gamma-Chl...	0.000	6.256	0	1058263	N.D.	0.352 #
16)	A 4,4'-DDD	0.000	6.951f	0	10299707	N.D.	4.647 #
23)	Chlordane-1	4.301	0.000	8171802	0	70.170	N.D. #
25)	Chlordane-3	0.000	6.256	0	1058263	N.D.	2.617 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012321\
Data File : PL064315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2021 17:53
Operator : AR\AJ
Sample : M1169-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 02:13:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

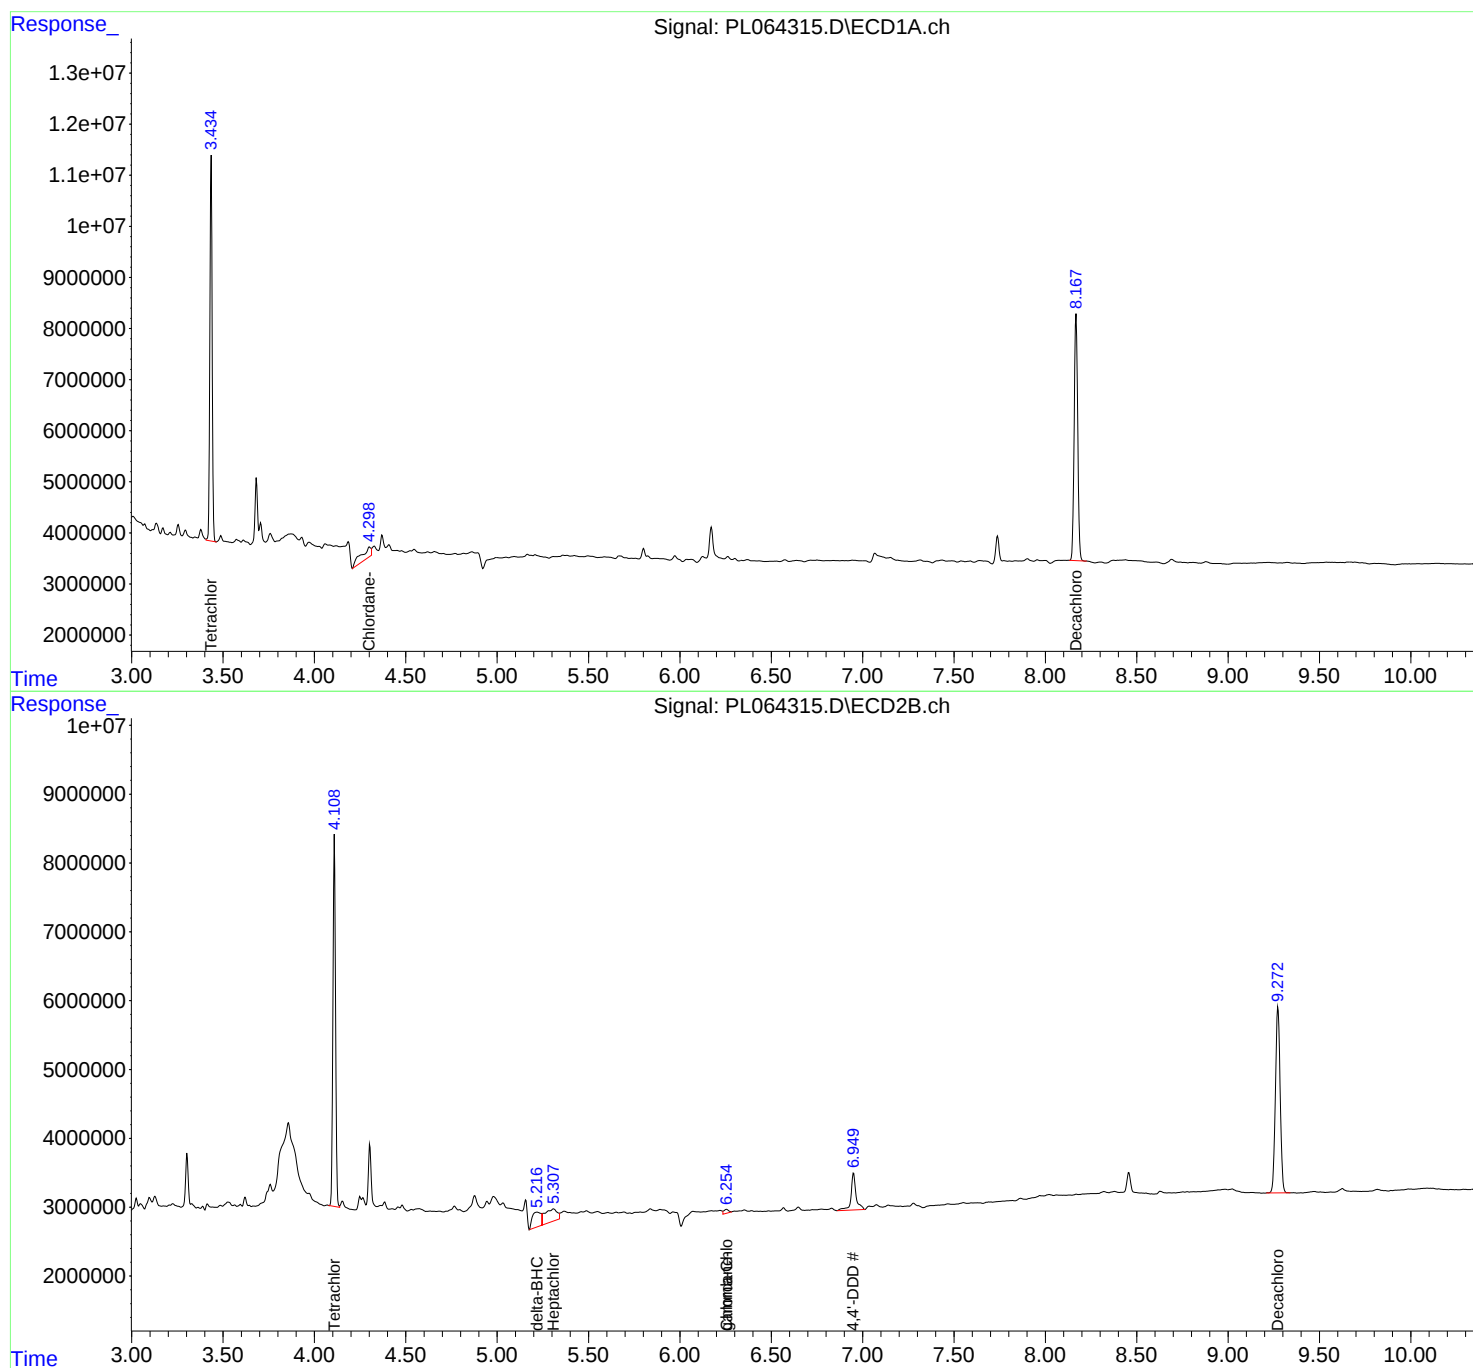


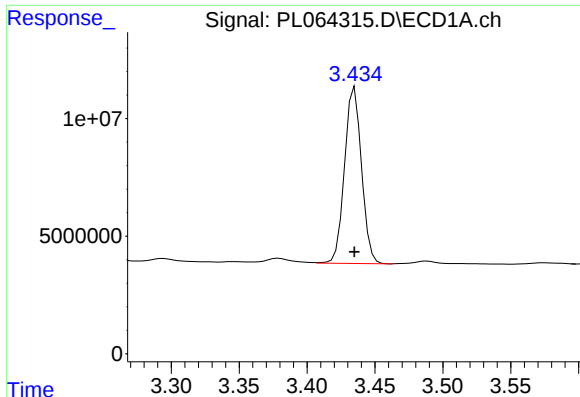

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 65187590
Conc: 21.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

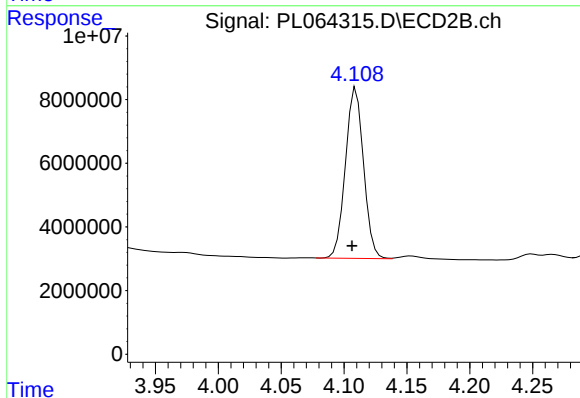


#1 Tetrachloro-m-xylene

R.T.: 4.110 min
Delta R.T.: 0.003 min
Response: 53717185
Conc: 21.01 ng/ml

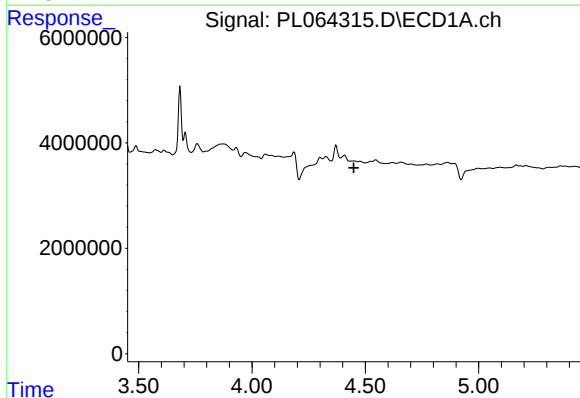


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

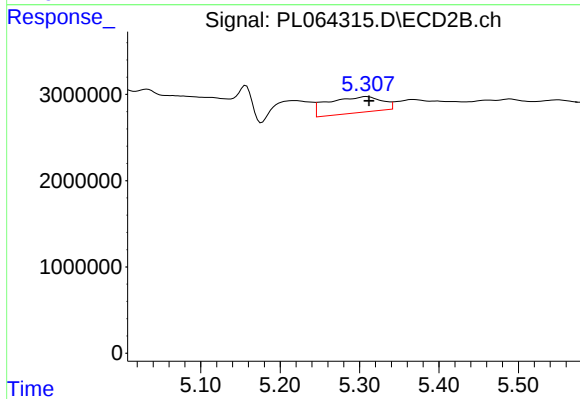

#4 Heptachlor

R.T.: 5.309 min
Delta R.T.: -0.003 min
Response: 8813378
Conc: 2.45 ng/ml

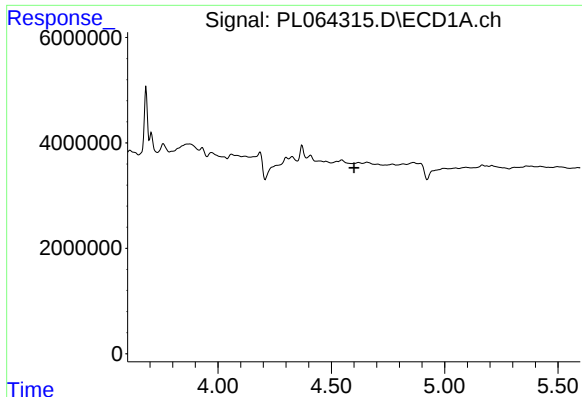

#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.601 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#7 delta-BHC


R.T.: 5.218 min
Delta R.T.: 0.021 min
Response: 7031267
Conc: 2.21 ng/ml

#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.362 min
Response: 0
Conc: N.D.

#10 gamma-Chlordane


R.T.: 6.256 min
Delta R.T.: 0.004 min
Response: 1058263
Conc: 0.35 ng/ml

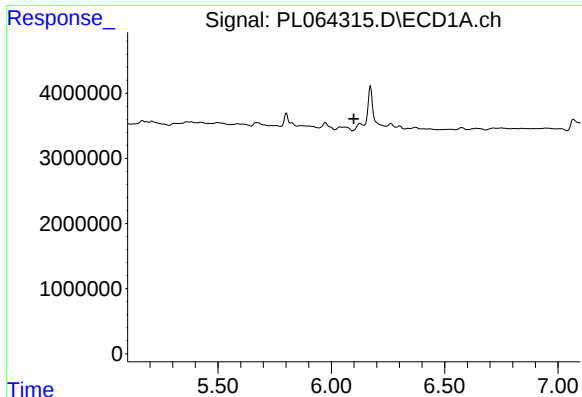

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

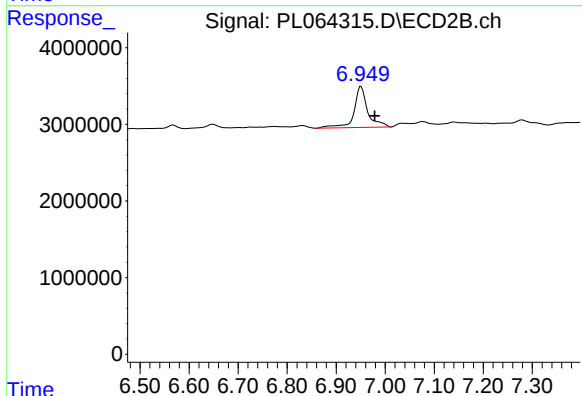


#16 4,4'-DDD

R.T.: 6.951 min
Delta R.T.: -0.028 min
Response: 10299707
Conc: 4.65 ng/ml

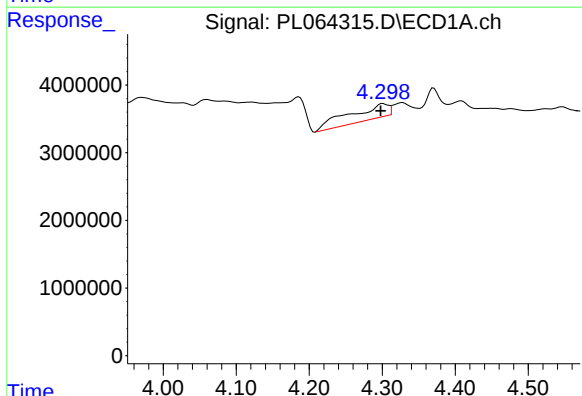


#23 Chlordane-1

R.T.: 4.301 min
Delta R.T.: 0.003 min
Response: 8171802
Conc: 70.17 ng/ml

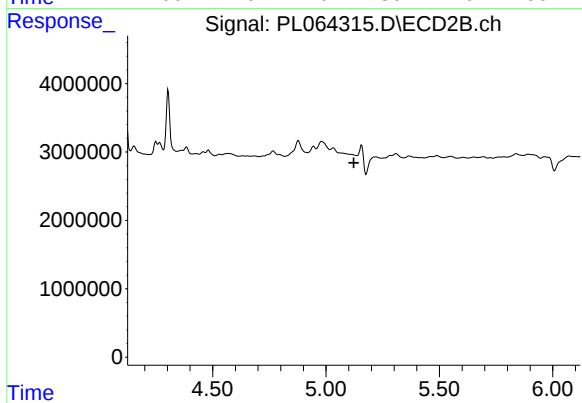

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.123 min
Response: 0
Conc: N.D.

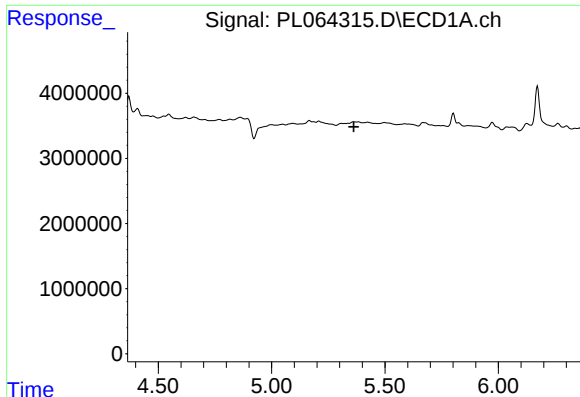

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

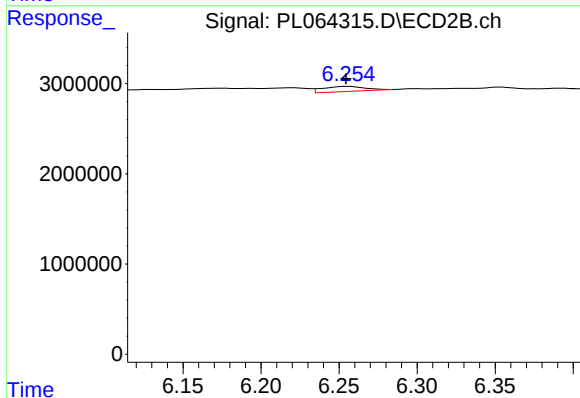


#25 Chlordane-3

R.T.: 6.256 min
Delta R.T.: 0.001 min
Response: 1058263
Conc: 2.62 ng/ml

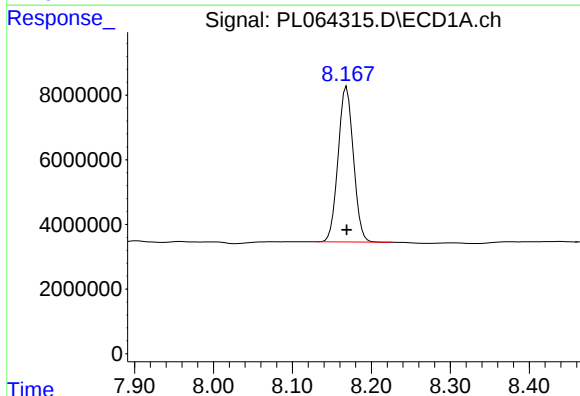

#28 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.000 min
Response: 64582933
Conc: 21.16 ng/ml

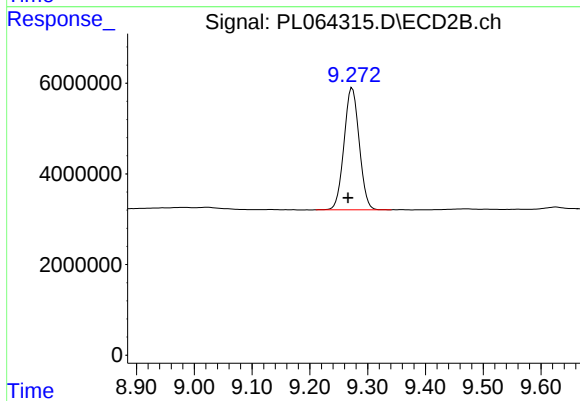

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.007 min
Response: 48853223
Conc: 20.58 ng/ml