

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012321\
 Data File : PL064318.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2021 18:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 02:14:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.109	57331280	46647395	19.120	18.247
28)	SA Decachlor...	8.168	9.273	58439287	44038187	19.147	18.555
Target Compounds							
4)	MA Heptachlor	0.000	5.284f	0	6796287	N.D.	1.892 #
7)	B delta-BHC	4.622f	5.224f	2137616	3555678	0.462	1.120 #
8)	B Heptachlo...	0.000	6.016	0	4462087	N.D.	1.713 #
14)	MA Endrin	5.973	0.000	1999391	0	0.576	N.D. #
16)	A 4,4'-DDD	0.000	6.951f	0	7482026	N.D.	3.376 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012321\
Data File : PL064318.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2021 18:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 02:14:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

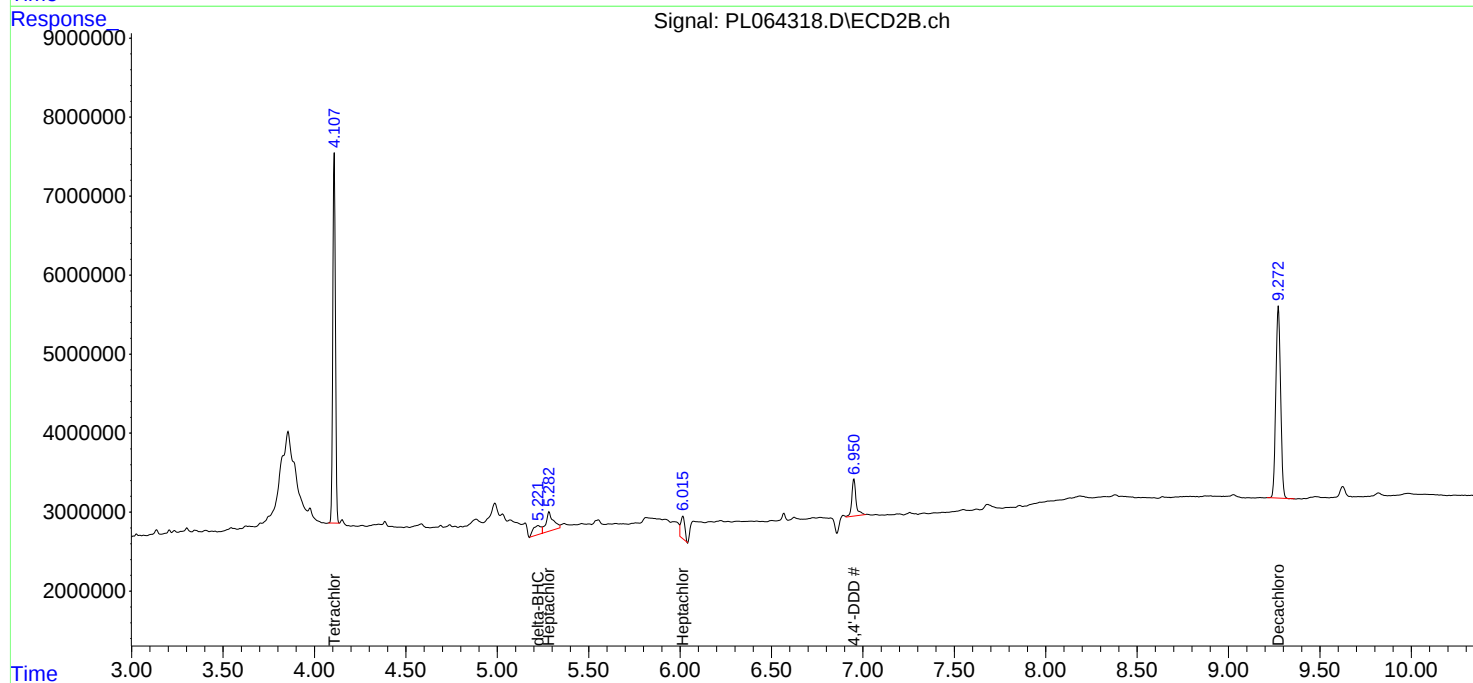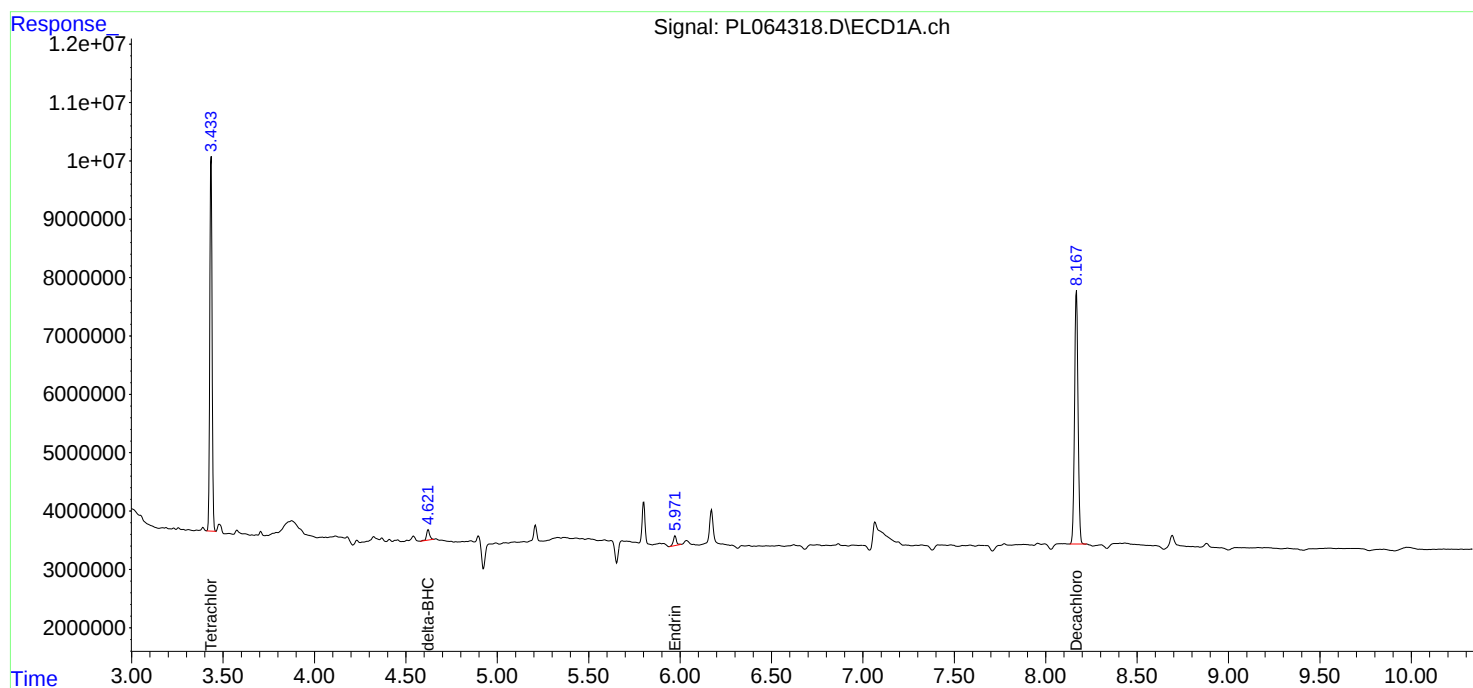


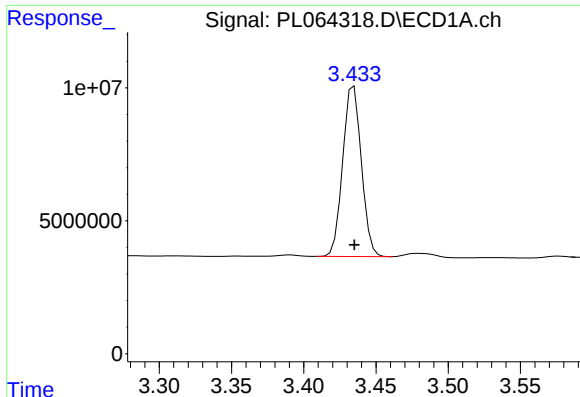

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 57331280
Conc: 19.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

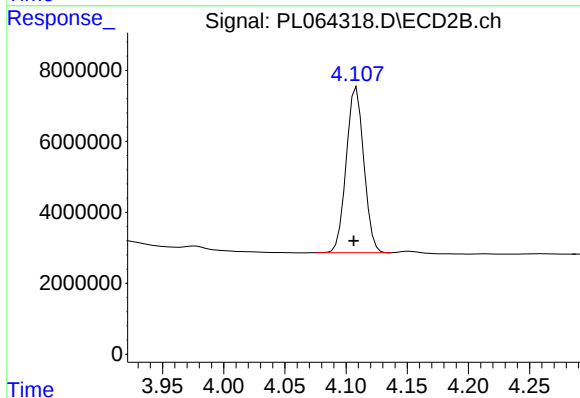


#1 Tetrachloro-m-xylene

R.T.: 4.109 min
Delta R.T.: 0.002 min
Response: 46647395
Conc: 18.25 ng/ml

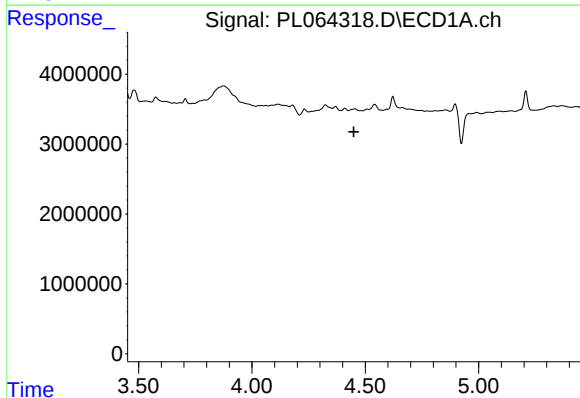


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

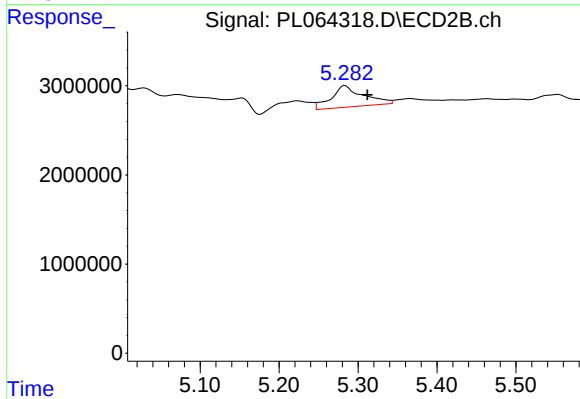

#4 Heptachlor


R.T.: 5.284 min
Delta R.T.: -0.028 min
Response: 6796287
Conc: 1.89 ng/ml

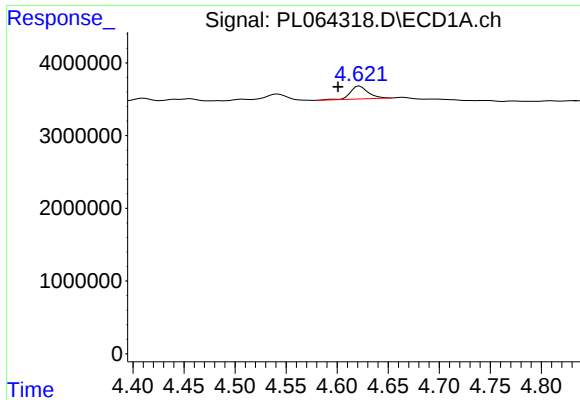

#7 delta-BHC


R.T.: 4.622 min
Delta R.T.: 0.021 min
Response: 2137616
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

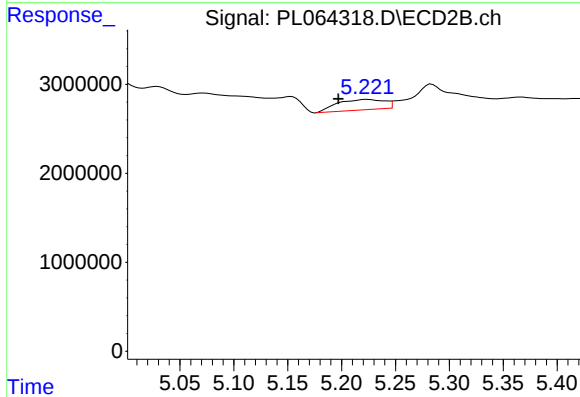


#7 delta-BHC

R.T.: 5.224 min
Delta R.T.: 0.027 min
Response: 3555678
Conc: 1.12 ng/ml

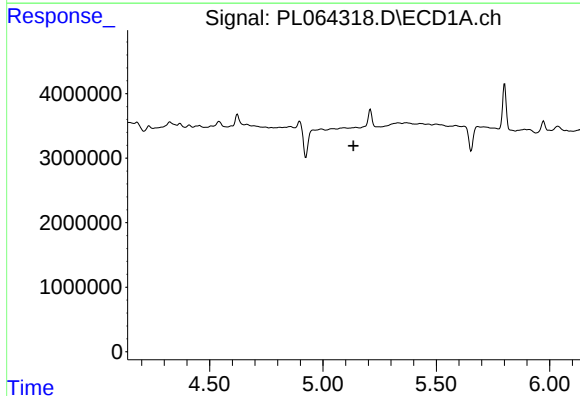


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.135 min
Response: 0
Conc: N.D.

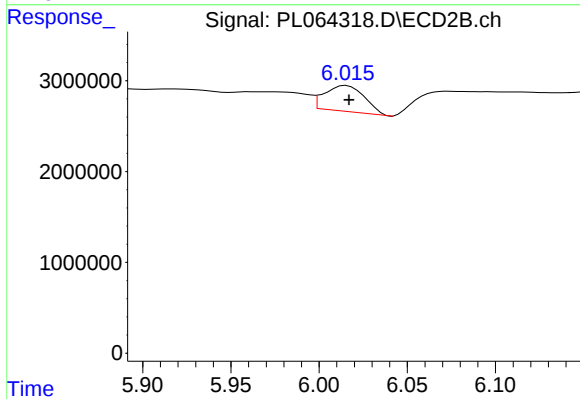

#8 Heptachlor epoxide


R.T.: 6.016 min
Delta R.T.: -0.002 min
Response: 4462087
Conc: 1.71 ng/ml

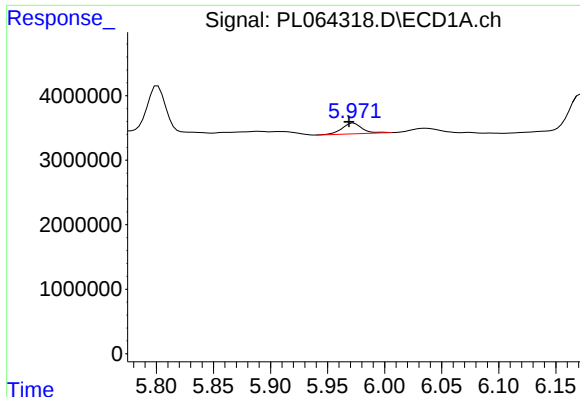

#14 Endrin


R.T.: 5.973 min
Delta R.T.: 0.004 min
Response: 1999391
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

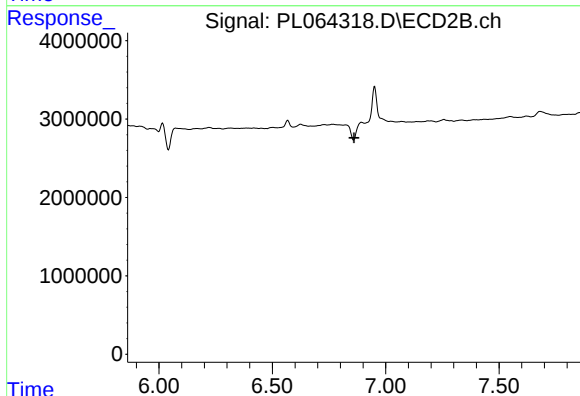


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.861 min
Response: 0
Conc: N.D.

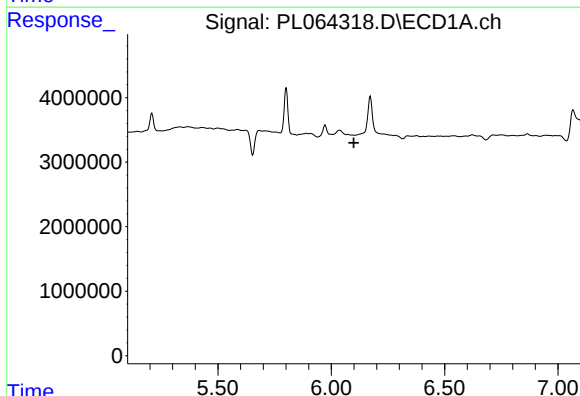


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.099 min
Response: 0
Conc: N.D.

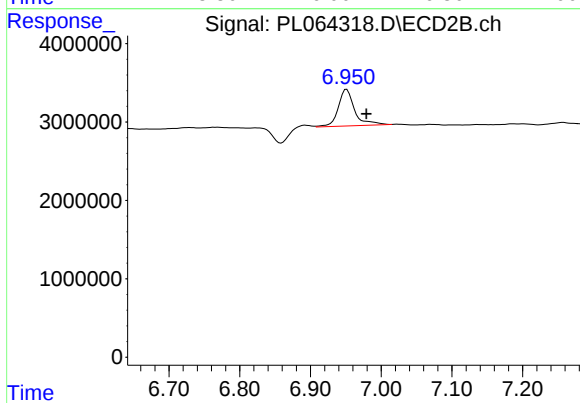

#16 4,4'-DDD


R.T.: 6.951 min
Delta R.T.: -0.028 min
Response: 7482026
Conc: 3.38 ng/ml

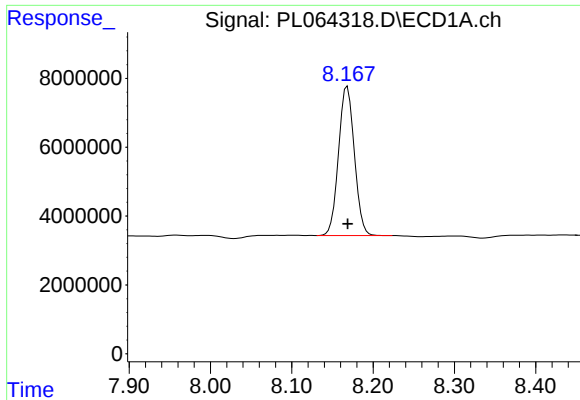

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 58439287
Conc: 19.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

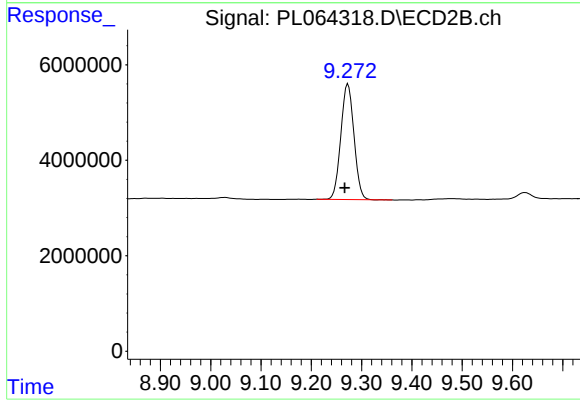

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.007 min
Response: 44038187
Conc: 18.55 ng/ml