

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012323\
 Data File : PL080470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2023 14:35
 Operator : AR\AJ
 Sample : 01243-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TJRC-011923-B4-30-40

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/24/2023
 Supervised By :Ankita Jodhani 01/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 21:03:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.350	2.689	42698124	44715946	19.907m	20.358
2)	SA Decachlor...	8.789	7.839	28858967	37046578	16.484	15.549

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012323\
Data File : PL080470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2023 14:35
Operator : AR\AJ
Sample : 01243-08
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
TJRC-011923-B4-30-40


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/24/2023
Supervised By : Ankita Jodhani 01/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 21:03:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

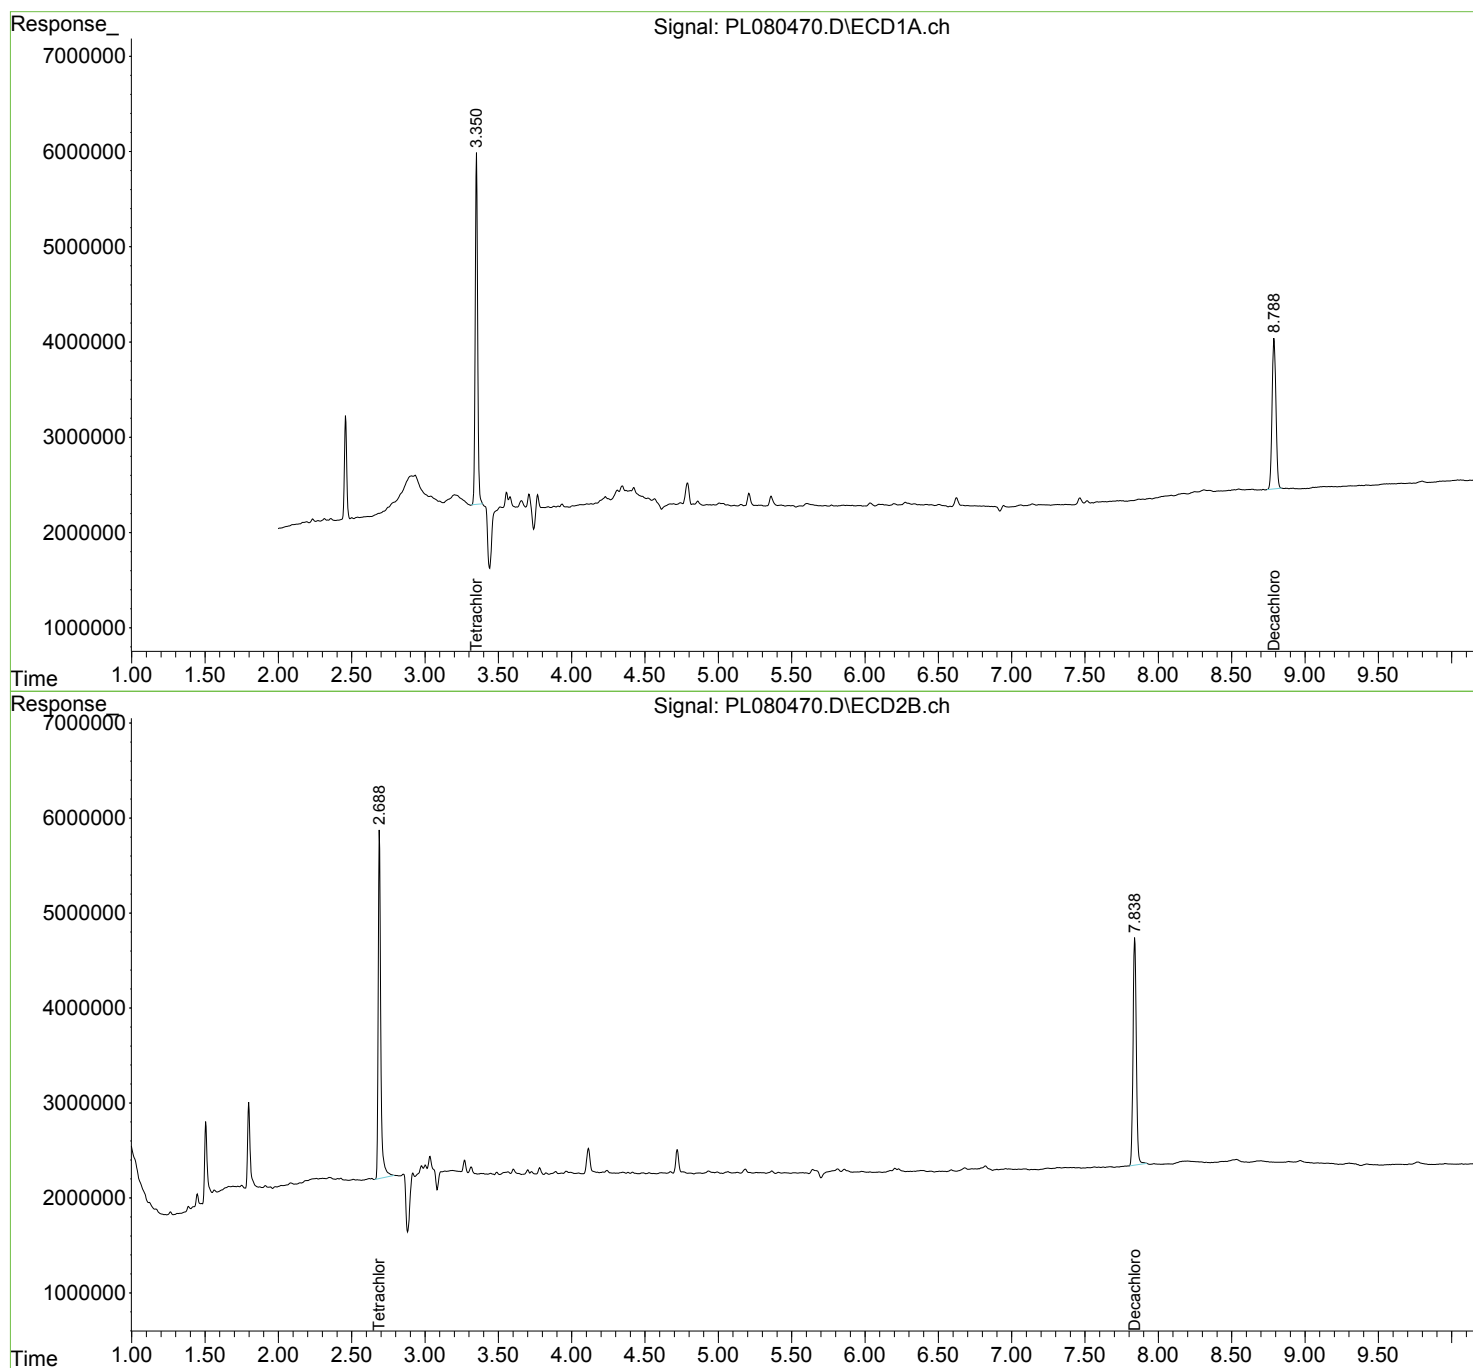

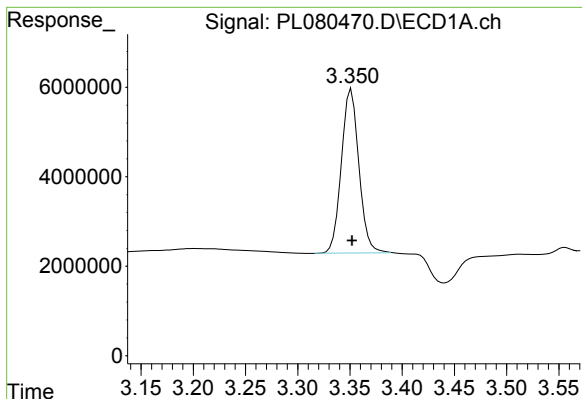


#1 Tetrachloro-m-xylene

R.T.: 3.350 min
Delta R.T.: -0.002 min
Response: 42698124
Conc: 19.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
TJRC-011923-B4-30-40


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/24/2023
Supervised By :Ankita Jodhani 01/24/2023

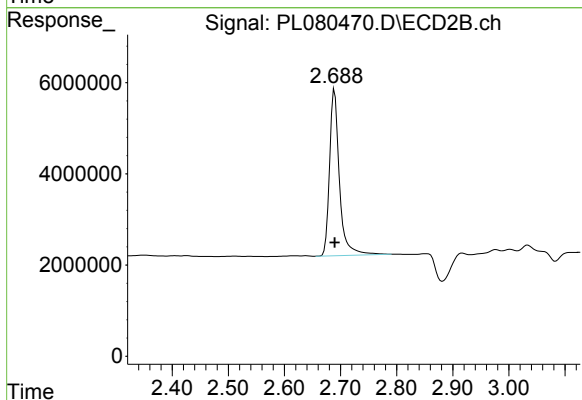


#1 Tetrachloro-m-xylene

R.T.: 2.689 min
Delta R.T.: 0.000 min
Response: 44715946
Conc: 20.36 ng/ml

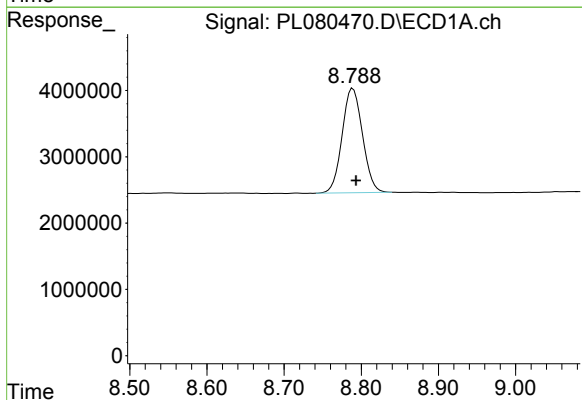

#28 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: -0.004 min
Response: 28858967
Conc: 16.48 ng/ml

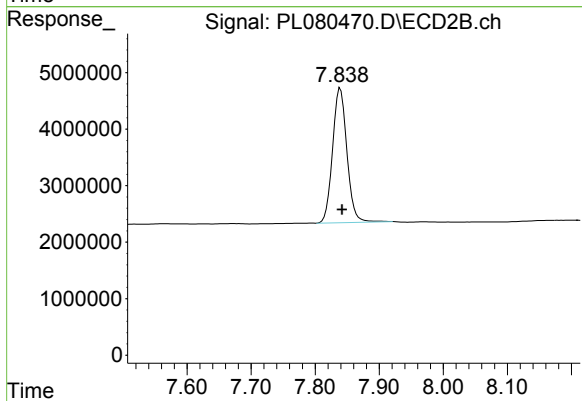

#28 Decachlorobiphenyl

R.T.: 7.839 min
Delta R.T.: -0.003 min
Response: 37046578
Conc: 15.55 ng/ml