

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012323\
 Data File : PL080472.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2023 15:03
 Operator : AR\AJ
 Sample : 01251-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/24/2023
 Supervised By : Ankita Jodhani 01/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 21:04:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.349	2.689	41991576	44396520	19.578m	20.213
28)	SA Decachlor...	8.789	7.838	27924598	36140041	15.950	15.169
Target Compounds							
17)	MA 4,4'-DDT	6.813	5.951	1944320	1844591	0.936m	0.878m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012323\
Data File : PL080472.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2023 15:03
Operator : AR\AJ
Sample : 01251-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/24/2023
Supervised By : Ankita Jodhani 01/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 21:04:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

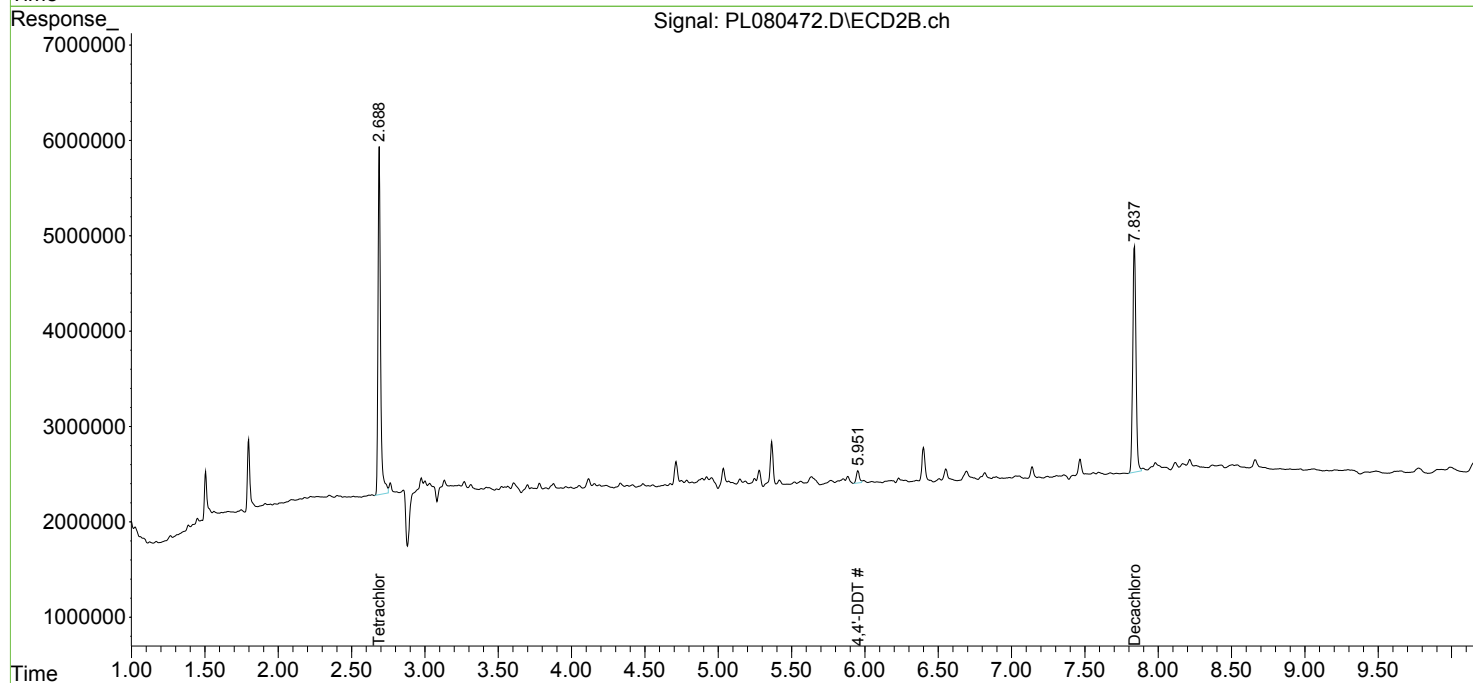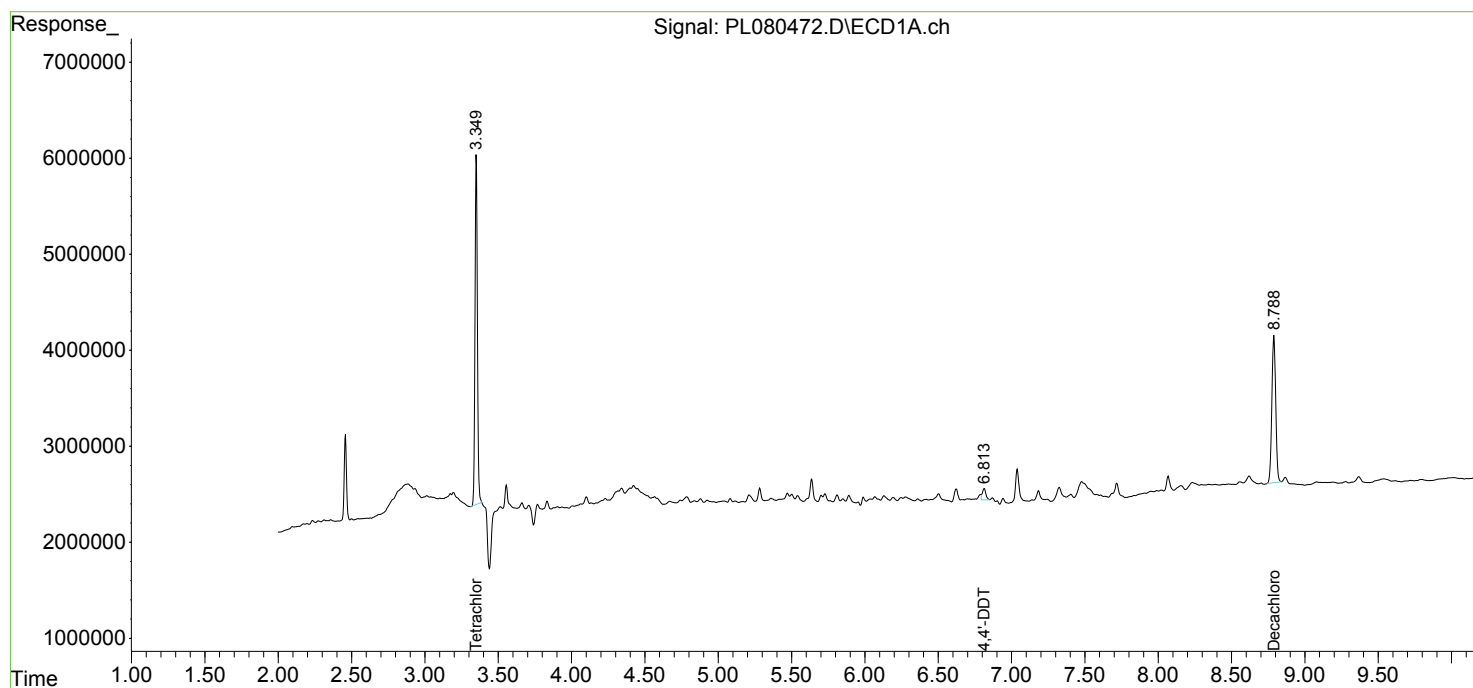

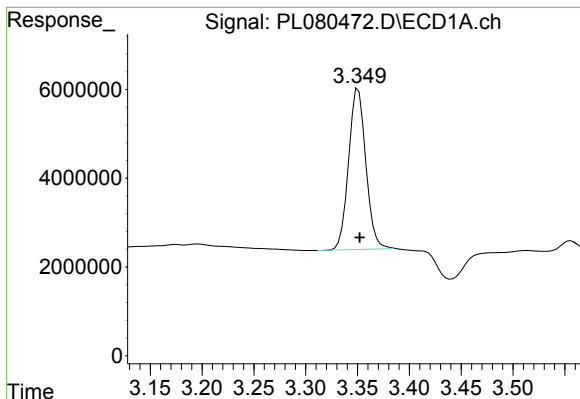


#1 Tetrachloro-m-xylene

R.T.: 3.349 min
Delta R.T.: -0.003 min
Response: 41991576
Conc: 19.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/24/2023
Supervised By :Ankita Jodhani 01/24/2023

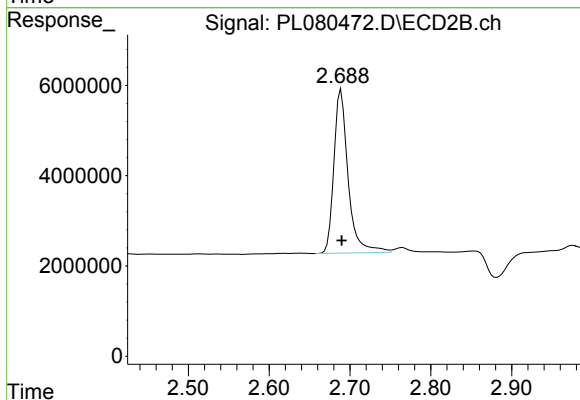


#1 Tetrachloro-m-xylene

R.T.: 2.689 min
Delta R.T.: 0.000 min
Response: 44396520
Conc: 20.21 ng/ml

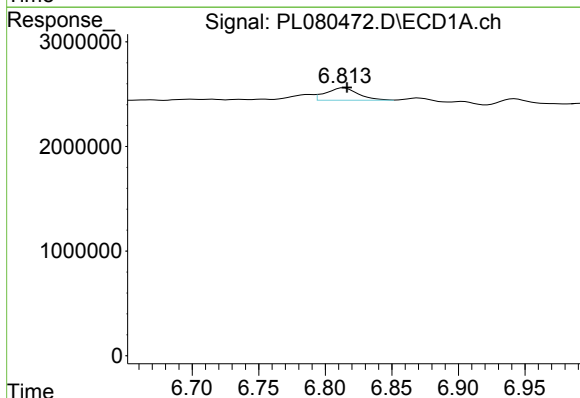


#17 4,4'-DDT

R.T.: 6.813 min
Delta R.T.: -0.004 min
Response: 1944320
Conc: 0.94 ng/ml m

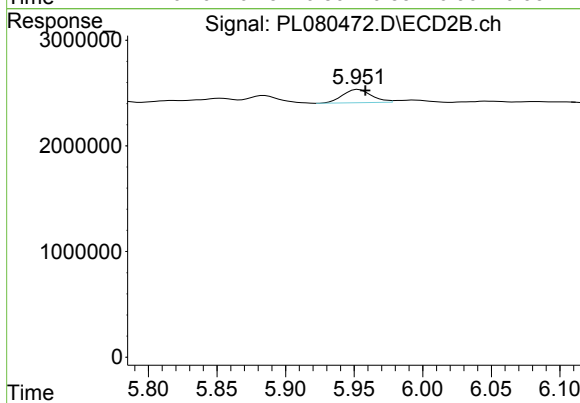

#17 4,4'-DDT

R.T.: 5.951 min
Delta R.T.: -0.007 min
Response: 1844591
Conc: 0.88 ng/ml m

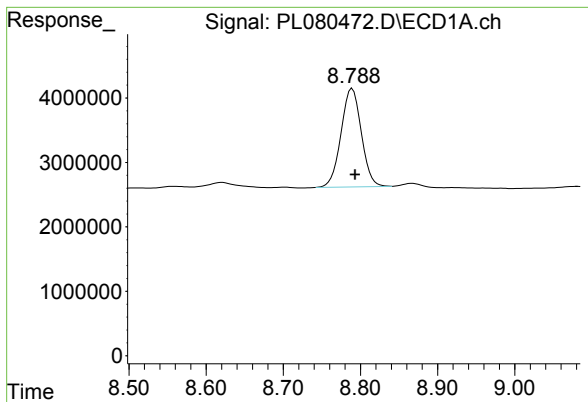


#28 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: -0.004 min
Response: 27924598
Conc: 15.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/24/2023
Supervised By :Ankita Jodhani 01/24/2023

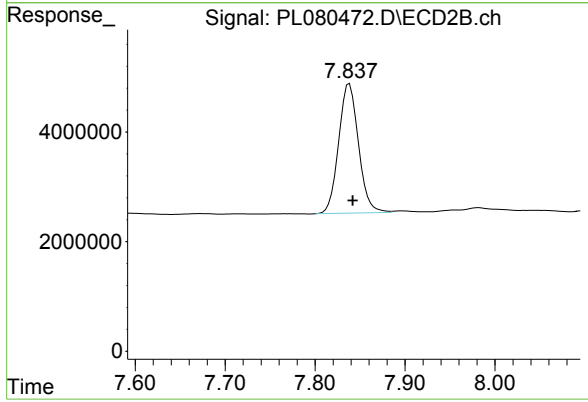

#28 Decachlorobiphenyl

R.T.: 7.838 min
Delta R.T.: -0.004 min
Response: 36140041
Conc: 15.17 ng/ml