

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012324\
 Data File : PL087915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2024 16:32
 Operator : AR\AJ
 Sample : P1187-07
 Misc : PEST LOD 2.5PPB
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 00:31:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 03:17:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.673	62818626	26869314	20.983	22.181
28)	SA Decachlor...	8.977	7.858	67117052	31360486	23.566	24.755
Target Compounds							
2)	A alpha-BHC	3.875	3.176	8997318	3520652	2.005	1.910
3)	MA gamma-BHC...	4.208	3.507	9132838	3689028	2.094	2.030
4)	MA Heptachlor	4.801	3.848	10494173	3502026	2.388	1.966
5)	MB Aldrin	5.144	4.128	9271603	3429649	2.163	1.943
6)	B beta-BHC	4.409	3.808	4781638	1409447	2.570	1.843 #
7)	B delta-BHC	4.655	4.037	10450658	3118938	2.484	1.797 #
8)	B Heptachlo...	5.574	4.636	9801472	3588108	2.558	2.251
9)	A Endosulfan I	5.960	5.007	8974567	3357269	2.489	2.170
10)	B gamma-Chl...	5.833	4.889	10163917	3748004	2.629	2.322
11)	B alpha-Chl...	5.913	4.953	9727747	3764911	2.531	2.269
12)	B 4,4'-DDE	6.094	5.151	7222026	2735375	2.259	2.034
13)	MA Dieldrin	6.239	5.275	8766957	3502825	2.354	2.204
14)	MA Endrin	6.469	5.550	7192519	3065680	2.290	2.162
15)	B Endosulfa...	6.690	5.847	8144765	3410709	2.540	2.491
16)	A 4,4'-DDD	6.614	5.709	5367022	2436916	2.081	2.161
17)	MA 4,4'-DDT	6.932	5.962	7131284	2782255	2.494	2.235
18)	B Endrin al...	6.822	6.028	6491897	2894543	2.581	2.491
19)	B Endosulfa...	7.059	6.254	7976465	3293231	2.608	2.509
20)	A Methoxychlor	7.417	6.548	4097926	1682366	2.524	2.286
21)	B Endrin ke...	7.545	6.760	8262643	3472839	2.540	2.265
22)	Mirex	8.022	6.941	8151850	3716032	2.907	2.770
24)	Chlordane-2	5.144f	0.000	9271603	0	62.872	N.D. #
25)	Chlordane-3	5.833	4.889	10163917	3748004	18.272	23.683 #
26)	Chlordane-4	5.913	4.953	9727747	3764911	14.063	22.035 #
27)	Chlordane-5	0.000	5.631	0	10541	N.D.	0.224 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012324\
Data File : PL087915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2024 16:32
Operator : AR\AJ
Sample : P1187-07
Misc : PEST LOD 2.5PPB
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 00:31:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:17:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

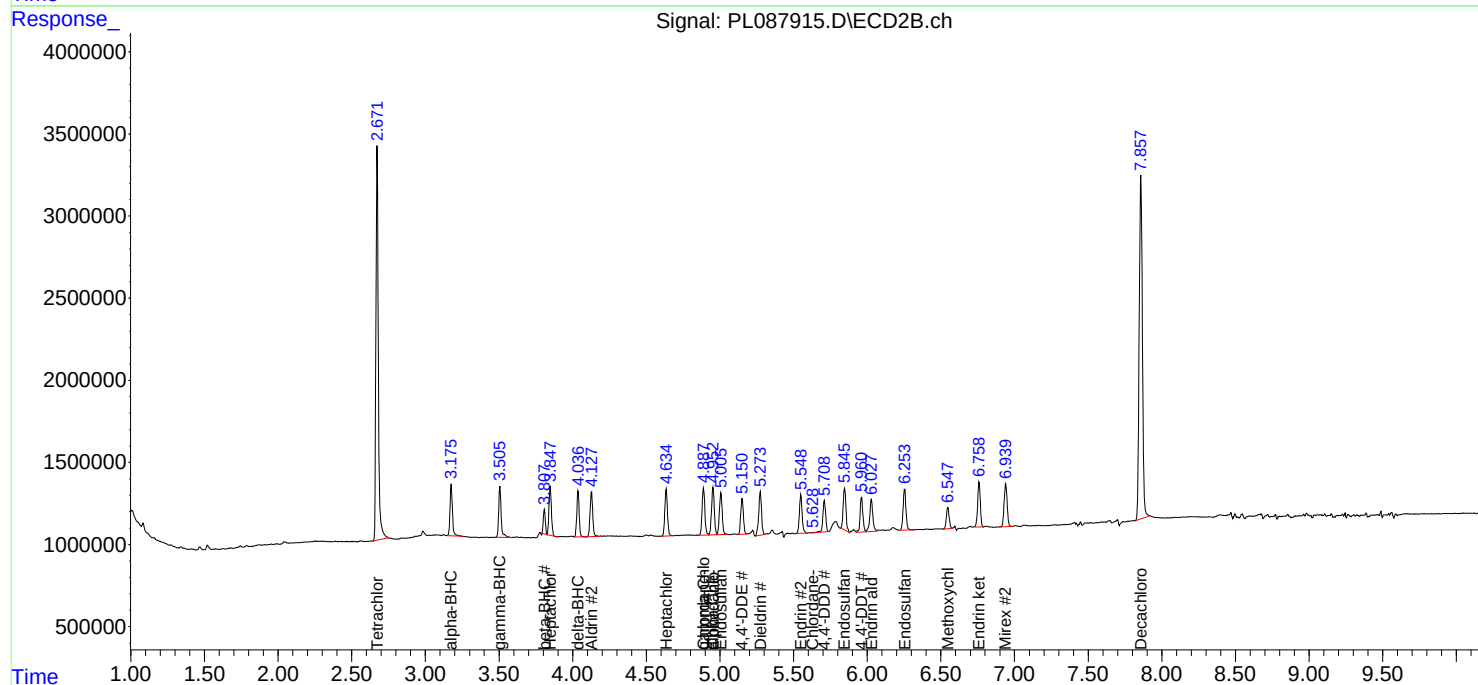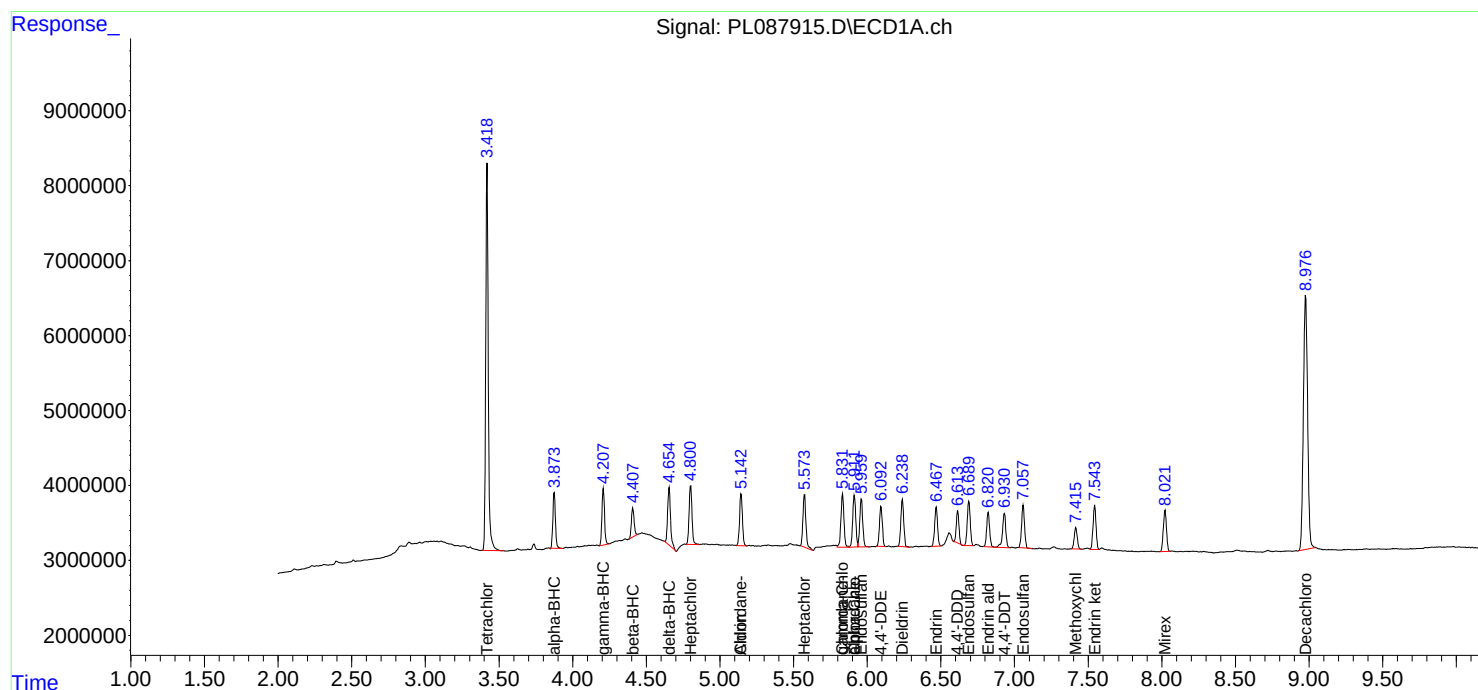


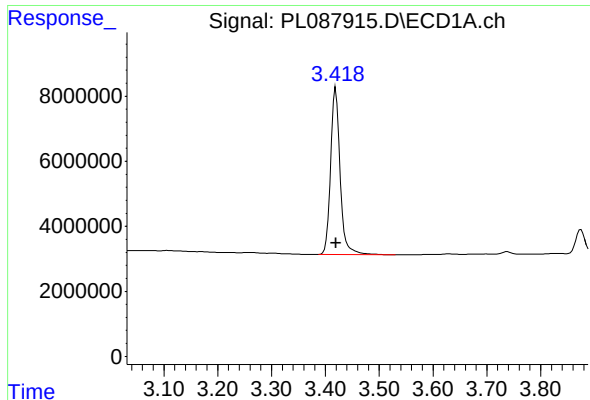

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 62818626
Conc: 20.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

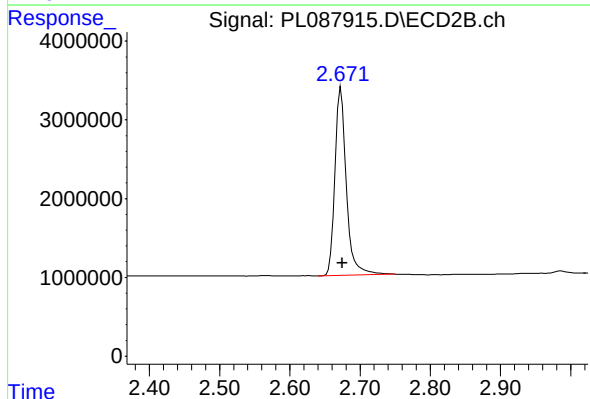


#1 Tetrachloro-m-xylene

R.T.: 2.673 min
Delta R.T.: -0.002 min
Response: 26869314
Conc: 22.18 ng/ml

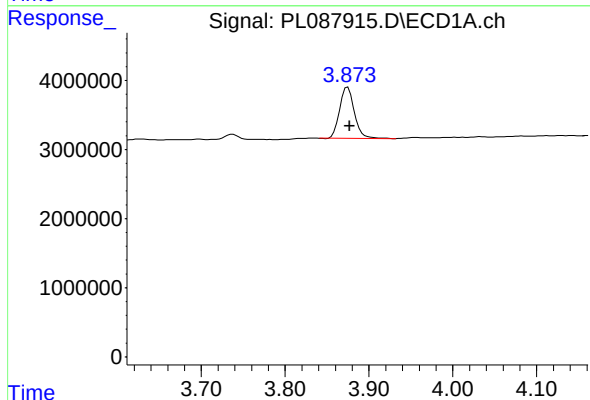


#2 alpha-BHC

R.T.: 3.875 min
Delta R.T.: -0.002 min
Response: 8997318
Conc: 2.01 ng/ml

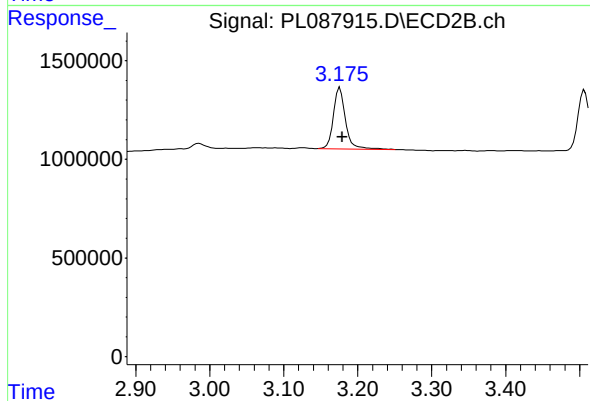

#2 alpha-BHC


R.T.: 3.176 min
Delta R.T.: -0.003 min
Response: 3520652
Conc: 1.91 ng/ml

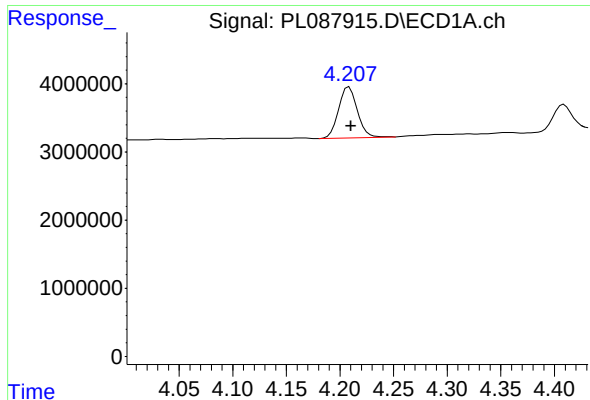

#3 gamma-BHC (Lindane)


R.T.: 4.208 min
Delta R.T.: -0.002 min
Response: 9132838
Conc: 2.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

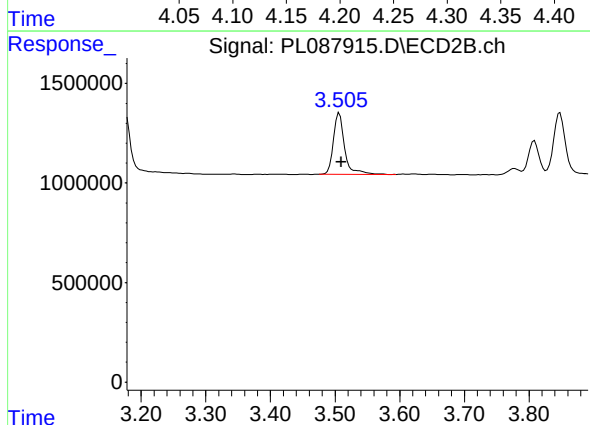


#3 gamma-BHC (Lindane)

R.T.: 3.507 min
Delta R.T.: -0.003 min
Response: 3689028
Conc: 2.03 ng/ml

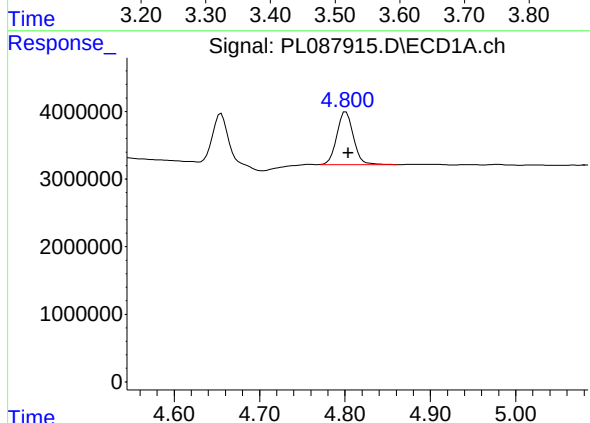


#4 Heptachlor

R.T.: 4.801 min
Delta R.T.: -0.002 min
Response: 10494173
Conc: 2.39 ng/ml

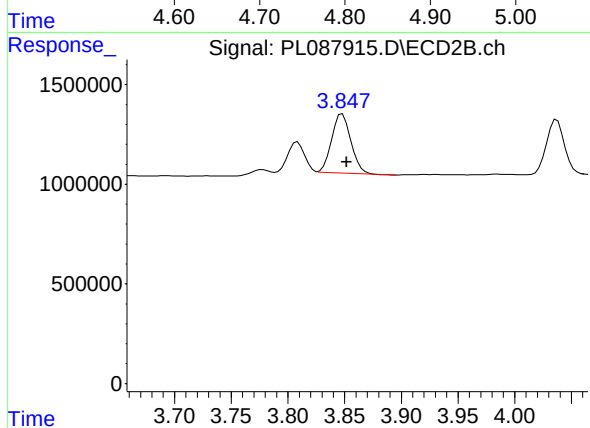

#4 Heptachlor


R.T.: 3.848 min
Delta R.T.: -0.004 min
Response: 3502026
Conc: 1.97 ng/ml

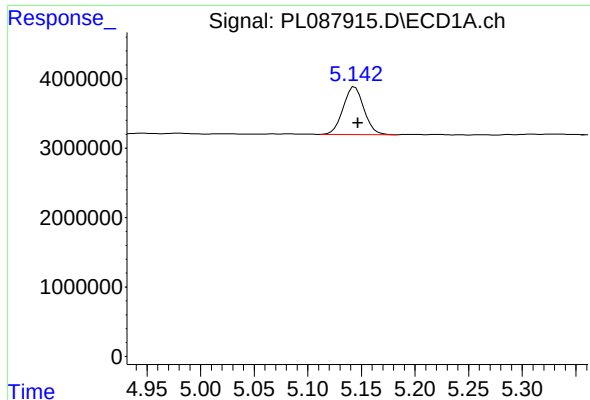

#5 Aldrin


R.T.: 5.144 min
Delta R.T.: -0.003 min
Response: 9271603
Conc: 2.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

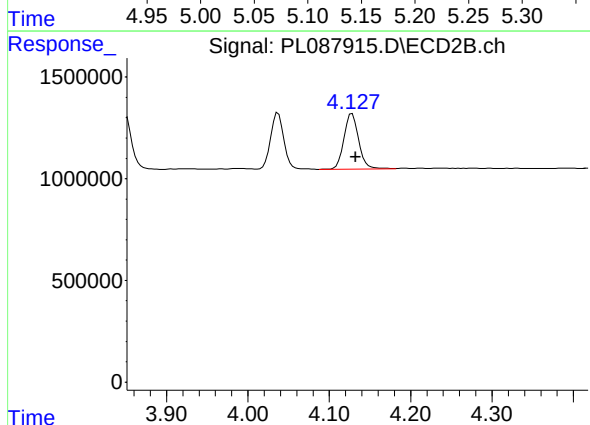


#5 Aldrin

R.T.: 4.128 min
Delta R.T.: -0.004 min
Response: 3429649
Conc: 1.94 ng/ml

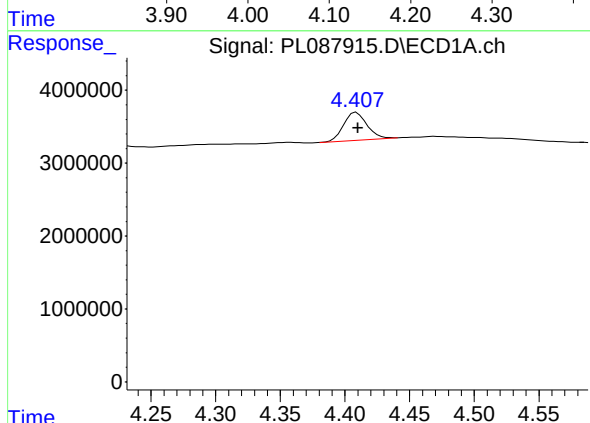


#6 beta-BHC

R.T.: 4.409 min
Delta R.T.: -0.001 min
Response: 4781638
Conc: 2.57 ng/ml

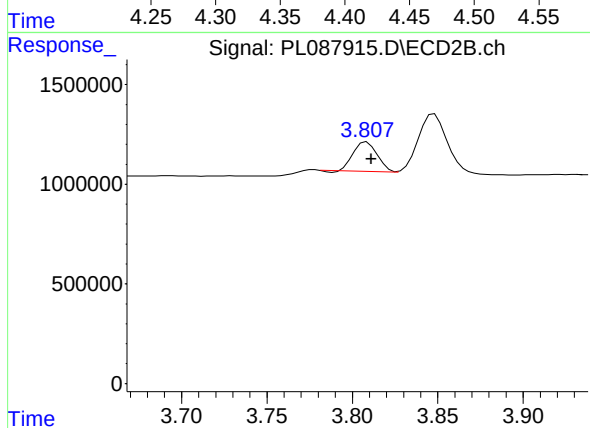

#6 beta-BHC


R.T.: 3.808 min
Delta R.T.: -0.003 min
Response: 1409447
Conc: 1.84 ng/ml

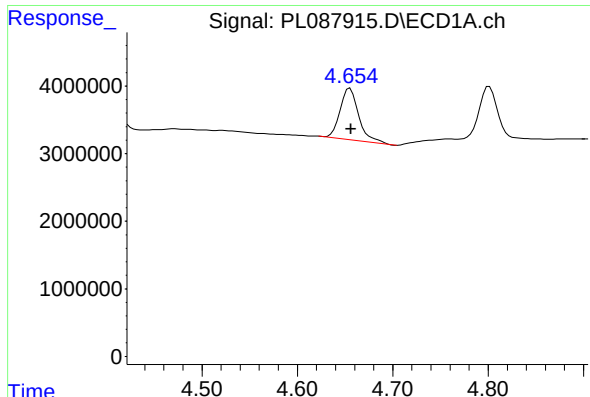

#7 delta-BHC


R.T.: 4.655 min
Delta R.T.: -0.001 min
Response: 10450658
Conc: 2.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

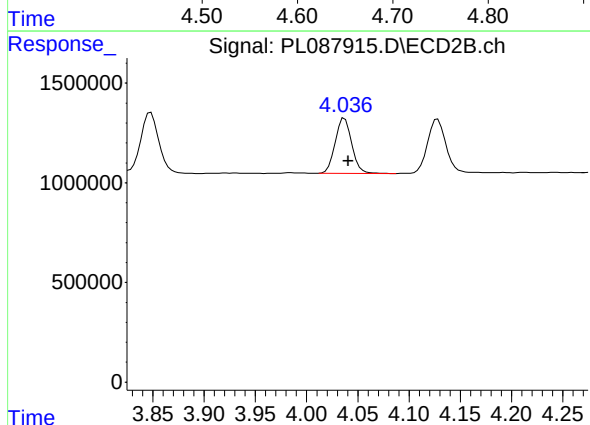


#7 delta-BHC

R.T.: 4.037 min
Delta R.T.: -0.003 min
Response: 3118938
Conc: 1.80 ng/ml

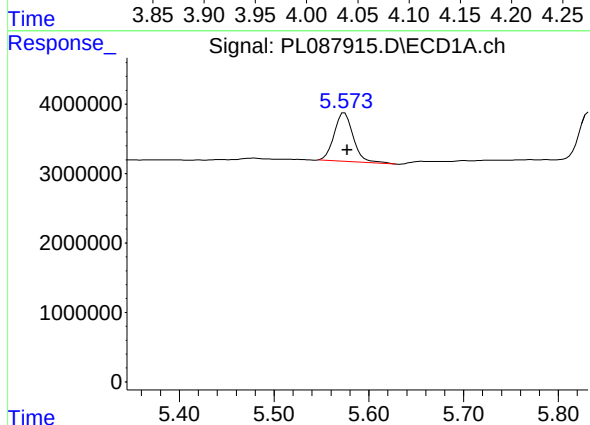


#8 Heptachlor epoxide

R.T.: 5.574 min
Delta R.T.: -0.003 min
Response: 9801472
Conc: 2.56 ng/ml

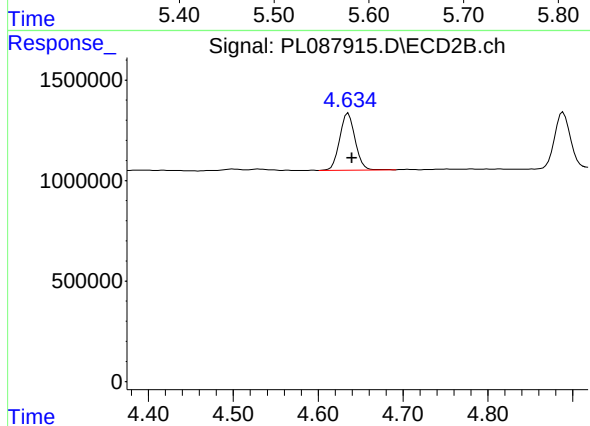

#8 Heptachlor epoxide


R.T.: 4.636 min
Delta R.T.: -0.005 min
Response: 3588108
Conc: 2.25 ng/ml

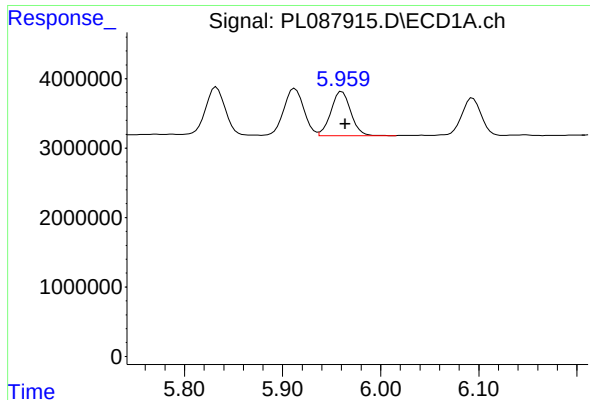

#9 Endosulfan I


R.T.: 5.960 min
Delta R.T.: -0.003 min
Response: 8974567
Conc: 2.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

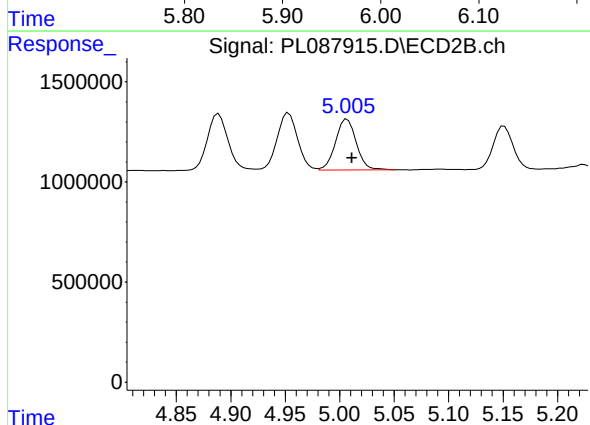


#9 Endosulfan I

R.T.: 5.007 min
Delta R.T.: -0.004 min
Response: 3357269
Conc: 2.17 ng/ml

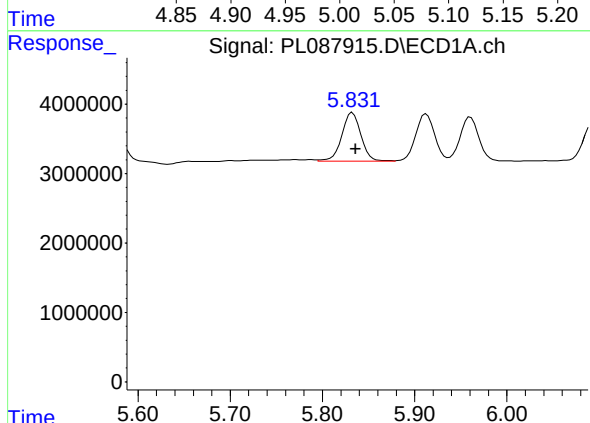


#10 gamma-Chlordane

R.T.: 5.833 min
Delta R.T.: -0.003 min
Response: 10163917
Conc: 2.63 ng/ml

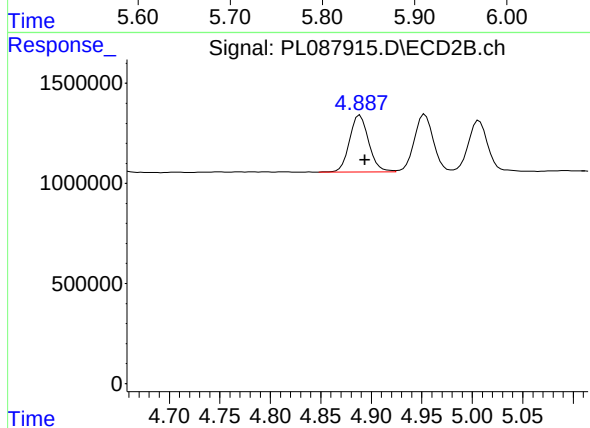

#10 gamma-Chlordane

R.T.: 4.889 min
Delta R.T.: -0.005 min
Response: 3748004
Conc: 2.32 ng/ml

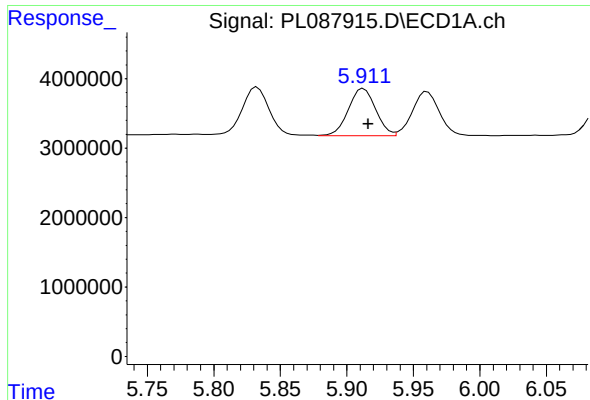

#11 alpha-Chlordane


R.T.: 5.913 min
Delta R.T.: -0.003 min
Response: 9727747
Conc: 2.53 ng/ml

Instrument :

ECD_L


ClientSampleId :

LOD-MDL-WATER-01-QT1-2024

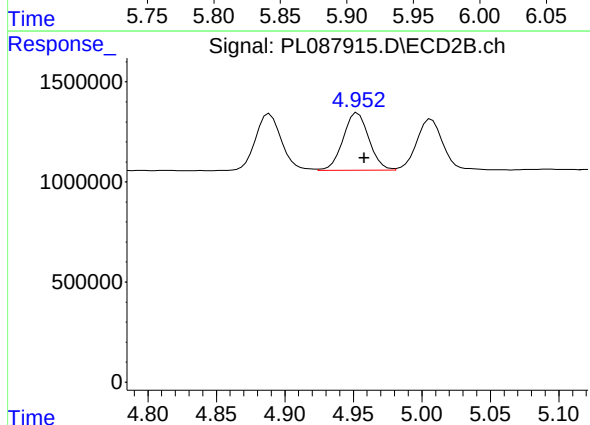


#11 alpha-Chlordane

R.T.: 4.953 min
Delta R.T.: -0.005 min
Response: 3764911
Conc: 2.27 ng/ml

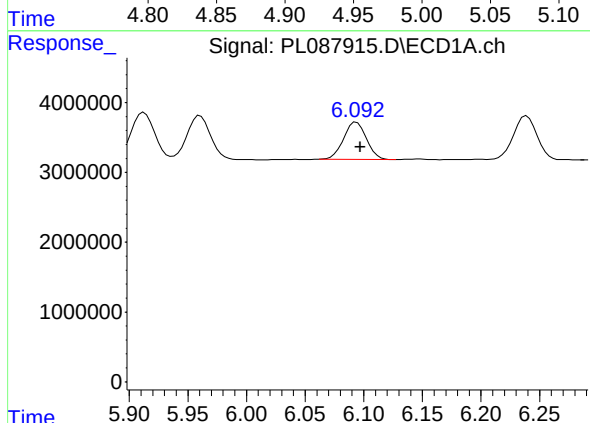


#12 4,4'-DDE

R.T.: 6.094 min
Delta R.T.: -0.003 min
Response: 7222026
Conc: 2.26 ng/ml

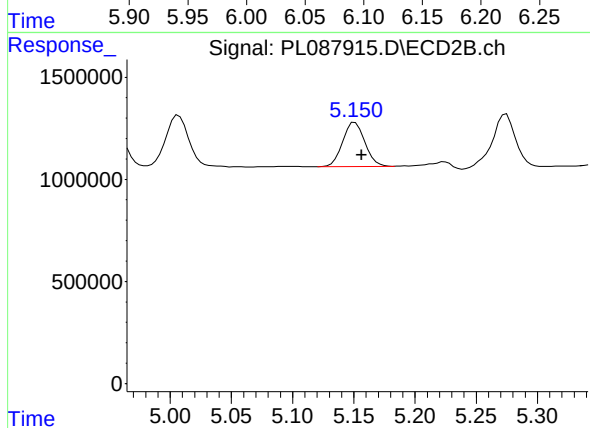

#12 4,4'-DDE


R.T.: 5.151 min
Delta R.T.: -0.005 min
Response: 2735375
Conc: 2.03 ng/ml

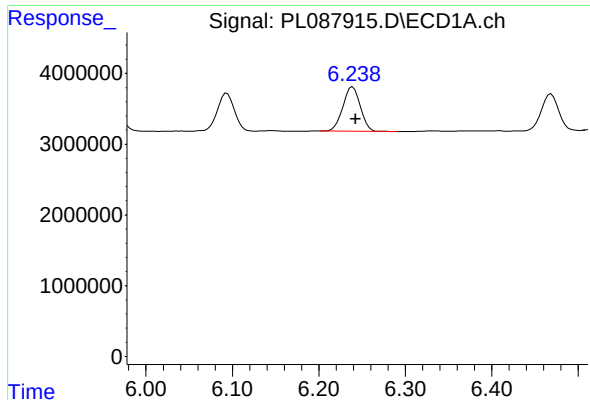

#13 Dieldrin


R.T.: 6.239 min
Delta R.T.: -0.003 min
Response: 8766957
Conc: 2.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

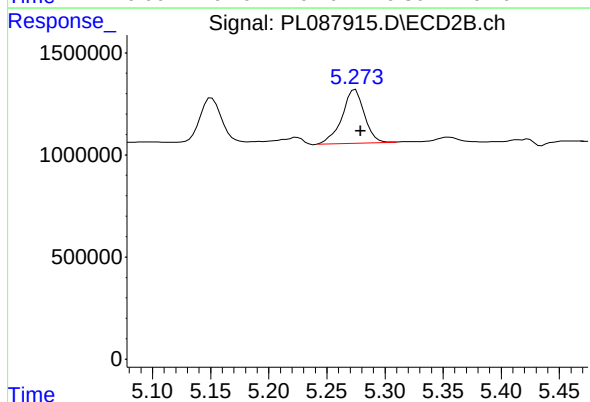


#13 Dieldrin

R.T.: 5.275 min
Delta R.T.: -0.004 min
Response: 3502825
Conc: 2.20 ng/ml

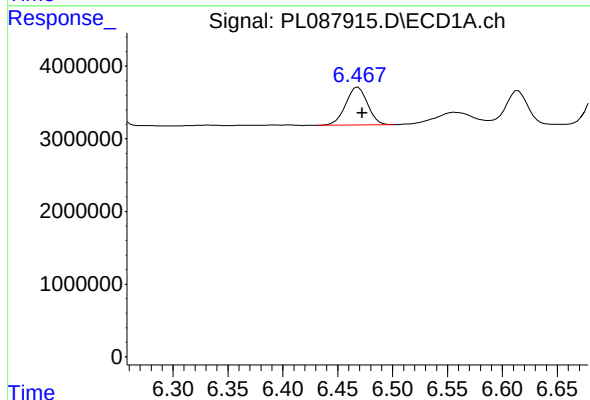


#14 Endrin

R.T.: 6.469 min
Delta R.T.: -0.004 min
Response: 7192519
Conc: 2.29 ng/ml

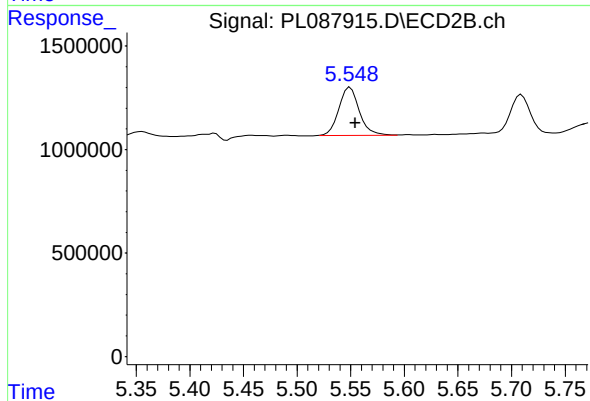

#14 Endrin


R.T.: 5.550 min
Delta R.T.: -0.005 min
Response: 3065680
Conc: 2.16 ng/ml

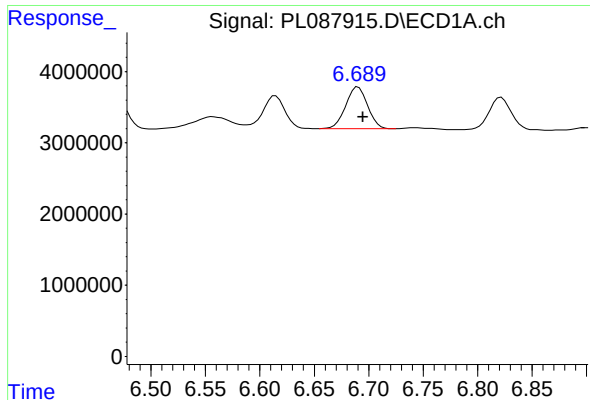

#15 Endosulfan II


R.T.: 6.690 min
Delta R.T.: -0.004 min
Response: 8144765
Conc: 2.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

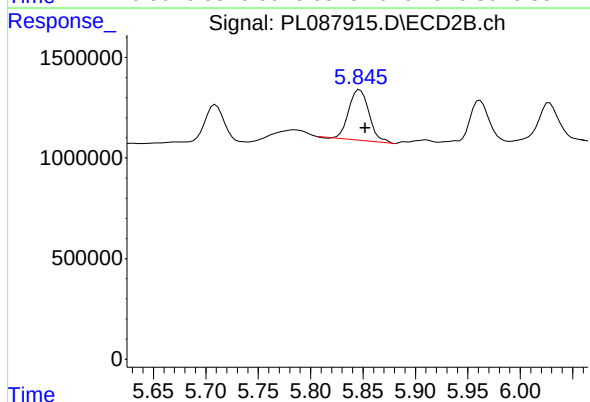


#15 Endosulfan II

R.T.: 5.847 min
Delta R.T.: -0.005 min
Response: 3410709
Conc: 2.49 ng/ml

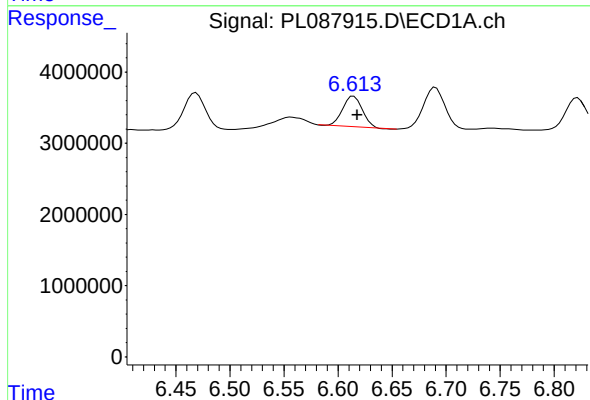


#16 4,4'-DDD

R.T.: 6.614 min
Delta R.T.: -0.003 min
Response: 5367022
Conc: 2.08 ng/ml

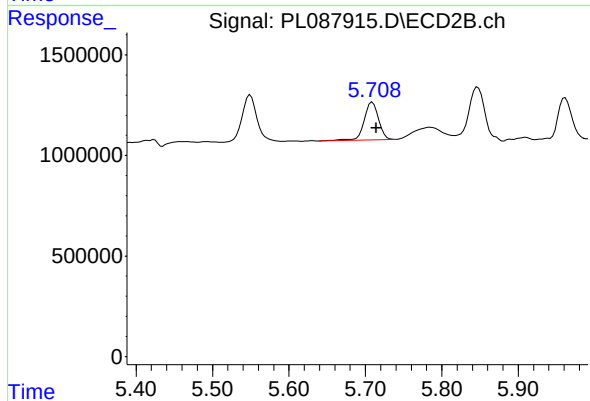

#16 4,4'-DDD


R.T.: 5.709 min
Delta R.T.: -0.005 min
Response: 2436916
Conc: 2.16 ng/ml

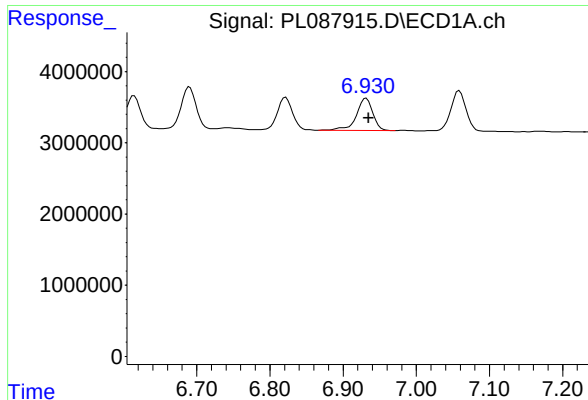

#17 4,4'-DDT


R.T.: 6.932 min
Delta R.T.: -0.003 min
Response: 7131284
Conc: 2.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

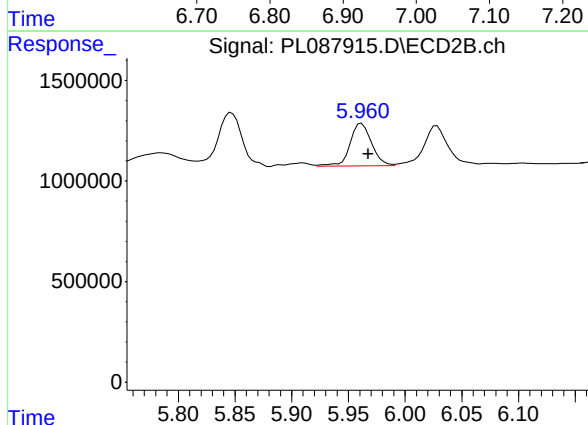


#17 4,4'-DDT

R.T.: 5.962 min
Delta R.T.: -0.006 min
Response: 2782255
Conc: 2.24 ng/ml

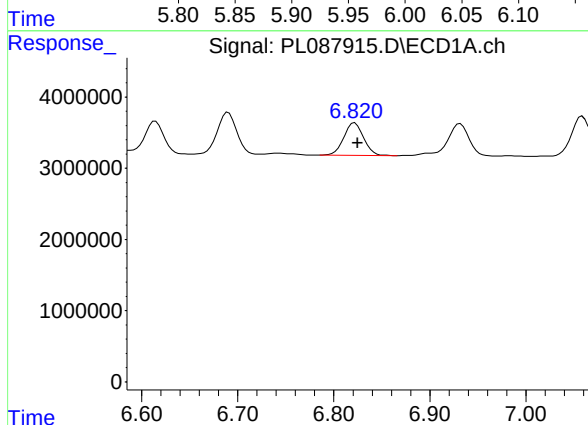


#18 Endrin aldehyde

R.T.: 6.822 min
Delta R.T.: -0.003 min
Response: 6491897
Conc: 2.58 ng/ml

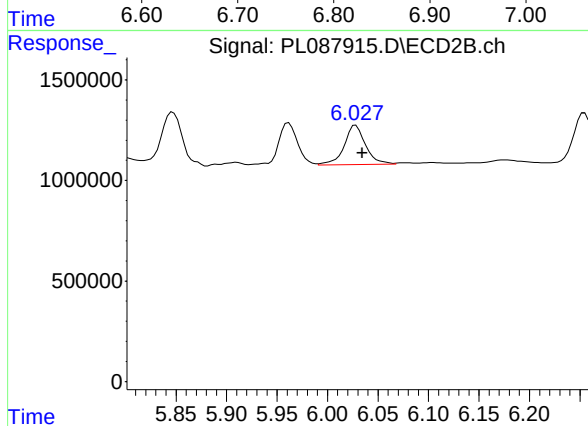

#18 Endrin aldehyde


R.T.: 6.028 min
Delta R.T.: -0.007 min
Response: 2894543
Conc: 2.49 ng/ml

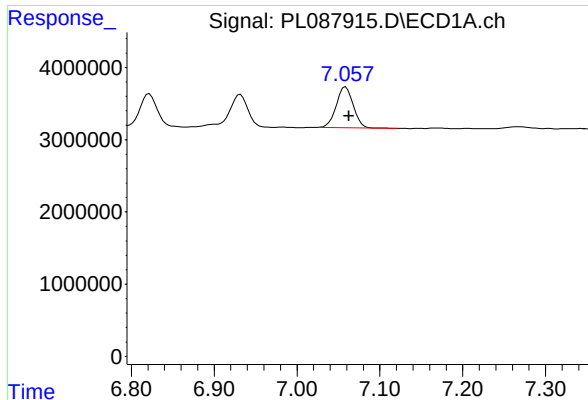

#19 Endosulfan Sulfate


R.T.: 7.059 min
Delta R.T.: -0.004 min
Response: 7976465
Conc: 2.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

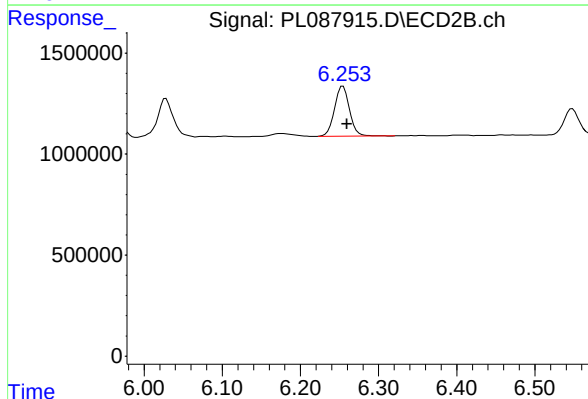


#19 Endosulfan Sulfate

R.T.: 6.254 min
Delta R.T.: -0.005 min
Response: 3293231
Conc: 2.51 ng/ml

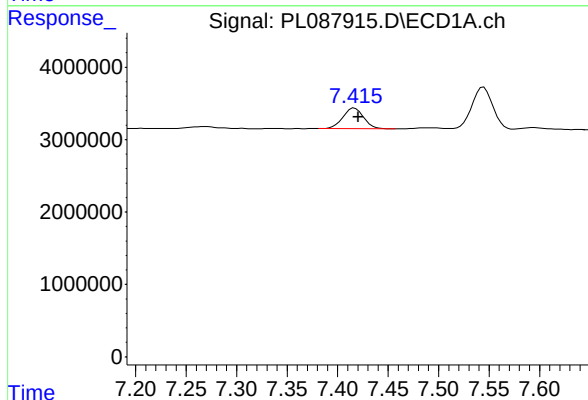


#20 Methoxychlor

R.T.: 7.417 min
Delta R.T.: -0.004 min
Response: 4097926
Conc: 2.52 ng/ml

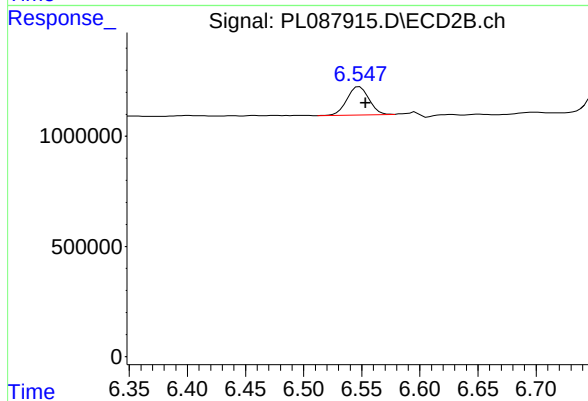

#20 Methoxychlor

R.T.: 6.548 min
Delta R.T.: -0.006 min
Response: 1682366
Conc: 2.29 ng/ml

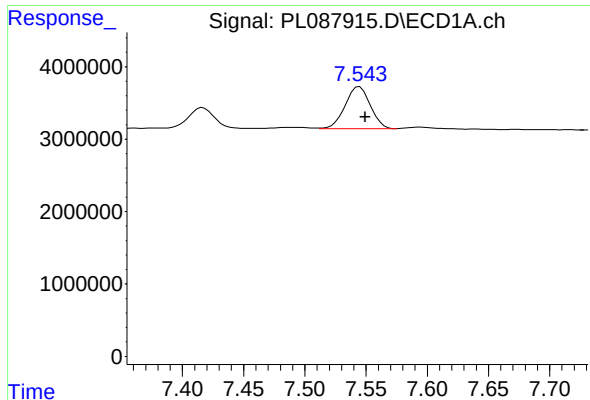

#21 Endrin ketone


R.T.: 7.545 min
Delta R.T.: -0.005 min
Response: 8262643
Conc: 2.54 ng/ml

Instrument :

ECD_L


ClientSampleId :

LOD-MDL-WATER-01-QT1-2024

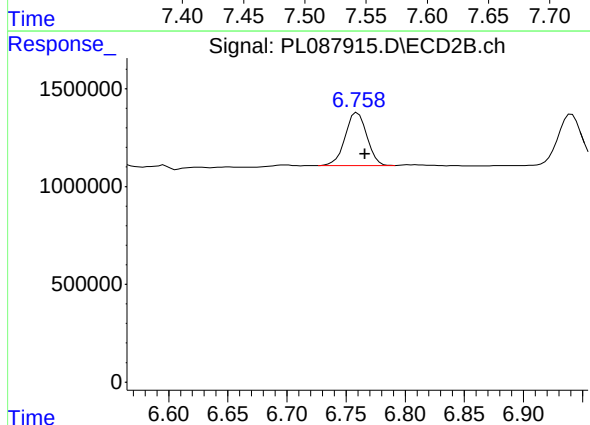


#21 Endrin ketone

R.T.: 6.760 min
Delta R.T.: -0.006 min
Response: 3472839
Conc: 2.27 ng/ml

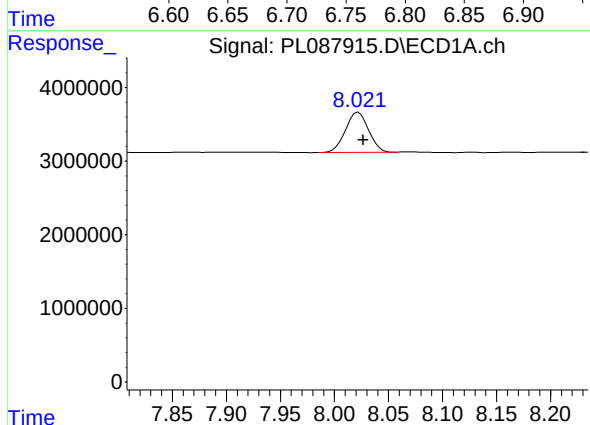


#22 Mirex

R.T.: 8.022 min
Delta R.T.: -0.004 min
Response: 8151850
Conc: 2.91 ng/ml

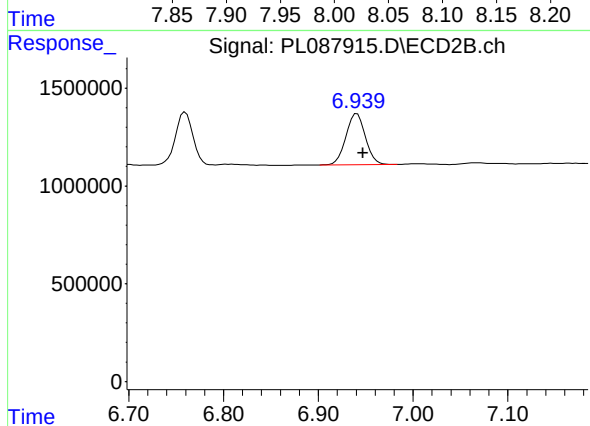

#22 Mirex


R.T.: 6.941 min
Delta R.T.: -0.006 min
Response: 3716032
Conc: 2.77 ng/ml

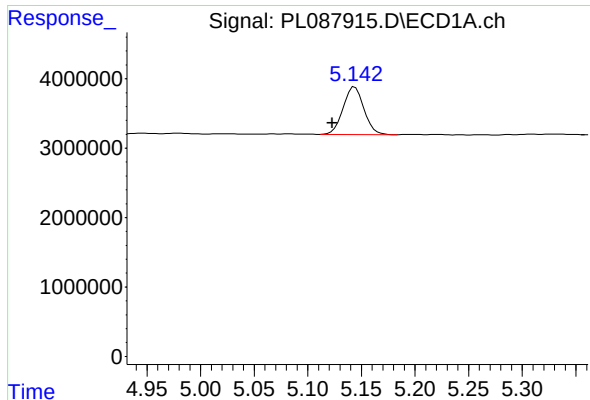

#24 Chlordane-2


R.T.: 5.144 min
Delta R.T.: 0.021 min
Response: 9271603
Conc: 62.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

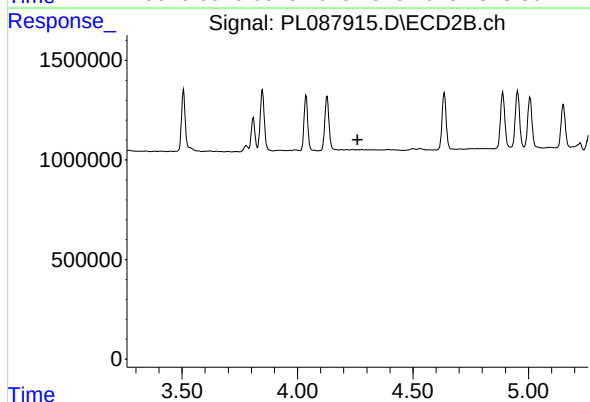


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.259 min
Response: 0
Conc: N.D.

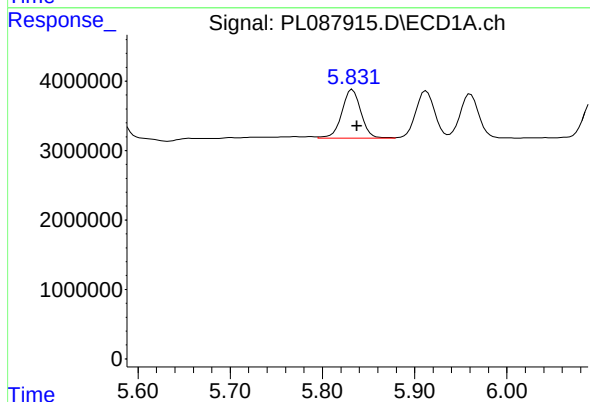


#25 Chlordane-3

R.T.: 5.833 min
Delta R.T.: -0.005 min
Response: 10163917
Conc: 18.27 ng/ml

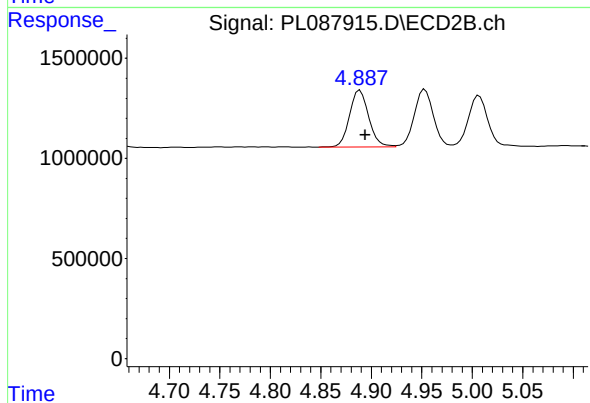

#25 Chlordane-3


R.T.: 4.889 min
Delta R.T.: -0.005 min
Response: 3748004
Conc: 23.68 ng/ml

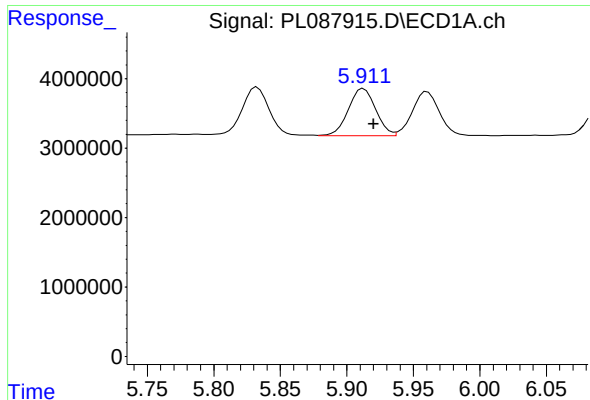

#26 Chlordane-4


R.T.: 5.913 min
Delta R.T.: -0.007 min
Response: 9727747
Conc: 14.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

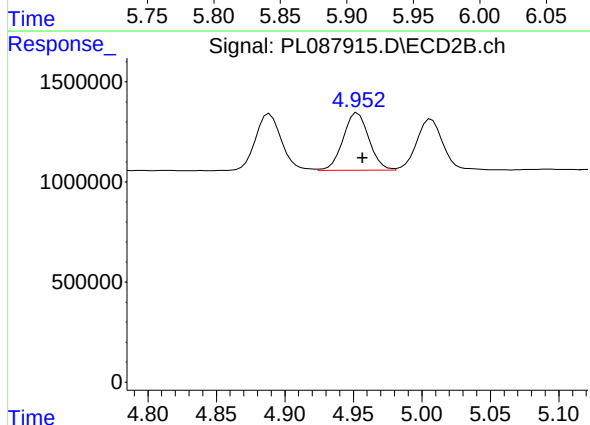


#26 Chlordane-4

R.T.: 4.953 min
Delta R.T.: -0.003 min
Response: 3764911
Conc: 22.04 ng/ml

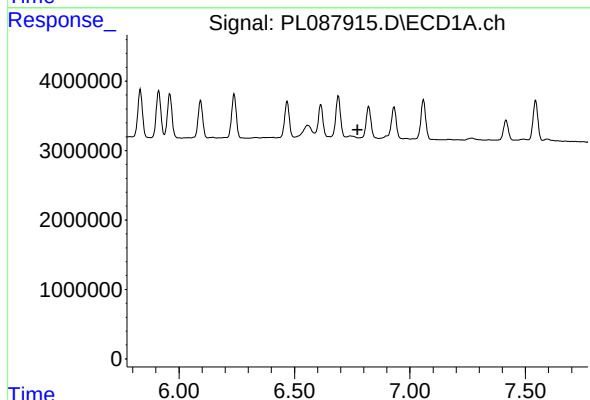


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.773 min
Response: 0
Conc: N.D.

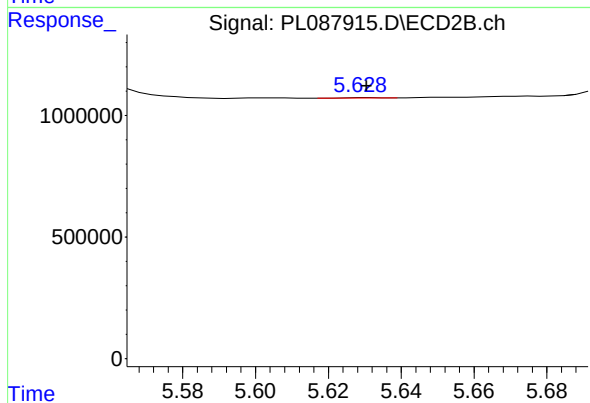

#27 Chlordane-5


R.T.: 5.631 min
Delta R.T.: 0.000 min
Response: 10541
Conc: 0.22 ng/ml

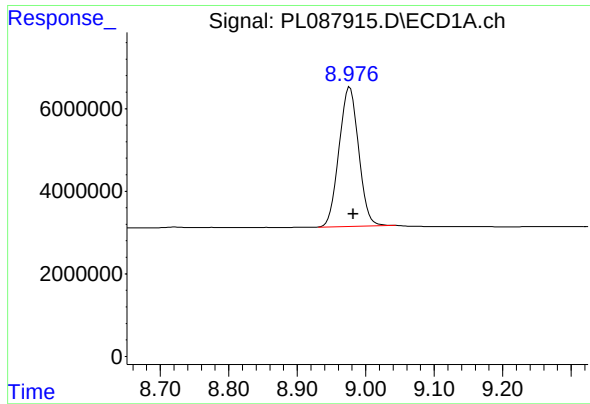

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.005 min
Response: 67117052
Conc: 23.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

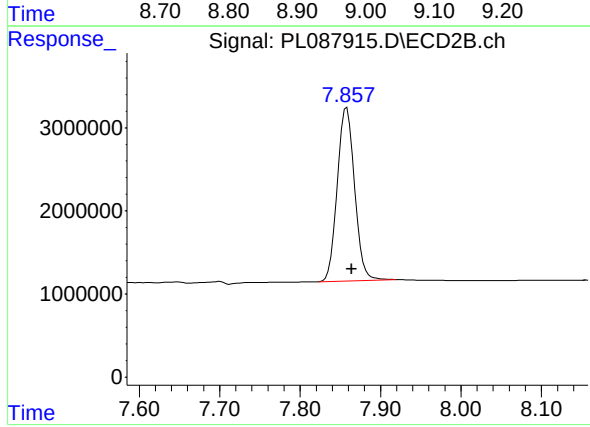

#28 Decachlorobiphenyl

R.T.: 7.858 min
Delta R.T.: -0.006 min
Response: 31360486
Conc: 24.76 ng/ml