

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012420\
 Data File : PL056065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2020 00:10
 Operator : AJ\MA
 Sample : L1247-21
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-10-9-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 02:45:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	3.966	224.0E6	67804437	23.375	23.991
28)	SA Decachlor...	8.233	8.953	209.4E6	48334285	20.024	21.098
Target Compounds							
4)	MA Heptachlor	4.518	0.000	8684170	0	0.582	N.D. #
6)	B beta-BHC	4.473	0.000	5019541	0	0.782	N.D. #
11)	B alpha-Chl...	5.478	0.000	32777227	0	2.371	N.D. #
13)	MA Dieldrin	5.792	0.000	5667297	0	0.410	N.D. #
14)	MA Endrin	6.036	0.000	15755167	0	1.247	N.D. #
15)	B Endosulfa...	0.000	6.849	0	2017627	N.D.	0.752 #
17)	MA 4,4'-DDT	6.399	0.000	4102372	0	0.405	N.D. #
19)	B Endosulfa...	6.721f	0.000	43254	0	0.004	N.D. #
20)	A Methoxychlor	6.935	0.000	3521563	0	0.675	N.D. #
23)	Chlordane-1	4.379f	0.000	10495964	0	28.627	N.D. #
24)	Chlordane-2	4.879f	0.000	3252963	0	7.517	N.D. #
26)	Chlordane-4	5.478	0.000	32777227	0	31.787	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012420\
Data File : PL056065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2020 00:10
Operator : AJ\MA
Sample : L1247-21
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-10-9-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 02:45:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

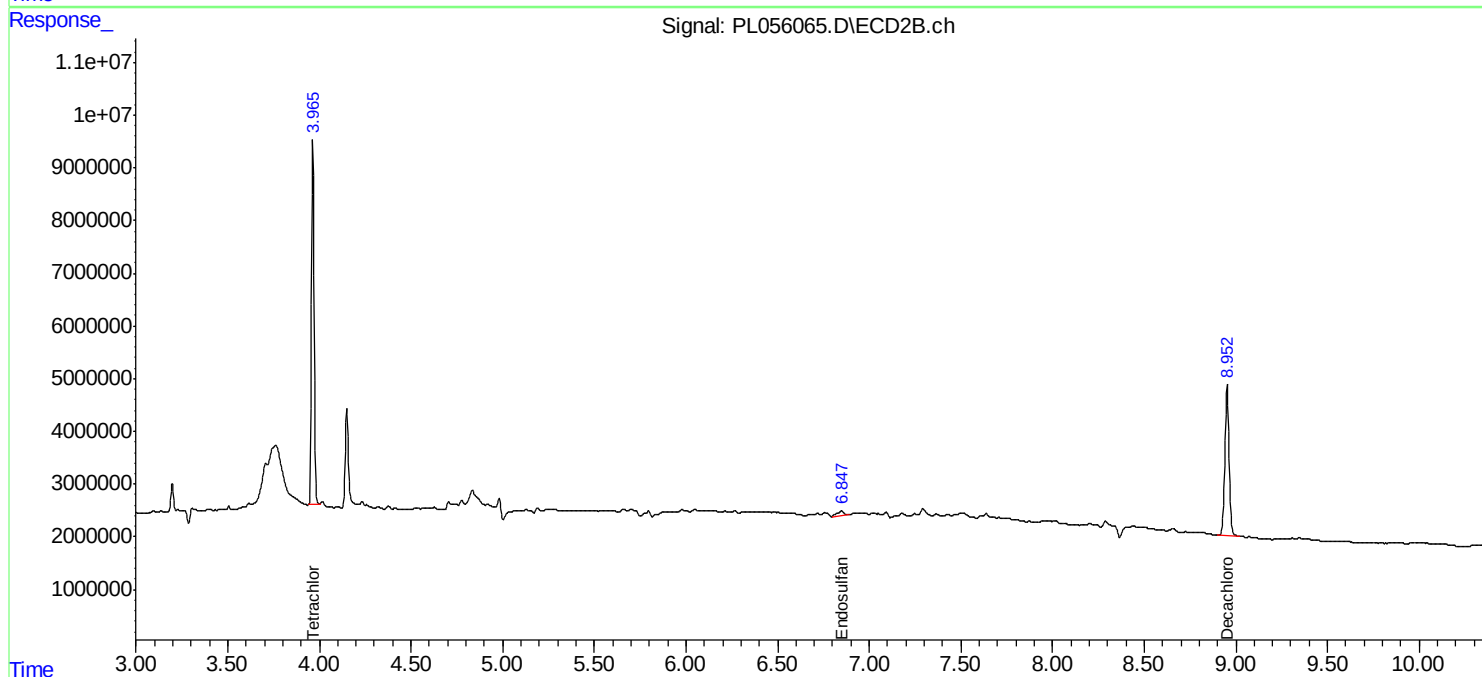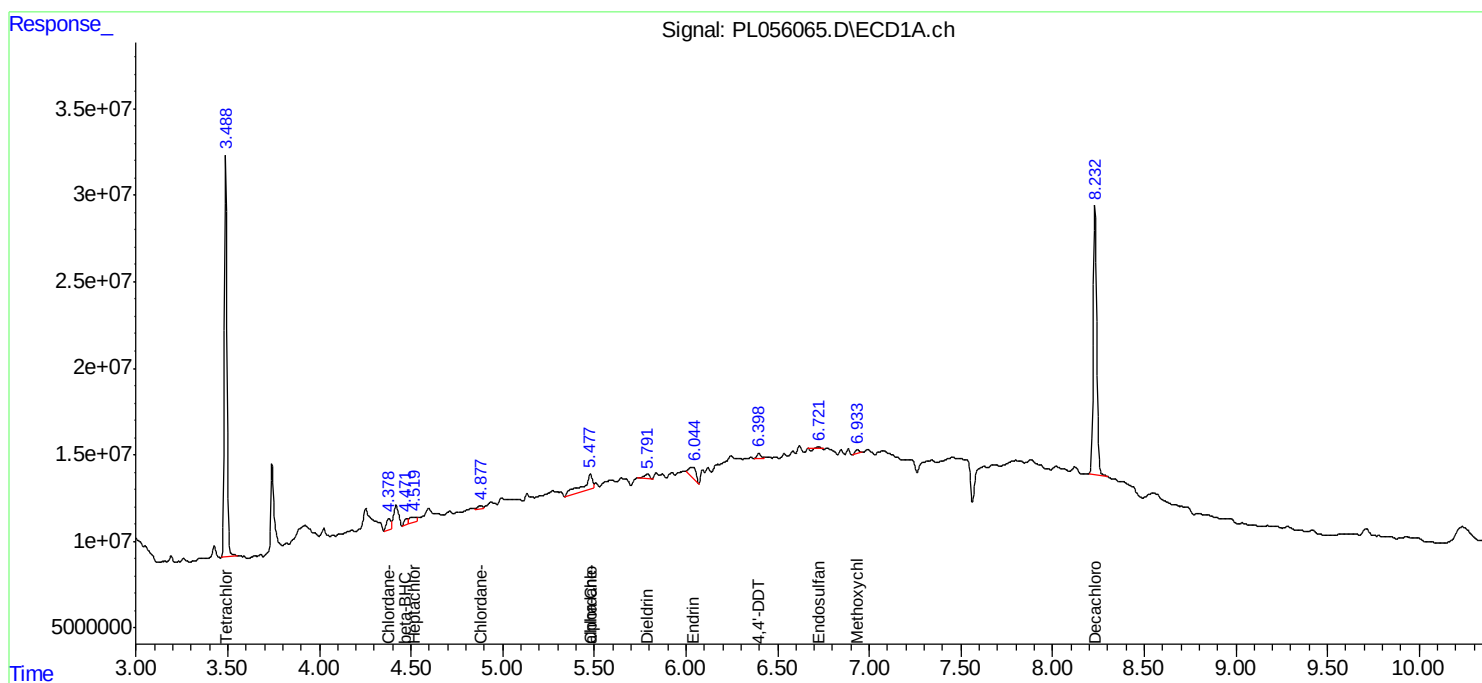


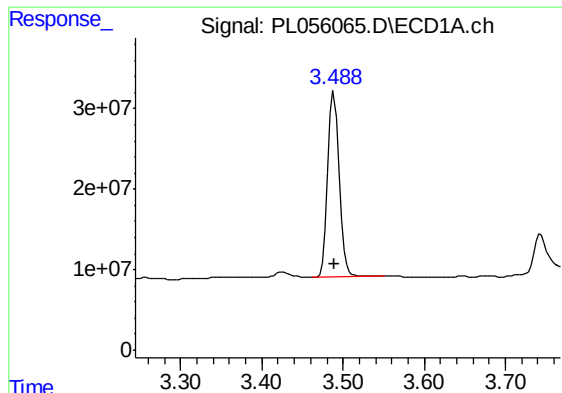

#1 Tetrachloro-m-xylene


R.T.: 3.489 min
Delta R.T.: -0.001 min
Response: 224039075
Conc: 23.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10-9-COMP

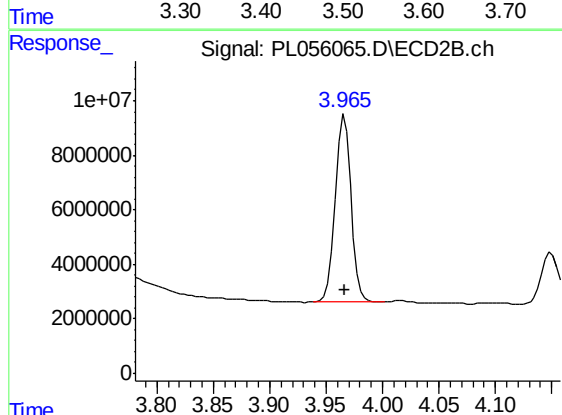


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 67804437
Conc: 23.99 ng/ml

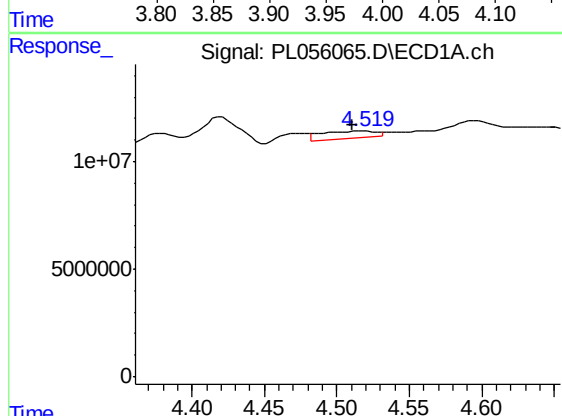


#4 Heptachlor

R.T.: 4.518 min
Delta R.T.: 0.008 min
Response: 8684170
Conc: 0.58 ng/ml

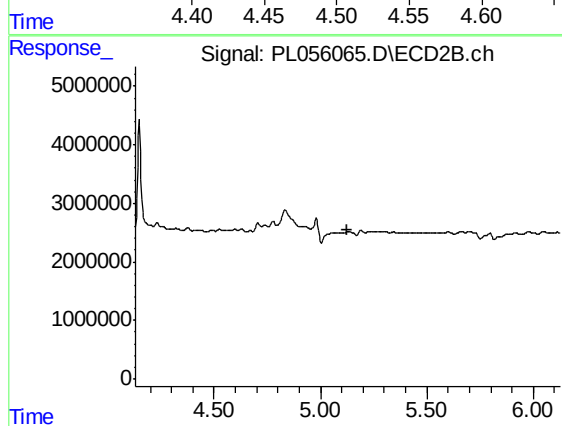

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.129 min
Response: 0
Conc: N.D.

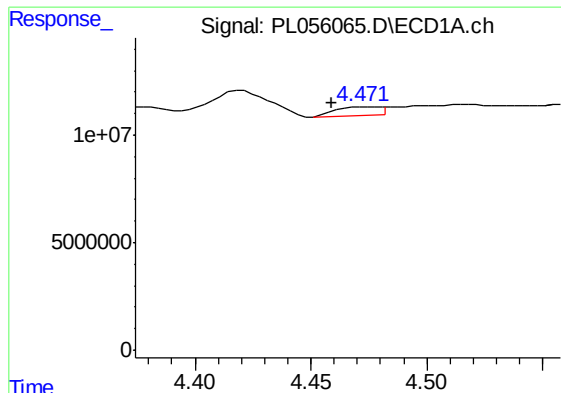

#6 beta-BHC


R.T.: 4.473 min
Delta R.T.: 0.014 min
Response: 5019541
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10-9-COMP

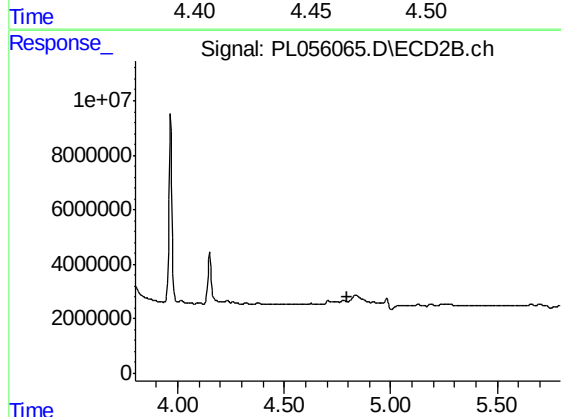


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.798 min
Response: 0
Conc: N.D.

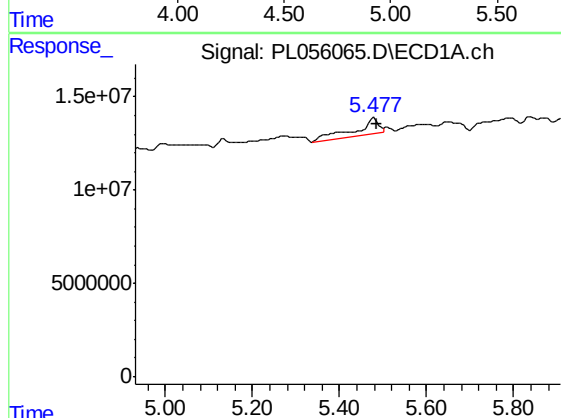


#11 alpha-Chlordane

R.T.: 5.478 min
Delta R.T.: -0.008 min
Response: 32777227
Conc: 2.37 ng/ml

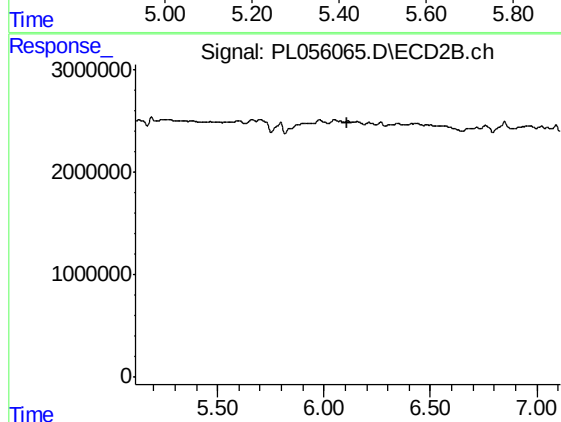

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

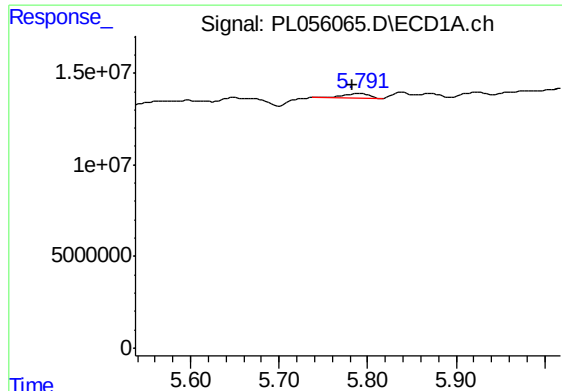

#13 Dieldrin


R.T.: 5.792 min
Delta R.T.: 0.009 min
Response: 5667297
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10-9-COMP

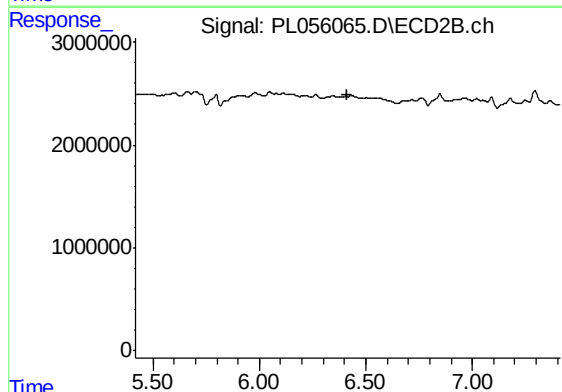


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

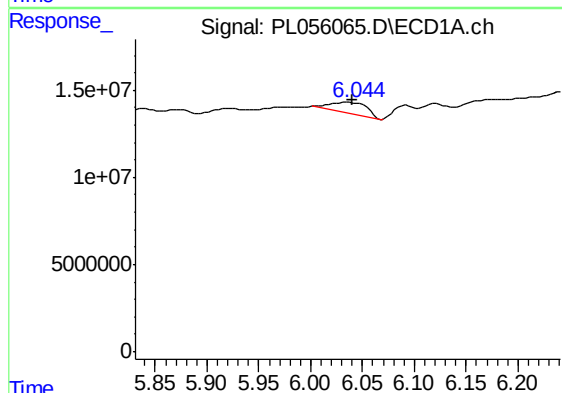


#14 Endrin

R.T.: 6.036 min
Delta R.T.: -0.004 min
Response: 15755167
Conc: 1.25 ng/ml

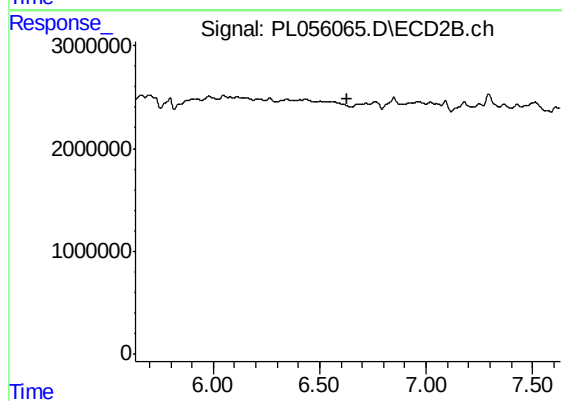

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

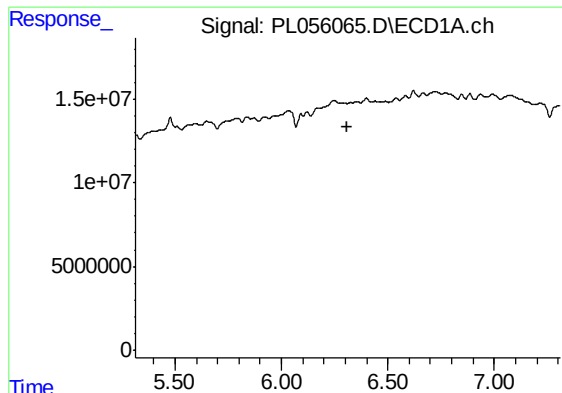

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.312 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-10-9-COMP

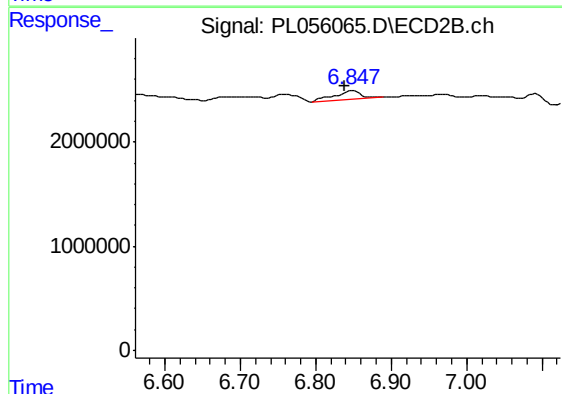


#15 Endosulfan II

R.T.: 6.849 min
Delta R.T.: 0.010 min
Response: 2017627
Conc: 0.75 ng/ml

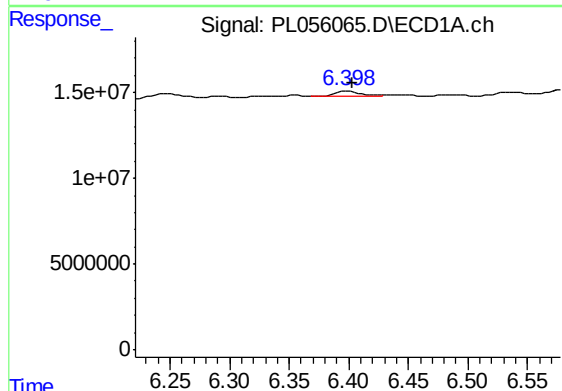


#17 4,4'-DDT

R.T.: 6.399 min
Delta R.T.: -0.004 min
Response: 4102372
Conc: 0.41 ng/ml

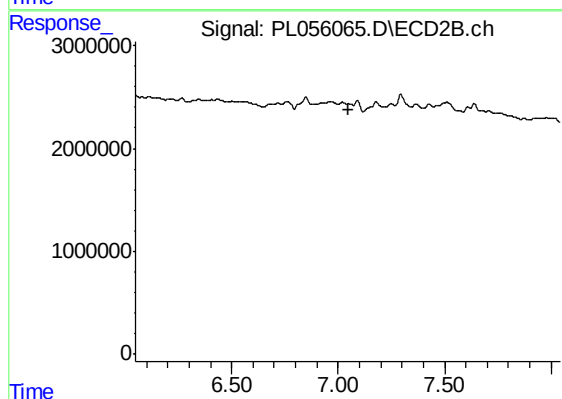

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.047 min
Response: 0
Conc: N.D.

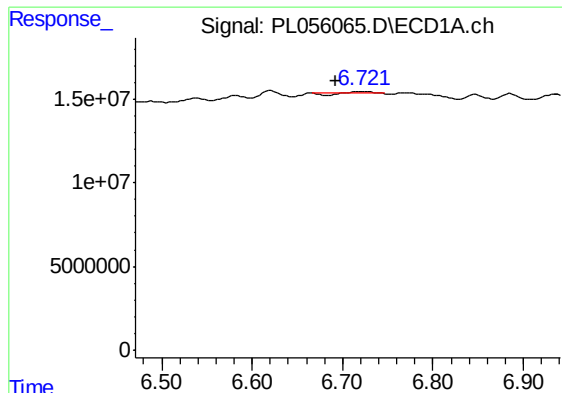

#19 Endosulfan Sulfate


R.T.: 6.721 min
Delta R.T.: 0.029 min
Response: 43254
Conc: 0.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10-9-COMP

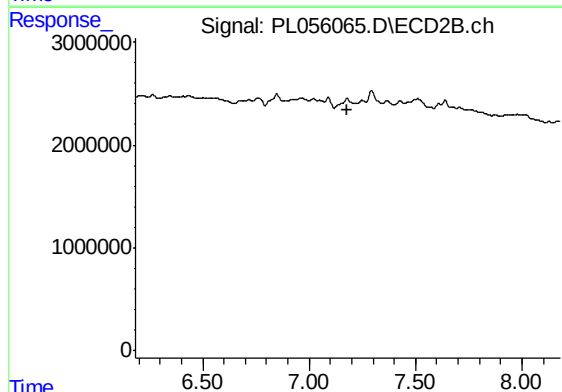


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

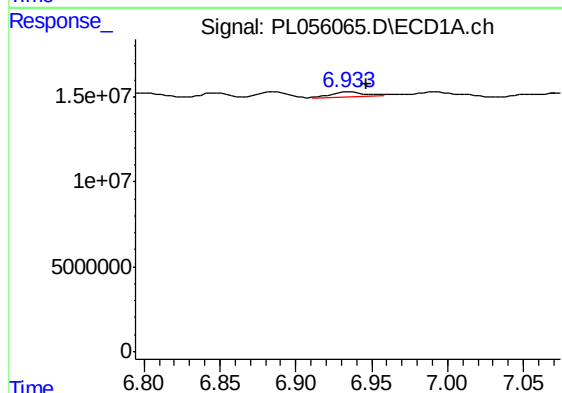


#20 Methoxychlor

R.T.: 6.935 min
Delta R.T.: -0.012 min
Response: 3521563
Conc: 0.67 ng/ml

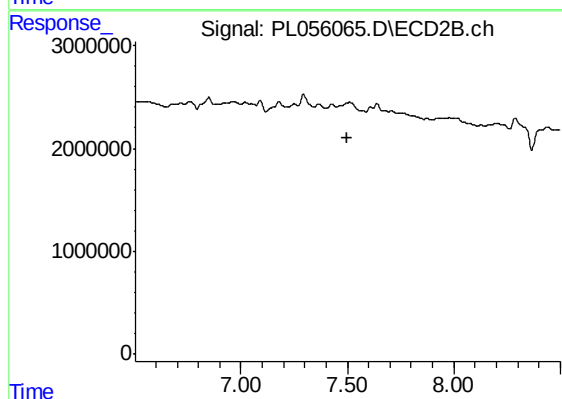

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.501 min
Response: 0
Conc: N.D.

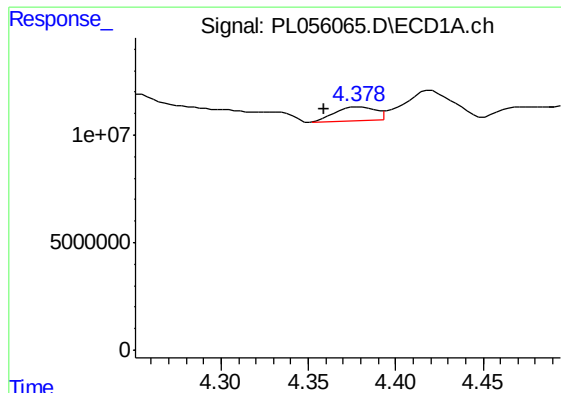

#23 Chlordane-1


R.T.: 4.379 min
Delta R.T.: 0.020 min
Response: 10495964
Conc: 28.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10-9-COMP

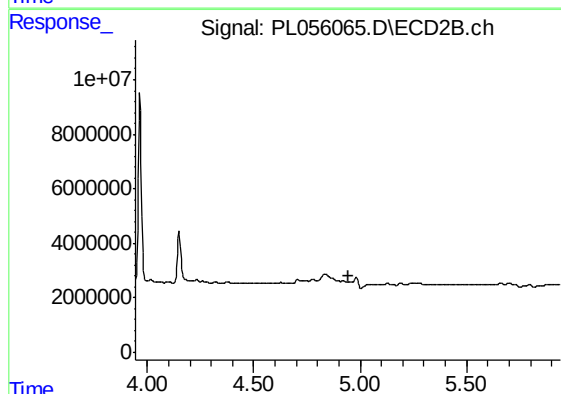


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.943 min
Response: 0
Conc: N.D.

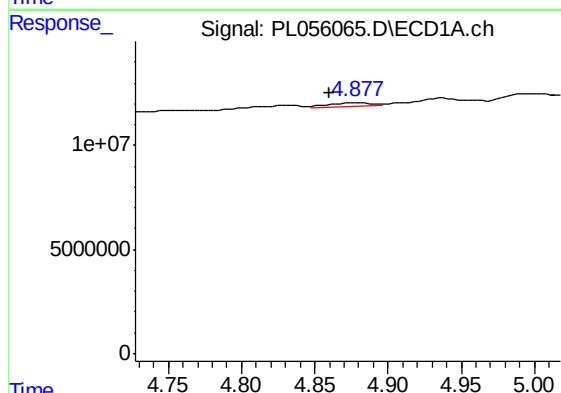


#24 Chlordane-2

R.T.: 4.879 min
Delta R.T.: 0.019 min
Response: 3252963
Conc: 7.52 ng/ml

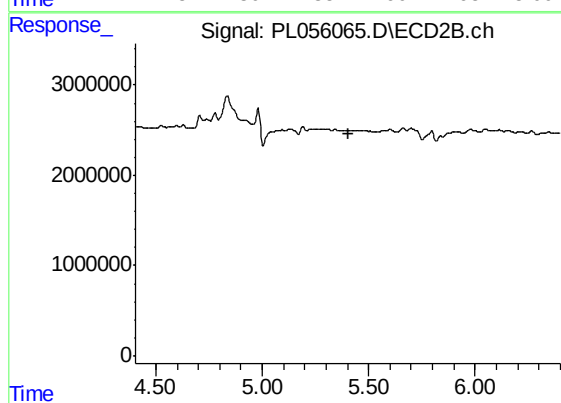

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.403 min
Response: 0
Conc: N.D.

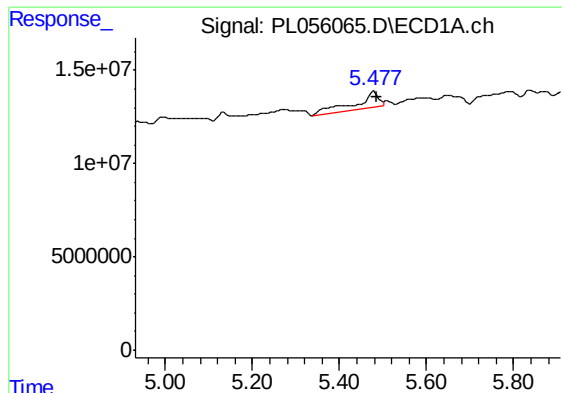

#26 Chlordane-4


R.T.: 5.478 min
Delta R.T.: -0.008 min
Response: 32777227
Conc: 31.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10-9-COMP

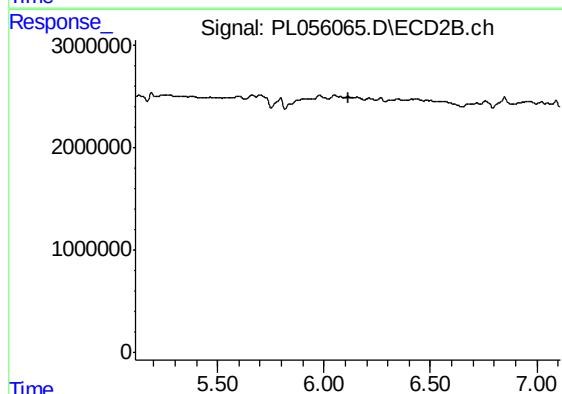


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

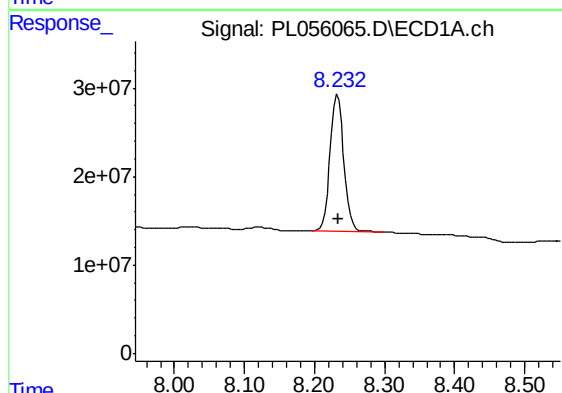

#28 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: 0.000 min
Response: 209364346
Conc: 20.02 ng/ml

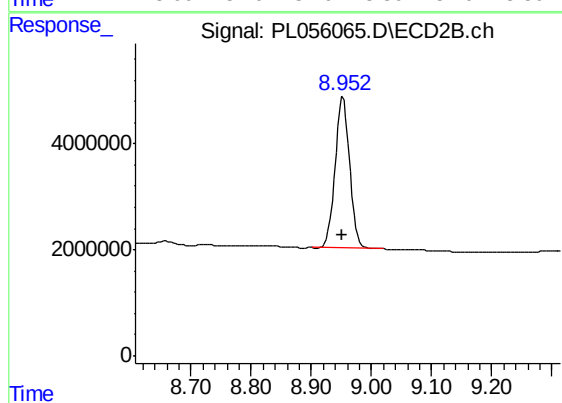

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: 0.000 min
Response: 48334285
Conc: 21.10 ng/ml