

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012420\
 Data File : PL056066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2020 00:24
 Operator : AJ\MA
 Sample : L1247-29
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-13-15-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 02:45:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.966	221.6E6	66633038	23.116	23.576
28)	SA Decachlor...	8.234	8.954	215.1E6	48599755	20.576	21.214
Target Compounds							
4)	MA Heptachlor	4.519	0.000	12388044	0	0.830	N.D. #
11)	B alpha-Chl...	5.479	0.000	14975698	0	1.083	N.D. #
13)	MA Dieldrin	5.795	0.000	5115079	0	0.370	N.D. #
15)	B Endosulfa...	6.333f	0.000	247449	0	0.022	N.D. #
19)	B Endosulfa...	6.721f	0.000	1764130	0	0.163	N.D. #
23)	Chlordane-1	4.381f	0.000	7580025	0	20.674	N.D. #
24)	Chlordane-2	4.886f	0.000	2507396	0	5.794	N.D. #
26)	Chlordane-4	5.479	0.000	14975698	0	14.523	N.D. #
27)	Chlordane-5	6.333	0.000	247449	0	0.633	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012420\
Data File : PL056066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2020 00:24
Operator : AJ\MA
Sample : L1247-29
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-13-15-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 02:45:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

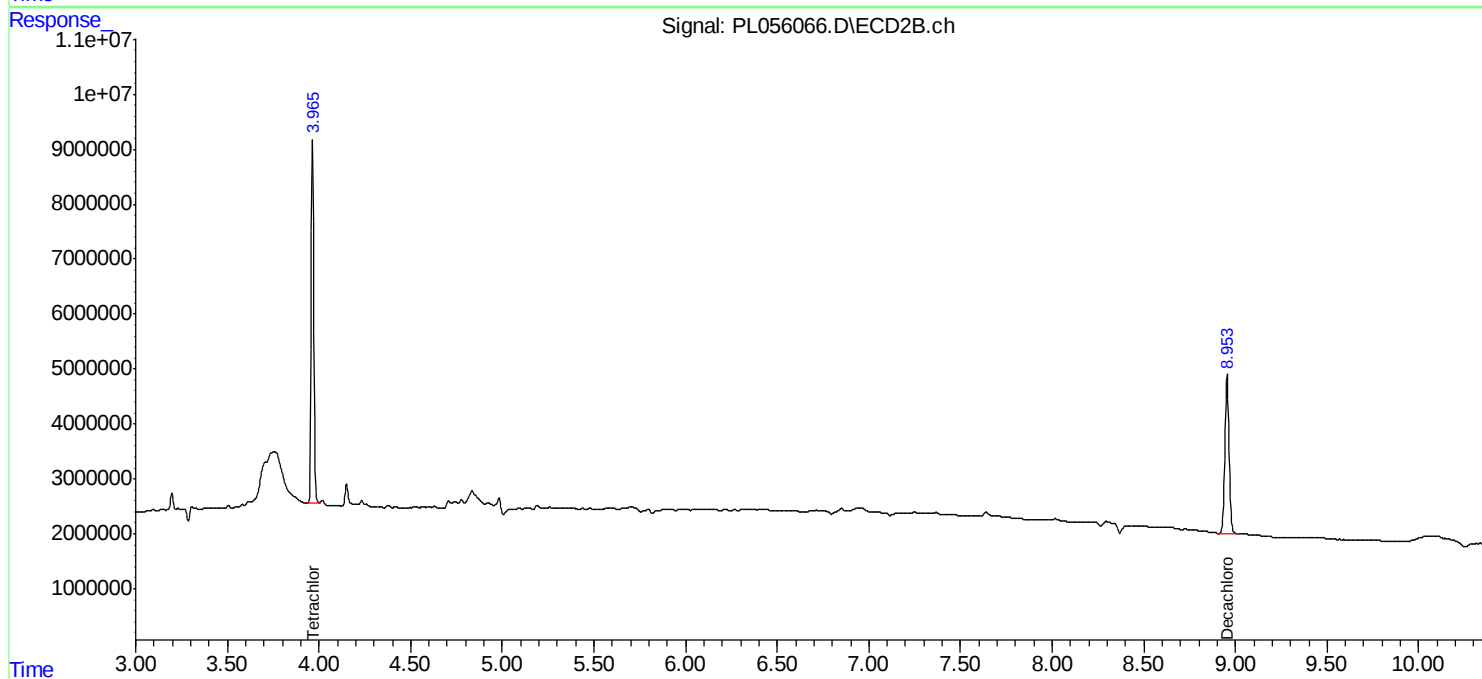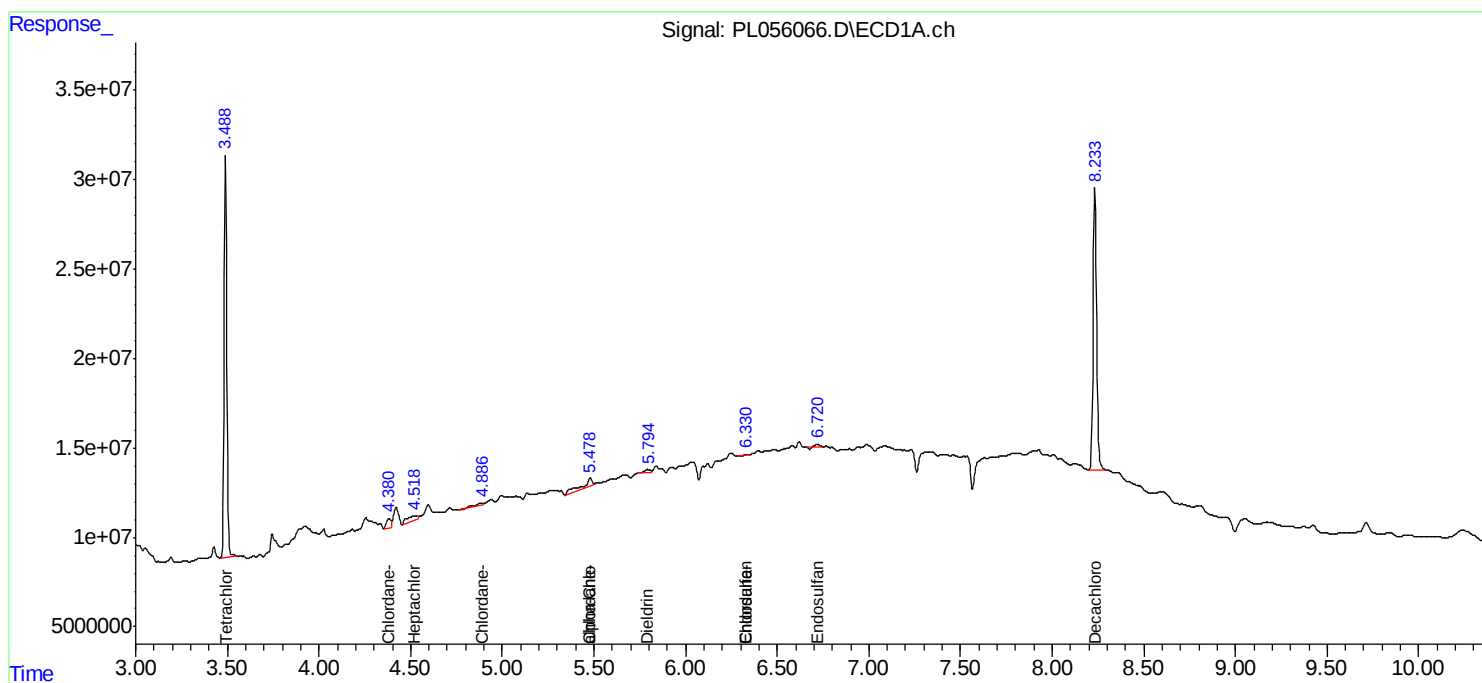


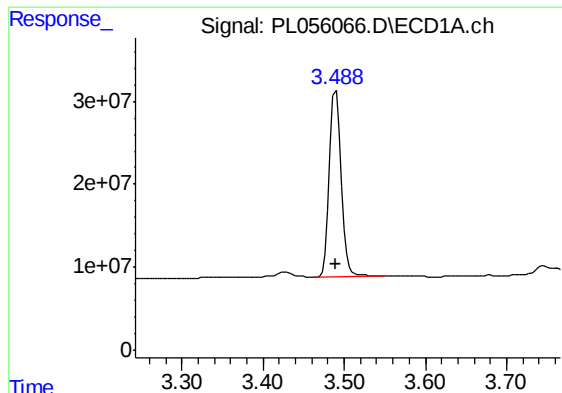

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 221552656
Conc: 23.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13-15-COMP

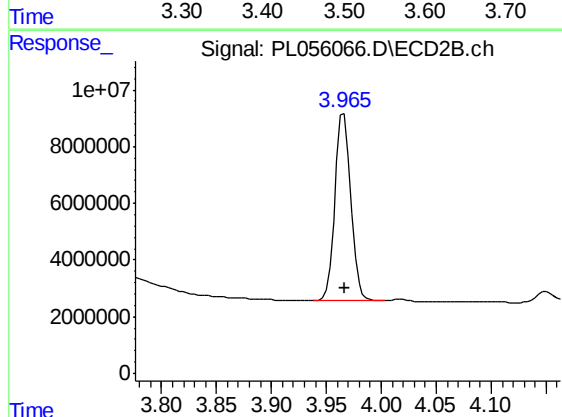


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 66633038
Conc: 23.58 ng/ml

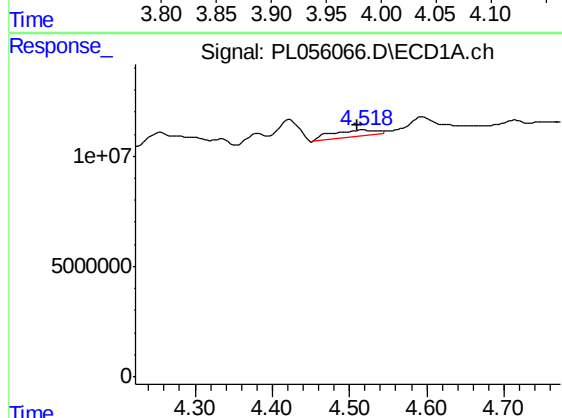


#4 Heptachlor

R.T.: 4.519 min
Delta R.T.: 0.008 min
Response: 12388044
Conc: 0.83 ng/ml

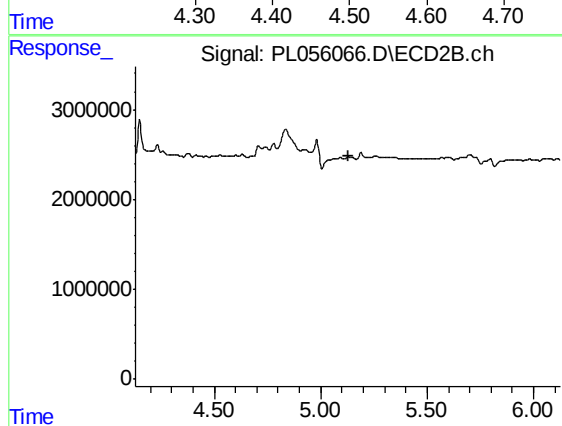

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.129 min
Response: 0
Conc: N.D.

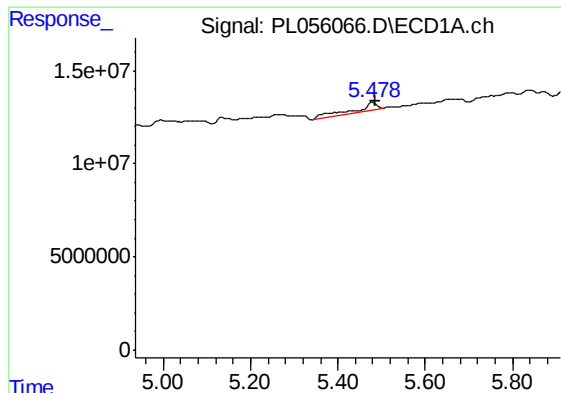

#11 alpha-Chlordane


R.T.: 5.479 min
Delta R.T.: -0.007 min
Response: 14975698
Conc: 1.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13-15-COMP

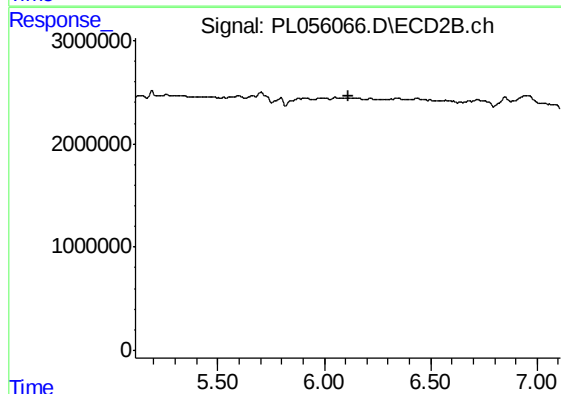


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

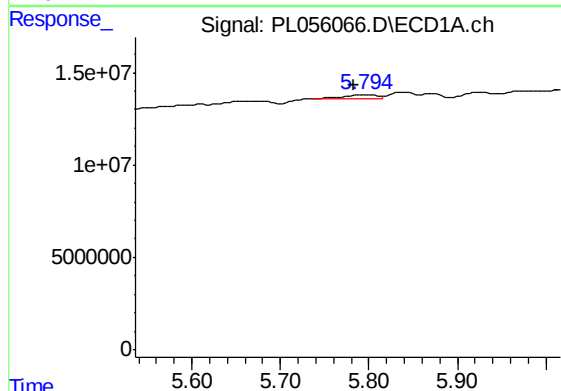


#13 Dieldrin

R.T.: 5.795 min
Delta R.T.: 0.012 min
Response: 5115079
Conc: 0.37 ng/ml

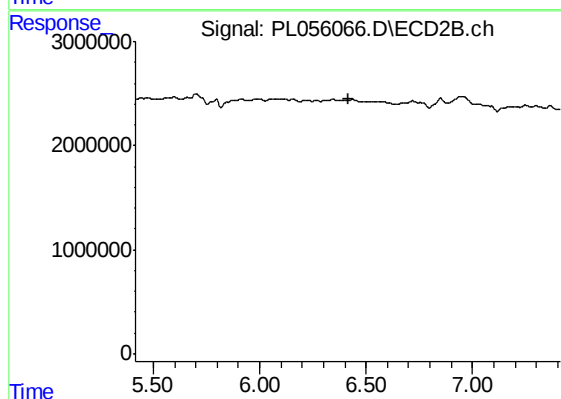

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

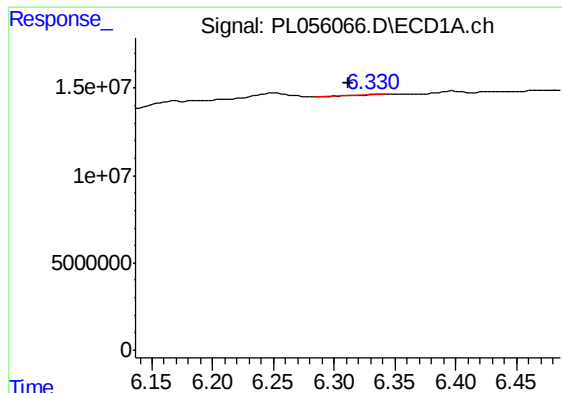

#15 Endosulfan II


R.T.: 6.333 min
Delta R.T.: 0.021 min
Response: 247449
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13-15-COMP

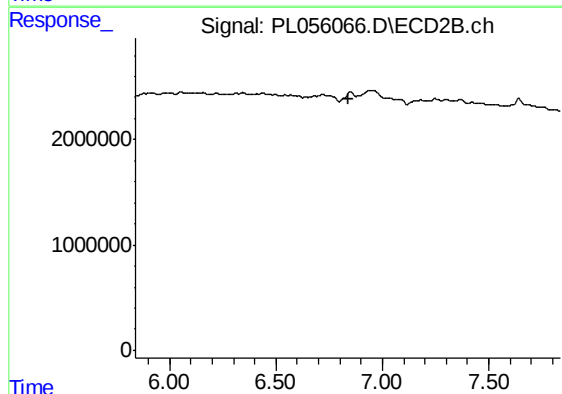


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.839 min
Response: 0
Conc: N.D.

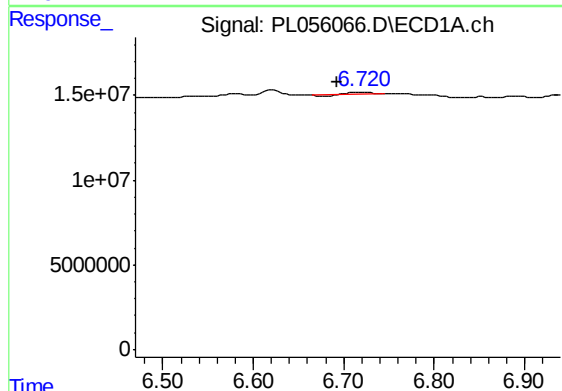


#19 Endosulfan Sulfate

R.T.: 6.721 min
Delta R.T.: 0.029 min
Response: 1764130
Conc: 0.16 ng/ml

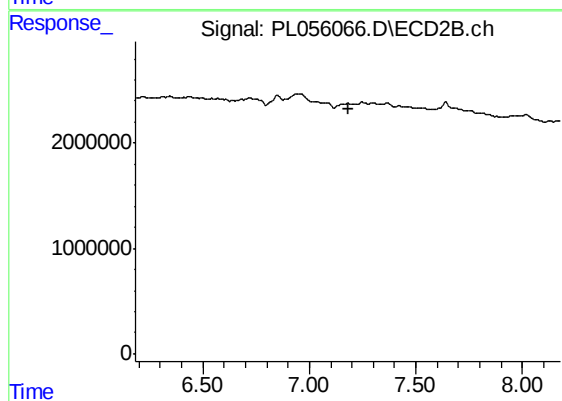

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

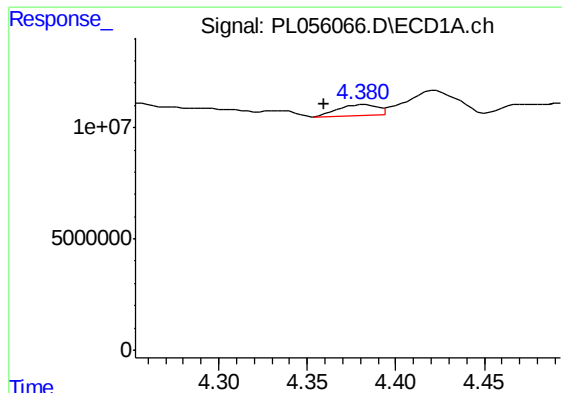

#23 Chlordane-1


R.T.: 4.381 min
Delta R.T.: 0.022 min
Response: 7580025
Conc: 20.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13-15-COMP

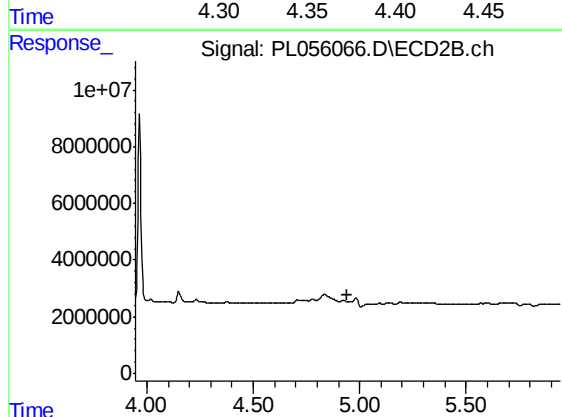


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.943 min
Response: 0
Conc: N.D.

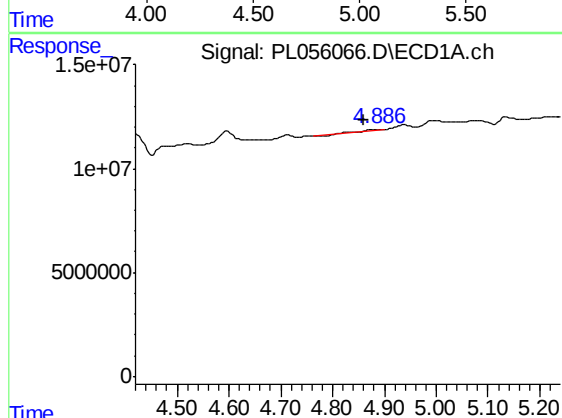


#24 Chlordane-2

R.T.: 4.886 min
Delta R.T.: 0.026 min
Response: 2507396
Conc: 5.79 ng/ml

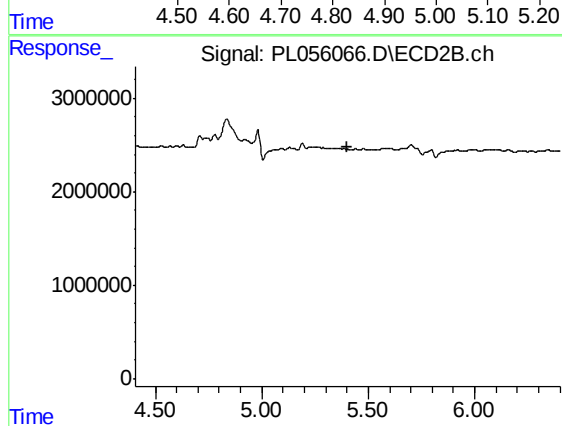

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.403 min
Response: 0
Conc: N.D.

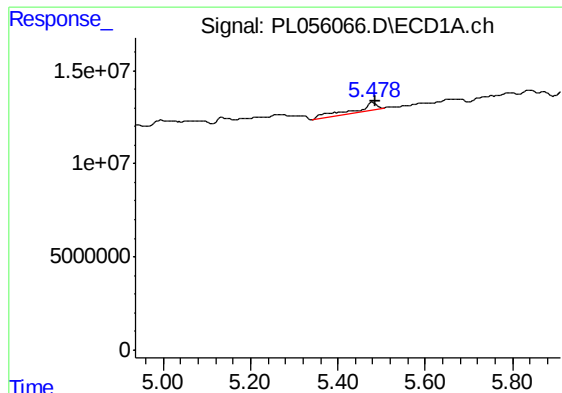

#26 Chlordane-4


R.T.: 5.479 min
Delta R.T.: -0.006 min
Response: 14975698
Conc: 14.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13-15-COMP

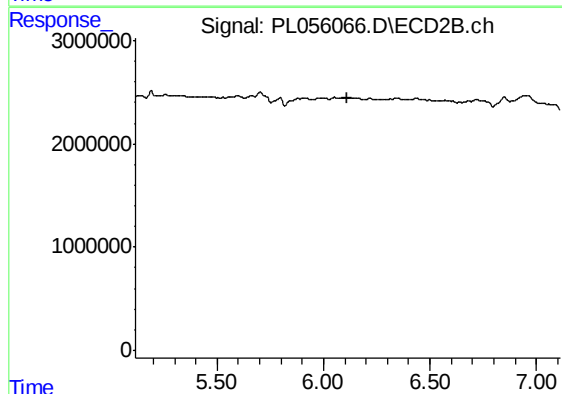


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

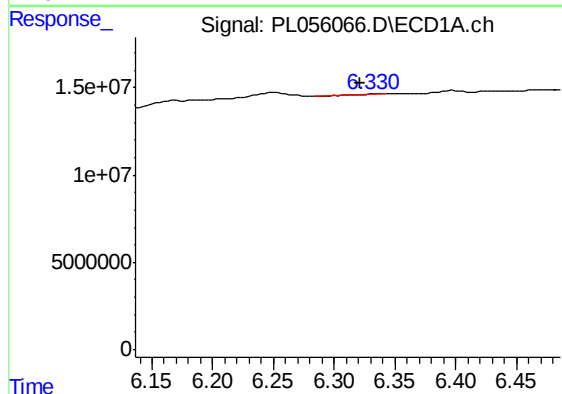


#27 Chlordane-5

R.T.: 6.333 min
Delta R.T.: 0.012 min
Response: 247449
Conc: 0.63 ng/ml

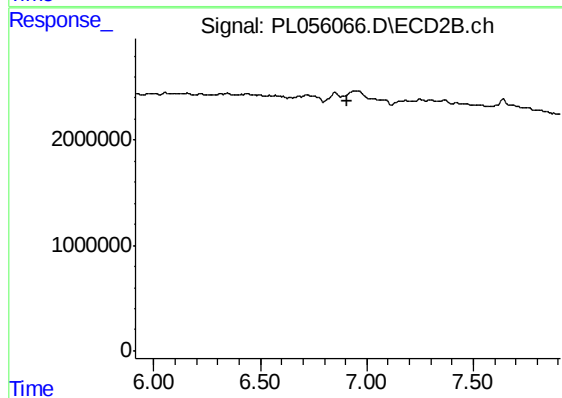

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.910 min
Response: 0
Conc: N.D.

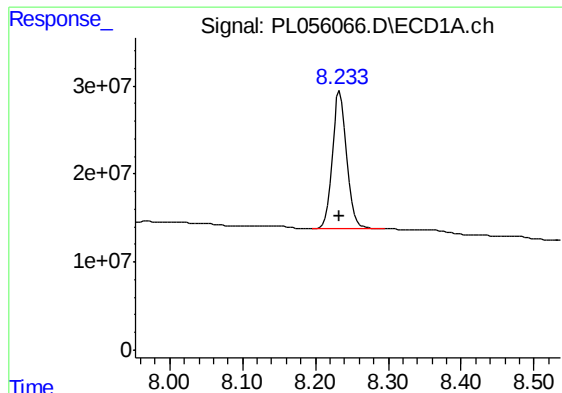

#28 Decachlorobiphenyl

R.T.: 8.234 min
Delta R.T.: 0.000 min
Response: 215131657
Conc: 20.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13-15-COMP

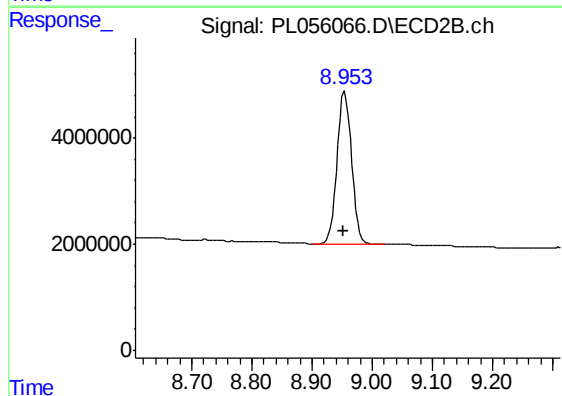

#28 Decachlorobiphenyl

R.T.: 8.954 min
Delta R.T.: 0.002 min
Response: 48599755
Conc: 21.21 ng/ml