

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012420\
 Data File : PL056031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2020 14:35
 Operator : AJ\MA
 Sample : L1234-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NS-TP

Manual Integrations
 APPROVED

mohammad
 1/27/2020 2:09:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 22:17:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	3.966	136.1E6	36499563	14.200m	12.914
28)	SA Decachlor...	8.232	8.953	110.4E6	27574175	10.555	12.036

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012420\
Data File : PL056031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2020 14:35
Operator : AJ\MA
Sample : L1234-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NS-TP


Manual Integrations
APPROVED

mohammad
1/27/2020 2:09:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 22:17:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

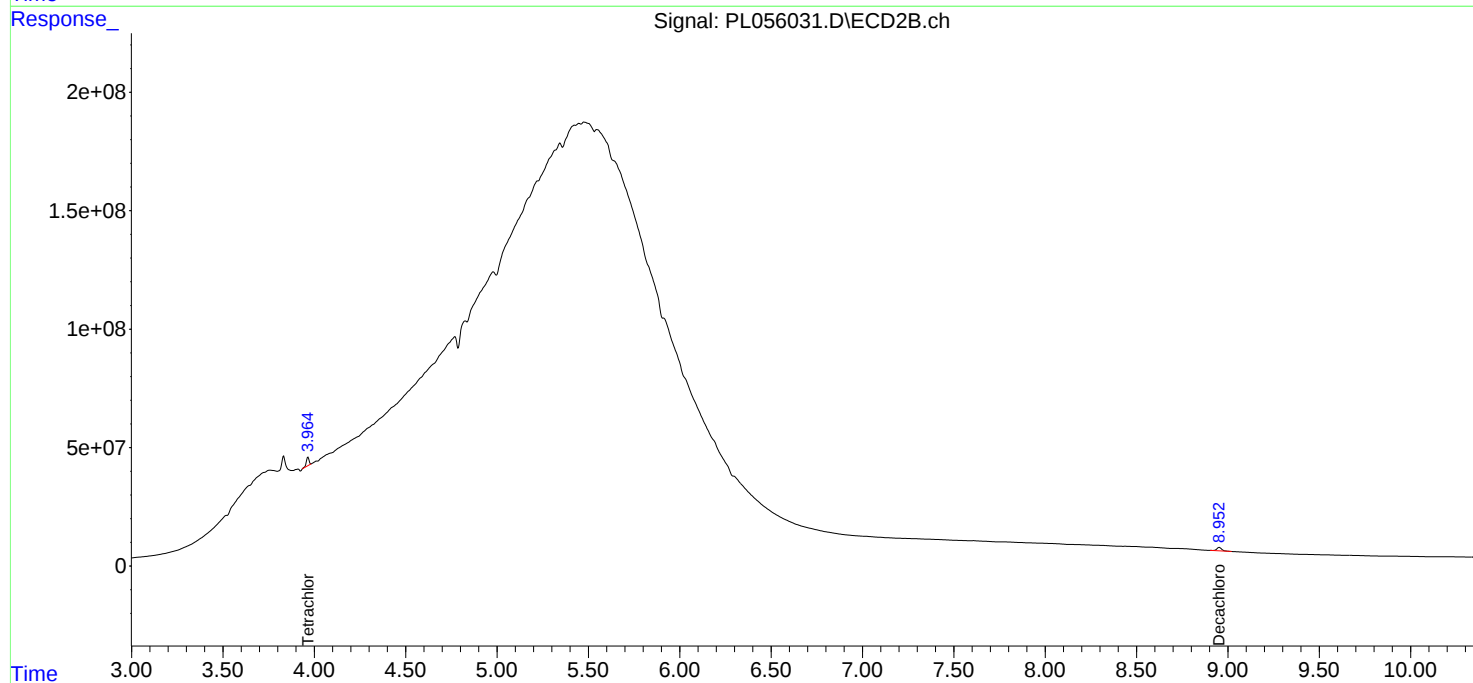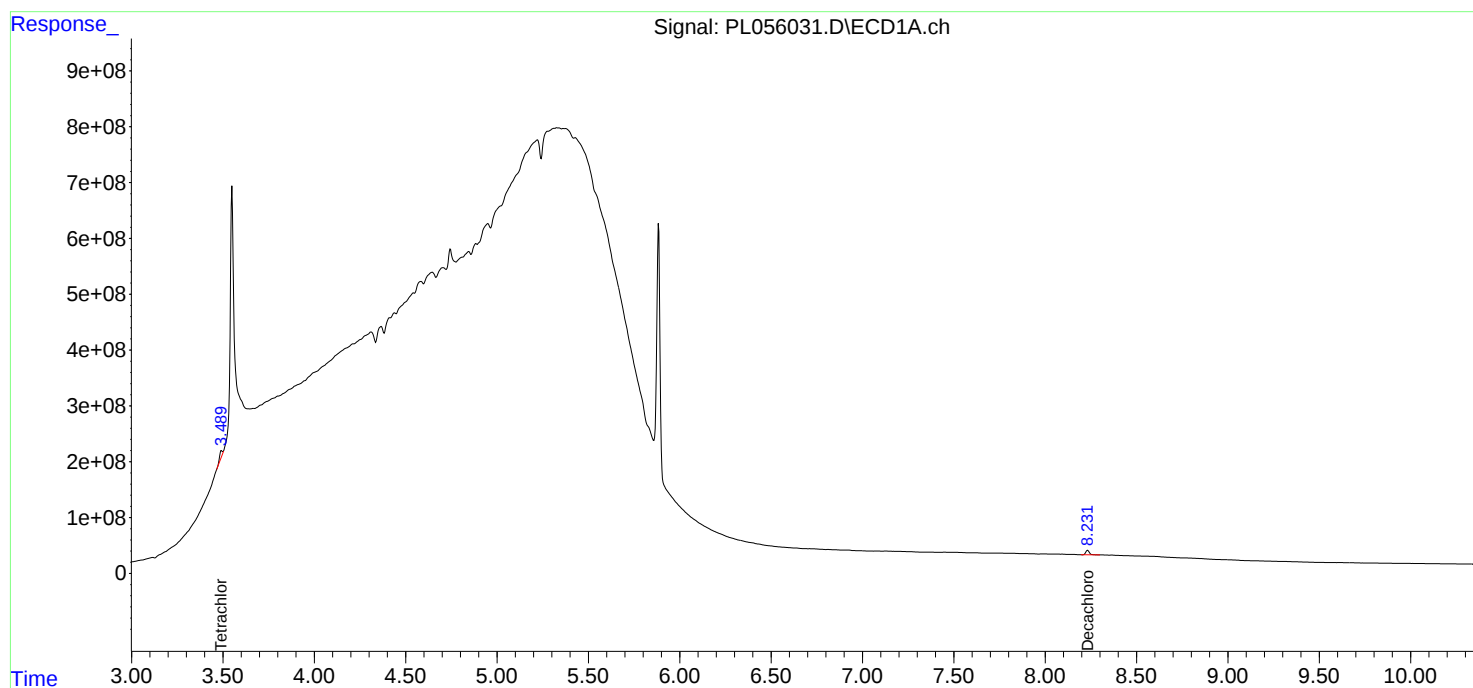

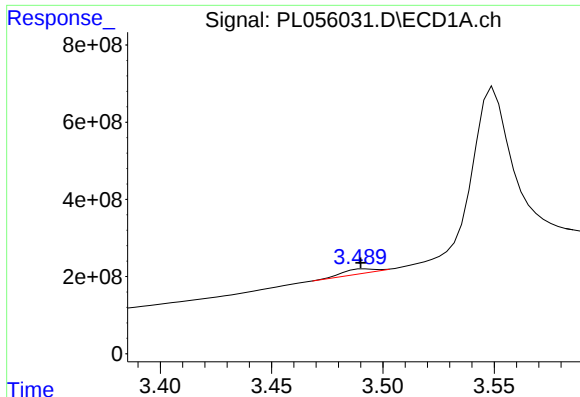


#1 Tetrachloro-m-xylene

R.T.: 3.489 min
Delta R.T.: -0.001 min
Response: 136098753
Conc: 14.20 ng/ml m

Instrument :
ECD_L
ClientSampleId :
NS-TP


Manual Integrations
APPROVED

mohammad
1/27/2020 2:09:08 PM

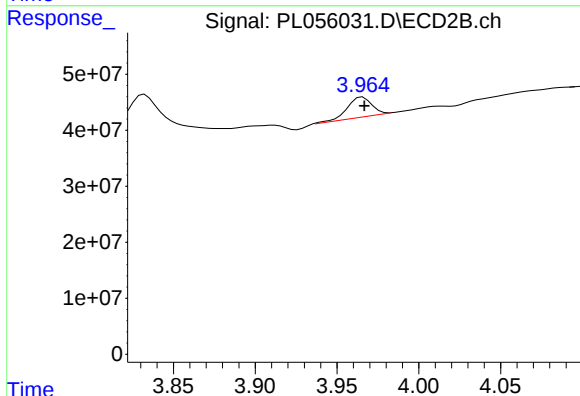


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: -0.001 min
Response: 36499563
Conc: 12.91 ng/ml

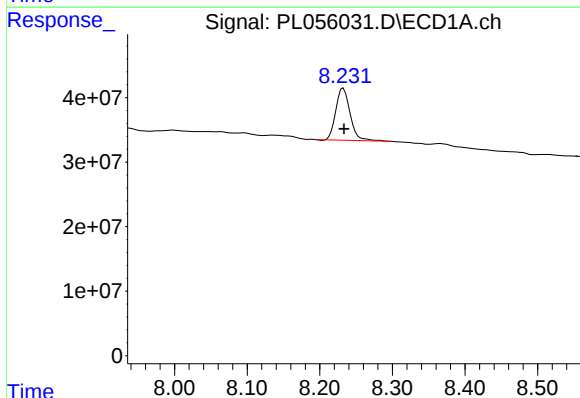

#28 Decachlorobiphenyl

R.T.: 8.232 min
Delta R.T.: 0.000 min
Response: 110354812
Conc: 10.55 ng/ml

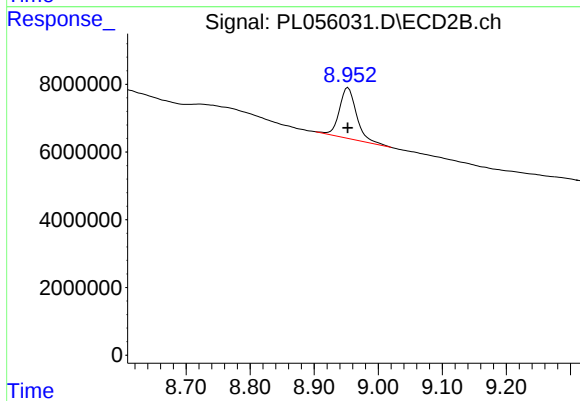

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: 0.000 min
Response: 27574175
Conc: 12.04 ng/ml