

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012421\
 Data File : PL064349.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2021 15:09
 Operator : AR\AJ
 Sample : M1209-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 16:24:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.108	33755334	27950538	11.257	10.933
28)	SA Decachlor...	8.167	9.272	28445270	21756753	9.320	9.167
Target Compounds							
4)	MA Heptachlor	0.000	5.305	0	4994478	N.D.	1.391 #
10)	B gamma-Chl...	5.384f	0.000	2078973	0	0.537	N.D. #
11)	B alpha-Chl...	0.000	6.328	0	2454701	N.D.	0.806 #
16)	A 4,4'-DDD	0.000	6.949f	0	8284635	N.D.	3.738 #
25)	Chlordane-3	5.384f	0.000	2078973	0	5.203	N.D. #
26)	Chlordane-4	0.000	6.328	0	2454701	N.D.	4.966 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012421\
Data File : PL064349.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2021 15:09
Operator : AR\AJ
Sample : M1209-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 16:24:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

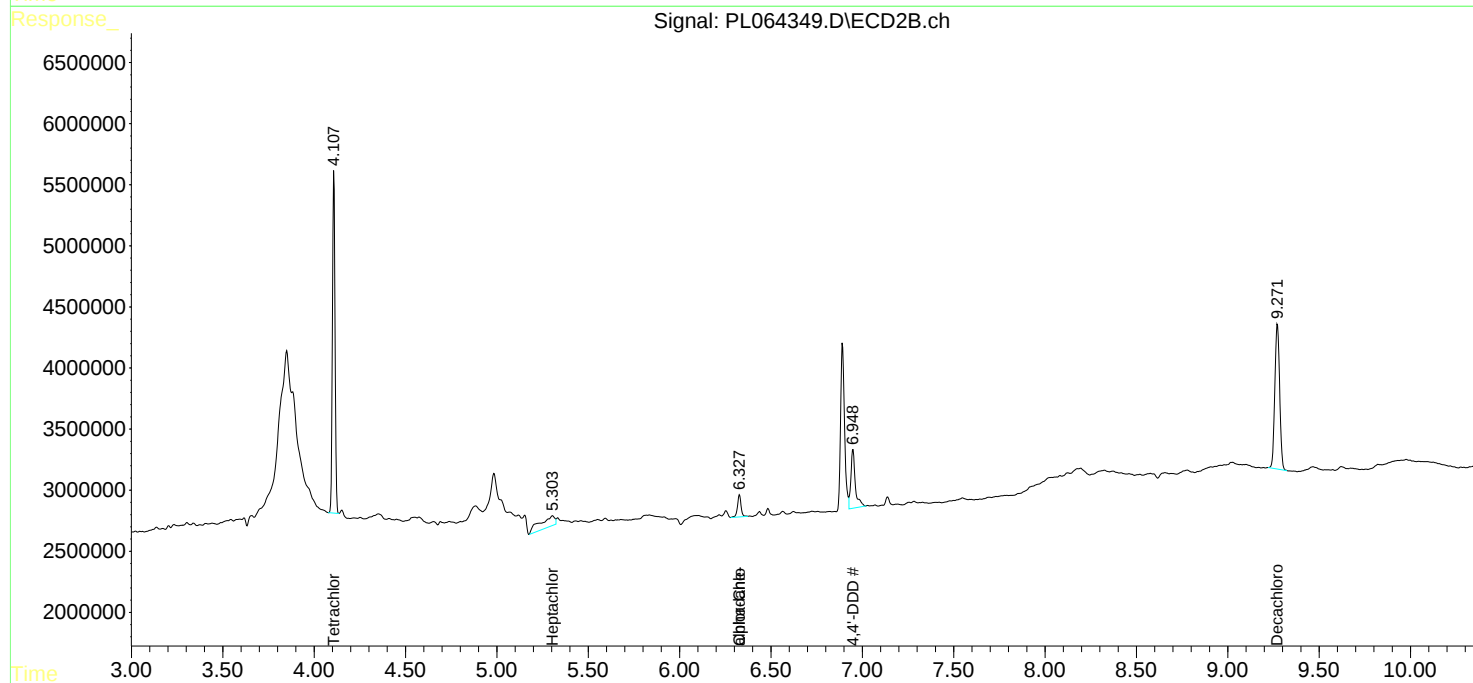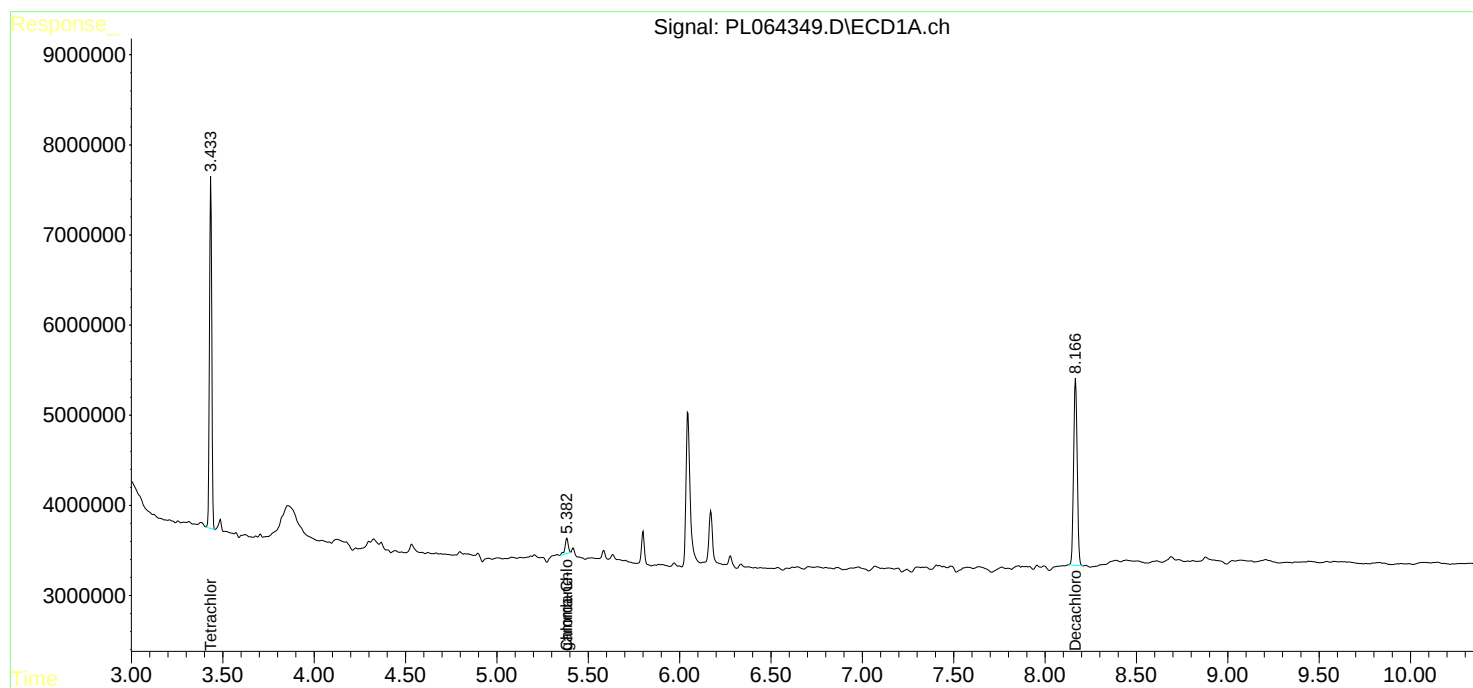


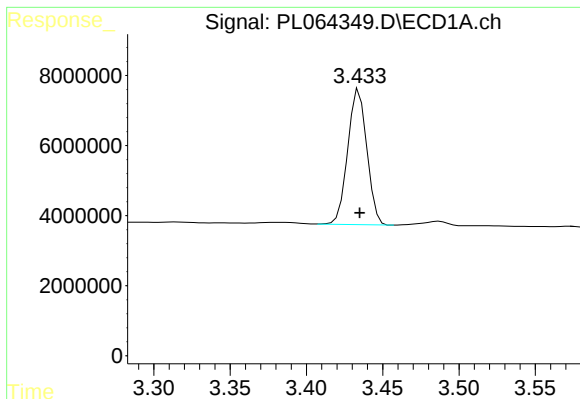

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 33755334
Conc: 11.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

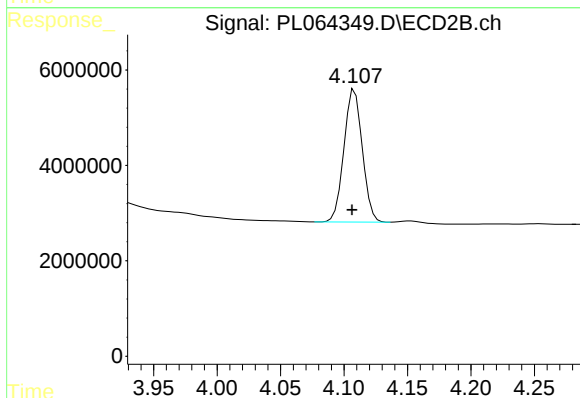


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.002 min
Response: 27950538
Conc: 10.93 ng/ml

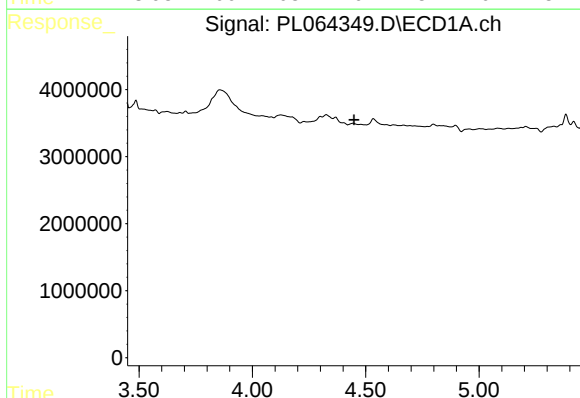


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

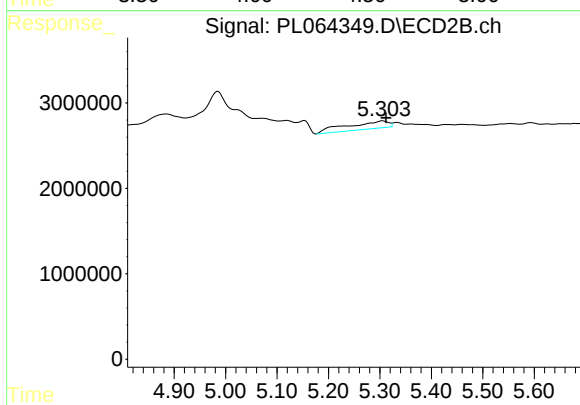

#4 Heptachlor


R.T.: 5.305 min
Delta R.T.: -0.007 min
Response: 4994478
Conc: 1.39 ng/ml

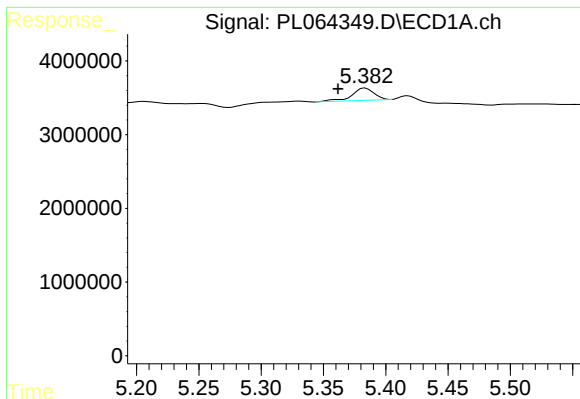

#10 gamma-Chlordane


R.T.: 5.384 min
Delta R.T.: 0.022 min
Response: 2078973
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

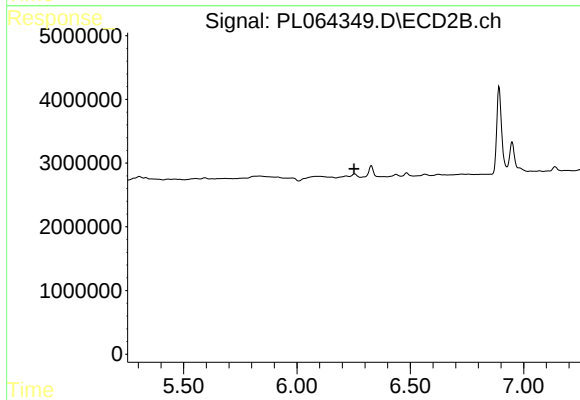


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.252 min
Response: 0
Conc: N.D.

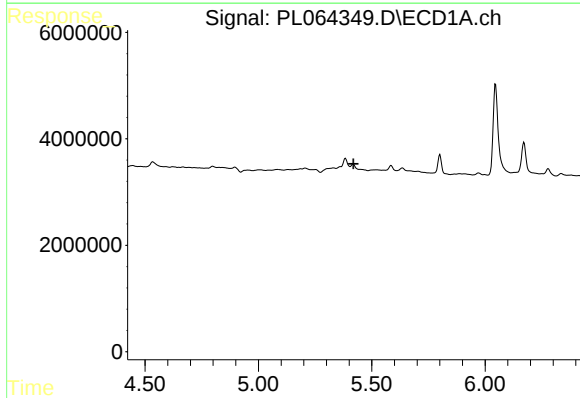


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.420 min
Response: 0
Conc: N.D.

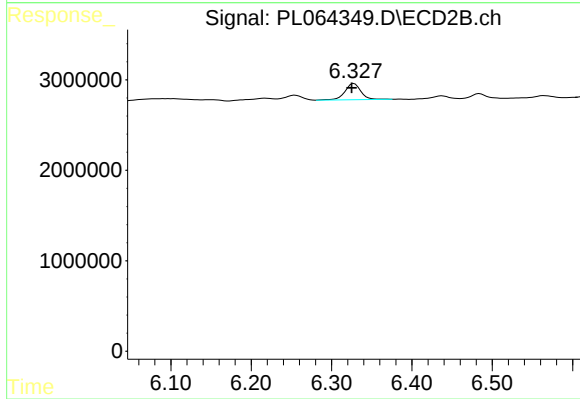

#11 alpha-Chlordane


R.T.: 6.328 min
Delta R.T.: 0.003 min
Response: 2454701
Conc: 0.81 ng/ml

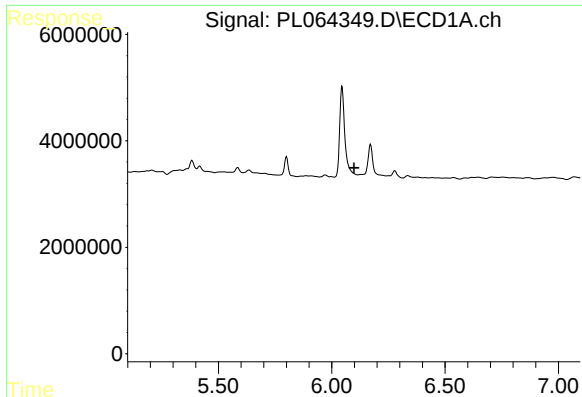

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

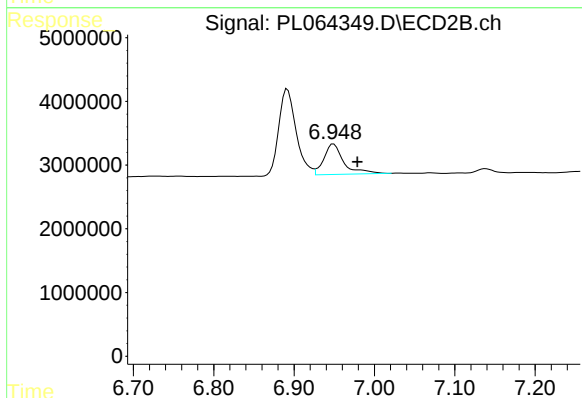


#16 4,4'-DDD

R.T.: 6.949 min
Delta R.T.: -0.030 min
Response: 8284635
Conc: 3.74 ng/ml

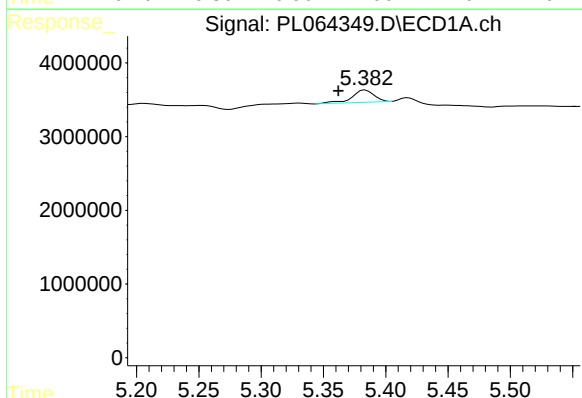


#25 Chlordane-3

R.T.: 5.384 min
Delta R.T.: 0.022 min
Response: 2078973
Conc: 5.20 ng/ml

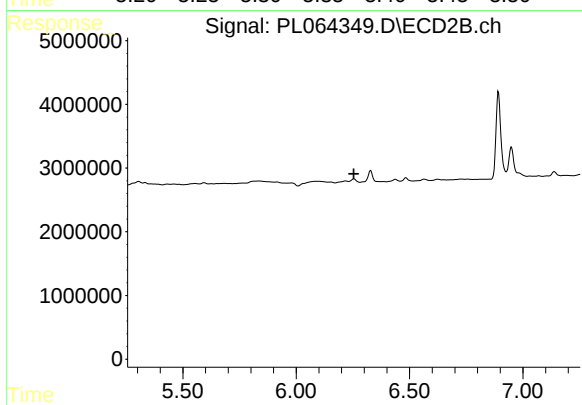

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.255 min
Response: 0
Conc: N.D.

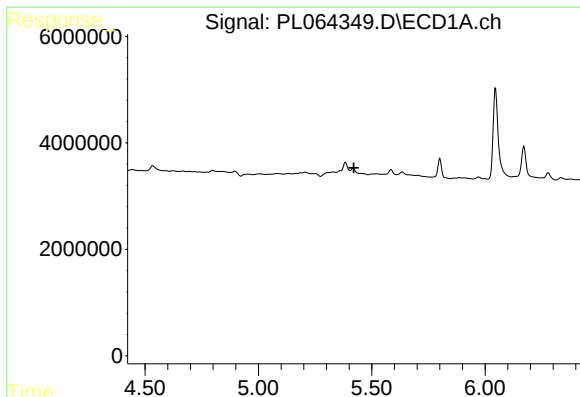

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

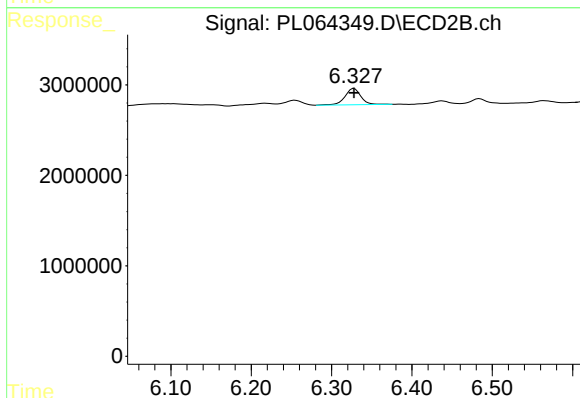


#26 Chlordane-4

R.T.: 6.328 min
Delta R.T.: 0.000 min
Response: 2454701
Conc: 4.97 ng/ml

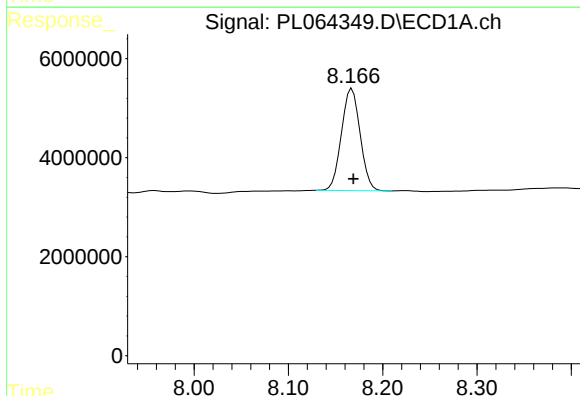

#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: -0.001 min
Response: 28445270
Conc: 9.32 ng/ml

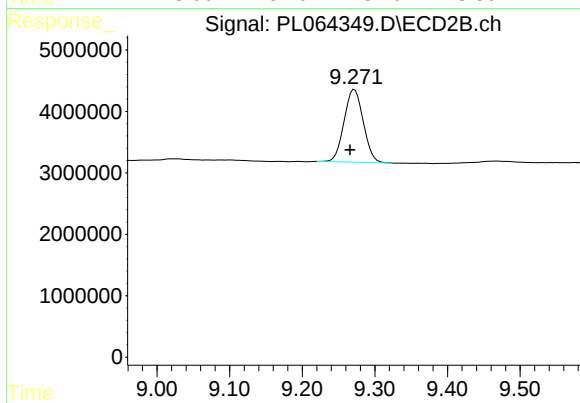

#28 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: 0.006 min
Response: 21756753
Conc: 9.17 ng/ml