

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012421\
 Data File : PL064355.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2021 17:13
 Operator : AR\AJ
 Sample : PB134288BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 02:55:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.109	59902171	49563136	19.977	19.387
28)	SA Decachlor...	8.168	9.274	53104086	38590819	17.399	16.260
Target Compounds							
4)	MA Heptachlor	4.450	5.302	1574571	5883202	0.359	1.638 #
10)	B gamma-Chl...	0.000	6.259	0	508229	N.D.	0.169 #
15)	B Endosulfa...	0.000	7.082	0	5255803	N.D.	2.081 #
16)	A 4,4'-DDD	0.000	6.950f	0	6890326	N.D.	3.109 #
20)	A Methoxychlor	0.000	7.720f	0	15889844	N.D.	11.760 #
22)	Mirex	0.000	8.342	0	4648308	N.D.	2.291 #
23)	Chlordane-1	4.326f	0.000	14356198	0	123.275	N.D. #
25)	Chlordane-3	0.000	6.259	0	508229	N.D.	1.257 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012421\
Data File : PL064355.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2021 17:13
Operator : AR\AJ
Sample : PB134288BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 02:55:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

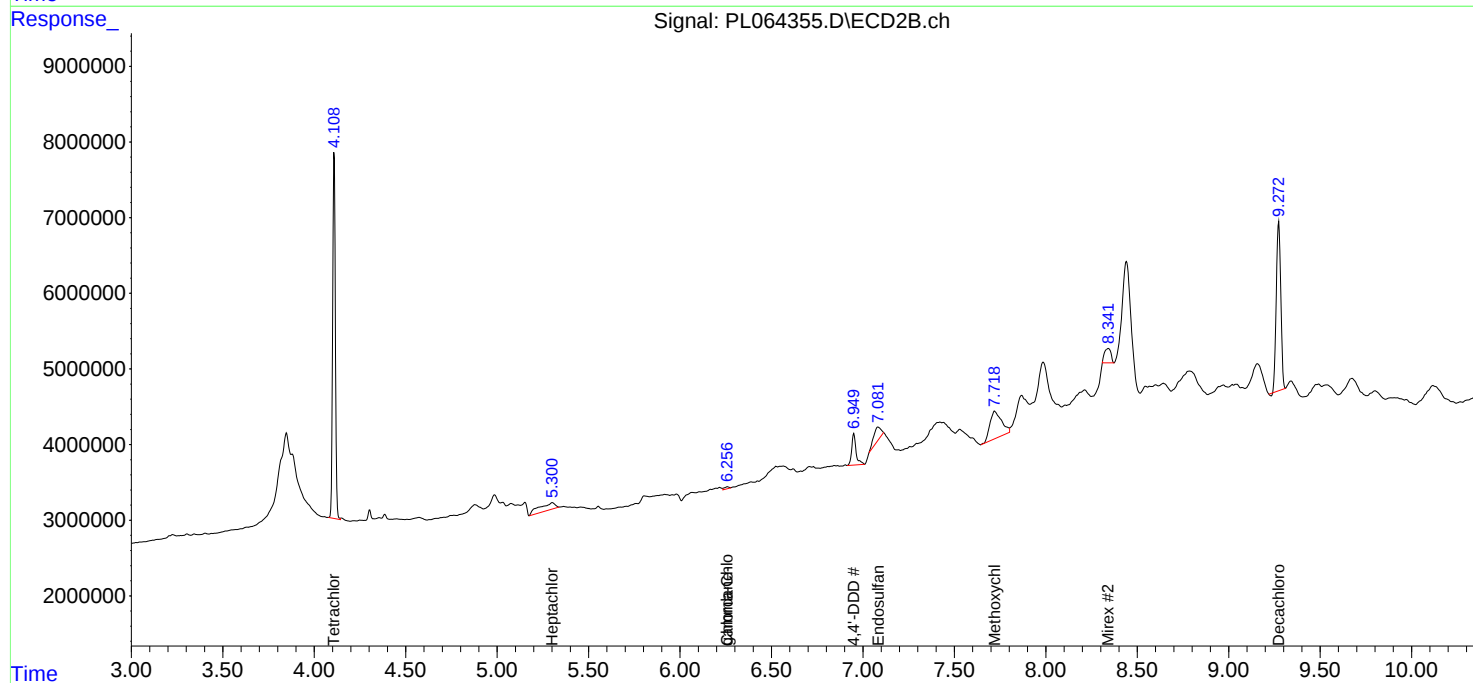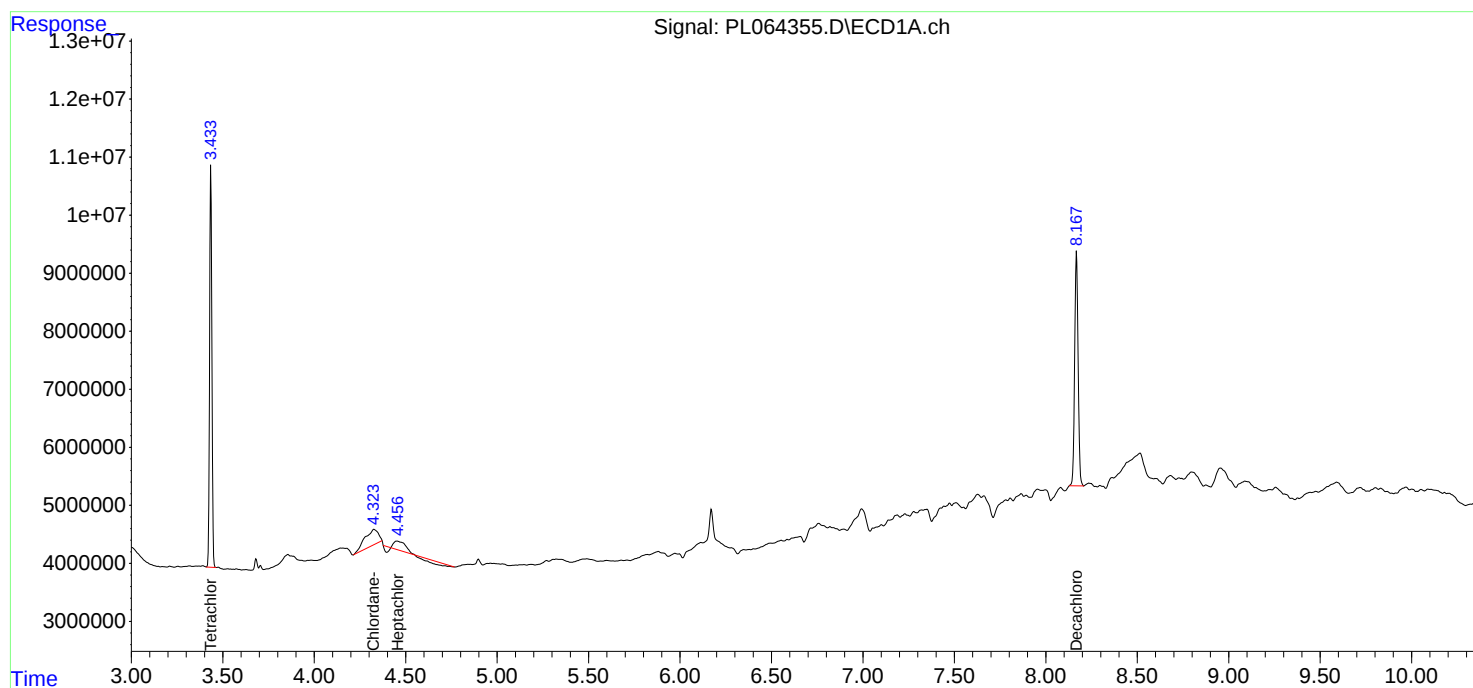


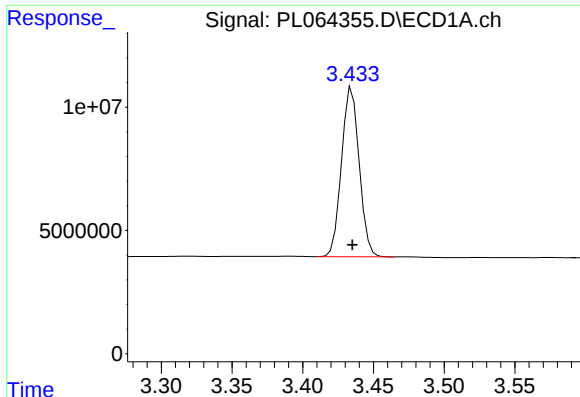

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 59902171
Conc: 19.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

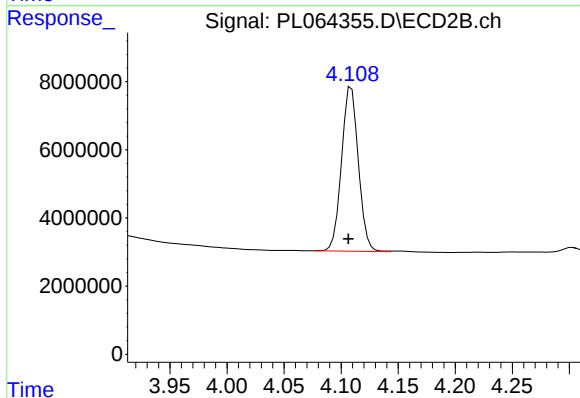


#1 Tetrachloro-m-xylene

R.T.: 4.109 min
Delta R.T.: 0.003 min
Response: 49563136
Conc: 19.39 ng/ml

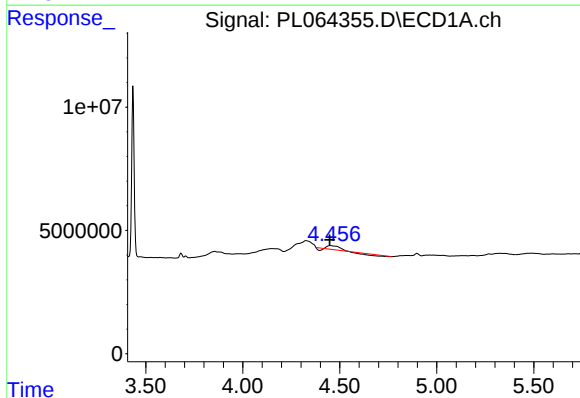


#4 Heptachlor

R.T.: 4.450 min
Delta R.T.: 0.001 min
Response: 1574571
Conc: 0.36 ng/ml

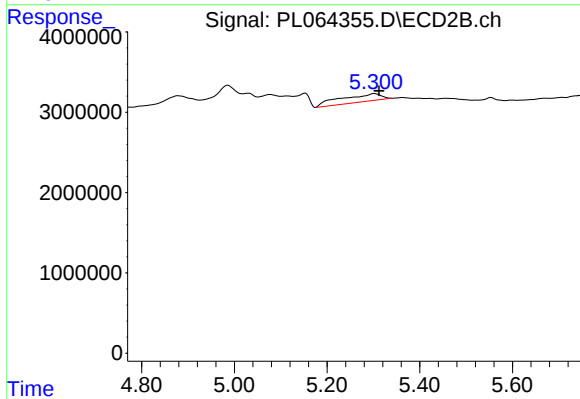

#4 Heptachlor


R.T.: 5.302 min
Delta R.T.: -0.010 min
Response: 5883202
Conc: 1.64 ng/ml

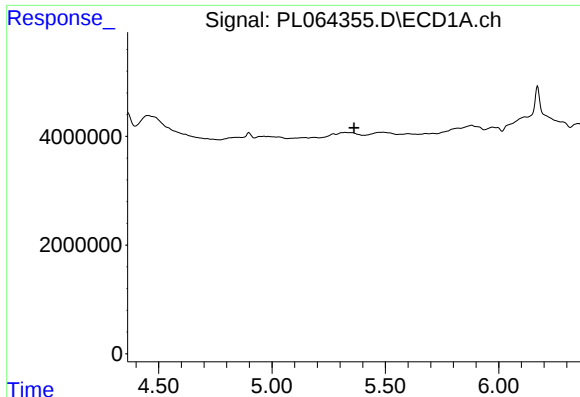

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

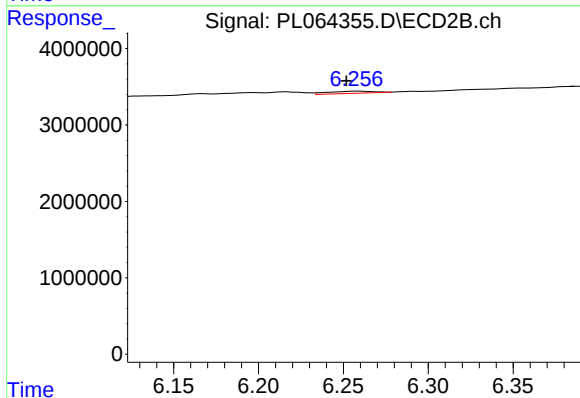


#10 gamma-Chlordane

R.T.: 6.259 min
Delta R.T.: 0.007 min
Response: 508229
Conc: 0.17 ng/ml

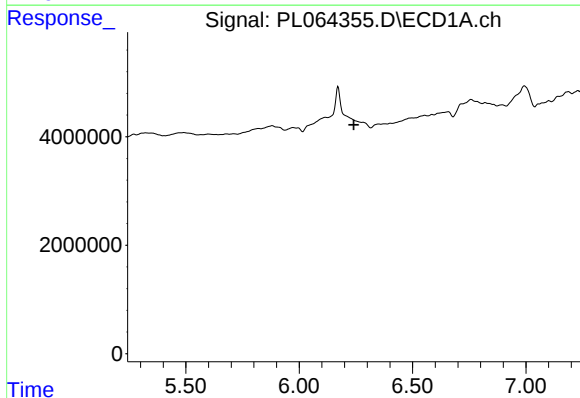


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

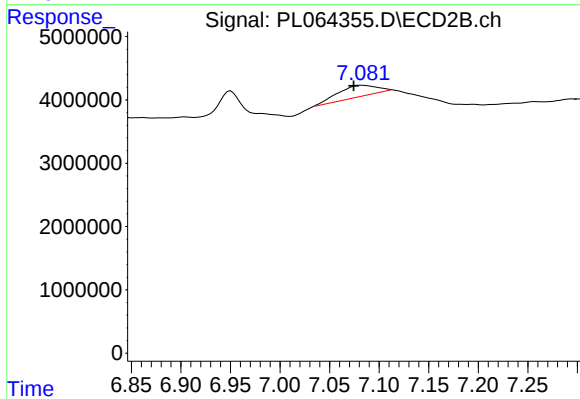

#15 Endosulfan II


R.T.: 7.082 min
Delta R.T.: 0.008 min
Response: 5255803
Conc: 2.08 ng/ml

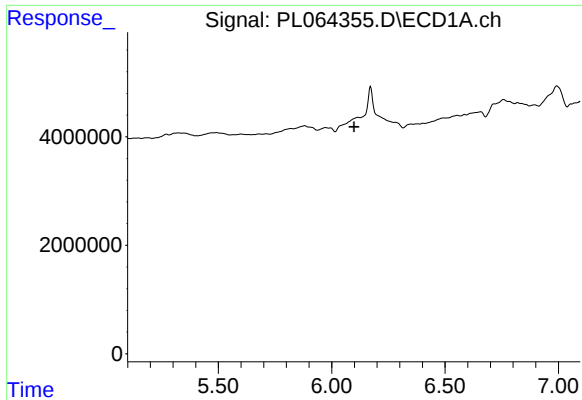

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

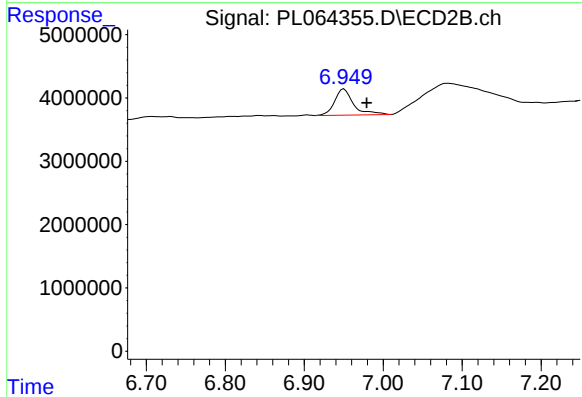


#16 4,4'-DDD

R.T.: 6.950 min
Delta R.T.: -0.029 min
Response: 6890326
Conc: 3.11 ng/ml

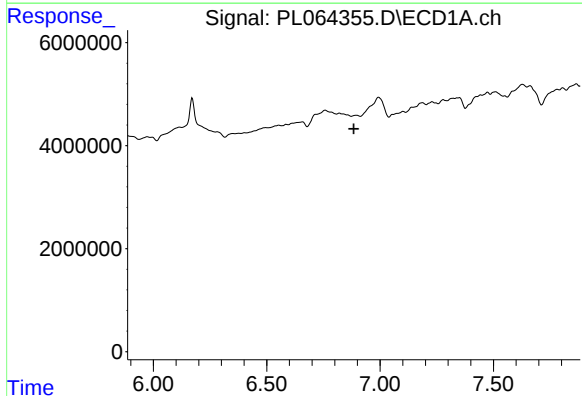


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.885 min
Response: 0
Conc: N.D.

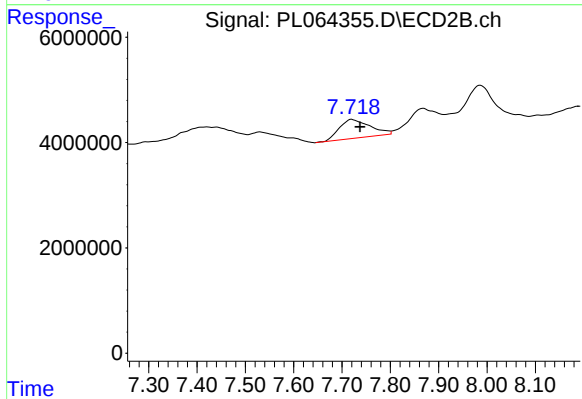

#20 Methoxychlor

R.T.: 7.720 min
Delta R.T.: -0.017 min
Response: 15889844
Conc: 11.76 ng/ml

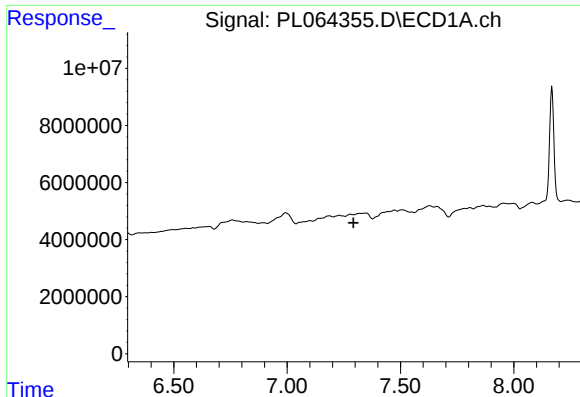

#22 Mirex


R.T.: 0.000 min

Exp R.T.: 7.293 min

Response: 0

Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

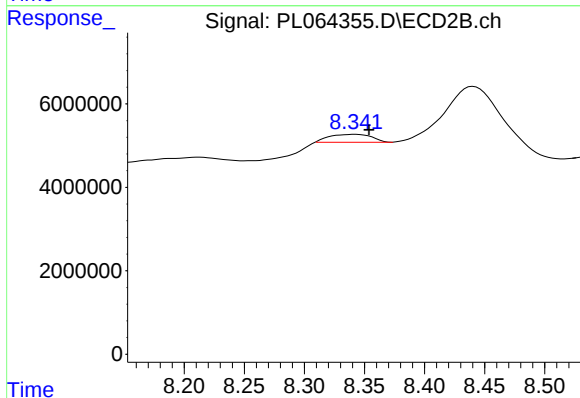


#22 Mirex

R.T.: 8.342 min

Delta R.T.: -0.012 min

Response: 4648308

Conc: 2.29 ng/ml

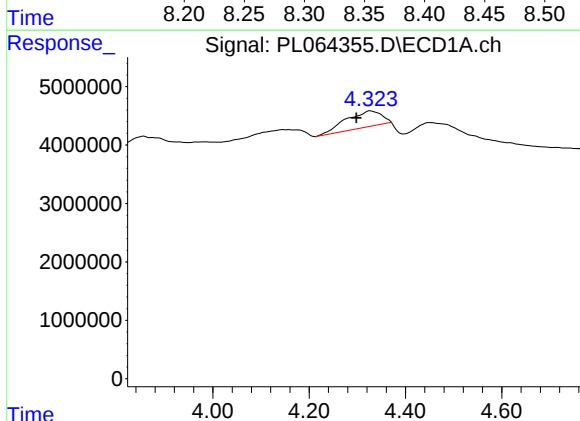


#23 Chlordane-1

R.T.: 4.326 min

Delta R.T.: 0.028 min

Response: 14356198

Conc: 123.27 ng/ml

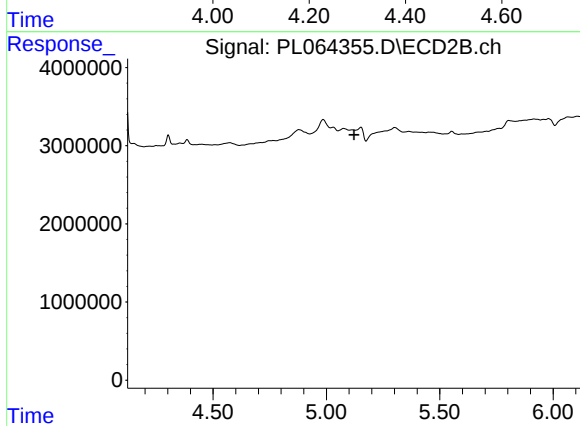


#23 Chlordane-1

R.T.: 0.000 min

Exp R.T.: 5.123 min

Response: 0


Conc: N.D.

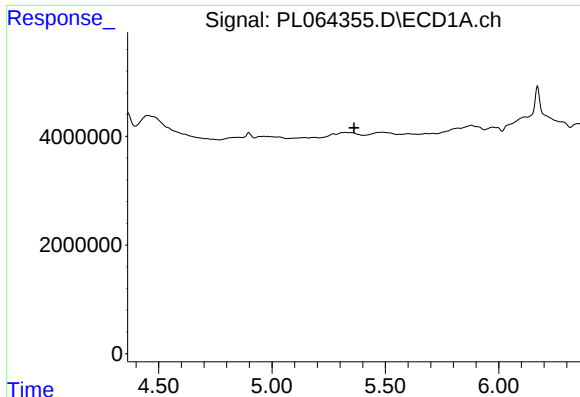

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

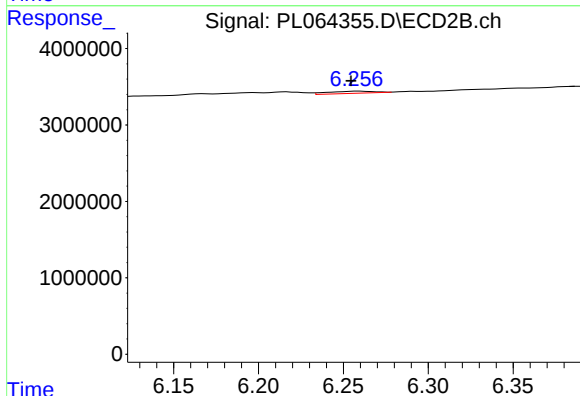


#25 Chlordane-3

R.T.: 6.259 min
Delta R.T.: 0.005 min
Response: 508229
Conc: 1.26 ng/ml

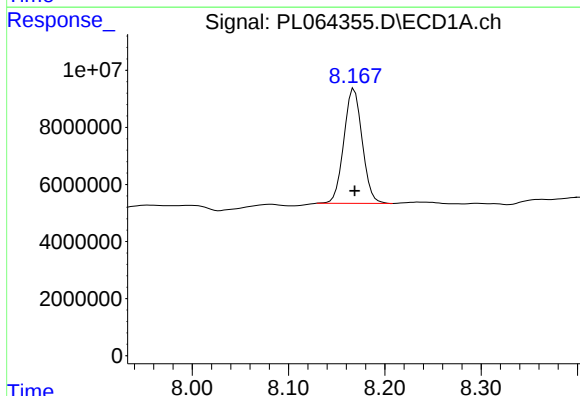

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 53104086
Conc: 17.40 ng/ml

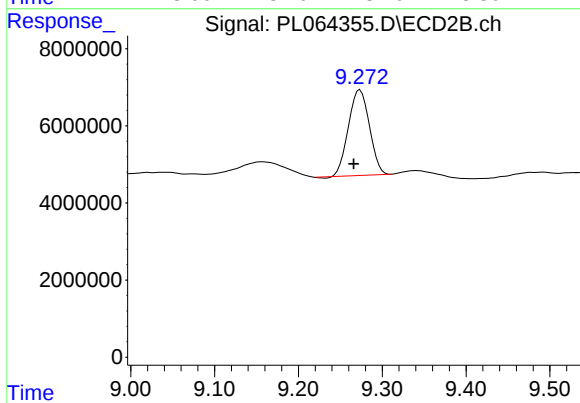

#28 Decachlorobiphenyl

R.T.: 9.274 min
Delta R.T.: 0.007 min
Response: 38590819
Conc: 16.26 ng/ml