

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012421\
 Data File : PL064368.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2021 20:20
 Operator : AR\AJ
 Sample : M1208-03 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 02:58:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.108	5382119	3956926	1.795	1.548
28)	SA Decachlor...	8.166	9.270	4646347	3689654	1.522	1.555
Target Compounds							
4)	MA Heptachlor	4.447	5.313	1834710	2509185	0.419	0.699 #
5)	MB Aldrin	4.693	5.625	3140505	2497475	0.784	0.805
10)	B gamma-Chl...	5.360	6.255	4832805	4405926	1.248	1.466
11)	B alpha-Chl...	5.418	6.328	6313037	6937771	1.650	2.279 #
12)	B 4,4'-DDE	5.584	6.484	3581804	3753914	1.017	1.409 #
16)	A 4,4'-DDD	0.000	6.983	0	1670734	N.D.	0.754 #
23)	Chlordane-1	4.297	5.122	2711137	1792695	23.280	16.052 #
24)	Chlordane-2	4.795	5.598	3321733	1858032	23.602	14.656 #
25)	Chlordane-3	5.360	6.255	4832805	4405926	12.095	10.897
26)	Chlordane-4	5.418	6.328	6313037	6937771	19.187	14.036 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012421\
Data File : PL064368.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2021 20:20
Operator : AR\AJ
Sample : M1208-03 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 02:58:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

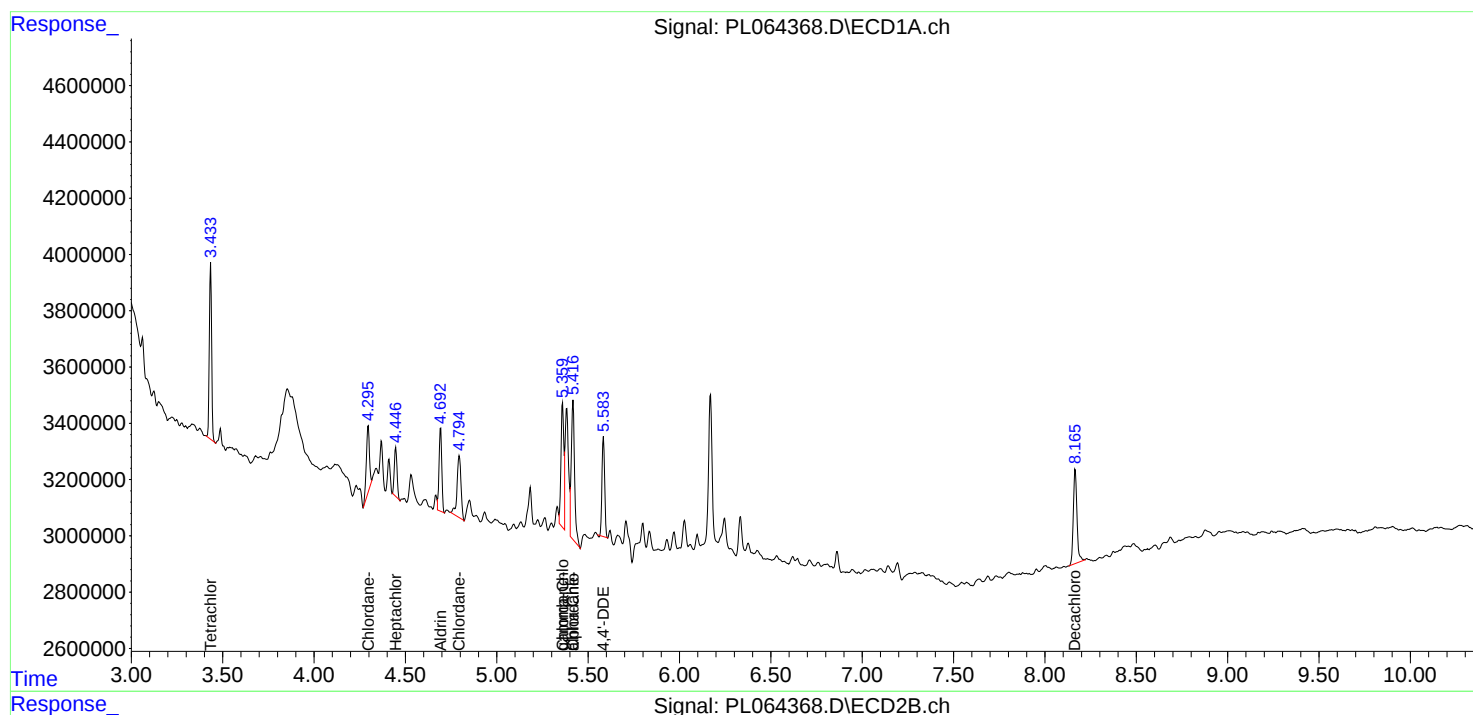


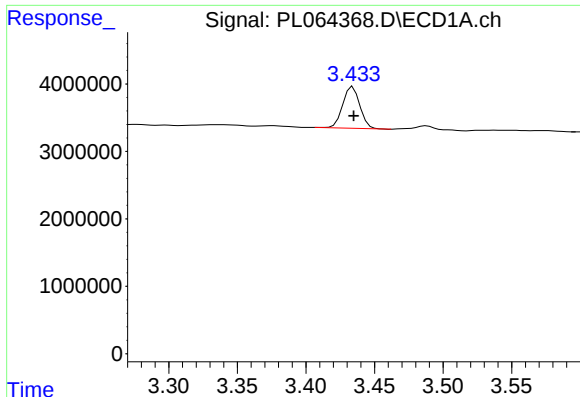

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 5382119
Conc: 1.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

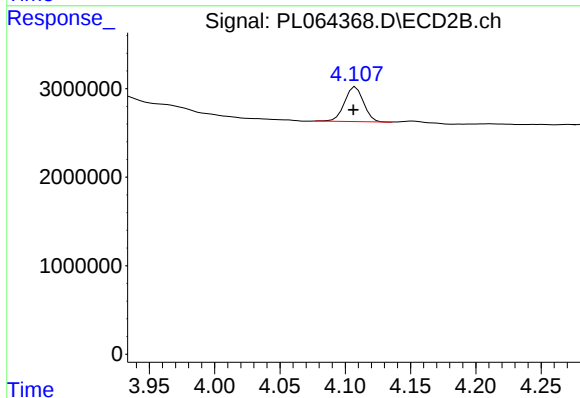


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.002 min
Response: 3956926
Conc: 1.55 ng/ml

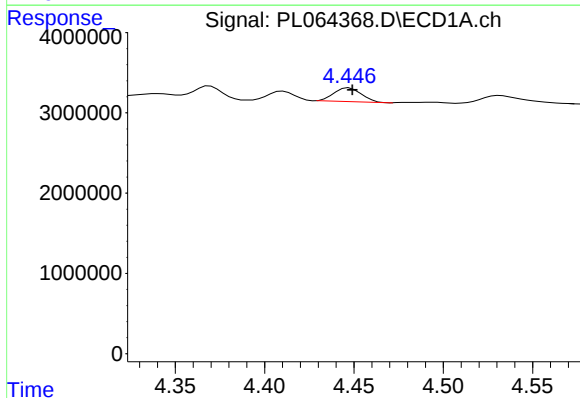


#4 Heptachlor

R.T.: 4.447 min
Delta R.T.: -0.002 min
Response: 1834710
Conc: 0.42 ng/ml

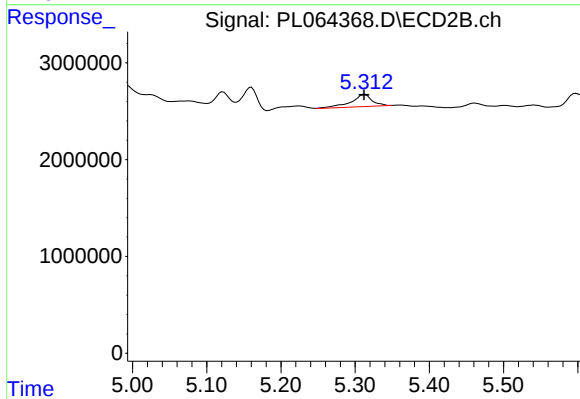

#4 Heptachlor


R.T.: 5.313 min
Delta R.T.: 0.000 min
Response: 2509185
Conc: 0.70 ng/ml

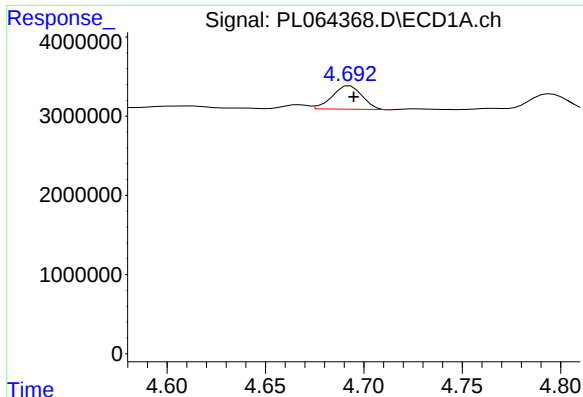

#5 Aldrin


R.T.: 4.693 min
Delta R.T.: -0.002 min
Response: 3140505
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

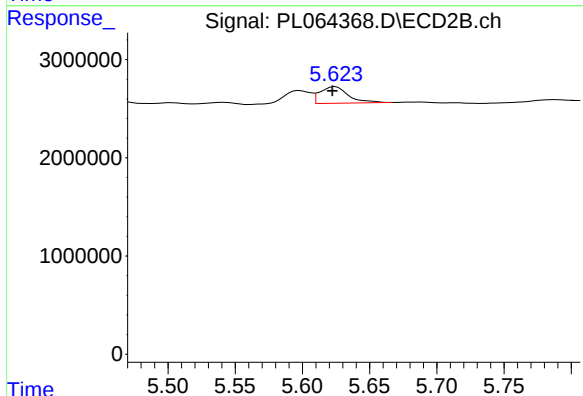


#5 Aldrin

R.T.: 5.625 min
Delta R.T.: 0.002 min
Response: 2497475
Conc: 0.80 ng/ml

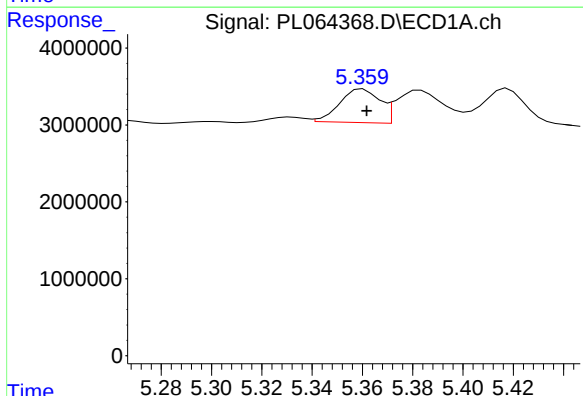


#10 gamma-Chlordane

R.T.: 5.360 min
Delta R.T.: -0.002 min
Response: 4832805
Conc: 1.25 ng/ml

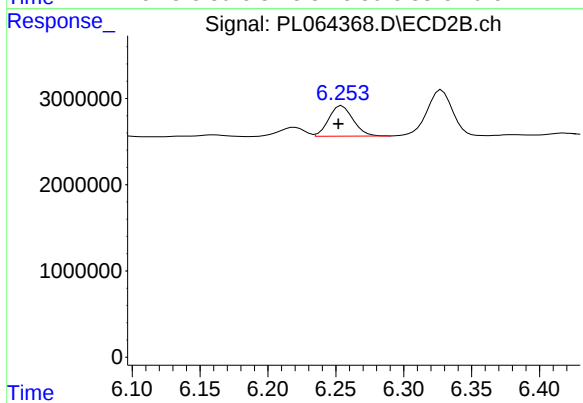

#10 gamma-Chlordane


R.T.: 6.255 min
Delta R.T.: 0.003 min
Response: 4405926
Conc: 1.47 ng/ml

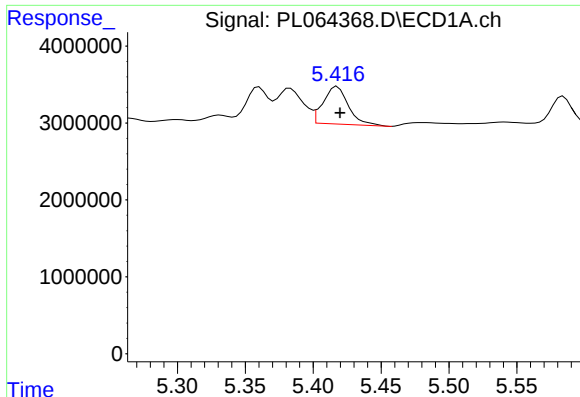

#11 alpha-Chlordane


R.T.: 5.418 min
Delta R.T.: -0.002 min
Response: 6313037
Conc: 1.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

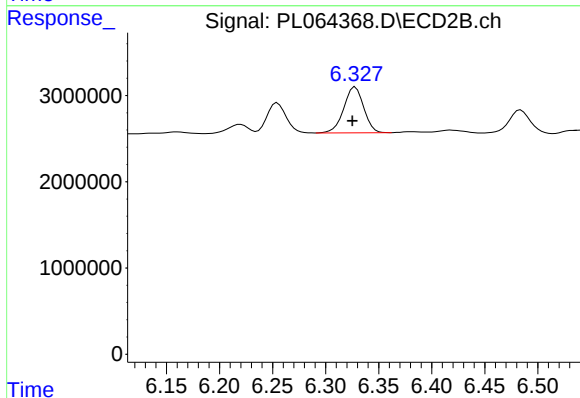


#11 alpha-Chlordane

R.T.: 6.328 min
Delta R.T.: 0.003 min
Response: 6937771
Conc: 2.28 ng/ml

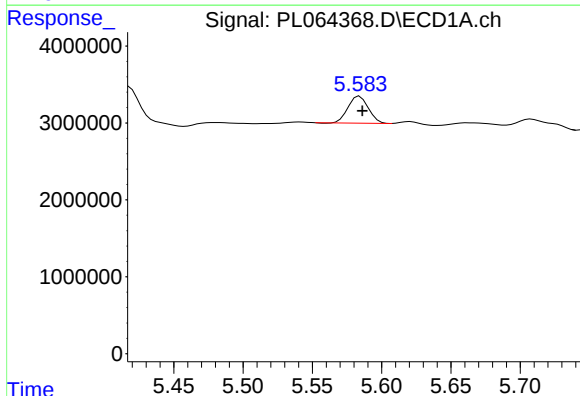


#12 4,4'-DDE

R.T.: 5.584 min
Delta R.T.: -0.002 min
Response: 3581804
Conc: 1.02 ng/ml

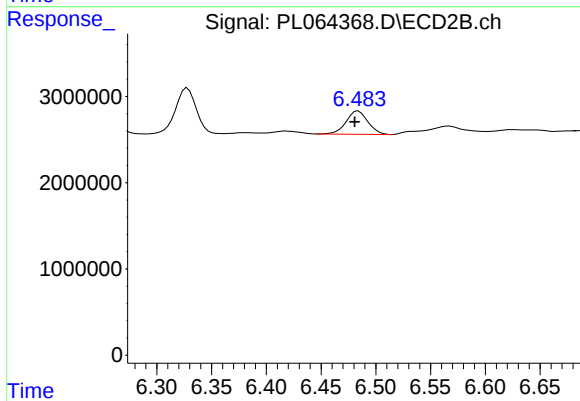

#12 4,4'-DDE


R.T.: 6.484 min
Delta R.T.: 0.003 min
Response: 3753914
Conc: 1.41 ng/ml

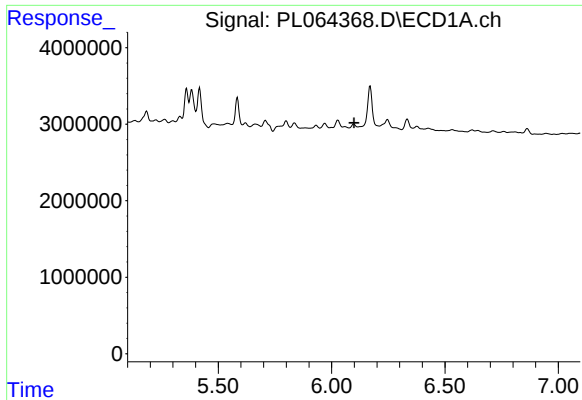

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

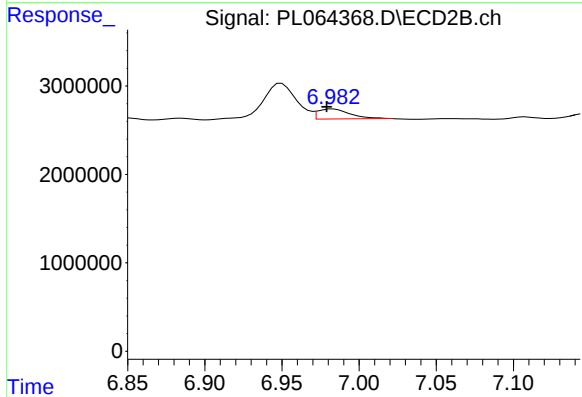


#16 4,4'-DDD

R.T.: 6.983 min
Delta R.T.: 0.004 min
Response: 1670734
Conc: 0.75 ng/ml

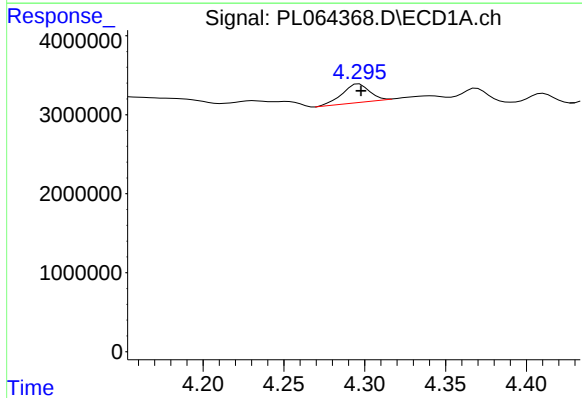


#23 Chlordane-1

R.T.: 4.297 min
Delta R.T.: -0.001 min
Response: 2711137
Conc: 23.28 ng/ml

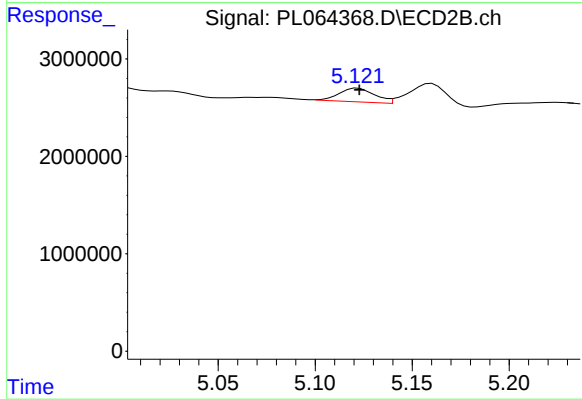

#23 Chlordane-1


R.T.: 5.122 min
Delta R.T.: 0.000 min
Response: 1792695
Conc: 16.05 ng/ml

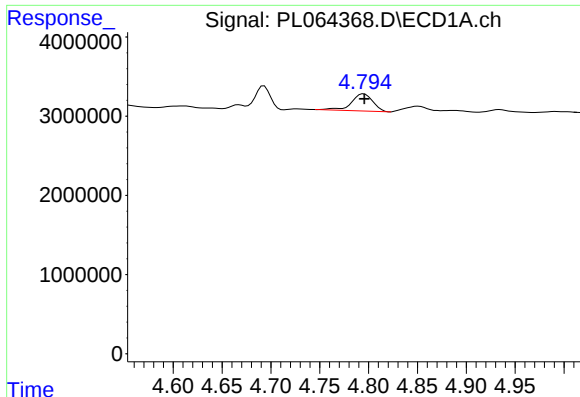

#24 Chlordane-2


R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 3321733
Conc: 23.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

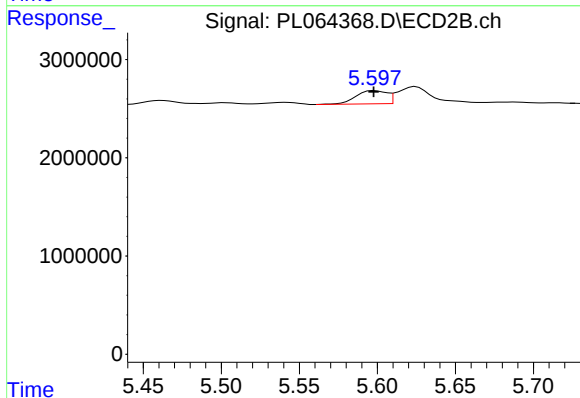


#24 Chlordane-2

R.T.: 5.598 min
Delta R.T.: 0.000 min
Response: 1858032
Conc: 14.66 ng/ml

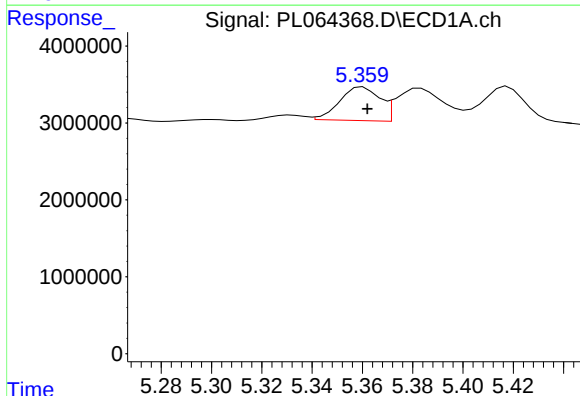


#25 Chlordane-3

R.T.: 5.360 min
Delta R.T.: -0.002 min
Response: 4832805
Conc: 12.10 ng/ml

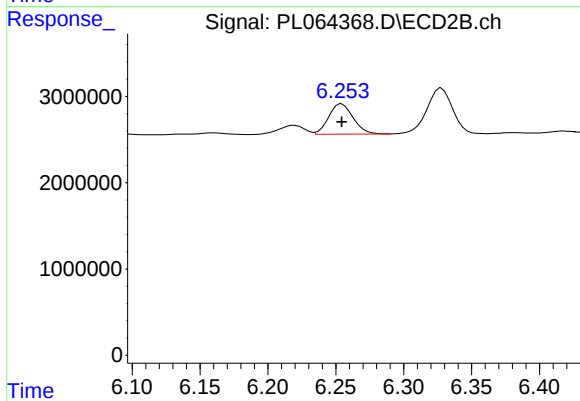

#25 Chlordane-3


R.T.: 6.255 min
Delta R.T.: 0.000 min
Response: 4405926
Conc: 10.90 ng/ml

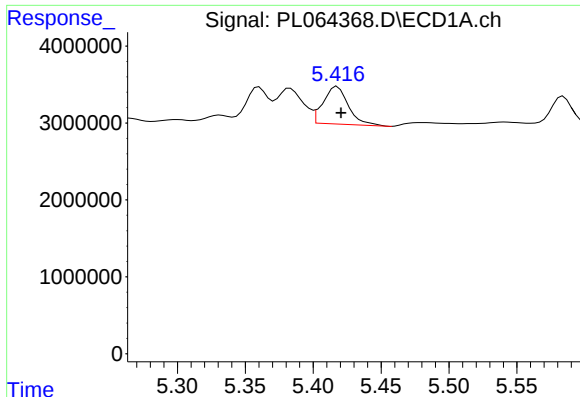

#26 Chlordane-4


R.T.: 5.418 min
Delta R.T.: -0.003 min
Response: 6313037
Conc: 19.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

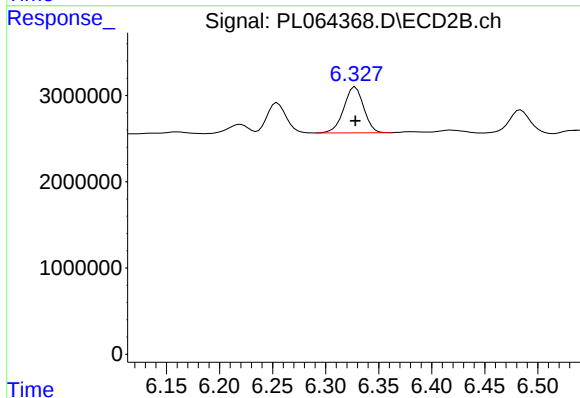


#26 Chlordane-4

R.T.: 6.328 min
Delta R.T.: 0.000 min
Response: 6937771
Conc: 14.04 ng/ml

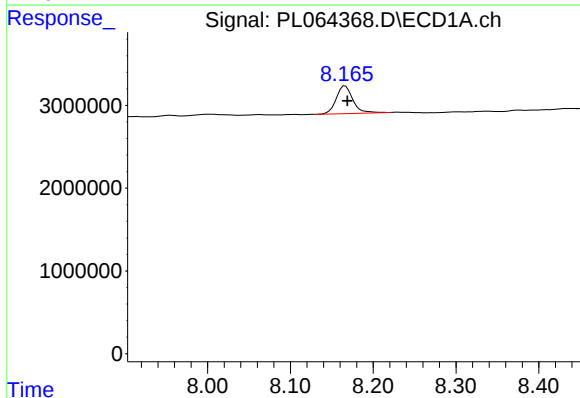

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: -0.003 min
Response: 4646347
Conc: 1.52 ng/ml

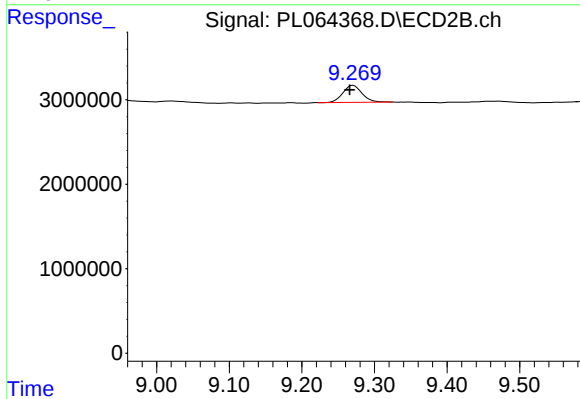

#28 Decachlorobiphenyl

R.T.: 9.270 min
Delta R.T.: 0.004 min
Response: 3689654
Conc: 1.55 ng/ml