

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012422\
 Data File : PL072195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2022 18:03
 Operator : AR\AJ
 Sample : N1242-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 02:07:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.491	3296684	9537015	5.938	5.872
28)	SA Decachlor...	10.320	11.387	7837394	13423811	8.822	8.320
Target Compounds							
7)	B delta-BHC	0.000	7.016f	0	788162	N.D.	0.320 #
8)	B Heptachlo...	0.000	7.955	0	400216	N.D.	0.200 #
9)	A Endosulfan I	0.000	8.371	0	36238	N.D.	0.020 #
10)	B gamma-Chl...	0.000	8.248f	0	422433	N.D.	0.209 #
11)	B alpha-Chl...	0.000	8.309	0	288753	N.D.	0.146 #
12)	B 4,4'-DDE	0.000	8.494	0	417640	N.D.	0.221 #
13)	MA Dieldrin	7.693	8.652	68351	28320	0.090	0.014 #
14)	MA Endrin	0.000	8.888	0	551542	N.D.	0.333 #
16)	A 4,4'-DDD	0.000	9.034	0	413742	N.D.	0.289 #
17)	MA 4,4'-DDT	8.396	0.000	207501	0	0.312	N.D. #
25)	Chlordane-3	0.000	8.248f	0	422433	N.D.	1.520 #
26)	Chlordane-4	0.000	8.309	0	288753	N.D.	0.870 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012422\
Data File : PL072195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2022 18:03
Operator : AR\AJ
Sample : N1242-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 02:07:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

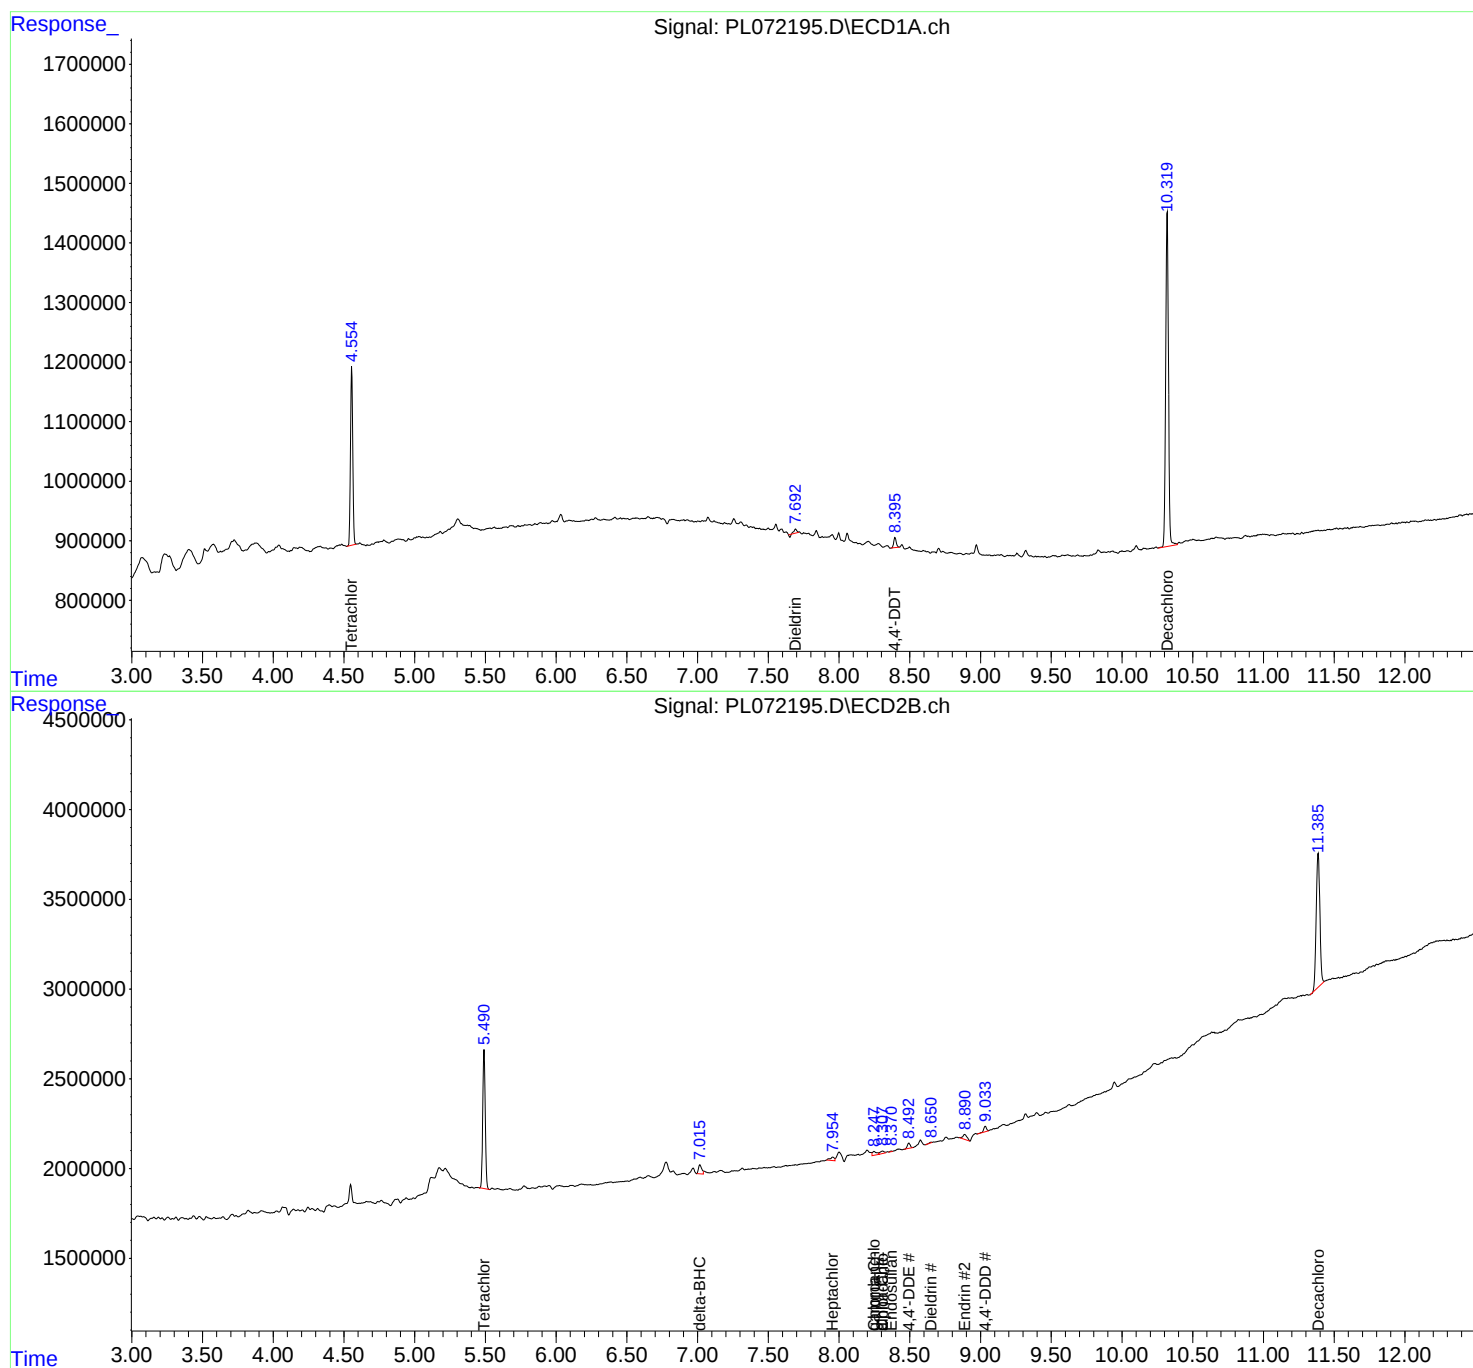


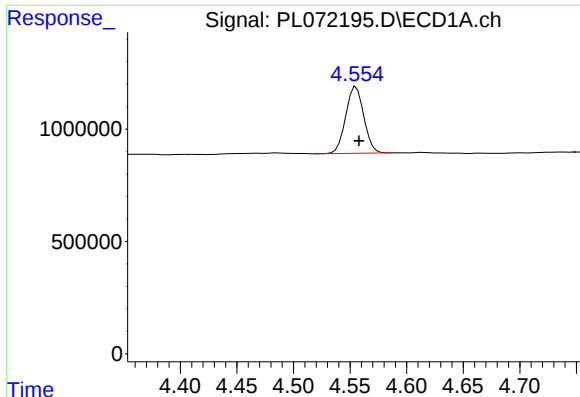

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 3296684
Conc: 5.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

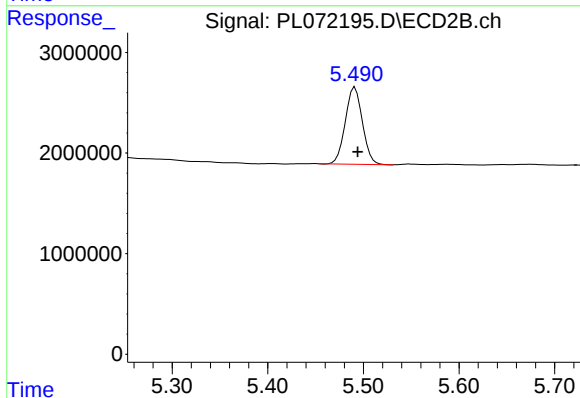


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 9537015
Conc: 5.87 ng/ml

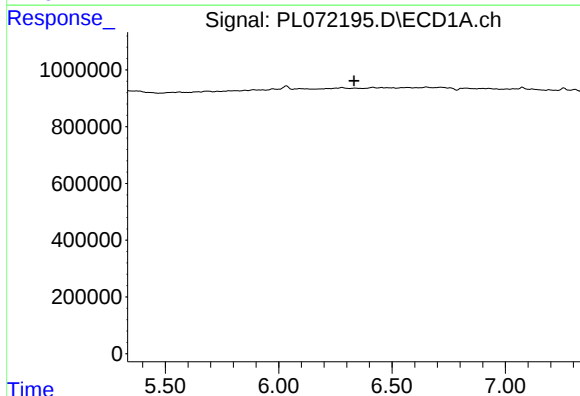


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

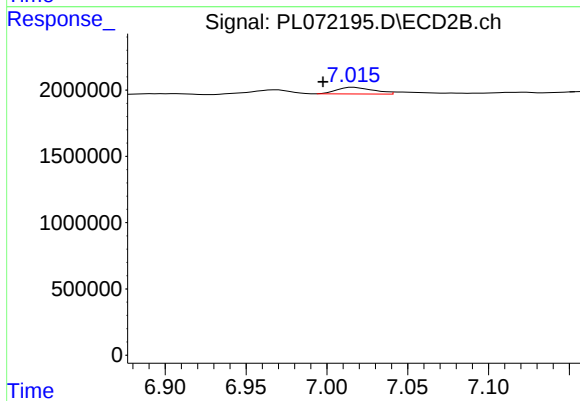

#7 delta-BHC


R.T.: 7.016 min
Delta R.T.: 0.019 min
Response: 788162
Conc: 0.32 ng/ml

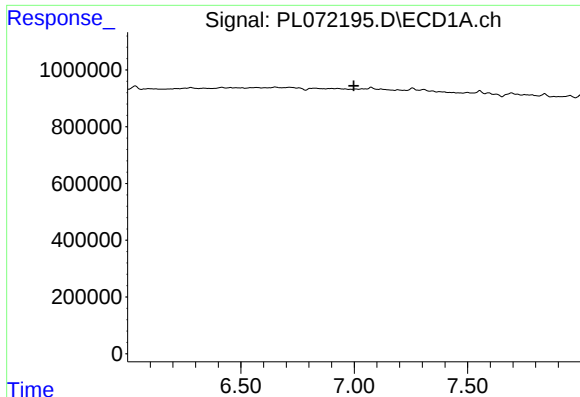

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.998 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

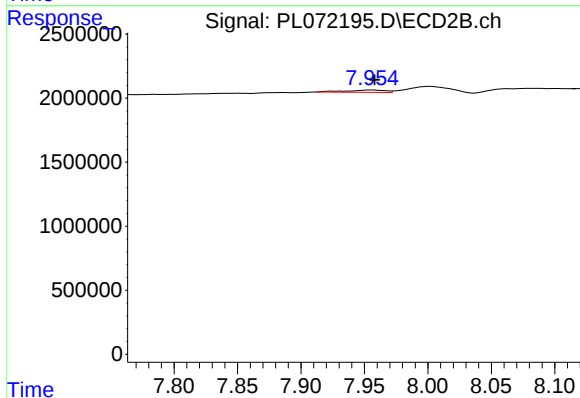


#8 Heptachlor epoxide

R.T.: 7.955 min
Delta R.T.: -0.003 min
Response: 400216
Conc: 0.20 ng/ml

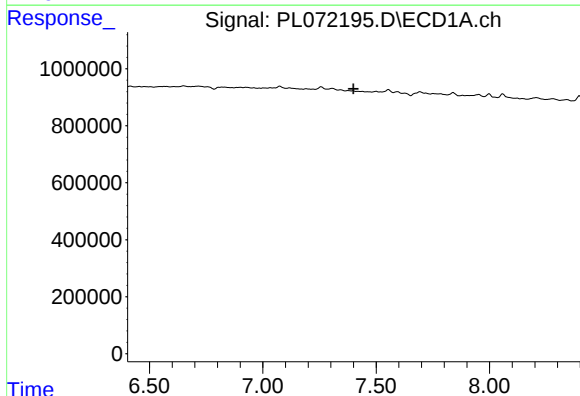


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

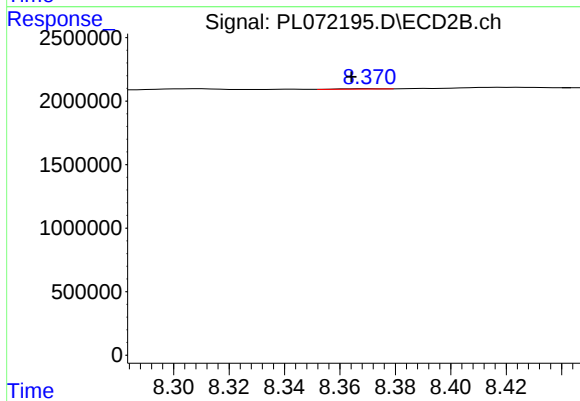

#9 Endosulfan I


R.T.: 8.371 min
Delta R.T.: 0.007 min
Response: 36238
Conc: 0.02 ng/ml

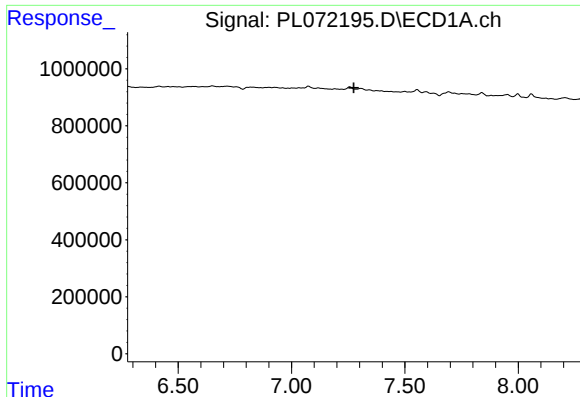

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

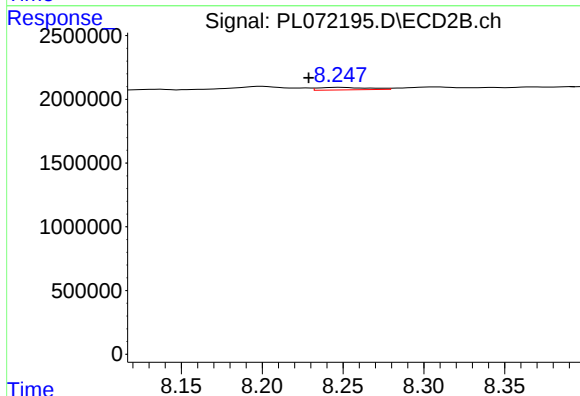


#10 gamma-Chlordane

R.T.: 8.248 min
Delta R.T.: 0.020 min
Response: 422433
Conc: 0.21 ng/ml

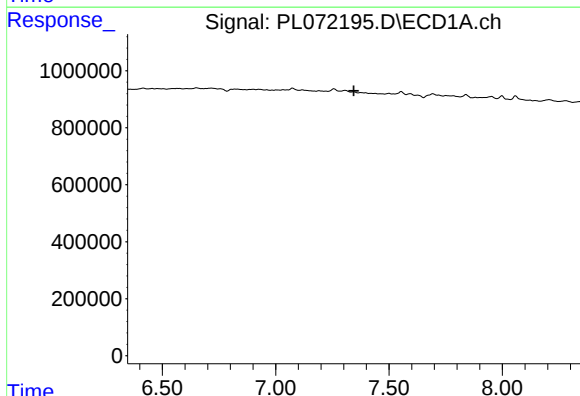


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

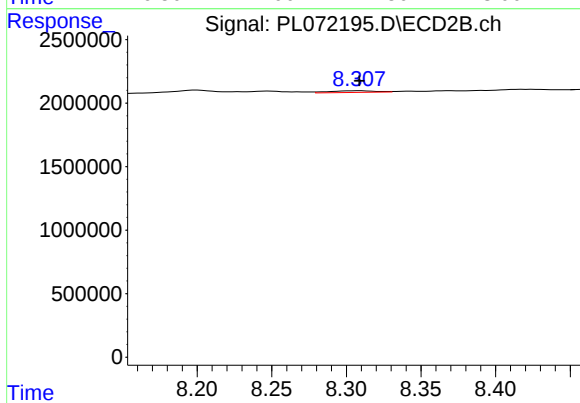

#11 alpha-Chlordane


R.T.: 8.309 min
Delta R.T.: 0.000 min
Response: 288753
Conc: 0.15 ng/ml

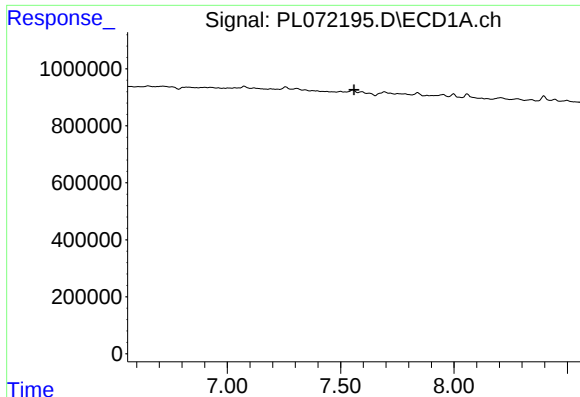

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.560 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

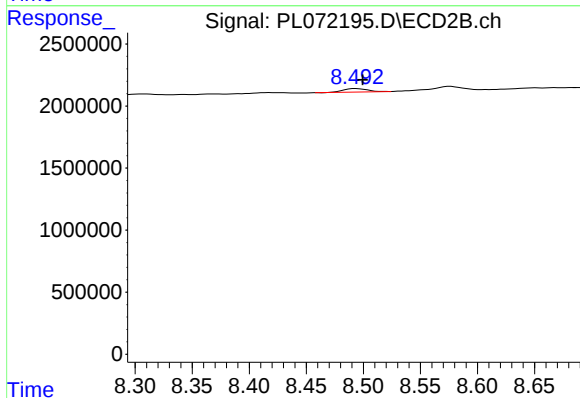


#12 4,4'-DDE

R.T.: 8.494 min
Delta R.T.: -0.006 min
Response: 417640
Conc: 0.22 ng/ml

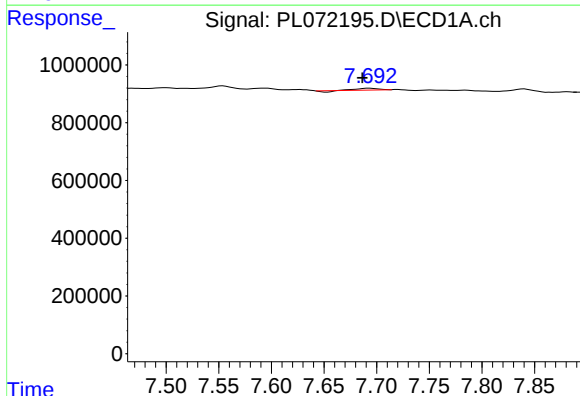


#13 Dieldrin

R.T.: 7.693 min
Delta R.T.: 0.007 min
Response: 68351
Conc: 0.09 ng/ml

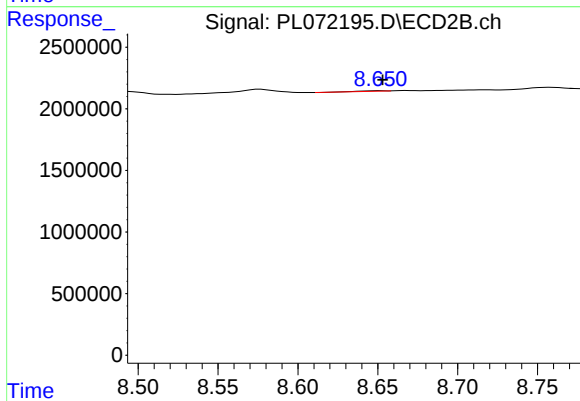

#13 Dieldrin


R.T.: 8.652 min
Delta R.T.: -0.001 min
Response: 28320
Conc: 0.01 ng/ml

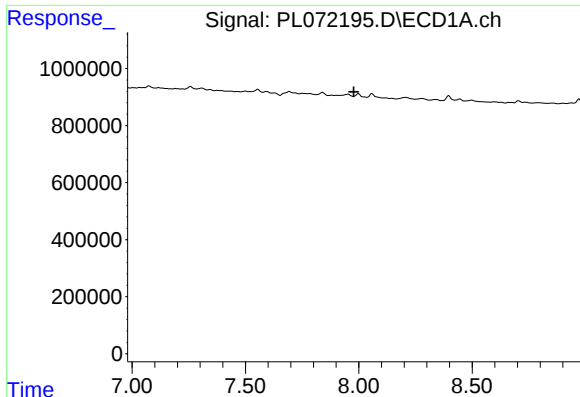

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 7.978 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

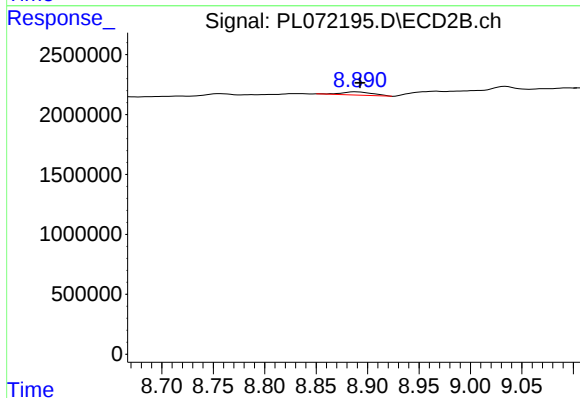


#14 Endrin

R.T.: 8.888 min
Delta R.T.: -0.005 min
Response: 551542
Conc: 0.33 ng/ml

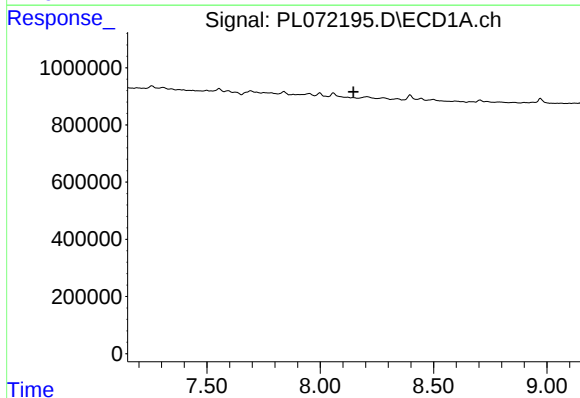


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

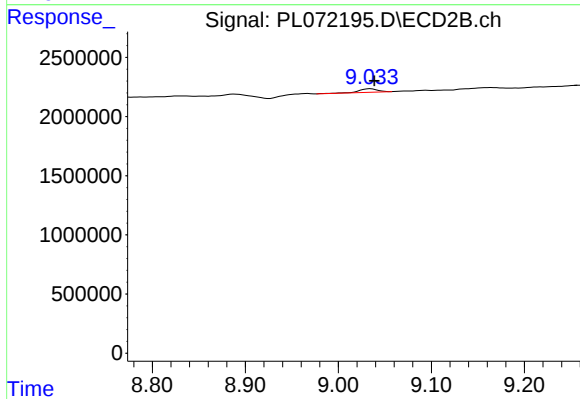

#16 4,4'-DDD


R.T.: 9.034 min
Delta R.T.: -0.004 min
Response: 413742
Conc: 0.29 ng/ml

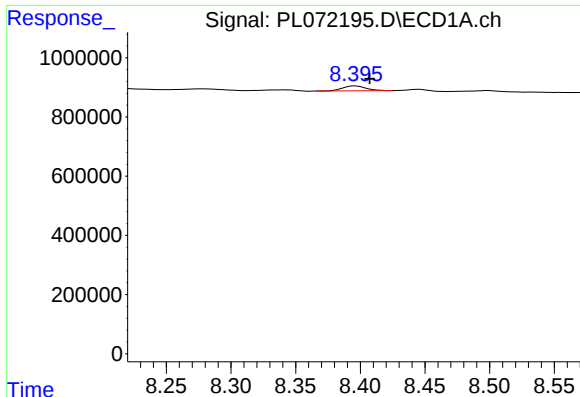

#17 4,4'-DDT


R.T.: 8.396 min
Delta R.T.: -0.011 min
Response: 207501
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

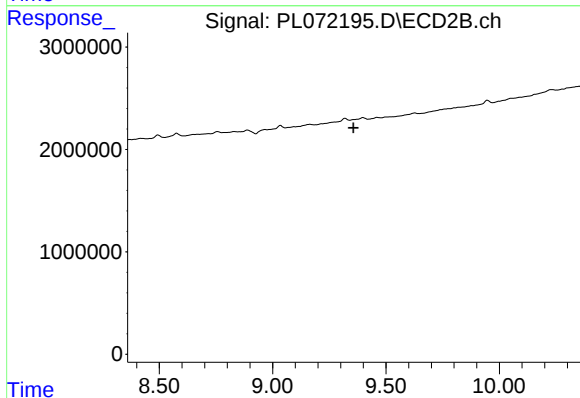


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.357 min
Response: 0
Conc: N.D.

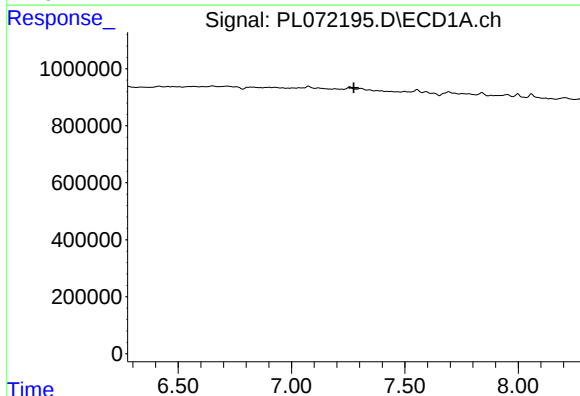


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.274 min
Response: 0
Conc: N.D.

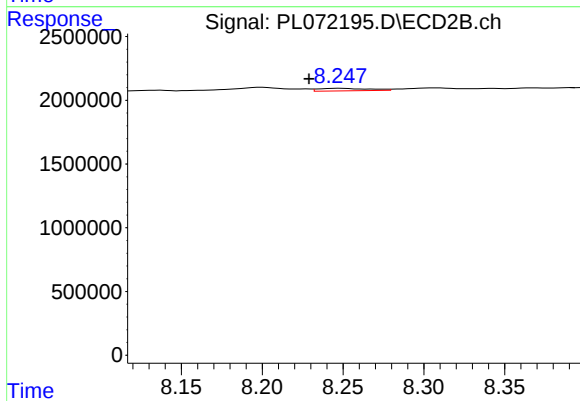

#25 Chlordane-3


R.T.: 8.248 min
Delta R.T.: 0.019 min
Response: 422433
Conc: 1.52 ng/ml

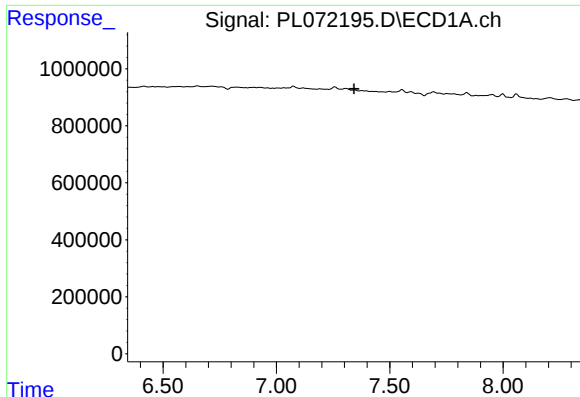

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

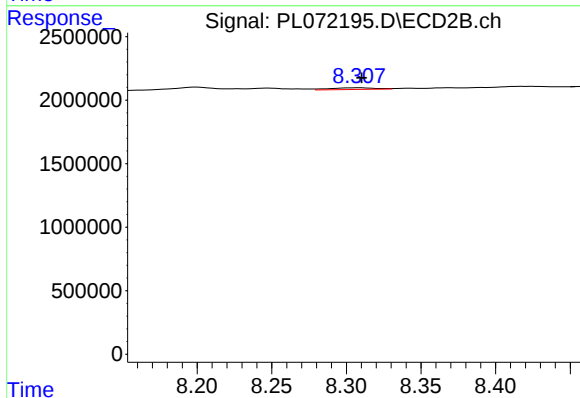


#26 Chlordane-4

R.T.: 8.309 min
Delta R.T.: -0.001 min
Response: 288753
Conc: 0.87 ng/ml

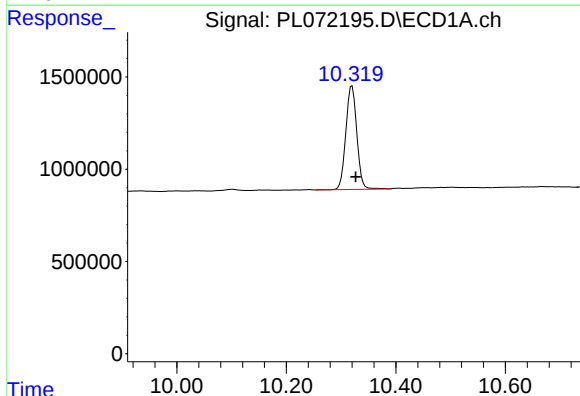

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: -0.007 min
Response: 7837394
Conc: 8.82 ng/ml

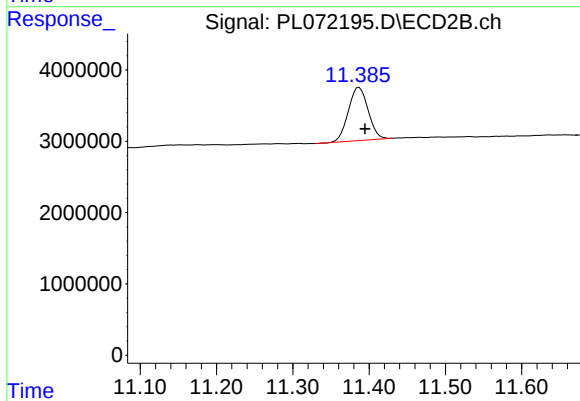

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: -0.008 min
Response: 13423811
Conc: 8.32 ng/ml