

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012422\
 Data File : PL072199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2022 19:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 02:08:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.492	10816077	31544121	19.482	19.422
28)	SA Decachlor...	10.319	11.387	15502713	29947112	17.449	18.560
Target Compounds							
7)	B delta-BHC	0.000	7.020f	0	682885	N.D.	0.278 #
9)	A Endosulfan I	0.000	8.346f	0	126691	N.D.	0.070 #
10)	B gamma-Chl...	0.000	8.235	0	157132	N.D.	0.078 #
14)	MA Endrin	7.999f	0.000	356176	0	0.508	N.D. #
15)	B Endosulfa...	0.000	9.149f	0	753952	N.D.	0.440 #
17)	MA 4,4'-DDT	0.000	9.351	0	93804	N.D.	0.059 #
19)	B Endosulfa...	0.000	9.502	0	298025	N.D.	0.191 #
21)	B Endrin ke...	0.000	9.981f	0	11513	N.D.	0.007 #
25)	Chlordane-3	0.000	8.235	0	157132	N.D.	0.566 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012422\
Data File : PL072199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2022 19:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 02:08:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

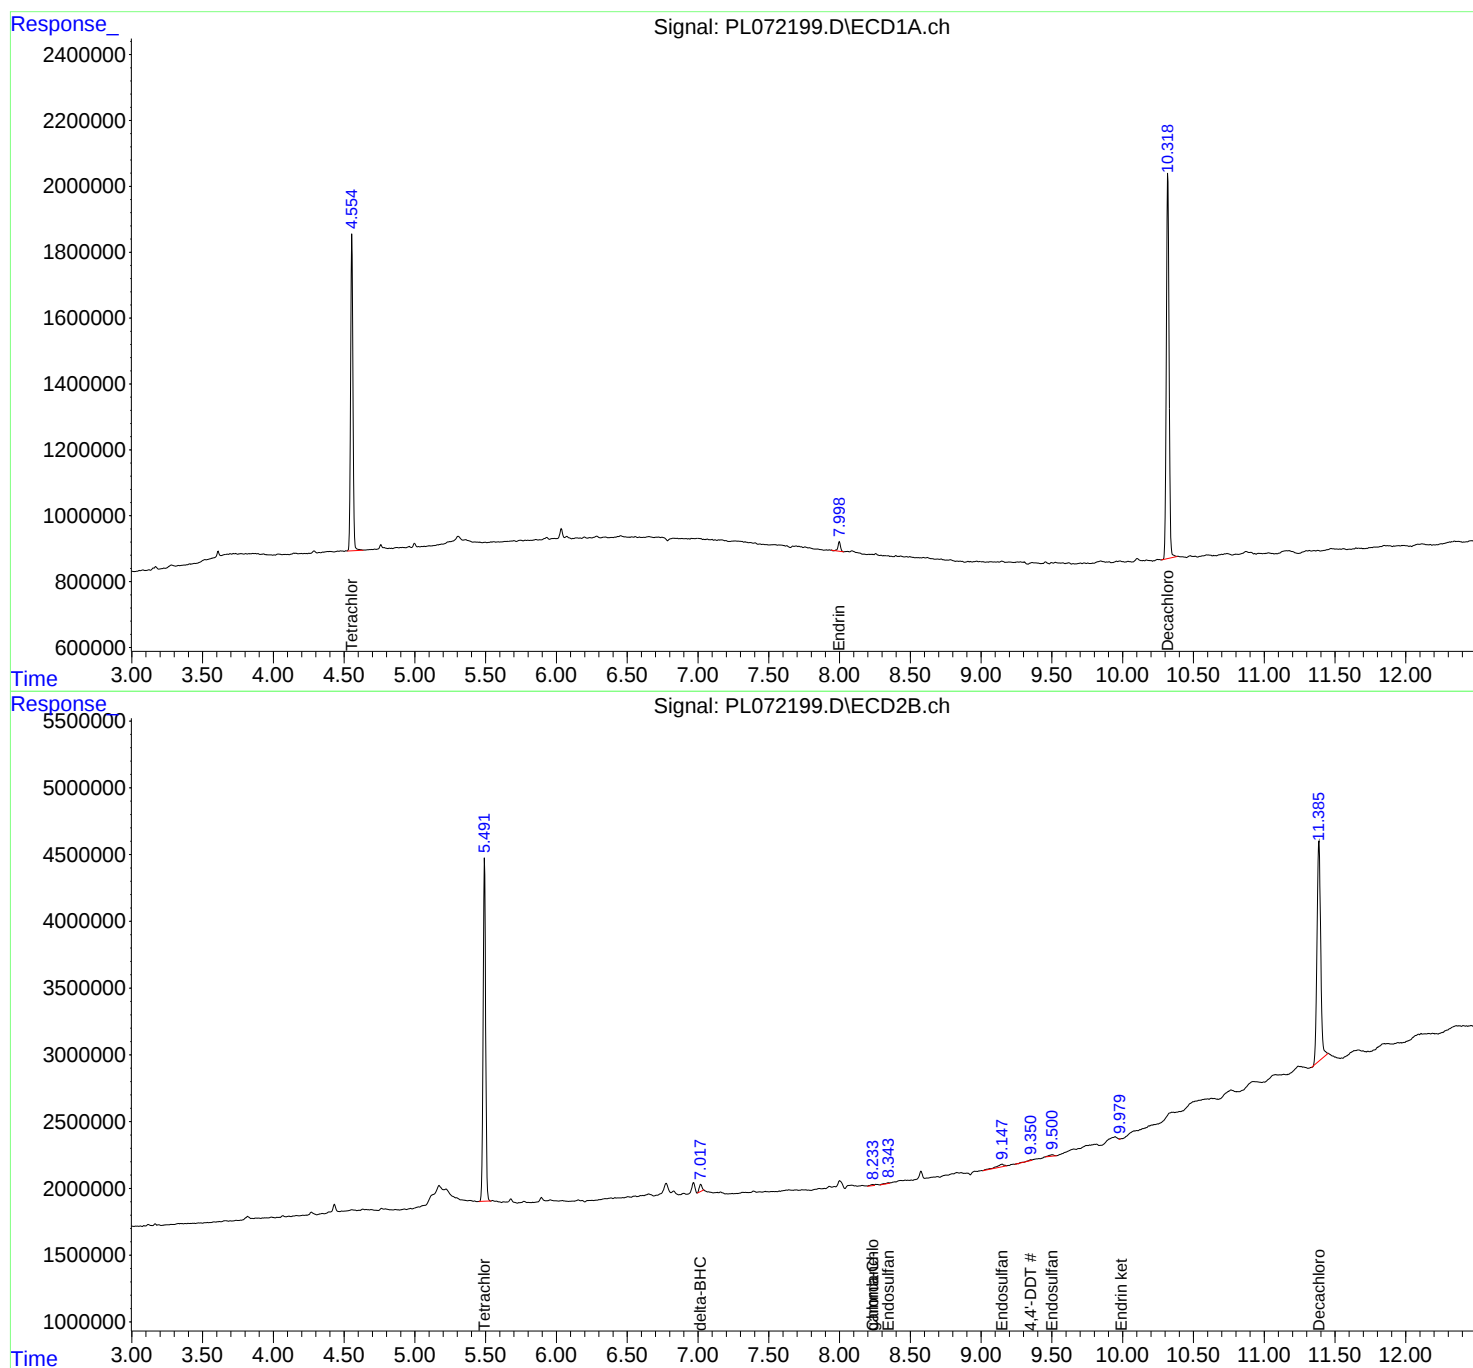


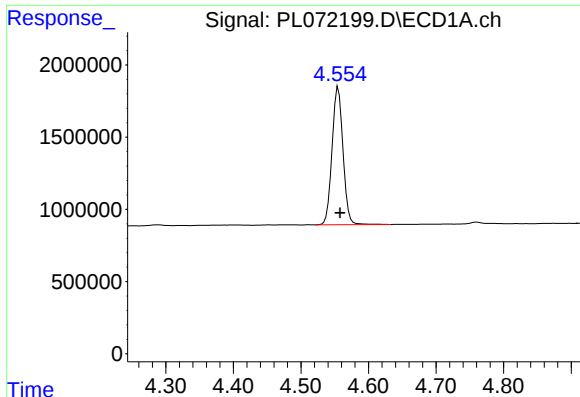

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 10816077
Conc: 19.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

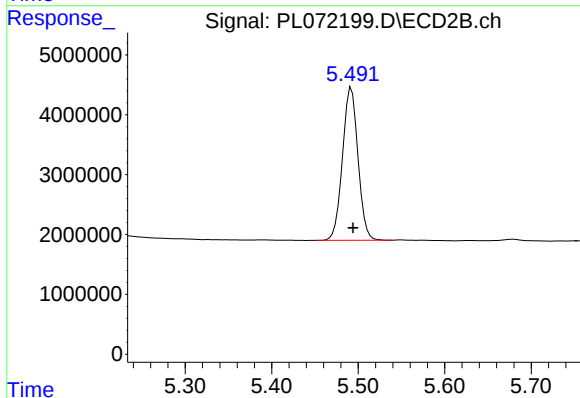


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 31544121
Conc: 19.42 ng/ml

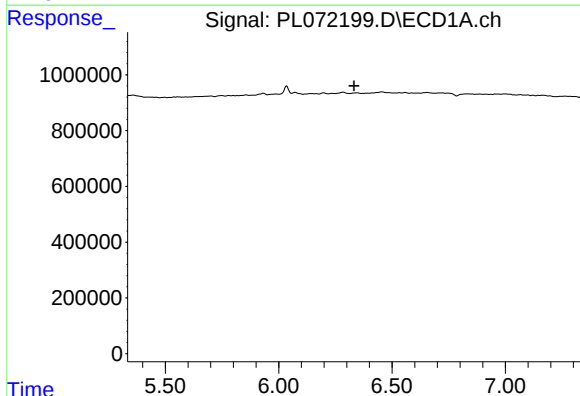


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

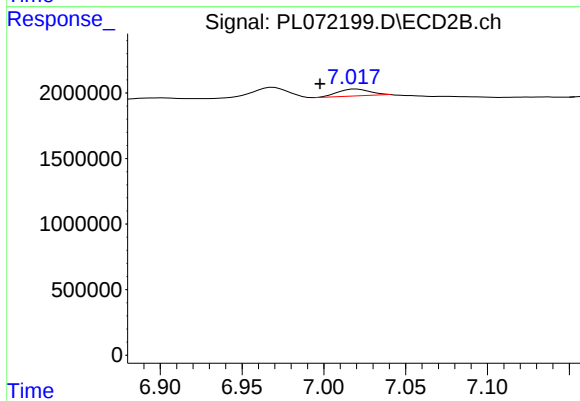

#7 delta-BHC


R.T.: 7.020 min
Delta R.T.: 0.022 min
Response: 682885
Conc: 0.28 ng/ml

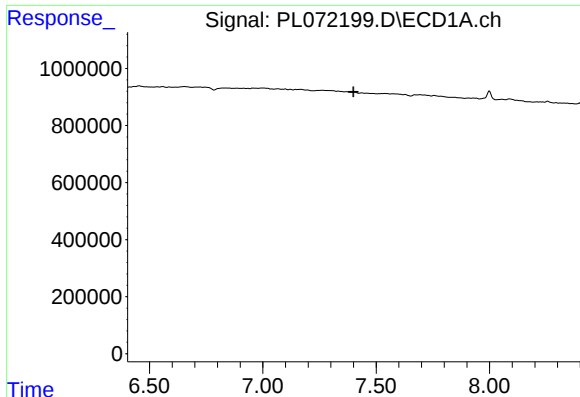

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

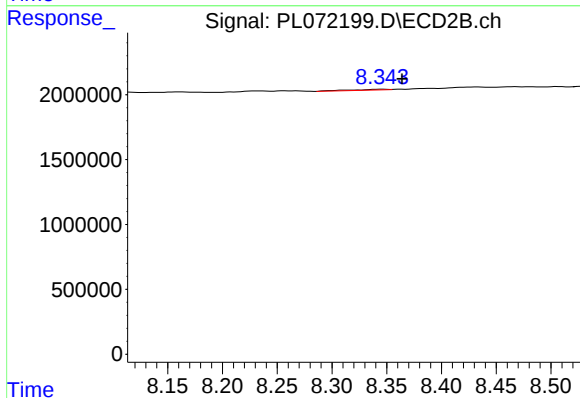


#9 Endosulfan I

R.T.: 8.346 min
Delta R.T.: -0.018 min
Response: 126691
Conc: 0.07 ng/ml

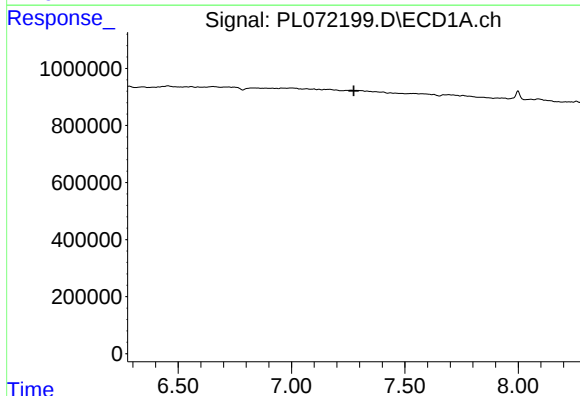


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

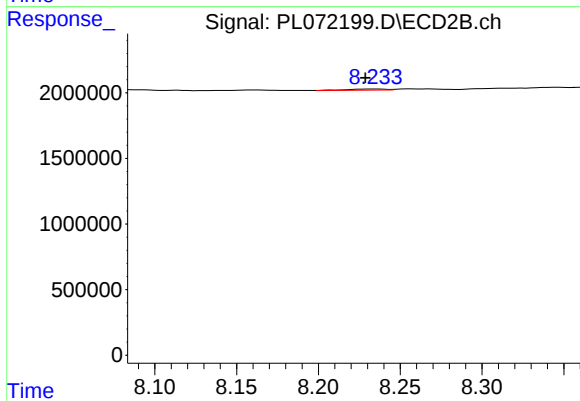

#10 gamma-Chlordane


R.T.: 8.235 min
Delta R.T.: 0.006 min
Response: 157132
Conc: 0.08 ng/ml

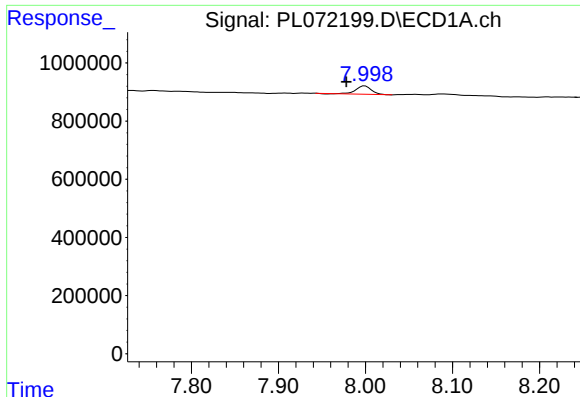

#14 Endrin


R.T.: 7.999 min
Delta R.T.: 0.021 min
Response: 356176
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

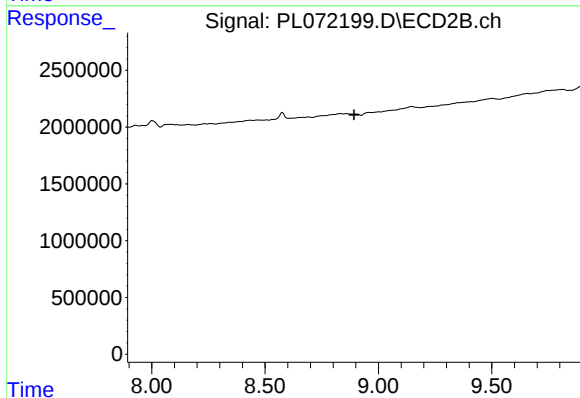


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

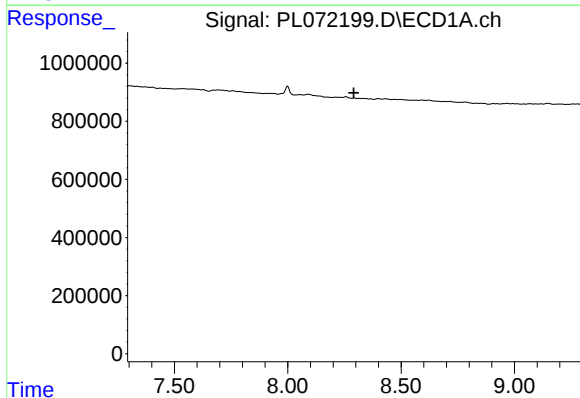


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.291 min
Response: 0
Conc: N.D.

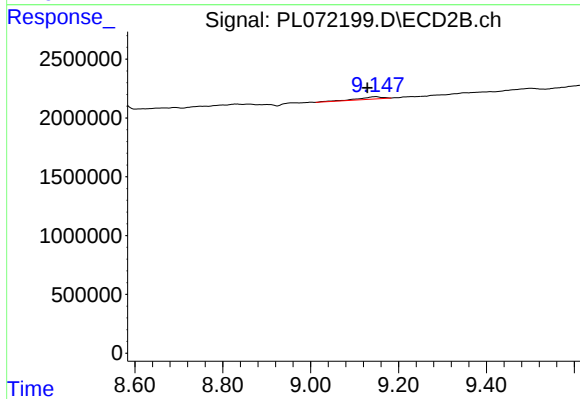

#15 Endosulfan II


R.T.: 9.149 min
Delta R.T.: 0.020 min
Response: 753952
Conc: 0.44 ng/ml

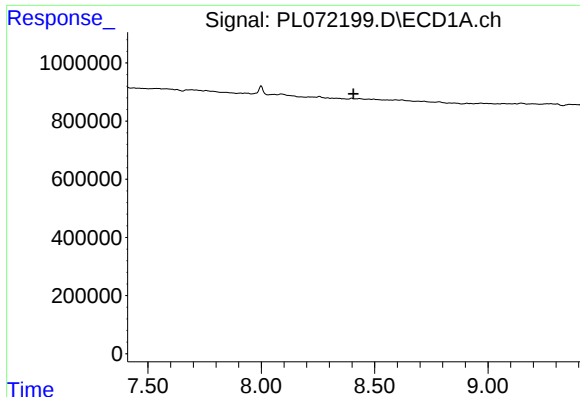

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

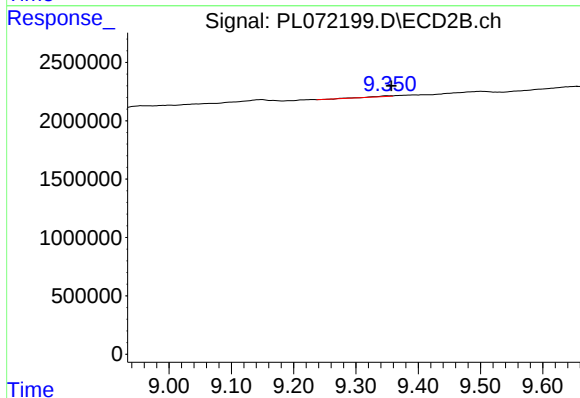


#17 4,4'-DDT

R.T.: 9.351 min
Delta R.T.: -0.006 min
Response: 93804
Conc: 0.06 ng/ml

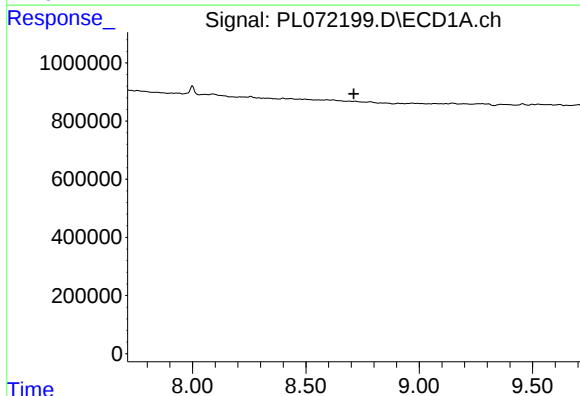


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

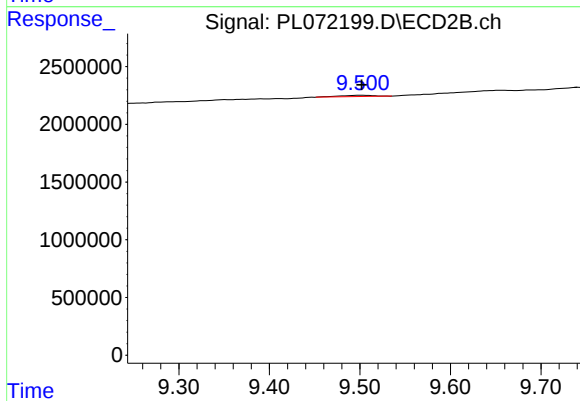

#19 Endosulfan Sulfate


R.T.: 9.502 min
Delta R.T.: 0.000 min
Response: 298025
Conc: 0.19 ng/ml

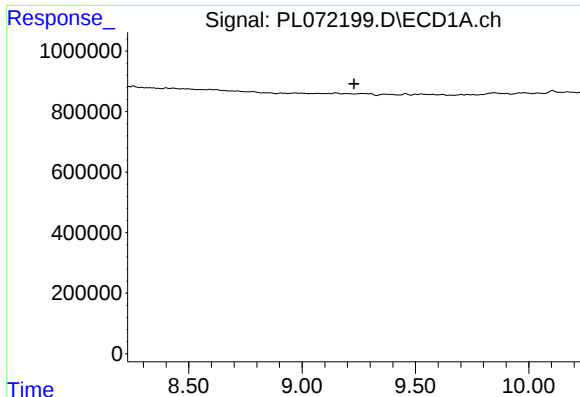

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.229 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

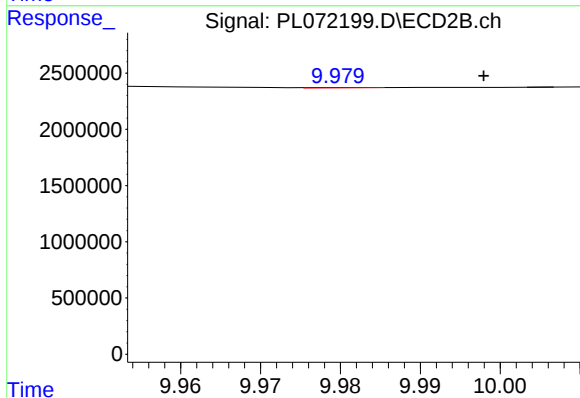


#21 Endrin ketone

R.T.: 9.981 min
Delta R.T.: -0.017 min
Response: 11513
Conc: 0.01 ng/ml

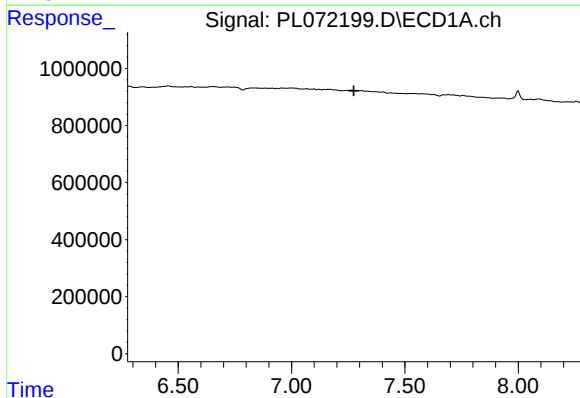


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

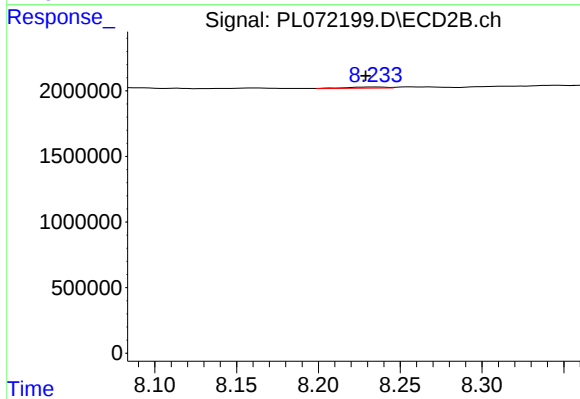

#25 Chlordane-3


R.T.: 8.235 min
Delta R.T.: 0.006 min
Response: 157132
Conc: 0.57 ng/ml

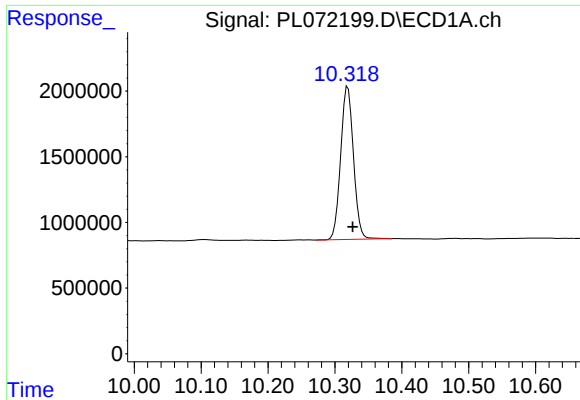

#28 Decachlorobiphenyl

R.T.: 10.319 min
Delta R.T.: -0.007 min
Response: 15502713
Conc: 17.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

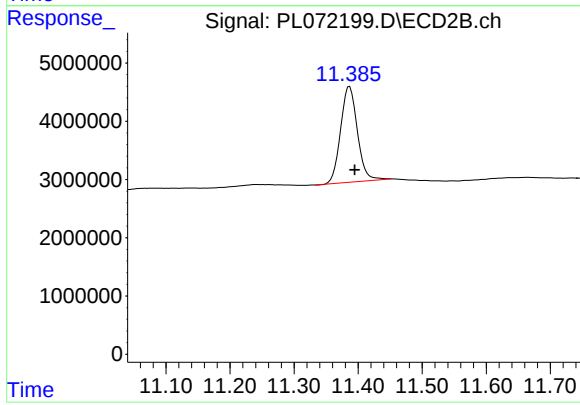

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: -0.008 min
Response: 29947112
Conc: 18.56 ng/ml