

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012422\
 Data File : PL072201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2022 21:35
 Operator : AR\AJ
 Sample : PB142226BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 02:09:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	11141619	32174316	20.068	19.810
28)	SA Decachlor...	10.320	11.387	17502589	32396126	19.700	20.078
Target Compounds							
3)	MA gamma-BHC...	0.000	6.501f	0	215893	N.D.	0.096 #
7)	B delta-BHC	0.000	7.016f	0	3533276	N.D.	1.436 #
9)	A Endosulfan I	0.000	8.372	0	14997	N.D.	0.008 #
10)	B gamma-Chl...	0.000	8.228	0	409165	N.D.	0.202 #
18)	B Endrin al...	0.000	9.288f	0	143377	N.D.	0.115 #
19)	B Endosulfa...	0.000	9.502	0	106179	N.D.	0.068 #
25)	Chlordane-3	0.000	8.228	0	409165	N.D.	1.473 #
27)	Chlordane-5	0.000	9.176f	0	30931	N.D.	0.507 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012422\
Data File : PL072201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2022 21:35
Operator : AR\AJ
Sample : PB142226BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 02:09:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

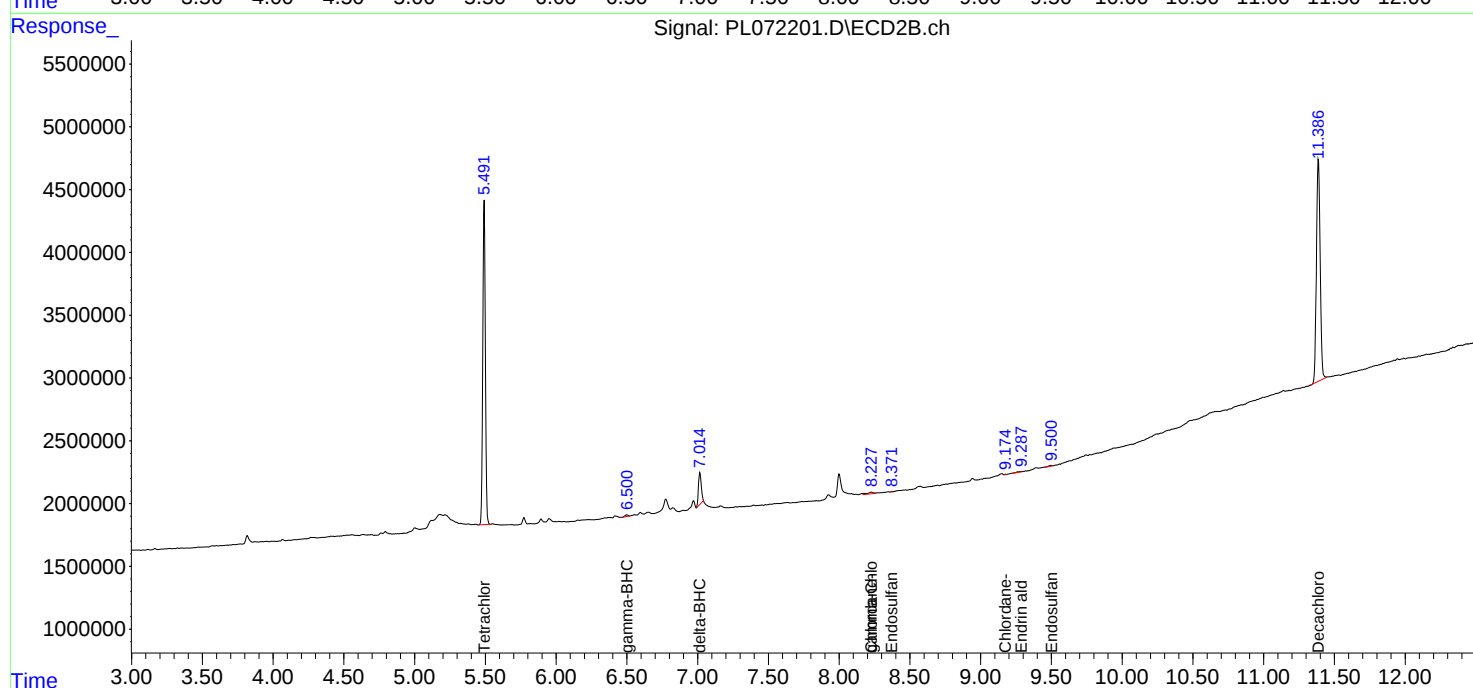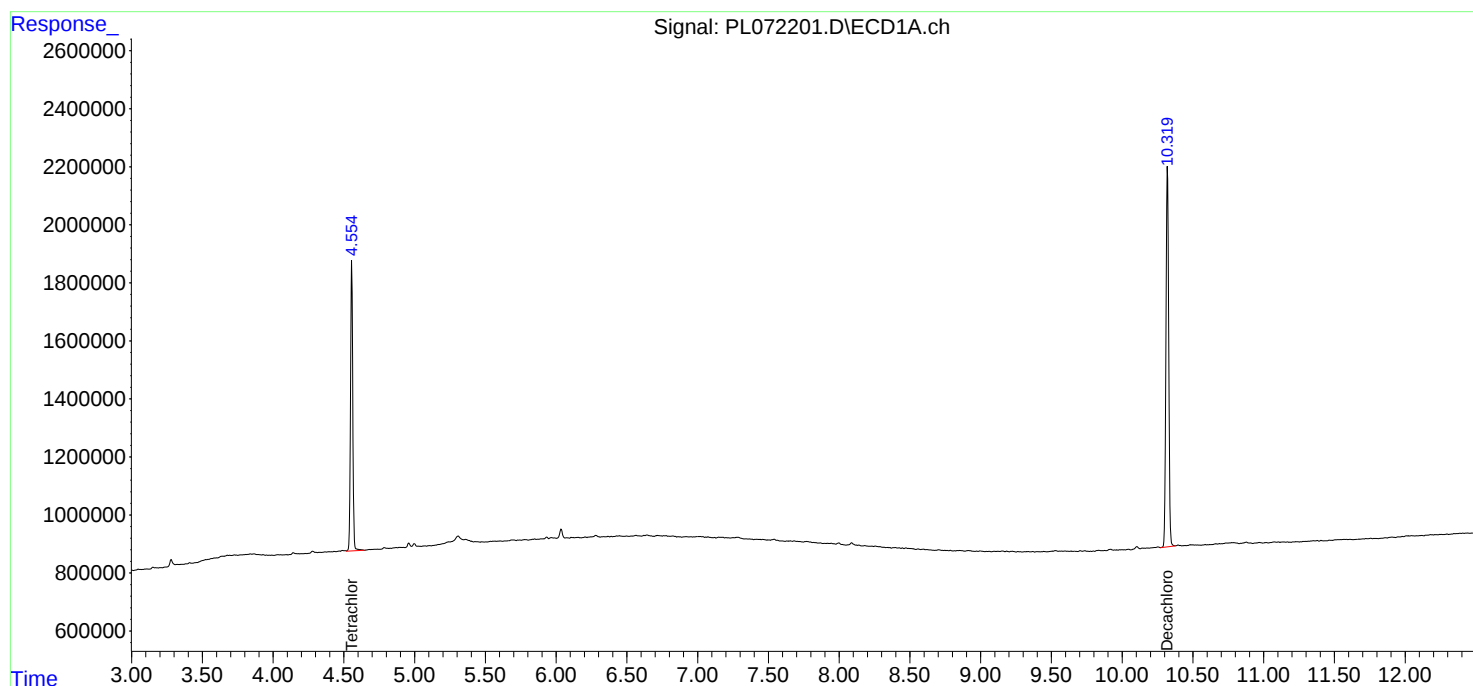


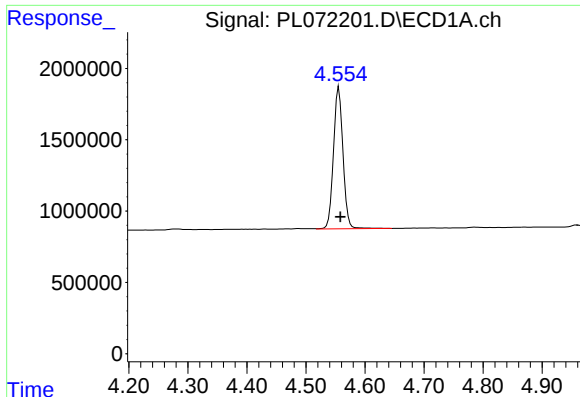

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 11141619
Conc: 20.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

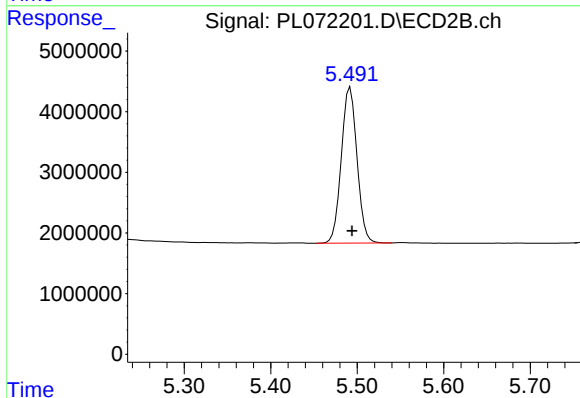


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 32174316
Conc: 19.81 ng/ml

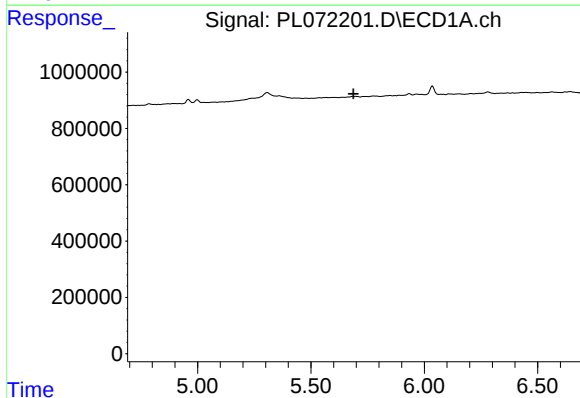


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.688 min
Response: 0
Conc: N.D.

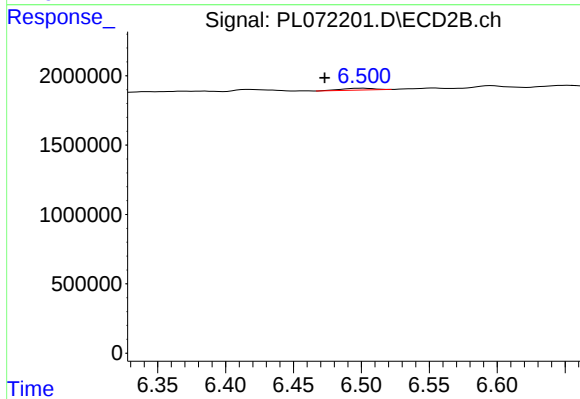

#3 gamma-BHC (Lindane)


R.T.: 6.501 min
Delta R.T.: 0.028 min
Response: 215893
Conc: 0.10 ng/ml

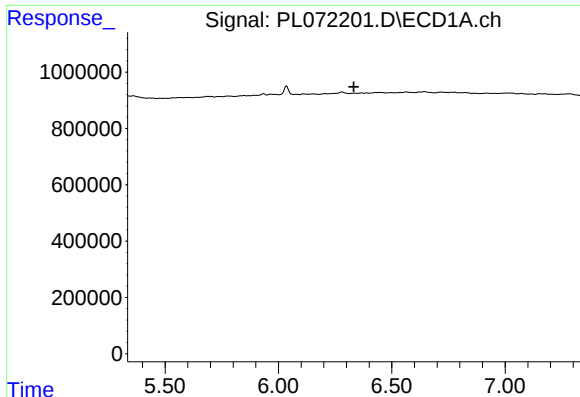

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

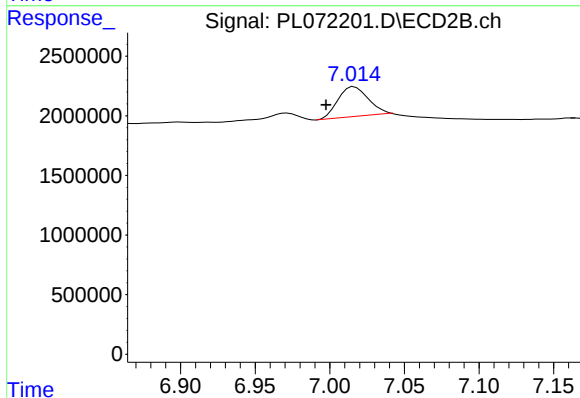


#7 delta-BHC

R.T.: 7.016 min
Delta R.T.: 0.019 min
Response: 3533276
Conc: 1.44 ng/ml

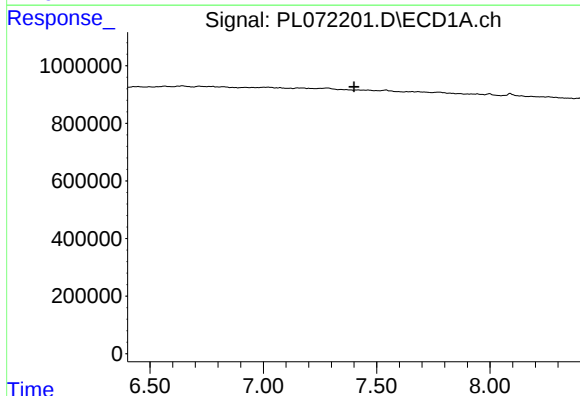


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

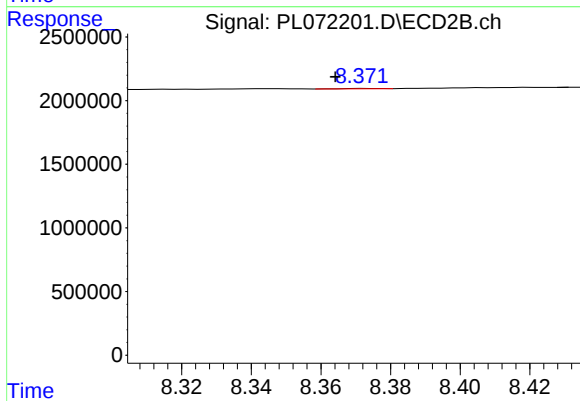

#9 Endosulfan I


R.T.: 8.372 min
Delta R.T.: 0.008 min
Response: 14997
Conc: 0.01 ng/ml

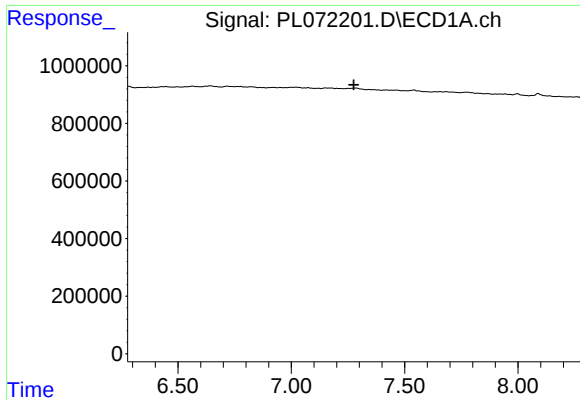

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

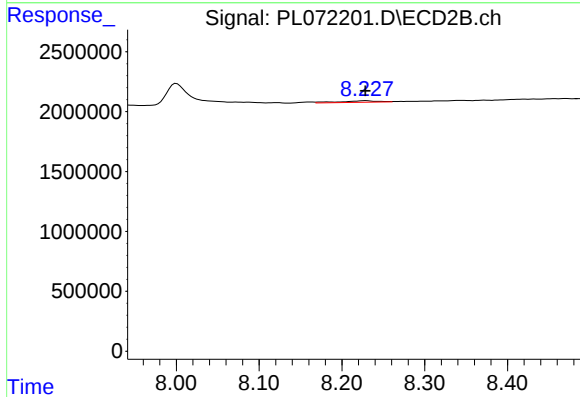


#10 gamma-Chlordane

R.T.: 8.228 min
Delta R.T.: 0.000 min
Response: 409165
Conc: 0.20 ng/ml

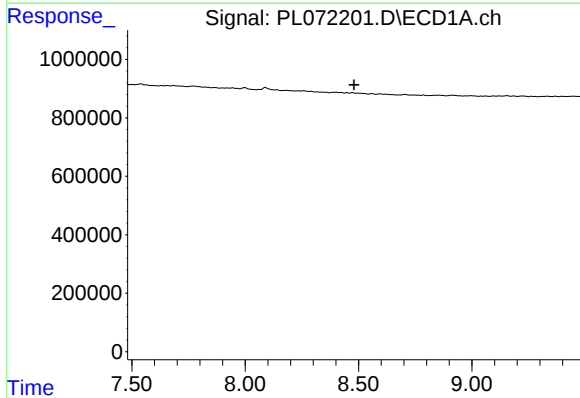


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

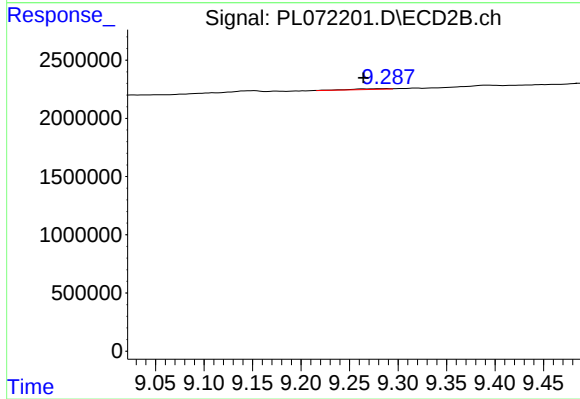

#18 Endrin aldehyde


R.T.: 9.288 min
Delta R.T.: 0.024 min
Response: 143377
Conc: 0.12 ng/ml

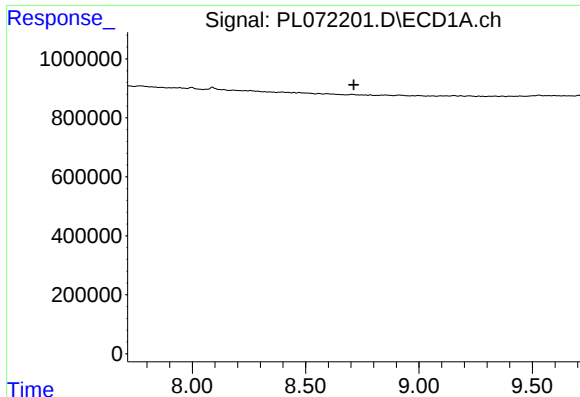

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

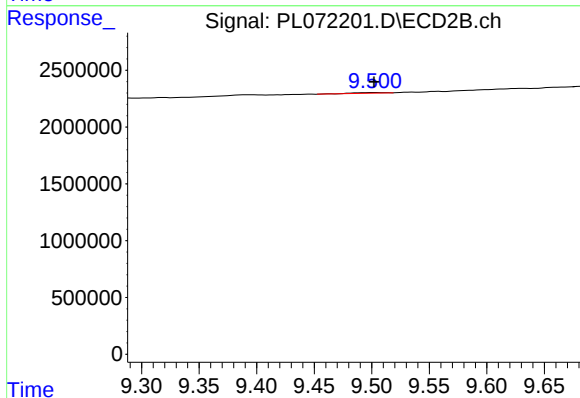


#19 Endosulfan Sulfate

R.T.: 9.502 min
Delta R.T.: 0.000 min
Response: 106179
Conc: 0.07 ng/ml

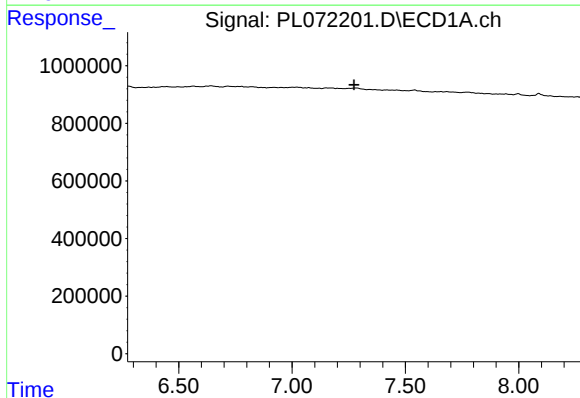


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

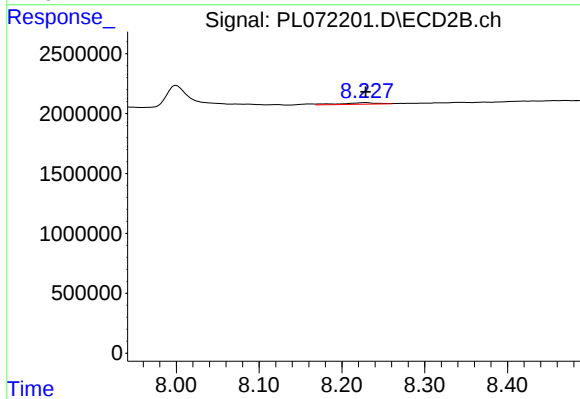

#25 Chlordane-3


R.T.: 8.228 min
Delta R.T.: 0.000 min
Response: 409165
Conc: 1.47 ng/ml

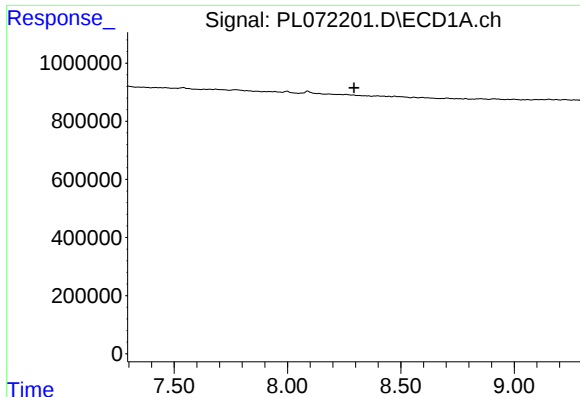

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

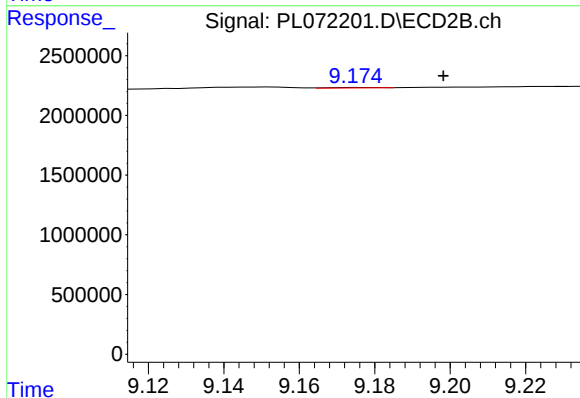


#27 Chlordane-5

R.T.: 9.176 min
Delta R.T.: -0.022 min
Response: 30931
Conc: 0.51 ng/ml

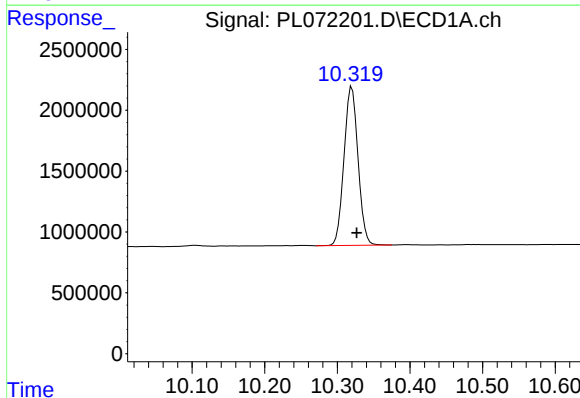

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: -0.006 min
Response: 17502589
Conc: 19.70 ng/ml

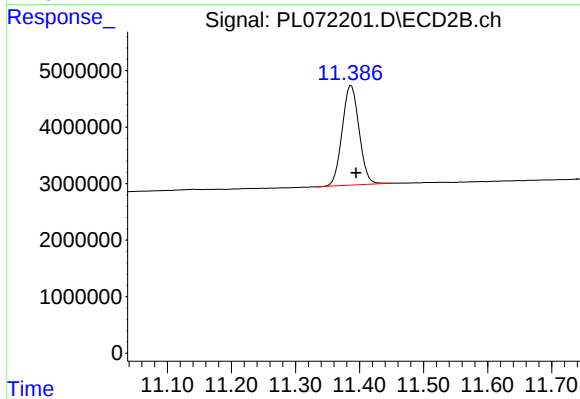

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: -0.008 min
Response: 32396126
Conc: 20.08 ng/ml