

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012422\
 Data File : PL072210.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2022 00:01
 Operator : AR\AJ
 Sample : PB142169TB
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 02:13:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.492	9818763	28646675	17.685	17.638
28)	SA Decachlor...	10.319	11.386	15786676	29034011	17.769	17.994
Target Compounds							
3)	MA gamma-BHC...	0.000	6.499f	0	48962	N.D.	0.022 #
7)	B delta-BHC	0.000	7.017f	0	1956100	N.D.	0.795 #
10)	B gamma-Chl...	0.000	8.224	0	31372	N.D.	0.016 #
14)	MA Endrin	0.000	8.916f	0	87633	N.D.	0.053 #
15)	B Endosulfa...	0.000	9.143	0	272005	N.D.	0.159 #
16)	A 4,4'-DDD	0.000	9.037	0	115890	N.D.	0.081 #
18)	B Endrin al...	0.000	9.290f	0	61410	N.D.	0.049 #
20)	A Methoxychlor	0.000	9.872f	0	61794	N.D.	0.075 #
21)	B Endrin ke...	0.000	9.993	0	62452	N.D.	0.038 #
22)	Mirex	0.000	10.489f	0	192581	N.D.	0.154 #
25)	Chlordane-3	0.000	8.224	0	31372	N.D.	0.113 #
27)	Chlordane-5	0.000	9.182f	0	36711	N.D.	0.602 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012422\
Data File : PL072210.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2022 00:01
Operator : AR\AJ
Sample : PB142169TB
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 02:13:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

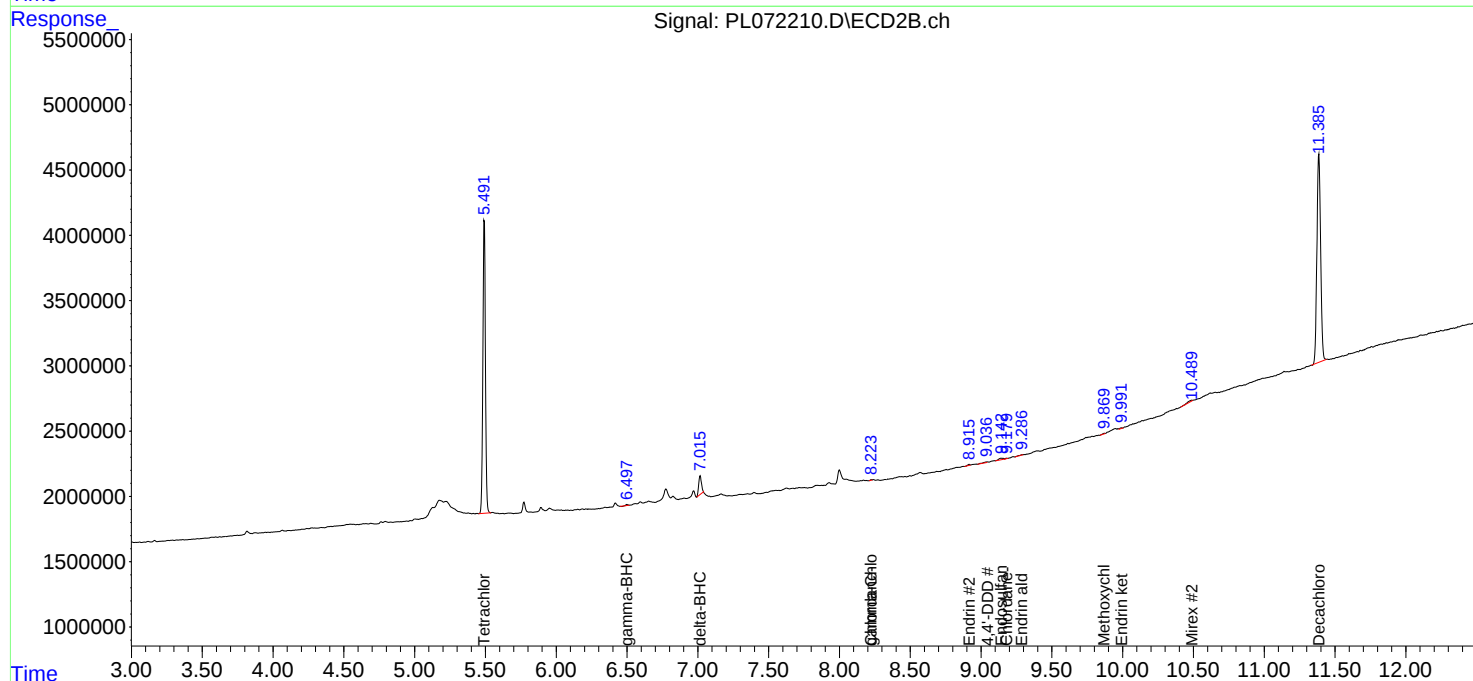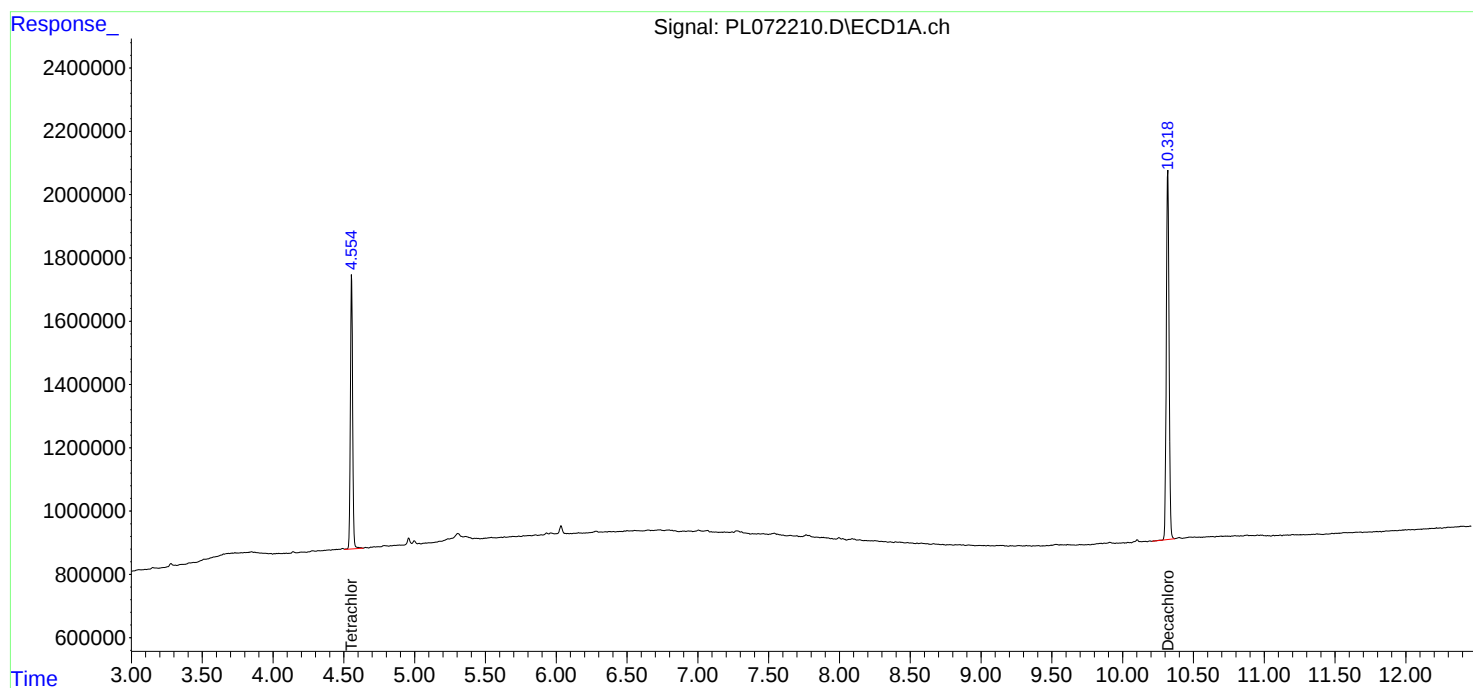


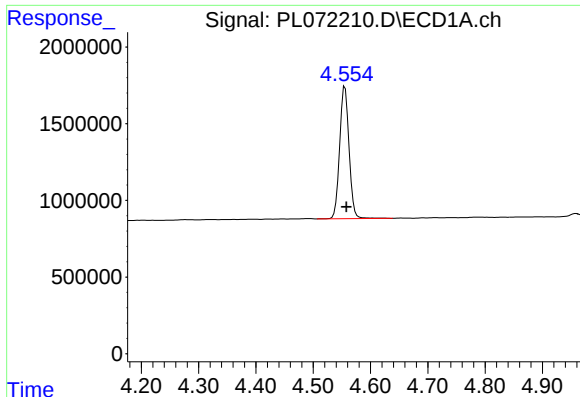

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 9818763
Conc: 17.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

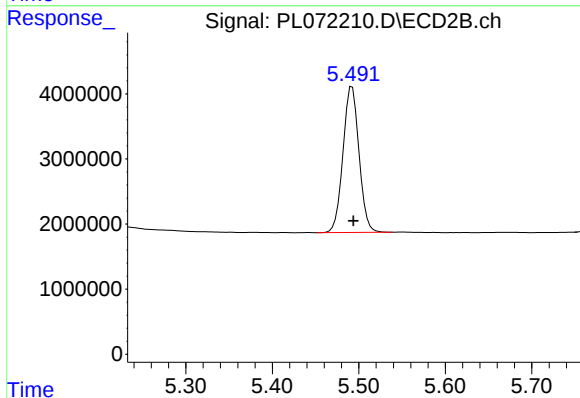


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 28646675
Conc: 17.64 ng/ml

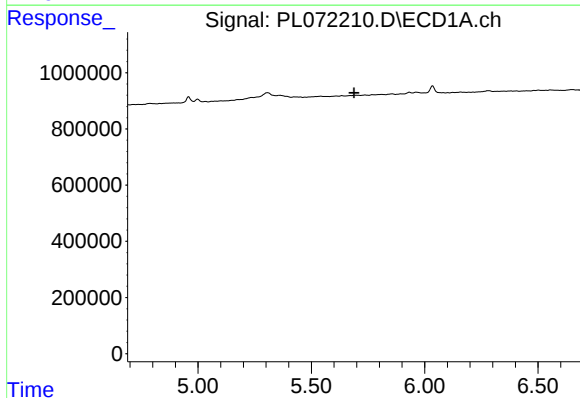


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.688 min
Response: 0
Conc: N.D.

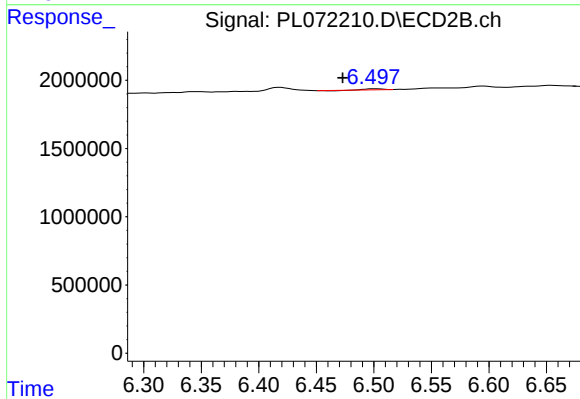

#3 gamma-BHC (Lindane)


R.T.: 6.499 min
Delta R.T.: 0.026 min
Response: 48962
Conc: 0.02 ng/ml

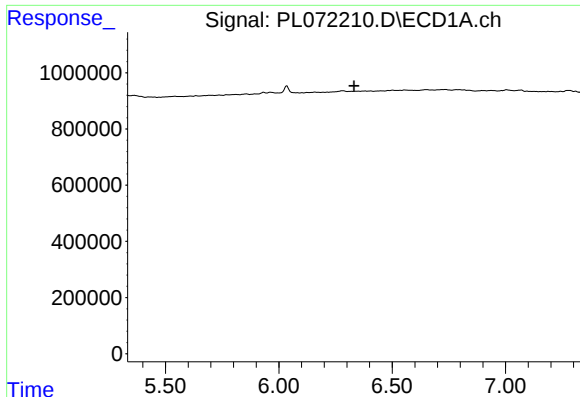

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

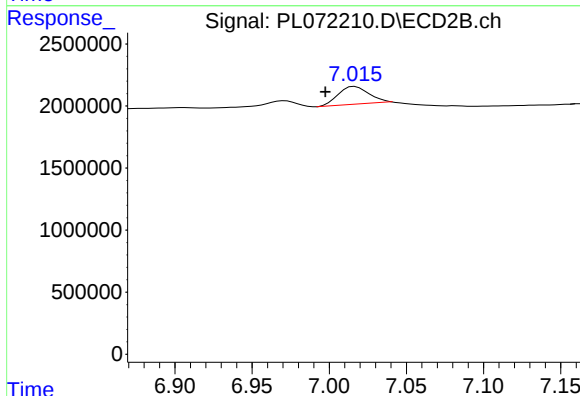


#7 delta-BHC

R.T.: 7.017 min
Delta R.T.: 0.019 min
Response: 1956100
Conc: 0.80 ng/ml

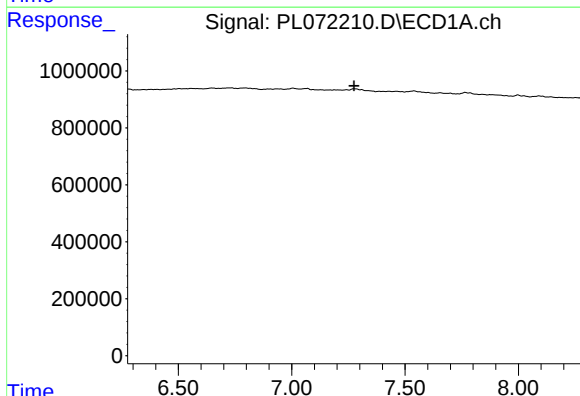


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

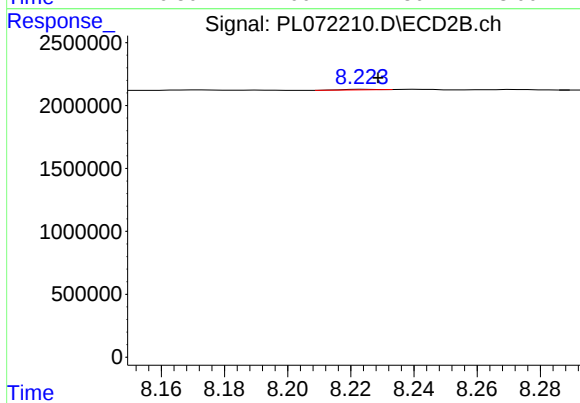

#10 gamma-Chlordane


R.T.: 8.224 min
Delta R.T.: -0.004 min
Response: 31372
Conc: 0.02 ng/ml

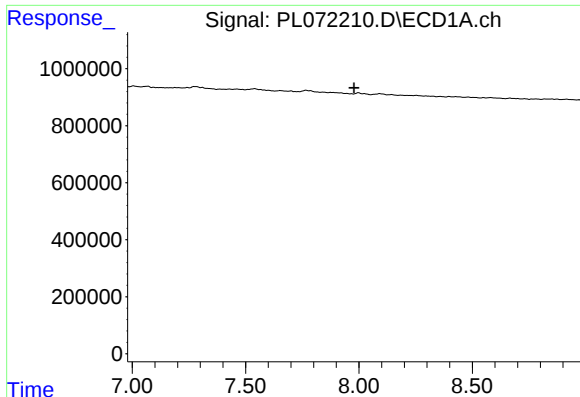

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 7.978 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

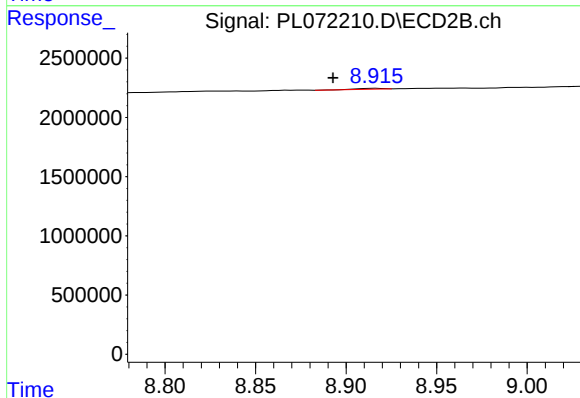


#14 Endrin

R.T.: 8.916 min
Delta R.T.: 0.024 min
Response: 87633
Conc: 0.05 ng/ml

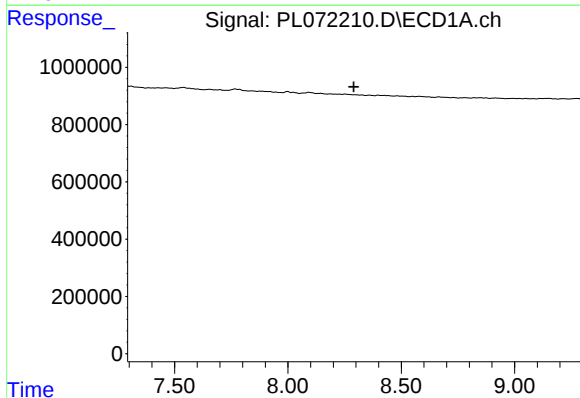


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

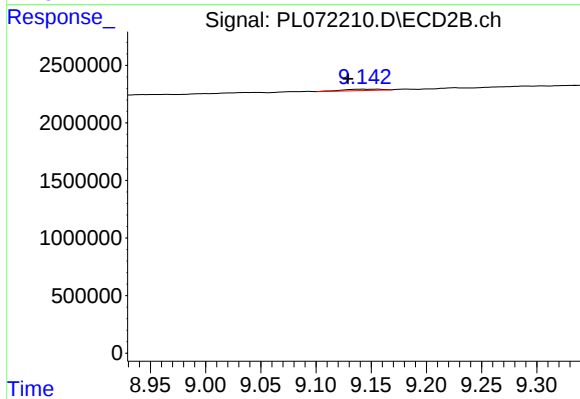

#15 Endosulfan II


R.T.: 9.143 min
Delta R.T.: 0.014 min
Response: 272005
Conc: 0.16 ng/ml

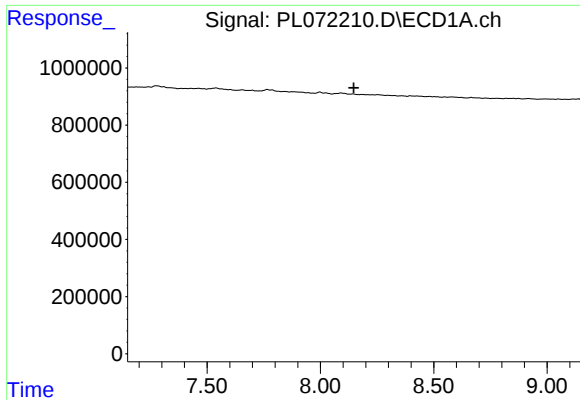

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

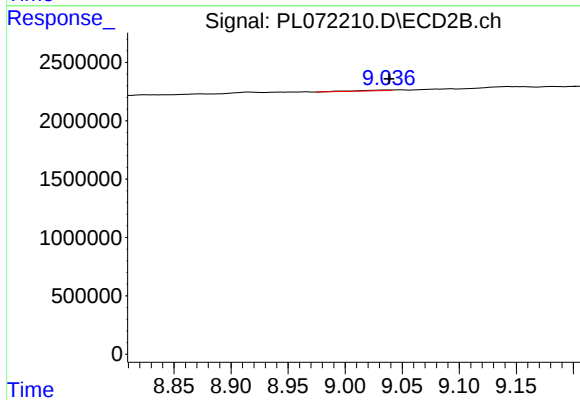


#16 4,4'-DDD

R.T.: 9.037 min
Delta R.T.: -0.002 min
Response: 115890
Conc: 0.08 ng/ml

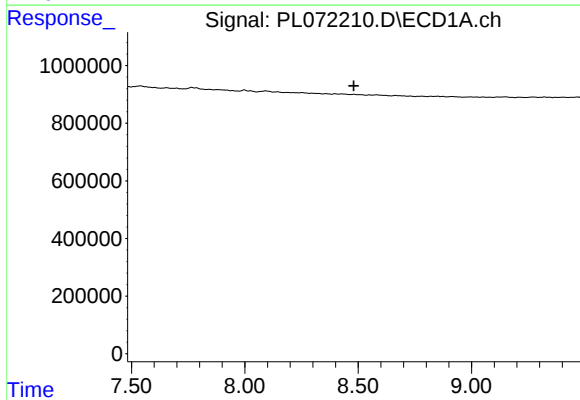


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

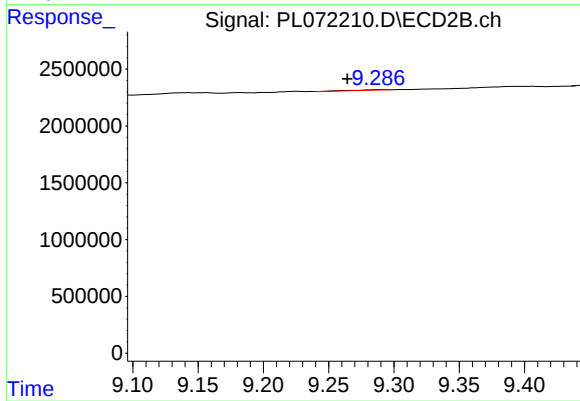

#18 Endrin aldehyde


R.T.: 9.290 min
Delta R.T.: 0.026 min
Response: 61410
Conc: 0.05 ng/ml

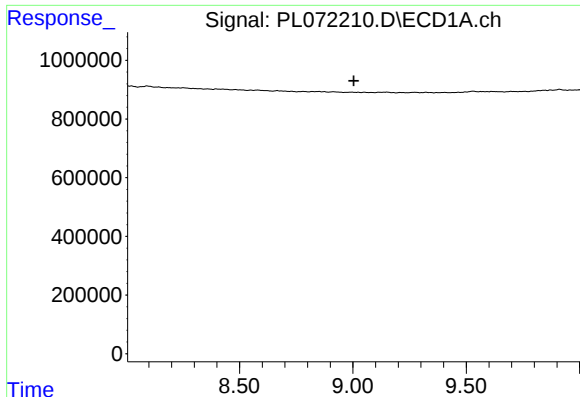

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

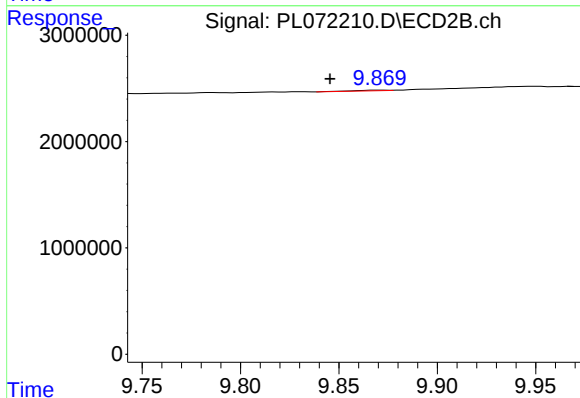


#20 Methoxychlor

R.T.: 9.872 min
Delta R.T.: 0.026 min
Response: 61794
Conc: 0.07 ng/ml

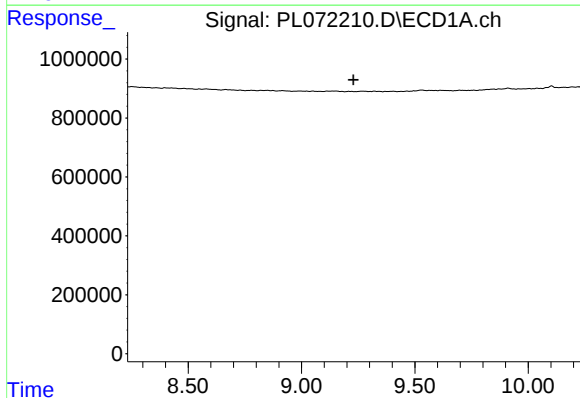


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.229 min
Response: 0
Conc: N.D.

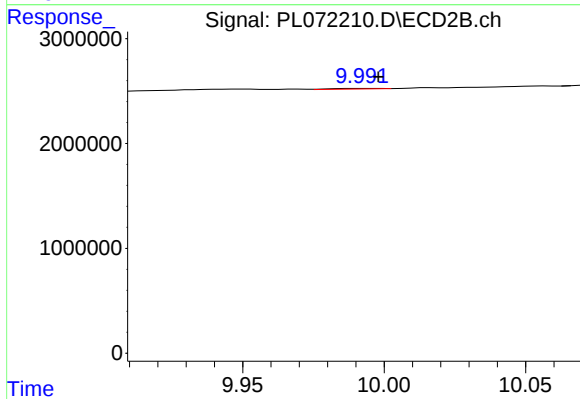

#21 Endrin ketone


R.T.: 9.993 min
Delta R.T.: -0.005 min
Response: 62452
Conc: 0.04 ng/ml

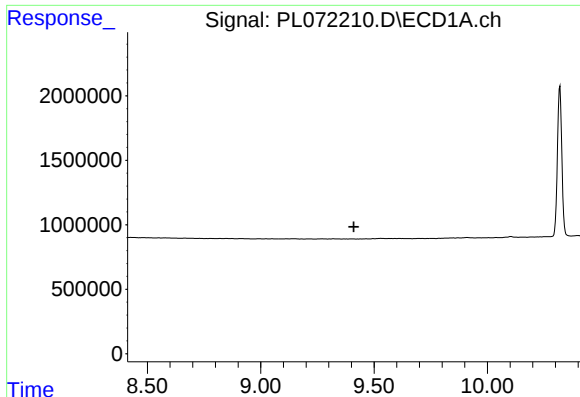

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

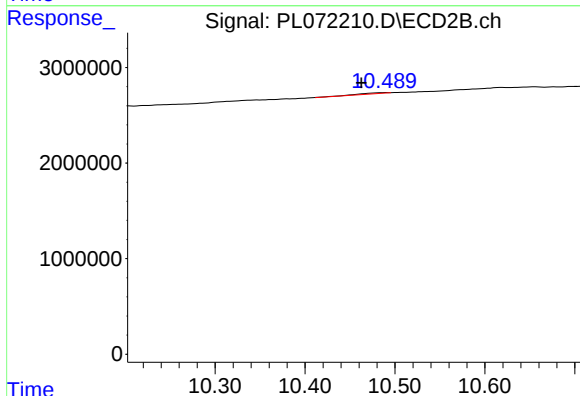


#22 Mirex

R.T.: 10.489 min
Delta R.T.: 0.026 min
Response: 192581
Conc: 0.15 ng/ml

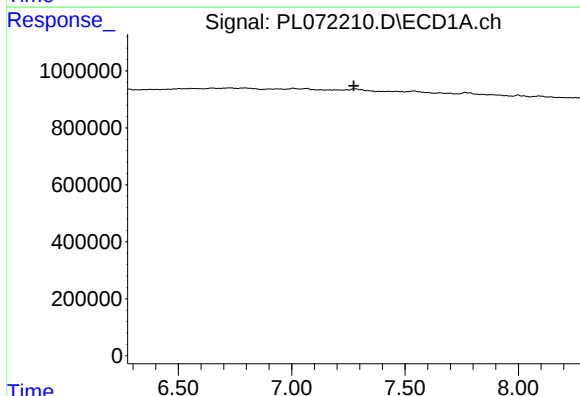


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

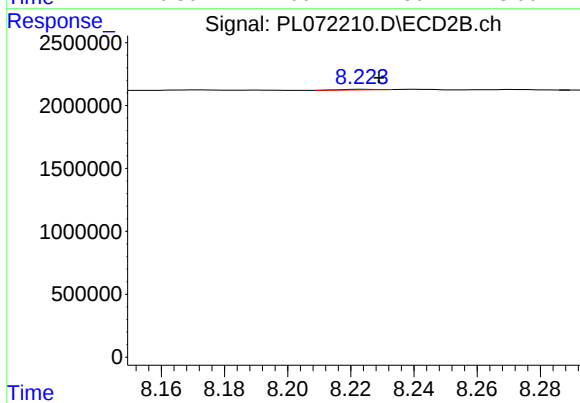

#25 Chlordane-3


R.T.: 8.224 min
Delta R.T.: -0.005 min
Response: 31372
Conc: 0.11 ng/ml

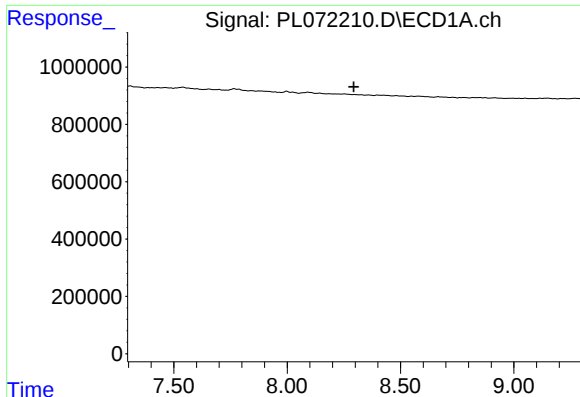

#27 Chlorine-5


R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

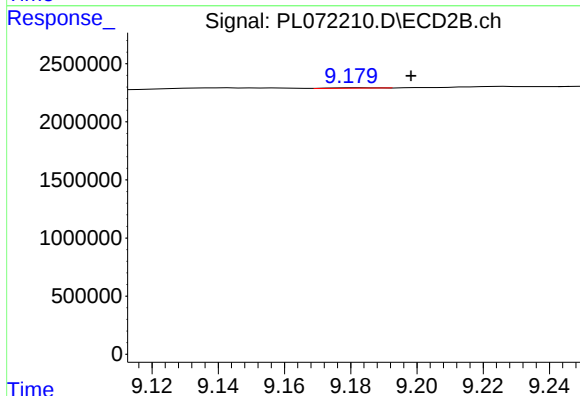


#27 Chlorine-5

R.T.: 9.182 min
Delta R.T.: -0.016 min
Response: 36711
Conc: 0.60 ng/ml

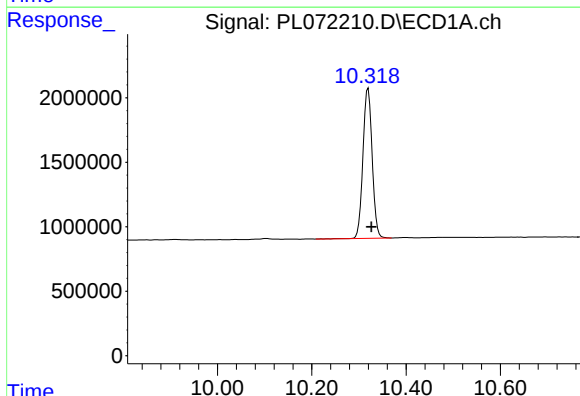

#28 Decachlorobiphenyl

R.T.: 10.319 min
Delta R.T.: -0.007 min
Response: 15786676
Conc: 17.77 ng/ml

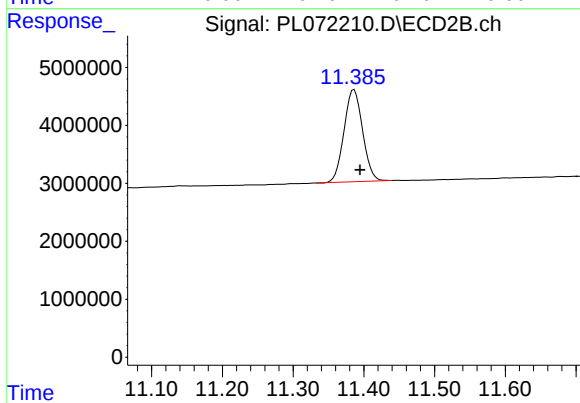

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.008 min
Response: 29034011
Conc: 17.99 ng/ml