

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012422\
 Data File : PL072214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2022 01:07
 Operator : AR\AJ
 Sample : N1235-02
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 02:15:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.493	10672376	32905375	19.223	20.260
28)	SA Decachlor...	10.321	11.388	16909427	30918836	19.033	19.163
Target Compounds							
2)	A alpha-BHC	0.000	6.055f	0	470852	N.D.	0.195 #
5)	MB Aldrin	0.000	7.511f	0	264231	N.D.	0.119 #
7)	B delta-BHC	0.000	7.019f	0	1558473	N.D.	0.633 #
9)	A Endosulfan I	0.000	8.346f	0	152184	N.D.	0.084 #
10)	B gamma-Chl...	0.000	8.226	0	319966	N.D.	0.158 #
15)	B Endosulfa...	0.000	9.149f	0	1199582	N.D.	0.700 #
17)	MA 4,4'-DDT	0.000	9.355	0	110987	N.D.	0.070 #
19)	B Endosulfa...	0.000	9.487	0	11482	N.D.	0.007 #
22)	Mirex	0.000	10.478f	0	198198	N.D.	0.159 #
25)	Chlordane-3	0.000	8.226	0	319966	N.D.	1.152 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012422\
Data File : PL072214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2022 01:07
Operator : AR\AJ
Sample : N1235-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 02:15:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

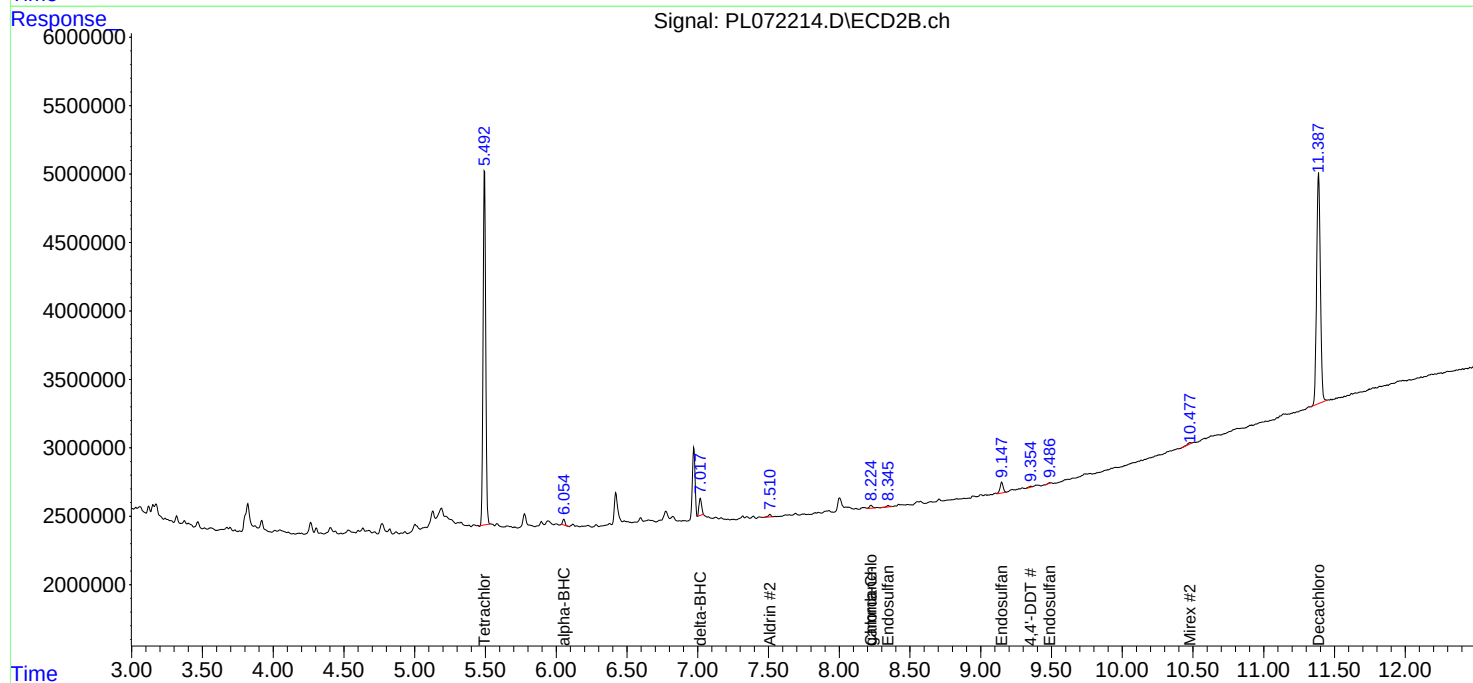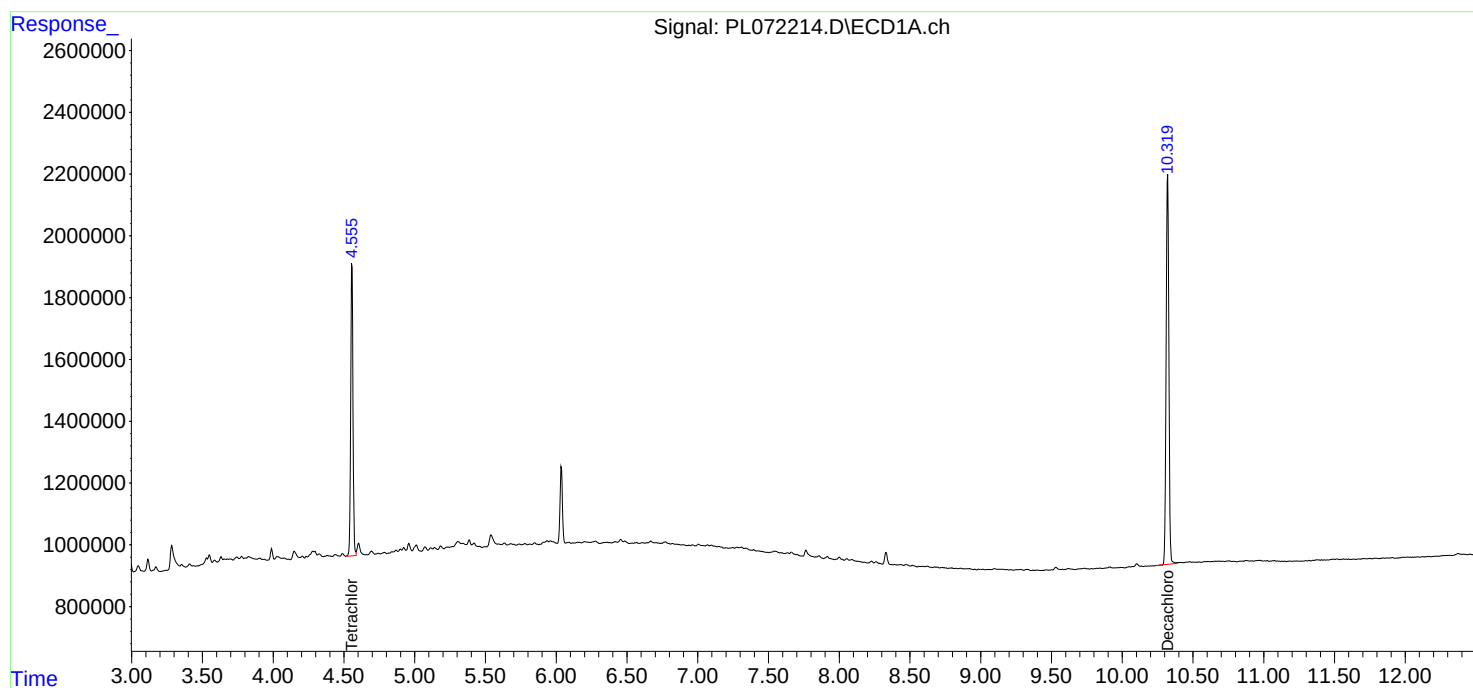


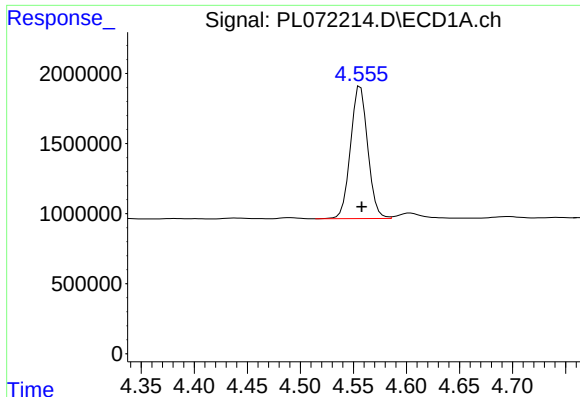

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: -0.001 min
Response: 10672376
Conc: 19.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

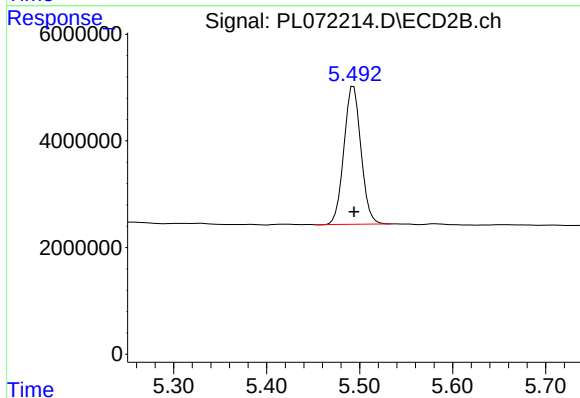


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 32905375
Conc: 20.26 ng/ml

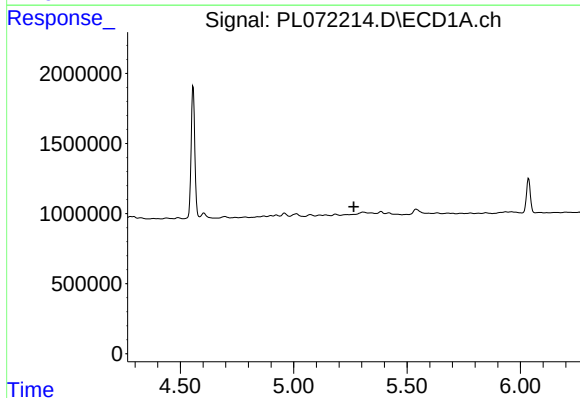


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.265 min
Response: 0
Conc: N.D.

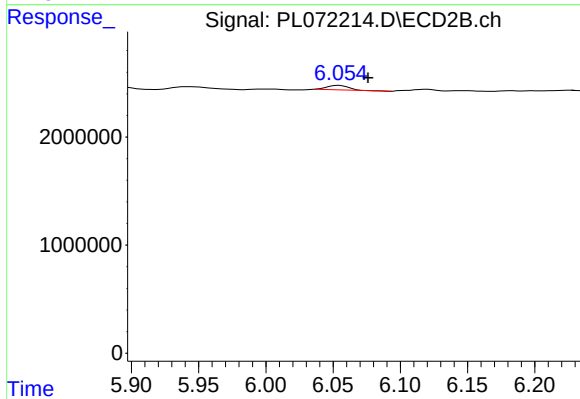

#2 alpha-BHC


R.T.: 6.055 min
Delta R.T.: -0.021 min
Response: 470852
Conc: 0.20 ng/ml

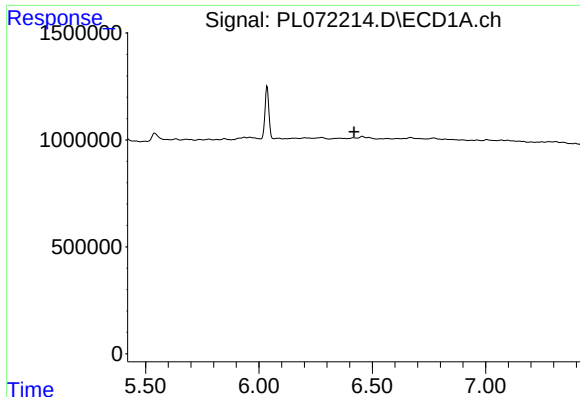

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

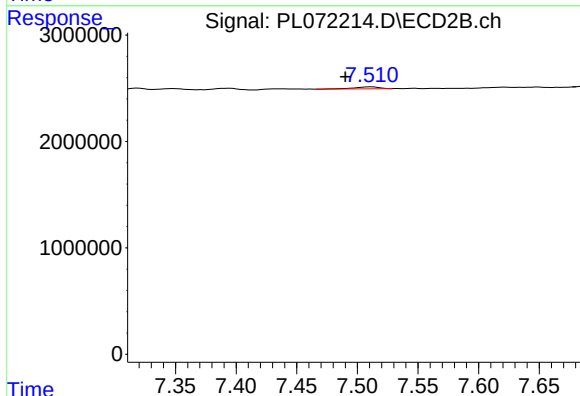


#5 Aldrin

R.T.: 7.511 min
Delta R.T.: 0.021 min
Response: 264231
Conc: 0.12 ng/ml

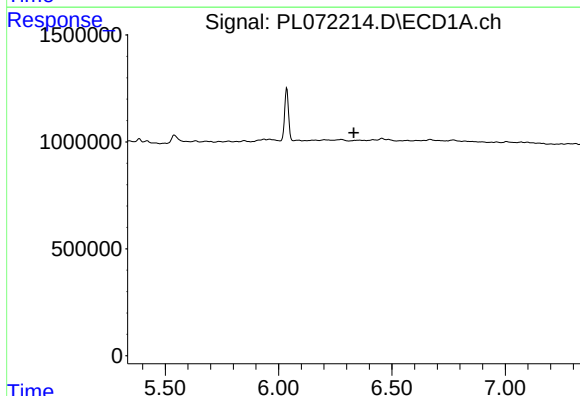


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

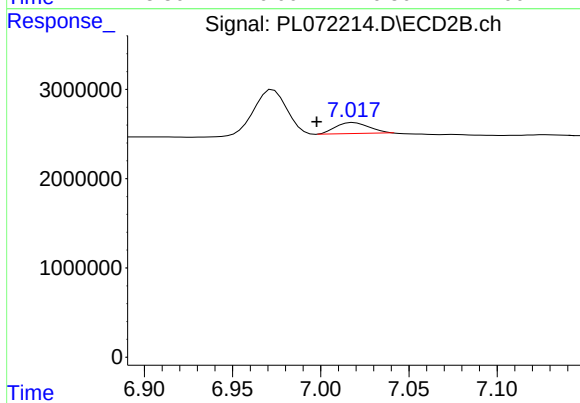

#7 delta-BHC


R.T.: 7.019 min
Delta R.T.: 0.021 min
Response: 1558473
Conc: 0.63 ng/ml

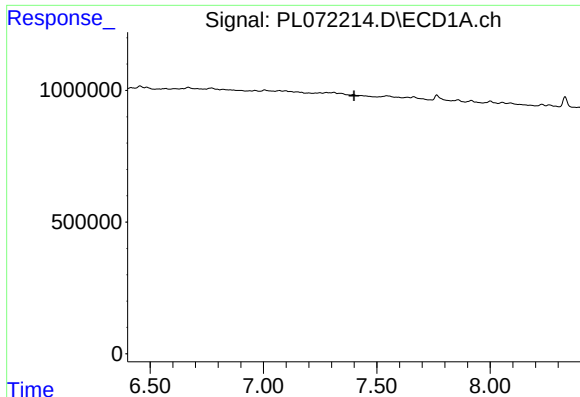

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

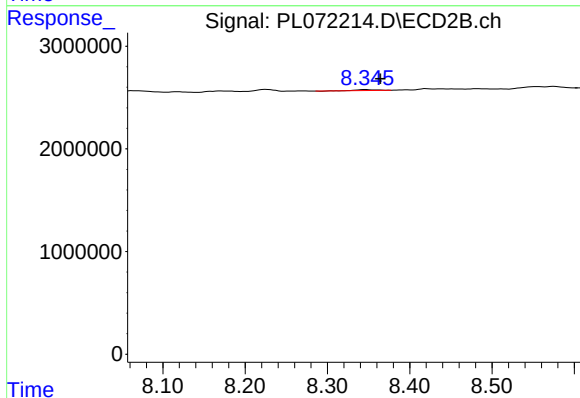


#9 Endosulfan I

R.T.: 8.346 min
Delta R.T.: -0.018 min
Response: 152184
Conc: 0.08 ng/ml

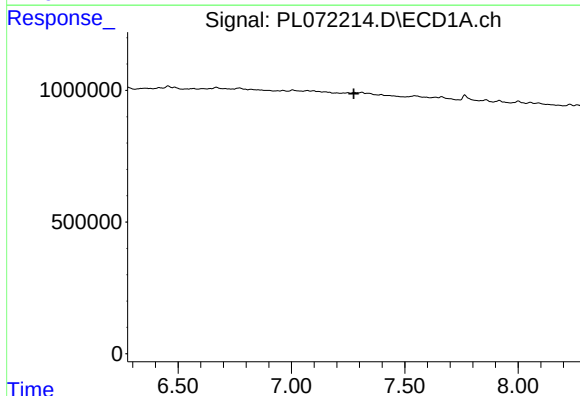


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

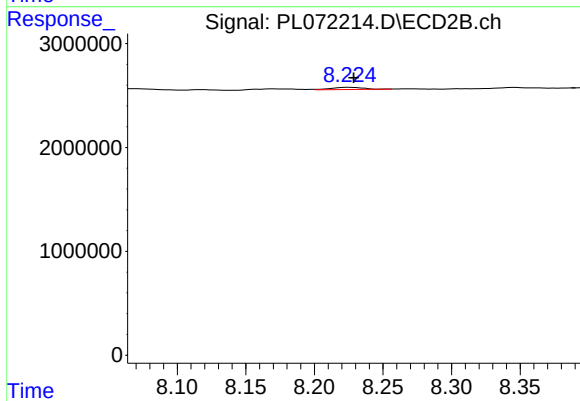

#10 gamma-Chlordane


R.T.: 8.226 min
Delta R.T.: -0.003 min
Response: 319966
Conc: 0.16 ng/ml

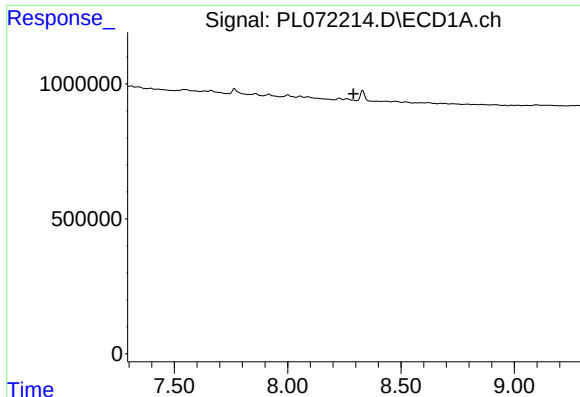

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

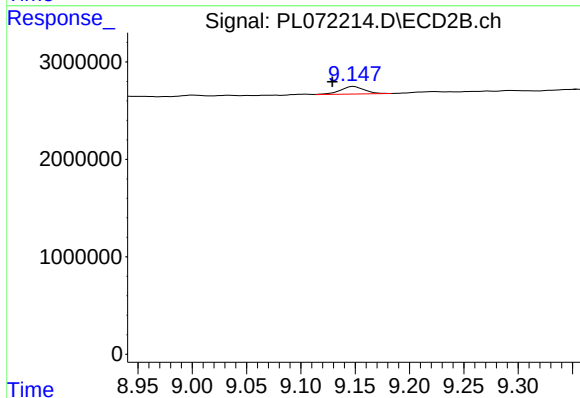


#15 Endosulfan II

R.T.: 9.149 min
Delta R.T.: 0.020 min
Response: 1199582
Conc: 0.70 ng/ml

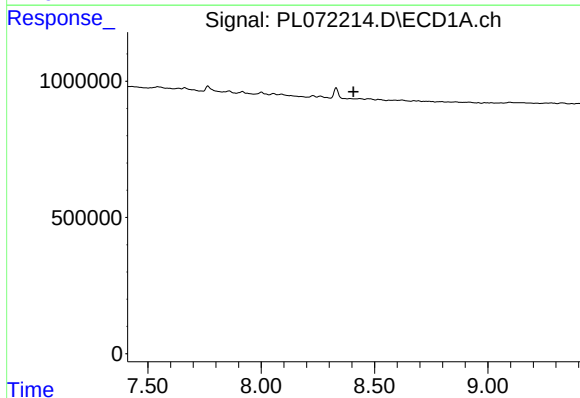


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

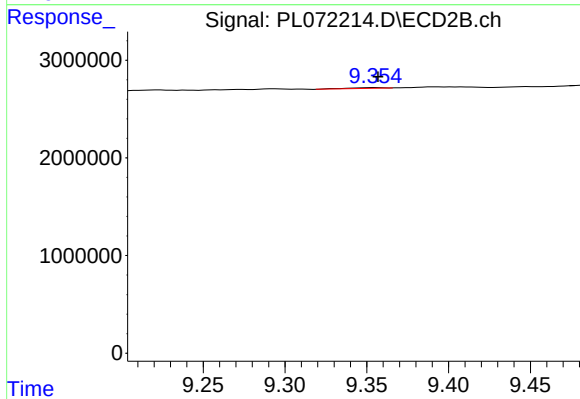

#17 4,4'-DDT


R.T.: 9.355 min
Delta R.T.: -0.002 min
Response: 110987
Conc: 0.07 ng/ml

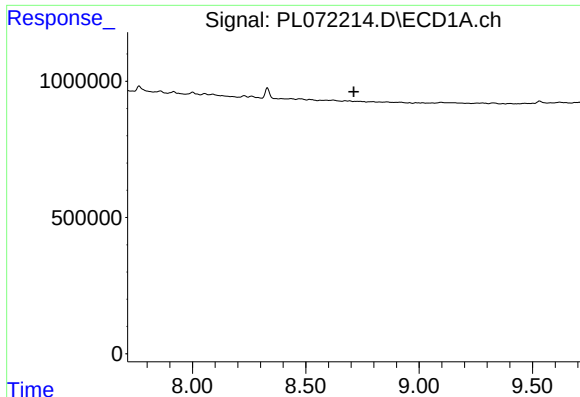

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

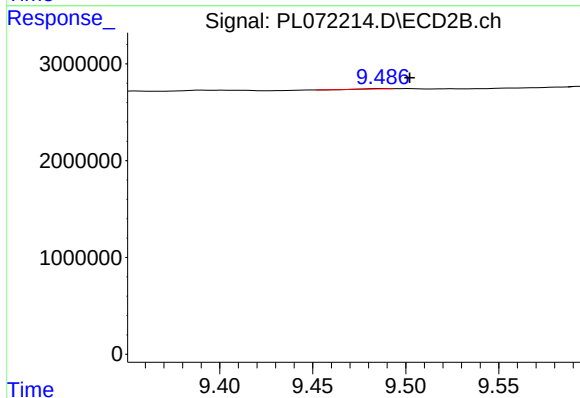


#19 Endosulfan Sulfate

R.T.: 9.487 min
Delta R.T.: -0.015 min
Response: 11482
Conc: 0.01 ng/ml

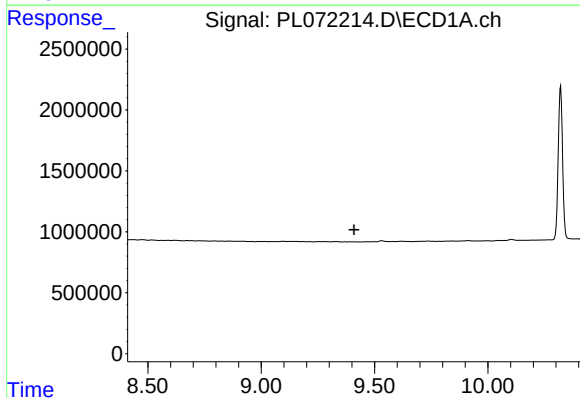


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 9.410 min
Response: 0
Conc: N.D.

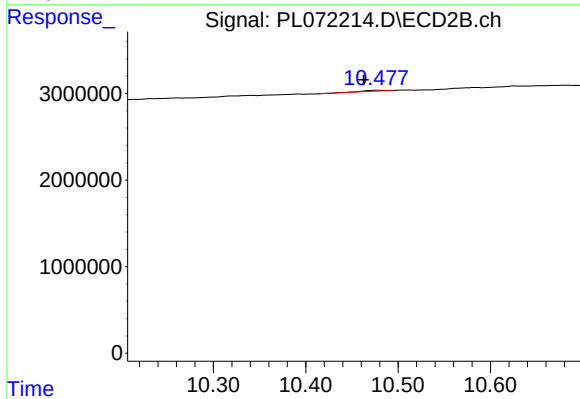

#22 Mirex


R.T.: 10.478 min
Delta R.T.: 0.015 min
Response: 198198
Conc: 0.16 ng/ml

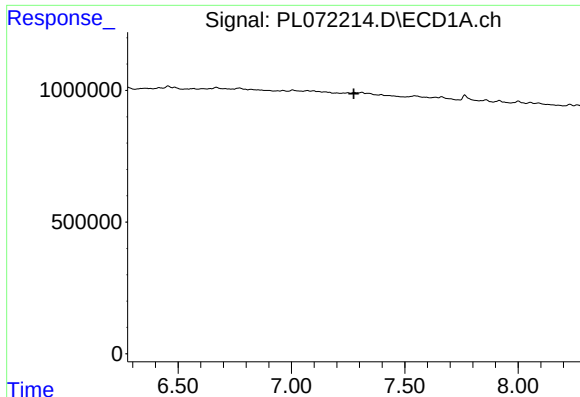

#25 Chlorine-3


R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

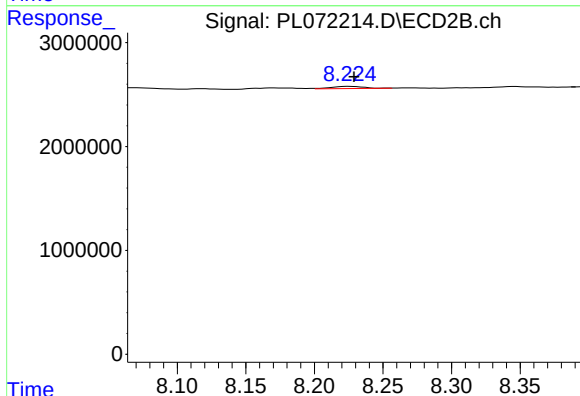


#25 Chlorine-3

R.T.: 8.226 min
Delta R.T.: -0.003 min
Response: 319966
Conc: 1.15 ng/ml

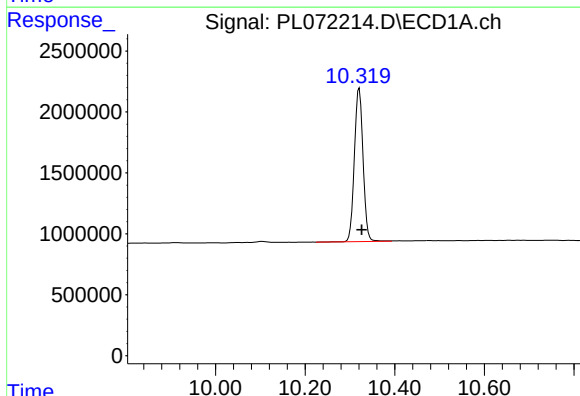

#28 Decachlorobiphenyl

R.T.: 10.321 min
Delta R.T.: -0.006 min
Response: 16909427
Conc: 19.03 ng/ml

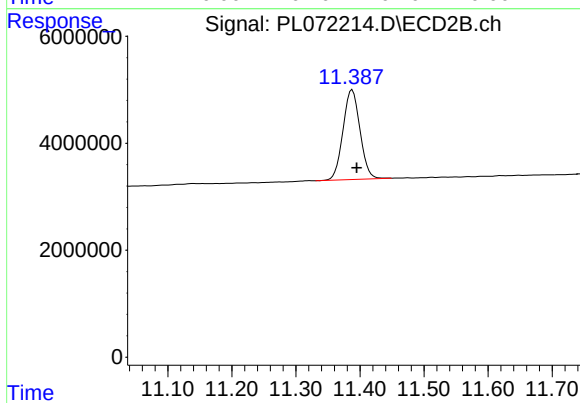

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: -0.007 min
Response: 30918836
Conc: 19.16 ng/ml