

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012422\
 Data File : PL072183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2022 14:21
 Operator : AR\AJ
 Sample : N1217-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-242

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/25/2022
 Supervised By : Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 02:03:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.566	5.496	6219088	13871606	11.202m	8.541m
2) SA Decachlor...	10.321	11.389	11679433	20852807	13.146m	12.924

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012422\
Data File : PL072183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2022 14:21
Operator : AR\AJ
Sample : N1217-08
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VNJ-242


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/25/2022
Supervised By : Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 02:03:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

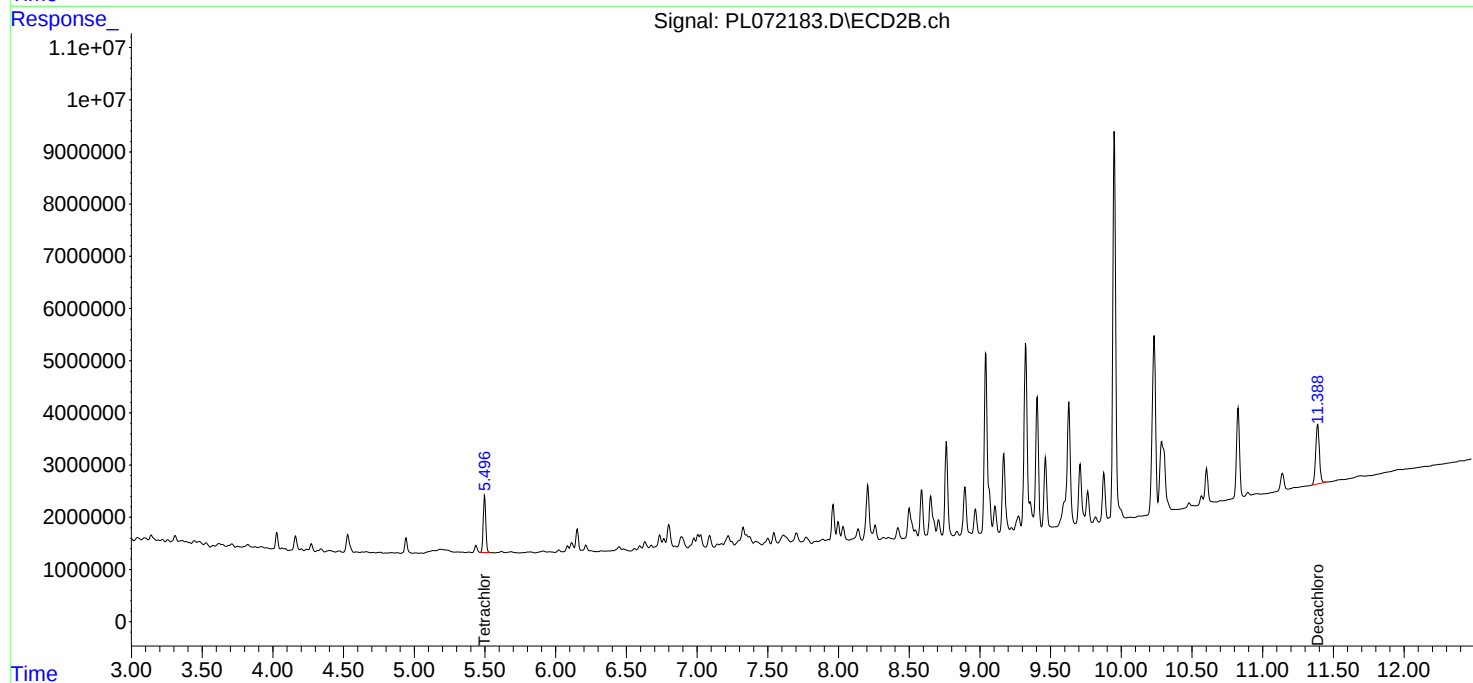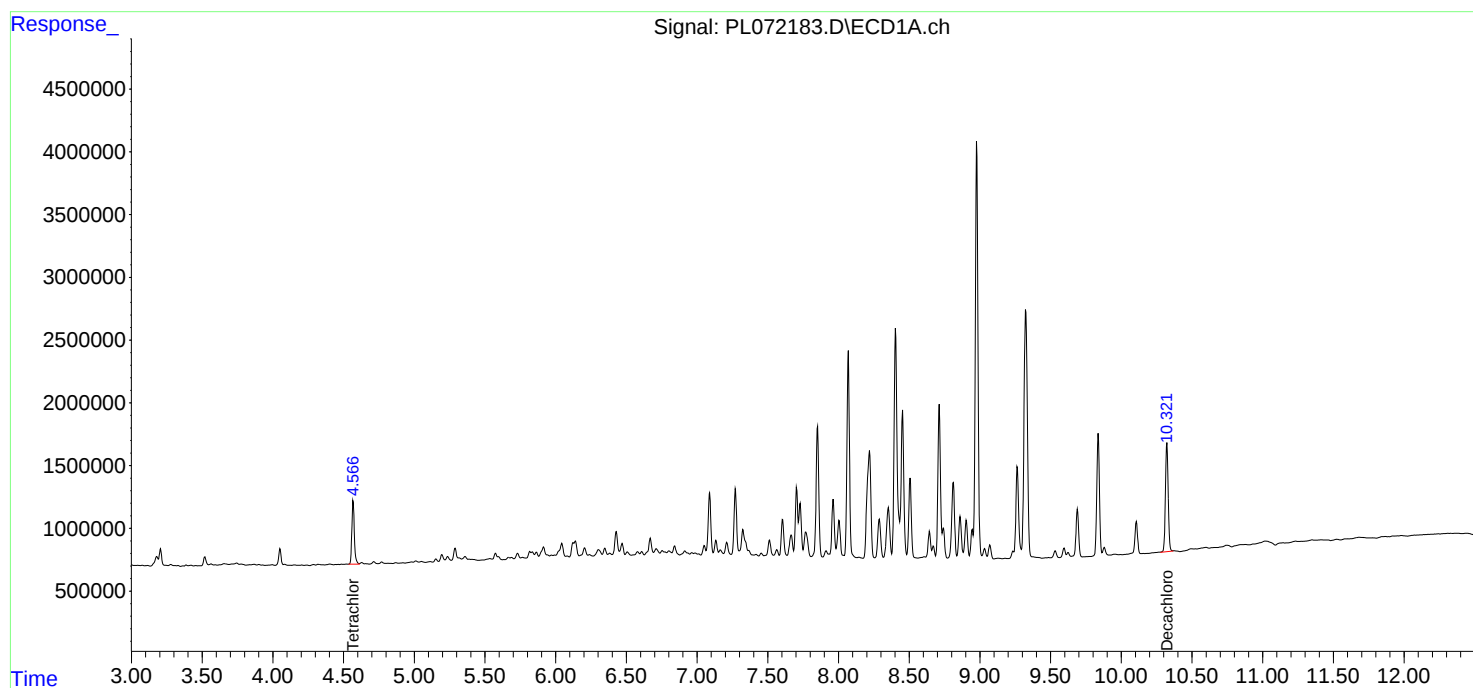

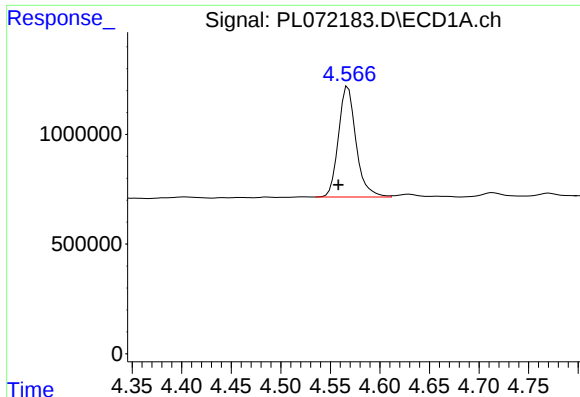


#1 Tetrachloro-m-xylene

R.T.: 4.566 min
Delta R.T.: 0.008 min
Response: 6219088
Conc: 11.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-242


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/25/2022
Supervised By :Ankita Jodhani 01/25/2022

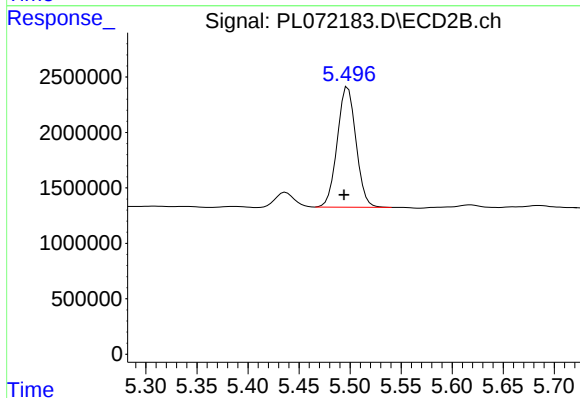


#1 Tetrachloro-m-xylene

R.T.: 5.496 min
Delta R.T.: 0.002 min
Response: 13871606
Conc: 8.54 ng/ml m

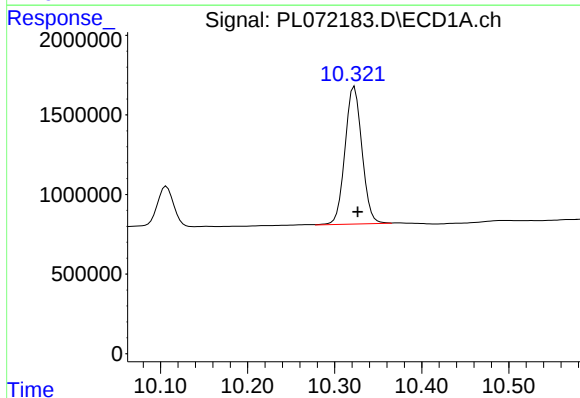

#28 Decachlorobiphenyl

R.T.: 10.321 min
Delta R.T.: -0.005 min
Response: 11679433
Conc: 13.15 ng/ml m

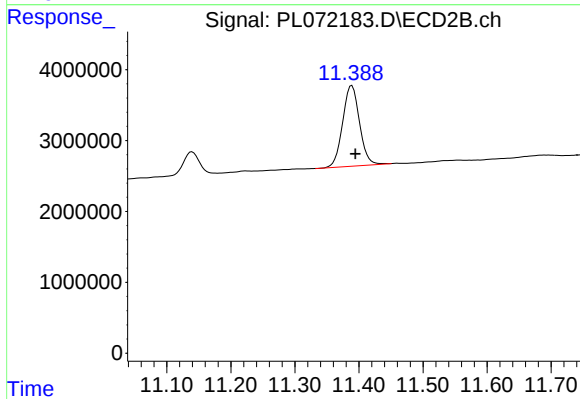

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: -0.006 min
Response: 20852807
Conc: 12.92 ng/ml