

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012422\
 Data File : PL072205.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2022 22:24
 Operator : AR\AJ
 Sample : N1210-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20220027-KEANSBURG-1-COMP-SPLP-LEACHATE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/25/2022
 Supervised By :Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 02:10:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.556	5.492	11470163	34592720	20.660	21.299
2) SA Decachlor...	10.318	11.387	15257099	28314229	17.173m	17.548

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012422\
Data File : PL072205.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2022 22:24
Operator : AR\AJ
Sample : N1210-06
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
20220027-KEANSBURG-1-COMP-SPLP-LEACHATE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/25/2022
Supervised By : Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 02:10:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

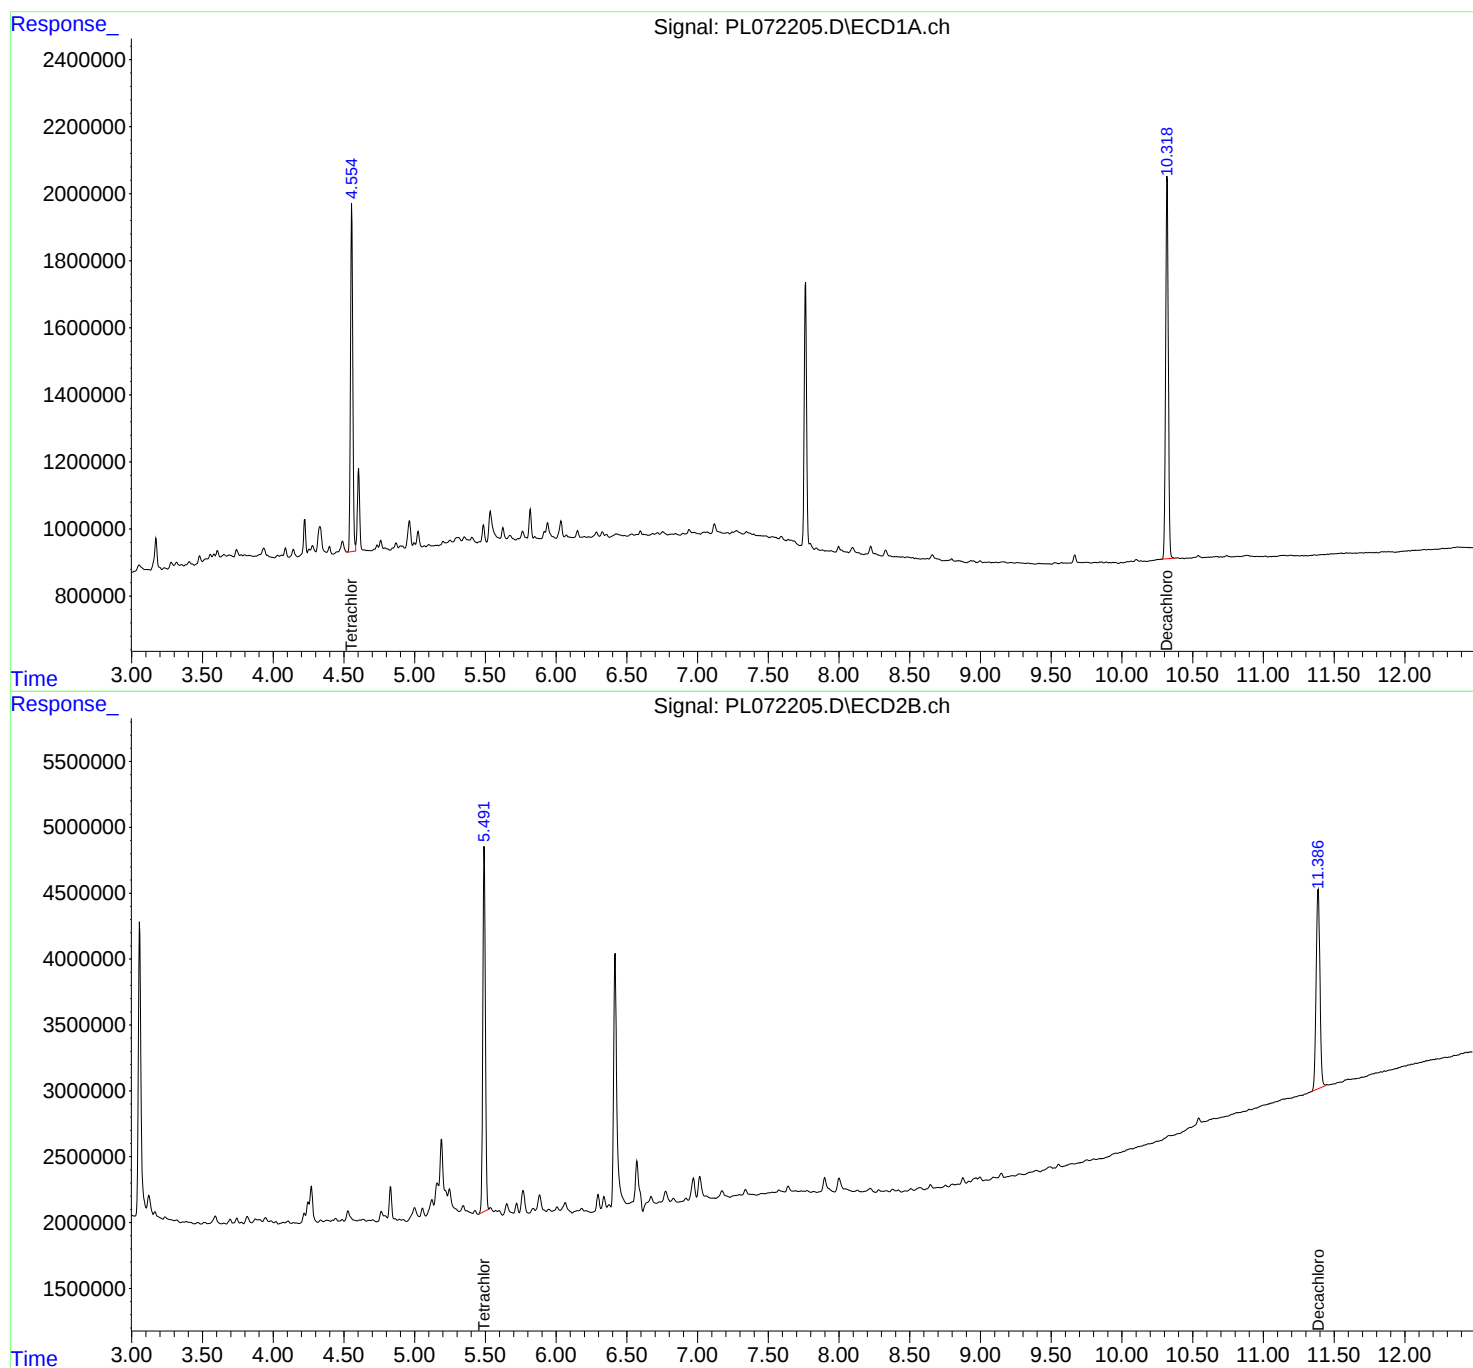

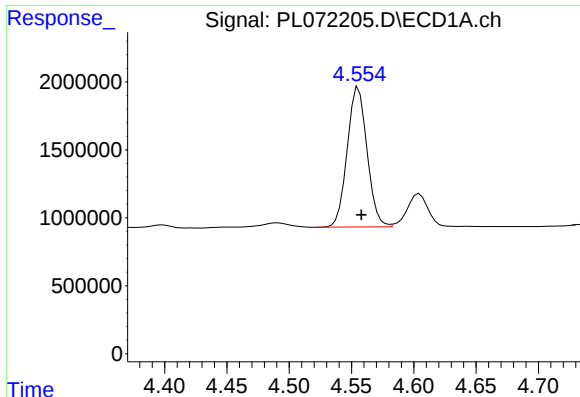


#1 Tetrachloro-m-xylene

R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 11470163
Conc: 20.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
20220027-KEANSBURG-1-COMP-SPLP-LEACHATE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/25/2022
Supervised By :Ankita Jodhani 01/25/2022

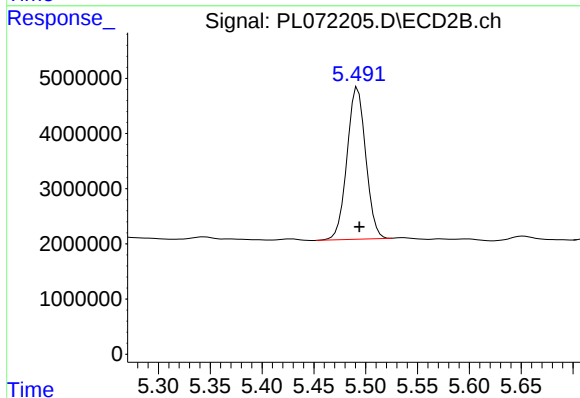


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 34592720
Conc: 21.30 ng/ml

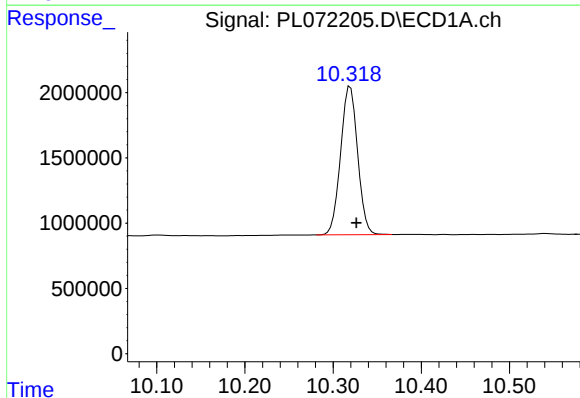

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.008 min
Response: 15257099
Conc: 17.17 ng/ml m

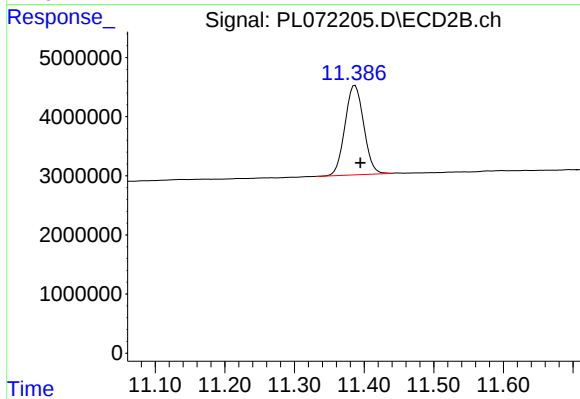

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: -0.008 min
Response: 28314229
Conc: 17.55 ng/ml