

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012424\
 Data File : PL087924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2024 10:04
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 00:59:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 03:17:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	2.673	123.3E6	66423830	41.173	54.835 #
28)	SA Decachlor...	8.981	7.859	124.3E6	58162750	43.638	45.912
Target Compounds							
23)	Chlordane-1	4.589	3.675	53788193	19314950	402.981	413.259
24)	Chlordane-2	5.123	4.257	60602296	23205036	410.951	414.756
25)	Chlordane-3	5.838	4.891	229.2E6	67931729	411.990	429.251
26)	Chlordane-4	5.921	4.953	281.5E6	70933944	406.996	415.163
27)	Chlordane-5	6.772	5.627	45471467	19916872	403.214m	423.117



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012424\
Data File : PL087924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2024 10:04
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 00:59:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:17:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

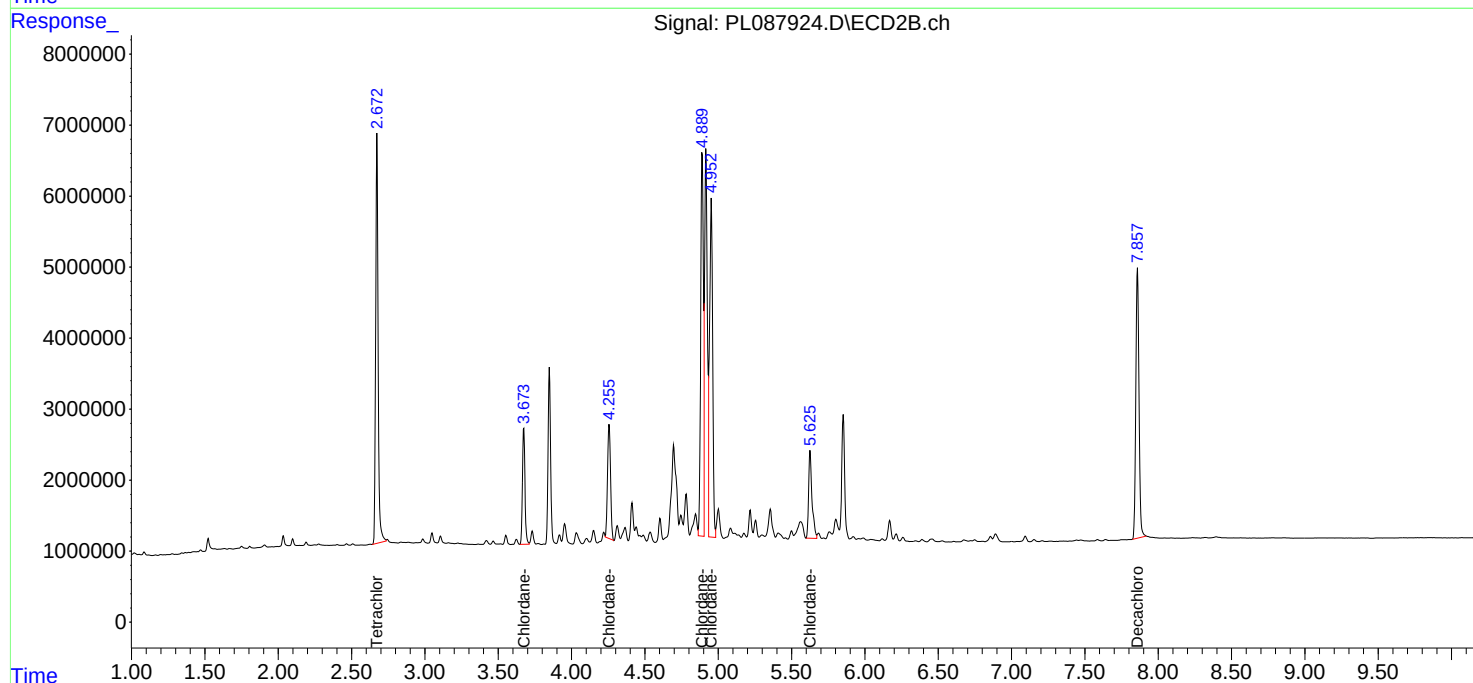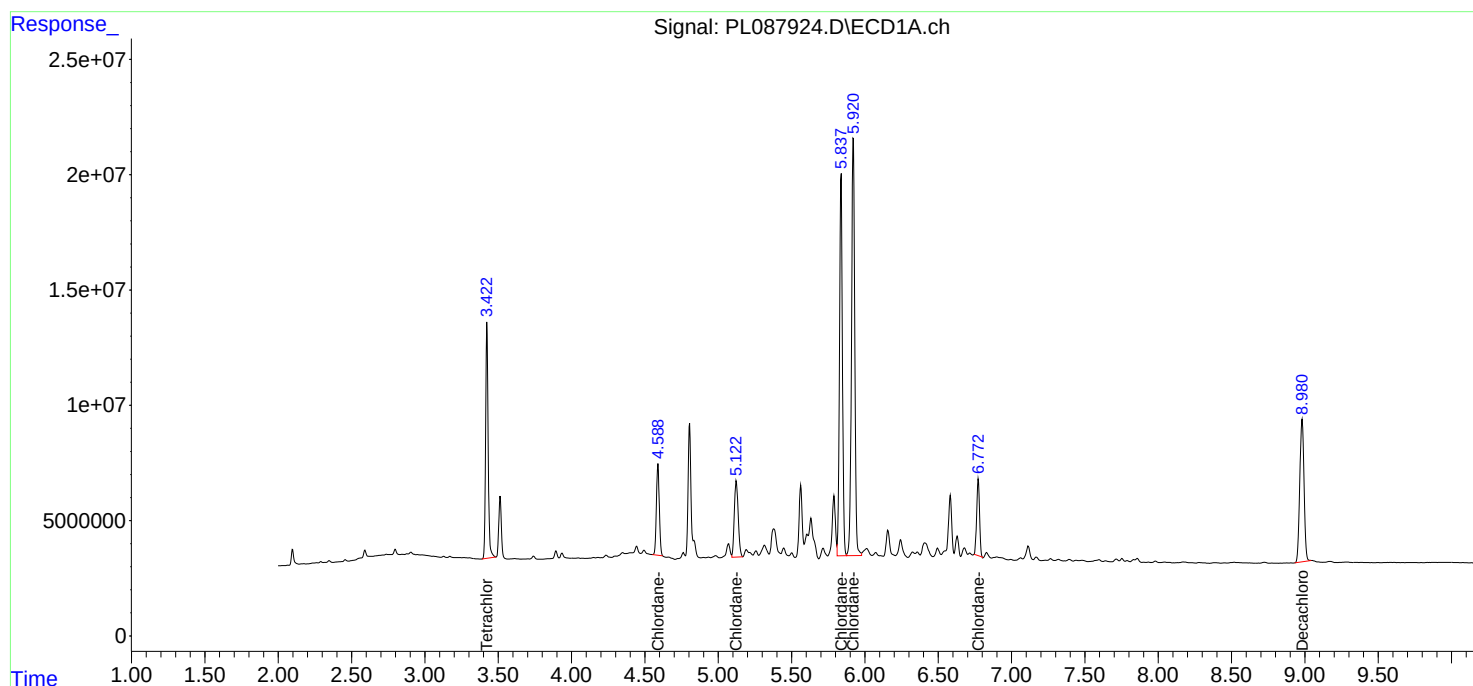


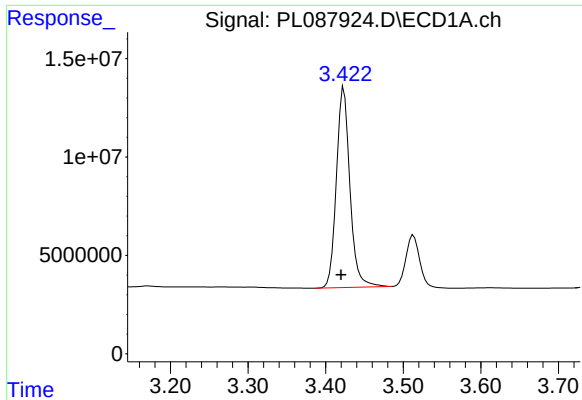

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: 0.003 min
Response: 123261028
Conc: 41.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

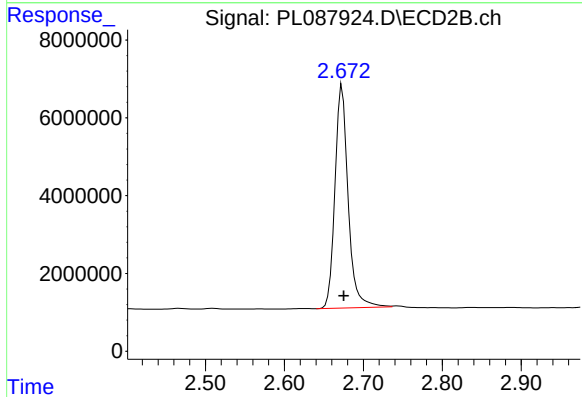


#1 Tetrachloro-m-xylene

R.T.: 2.673 min
Delta R.T.: -0.002 min
Response: 66423830
Conc: 54.83 ng/ml

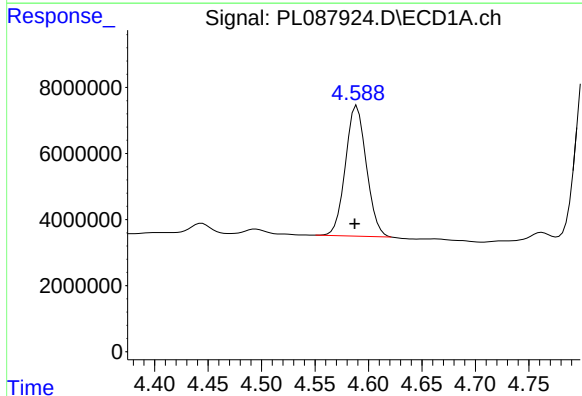


#23 Chlordane-1

R.T.: 4.589 min
Delta R.T.: 0.002 min
Response: 53788193
Conc: 402.98 ng/ml

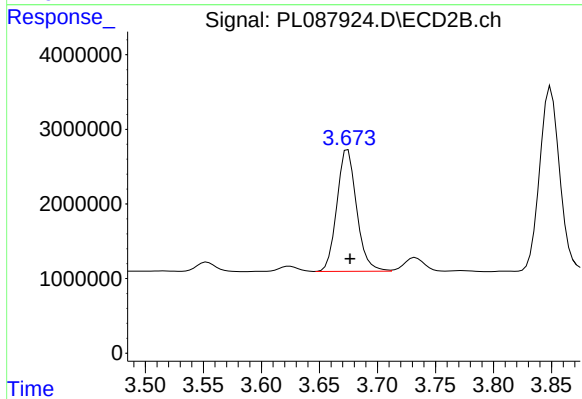

#23 Chlordane-1


R.T.: 3.675 min
Delta R.T.: -0.002 min
Response: 19314950
Conc: 413.26 ng/ml

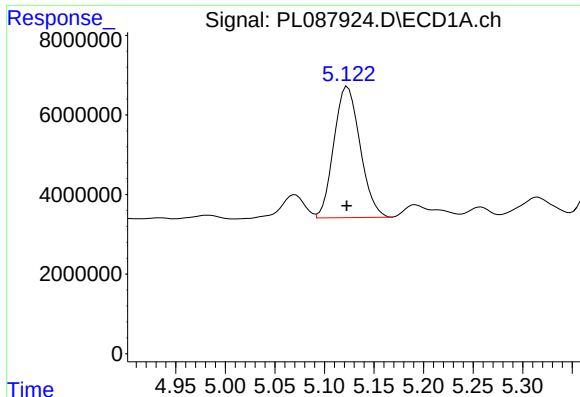

#24 Chlordane-2


R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 60602296
Conc: 410.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

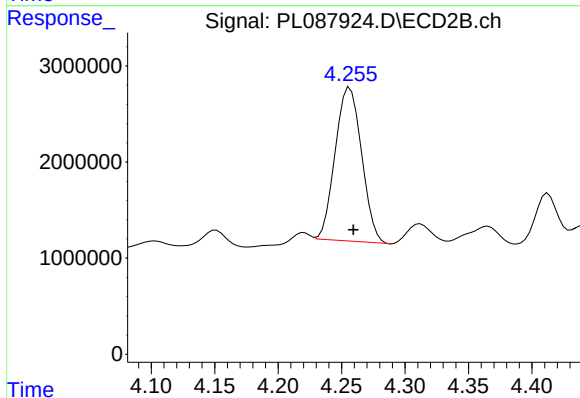


#24 Chlordane-2

R.T.: 4.257 min
Delta R.T.: -0.003 min
Response: 23205036
Conc: 414.76 ng/ml

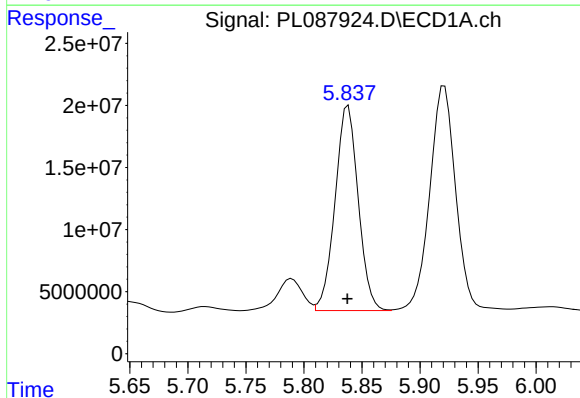


#25 Chlordane-3

R.T.: 5.838 min
Delta R.T.: 0.000 min
Response: 229175765
Conc: 411.99 ng/ml

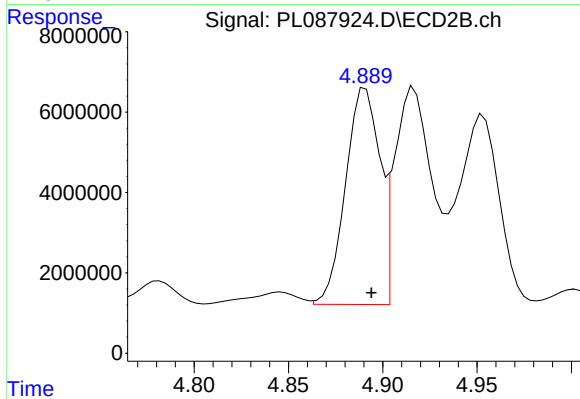

#25 Chlordane-3


R.T.: 4.891 min
Delta R.T.: -0.003 min
Response: 67931729
Conc: 429.25 ng/ml

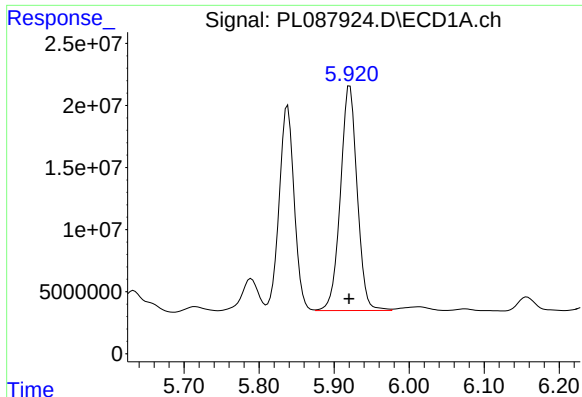

#26 Chlordane-4


R.T.: 5.921 min
Delta R.T.: 0.001 min
Response: 281526458
Conc: 407.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

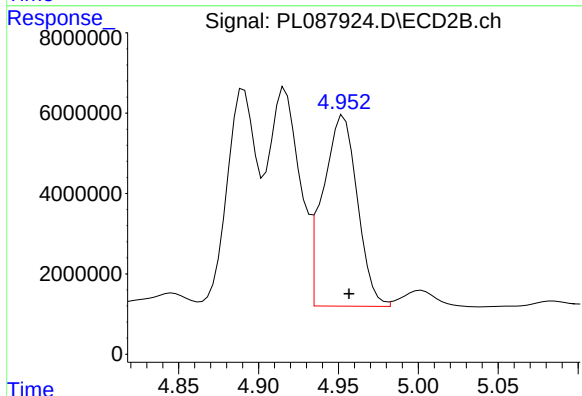


#26 Chlordane-4

R.T.: 4.953 min
Delta R.T.: -0.003 min
Response: 70933944
Conc: 415.16 ng/ml

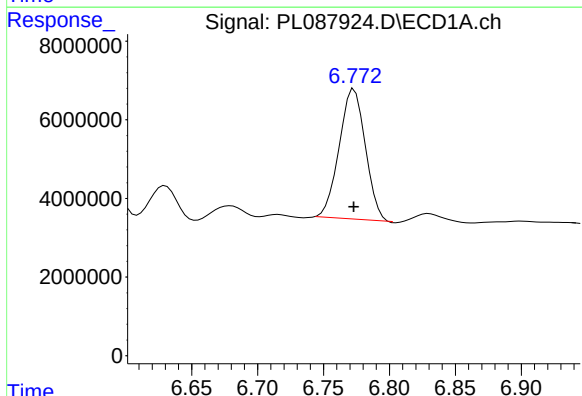


#27 Chlordane-5

R.T.: 6.772 min
Delta R.T.: -0.001 min
Response: 45471467
Conc: 403.21 ng/ml m

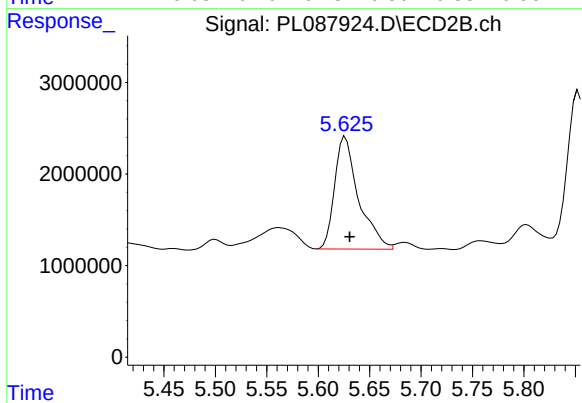

#27 Chlordane-5

R.T.: 5.627 min
Delta R.T.: -0.004 min
Response: 19916872
Conc: 423.12 ng/ml

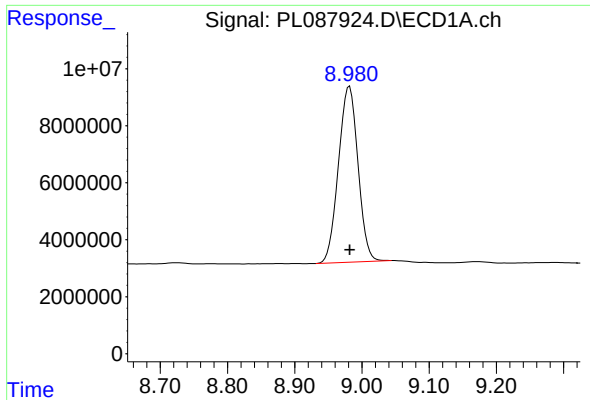

#28 Decachlorobiphenyl


R.T.: 8.981 min

Delta R.T.: 0.000 min

Response: 124280618

Conc: 43.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

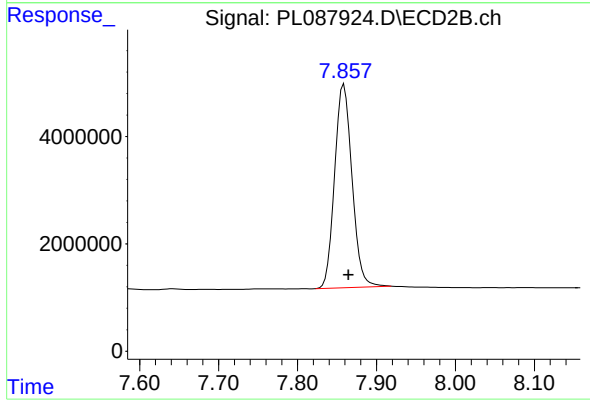

#28 Decachlorobiphenyl

R.T.: 7.859 min

Delta R.T.: -0.005 min

Response: 58162750

Conc: 45.91 ng/ml