

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012424\
 Data File : PL087936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2024 17:09
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 01:03:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 03:17:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.672	130.1E6	69198497	43.461	57.125 #
28)	SA Decachlor...	8.977	7.858	130.5E6	62005461	45.818	48.946
Target Compounds							
23)	Chlordane-1	4.585	3.674	57624957	20598784	431.726	440.727
24)	Chlordane-2	5.119	4.256	63992390	24750471	433.939	442.379
25)	Chlordane-3	5.834	4.890	245.2E6	72992768	440.872	461.231
26)	Chlordane-4	5.918	4.952	299.7E6	75620675	433.325	442.594
27)	Chlordane-5	6.768	5.626	49420585	21192326	438.232m	450.213



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012424\
Data File : PL087936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2024 17:09
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 01:03:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:17:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

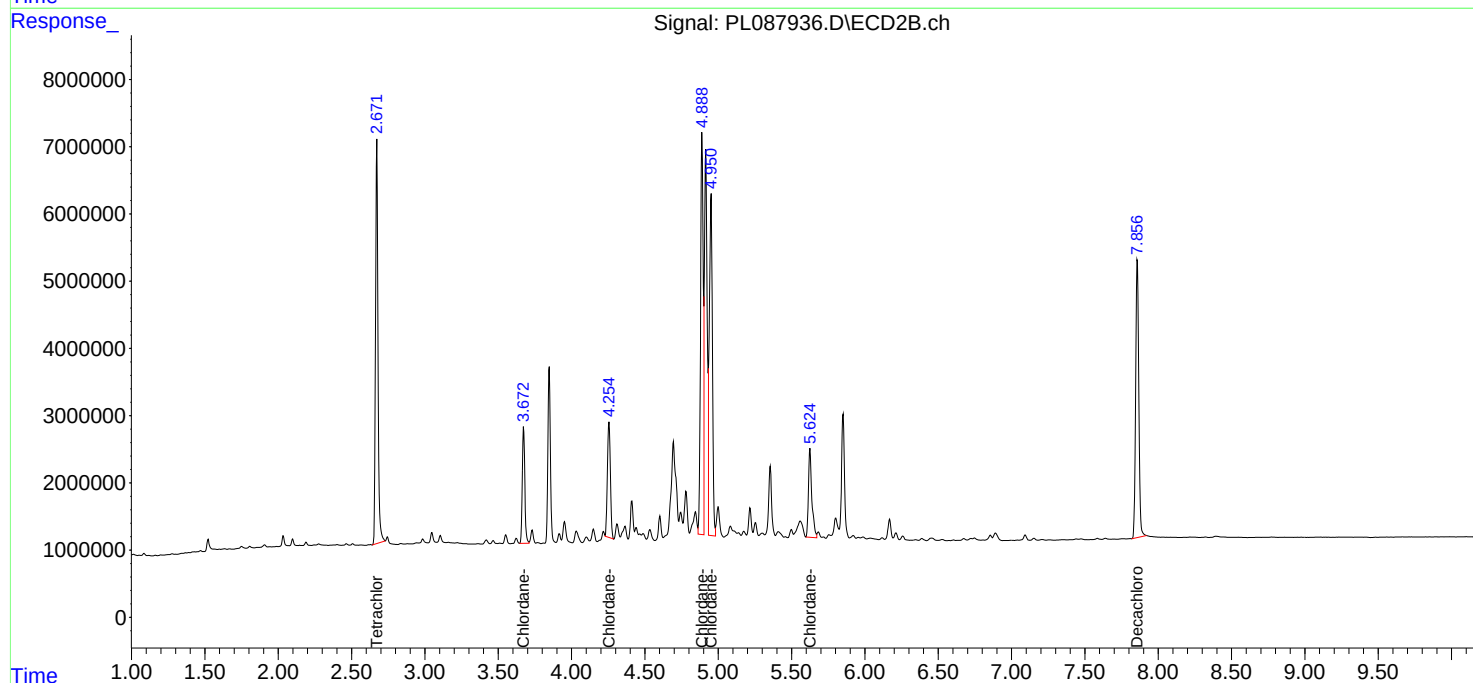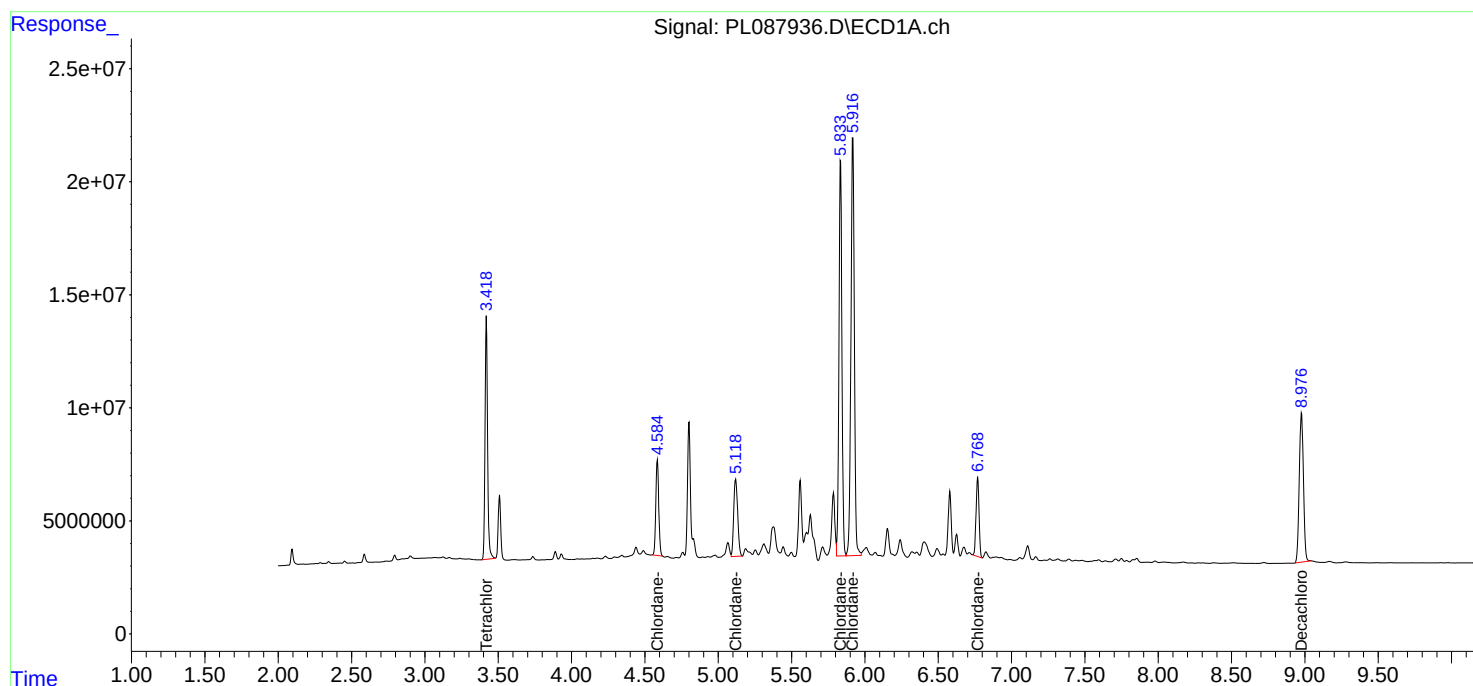


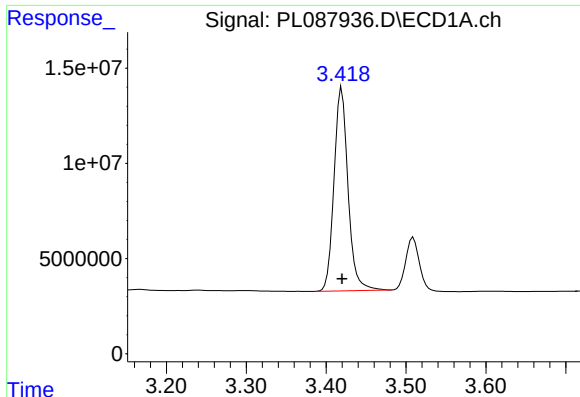

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 130111417
Conc: 43.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

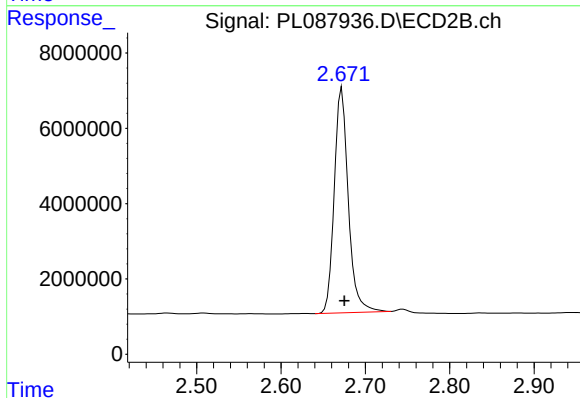


#1 Tetrachloro-m-xylene

R.T.: 2.672 min
Delta R.T.: -0.003 min
Response: 69198497
Conc: 57.13 ng/ml

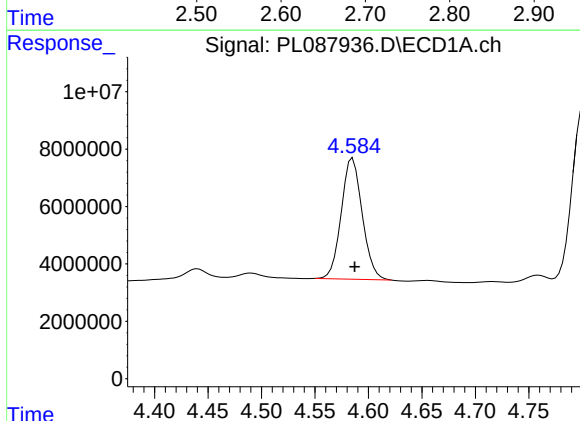


#23 Chlordane-1

R.T.: 4.585 min
Delta R.T.: -0.002 min
Response: 57624957
Conc: 431.73 ng/ml

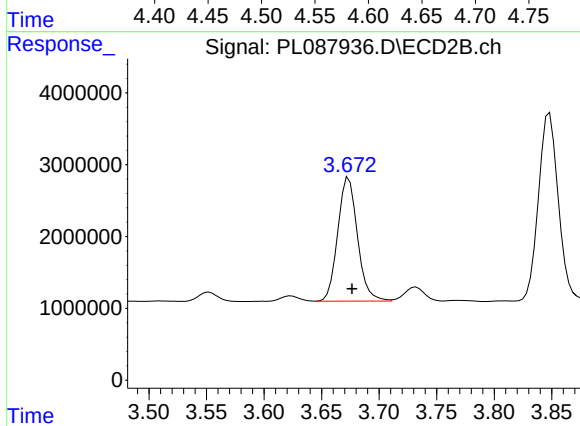

#23 Chlordane-1


R.T.: 3.674 min
Delta R.T.: -0.003 min
Response: 20598784
Conc: 440.73 ng/ml

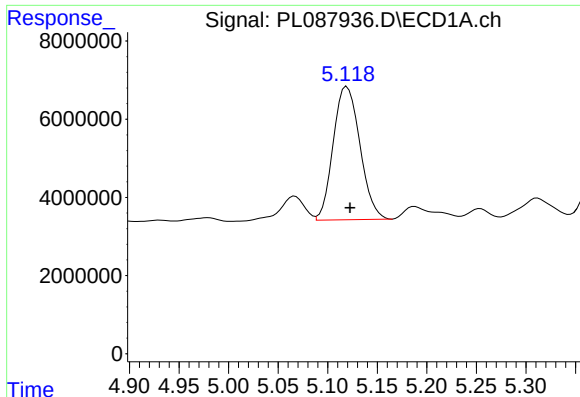

#24 Chlordane-2


R.T.: 5.119 min
Delta R.T.: -0.003 min
Response: 63992390
Conc: 433.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

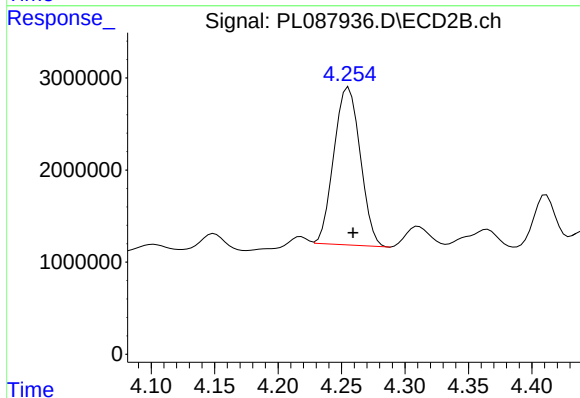


#24 Chlordane-2

R.T.: 4.256 min
Delta R.T.: -0.004 min
Response: 24750471
Conc: 442.38 ng/ml

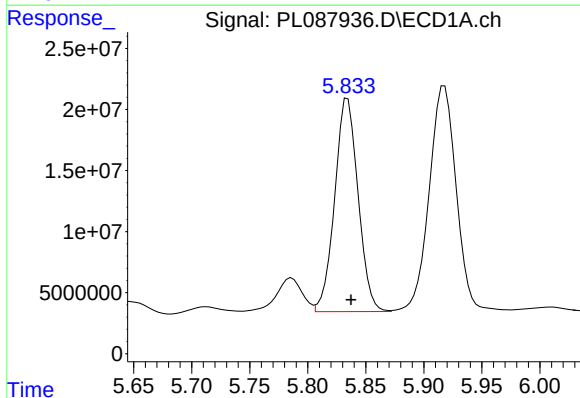


#25 Chlordane-3

R.T.: 5.834 min
Delta R.T.: -0.003 min
Response: 245241450
Conc: 440.87 ng/ml

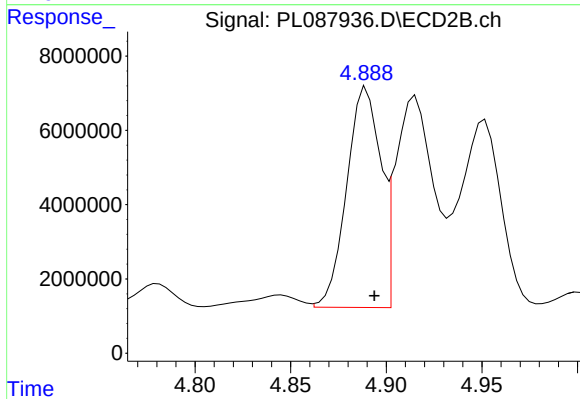

#25 Chlordane-3


R.T.: 4.890 min
Delta R.T.: -0.004 min
Response: 72992768
Conc: 461.23 ng/ml

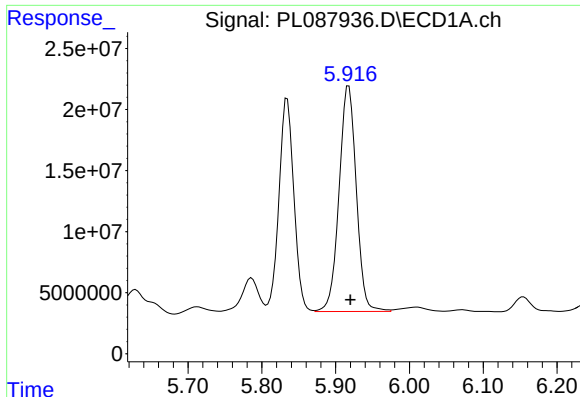

#26 Chlordane-4


R.T.: 5.918 min
Delta R.T.: -0.002 min
Response: 299739170
Conc: 433.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

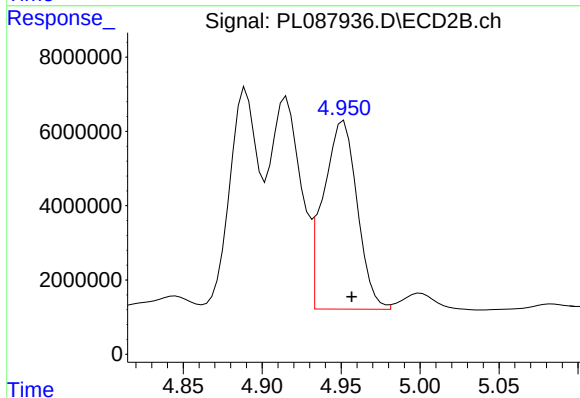


#26 Chlordane-4

R.T.: 4.952 min
Delta R.T.: -0.005 min
Response: 75620675
Conc: 442.59 ng/ml

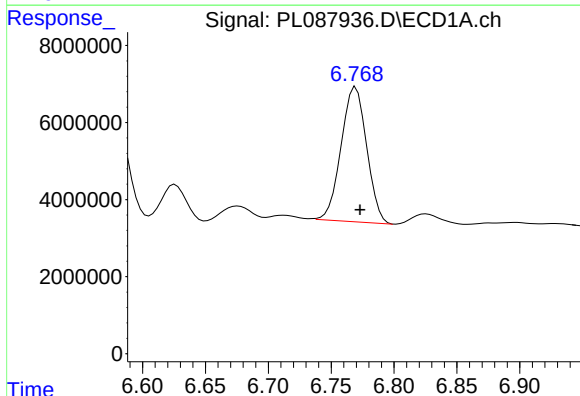


#27 Chlordane-5

R.T.: 6.768 min
Delta R.T.: -0.005 min
Response: 49420585
Conc: 438.23 ng/ml m

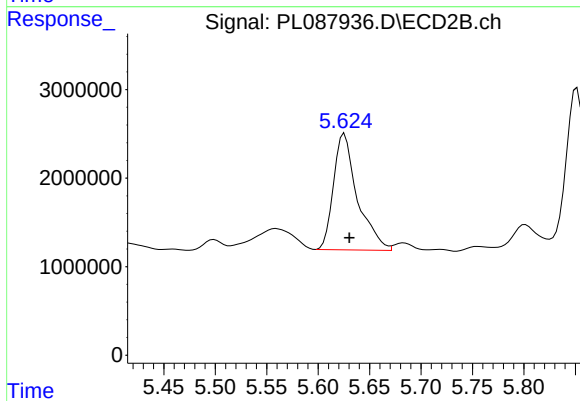

#27 Chlordane-5


R.T.: 5.626 min
Delta R.T.: -0.005 min
Response: 21192326
Conc: 450.21 ng/ml

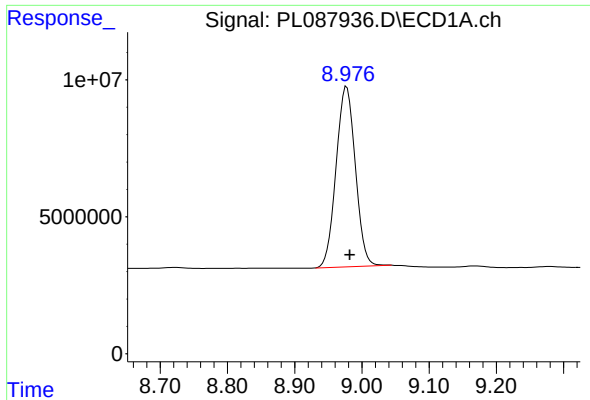

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.005 min
Response: 130489924
Conc: 45.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

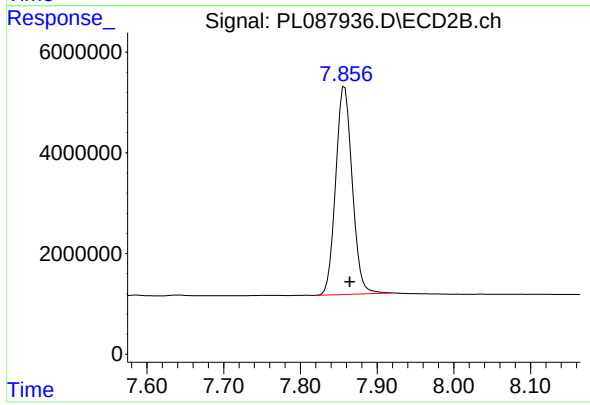

#28 Decachlorobiphenyl

R.T.: 7.858 min
Delta R.T.: -0.007 min
Response: 62005461
Conc: 48.95 ng/ml