

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012519\
 Data File : PL044231.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2019 17:55
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 23:56:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 25 13:56:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.367	3.987	143.2E6	49365610	23.623	22.631
28)	SA Decachlor...	8.052	9.046	139.3E6	47033003	20.092	21.202
Target Compounds							
6)	B beta-BHC	4.285f	0.000	8678037	0	2.503	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012519\
Data File : PL044231.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2019 17:55
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 23:56:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
Quant Title : GC Extractables
QLast Update : Fri Jan 25 13:56:36 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

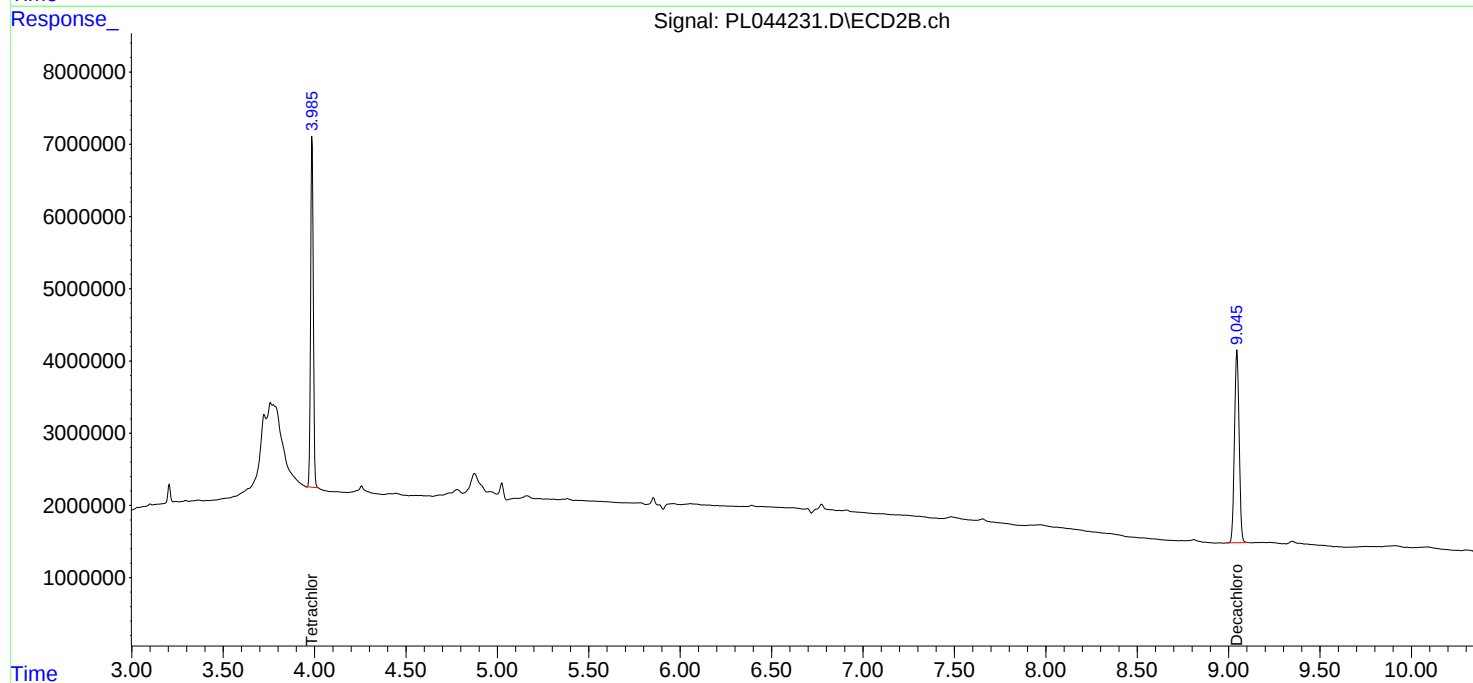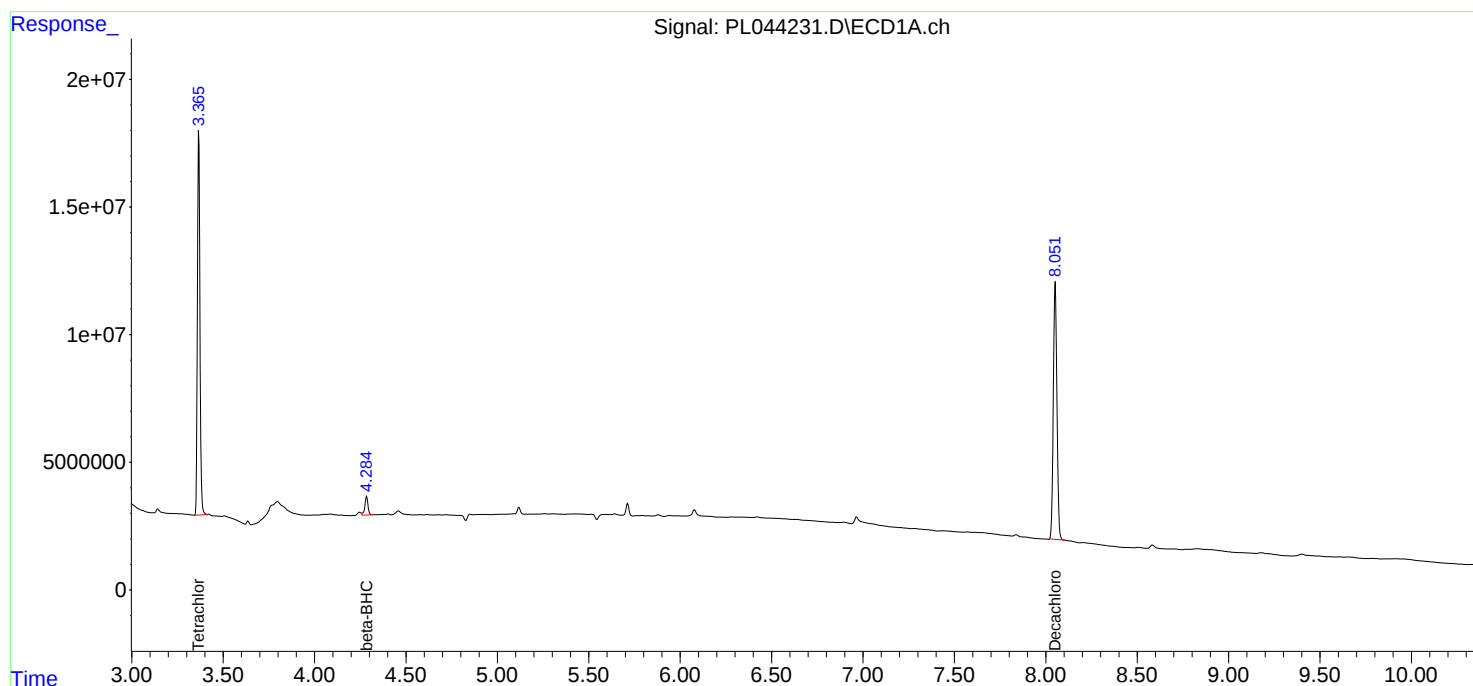


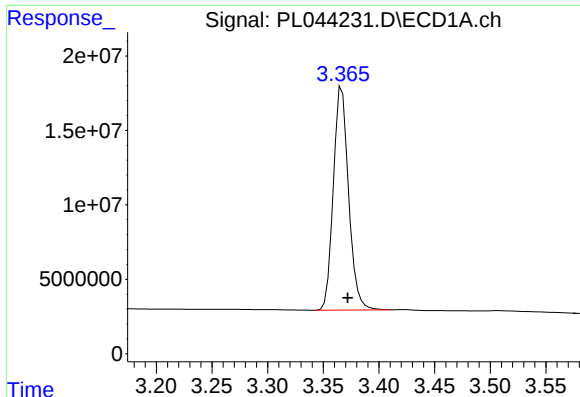

#1 Tetrachloro-m-xylene


R.T.: 3.367 min
Delta R.T.: -0.005 min
Response: 143166294
Conc: 23.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

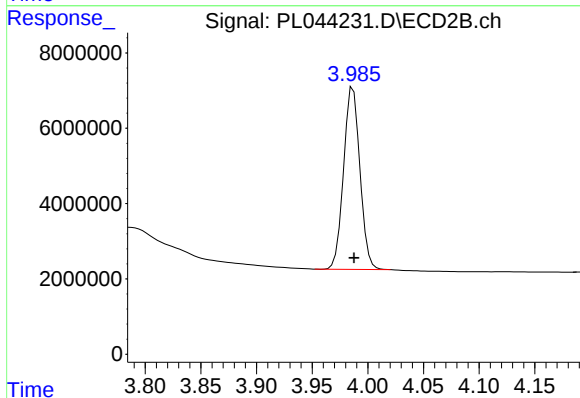


#1 Tetrachloro-m-xylene

R.T.: 3.987 min
Delta R.T.: 0.000 min
Response: 49365610
Conc: 22.63 ng/ml

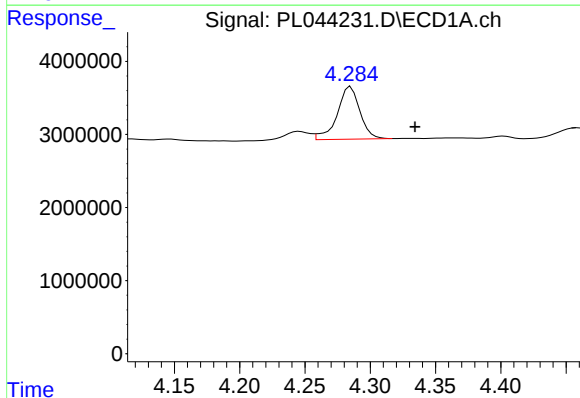


#6 beta-BHC

R.T.: 4.285 min
Delta R.T.: -0.049 min
Response: 8678037
Conc: 2.50 ng/ml

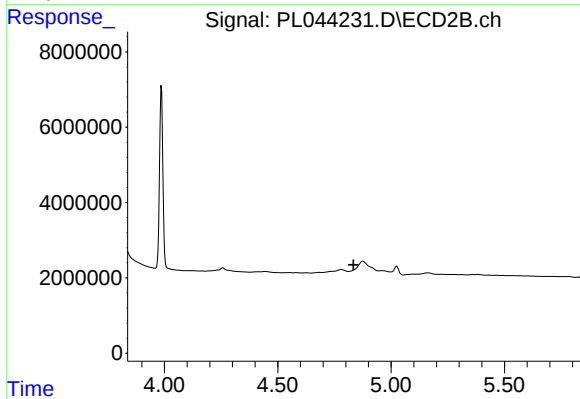

#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.835 min
Response: 0
Conc: N.D.

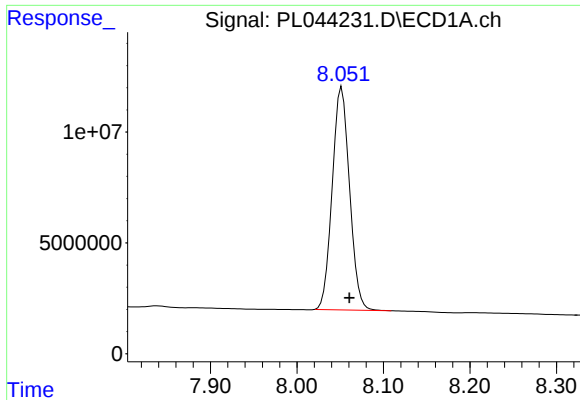

#28 Decachlorobiphenyl


R.T.: 8.052 min

Delta R.T.: -0.009 min

Response: 139338160

Conc: 20.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

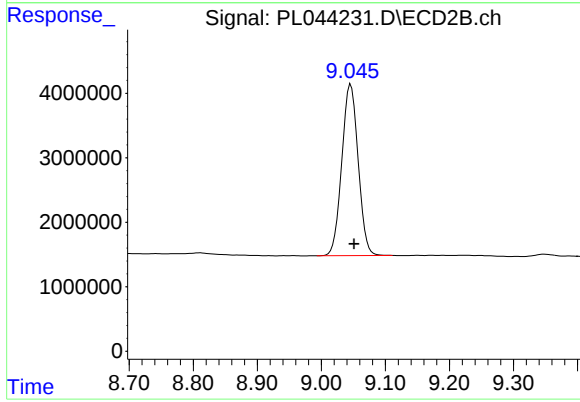

#28 Decachlorobiphenyl

R.T.: 9.046 min

Delta R.T.: -0.005 min

Response: 47033003

Conc: 21.20 ng/ml