

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012519\
 Data File : PL044242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2019 20:31
 Operator : AJ\SJ
 Sample : K1016-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-RO-2-012319

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 23:58:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 25 13:56:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.367	3.987	136.7E6	47475603	22.560	21.765
28)	SA Decachlor...	8.052	9.047	125.0E6	40118939	18.023	18.085
Target Compounds							
3)	MA gamma-BHC...	4.083	4.639	5004678	1132397	0.622	0.428 #
4)	MA Heptachlor	4.331f	5.169	4034466	2528274	0.512	0.974 #
5)	MB Aldrin	0.000	5.513f	0	1554561	N.D.	0.618 #
6)	B beta-BHC	4.331	0.000	4034466	0	1.164	N.D. #
10)	B gamma-Chl...	0.000	6.079	0	3274282	N.D.	1.298 #
13)	MA Dieldrin	5.600	0.000	7803584	0	1.038	N.D. #
18)	B Endrin al...	6.321	0.000	6801439	0	1.203	N.D. #
19)	B Endosulfa...	6.538	7.250	23450887	911367	4.112	0.474 #
20)	A Methoxychlor	0.000	7.507f	0	4331388	N.D.	4.235 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012519\
Data File : PL044242.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2019 20:31
Operator : AJ\SJ
Sample : K1016-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TR-05-RO-2-012319

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 23:58:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
Quant Title : GC Extractables
QLast Update : Fri Jan 25 13:56:36 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

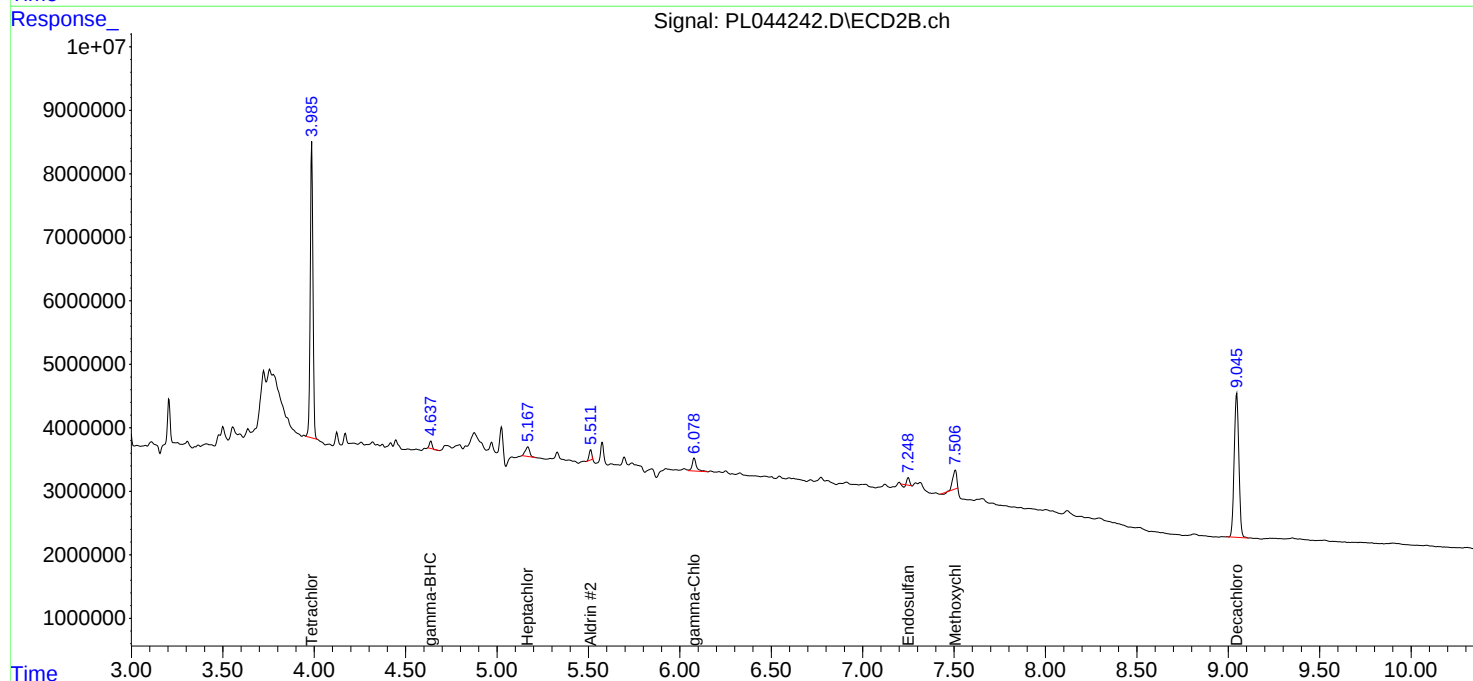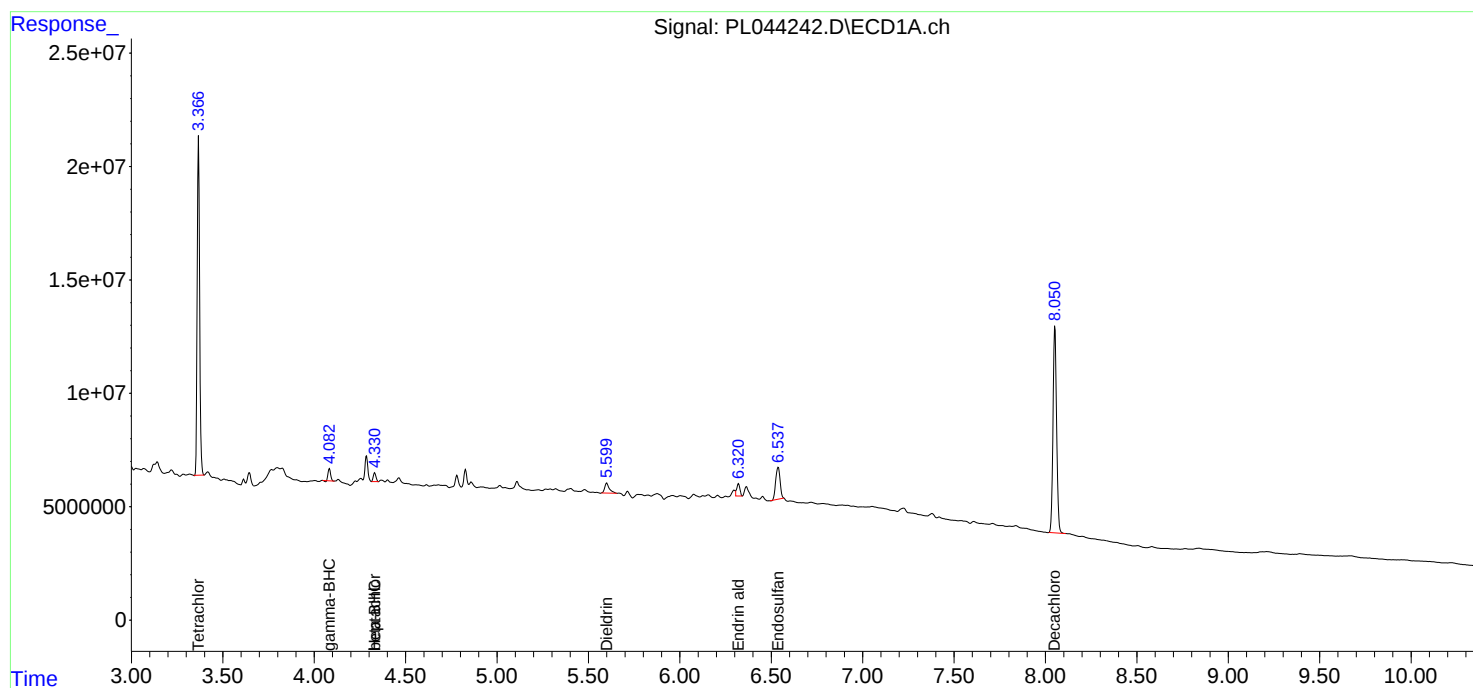


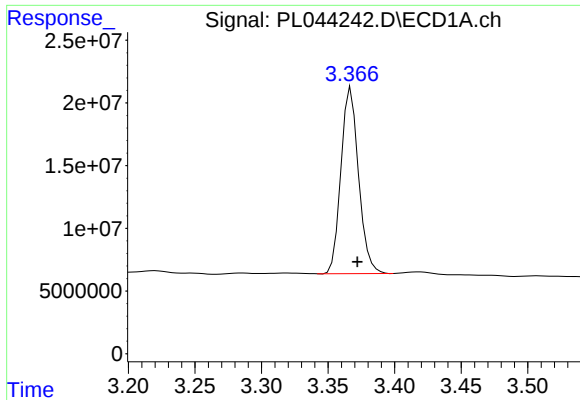

#1 Tetrachloro-m-xylene


R.T.: 3.367 min
Delta R.T.: -0.005 min
Response: 136723826
Conc: 22.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-RO-2-012319

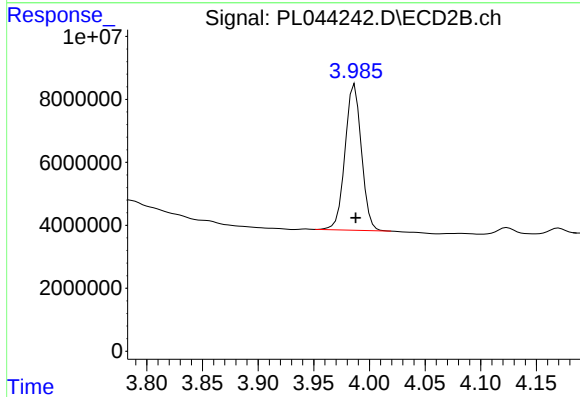


#1 Tetrachloro-m-xylene

R.T.: 3.987 min
Delta R.T.: 0.000 min
Response: 47475603
Conc: 21.76 ng/ml

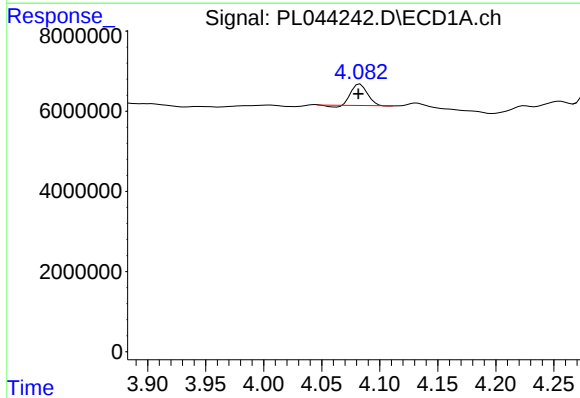


#3 gamma-BHC (Lindane)

R.T.: 4.083 min
Delta R.T.: 0.001 min
Response: 5004678
Conc: 0.62 ng/ml

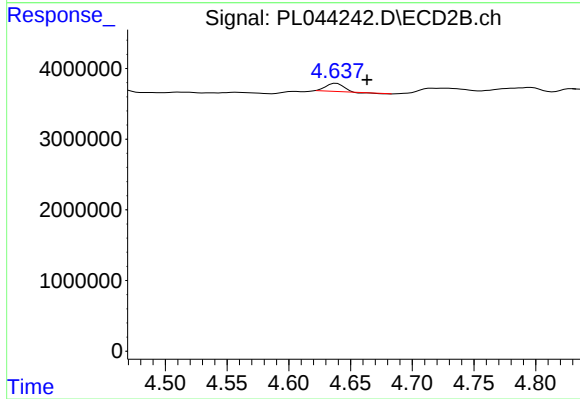

#3 gamma-BHC (Lindane)


R.T.: 4.639 min
Delta R.T.: -0.025 min
Response: 1132397
Conc: 0.43 ng/ml

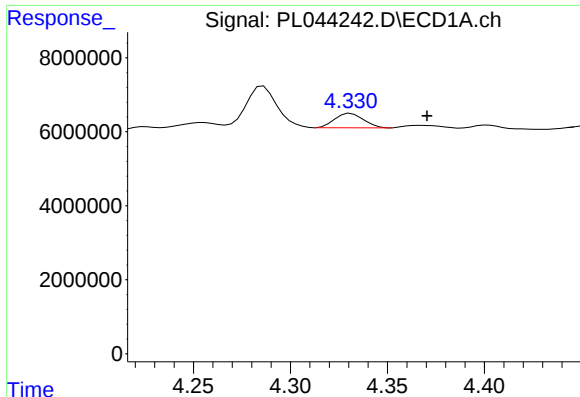

#4 Heptachlor


R.T.: 4.331 min
Delta R.T.: -0.039 min
Response: 4034466
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-RO-2-012319

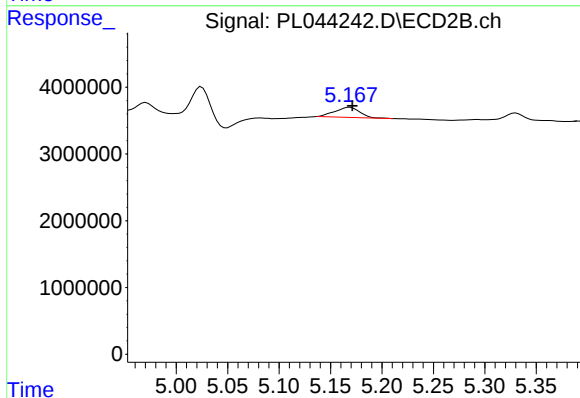


#4 Heptachlor

R.T.: 5.169 min
Delta R.T.: -0.003 min
Response: 2528274
Conc: 0.97 ng/ml

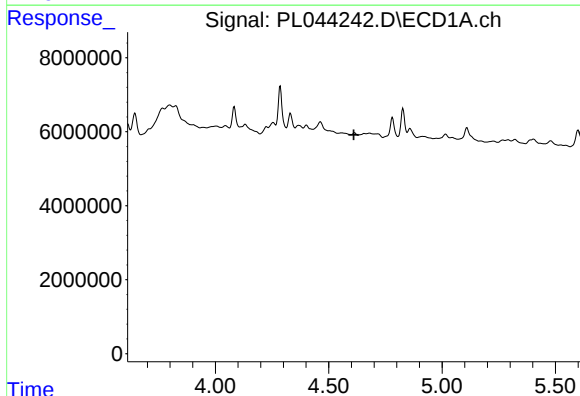


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.611 min
Response: 0
Conc: N.D.

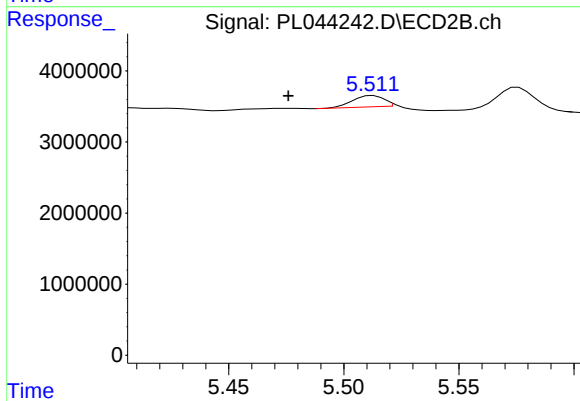

#5 Aldrin


R.T.: 5.513 min
Delta R.T.: 0.037 min
Response: 1554561
Conc: 0.62 ng/ml

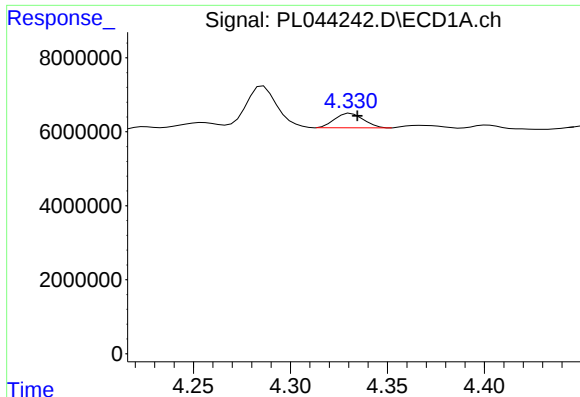

#6 beta-BHC


R.T.: 4.331 min
Delta R.T.: -0.003 min
Response: 4034466
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-RO-2-012319

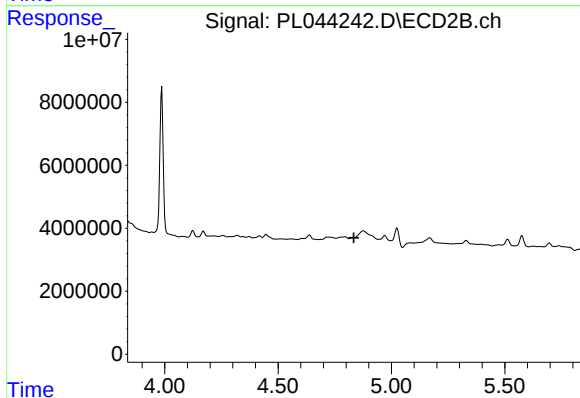


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.835 min
Response: 0
Conc: N.D.

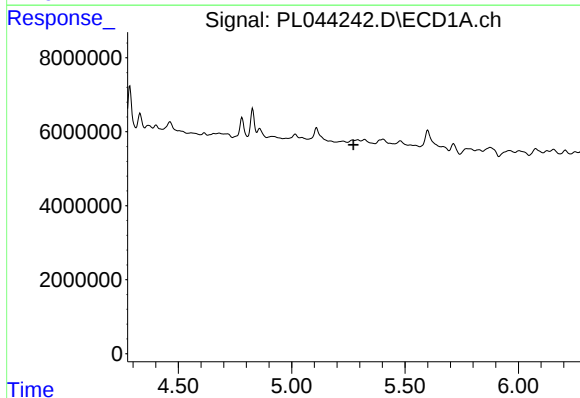


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.273 min
Response: 0
Conc: N.D.

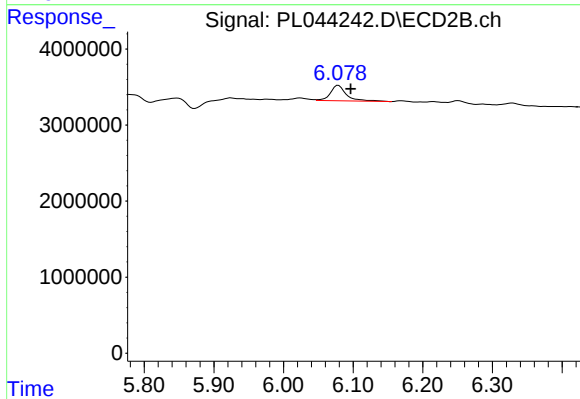

#10 gamma-Chlordane


R.T.: 6.079 min
Delta R.T.: -0.017 min
Response: 3274282
Conc: 1.30 ng/ml

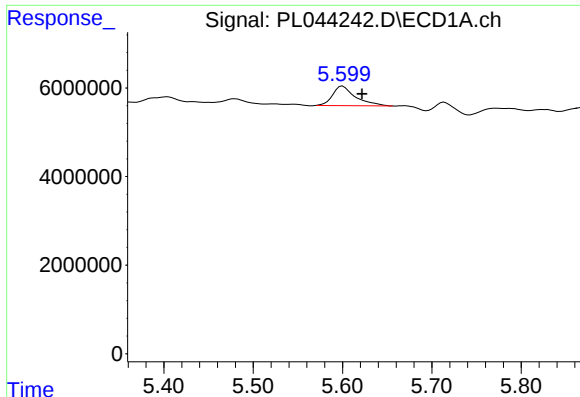

#13 Dieldrin


R.T.: 5.600 min
Delta R.T.: -0.022 min
Response: 7803584
Conc: 1.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-RO-2-012319

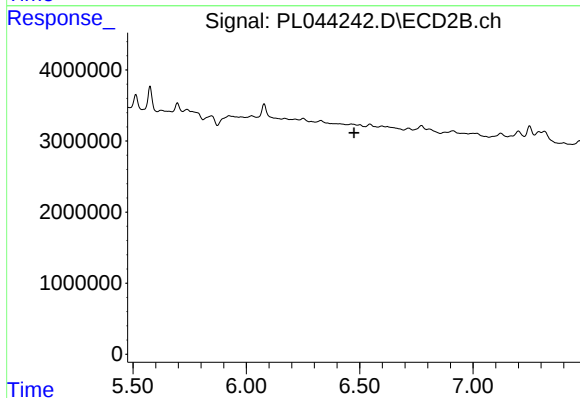


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.476 min
Response: 0
Conc: N.D.

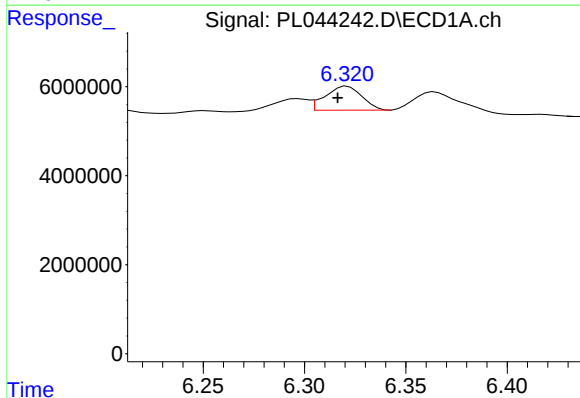


#18 Endrin aldehyde

R.T.: 6.321 min
Delta R.T.: 0.005 min
Response: 6801439
Conc: 1.20 ng/ml

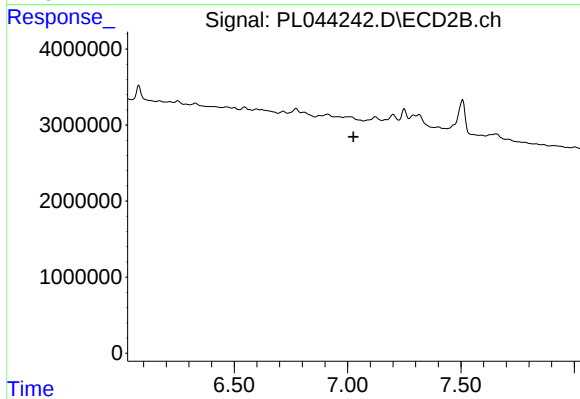

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.027 min
Response: 0
Conc: N.D.

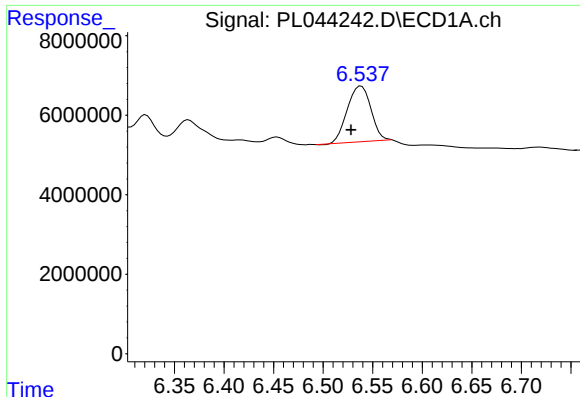

#19 Endosulfan Sulfate


R.T.: 6.538 min
Delta R.T.: 0.010 min
Response: 23450887
Conc: 4.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-RO-2-012319

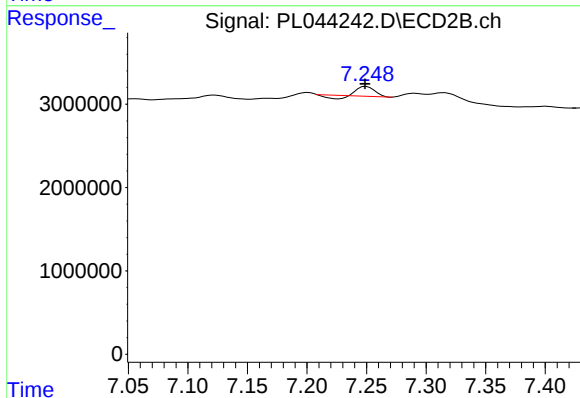


#19 Endosulfan Sulfate

R.T.: 7.250 min
Delta R.T.: 0.001 min
Response: 911367
Conc: 0.47 ng/ml

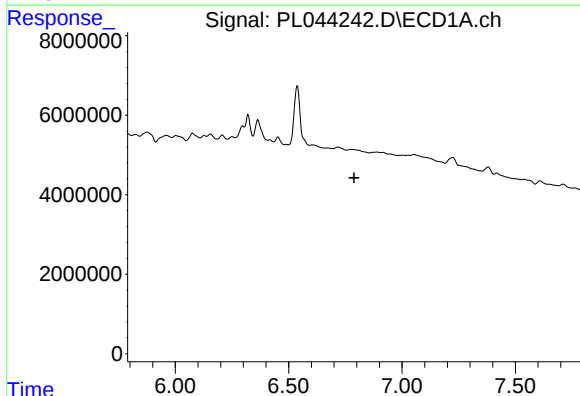


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.789 min
Response: 0
Conc: N.D.

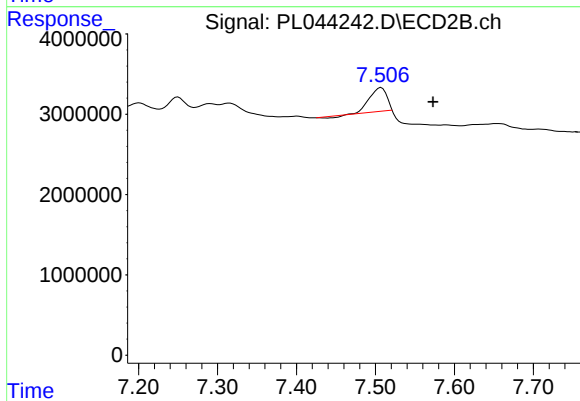

#20 Methoxychlor


R.T.: 7.507 min
Delta R.T.: -0.065 min
Response: 4331388
Conc: 4.23 ng/ml

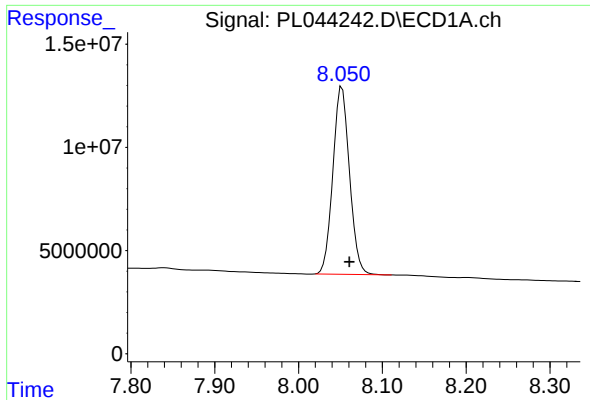

#28 Decachlorobiphenyl

R.T.: 8.052 min
Delta R.T.: -0.009 min
Response: 124989568
Conc: 18.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-RO-2-012319

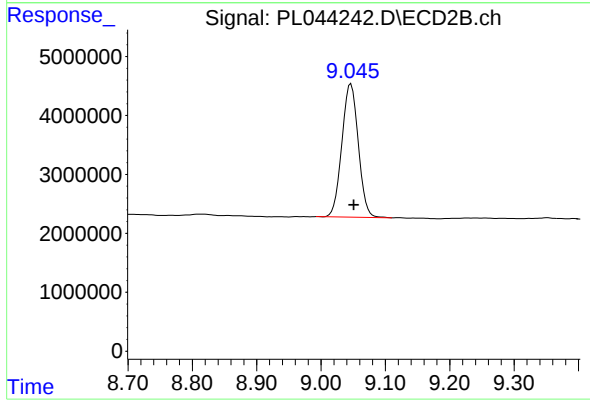

#28 Decachlorobiphenyl

R.T.: 9.047 min
Delta R.T.: -0.004 min
Response: 40118939
Conc: 18.08 ng/ml