

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012521\
 Data File : PL064372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2021 10:57
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 01:58:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	4.107	55117837	45121859	18.382	17.650
28)	SA Decachlor...	8.164	9.268	58509602	44105071	19.170	18.583
Target Compounds							
4)	MA Heptachlor	0.000	5.306	0	6555889	N.D.	1.825 #
7)	B delta-BHC	0.000	5.221f	0	5851504	N.D.	1.843 #
23)	Chlordane-1	4.323f	0.000	459441	0	3.945	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012521\
Data File : PL064372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2021 10:57
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 01:58:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

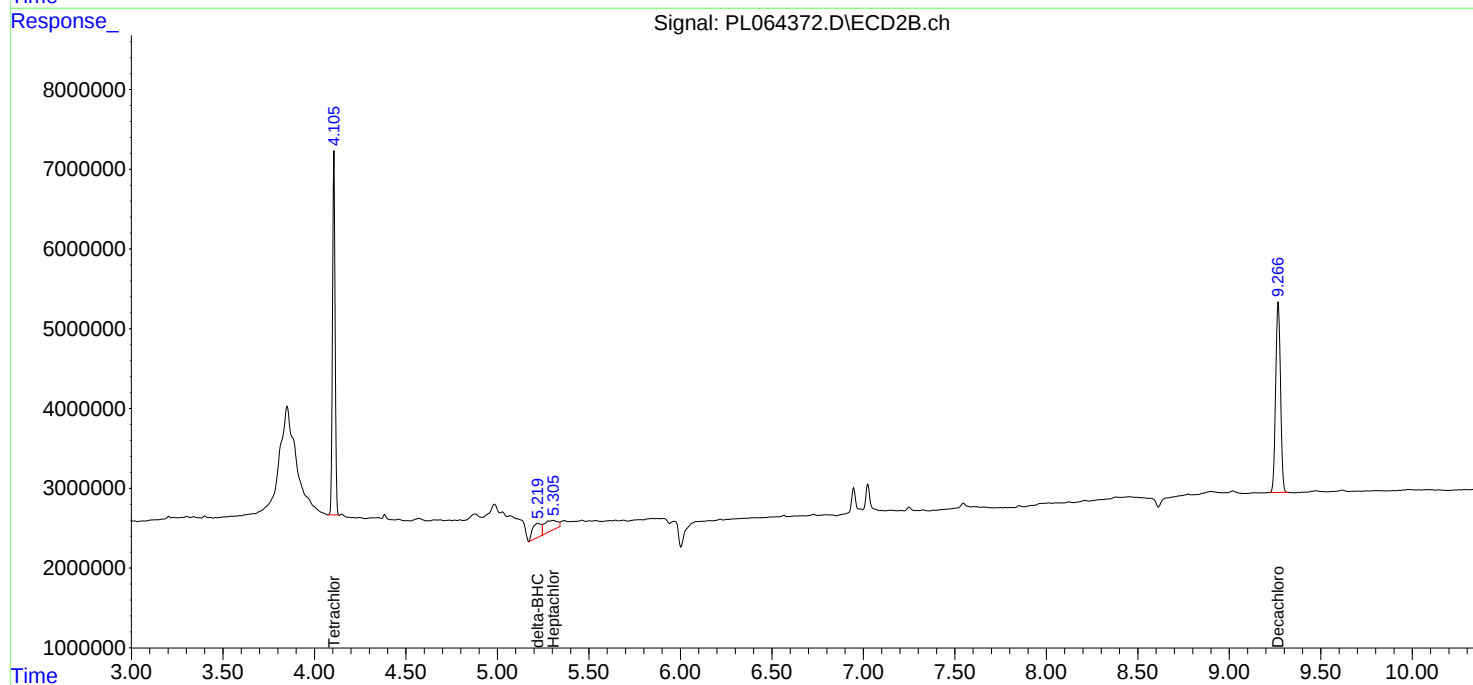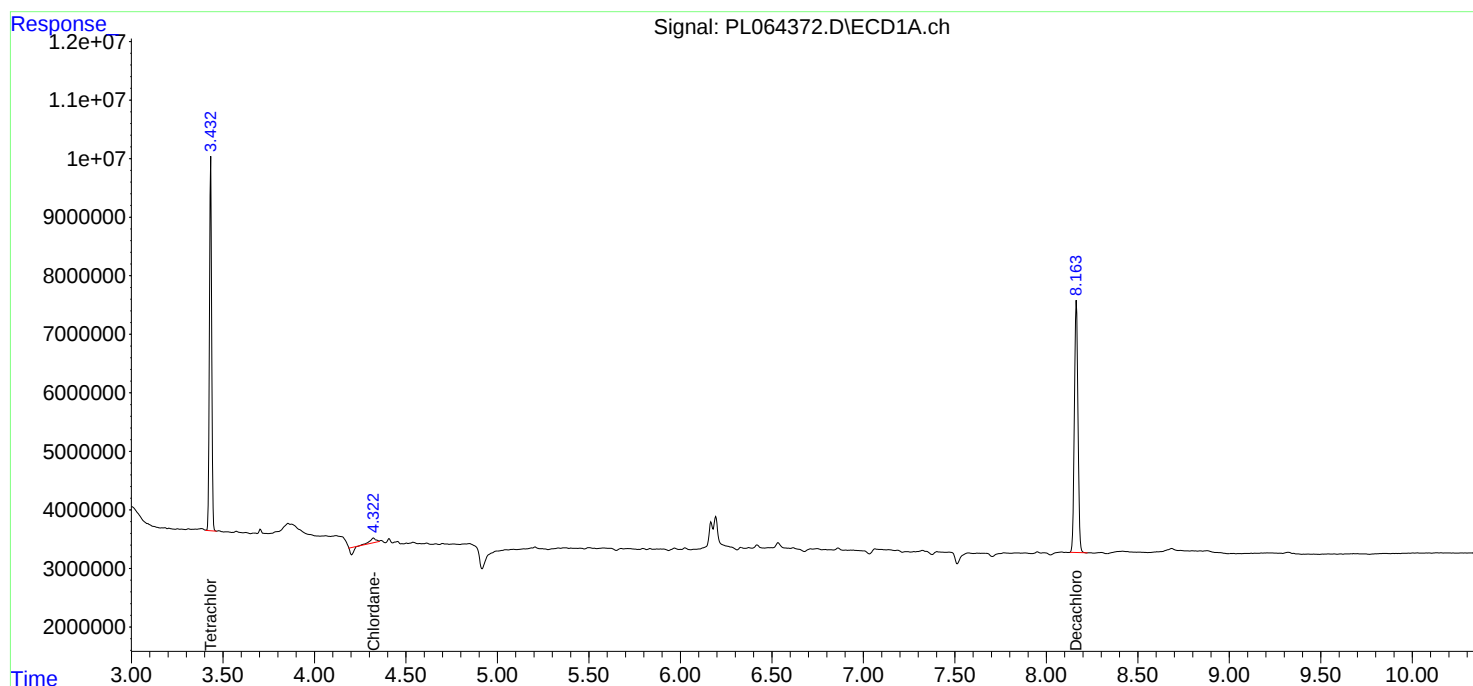


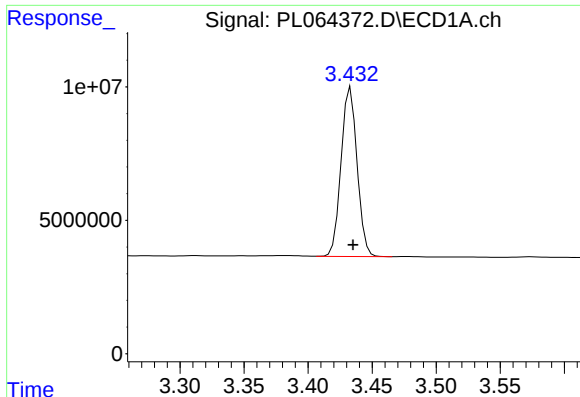

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: -0.002 min
Response: 55117837
Conc: 18.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

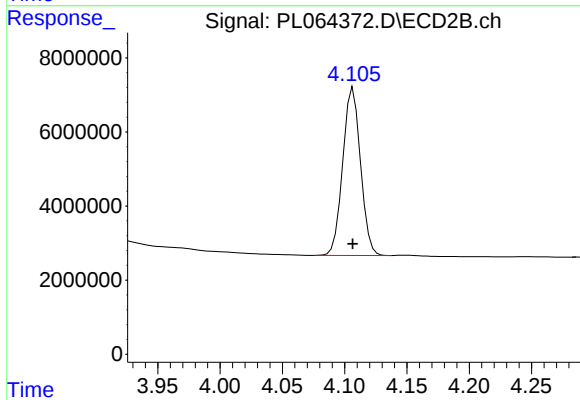


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 45121859
Conc: 17.65 ng/ml

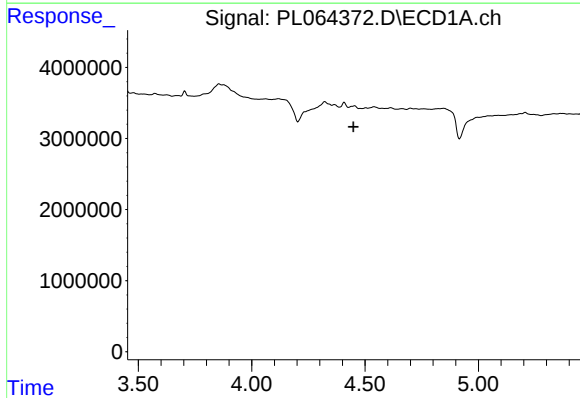


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

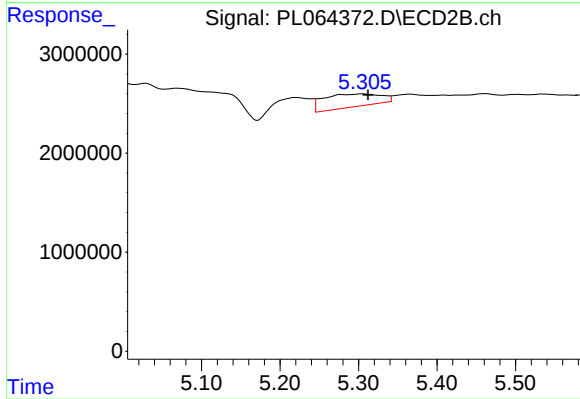

#4 Heptachlor


R.T.: 5.306 min
Delta R.T.: -0.006 min
Response: 6555889
Conc: 1.83 ng/ml

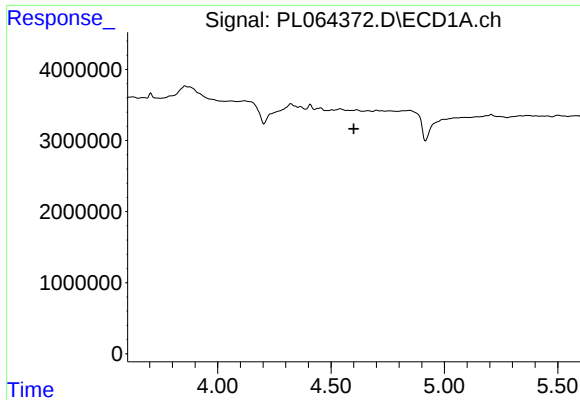

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.601 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

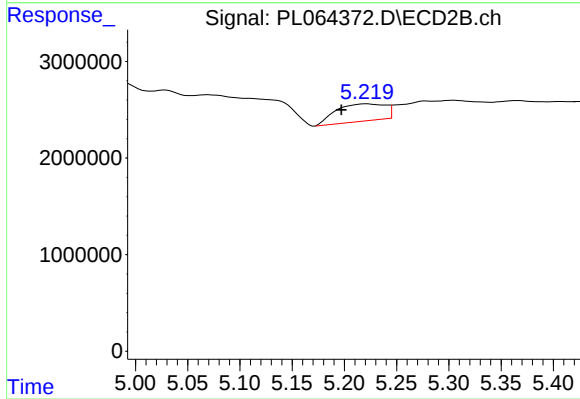


#7 delta-BHC

R.T.: 5.221 min
Delta R.T.: 0.024 min
Response: 5851504
Conc: 1.84 ng/ml

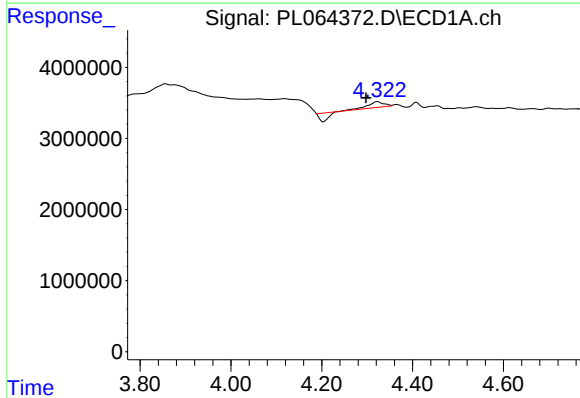


#23 Chlordane-1

R.T.: 4.323 min
Delta R.T.: 0.025 min
Response: 459441
Conc: 3.95 ng/ml

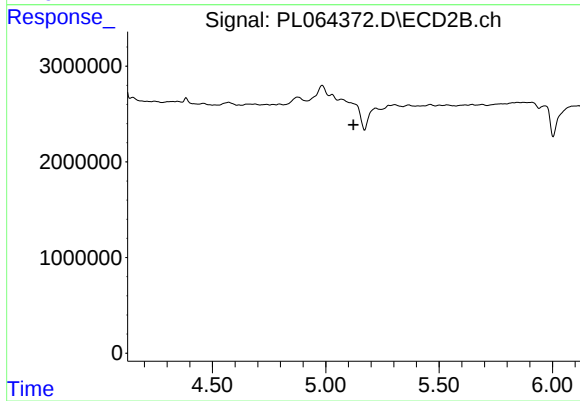

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.123 min
Response: 0
Conc: N.D.

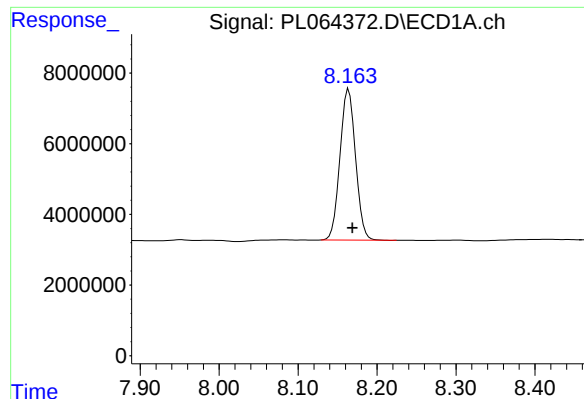

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: -0.005 min
Response: 58509602
Conc: 19.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

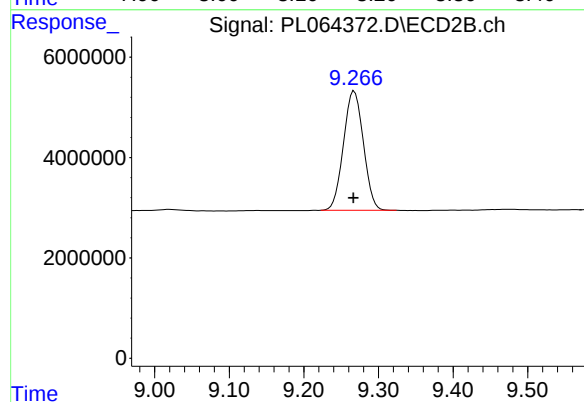

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.001 min
Response: 44105071
Conc: 18.58 ng/ml