

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012521\
 Data File : PL064388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2021 15:00
 Operator : AR\AJ
 Sample : PB134299BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 02:02:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.107	58841716	47340097	19.624	18.518
28)	SA Decachlor...	8.165	9.269	52456237	38964262	17.187	16.417
Target Compounds							
4)	MA Heptachlor	4.456	5.298	6515694	4689735	1.487	1.306
9)	A Endosulfan I	0.000	6.382	0	549285	N.D.	0.200 #
10)	B gamma-Chl...	0.000	6.248	0	10056932	N.D.	3.347 #
15)	B Endosulfa...	0.000	7.074	0	5558708	N.D.	2.200 #
20)	A Methoxychlor	0.000	7.717f	0	16477397	N.D.	12.195 #
21)	B Endrin ke...	0.000	7.913	0	2893477	N.D.	1.160 #
22)	Mirex	0.000	8.335f	0	3580839	N.D.	1.765 #
23)	Chlordane-1	4.324f	0.000	6341902	0	54.457	N.D. #
25)	Chlordane-3	0.000	6.248	0	10056932	N.D.	24.873 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012521\
Data File : PL064388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2021 15:00
Operator : AR\AJ
Sample : PB134299BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 02:02:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

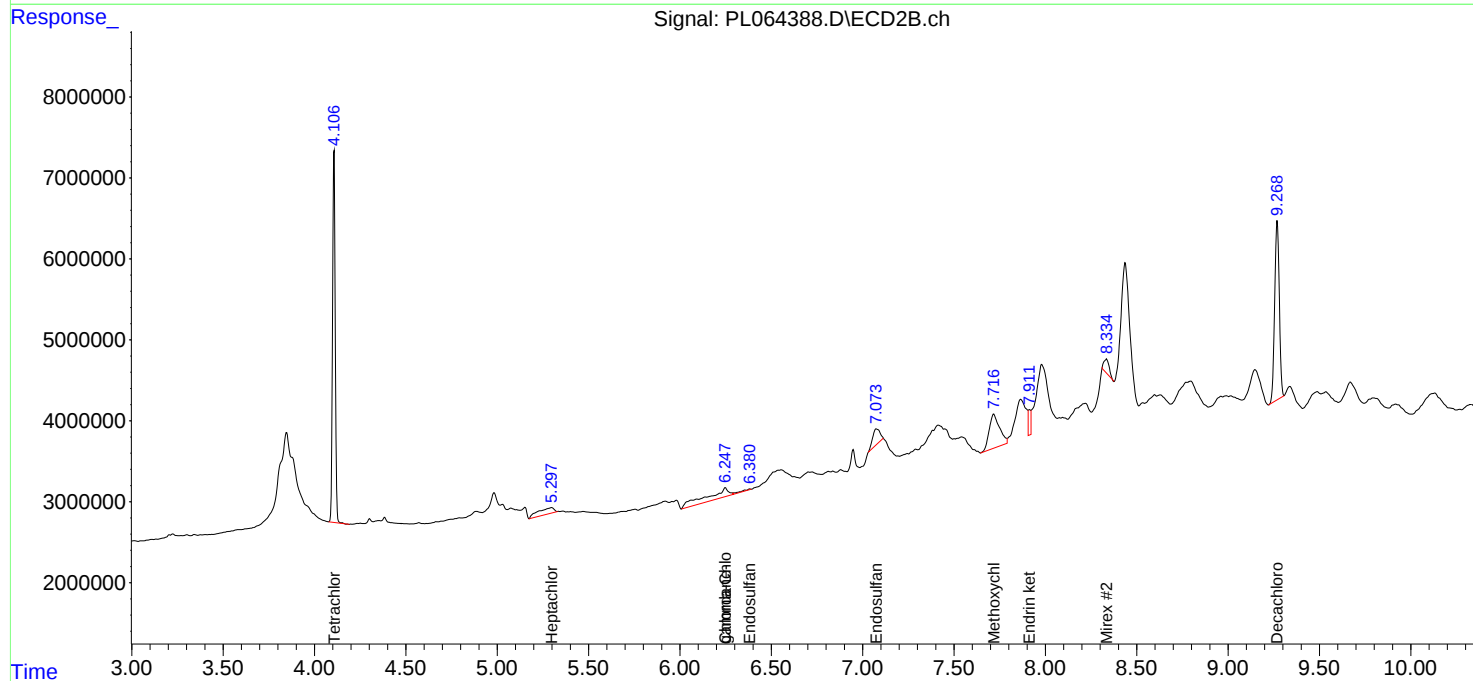


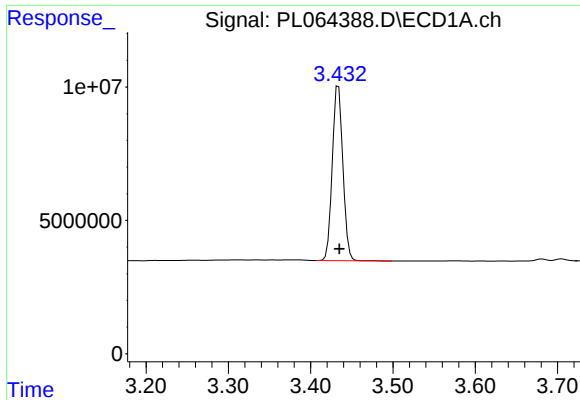

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: -0.001 min
Response: 58841716
Conc: 19.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

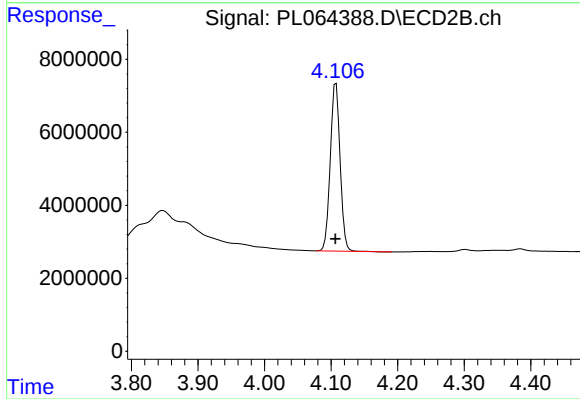


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.001 min
Response: 47340097
Conc: 18.52 ng/ml

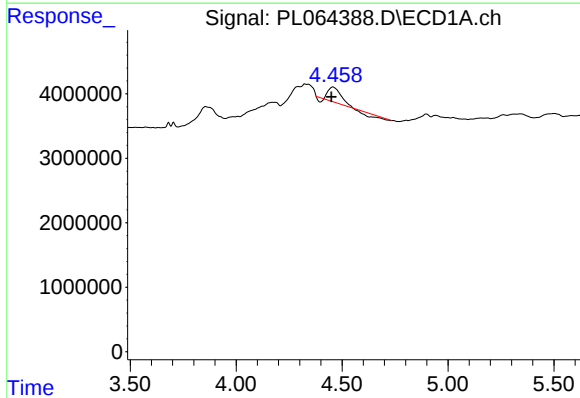


#4 Heptachlor

R.T.: 4.456 min
Delta R.T.: 0.007 min
Response: 6515694
Conc: 1.49 ng/ml

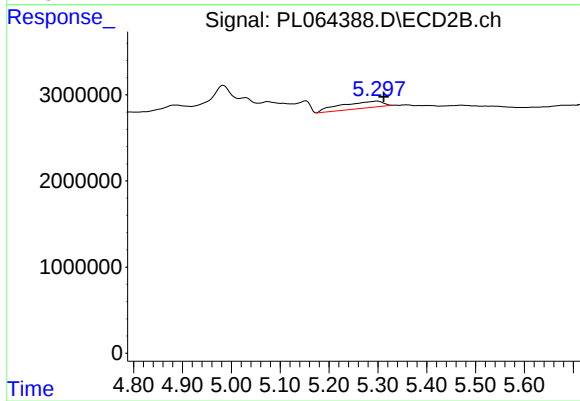

#4 Heptachlor


R.T.: 5.298 min
Delta R.T.: -0.014 min
Response: 4689735
Conc: 1.31 ng/ml

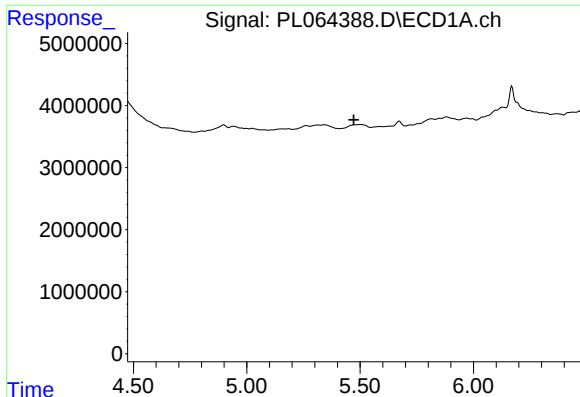

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

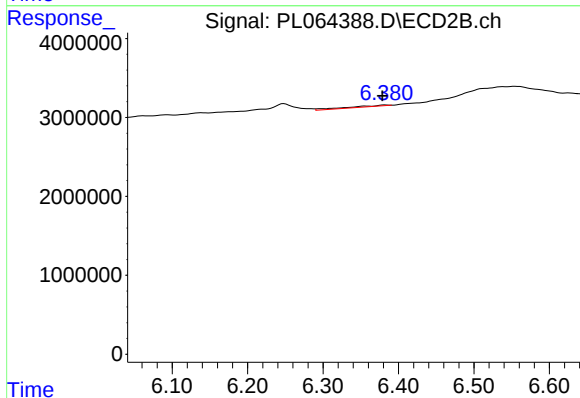


#9 Endosulfan I

R.T.: 6.382 min
Delta R.T.: 0.003 min
Response: 549285
Conc: 0.20 ng/ml

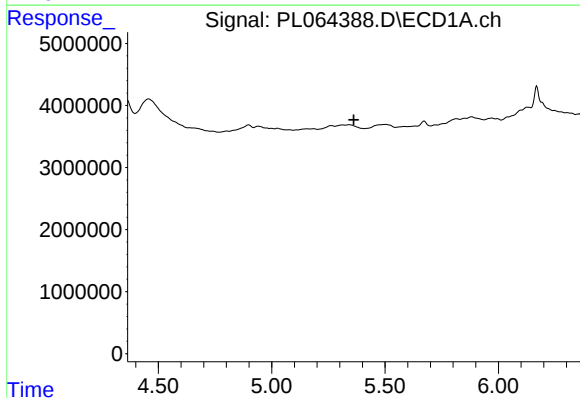


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.362 min
Response: 0
Conc: N.D.

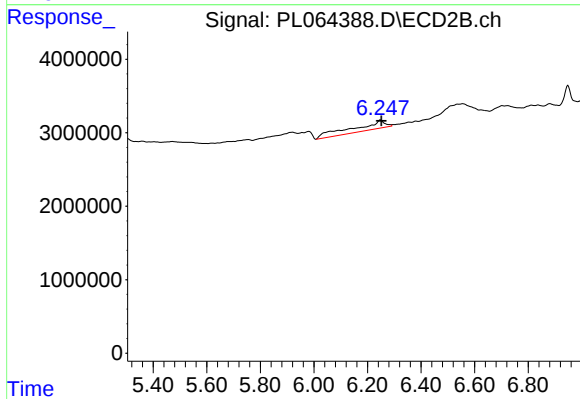

#10 gamma-Chlordane


R.T.: 6.248 min
Delta R.T.: -0.003 min
Response: 10056932
Conc: 3.35 ng/ml

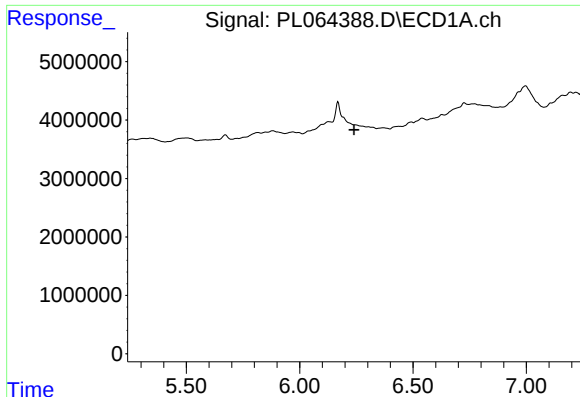

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

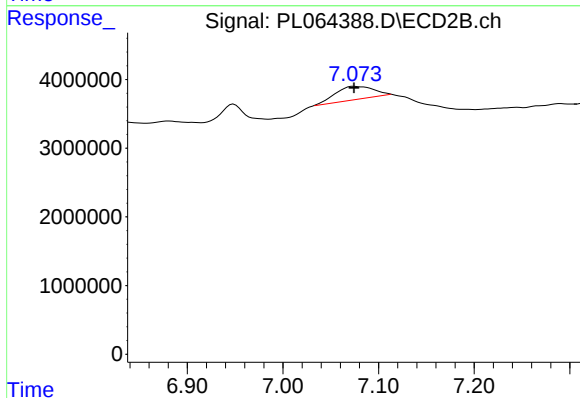


#15 Endosulfan II

R.T.: 7.074 min
Delta R.T.: 0.000 min
Response: 5558708
Conc: 2.20 ng/ml

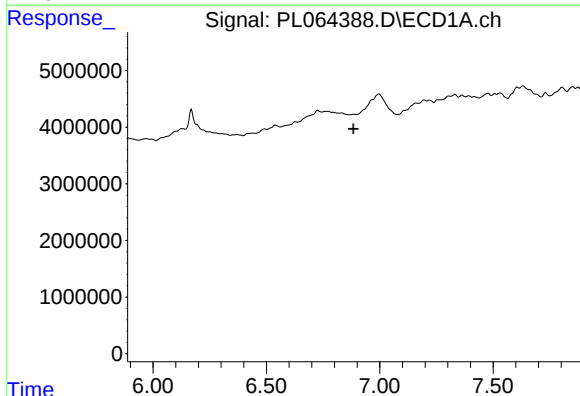


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.885 min
Response: 0
Conc: N.D.

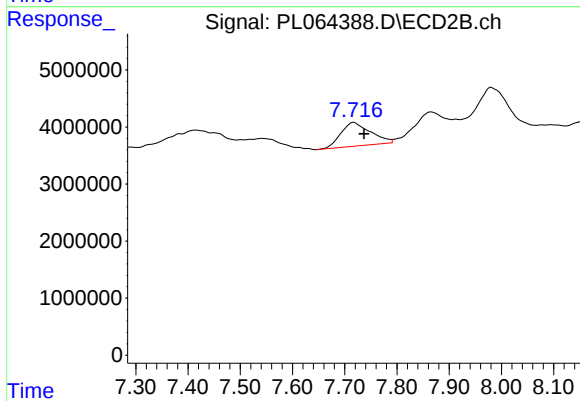

#20 Methoxychlor


R.T.: 7.717 min
Delta R.T.: -0.020 min
Response: 16477397
Conc: 12.20 ng/ml

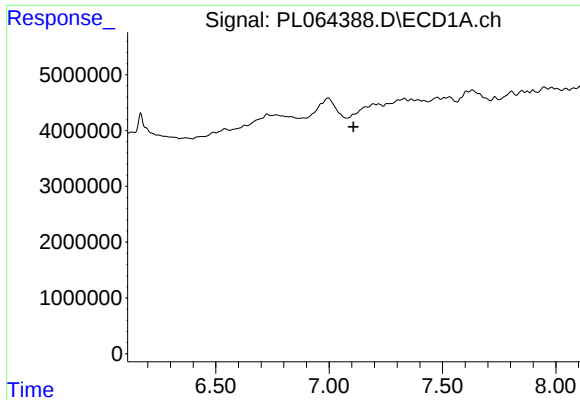

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.108 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

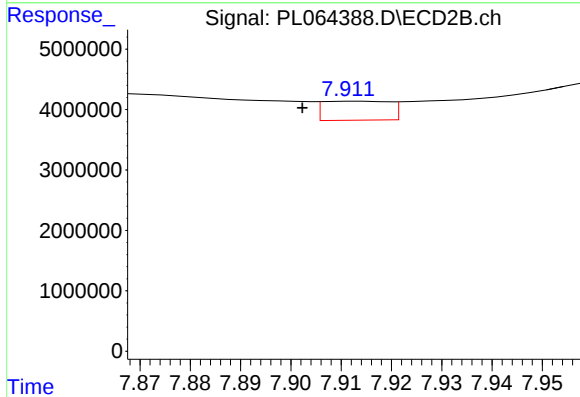


#21 Endrin ketone

R.T.: 7.913 min
Delta R.T.: 0.011 min
Response: 2893477
Conc: 1.16 ng/ml

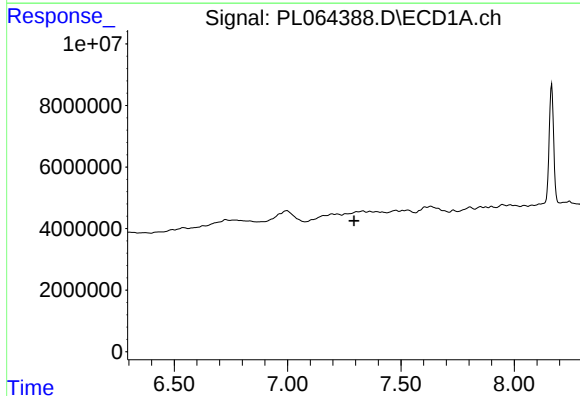


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.293 min
Response: 0
Conc: N.D.

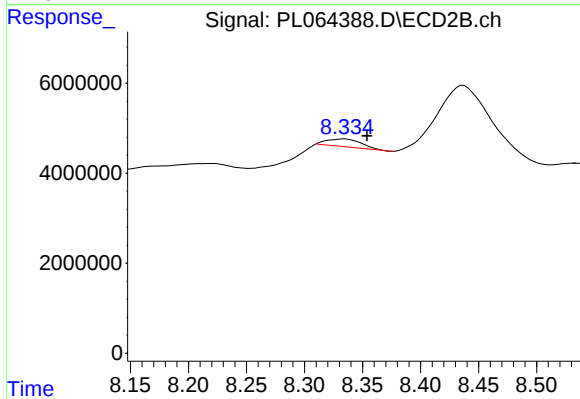

#22 Mirex


R.T.: 8.335 min
Delta R.T.: -0.019 min
Response: 3580839
Conc: 1.77 ng/ml

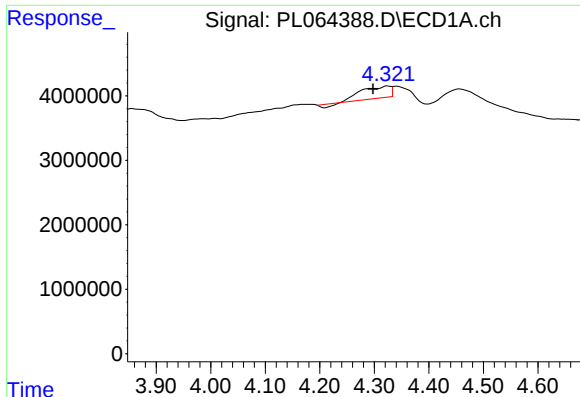

#23 Chlordane-1


R.T.: 4.324 min
Delta R.T.: 0.026 min
Response: 6341902
Conc: 54.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

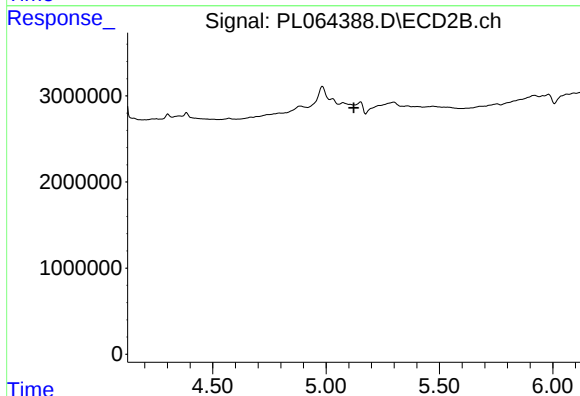


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.123 min
Response: 0
Conc: N.D.

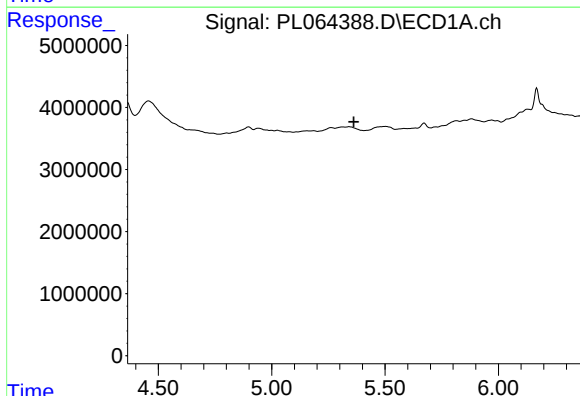


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.362 min
Response: 0
Conc: N.D.

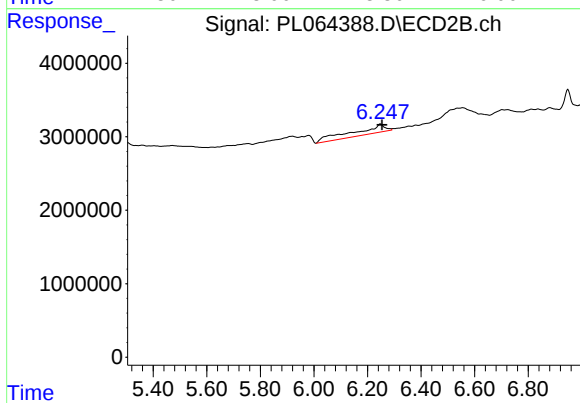

#25 Chlordane-3


R.T.: 6.248 min
Delta R.T.: -0.006 min
Response: 10056932
Conc: 24.87 ng/ml

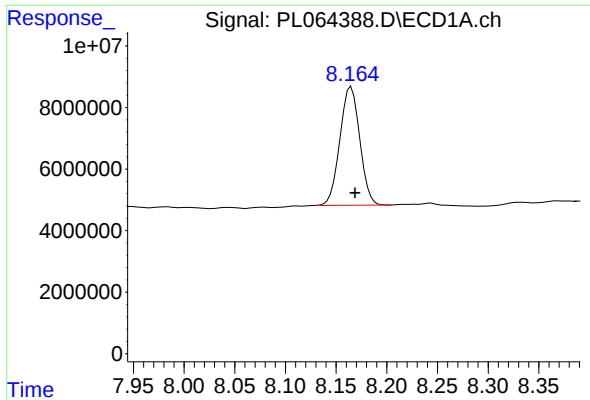

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: -0.004 min
Response: 52456237
Conc: 17.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

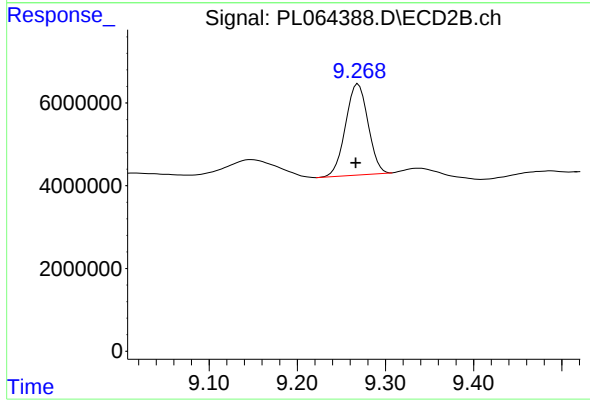

#28 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.003 min
Response: 38964262
Conc: 16.42 ng/ml