

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012521\
 Data File : PL064403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2021 18:54
 Operator : AR\AJ
 Sample : M1225-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 02:05:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.107	65389917	53234071	21.808	20.823
28)	SA Decachlor...	8.165	9.267	62166883	46833812	20.369	19.733
Target Compounds							
4)	MA Heptachlor	0.000	5.301	0	25302783	N.D.	7.045 #
10)	B gamma-Chl...	0.000	6.255	0	5965439	N.D.	1.985 #
11)	B alpha-Chl...	0.000	6.320	0	3081033	N.D.	1.012 #
12)	B 4,4'-DDE	5.583	6.481	8618735	4967378	2.447	1.865
16)	A 4,4'-DDD	6.098	6.980	572466	4575291	0.196	2.064 #
17)	MA 4,4'-DDT	6.335	7.280	4361124	5418722	1.461	2.392 #
25)	Chlordane-3	0.000	6.255	0	5965439	N.D.	14.754 #
26)	Chlordane-4	0.000	6.320	0	3081033	N.D.	6.233 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012521\
Data File : PL064403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2021 18:54
Operator : AR\AJ
Sample : M1225-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 02:05:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

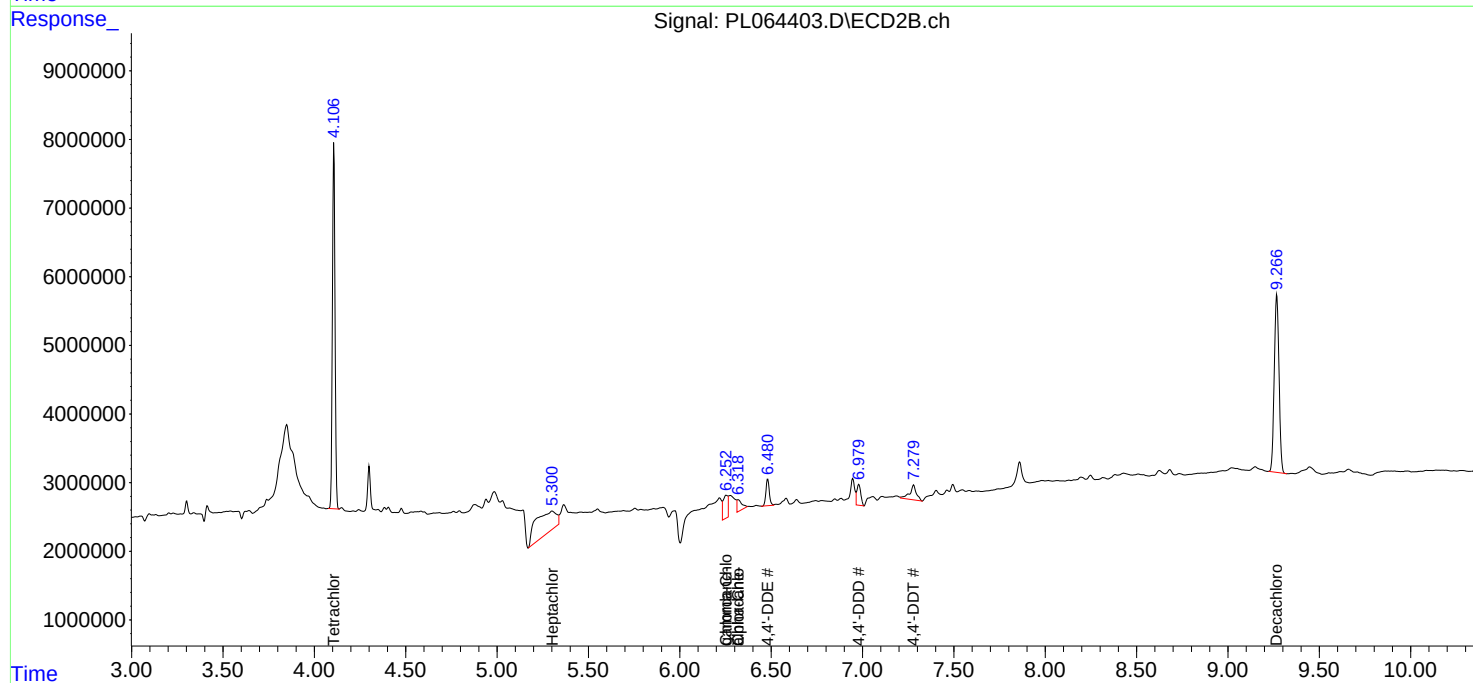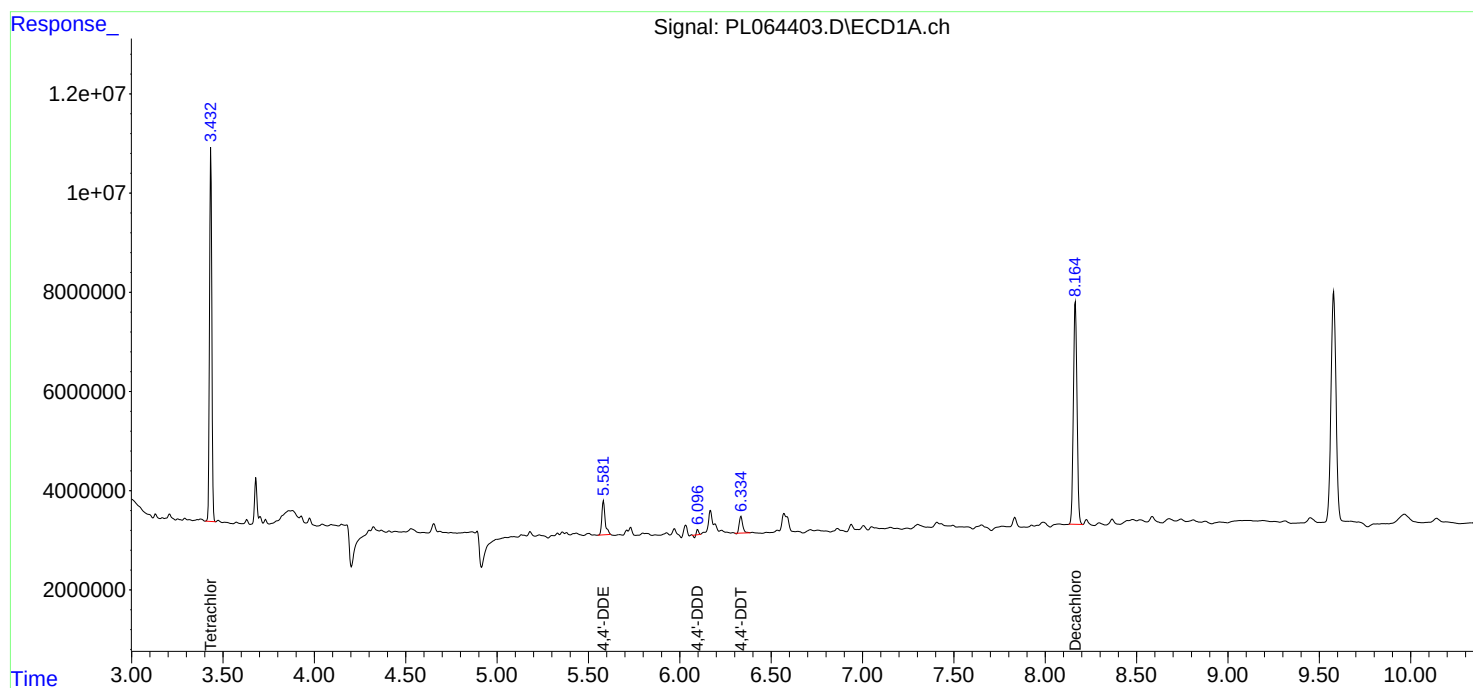


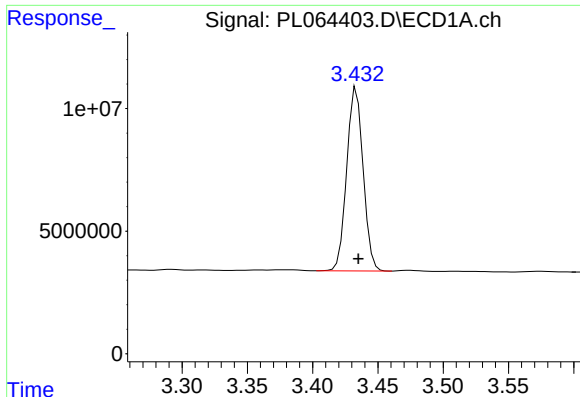

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: -0.001 min
Response: 65389917
Conc: 21.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

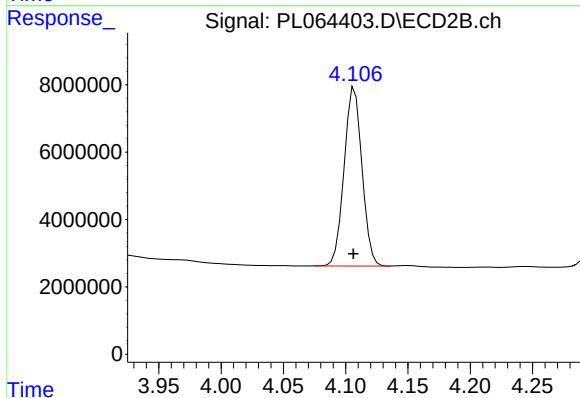


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 53234071
Conc: 20.82 ng/ml

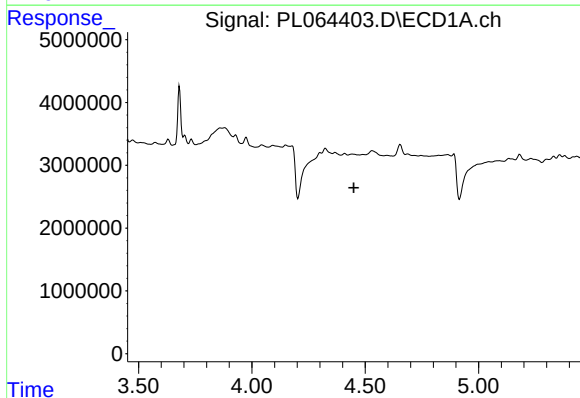


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

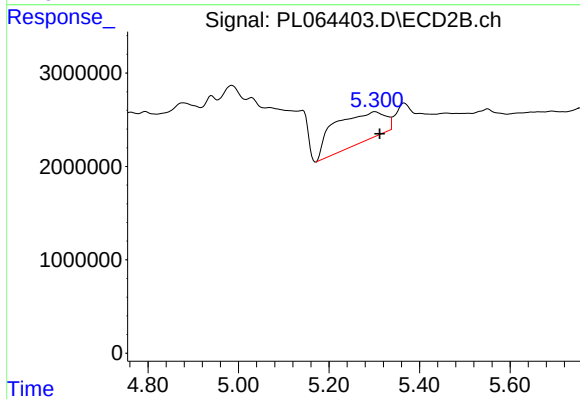

#4 Heptachlor


R.T.: 5.301 min
Delta R.T.: -0.011 min
Response: 25302783
Conc: 7.04 ng/ml

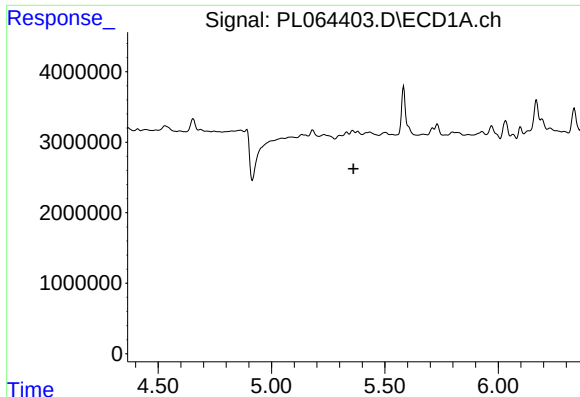

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

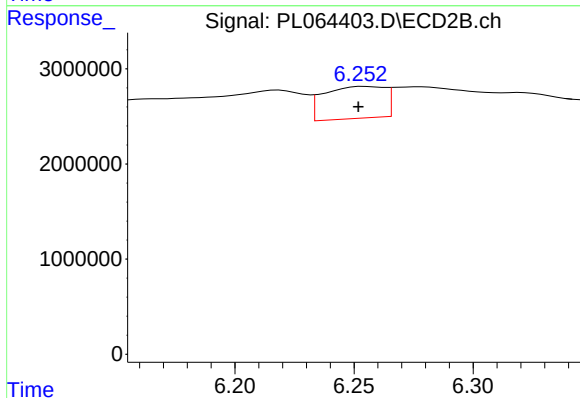


#10 gamma-Chlordane

R.T.: 6.255 min
Delta R.T.: 0.003 min
Response: 5965439
Conc: 1.99 ng/ml

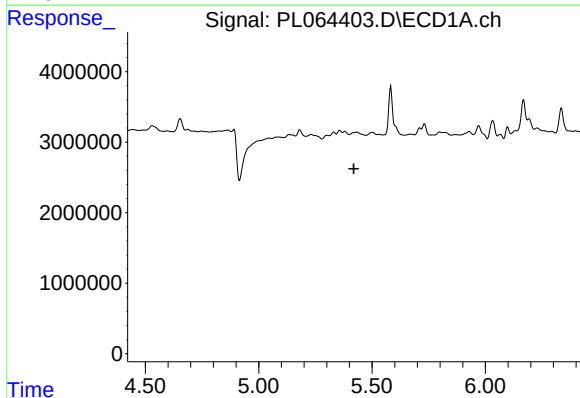


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.420 min
Response: 0
Conc: N.D.

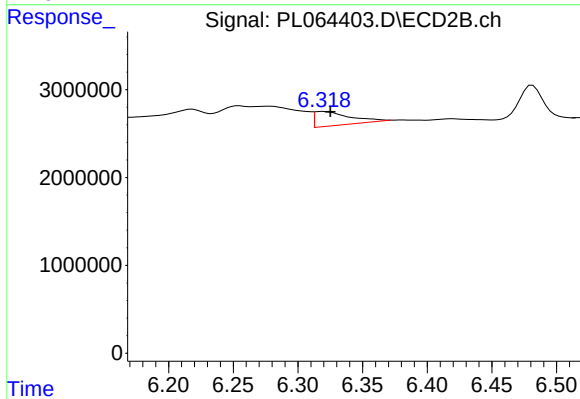

#11 alpha-Chlordane


R.T.: 6.320 min
Delta R.T.: -0.005 min
Response: 3081033
Conc: 1.01 ng/ml

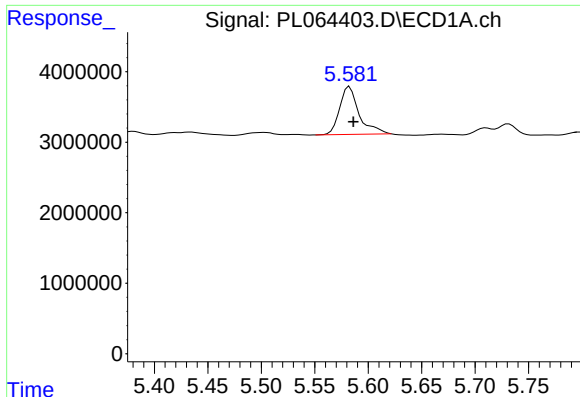

#12 4,4'-DDE


R.T.: 5.583 min
Delta R.T.: -0.003 min
Response: 8618735
Conc: 2.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

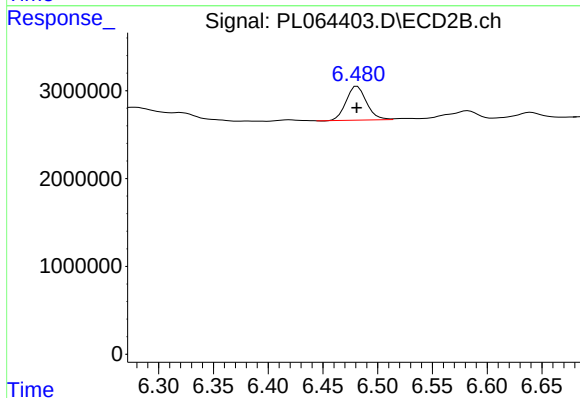


#12 4,4'-DDE

R.T.: 6.481 min
Delta R.T.: 0.000 min
Response: 4967378
Conc: 1.86 ng/ml

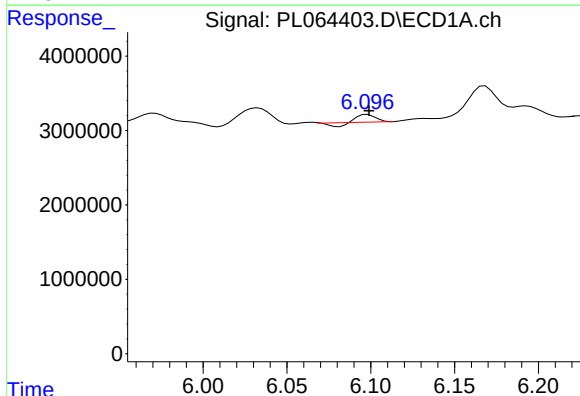


#16 4,4'-DDD

R.T.: 6.098 min
Delta R.T.: -0.001 min
Response: 572466
Conc: 0.20 ng/ml

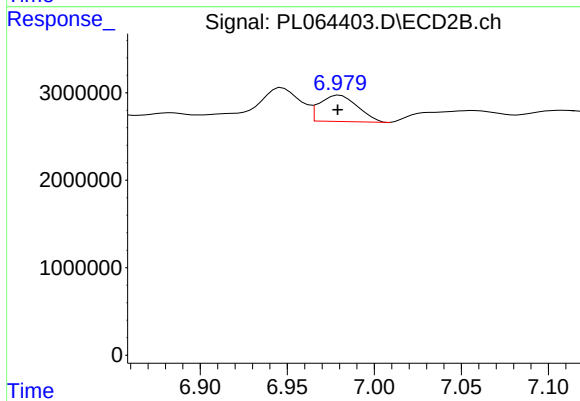

#16 4,4'-DDD


R.T.: 6.980 min
Delta R.T.: 0.001 min
Response: 4575291
Conc: 2.06 ng/ml

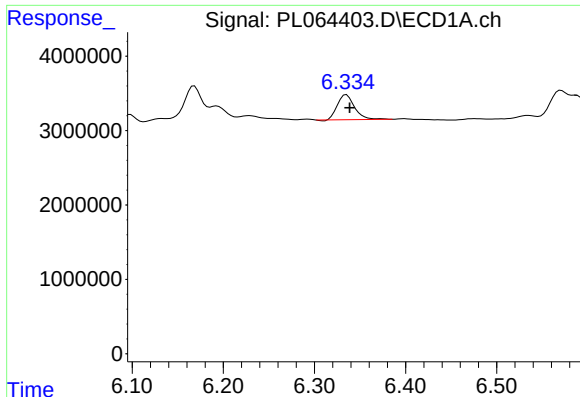

#17 4,4'-DDT


R.T.: 6.335 min
Delta R.T.: -0.004 min
Response: 4361124
Conc: 1.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

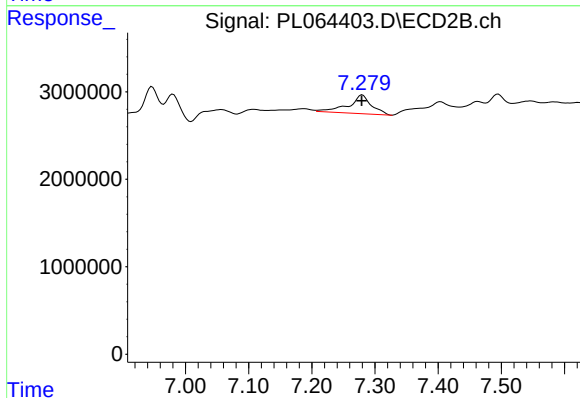


#17 4,4'-DDT

R.T.: 7.280 min
Delta R.T.: 0.000 min
Response: 5418722
Conc: 2.39 ng/ml

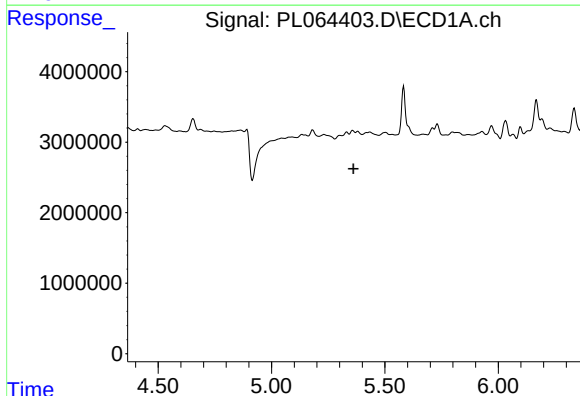


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.362 min
Response: 0
Conc: N.D.

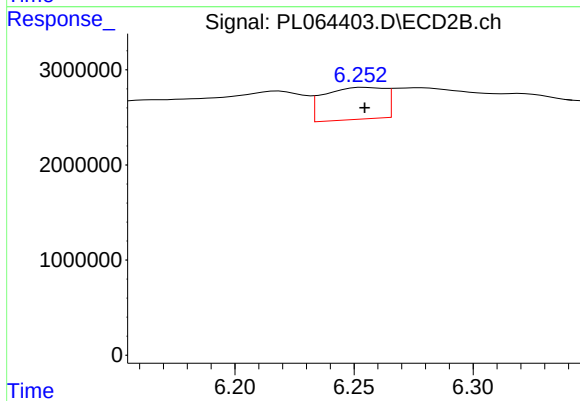

#25 Chlordane-3


R.T.: 6.255 min
Delta R.T.: 0.000 min
Response: 5965439
Conc: 14.75 ng/ml

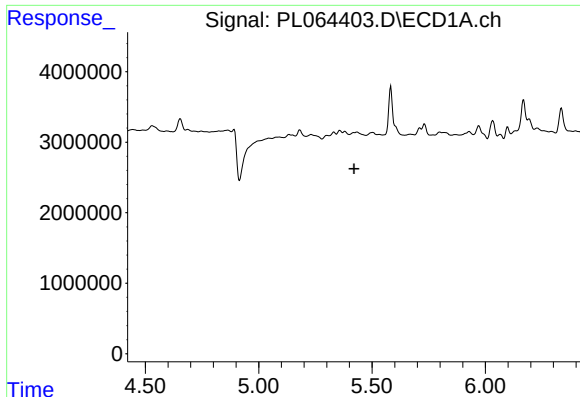

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

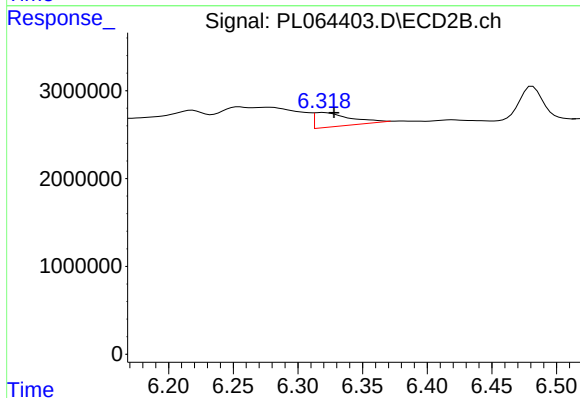


#26 Chlordane-4

R.T.: 6.320 min
Delta R.T.: -0.008 min
Response: 3081033
Conc: 6.23 ng/ml

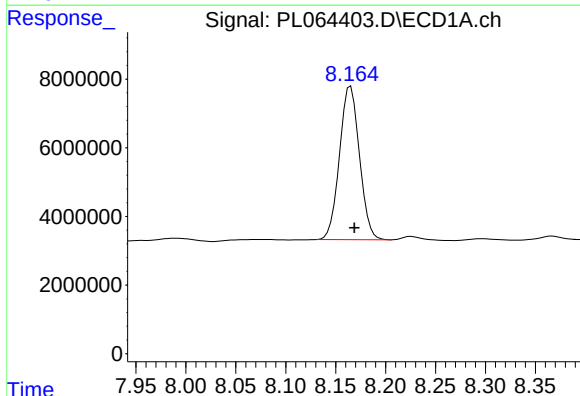

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: -0.004 min
Response: 62166883
Conc: 20.37 ng/ml

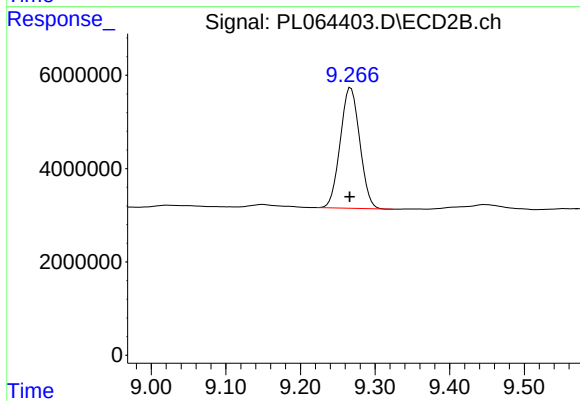

#28 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: 0.001 min
Response: 46833812
Conc: 19.73 ng/ml