

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012521\
 Data File : PL064385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2021 14:17
 Operator : AR\AJ
 Sample : M1188-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-230

Manual Integrations
 APPROVED

Ankita
 1/26/2021 10:13:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 02:01:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.107	55946391	46639851	18.658	18.244
28)	SA Decachlor...	8.165	9.268	42672460	40273407	13.981	16.969m
Target Compounds							
10)	B gamma-Chl...	5.356	6.253	3625955	14447949	0.936m	4.808 #
11)	B alpha-Chl...	5.417	6.326	3159971	2274450	0.826m	0.747m
12)	B 4,4'-DDE	5.586	6.484	4988858	5815673	1.416	2.183 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012521\
Data File : PL064385.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2021 14:17
Operator : AR\AJ
Sample : M1188-02
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-230


Manual Integrations
APPROVED

Ankita
1/26/2021 10:13:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 02:01:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

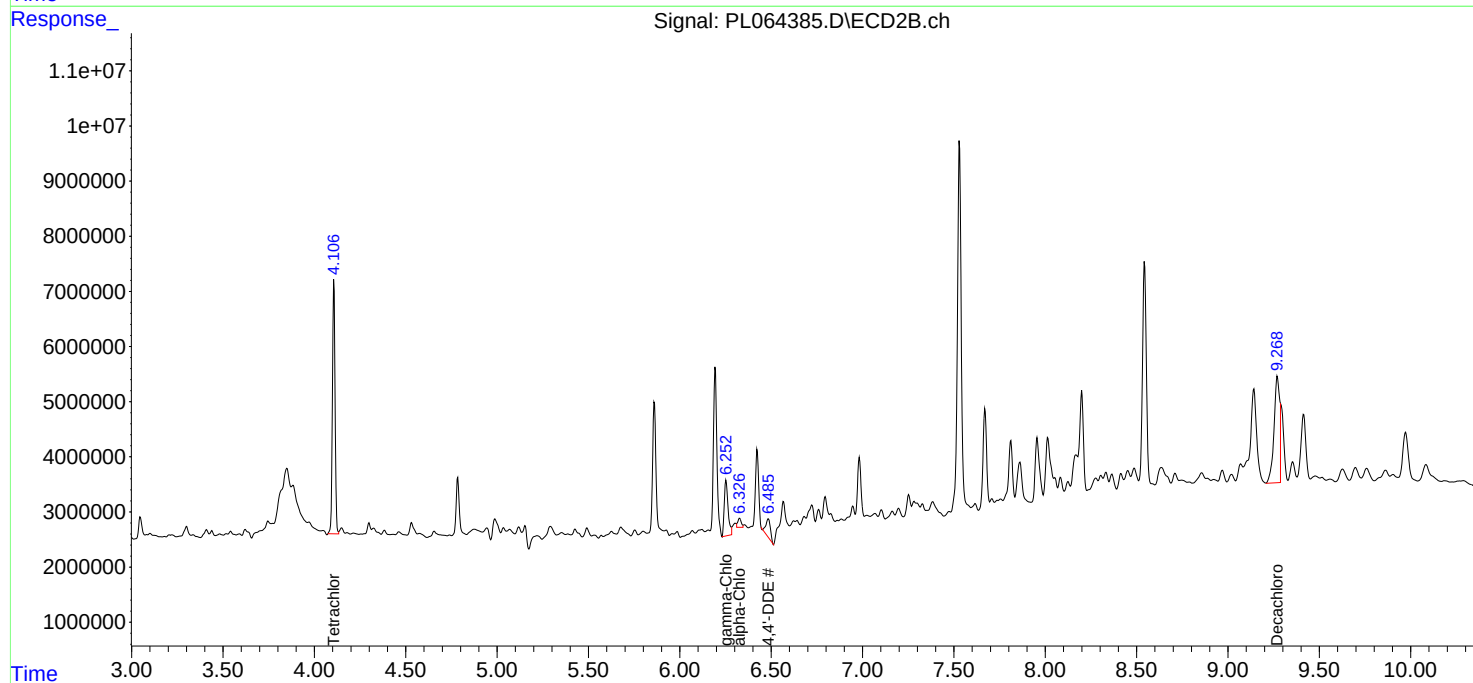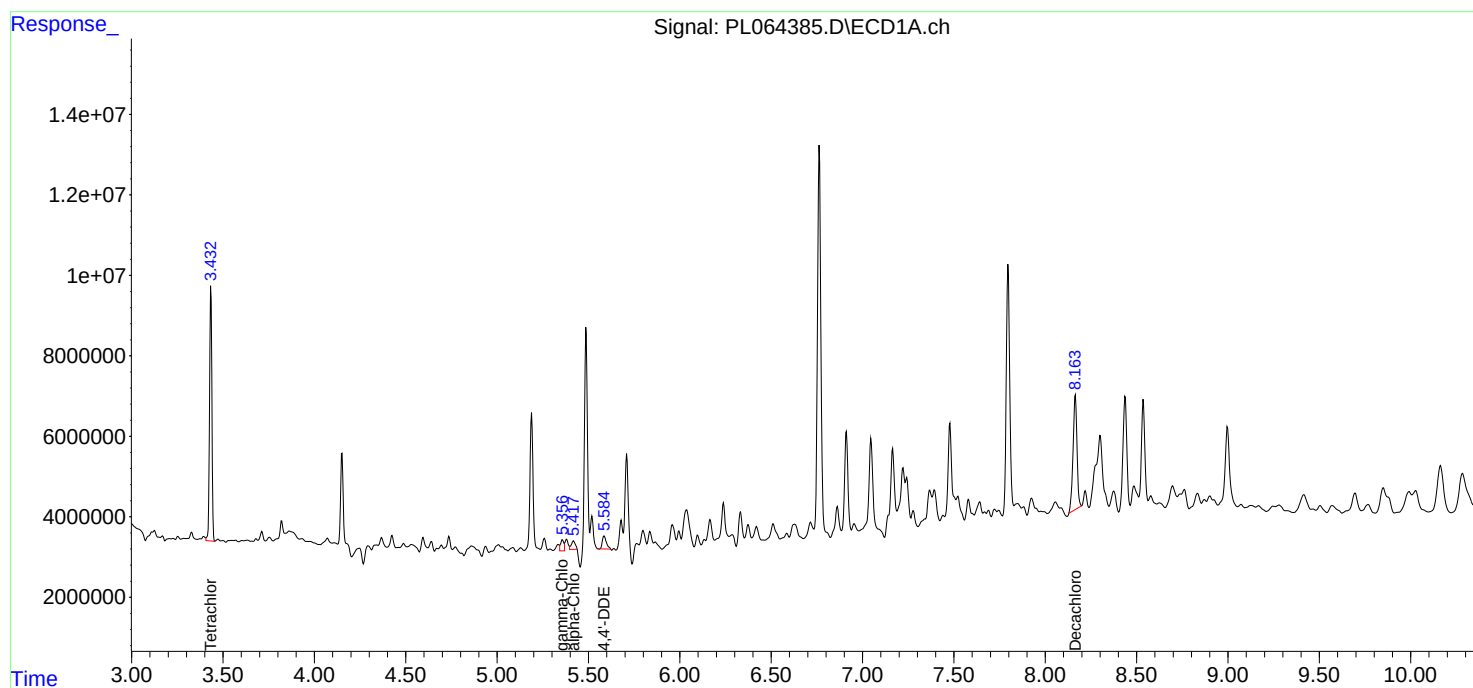

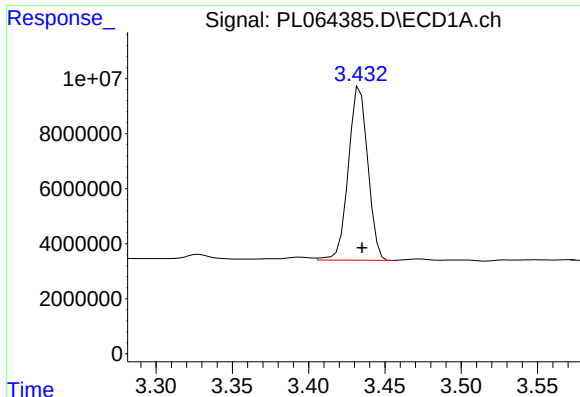


#1 Tetrachloro-m-xylene

R.T.: 3.434 min
Delta R.T.: -0.001 min
Response: 55946391
Conc: 18.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-230


Manual Integrations
APPROVED

Ankita
1/26/2021 10:13:54 AM

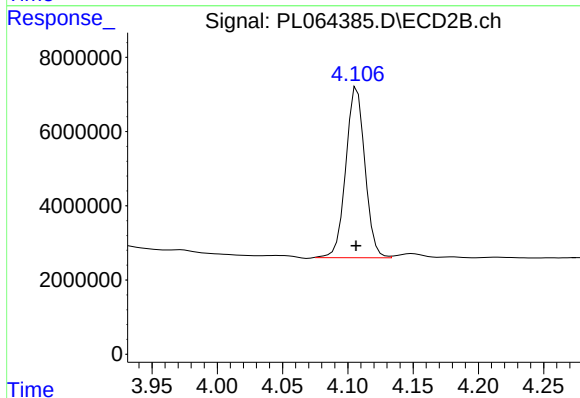


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 46639851
Conc: 18.24 ng/ml

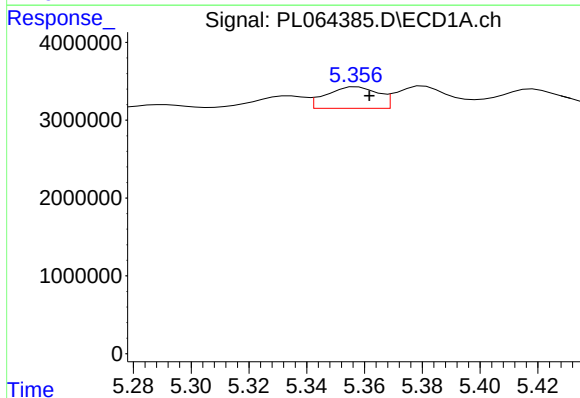


#10 gamma-Chlordane

R.T.: 5.356 min
Delta R.T.: -0.006 min
Response: 3625955
Conc: 0.94 ng/ml m

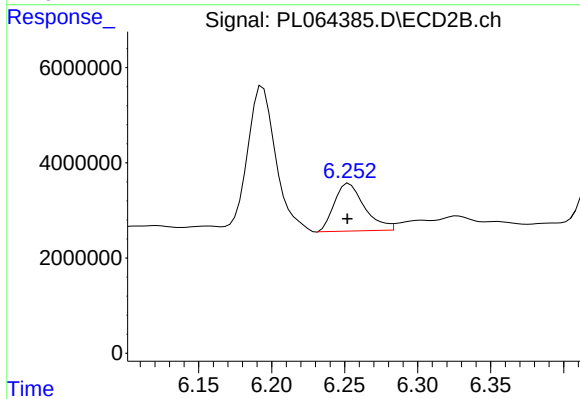

#10 gamma-Chlordane

R.T.: 6.253 min
Delta R.T.: 0.001 min
Response: 14447949
Conc: 4.81 ng/ml

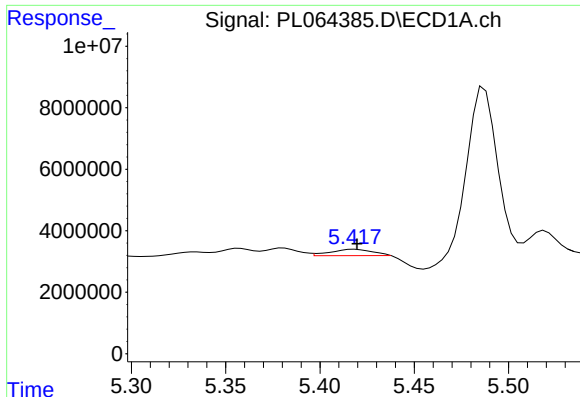


#11 alpha-Chlordane

R.T.: 5.417 min
Delta R.T.: -0.003 min
Response: 3159971
Conc: 0.83 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-230

Manual Integrations
APPROVED

Ankita
1/26/2021 10:13:54 AM

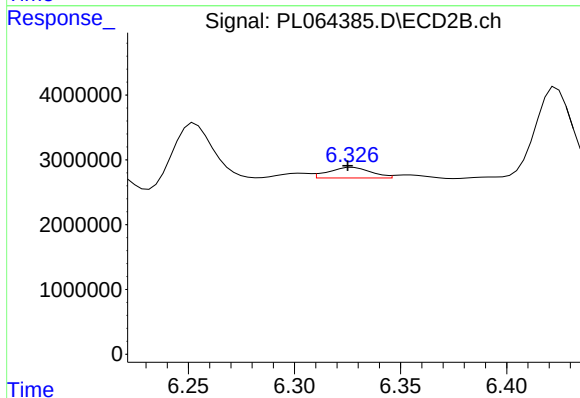


#11 alpha-Chlordane

R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 2274450
Conc: 0.75 ng/ml m


#12 4,4'-DDE

R.T.: 5.586 min
Delta R.T.: 0.000 min
Response: 4988858
Conc: 1.42 ng/ml

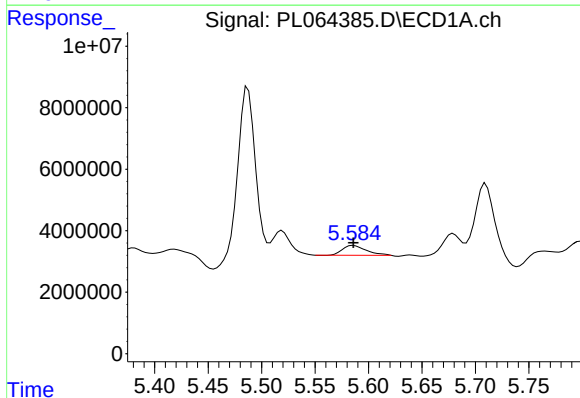

#12 4,4'-DDE

R.T.: 6.484 min
Delta R.T.: 0.004 min
Response: 5815673
Conc: 2.18 ng/ml

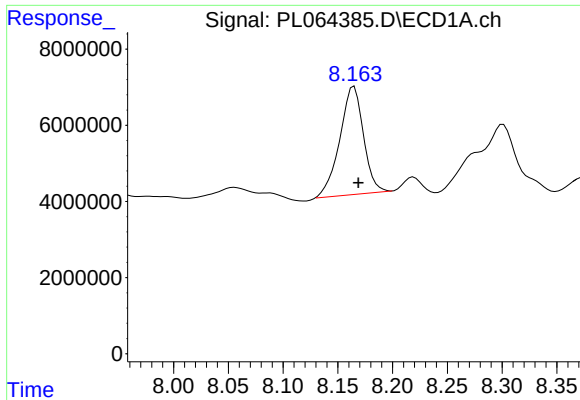


#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: -0.004 min
Response: 42672460
Conc: 13.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-230

Manual Integrations
APPROVED

Ankita
1/26/2021 10:13:54 AM

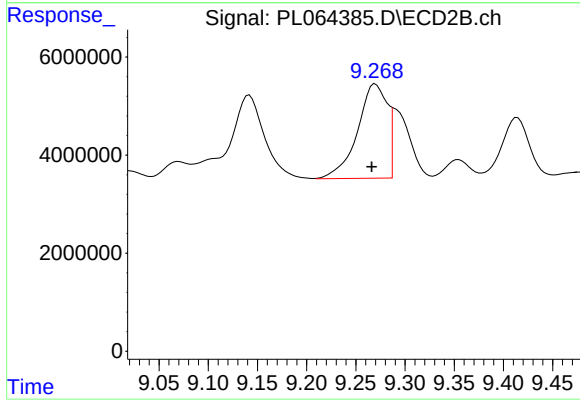

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.002 min
Response: 40273407
Conc: 16.97 ng/ml m