

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012521\
 Data File : PL064401.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2021 18:25
 Operator : AR\AJ
 Sample : M1225-04
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-4

Manual Integrations
 APPROVED

Ankita
 1/26/2021 10:14:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 02:05:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.107	69587030	54902756	23.207	21.476
28)	SA Decachlor...	8.165	9.269	57952082	43324791	18.988	18.254
Target Compounds							
12)	B 4,4'-DDE	5.583	6.483	21897184	15102376	6.216	5.670
13)	MA Dieldrin	5.709	6.641	4831183	1579958	1.299m	0.562 #
17)	MA 4,4'-DDT	6.335	7.282	16133619	11852858	5.404	5.233

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012521\
Data File : PL064401.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2021 18:25
Operator : AR\AJ
Sample : M1225-04
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
S-4


Manual Integrations
APPROVED

Ankita
1/26/2021 10:14:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 02:05:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

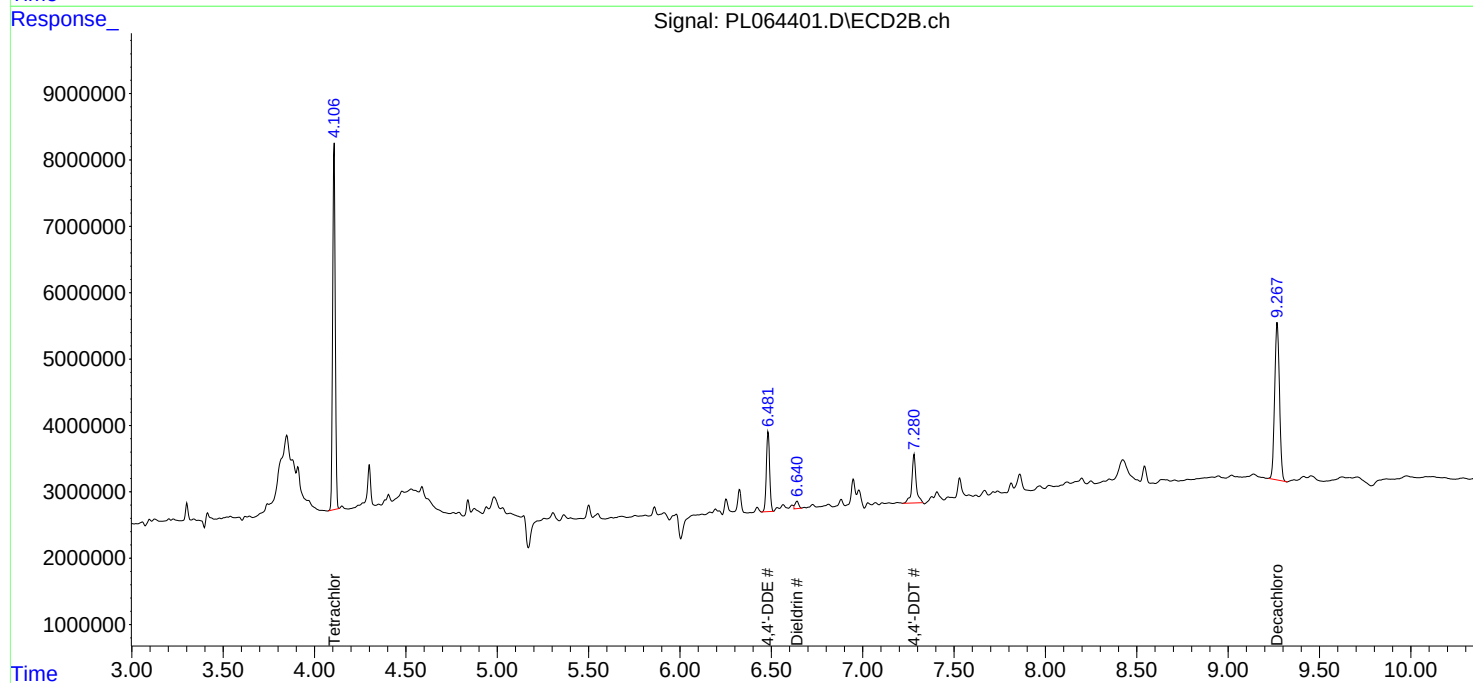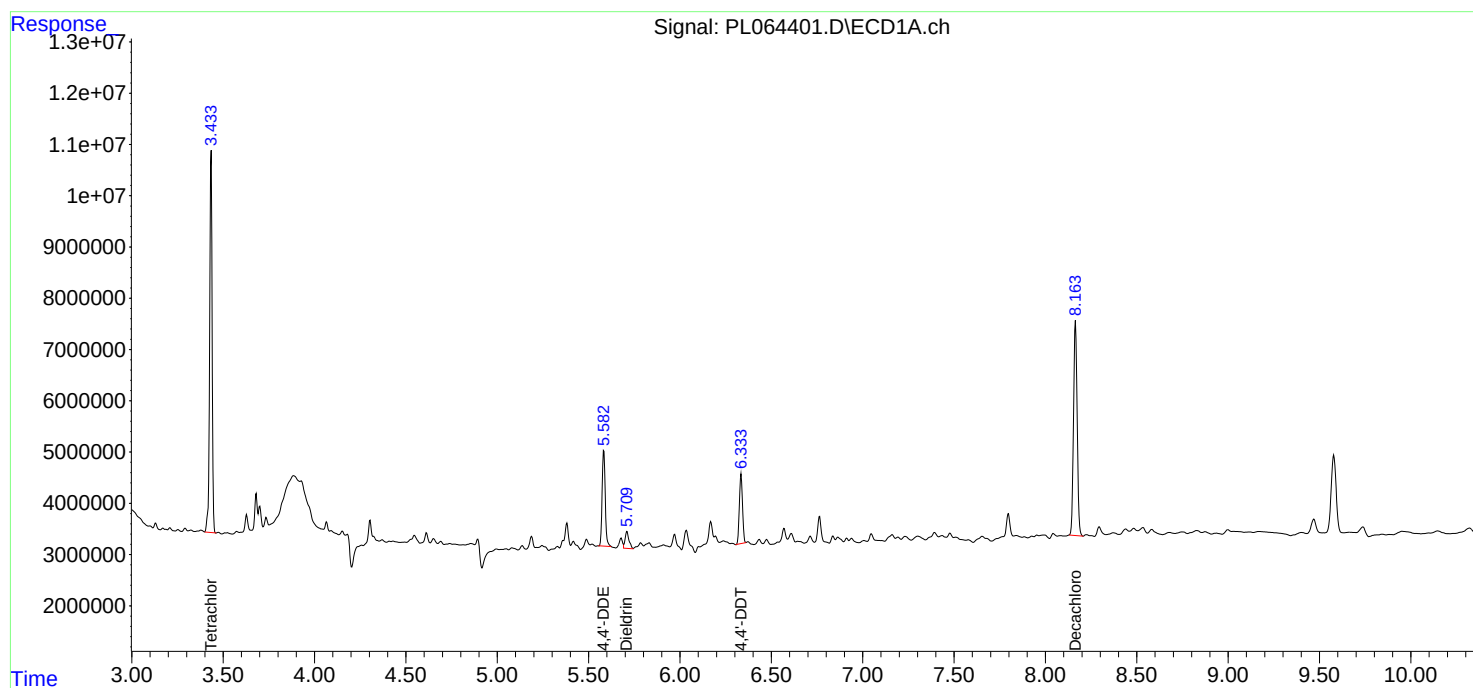

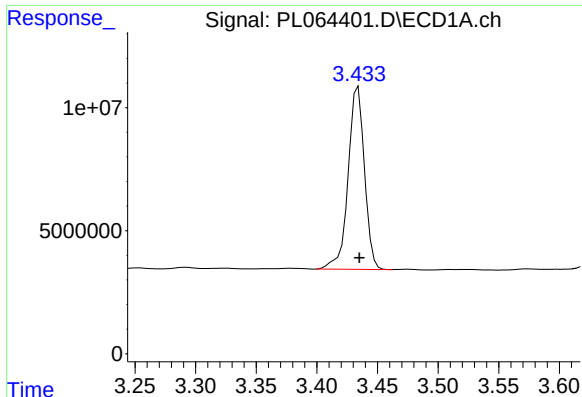


#1 Tetrachloro-m-xylene

R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 69587030
Conc: 23.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-4


Manual Integrations
APPROVED

Ankita
1/26/2021 10:14:10 AM

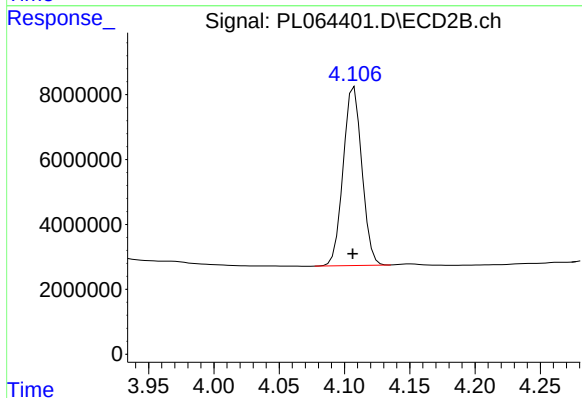


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.001 min
Response: 54902756
Conc: 21.48 ng/ml

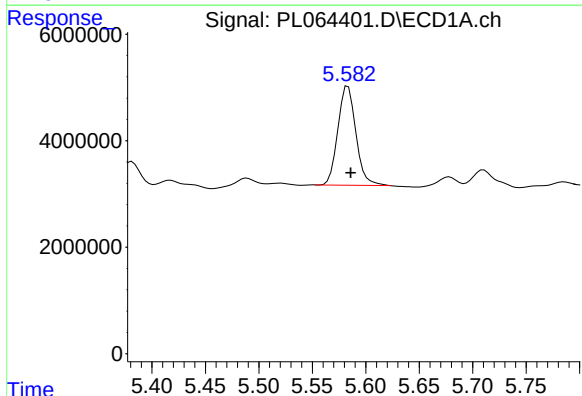


#12 4,4'-DDE

R.T.: 5.583 min
Delta R.T.: -0.003 min
Response: 21897184
Conc: 6.22 ng/ml

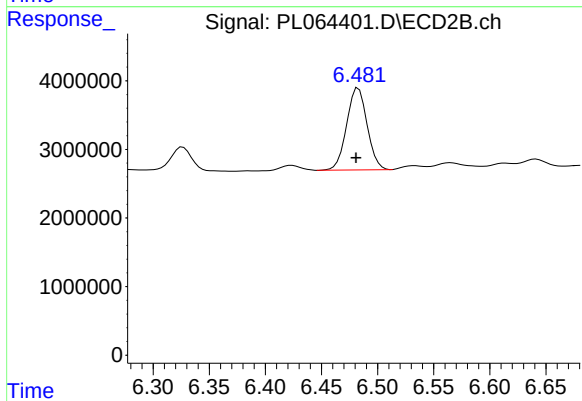

#12 4,4'-DDE

R.T.: 6.483 min
Delta R.T.: 0.002 min
Response: 15102376
Conc: 5.67 ng/ml

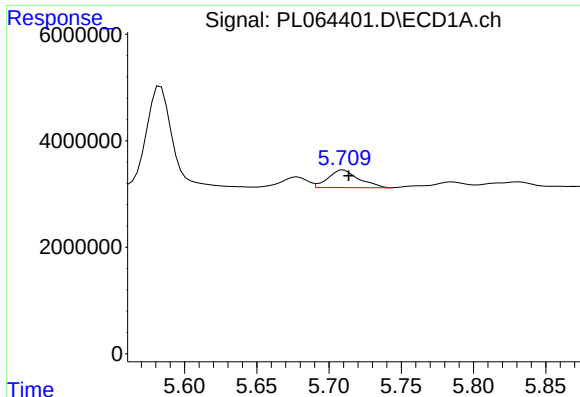


#13 Dieldrin

R.T.: 5.709 min
Delta R.T.: -0.005 min
Response: 4831183
Conc: 1.30 ng/ml m

Instrument :
ECD_L
ClientSampleId :
S-4


Manual Integrations
APPROVED

Ankita
1/26/2021 10:14:10 AM

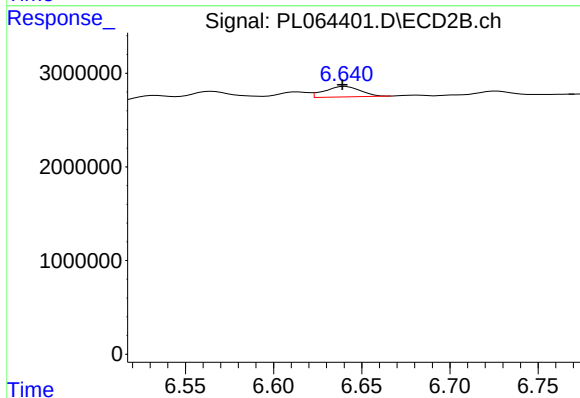


#13 Dieldrin

R.T.: 6.641 min
Delta R.T.: 0.002 min
Response: 1579958
Conc: 0.56 ng/ml

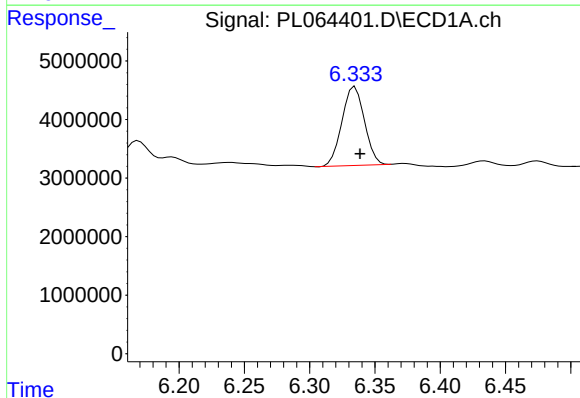


#17 4,4'-DDT

R.T.: 6.335 min
Delta R.T.: -0.004 min
Response: 16133619
Conc: 5.40 ng/ml

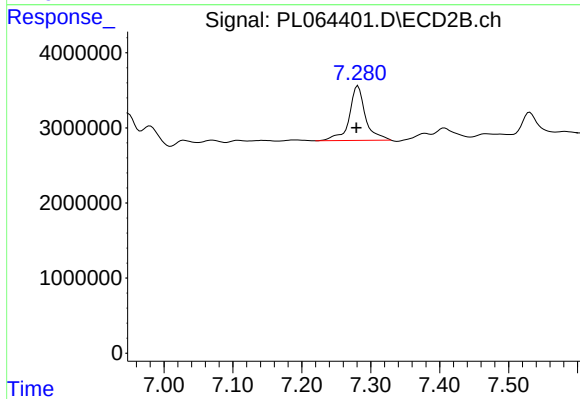

#17 4,4'-DDT

R.T.: 7.282 min
Delta R.T.: 0.002 min
Response: 11852858
Conc: 5.23 ng/ml

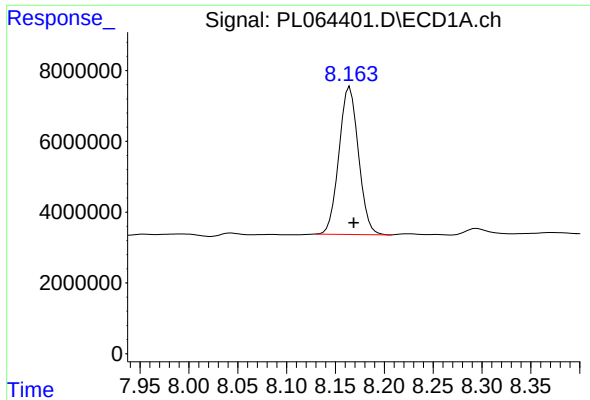


#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: -0.004 min
Response: 57952082
Conc: 18.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-4

Manual Integrations
APPROVED

Ankita
1/26/2021 10:14:10 AM

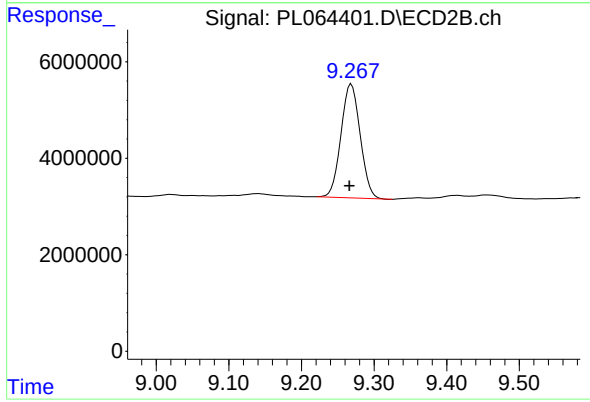

#28 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.002 min
Response: 43324791
Conc: 18.25 ng/ml