

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
 Data File : PL072231.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2022 14:19
 Operator : AR\AJ
 Sample : N1099-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 00:39:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	6222343	18565703	11.208	11.431
28)	SA Decachlor...	10.318	11.386	11311589	21888561	12.732	13.566
Target Compounds							
5)	MB Aldrin	0.000	7.511f	0	500974	N.D.	0.227 #
7)	B delta-BHC	0.000	7.017f	0	920759	N.D.	0.374 #
8)	B Heptachlo...	0.000	7.965	0	779417	N.D.	0.389 #
9)	A Endosulfan I	0.000	8.350	0	121699	N.D.	0.067 #
11)	B alpha-Chl...	0.000	8.317	0	786359	N.D.	0.397 #
15)	B Endosulfa...	8.263f	9.146f	8116	145163	0.011	0.085 #
19)	B Endosulfa...	8.699	0.000	246690	0	0.336	N.D. #
20)	A Methoxychlor	0.000	9.872f	0	2984631	N.D.	3.603 #
26)	Chlordane-4	0.000	8.317	0	786359	N.D.	2.368 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
Data File : PL072231.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2022 14:19
Operator : AR\AJ
Sample : N1099-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 00:39:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

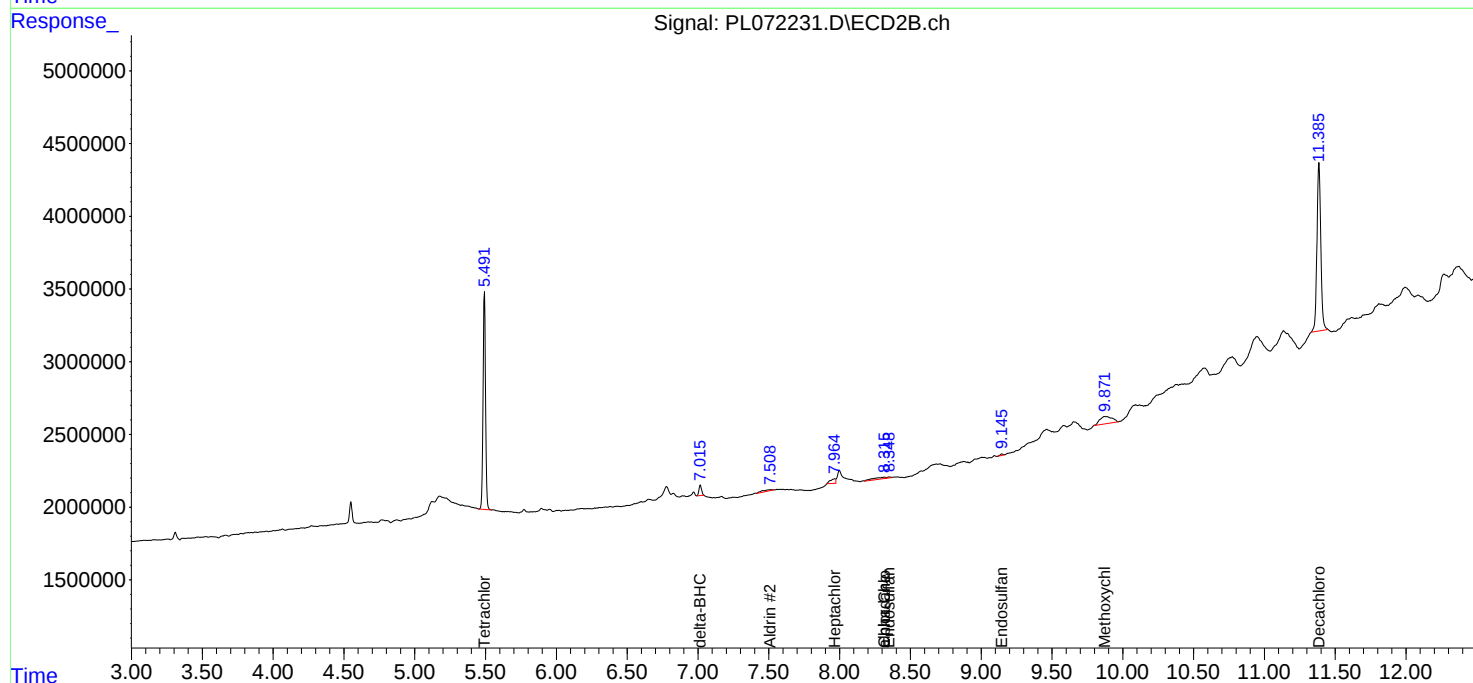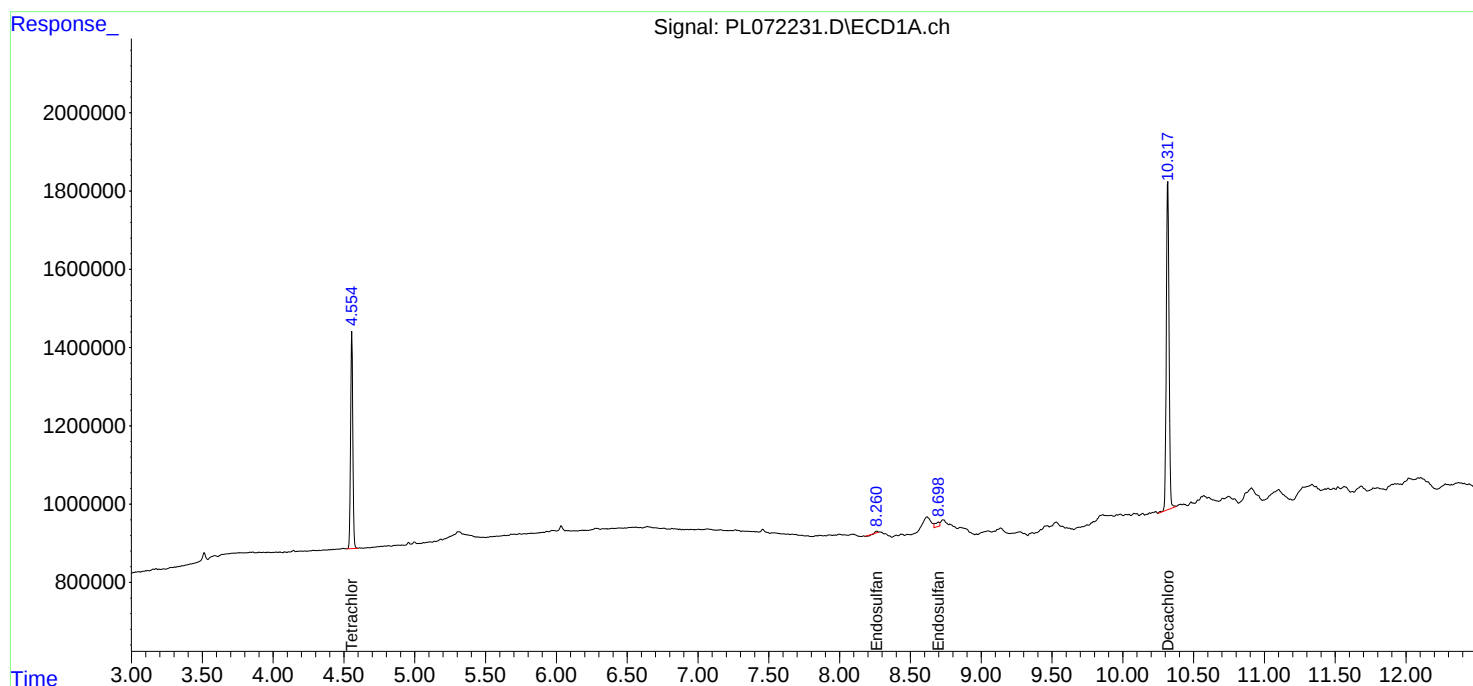


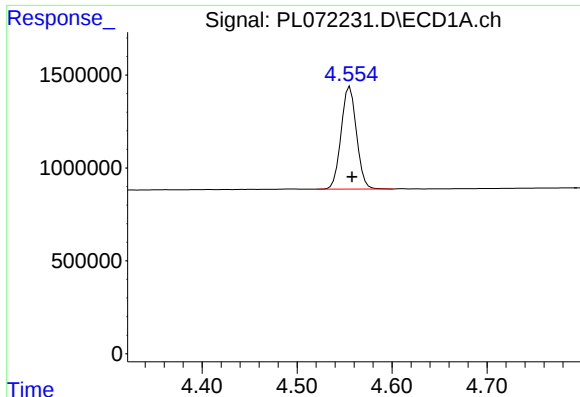

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 6222343
Conc: 11.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-02

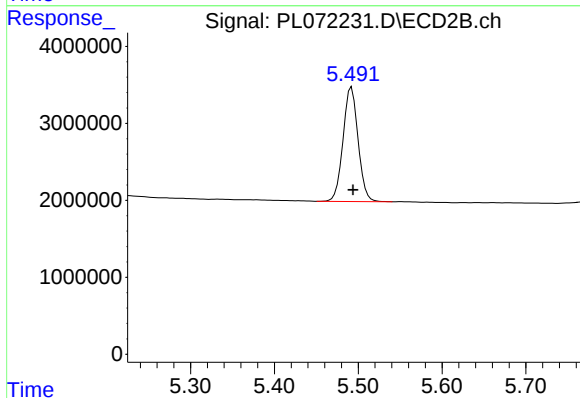


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 18565703
Conc: 11.43 ng/ml

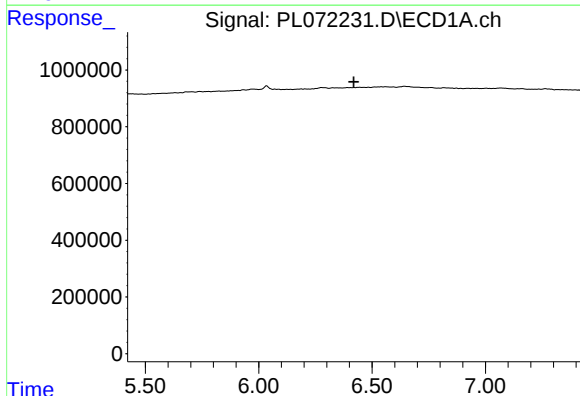


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.419 min
Response: 0
Conc: N.D.

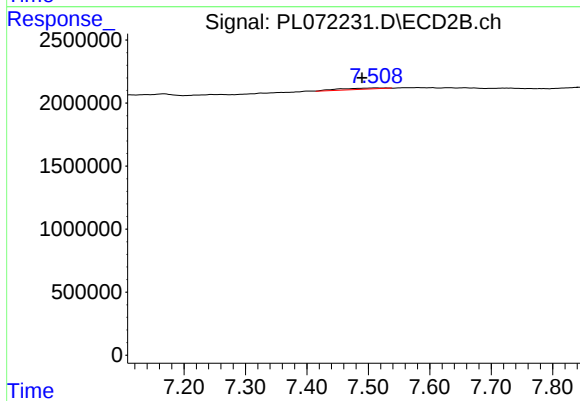

#5 Aldrin


R.T.: 7.511 min
Delta R.T.: 0.021 min
Response: 500974
Conc: 0.23 ng/ml

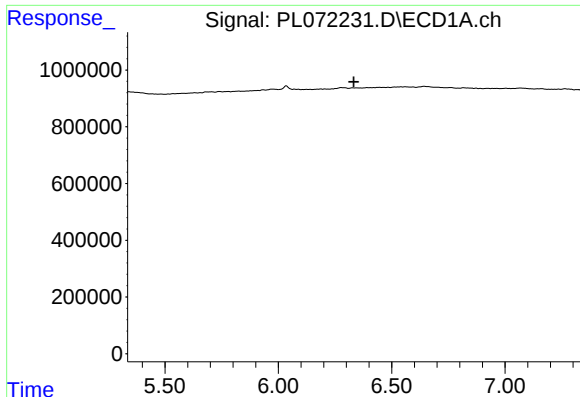

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-02

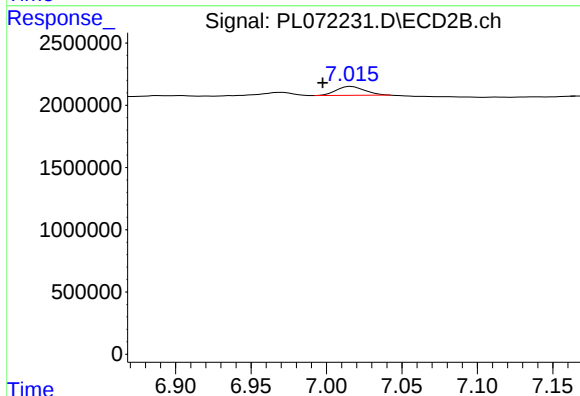


#7 delta-BHC

R.T.: 7.017 min
Delta R.T.: 0.019 min
Response: 920759
Conc: 0.37 ng/ml

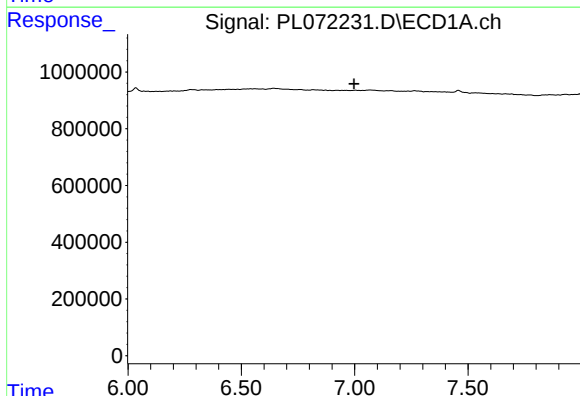


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.998 min
Response: 0
Conc: N.D.

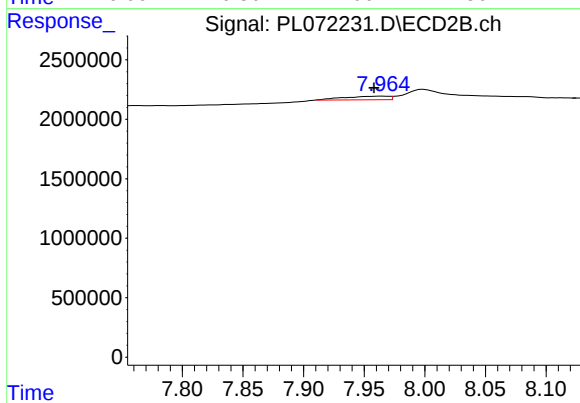

#8 Heptachlor epoxide


R.T.: 7.965 min
Delta R.T.: 0.007 min
Response: 779417
Conc: 0.39 ng/ml

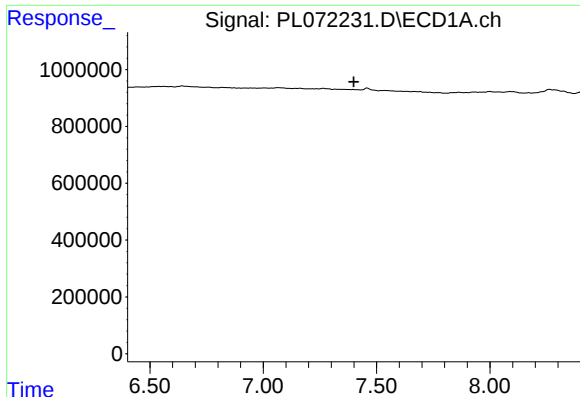

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-02

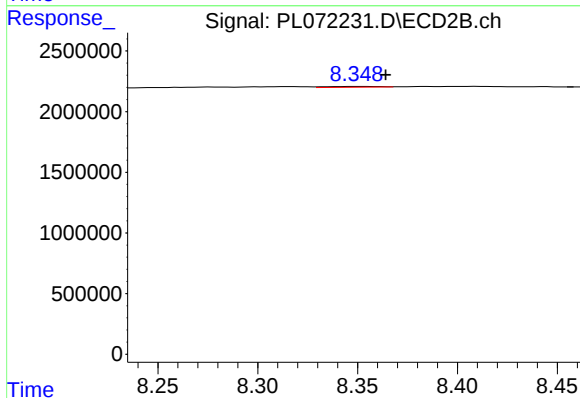


#9 Endosulfan I

R.T.: 8.350 min
Delta R.T.: -0.014 min
Response: 121699
Conc: 0.07 ng/ml

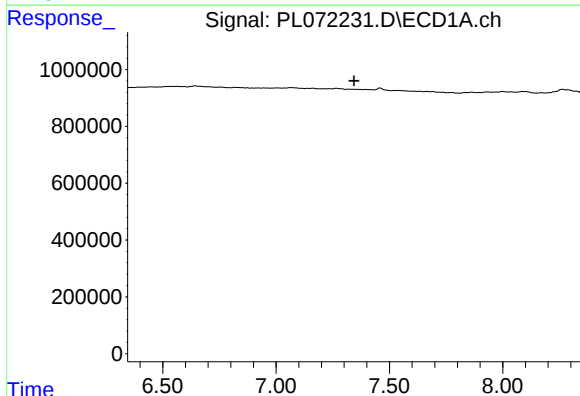


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

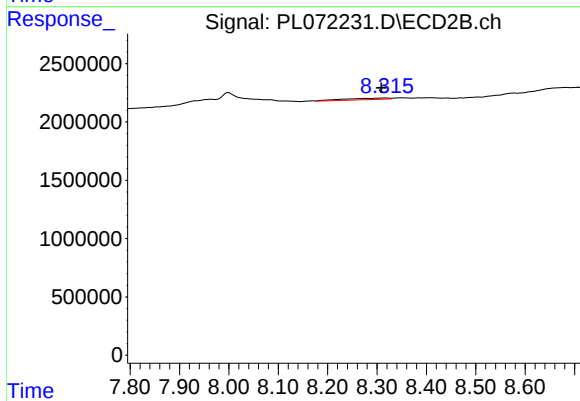

#11 alpha-Chlordane


R.T.: 8.317 min
Delta R.T.: 0.009 min
Response: 786359
Conc: 0.40 ng/ml

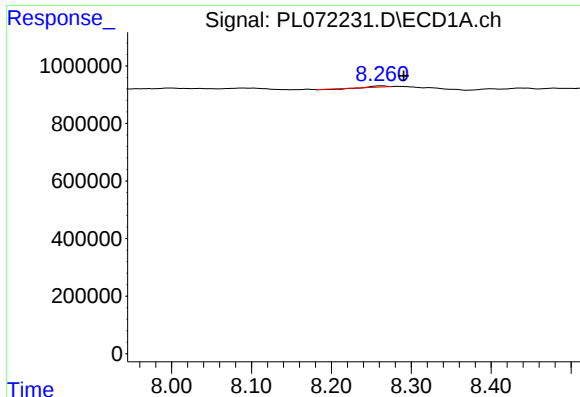

#15 Endosulfan II


R.T.: 8.263 min
Delta R.T.: -0.028 min
Response: 8116
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-02

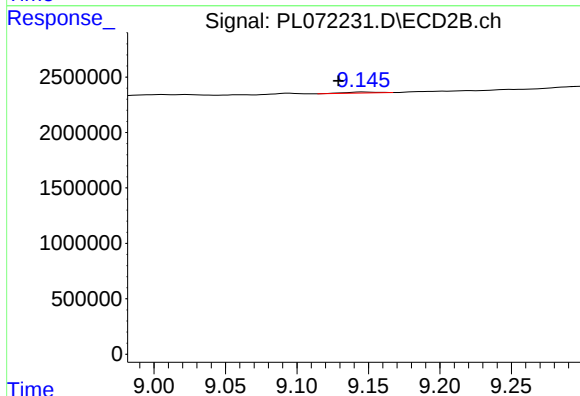


#15 Endosulfan II

R.T.: 9.146 min
Delta R.T.: 0.017 min
Response: 145163
Conc: 0.08 ng/ml

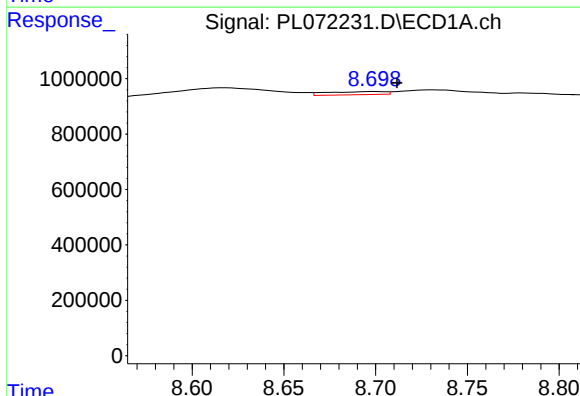


#19 Endosulfan Sulfate

R.T.: 8.699 min
Delta R.T.: -0.013 min
Response: 246690
Conc: 0.34 ng/ml

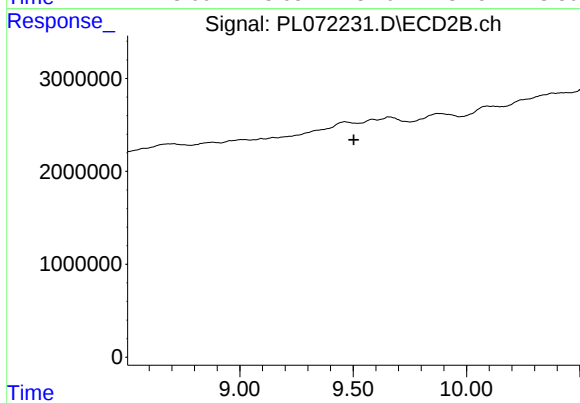

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.502 min
Response: 0
Conc: N.D.

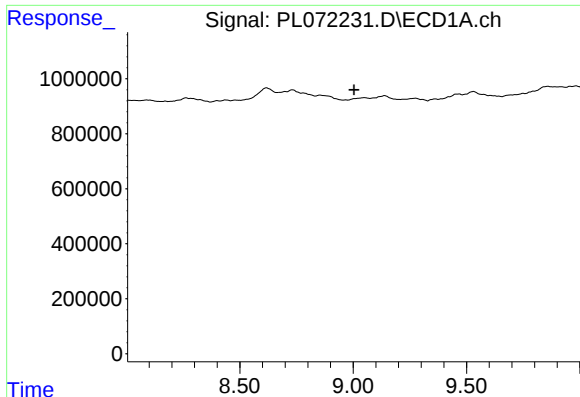

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-02

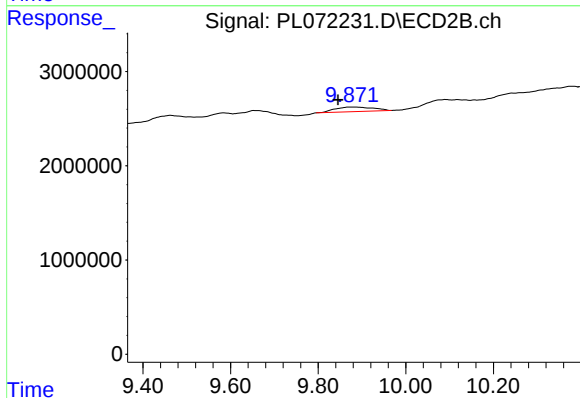


#20 Methoxychlor

R.T.: 9.872 min
Delta R.T.: 0.027 min
Response: 2984631
Conc: 3.60 ng/ml

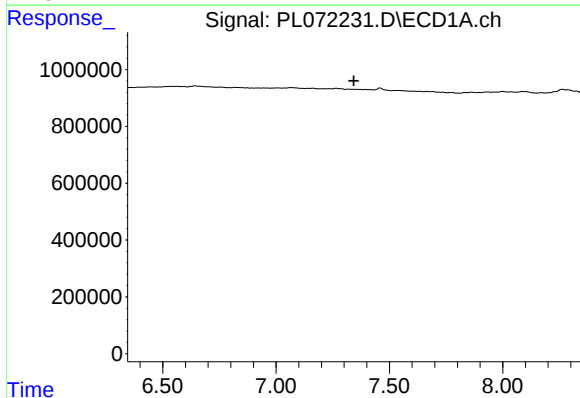


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

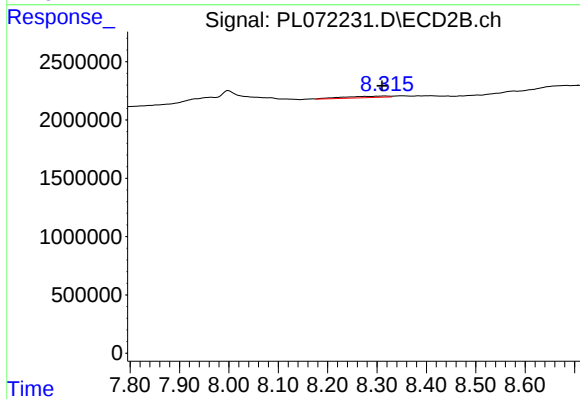

#26 Chlordane-4


R.T.: 8.317 min
Delta R.T.: 0.007 min
Response: 786359
Conc: 2.37 ng/ml

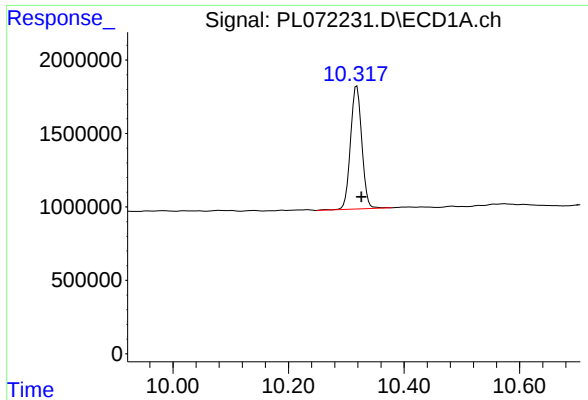

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.008 min
Response: 11311589
Conc: 12.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-02

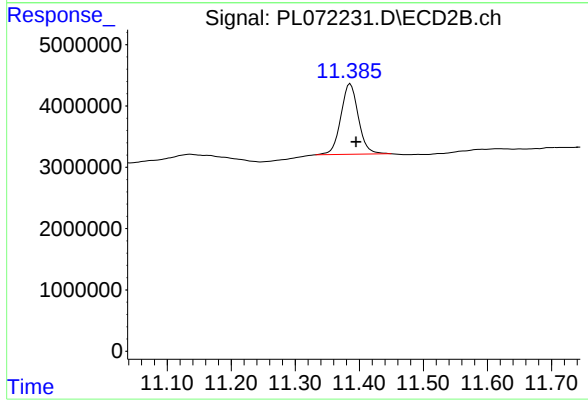

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.009 min
Response: 21888561
Conc: 13.57 ng/ml