

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
 Data File : PL072234.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2022 15:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 00:39:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	10086419	29892775	18.168	18.406
28)	SA Decachlor...	10.318	11.386	16863415	30320897	18.981	18.792
Target Compounds							
7)	B delta-BHC	0.000	7.016f	0	1365077	N.D.	0.555 #
10)	B gamma-Chl...	0.000	8.230	0	142742	N.D.	0.071 #
11)	B alpha-Chl...	0.000	8.324f	0	117281	N.D.	0.059 #
15)	B Endosulfa...	0.000	9.148f	0	209261	N.D.	0.122 #
16)	A 4,4'-DDD	0.000	9.027	0	60237	N.D.	0.042 #
18)	B Endrin al...	0.000	9.288f	0	52209	N.D.	0.042 #
19)	B Endosulfa...	0.000	9.522f	0	116376	N.D.	0.075 #
25)	Chlordane-3	0.000	8.230	0	142742	N.D.	0.514 #
26)	Chlordane-4	0.000	8.324	0	117281	N.D.	0.353 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
Data File : PL072234.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2022 15:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 00:39:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

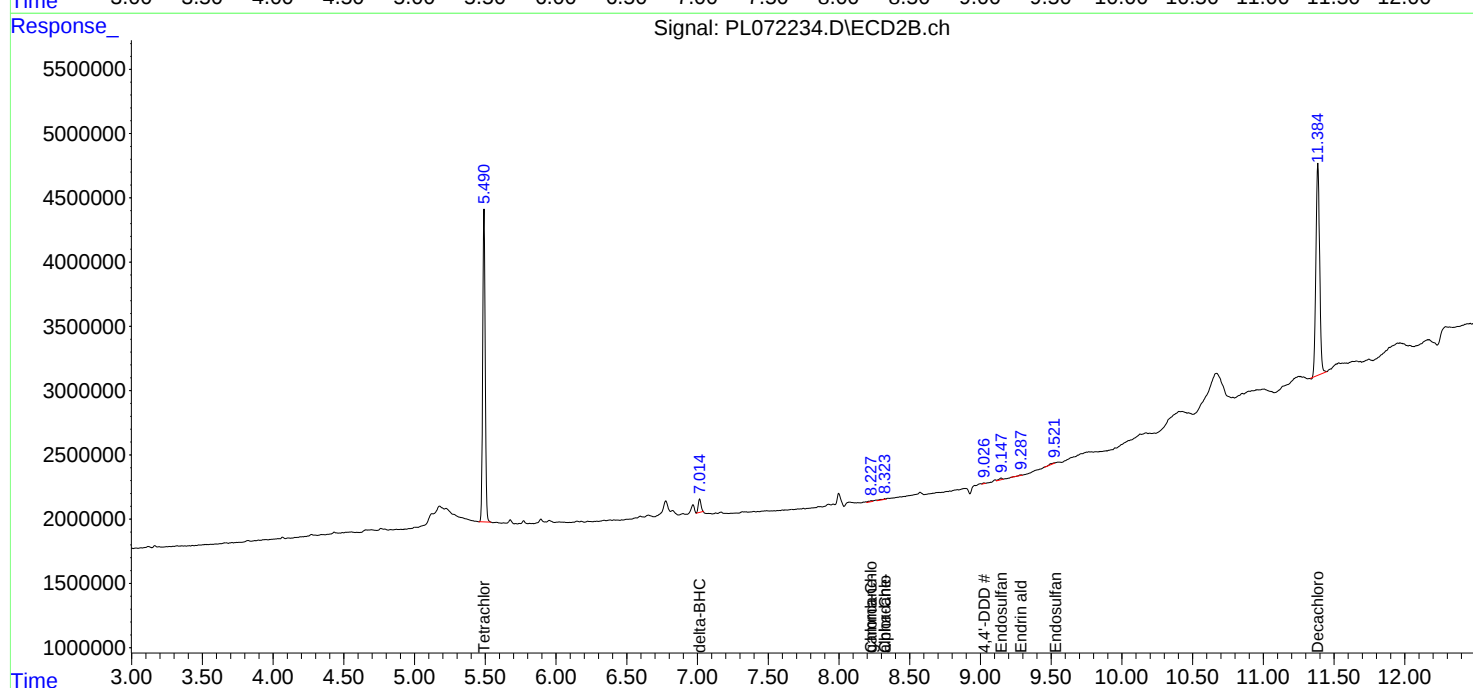


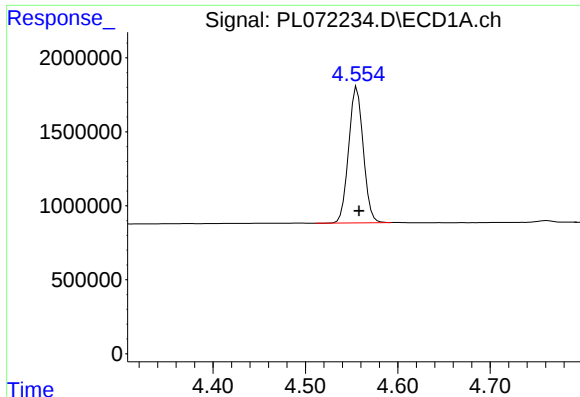

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 10086419
Conc: 18.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

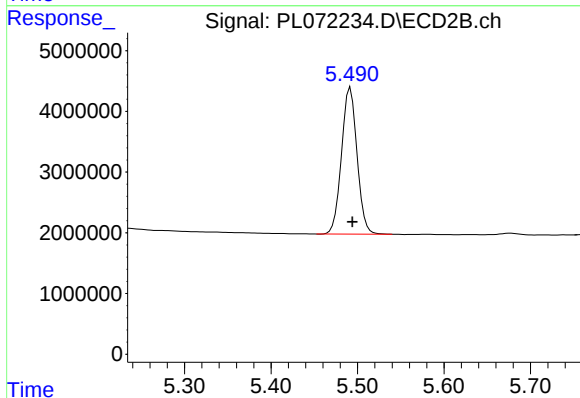


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 29892775
Conc: 18.41 ng/ml

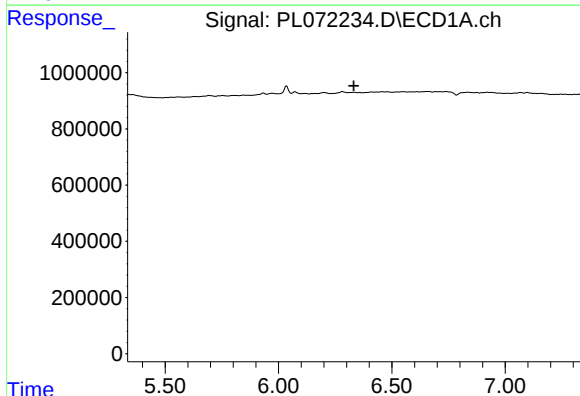


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

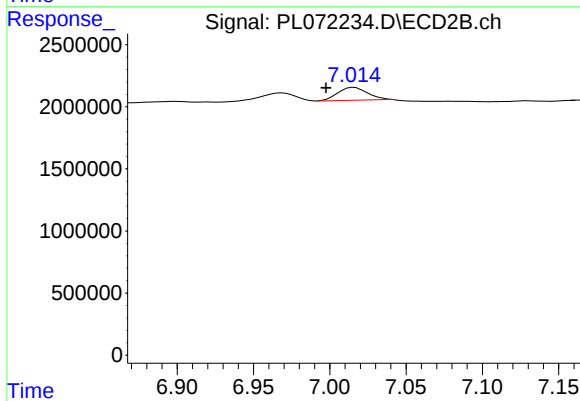

#7 delta-BHC


R.T.: 7.016 min
Delta R.T.: 0.018 min
Response: 1365077
Conc: 0.55 ng/ml

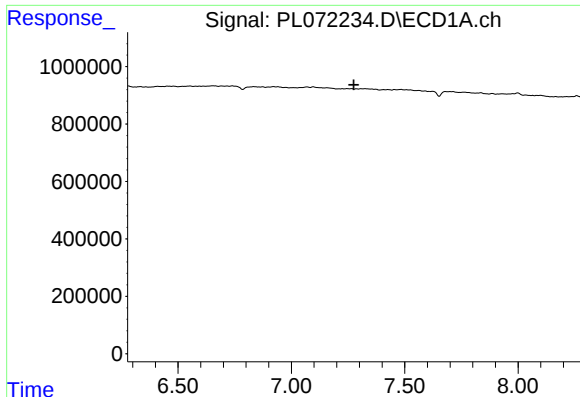

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

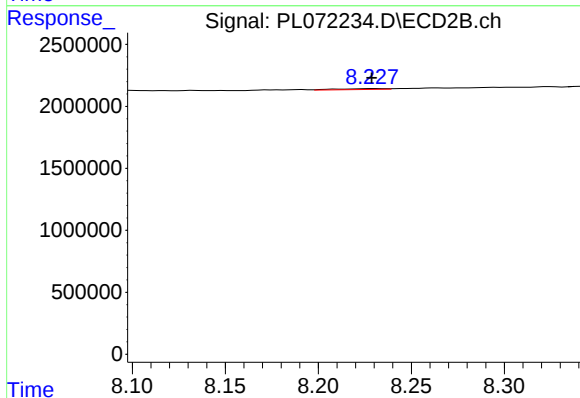


#10 gamma-Chlordane

R.T.: 8.230 min
Delta R.T.: 0.000 min
Response: 142742
Conc: 0.07 ng/ml

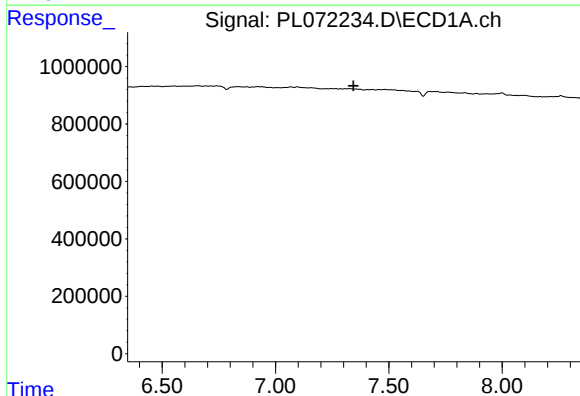


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

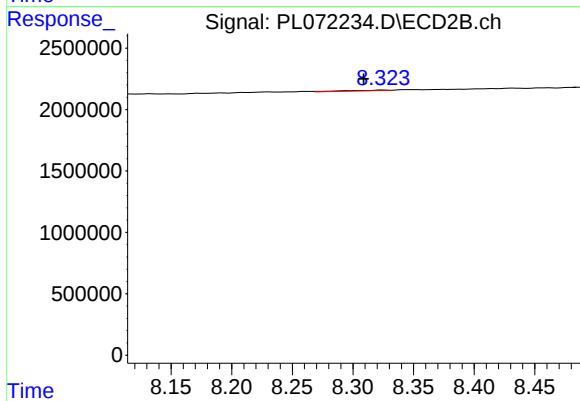

#11 alpha-Chlordane


R.T.: 8.324 min
Delta R.T.: 0.015 min
Response: 117281
Conc: 0.06 ng/ml

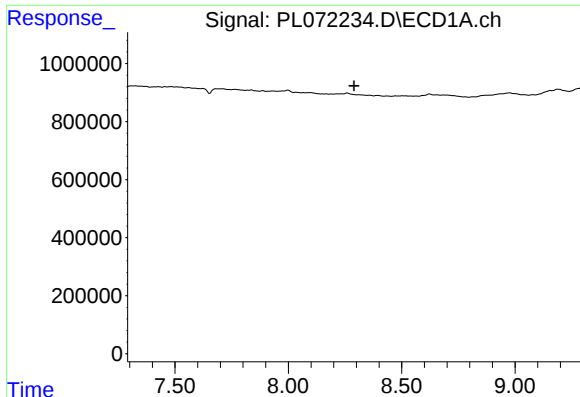

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

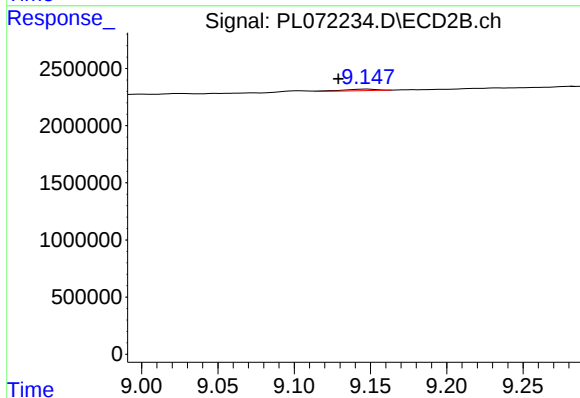


#15 Endosulfan II

R.T.: 9.148 min
Delta R.T.: 0.019 min
Response: 209261
Conc: 0.12 ng/ml

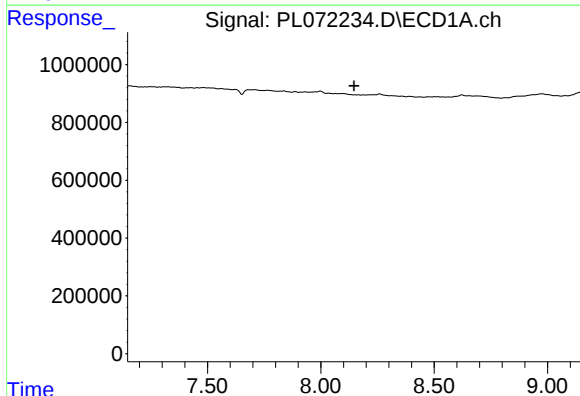


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

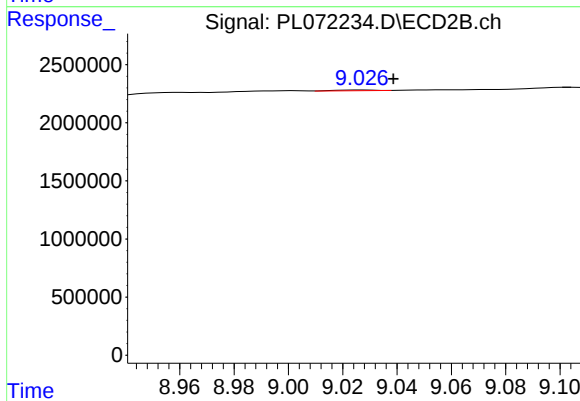

#16 4,4'-DDD


R.T.: 9.027 min
Delta R.T.: -0.012 min
Response: 60237
Conc: 0.04 ng/ml

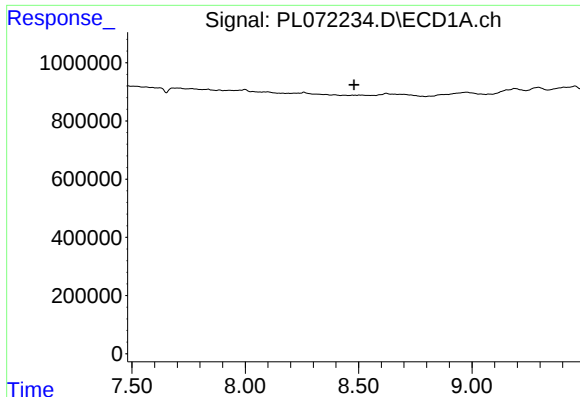

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

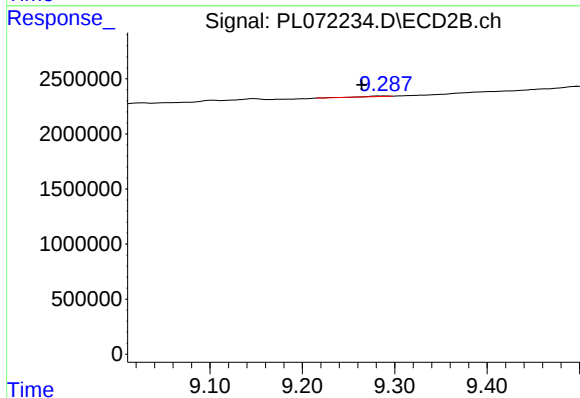


#18 Endrin aldehyde

R.T.: 9.288 min
Delta R.T.: 0.024 min
Response: 52209
Conc: 0.04 ng/ml

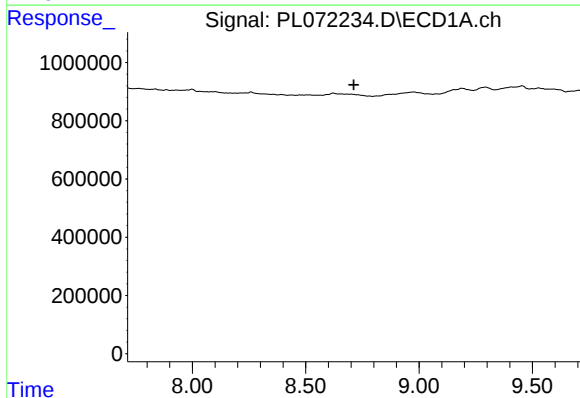


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

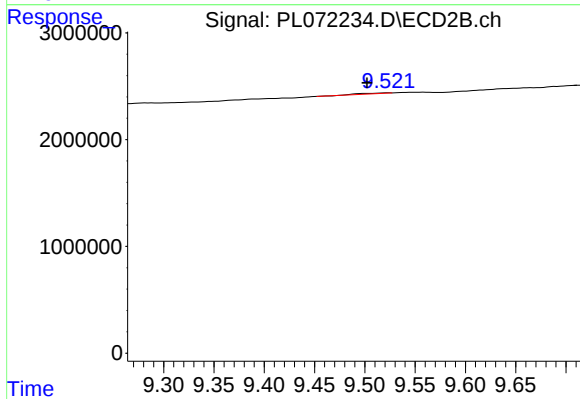

#19 Endosulfan Sulfate


R.T.: 9.522 min
Delta R.T.: 0.020 min
Response: 116376
Conc: 0.07 ng/ml

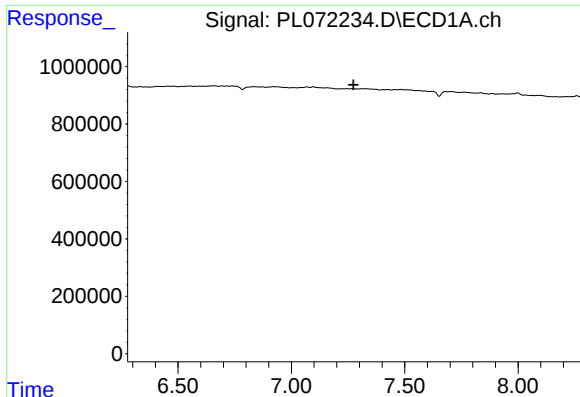

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

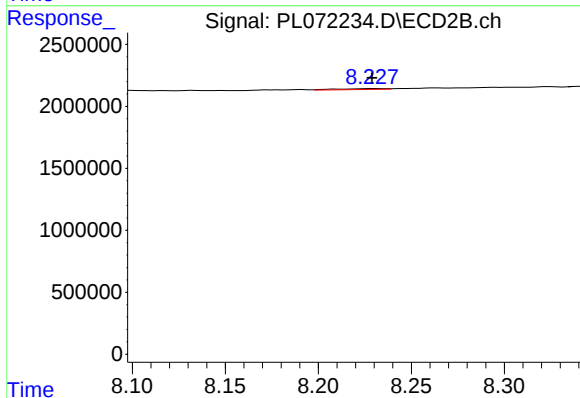


#25 Chlordane-3

R.T.: 8.230 min
Delta R.T.: 0.000 min
Response: 142742
Conc: 0.51 ng/ml

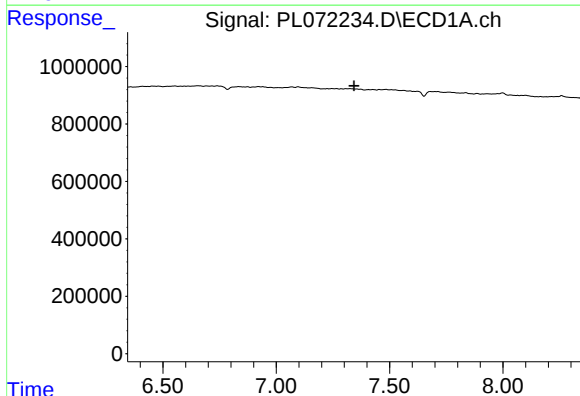


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

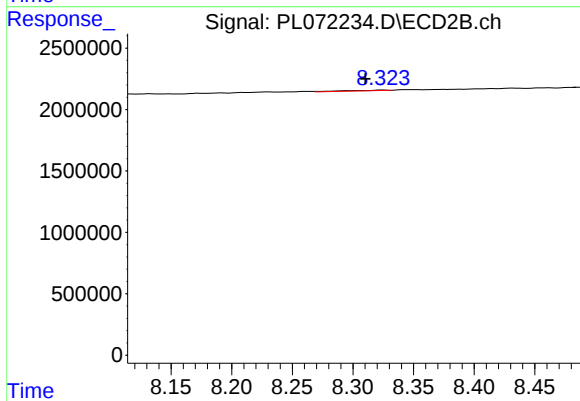

#26 Chlordane-4


R.T.: 8.324 min
Delta R.T.: 0.014 min
Response: 117281
Conc: 0.35 ng/ml

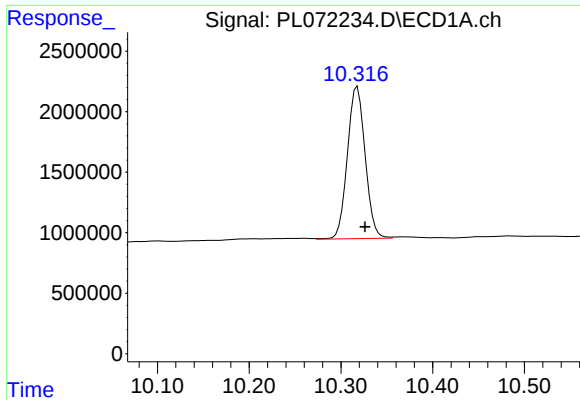

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.009 min
Response: 16863415
Conc: 18.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

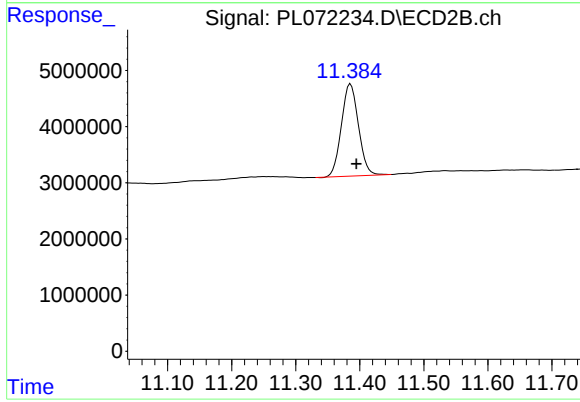

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.009 min
Response: 30320897
Conc: 18.79 ng/ml